

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051220\
 Data File : PL058635.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2020 22:13
 Operator : AJ\MA
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 03:53:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Wed May 13 03:51:19 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.533	4.078	202.9E6	218.4E6	103.340	102.254
28)	SA Decachlor...	8.323	9.192	123.6E6	164.7E6	97.494	96.420
Target Compounds							
23)	Chlordane-1	4.417	5.083	49381097	79912230	1001.449	996.059
24)	Chlordane-2	4.922	5.554	52135724	82400210	967.834	969.919
25)	Chlordane-3	5.497	6.203	146.6E6	314.8E6	1036.547	1041.114
26)	Chlordane-4	5.556	6.278	118.9E6	371.7E6	1023.796	1025.214
27)	Chlordane-5	6.395	7.087	48975468	62564624	1011.500	1005.976



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051220\
Data File : PL058635.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2020 22:13
Operator : AJ\MA
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 03:53:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Wed May 13 03:51:19 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

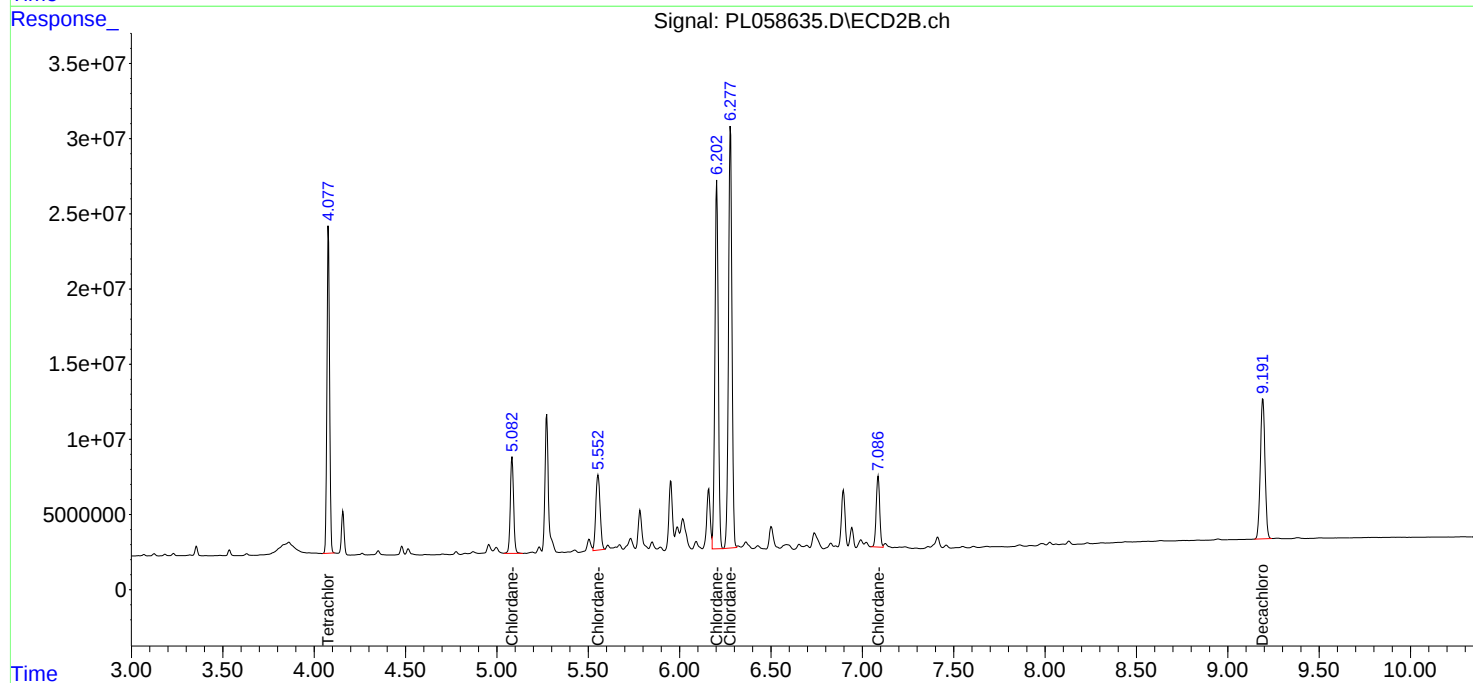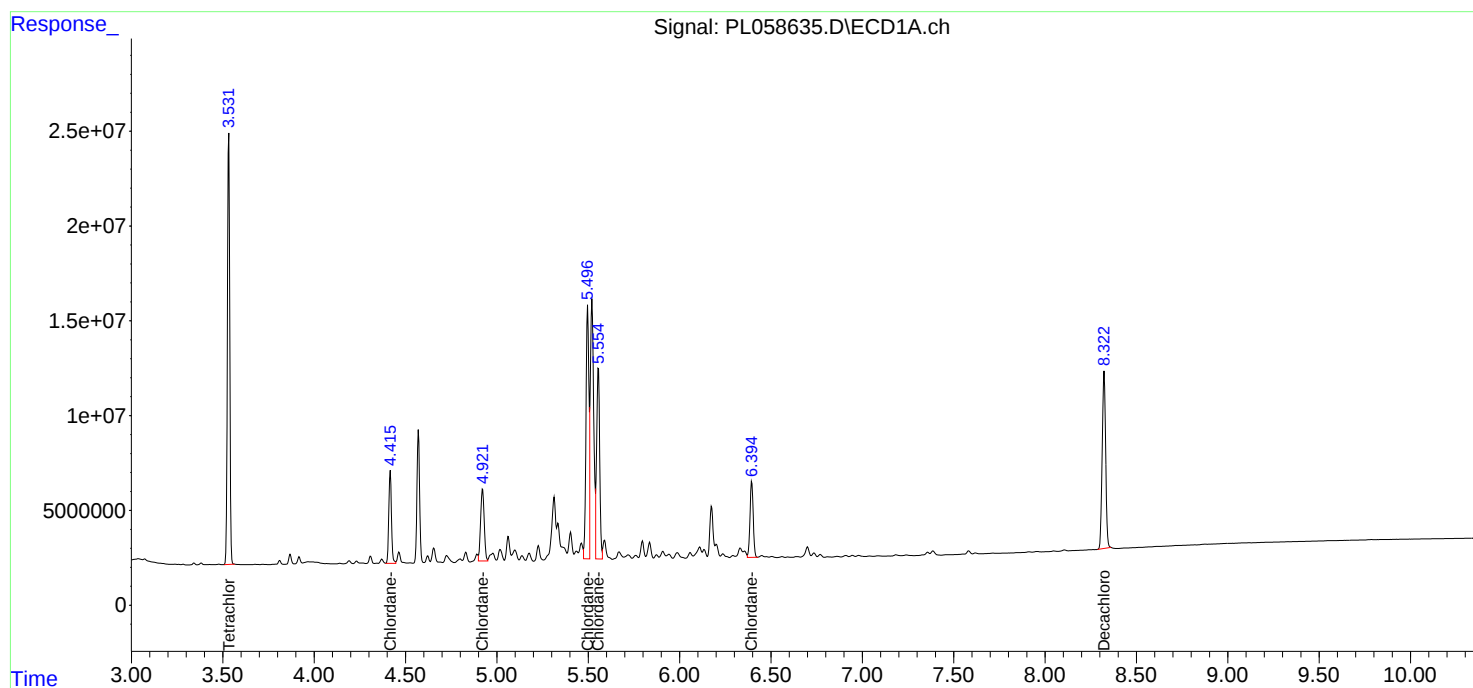


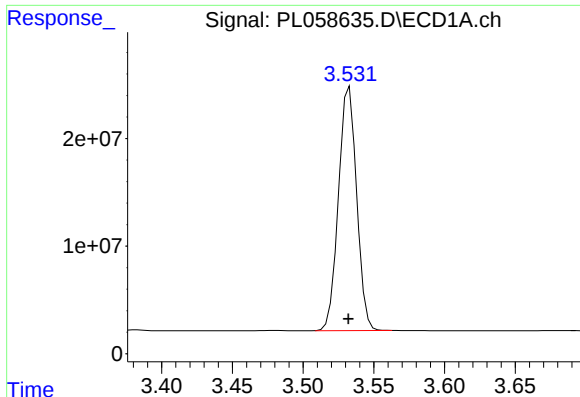

#1 Tetrachloro-m-xylene


R.T.: 3.533 min
Delta R.T.: 0.000 min
Response: 202894302
Conc: 103.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

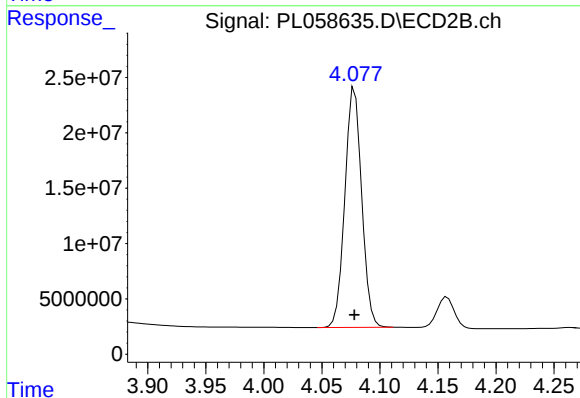


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 218413026
Conc: 102.25 ng/ml

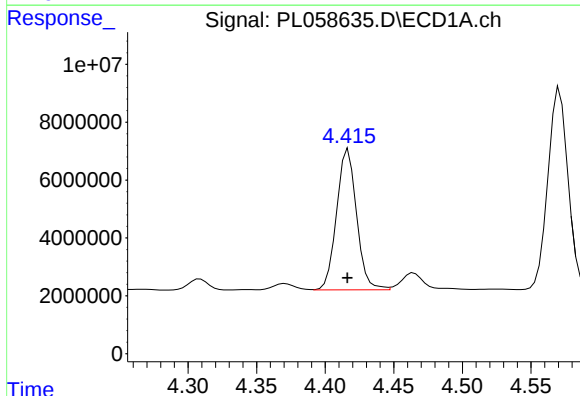


#23 Chlordane-1

R.T.: 4.417 min
Delta R.T.: 0.000 min
Response: 49381097
Conc: 1001.45 ng/ml

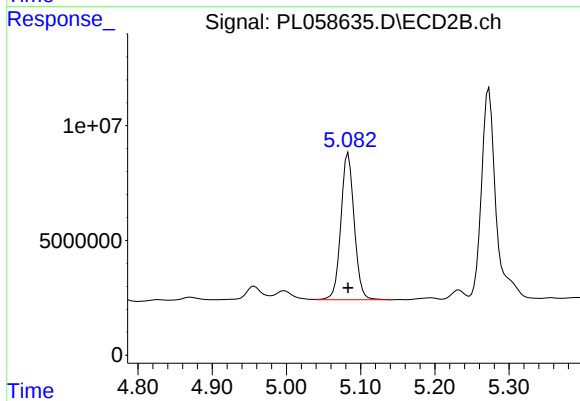

#23 Chlordane-1


R.T.: 5.083 min
Delta R.T.: 0.000 min
Response: 79912230
Conc: 996.06 ng/ml

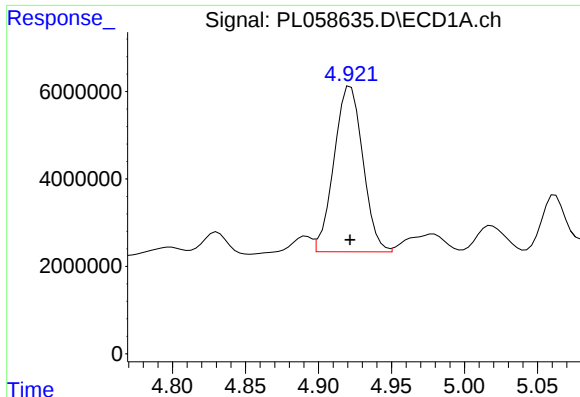

#24 Chlordane-2


R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 52135724
Conc: 967.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

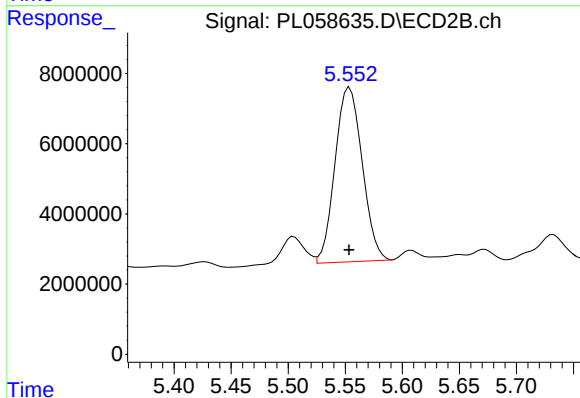


#24 Chlordane-2

R.T.: 5.554 min
Delta R.T.: 0.000 min
Response: 82400210
Conc: 969.92 ng/ml

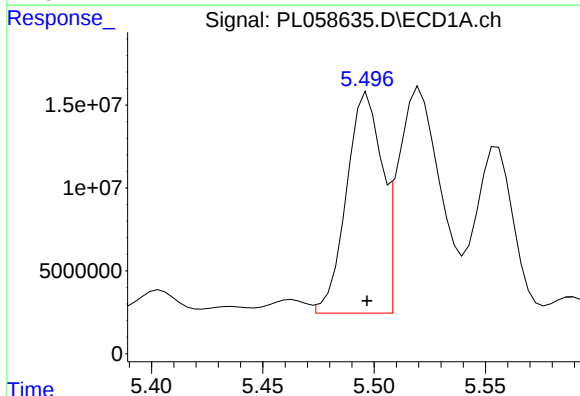


#25 Chlordane-3

R.T.: 5.497 min
Delta R.T.: 0.000 min
Response: 146621691
Conc: 1036.55 ng/ml

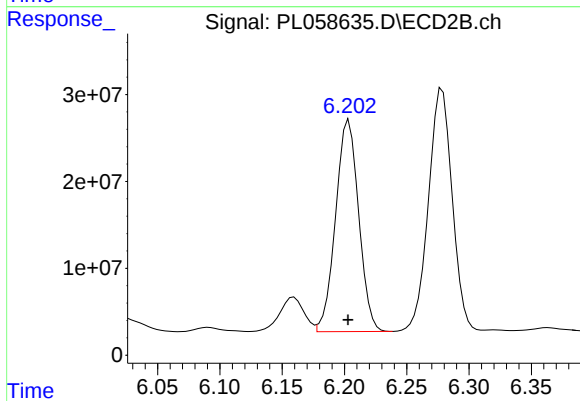

#25 Chlordane-3


R.T.: 6.203 min
Delta R.T.: 0.000 min
Response: 314836142
Conc: 1041.11 ng/ml

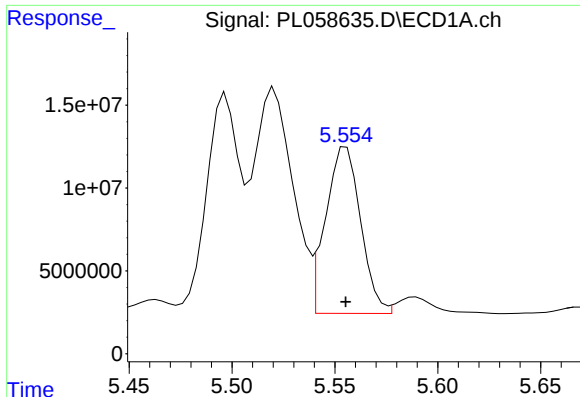

#26 Chlordane-4


R.T.: 5.556 min
Delta R.T.: 0.000 min
Response: 118859826
Conc: 1023.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

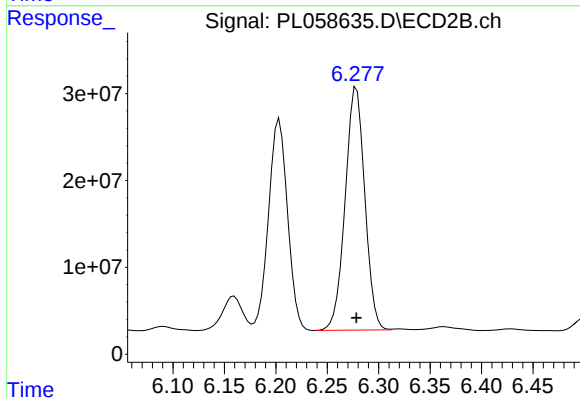


#26 Chlordane-4

R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 371704101
Conc: 1025.21 ng/ml

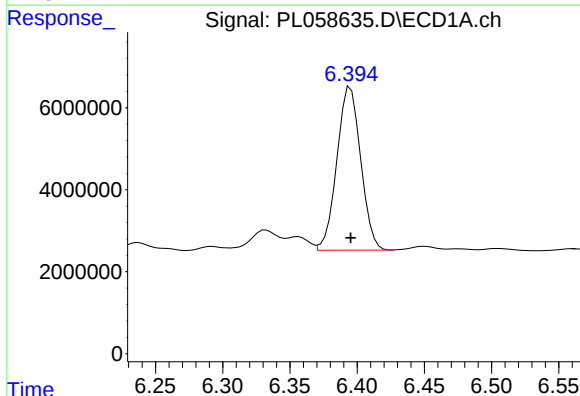


#27 Chlordane-5

R.T.: 6.395 min
Delta R.T.: 0.000 min
Response: 48975468
Conc: 1011.50 ng/ml

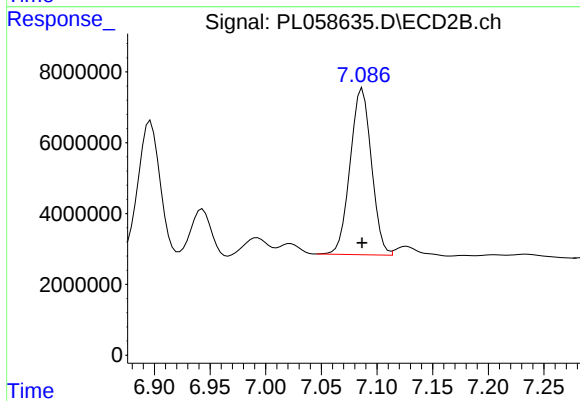

#27 Chlordane-5

R.T.: 7.087 min
Delta R.T.: 0.000 min
Response: 62564624
Conc: 1005.98 ng/ml

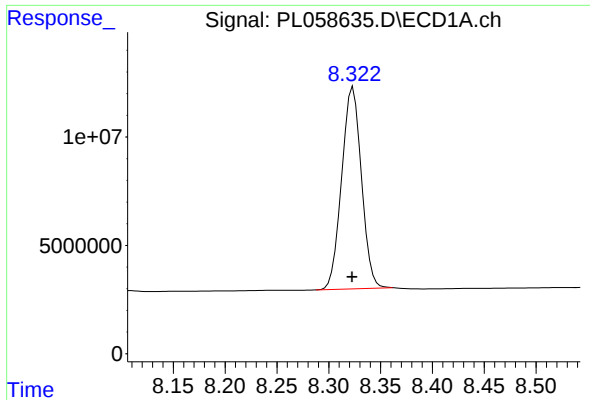

#28 Decachlorobiphenyl


R.T.: 8.323 min

Delta R.T.: 0.000 min

Response: 123590146

Conc: 97.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

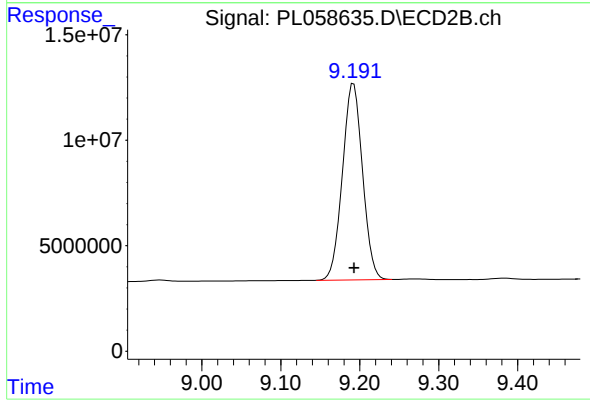

#28 Decachlorobiphenyl

R.T.: 9.192 min

Delta R.T.: 0.000 min

Response: 164650027

Conc: 96.42 ng/ml