

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051220\
 Data File : PL058636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2020 22:27
 Operator : AJ\MA
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 03:53:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Wed May 13 03:51:19 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.532	4.078	151.7E6	163.8E6	77.251	76.693
28)	SA Decachlor...	8.324	9.193	94224958	126.9E6	74.329	74.327
Target Compounds							
23)	Chlordane-1	4.416	5.083	37280624	60542168	756.051	754.623
24)	Chlordane-2	4.922	5.553	40124084	63461074	744.853	746.990
25)	Chlordane-3	5.497	6.203	109.1E6	235.8E6	771.163	779.613
26)	Chlordane-4	5.555	6.278	89132526	280.4E6	767.740	773.390
27)	Chlordane-5	6.395	7.087	36832462	47535868	760.708	764.329



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051220\
Data File : PL058636.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2020 22:27
Operator : AJ\MA
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 03:53:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Wed May 13 03:51:19 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

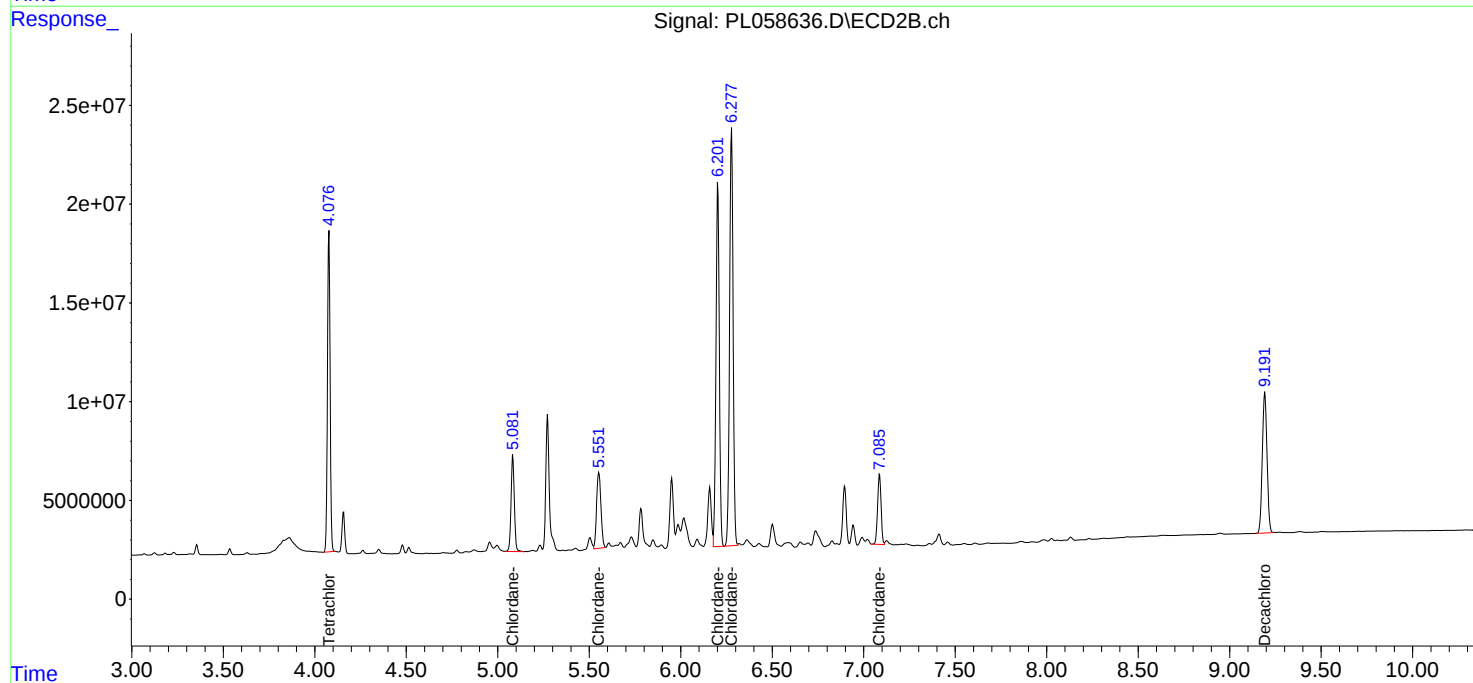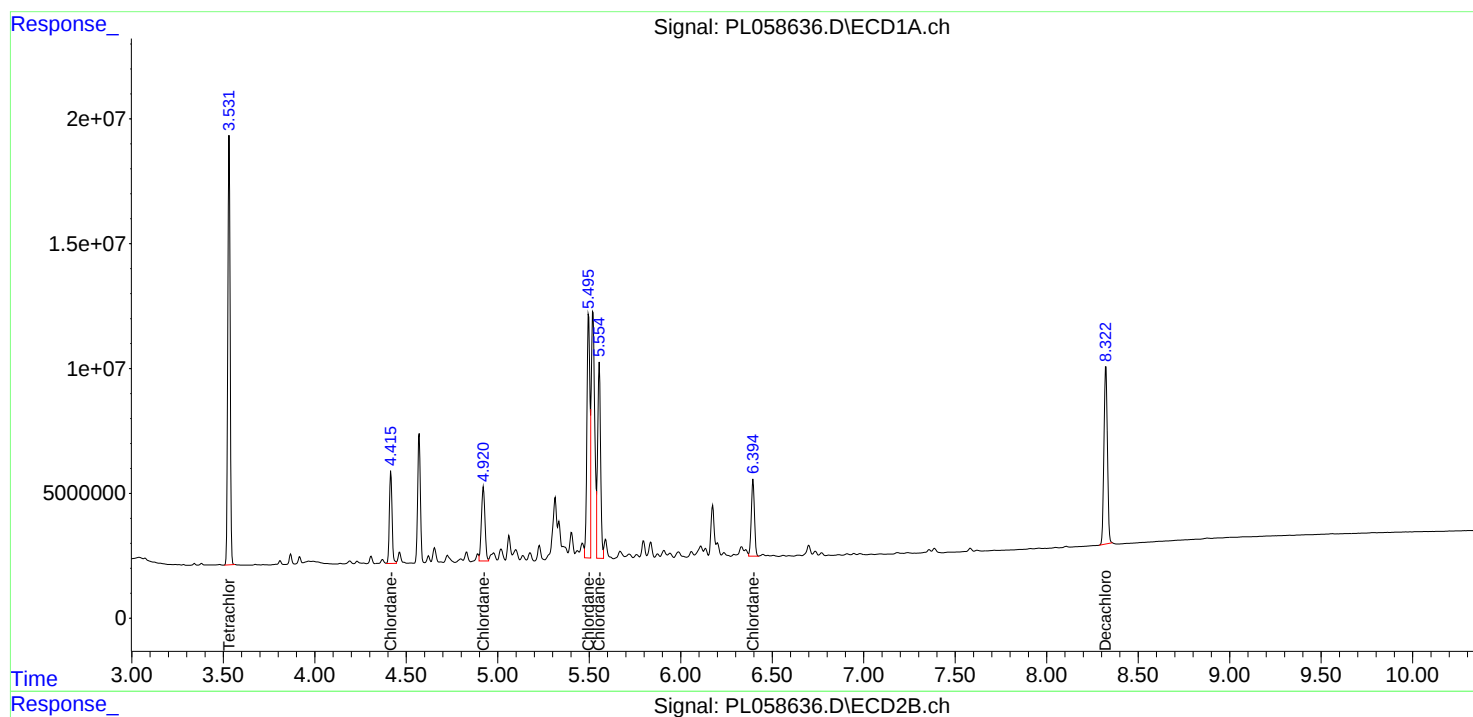


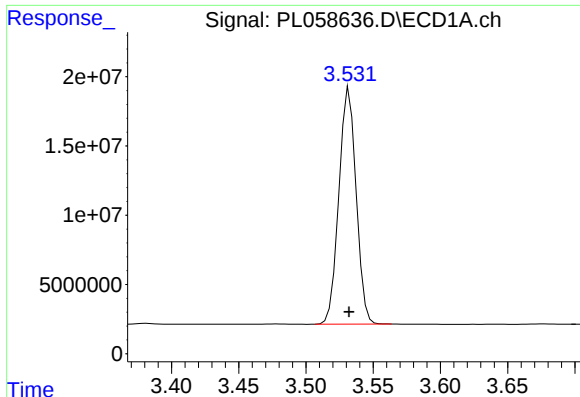

#1 Tetrachloro-m-xylene


R.T.: 3.532 min
Delta R.T.: 0.000 min
Response: 151671708
Conc: 77.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

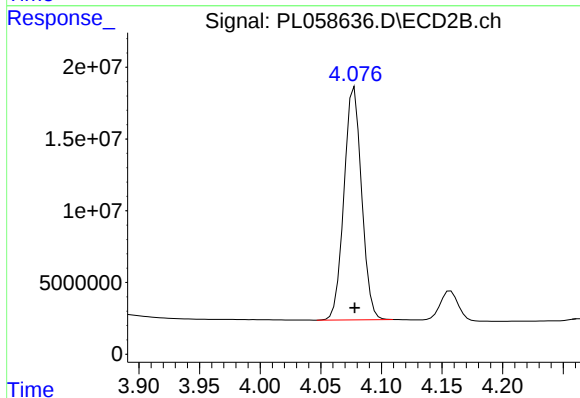


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 163815368
Conc: 76.69 ng/ml

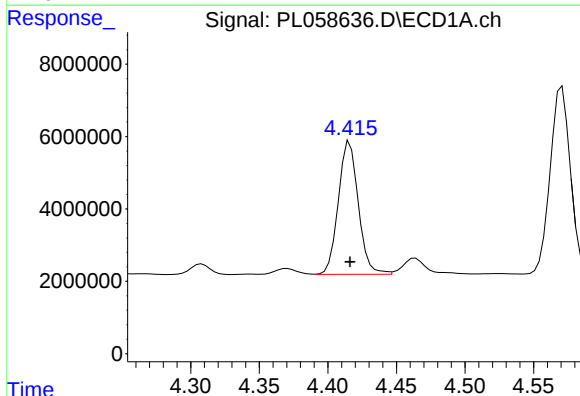


#23 Chlordane-1

R.T.: 4.416 min
Delta R.T.: 0.000 min
Response: 37280624
Conc: 756.05 ng/ml

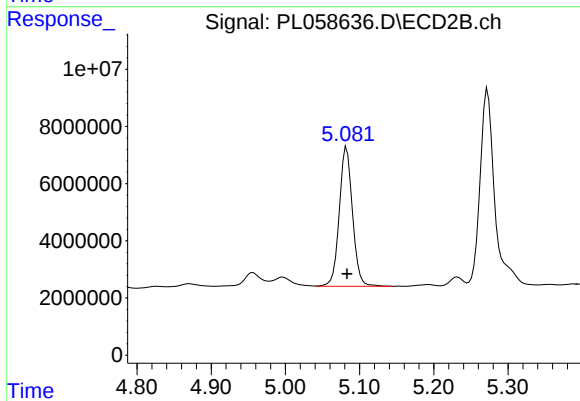

#23 Chlordane-1


R.T.: 5.083 min
Delta R.T.: 0.000 min
Response: 60542168
Conc: 754.62 ng/ml

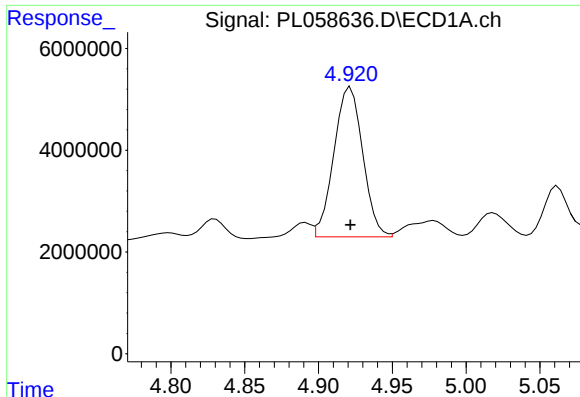

#24 Chlordane-2


R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 40124084
Conc: 744.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

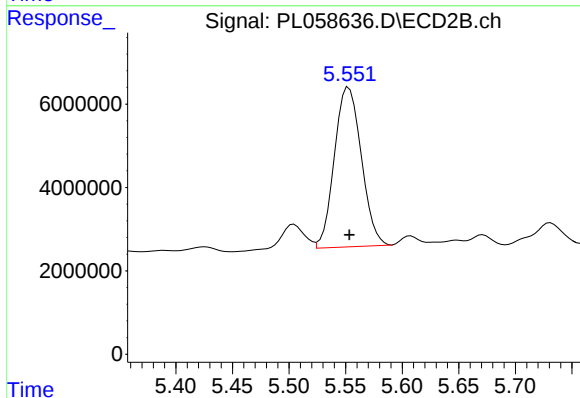


#24 Chlordane-2

R.T.: 5.553 min
Delta R.T.: 0.000 min
Response: 63461074
Conc: 746.99 ng/ml

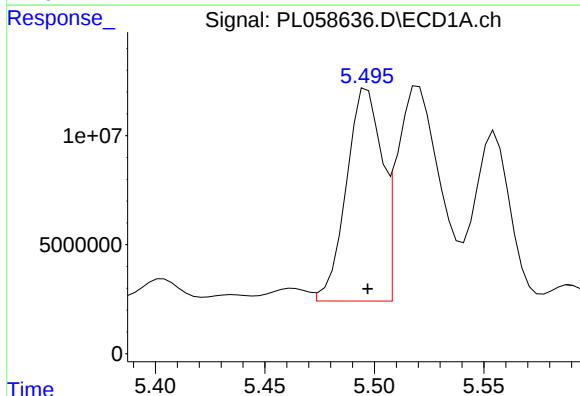


#25 Chlordane-3

R.T.: 5.497 min
Delta R.T.: 0.000 min
Response: 109082514
Conc: 771.16 ng/ml

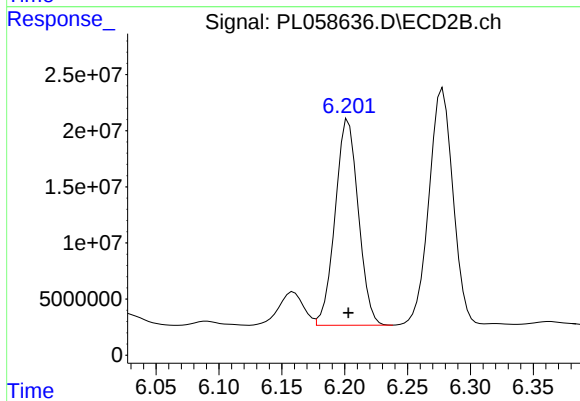

#25 Chlordane-3


R.T.: 6.203 min
Delta R.T.: 0.000 min
Response: 235757240
Conc: 779.61 ng/ml

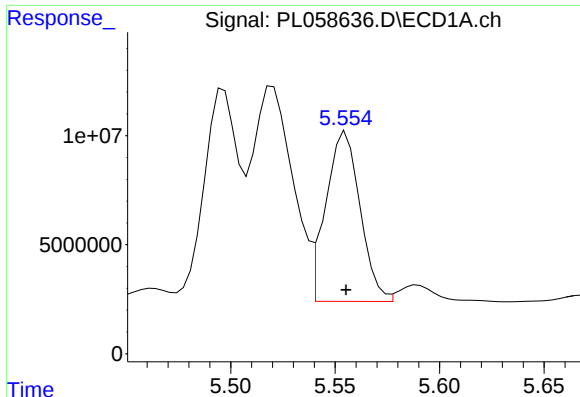

#26 Chlordane-4


R.T.: 5.555 min
Delta R.T.: 0.000 min
Response: 89132526
Conc: 767.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

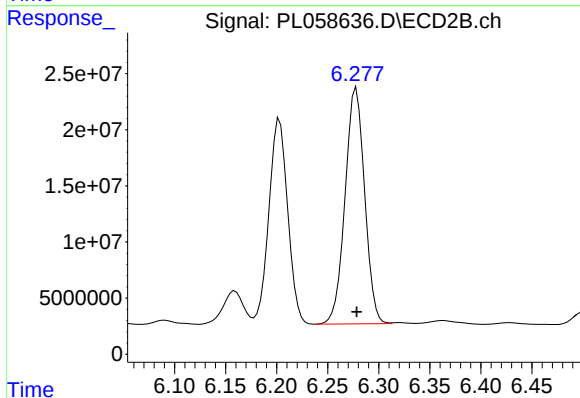


#26 Chlordane-4

R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 280401970
Conc: 773.39 ng/ml

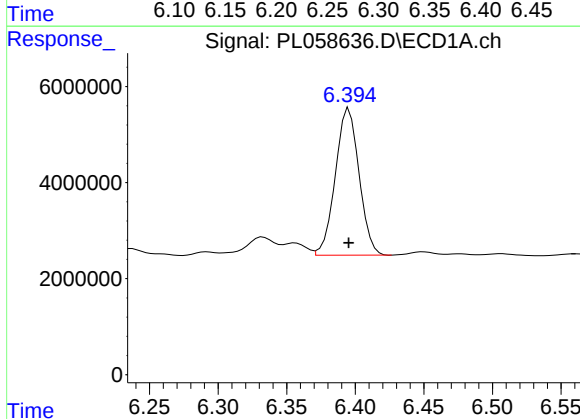


#27 Chlordane-5

R.T.: 6.395 min
Delta R.T.: 0.000 min
Response: 36832462
Conc: 760.71 ng/ml

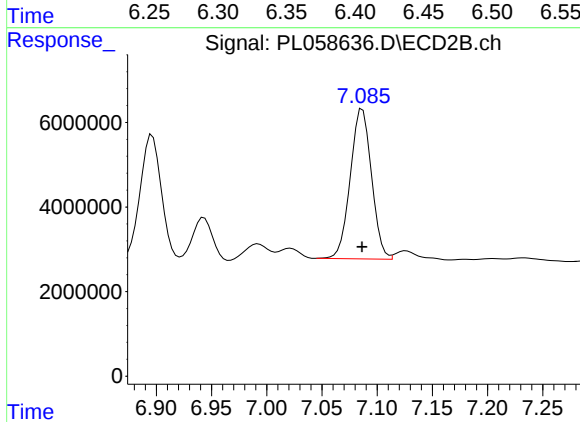

#27 Chlordane-5


R.T.: 7.087 min
Delta R.T.: 0.000 min
Response: 47535868
Conc: 764.33 ng/ml

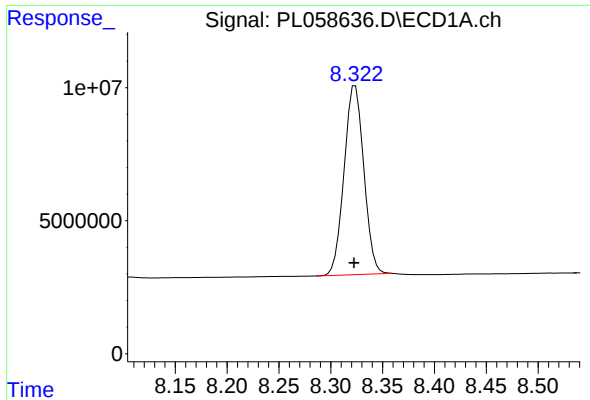

#28 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: 0.001 min
Response: 94224958
Conc: 74.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

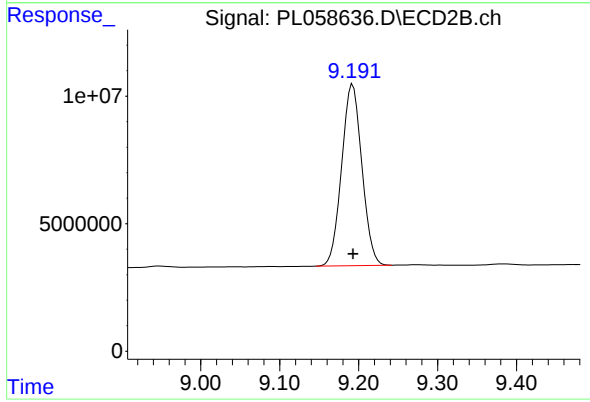

#28 Decachlorobiphenyl

R.T.: 9.193 min
Delta R.T.: 0.000 min
Response: 126922714
Conc: 74.33 ng/ml