

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051220\
 Data File : PL058637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2020 22:41
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 03:53:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Wed May 13 03:51:19 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.532	4.078	98168524	106.8E6	50.000	50.000
28)	SA Decachlor...	8.323	9.193	63383370	85381683	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.416	5.083	24654834	40114196	500.000	500.000
24)	Chlordane-2	4.922	5.553	26934215	42477883	500.000	500.000
25)	Chlordane-3	5.497	6.203	70725997	151.2E6	500.000	500.000
26)	Chlordane-4	5.555	6.278	58048610	181.3E6	500.000	500.000
27)	Chlordane-5	6.395	7.087	24209331	31096473	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051220\
Data File : PL058637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2020 22:41
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 03:53:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Wed May 13 03:51:19 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

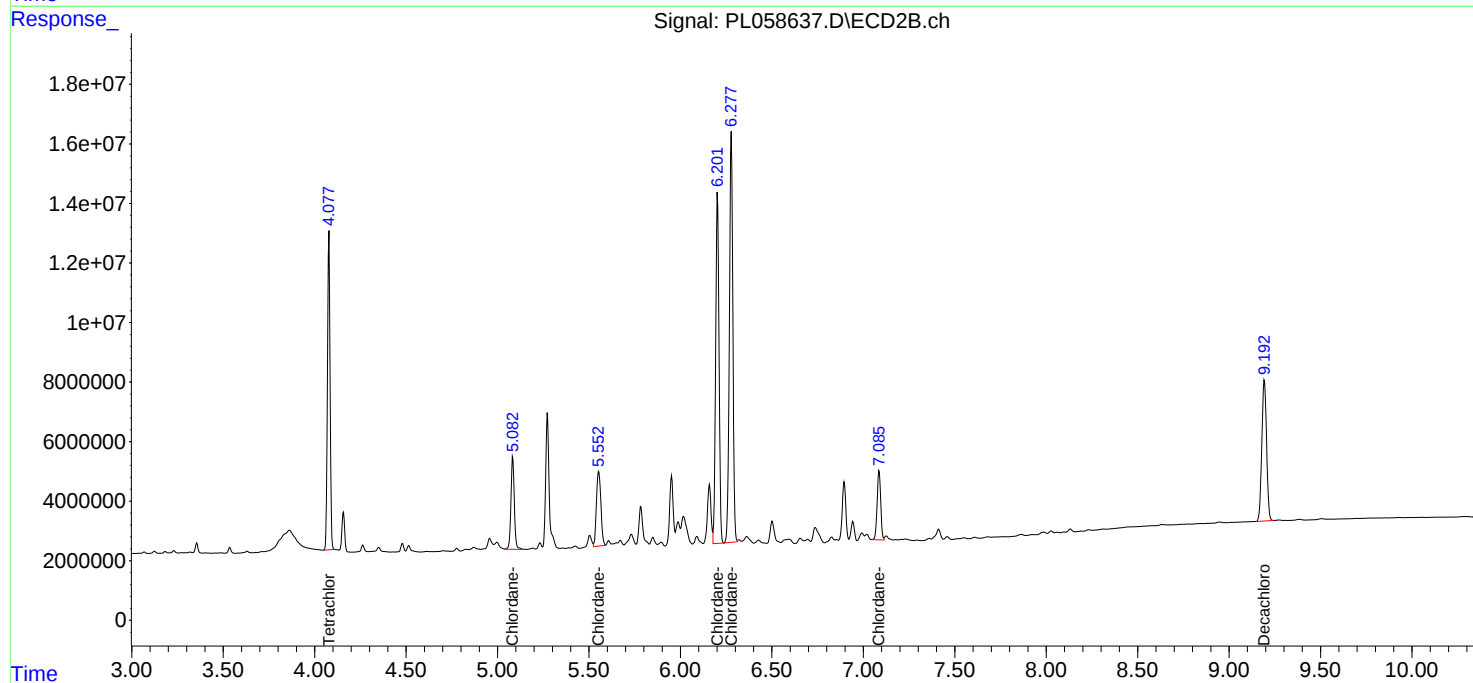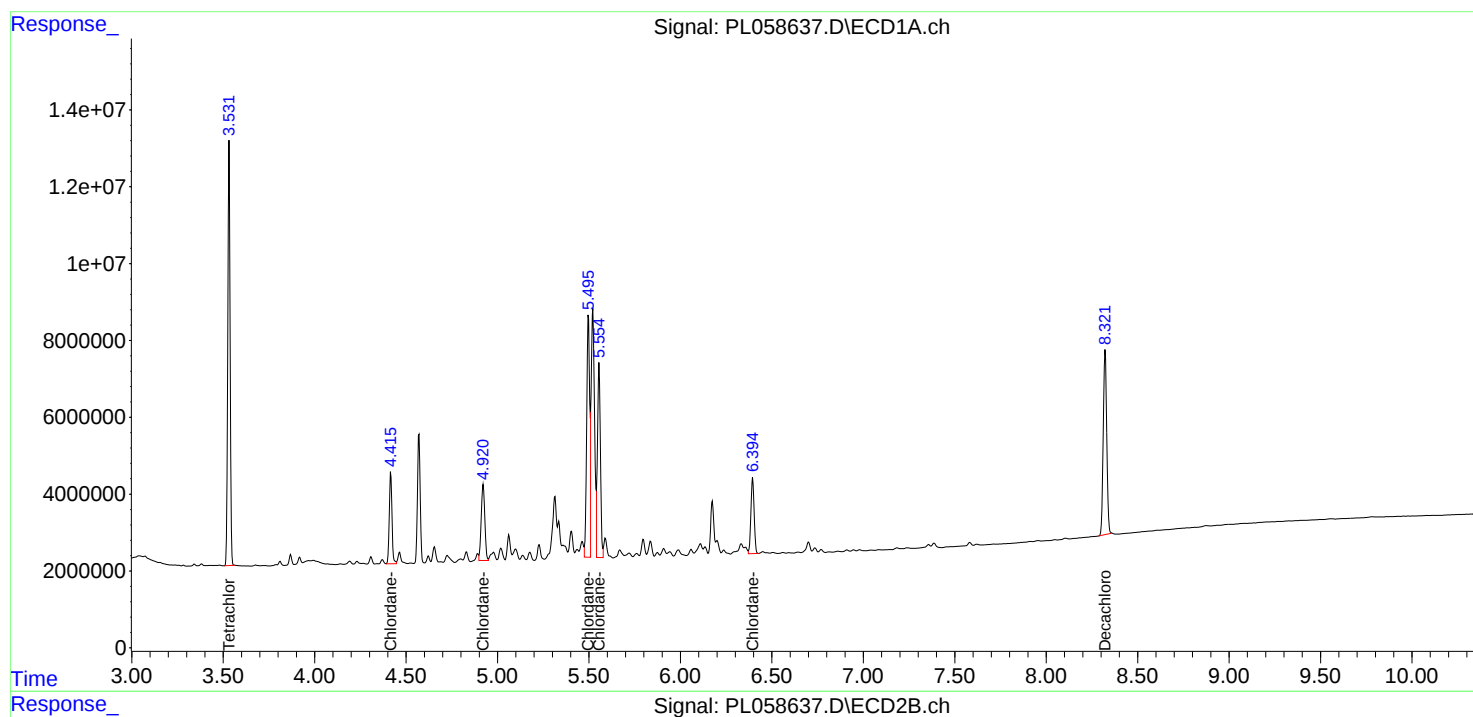


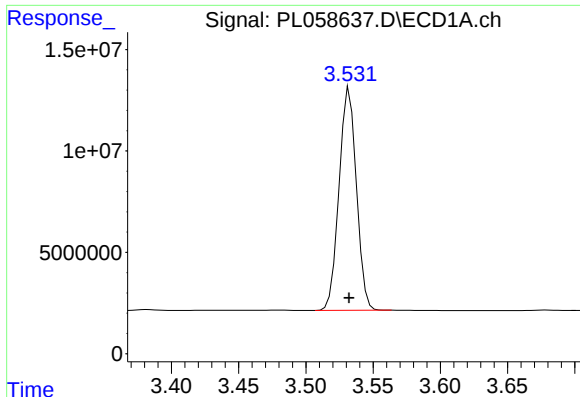

#1 Tetrachloro-m-xylene


R.T.: 3.532 min
Delta R.T.: 0.000 min
Response: 98168524
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

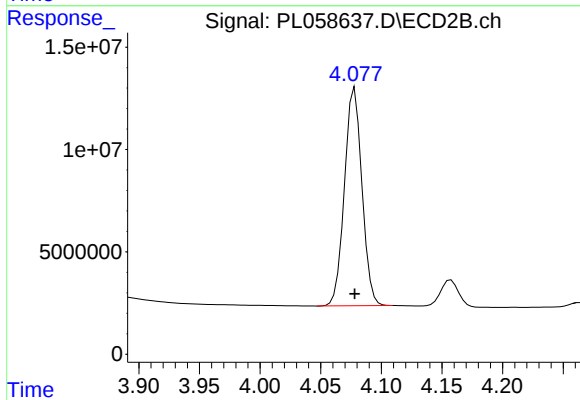


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 106799761
Conc: 50.00 ng/ml

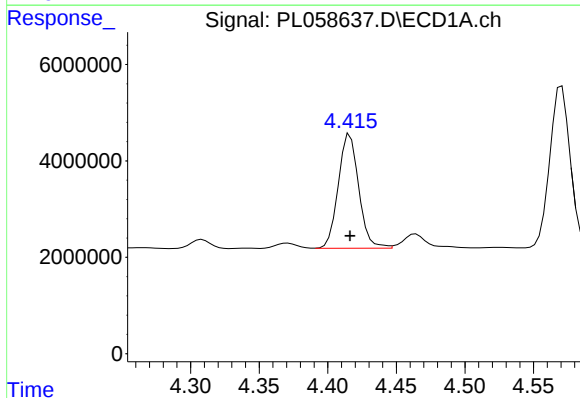


#23 Chlordane-1

R.T.: 4.416 min
Delta R.T.: 0.000 min
Response: 24654834
Conc: 500.00 ng/ml

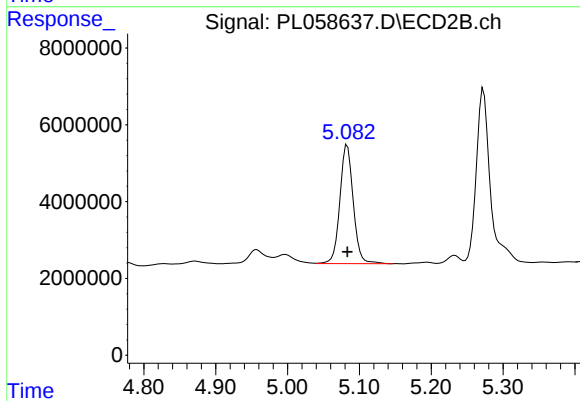

#23 Chlordane-1


R.T.: 5.083 min
Delta R.T.: 0.000 min
Response: 40114196
Conc: 500.00 ng/ml

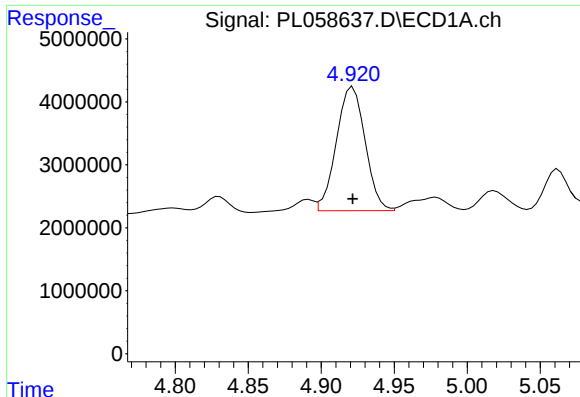

#24 Chlordane-2


R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 26934215
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

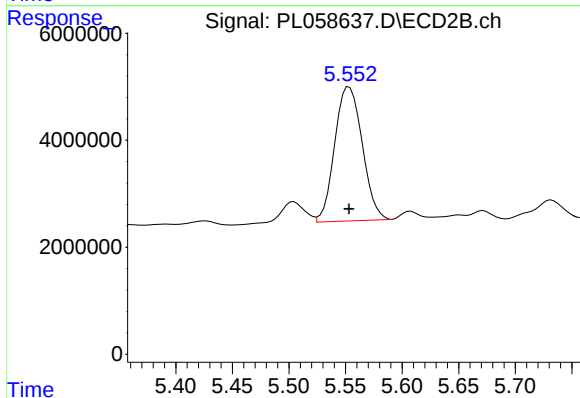


#24 Chlordane-2

R.T.: 5.553 min
Delta R.T.: 0.000 min
Response: 42477883
Conc: 500.00 ng/ml

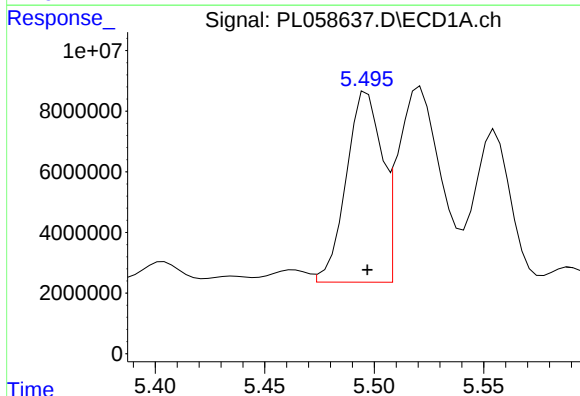


#25 Chlordane-3

R.T.: 5.497 min
Delta R.T.: 0.000 min
Response: 70725997
Conc: 500.00 ng/ml

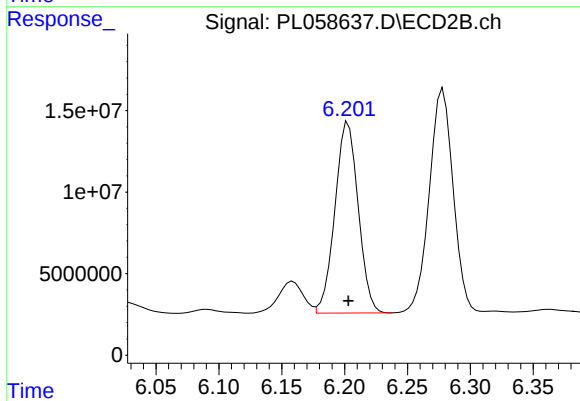

#25 Chlordane-3


R.T.: 6.203 min
Delta R.T.: 0.000 min
Response: 151201529
Conc: 500.00 ng/ml

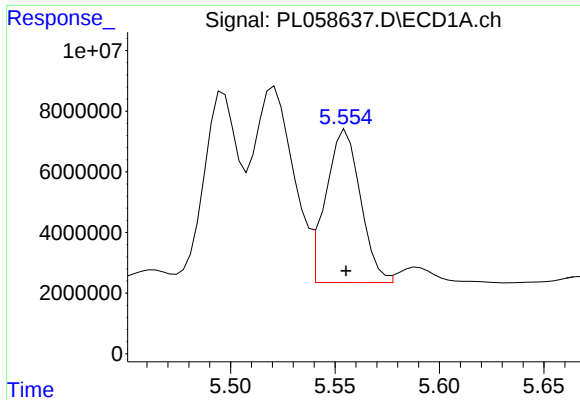

#26 Chlordane-4


R.T.: 5.555 min
Delta R.T.: 0.000 min
Response: 58048610
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

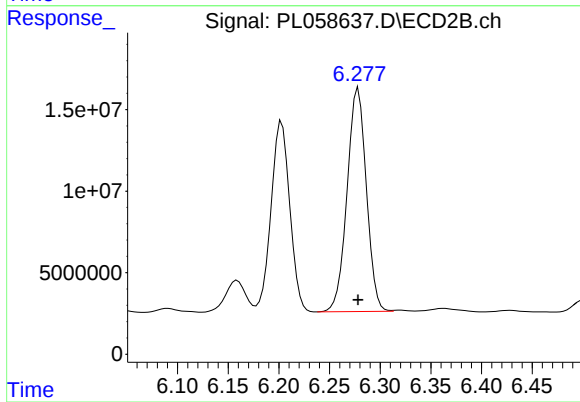


#26 Chlordane-4

R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 181281145
Conc: 500.00 ng/ml

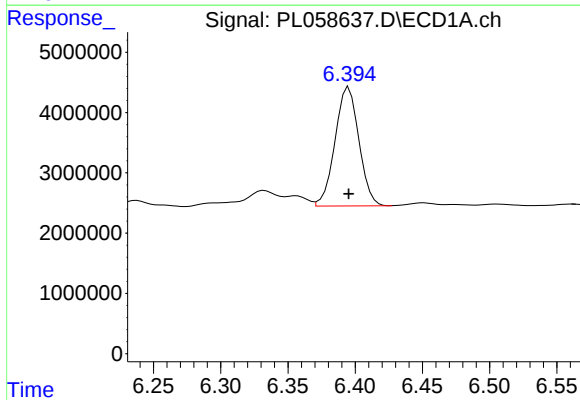


#27 Chlordane-5

R.T.: 6.395 min
Delta R.T.: 0.000 min
Response: 24209331
Conc: 500.00 ng/ml

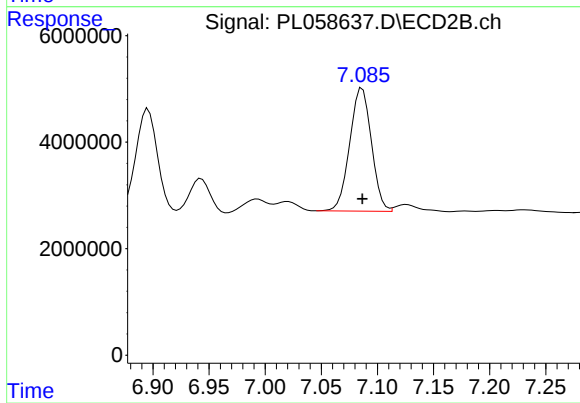

#27 Chlordane-5


R.T.: 7.087 min
Delta R.T.: 0.000 min
Response: 31096473
Conc: 500.00 ng/ml

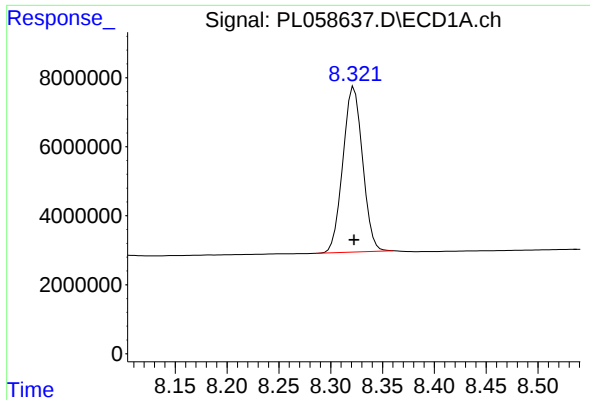

#28 Decachlorobiphenyl

R.T.: 8.323 min
Delta R.T.: 0.000 min
Response: 63383370
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

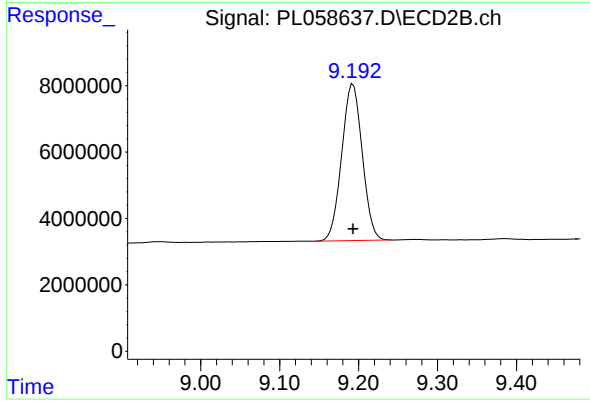

#28 Decachlorobiphenyl

R.T.: 9.193 min
Delta R.T.: 0.000 min
Response: 85381683
Conc: 50.00 ng/ml