

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051220\
 Data File : PL058646.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2020 00:48
 Operator : AJ\MA
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL051220CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 09:03:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Wed May 13 09:01:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.533	4.078	99800559	108.5E6	50.759	51.240
28)	SA Decachlor...	8.322	9.194	65703597	88172181	51.436	50.891
Target Compounds							
23)	Chlordane-1	4.416	5.083	25333799	41043440	505.173	512.876
24)	Chlordane-2	4.921	5.553	29000278	43354854	533.887	507.340
25)	Chlordane-3	5.497	6.203	73261972	155.9E6	523.657	514.670
26)	Chlordane-4	5.555	6.279	59587946	186.7E6	519.180	512.268
27)	Chlordane-5	6.395	7.087	25007549	32032808	512.367	513.103



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051220\
Data File : PL058646.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2020 00:48
Operator : AJ\MA
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL051220CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 09:03:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Wed May 13 09:01:52 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

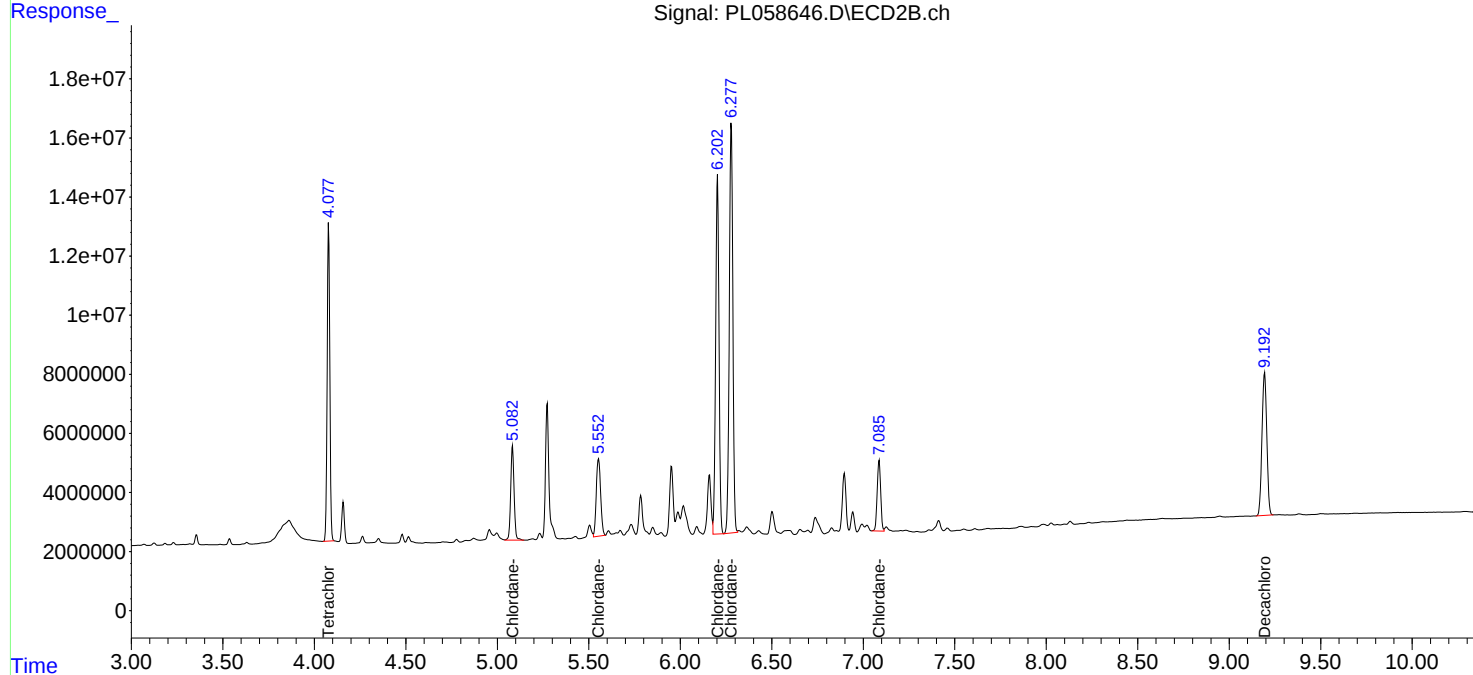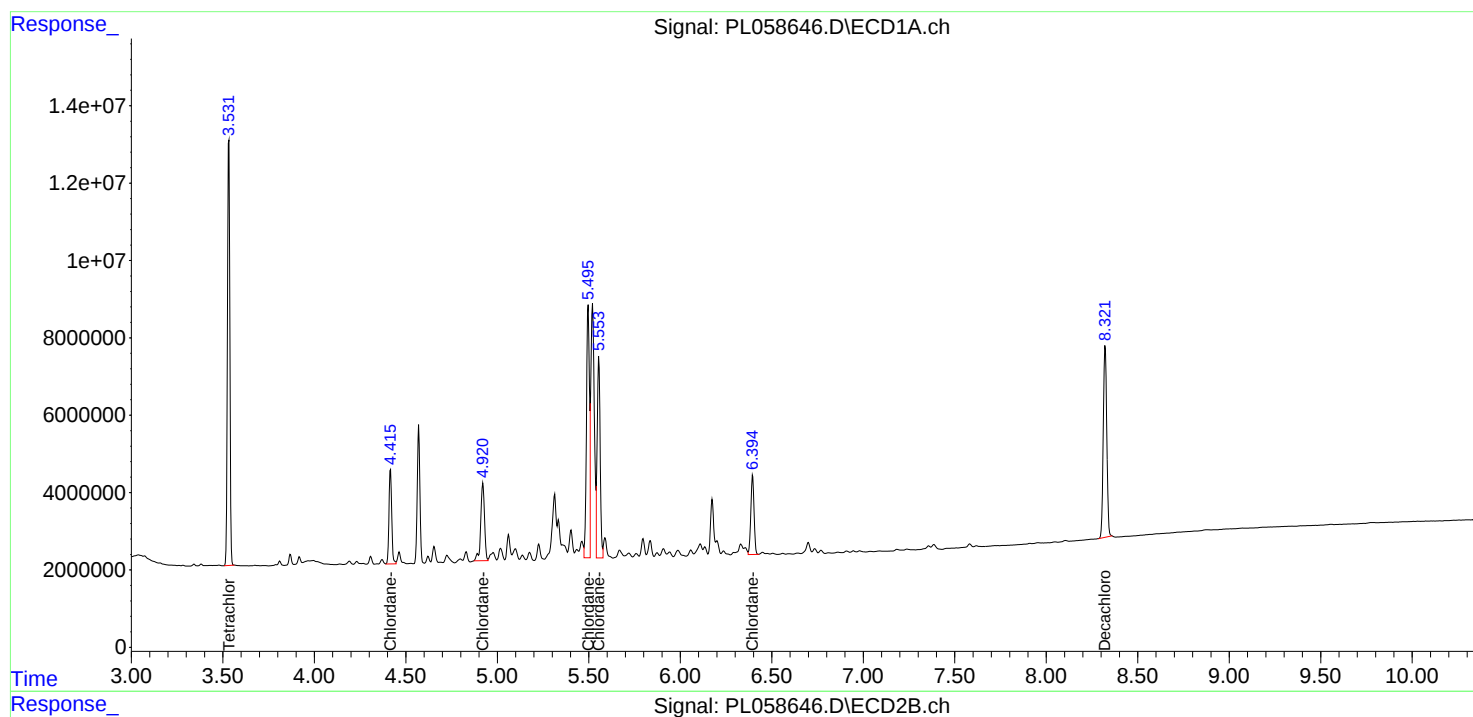


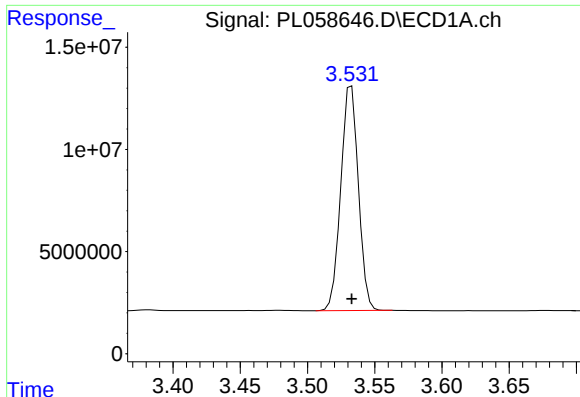

#1 Tetrachloro-m-xylene


R.T.: 3.533 min
Delta R.T.: 0.000 min
Response: 99800559
Conc: 50.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL051220CHLOR

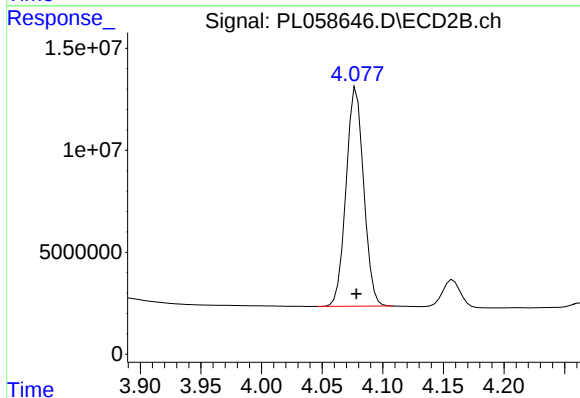


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 108524207
Conc: 51.24 ng/ml

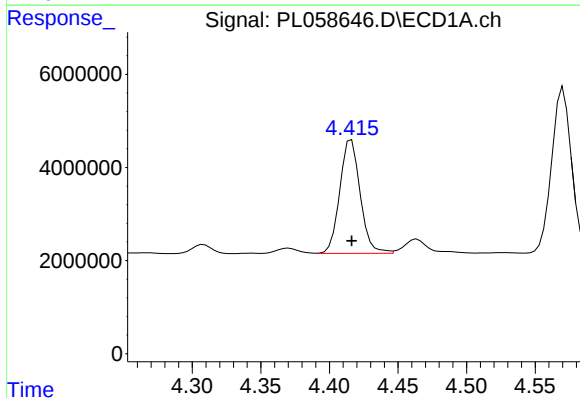


#23 Chlordane-1

R.T.: 4.416 min
Delta R.T.: 0.000 min
Response: 25333799
Conc: 505.17 ng/ml

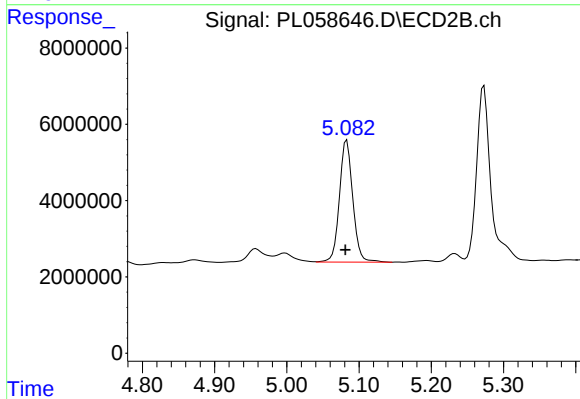

#23 Chlordane-1


R.T.: 5.083 min
Delta R.T.: 0.002 min
Response: 41043440
Conc: 512.88 ng/ml

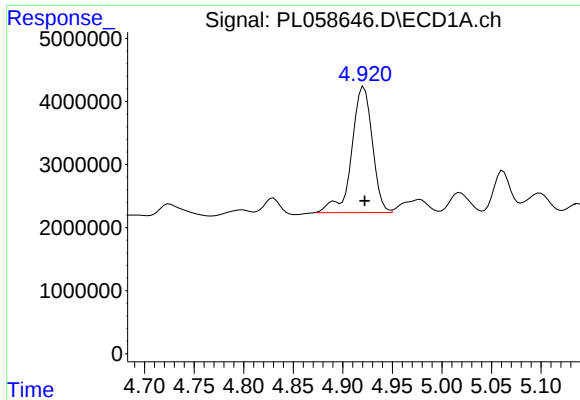

#24 Chlordane-2


R.T.: 4.921 min
Delta R.T.: 0.000 min
Response: 29000278
Conc: 533.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL051220CHLOR

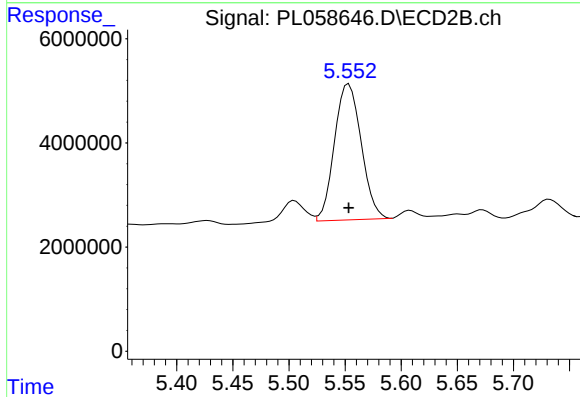


#24 Chlordane-2

R.T.: 5.553 min
Delta R.T.: 0.000 min
Response: 43354854
Conc: 507.34 ng/ml

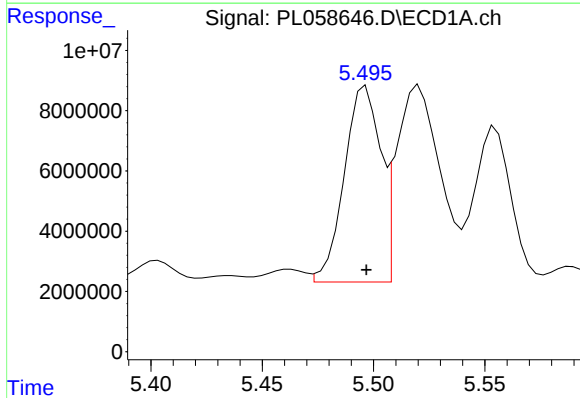


#25 Chlordane-3

R.T.: 5.497 min
Delta R.T.: 0.000 min
Response: 73261972
Conc: 523.66 ng/ml

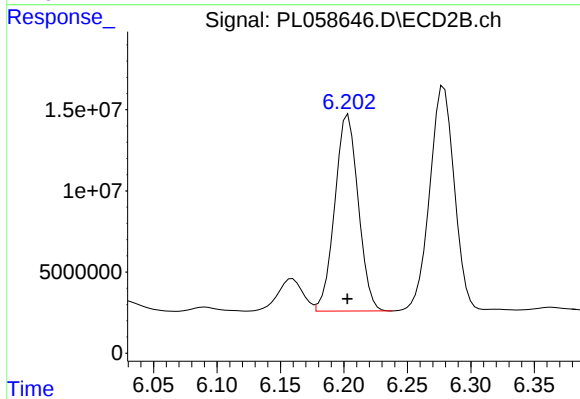

#25 Chlordane-3


R.T.: 6.203 min
Delta R.T.: 0.000 min
Response: 155885557
Conc: 514.67 ng/ml

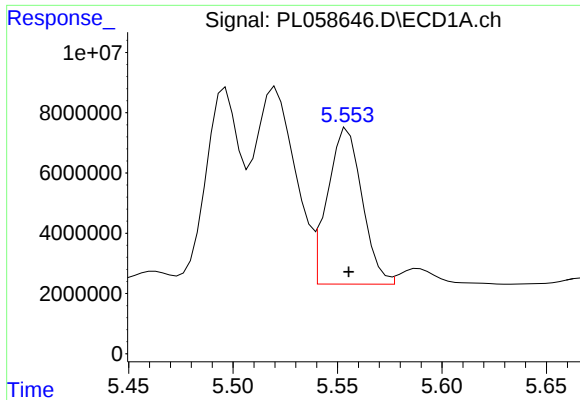

#26 Chlordane-4


R.T.: 5.555 min
Delta R.T.: 0.000 min
Response: 59587946
Conc: 519.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL051220CHLOR

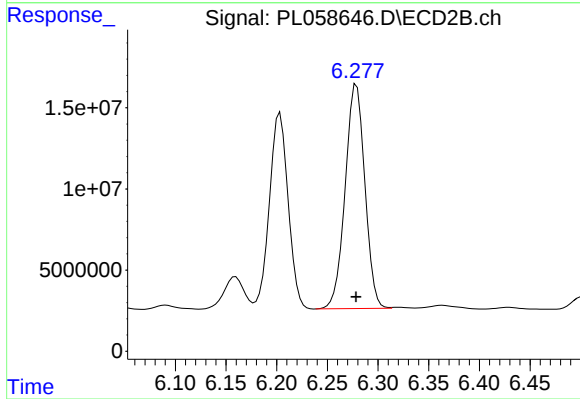


#26 Chlordane-4

R.T.: 6.279 min
Delta R.T.: 0.000 min
Response: 186701996
Conc: 512.27 ng/ml

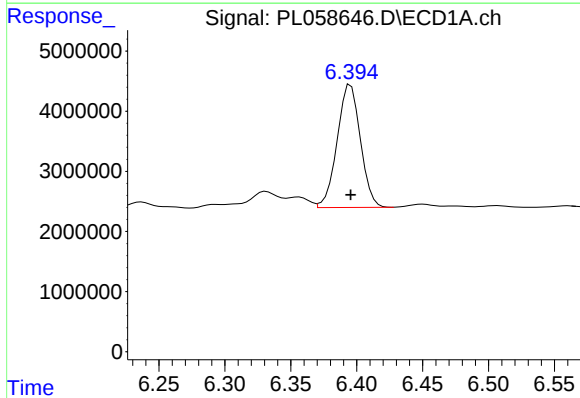


#27 Chlordane-5

R.T.: 6.395 min
Delta R.T.: 0.000 min
Response: 25007549
Conc: 512.37 ng/ml

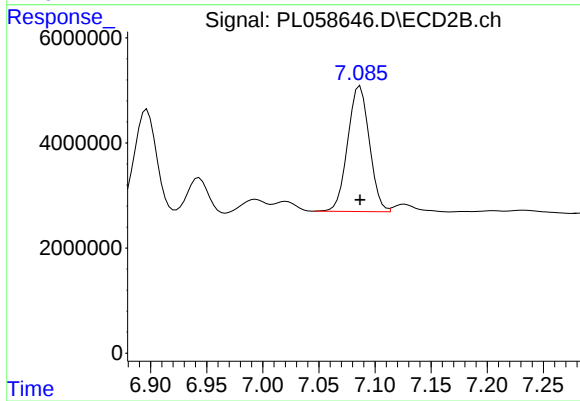

#27 Chlordane-5


R.T.: 7.087 min
Delta R.T.: 0.000 min
Response: 32032808
Conc: 513.10 ng/ml

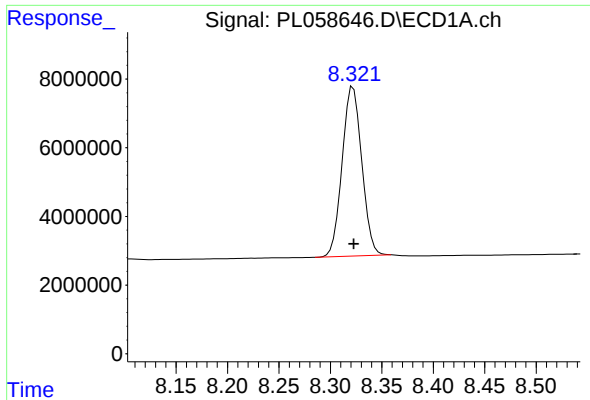

#28 Decachlorobiphenyl

R.T.: 8.322 min
Delta R.T.: 0.000 min
Response: 65703597
Conc: 51.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL051220CHLOR

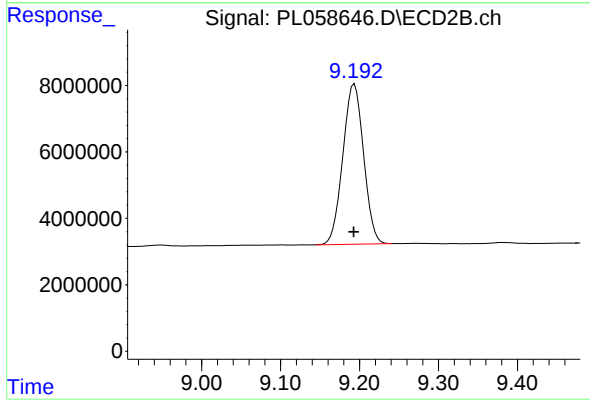

#28 Decachlorobiphenyl

R.T.: 9.194 min
Delta R.T.: 0.000 min
Response: 88172181
Conc: 50.89 ng/ml