

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051222\
 Data File : PL074652.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2022 08:41
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 14:47:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 16:19:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	0.000	10.425f	0	381591	N.D.	0.372 #
Target Compounds							
4)	MA Heptachlor	0.000	6.169f	0	353199	N.D.	0.233 #
5)	MB Aldrin	0.000	6.535f	0	229395	N.D.	0.153 #
6)	B beta-BHC	0.000	6.169f	0	353199	N.D.	0.445 #
8)	B Heptachlo...	8.138	0.000	18477228	0	32.488	N.D. #
9)	A Endosulfan I	8.520	7.466f	5604749	1721011	9.722	1.376 #
10)	B gamma-Chl...	0.000	7.349	0	1456483	N.D.	1.051 #
16)	A 4,4'-DDD	0.000	8.225	0	728432	N.D.	0.739 #
19)	B Endosulfa...	0.000	8.813f	0	228557	N.D.	0.210 #
25)	Chlordane-3	0.000	7.349	0	1456483	N.D.	11.222 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051222\
Data File : PL074652.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2022 08:41
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 14:47:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 16:19:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

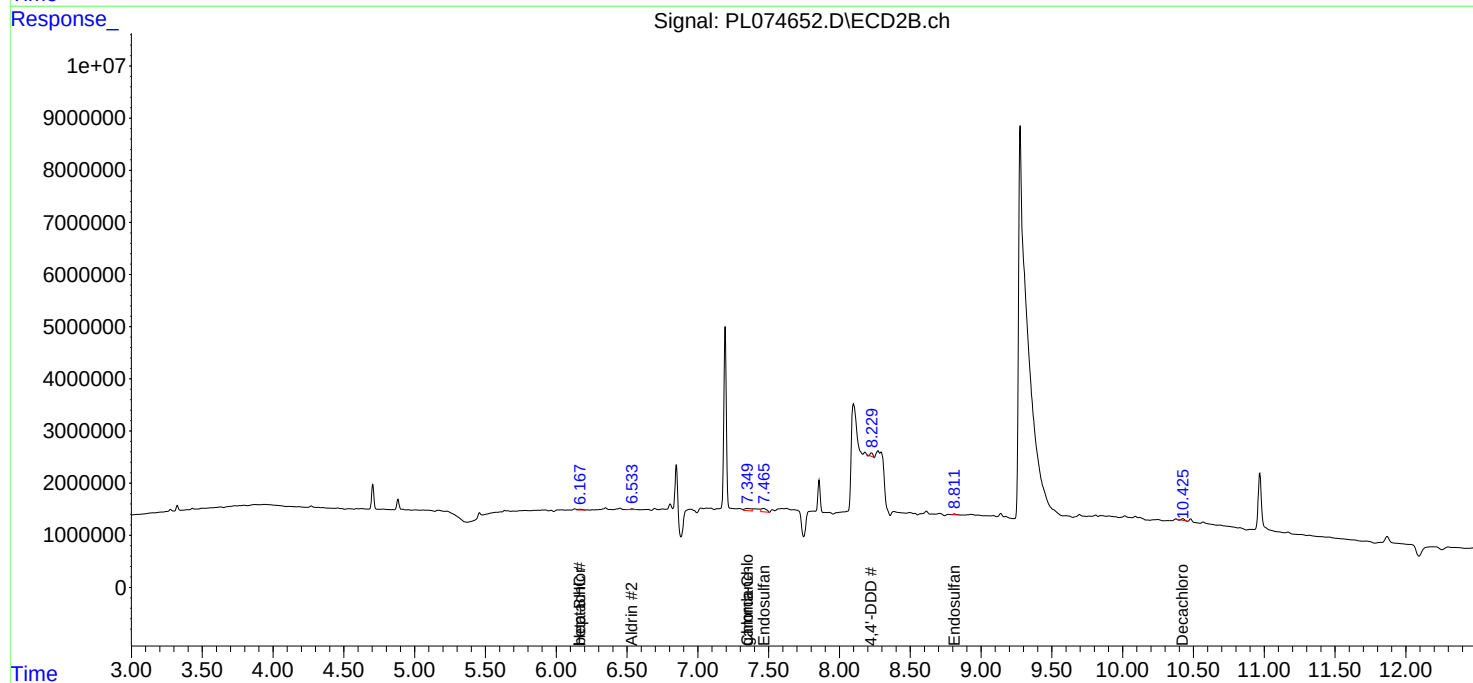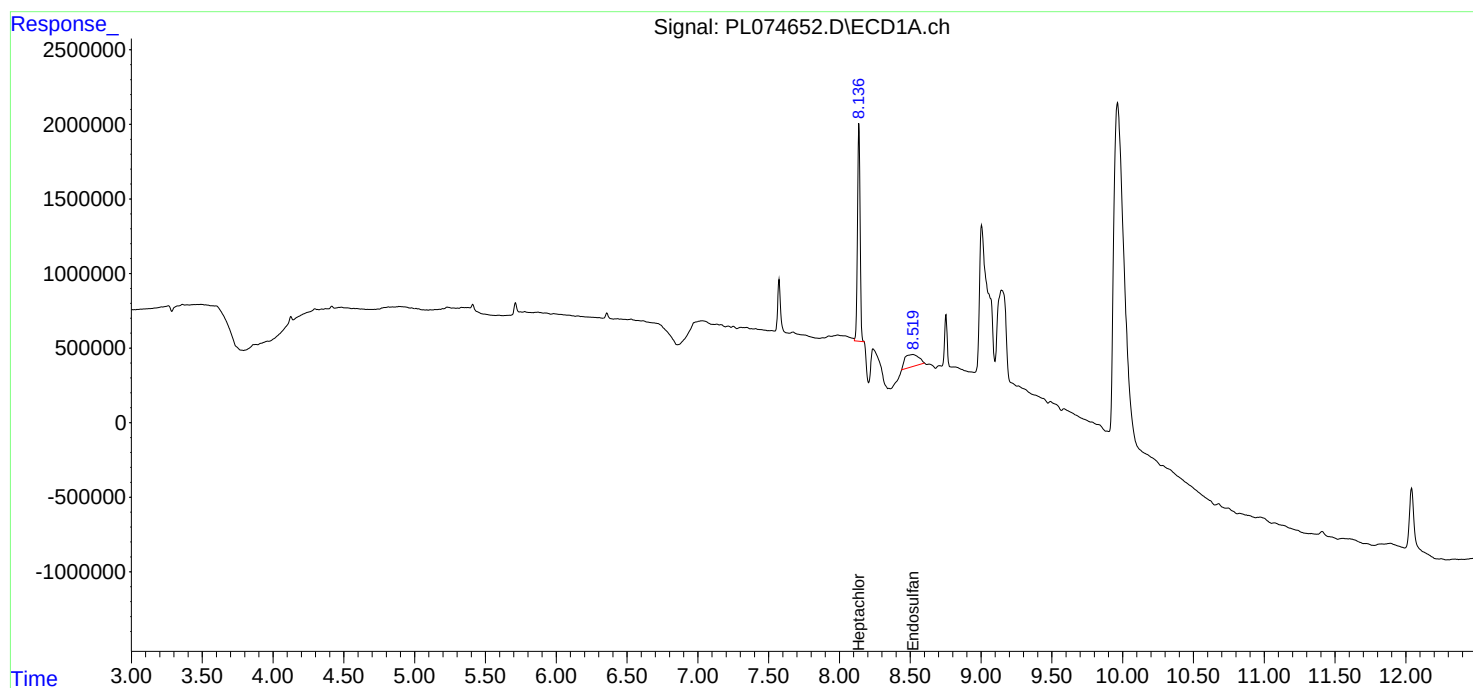


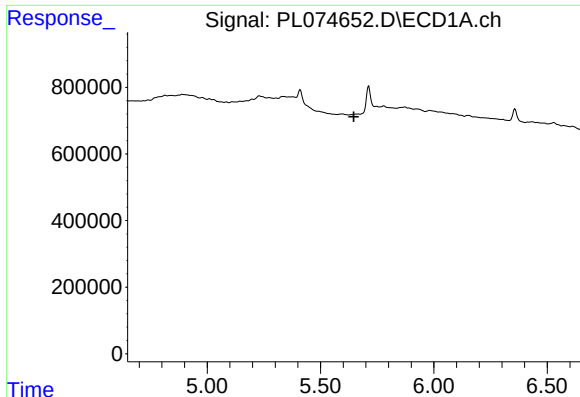

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 5.647 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

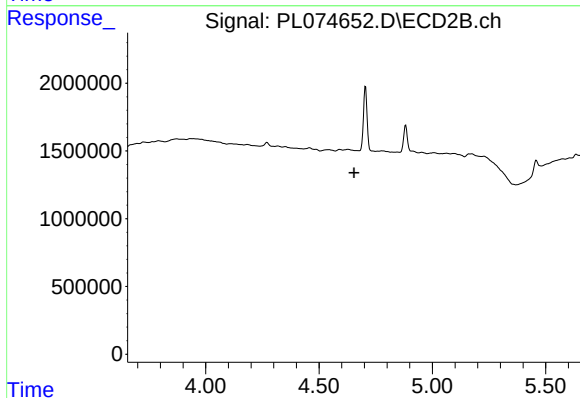


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.654 min
Response: 0
Conc: N.D.

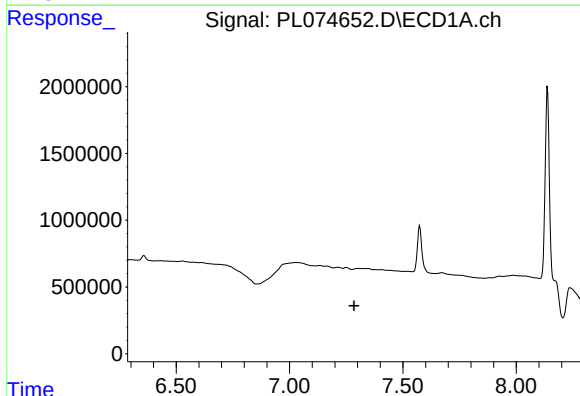


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.284 min
Response: 0
Conc: N.D.

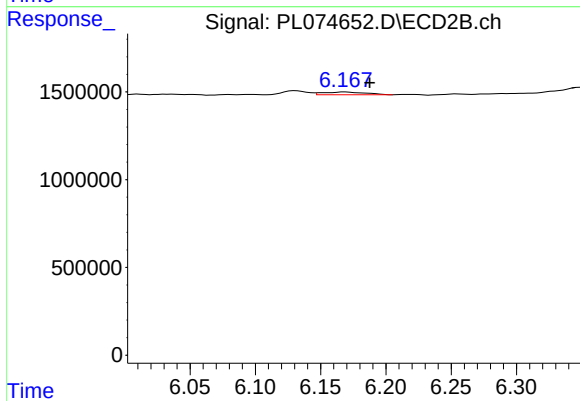

#4 Heptachlor


R.T.: 6.169 min
Delta R.T.: -0.019 min
Response: 353199
Conc: 0.23 ng/ml

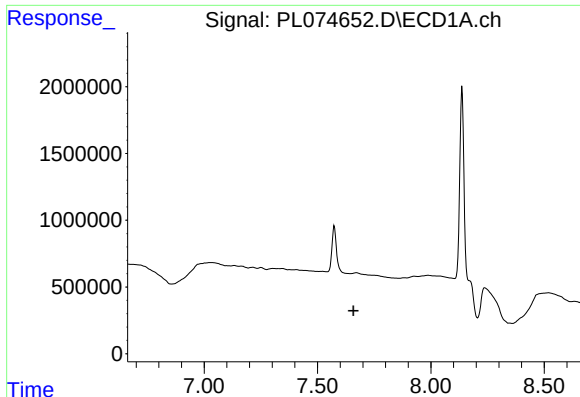

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 7.659 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

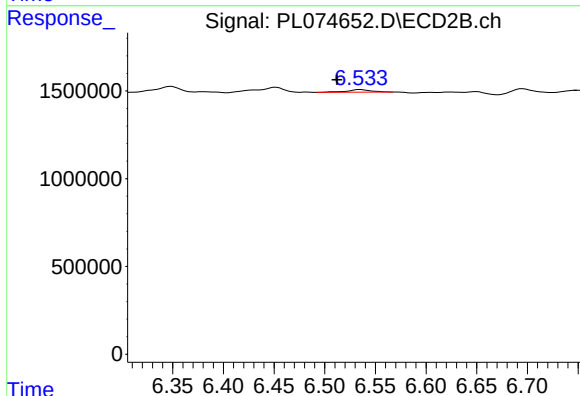


#5 Aldrin

R.T.: 6.535 min
Delta R.T.: 0.023 min
Response: 229395
Conc: 0.15 ng/ml

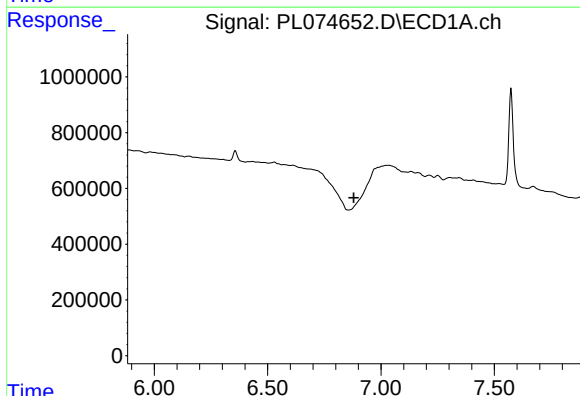


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 6.881 min
Response: 0
Conc: N.D.

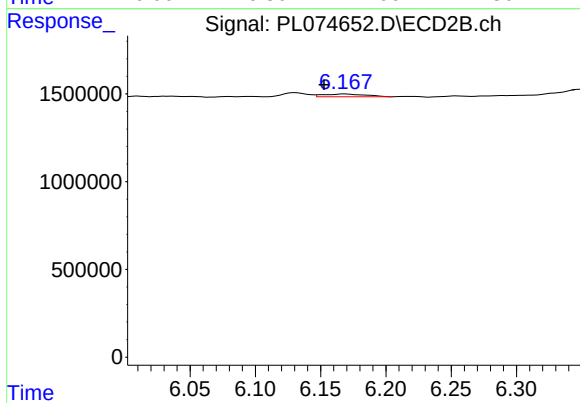

#6 beta-BHC


R.T.: 6.169 min
Delta R.T.: 0.016 min
Response: 353199
Conc: 0.44 ng/ml

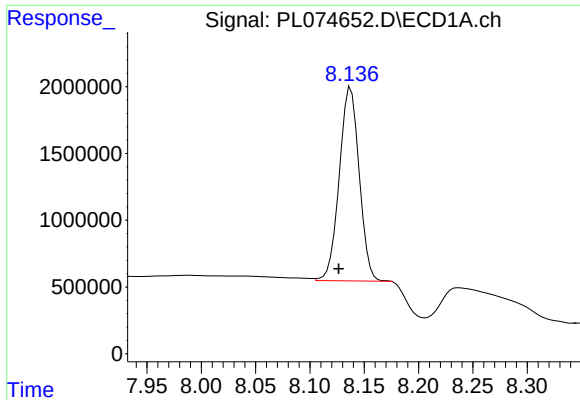

#8 Heptachlor epoxide


R.T.: 8.138 min
Delta R.T.: 0.011 min
Response: 18477228
Conc: 32.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

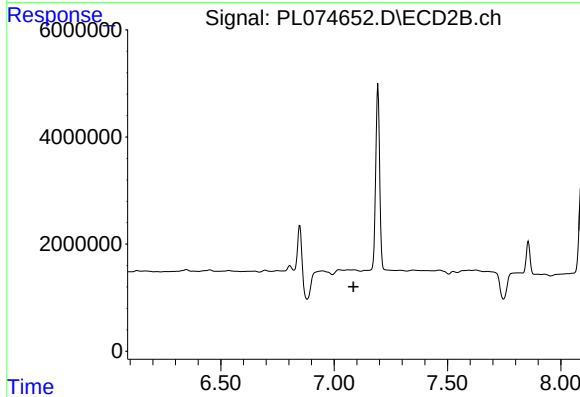


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.086 min
Response: 0
Conc: N.D.

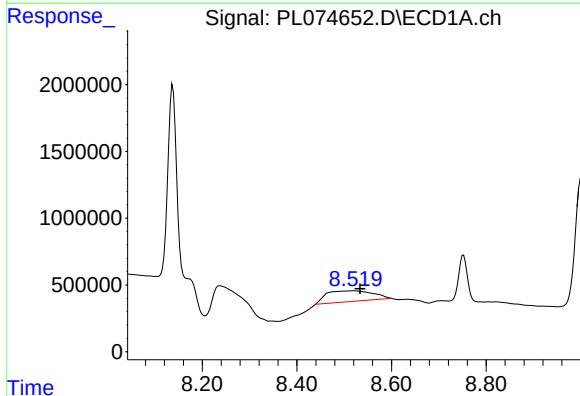


#9 Endosulfan I

R.T.: 8.520 min
Delta R.T.: -0.013 min
Response: 5604749
Conc: 9.72 ng/ml

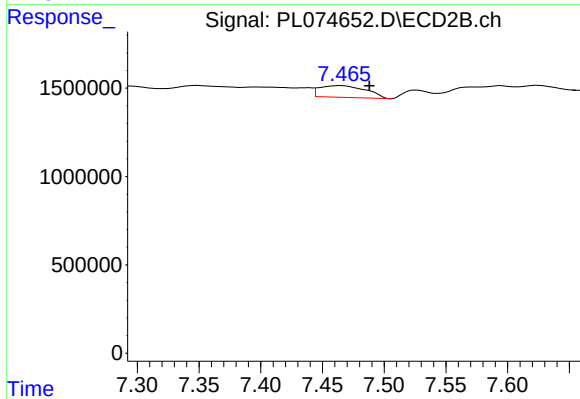

#9 Endosulfan I


R.T.: 7.466 min
Delta R.T.: -0.022 min
Response: 1721011
Conc: 1.38 ng/ml

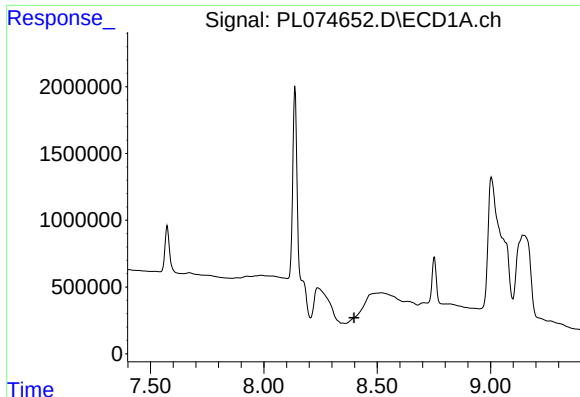

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

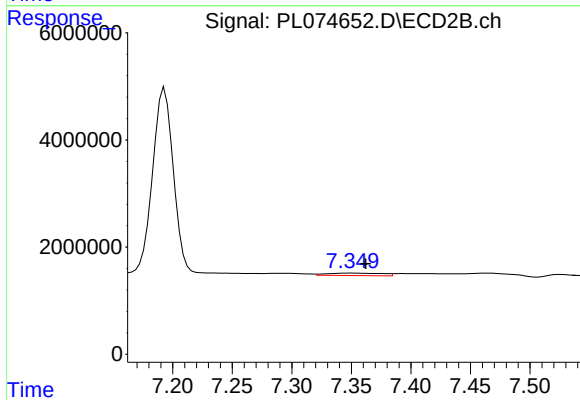


#10 gamma-Chlordane

R.T.: 7.349 min
Delta R.T.: -0.013 min
Response: 1456483
Conc: 1.05 ng/ml

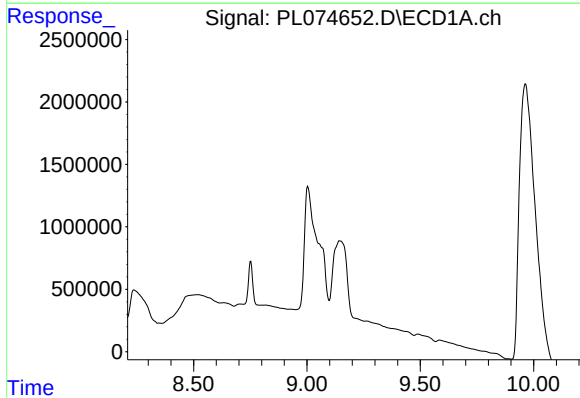


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 9.206 min
Response: 0
Conc: N.D.

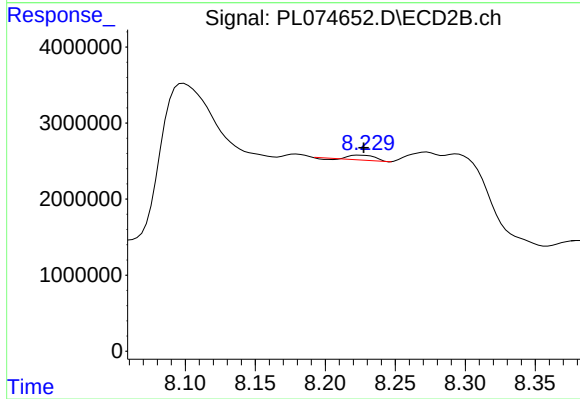

#16 4,4'-DDD


R.T.: 8.225 min
Delta R.T.: -0.003 min
Response: 728432
Conc: 0.74 ng/ml

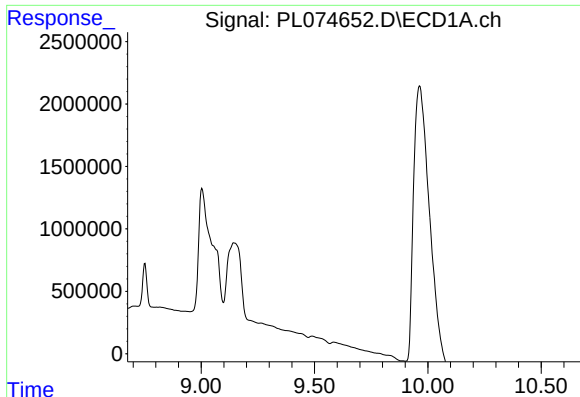

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 9.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

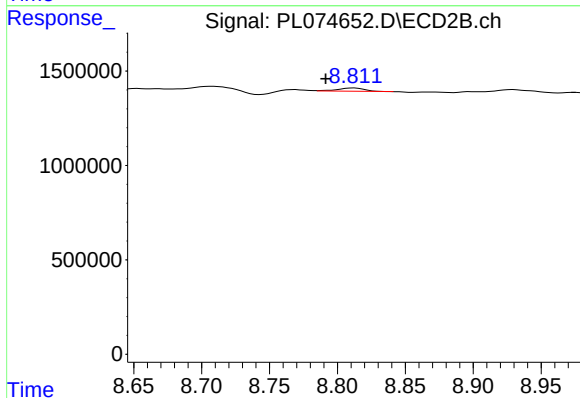


#19 Endosulfan Sulfate

R.T.: 8.813 min
Delta R.T.: 0.021 min
Response: 228557
Conc: 0.21 ng/ml

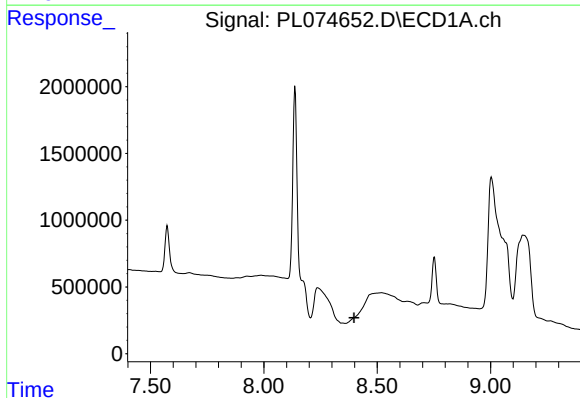


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 8.398 min
Response: 0
Conc: N.D.

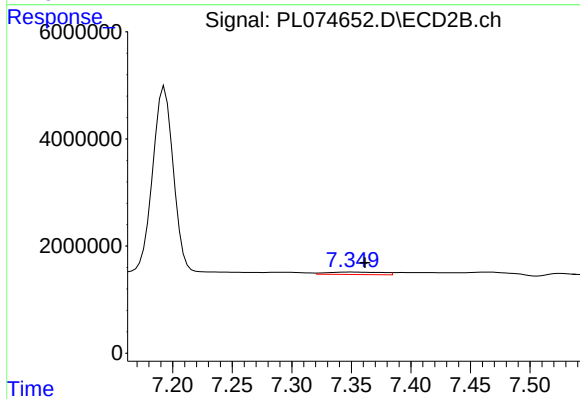

#25 Chlordane-3


R.T.: 7.349 min
Delta R.T.: -0.013 min
Response: 1456483
Conc: 11.22 ng/ml

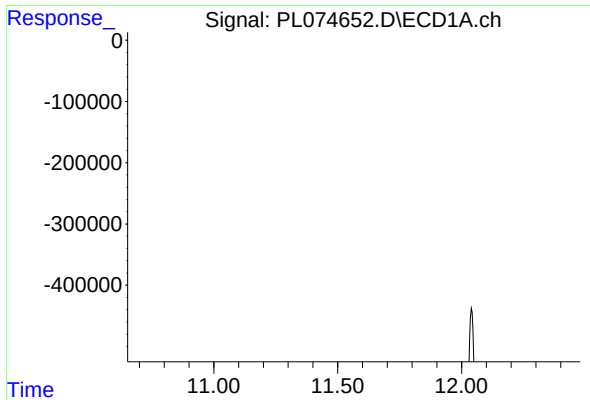

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 11.650 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

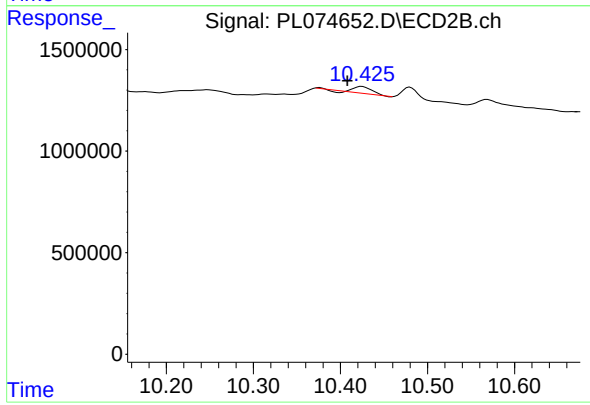

#28 Decachlorobiphenyl

R.T.: 10.425 min
Delta R.T.: 0.017 min
Response: 381591
Conc: 0.37 ng/ml