

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051222\
 Data File : PL074660.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2022 11:57
 Operator : AR\AJ
 Sample : N2749-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 03:07:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 16:19:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.647	4.652	5410917	13241192	10.657	9.647
28)	SA Decachlor...	11.647	10.403	7144766	16269609	15.999	15.851
Target Compounds							
6)	B beta-BHC	0.000	6.127f	0	418711	N.D.	0.527 #
8)	B Heptachlo...	8.129	7.074	2507698	205374	4.409	0.148 #
9)	A Endosulfan I	8.521	0.000	5218237	0	9.052	N.D. #
10)	B gamma-Chl...	8.372f	7.342f	88096	631810	0.170	0.456 #
12)	B 4,4'-DDE	8.662	7.641	260218	536627	0.562	0.456
13)	MA Dieldrin	8.817	7.778	400230	2454821	0.761	1.927 #
14)	MA Endrin	9.059	8.083f	909245	5923210	2.203	5.607 #
15)	B Endosulfa...	0.000	8.361	0	1276266	N.D.	1.130 #
16)	A 4,4'-DDD	9.206	0.000	1706907	0	3.775	N.D. #
17)	MA 4,4'-DDT	0.000	8.479	0	3234970	N.D.	3.233 #
19)	B Endosulfa...	0.000	8.790	0	1048477	N.D.	0.963 #
21)	B Endrin ke...	0.000	9.340f	0	438923	N.D.	0.394 #
23)	Chlordane-1	0.000	5.960f	0	231473	N.D.	5.107 #
25)	Chlordane-3	8.372f	7.342f	88096	631810	1.287	4.868 #
27)	Chlordane-5	0.000	8.141	0	2114695	N.D.	57.194 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051222\
Data File : PL074660.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2022 11:57
Operator : AR\AJ
Sample : N2749-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 03:07:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 16:19:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

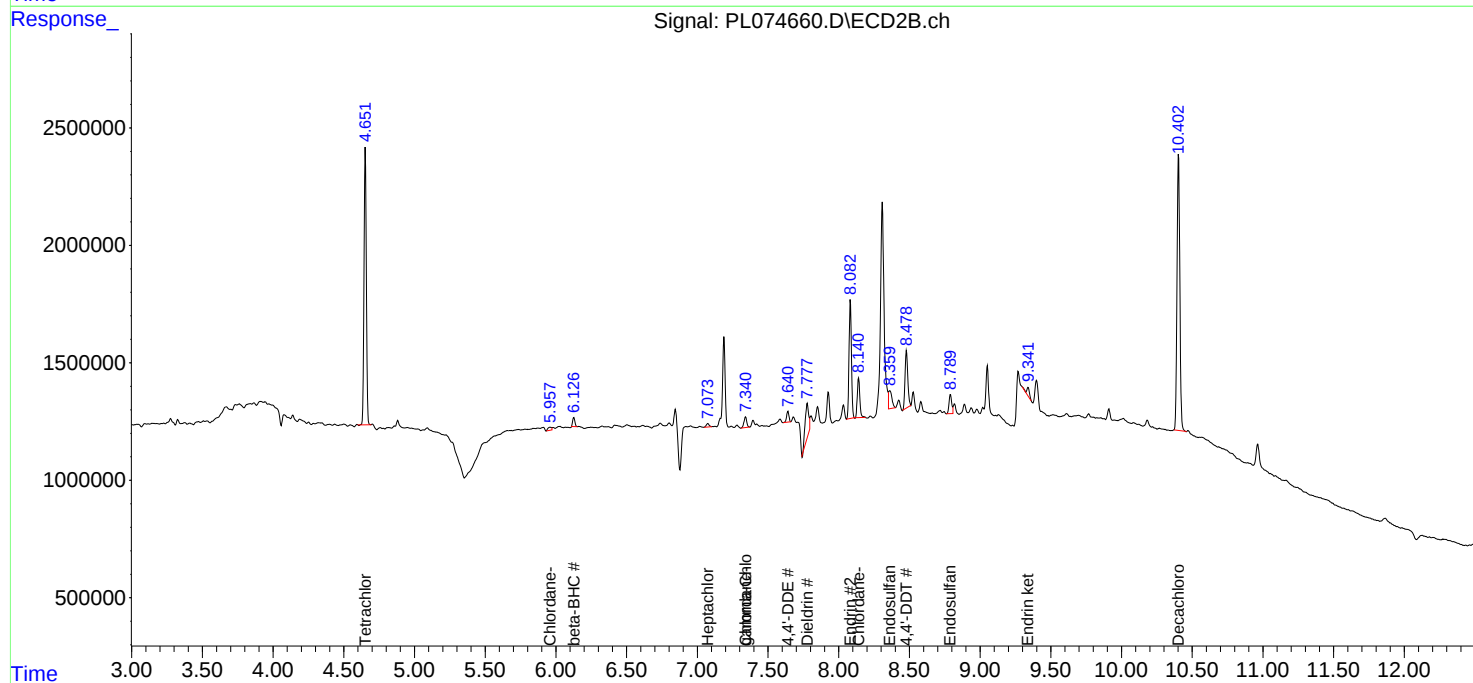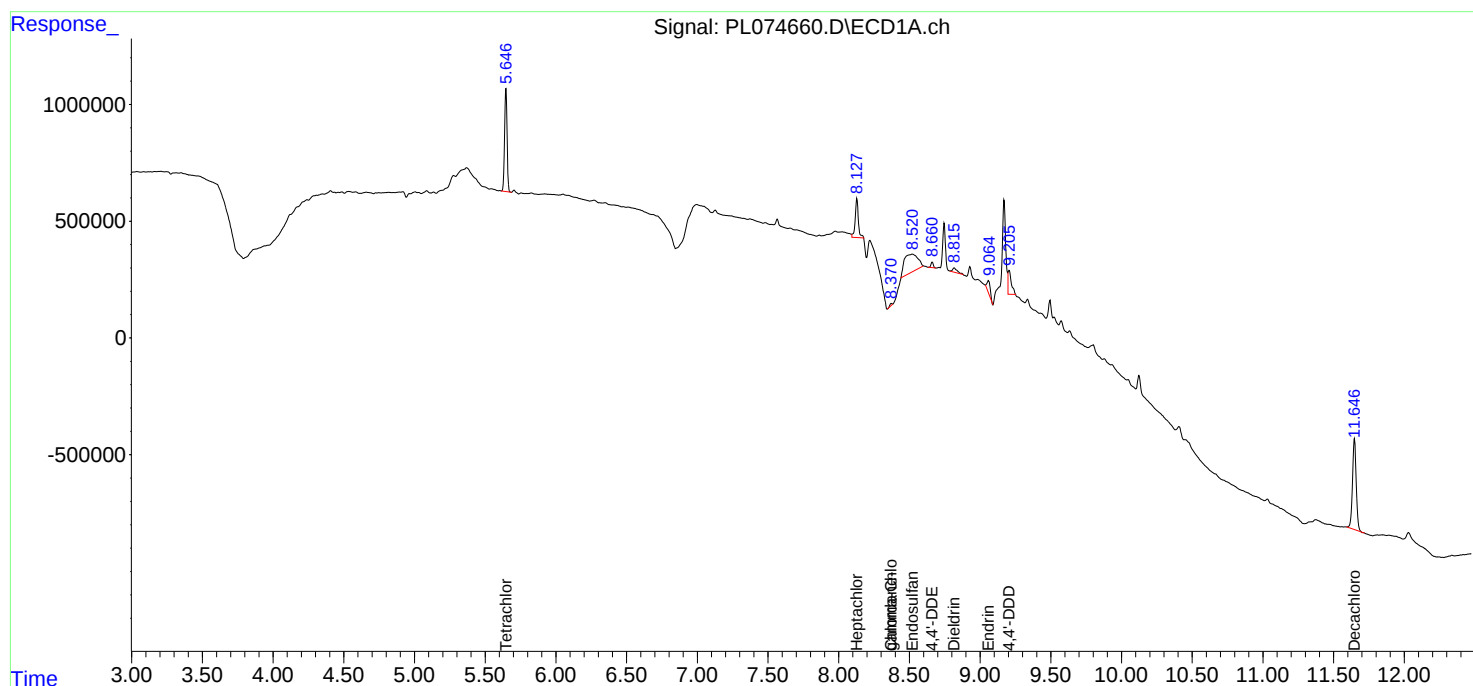


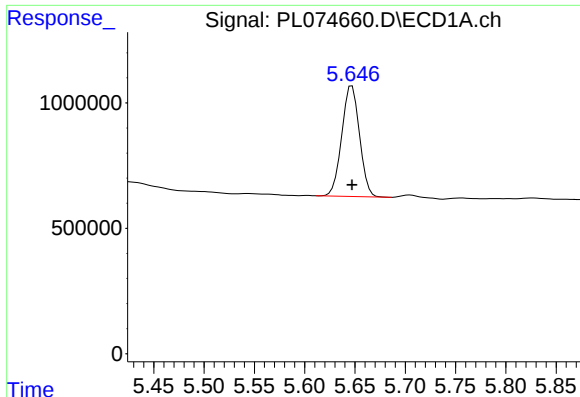

#1 Tetrachloro-m-xylene


R.T.: 5.647 min
Delta R.T.: 0.000 min
Response: 5410917
Conc: 10.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

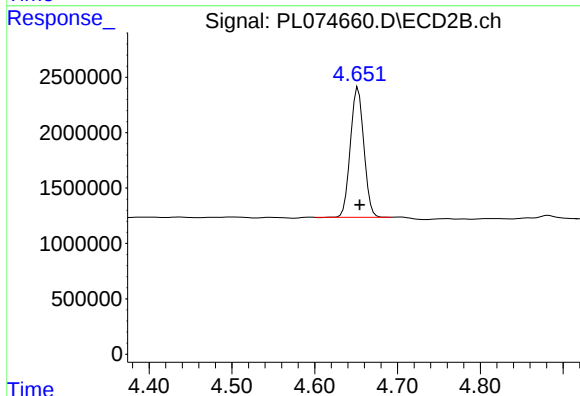


#1 Tetrachloro-m-xylene

R.T.: 4.652 min
Delta R.T.: -0.002 min
Response: 13241192
Conc: 9.65 ng/ml

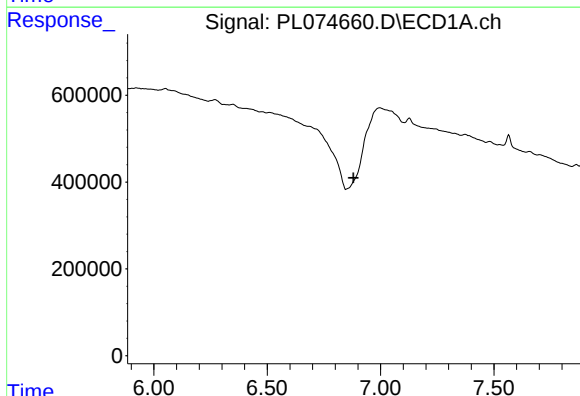


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.881 min
Response: 0
Conc: N.D.

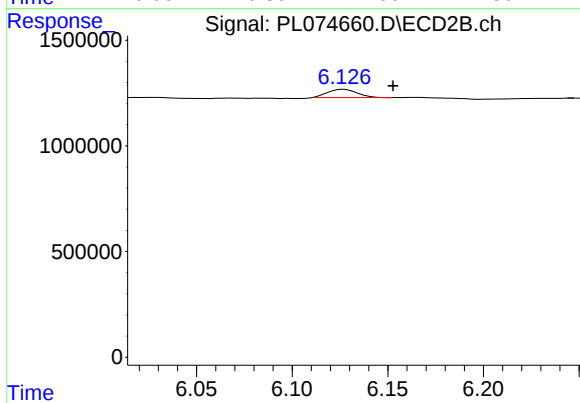

#6 beta-BHC


R.T.: 6.127 min
Delta R.T.: -0.025 min
Response: 418711
Conc: 0.53 ng/ml

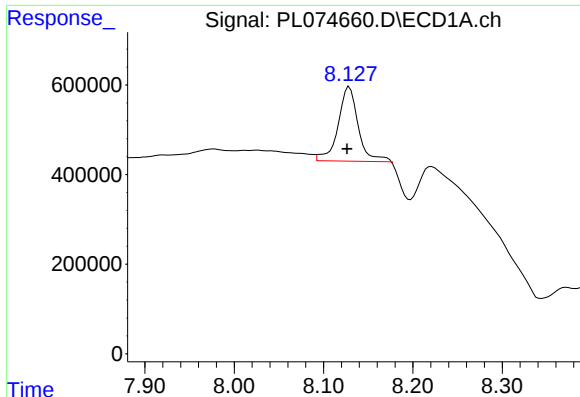

#8 Heptachlor epoxide


R.T.: 8.129 min
Delta R.T.: 0.002 min
Response: 2507698
Conc: 4.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

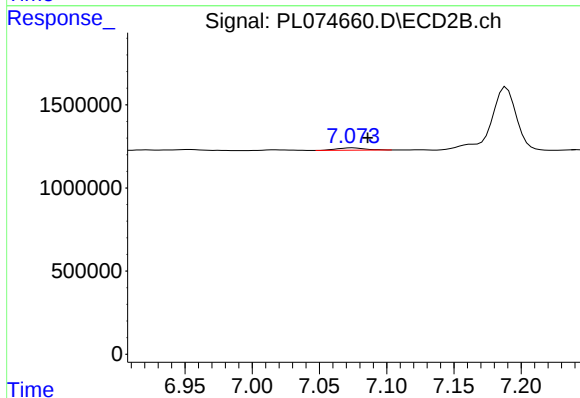


#8 Heptachlor epoxide

R.T.: 7.074 min
Delta R.T.: -0.011 min
Response: 205374
Conc: 0.15 ng/ml

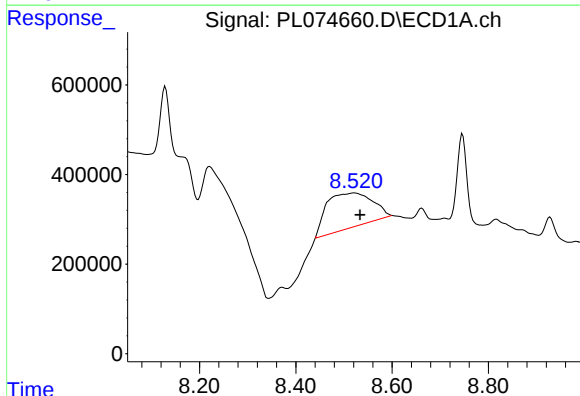


#9 Endosulfan I

R.T.: 8.521 min
Delta R.T.: -0.012 min
Response: 5218237
Conc: 9.05 ng/ml

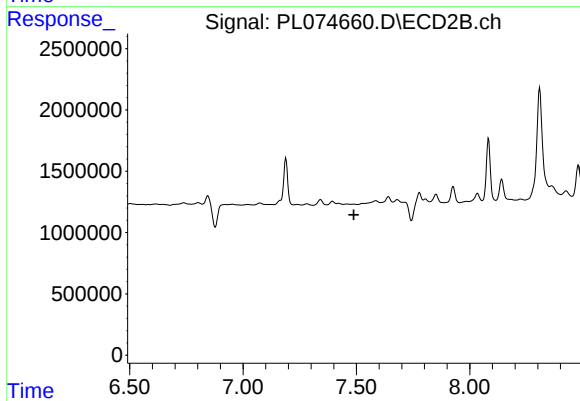

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 7.488 min
Response: 0
Conc: N.D.

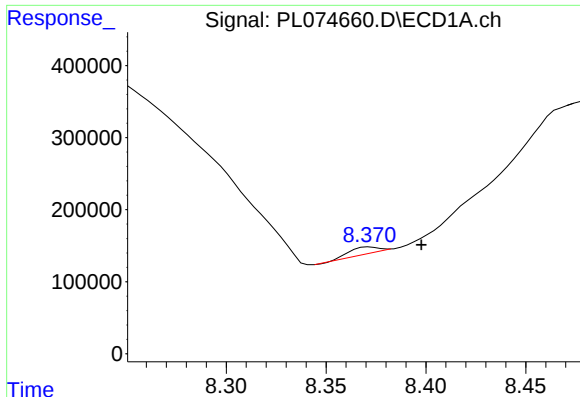

#10 gamma-Chlordane


R.T.: 8.372 min
Delta R.T.: -0.026 min
Response: 88096
Conc: 0.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

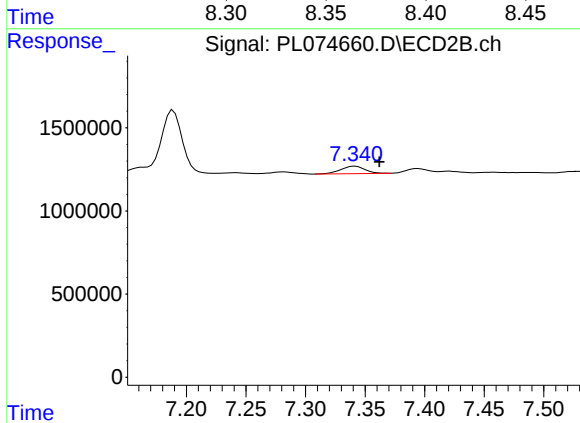


#10 gamma-Chlordane

R.T.: 7.342 min
Delta R.T.: -0.020 min
Response: 631810
Conc: 0.46 ng/ml

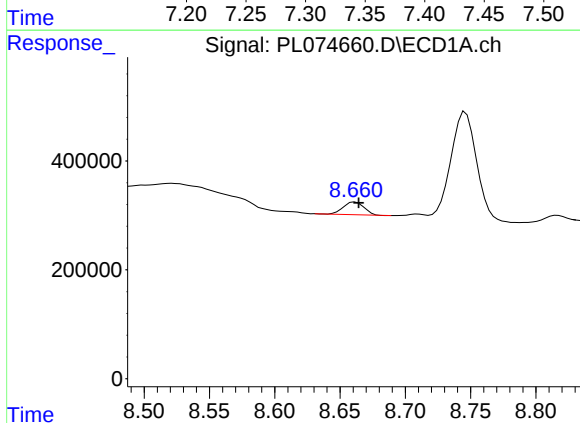


#12 4,4'-DDE

R.T.: 8.662 min
Delta R.T.: -0.003 min
Response: 260218
Conc: 0.56 ng/ml

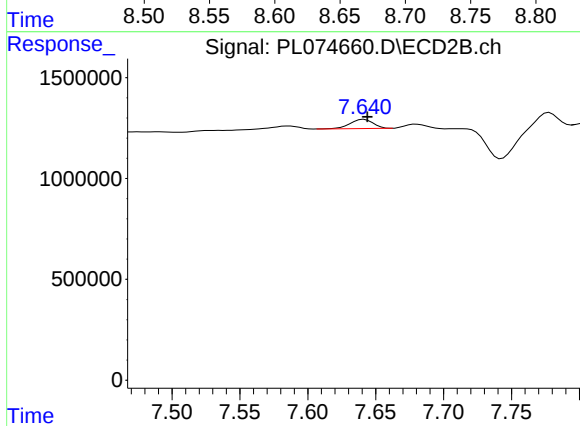

#12 4,4'-DDE


R.T.: 7.641 min
Delta R.T.: -0.003 min
Response: 536627
Conc: 0.46 ng/ml

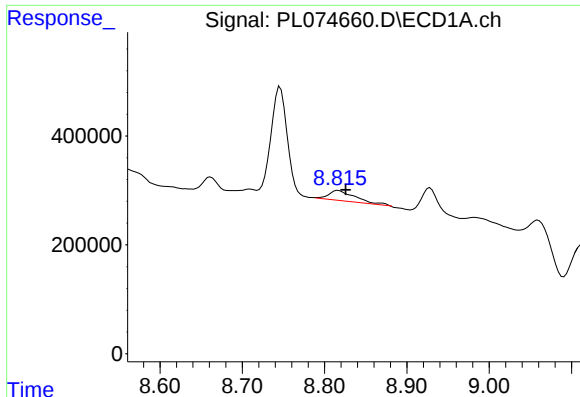

#13 Dieldrin


R.T.: 8.817 min
Delta R.T.: -0.009 min
Response: 400230
Conc: 0.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

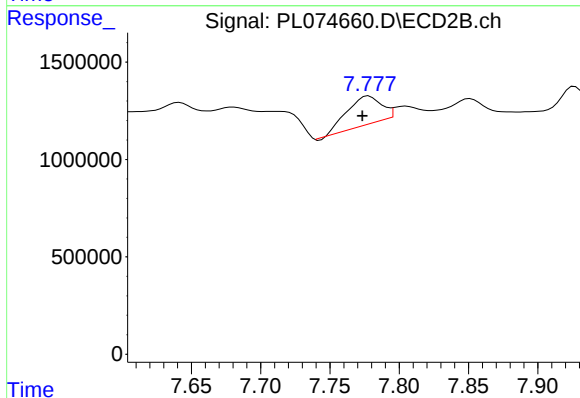


#13 Dieldrin

R.T.: 7.778 min
Delta R.T.: 0.005 min
Response: 2454821
Conc: 1.93 ng/ml

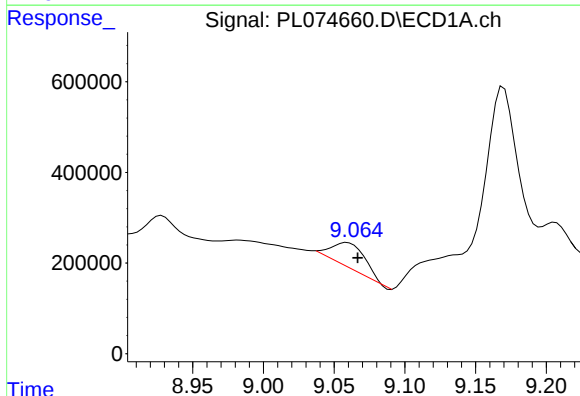


#14 Endrin

R.T.: 9.059 min
Delta R.T.: -0.007 min
Response: 909245
Conc: 2.20 ng/ml

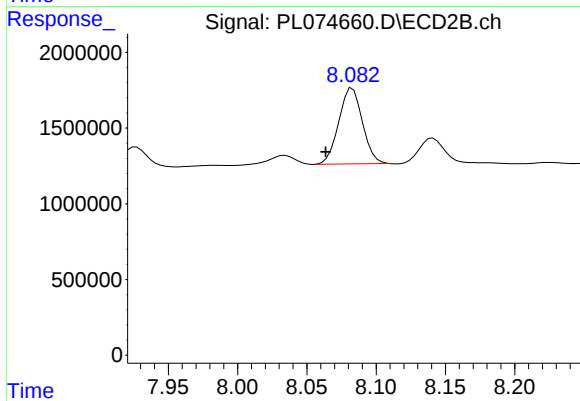

#14 Endrin


R.T.: 8.083 min
Delta R.T.: 0.019 min
Response: 5923210
Conc: 5.61 ng/ml

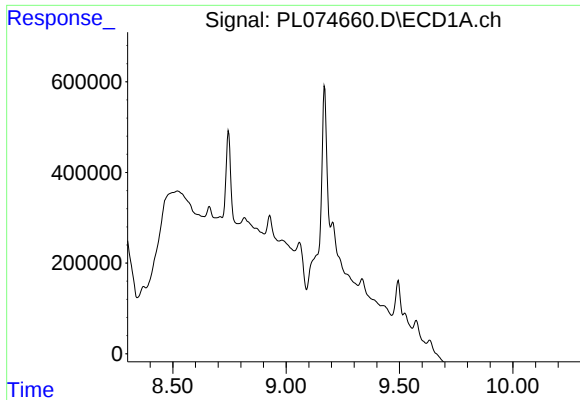

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 9.301 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

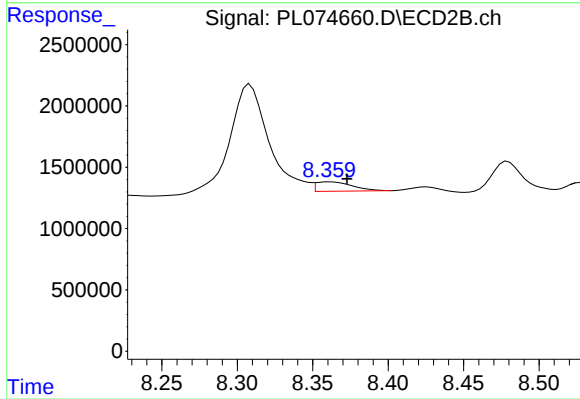


#15 Endosulfan II

R.T.: 8.361 min
Delta R.T.: -0.011 min
Response: 1276266
Conc: 1.13 ng/ml

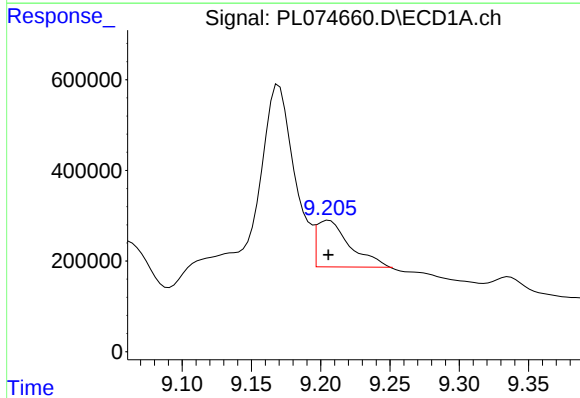


#16 4,4'-DDD

R.T.: 9.206 min
Delta R.T.: 0.000 min
Response: 1706907
Conc: 3.78 ng/ml

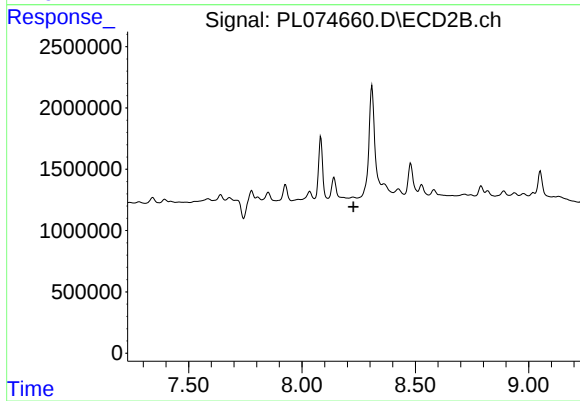

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.227 min
Response: 0
Conc: N.D.

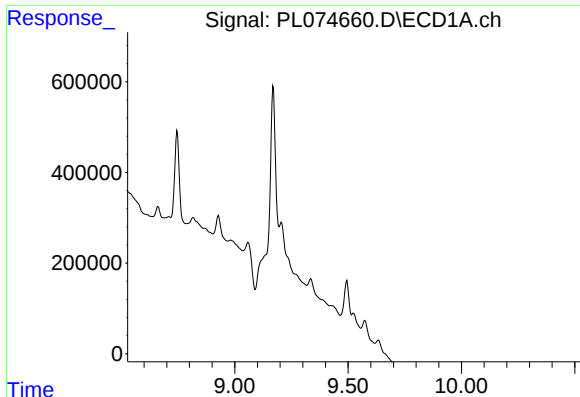

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.526 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

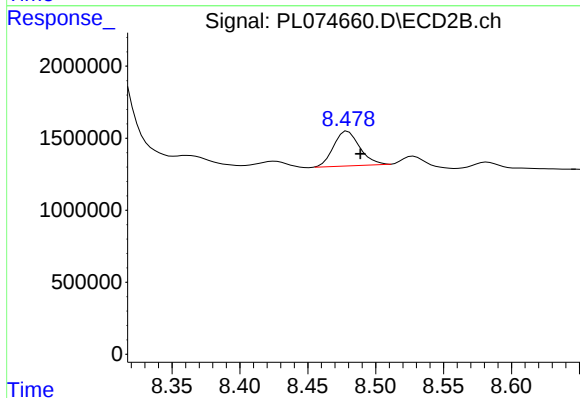


#17 4,4'-DDT

R.T.: 8.479 min
Delta R.T.: -0.009 min
Response: 3234970
Conc: 3.23 ng/ml

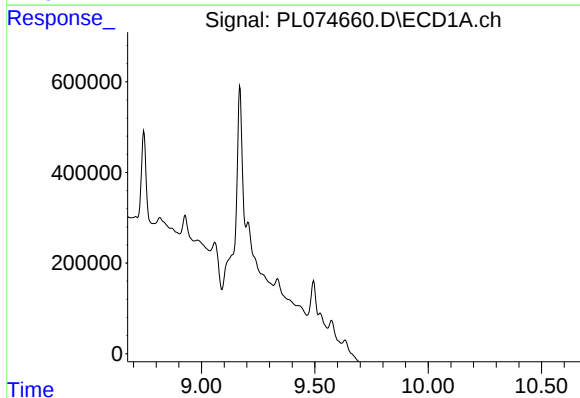


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 9.674 min
Response: 0
Conc: N.D.

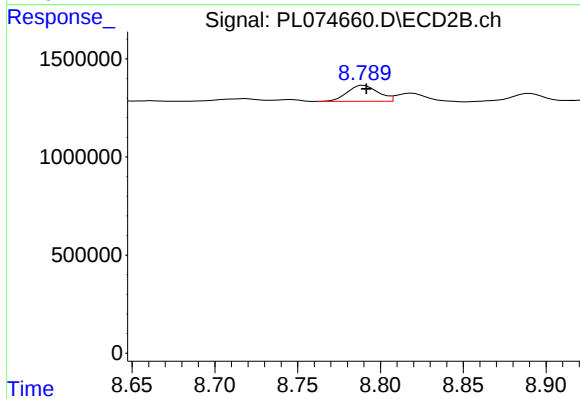

#19 Endosulfan Sulfate


R.T.: 8.790 min
Delta R.T.: -0.001 min
Response: 1048477
Conc: 0.96 ng/ml

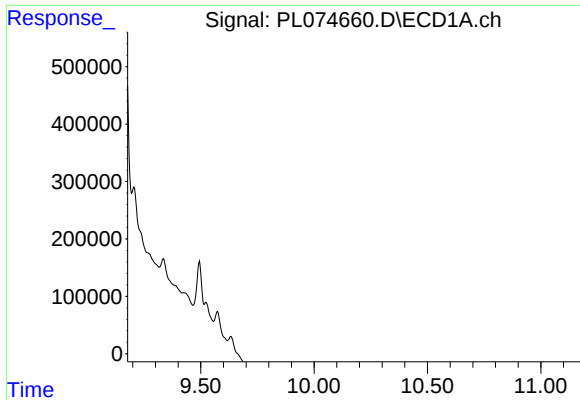

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 10.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

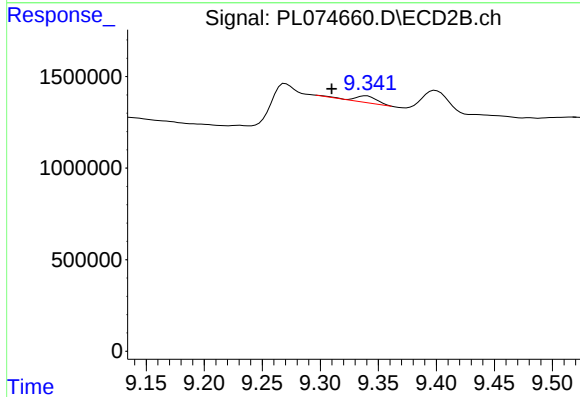


#21 Endrin ketone

R.T.: 9.340 min
Delta R.T.: 0.030 min
Response: 438923
Conc: 0.39 ng/ml

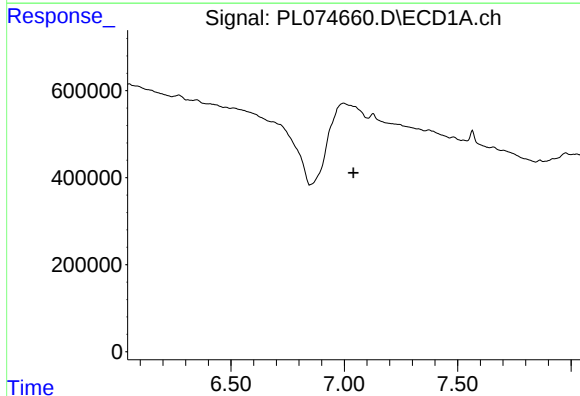


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 7.041 min
Response: 0
Conc: N.D.

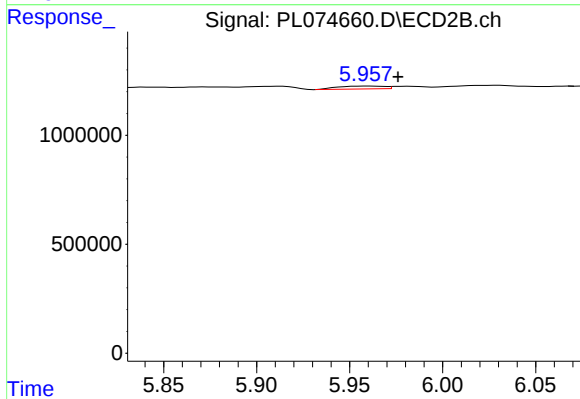

#23 Chlordane-1


R.T.: 5.960 min
Delta R.T.: -0.016 min
Response: 231473
Conc: 5.11 ng/ml

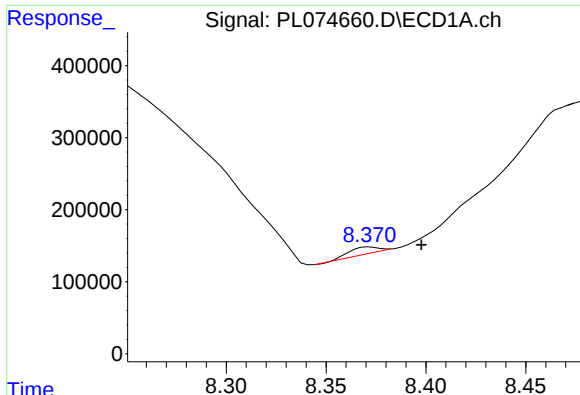

#25 Chlordane-3


R.T.: 8.372 min
Delta R.T.: -0.026 min
Response: 88096
Conc: 1.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

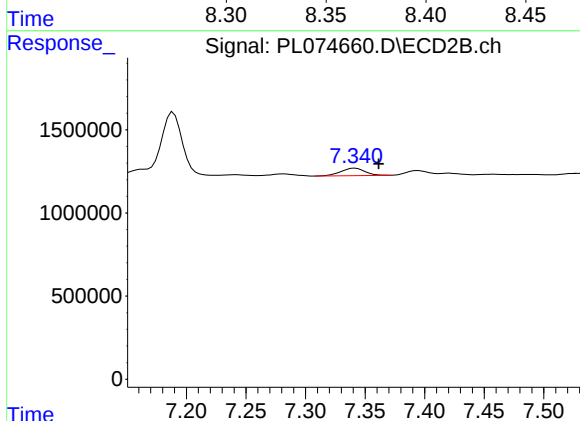


#25 Chlordane-3

R.T.: 7.342 min
Delta R.T.: -0.020 min
Response: 631810
Conc: 4.87 ng/ml

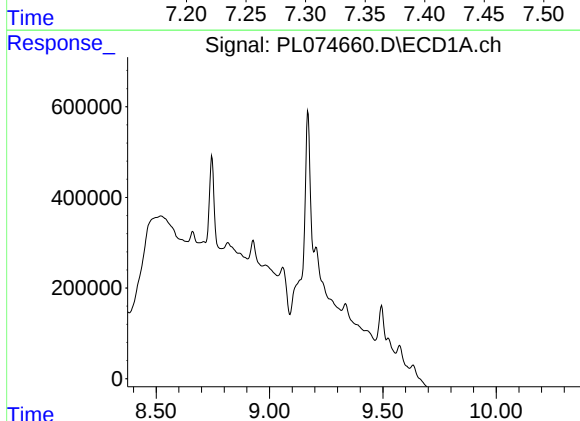


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.371 min
Response: 0
Conc: N.D.

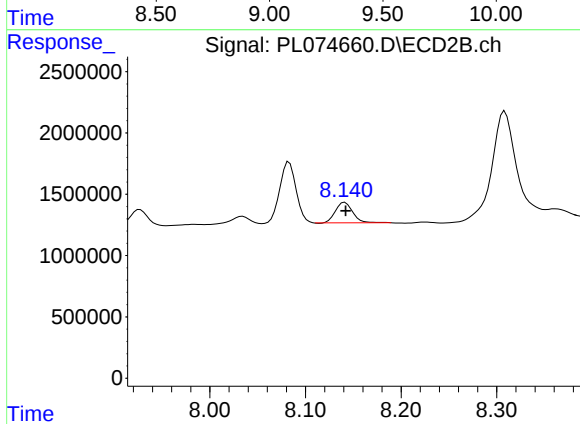

#27 Chlordane-5


R.T.: 8.141 min
Delta R.T.: -0.001 min
Response: 2114695
Conc: 57.19 ng/ml

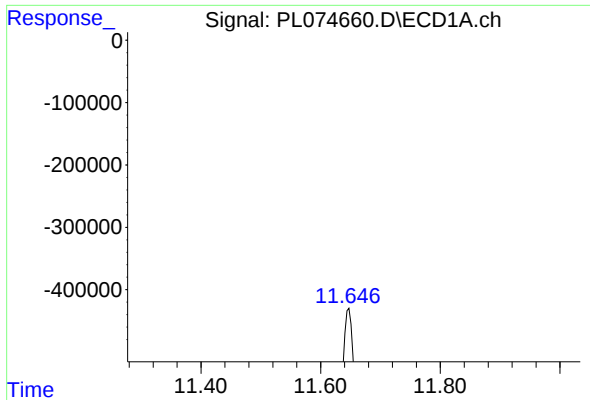

#28 Decachlorobiphenyl

R.T.: 11.647 min
Delta R.T.: -0.002 min
Response: 7144766
Conc: 16.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

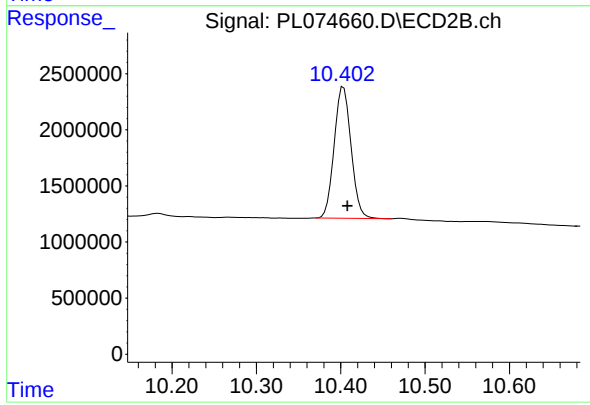

#28 Decachlorobiphenyl

R.T.: 10.403 min
Delta R.T.: -0.005 min
Response: 16269609
Conc: 15.85 ng/ml