

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051222\
 Data File : PL074662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2022 12:30
 Operator : AR\AJ
 Sample : N2749-04DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 03:08:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 16:19:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.647	4.652	1151853	3261635	2.269	2.376
28)	SA Decachlor...	11.647	10.404	1322702	3174846	2.962	3.093
Target Compounds							
6)	B beta-BHC	0.000	6.128f	0	378346	N.D.	0.477 #
7)	B delta-BHC	0.000	6.430f	0	417080	N.D.	0.267 #
8)	B Heptachlo...	8.129	0.000	499549	0	0.878	N.D. #
9)	A Endosulfan I	8.519	0.000	5218275	0	9.052	N.D. #
13)	MA Dieldrin	0.000	7.778	0	436572	N.D.	0.343 #
14)	MA Endrin	0.000	8.083f	0	1116028	N.D.	1.057 #
17)	MA 4,4'-DDT	0.000	8.481	0	536114	N.D.	0.536 #
19)	B Endosulfa...	0.000	8.791	0	205103	N.D.	0.188 #
23)	Chlordane-1	0.000	5.963	0	977709	N.D.	21.573 #
27)	Chlordane-5	0.000	8.142	0	483135	N.D.	13.067 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051222\
Data File : PL074662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2022 12:30
Operator : AR\AJ
Sample : N2749-04DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 03:08:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 16:19:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

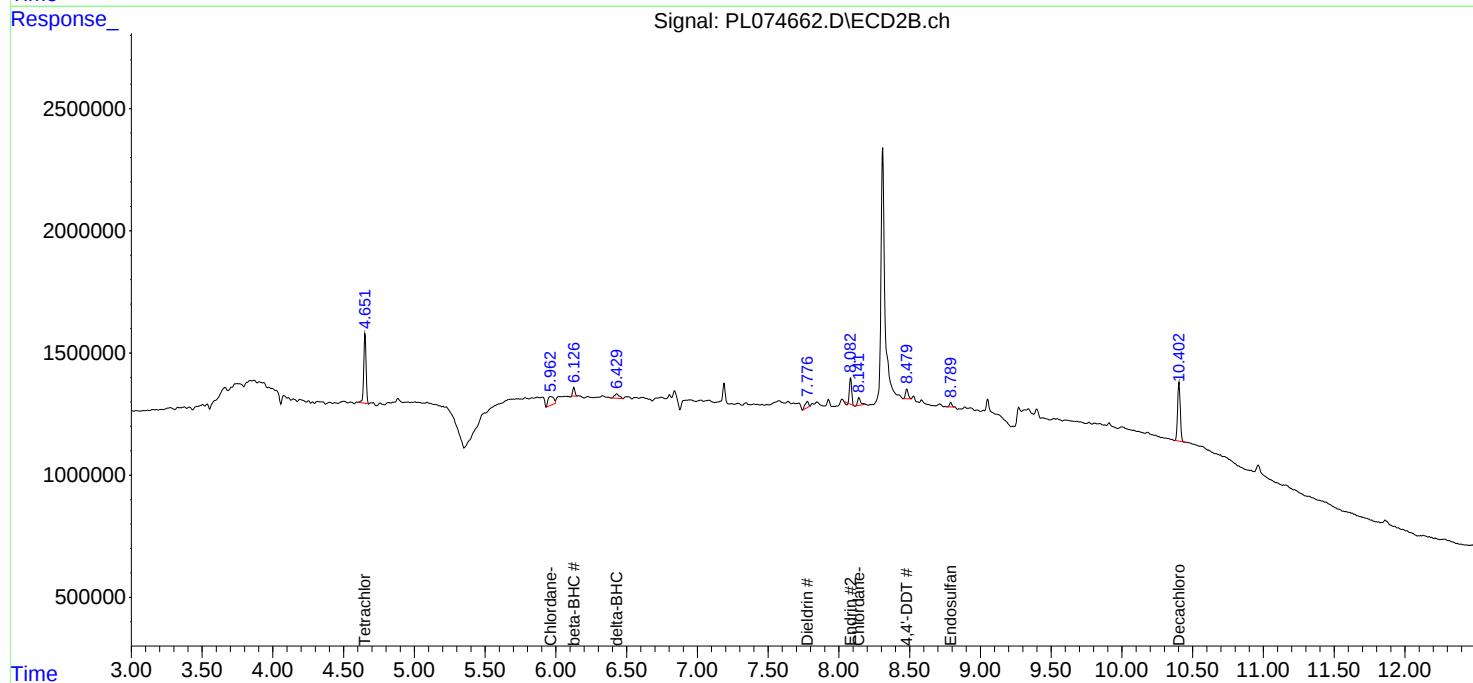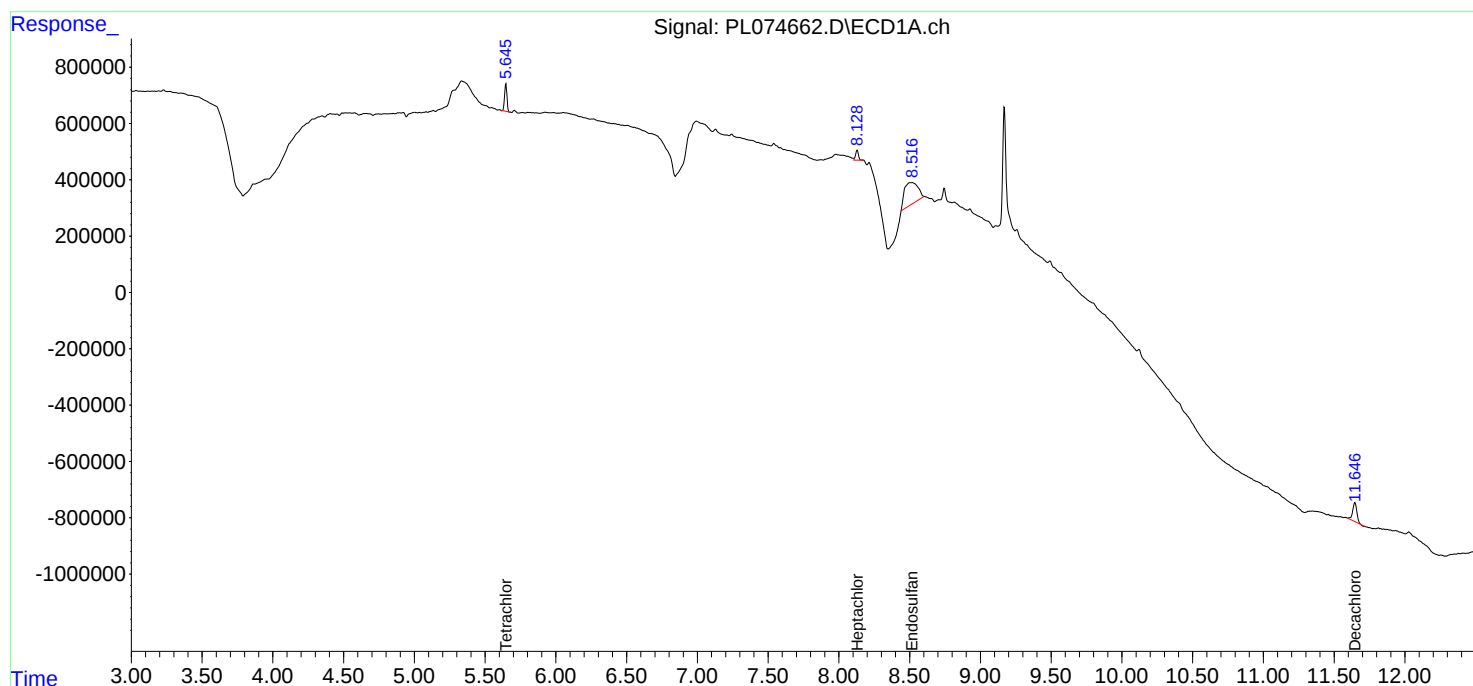


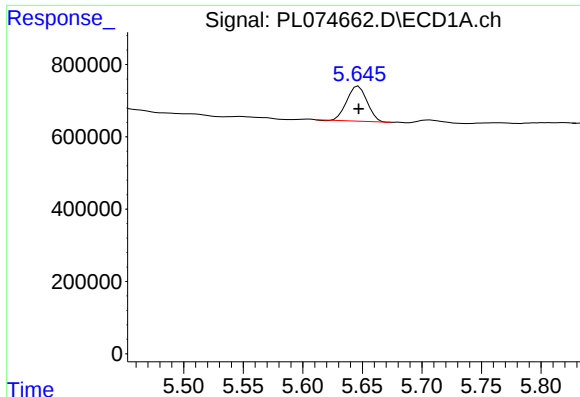

#1 Tetrachloro-m-xylene


R.T.: 5.647 min
Delta R.T.: 0.000 min
Response: 1151853
Conc: 2.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

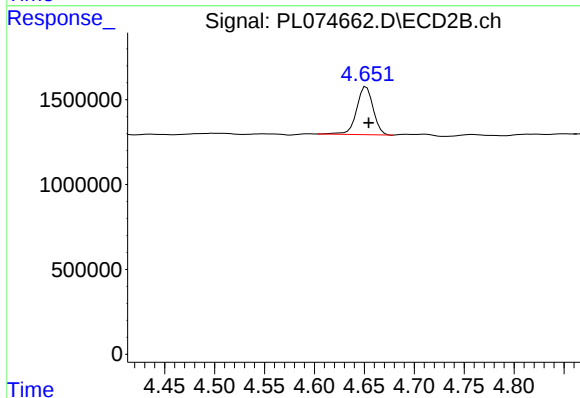


#1 Tetrachloro-m-xylene

R.T.: 4.652 min
Delta R.T.: -0.002 min
Response: 3261635
Conc: 2.38 ng/ml

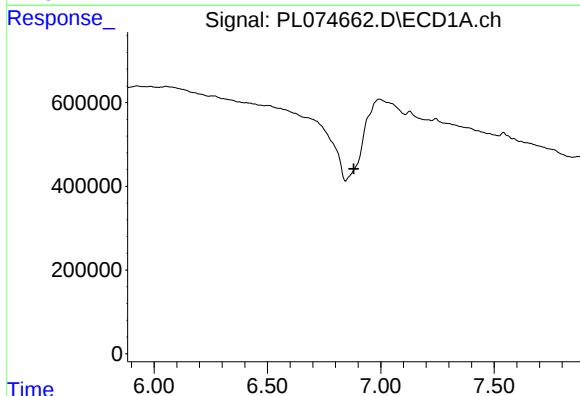


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.881 min
Response: 0
Conc: N.D.

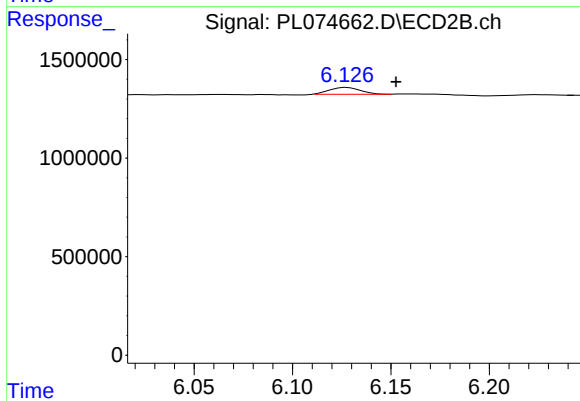

#6 beta-BHC


R.T.: 6.128 min
Delta R.T.: -0.025 min
Response: 378346
Conc: 0.48 ng/ml

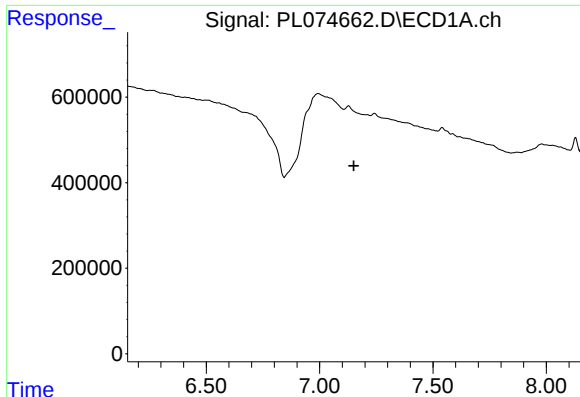

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

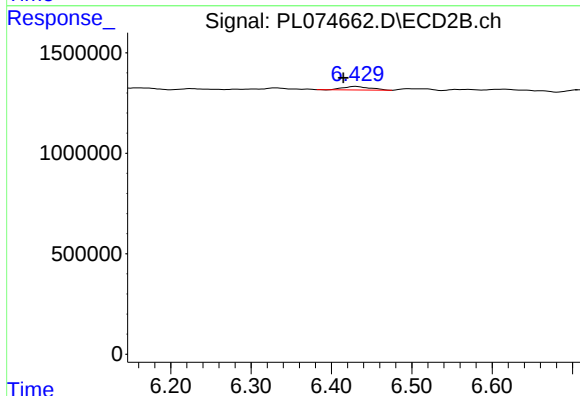


#7 delta-BHC

R.T.: 6.430 min
Delta R.T.: 0.016 min
Response: 417080
Conc: 0.27 ng/ml

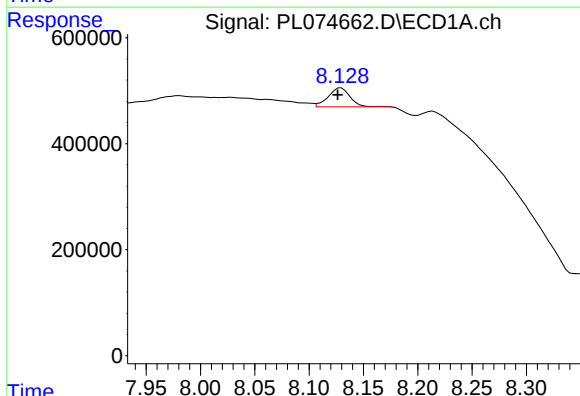


#8 Heptachlor epoxide

R.T.: 8.129 min
Delta R.T.: 0.003 min
Response: 499549
Conc: 0.88 ng/ml

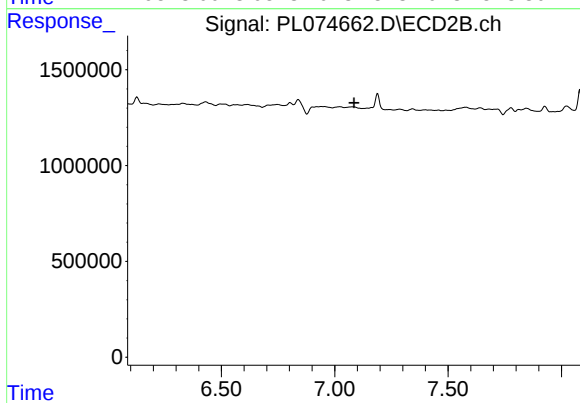

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.086 min
Response: 0
Conc: N.D.

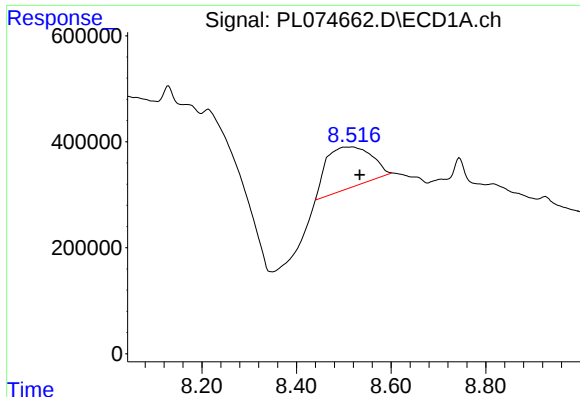

#9 Endosulfan I


R.T.: 8.519 min
Delta R.T.: -0.015 min
Response: 5218275
Conc: 9.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

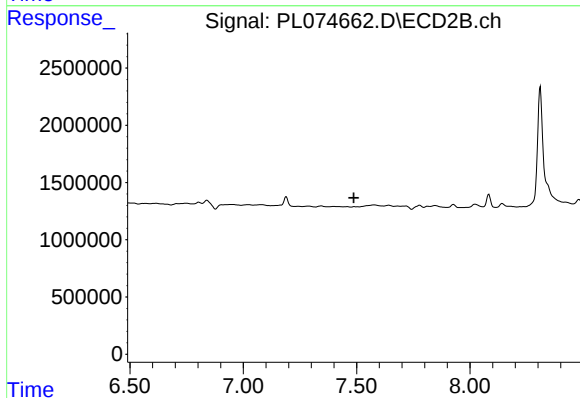


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.488 min
Response: 0
Conc: N.D.

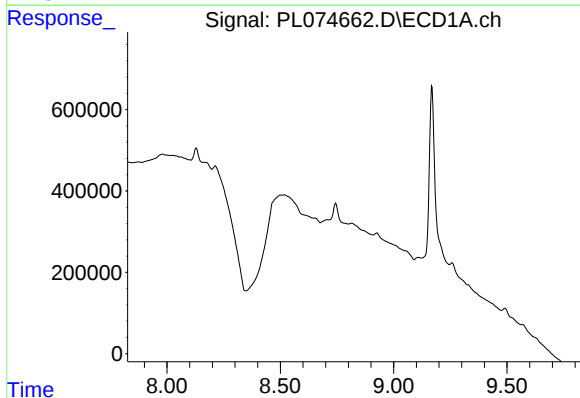


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.826 min
Response: 0
Conc: N.D.

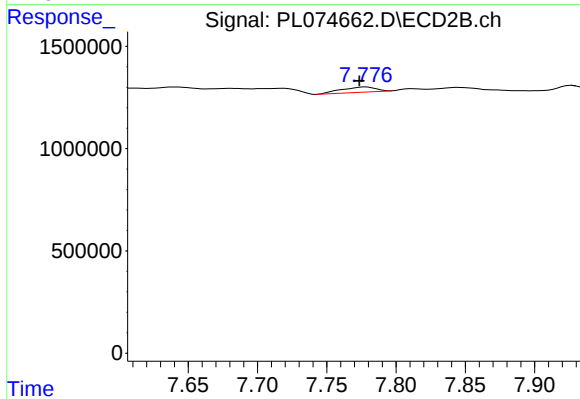

#13 Dieldrin


R.T.: 7.778 min
Delta R.T.: 0.005 min
Response: 436572
Conc: 0.34 ng/ml

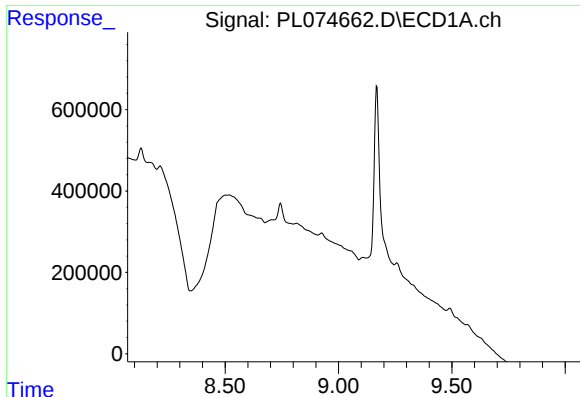

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.067 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

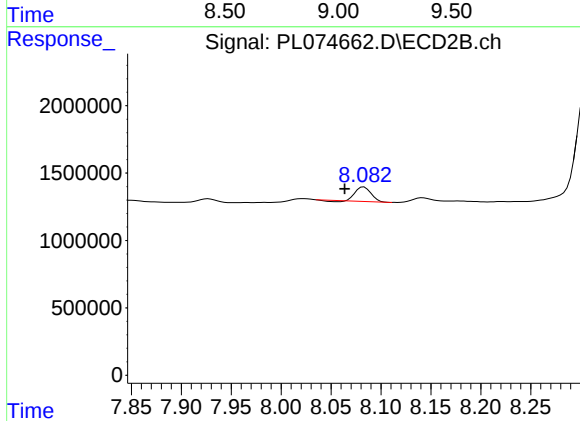


#14 Endrin

R.T.: 8.083 min
Delta R.T.: 0.019 min
Response: 1116028
Conc: 1.06 ng/ml

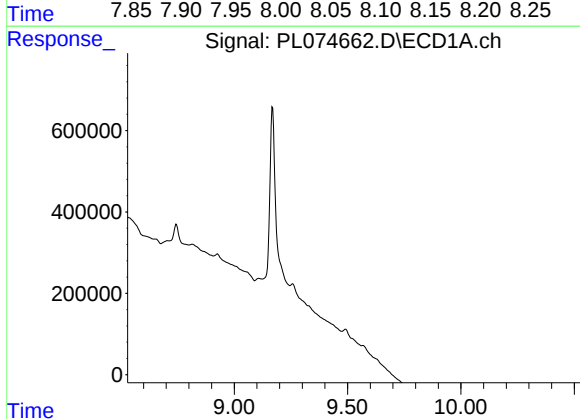


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 9.526 min
Response: 0
Conc: N.D.

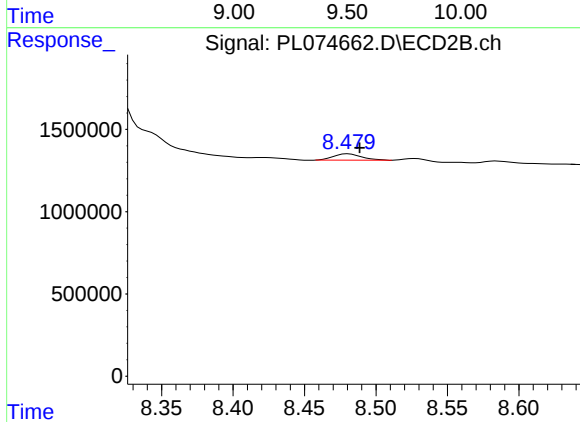

#17 4,4'-DDT


R.T.: 8.481 min
Delta R.T.: -0.008 min
Response: 536114
Conc: 0.54 ng/ml

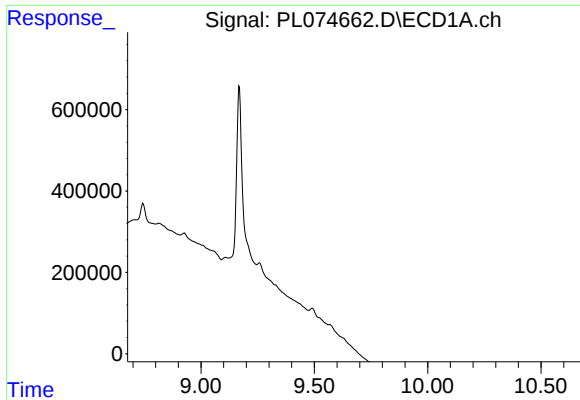

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 9.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

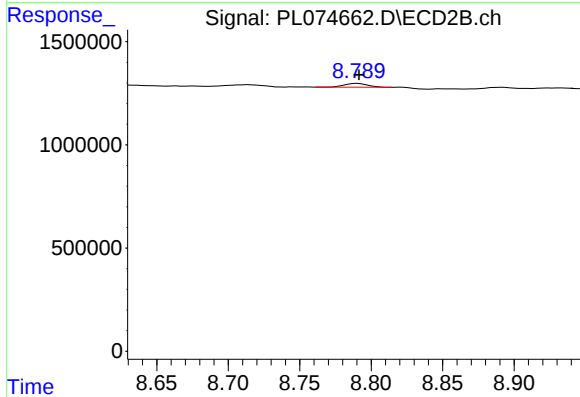


#19 Endosulfan Sulfate

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 205103
Conc: 0.19 ng/ml

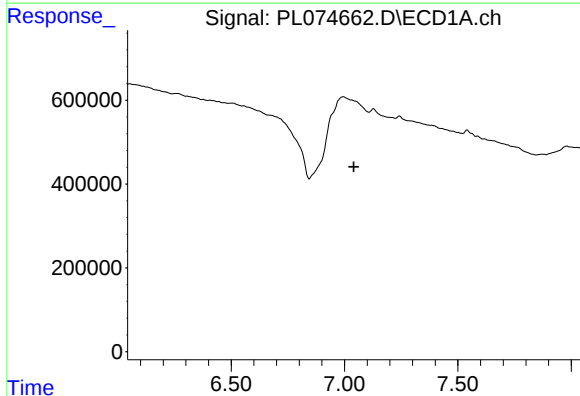


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

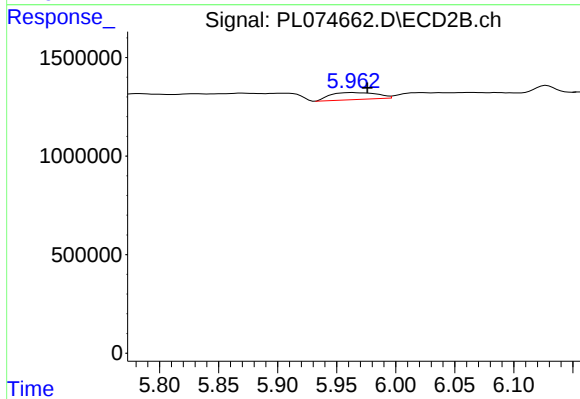

#23 Chlordane-1


R.T.: 5.963 min
Delta R.T.: -0.013 min
Response: 977709
Conc: 21.57 ng/ml

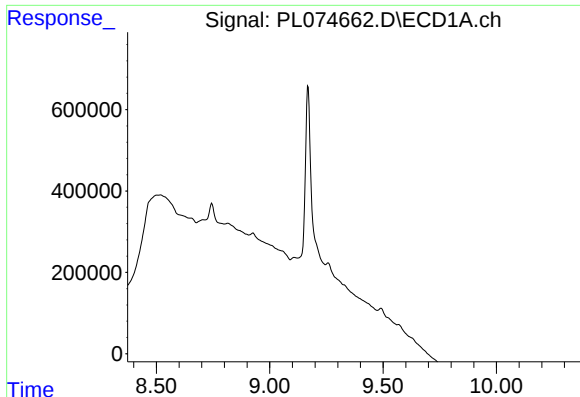

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.371 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

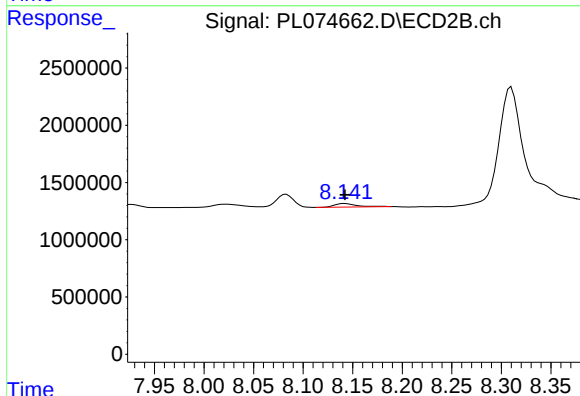


#27 Chlordane-5

R.T.: 8.142 min
Delta R.T.: 0.000 min
Response: 483135
Conc: 13.07 ng/ml

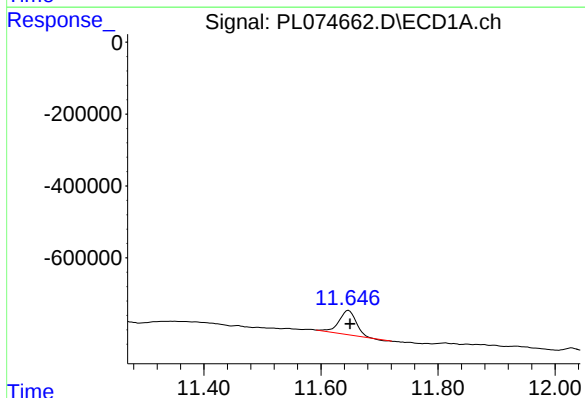

#28 Decachlorobiphenyl

R.T.: 11.647 min
Delta R.T.: -0.003 min
Response: 1322702
Conc: 2.96 ng/ml

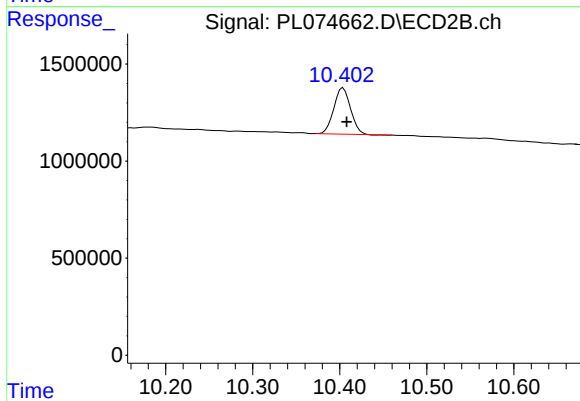

#28 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.004 min
Response: 3174846
Conc: 3.09 ng/ml