

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051222\
 Data File : PL074670.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2022 16:35
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 03:10:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 16:19:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.649	4.652	11828715	30662957	23.297	22.341
28)	SA Decachlor...	11.649	10.404	11748837	25951724	26.308	25.284
Target Compounds							
6)	B beta-BHC	0.000	6.127f	0	514942	N.D.	0.649 #
7)	B delta-BHC	0.000	6.413	0	438646	N.D.	0.281 #
9)	A Endosulfan I	8.528	7.484	5192699	113685	9.007	0.091 #
10)	B gamma-Chl...	0.000	7.360	0	210224	N.D.	0.152 #
11)	B alpha-Chl...	0.000	7.430	0	253184	N.D.	0.187 #
13)	MA Dieldrin	0.000	7.771	0	917036	N.D.	0.720 #
14)	MA Endrin	0.000	8.083f	0	685693	N.D.	0.649 #
18)	B Endrin al...	0.000	8.558	0	162098	N.D.	0.203 #
19)	B Endosulfa...	0.000	8.789	0	287160	N.D.	0.264 #
21)	B Endrin ke...	0.000	9.308	0	84605	N.D.	0.076 #
25)	Chlordane-3	0.000	7.360	0	210224	N.D.	1.620 #
26)	Chlordane-4	0.000	7.430	0	253184	N.D.	1.847 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051222\
Data File : PL074670.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2022 16:35
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 03:10:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 16:19:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

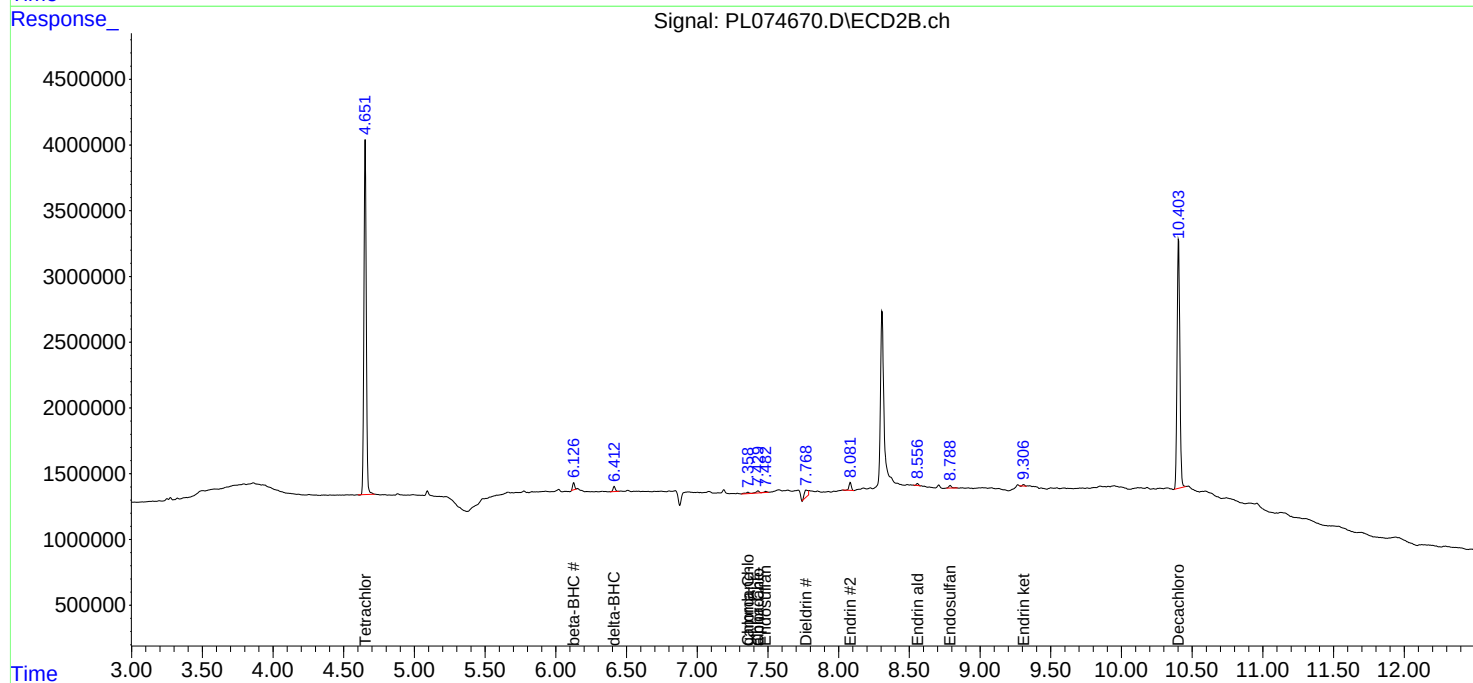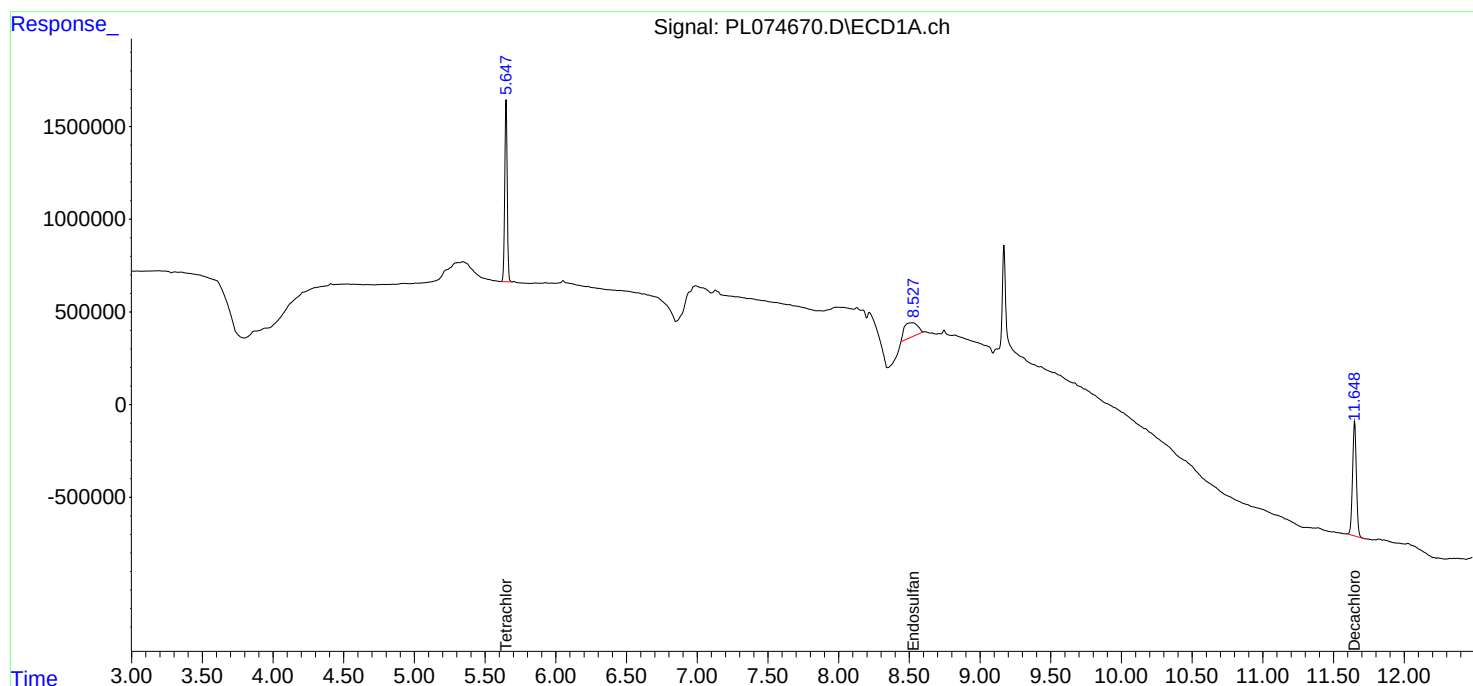


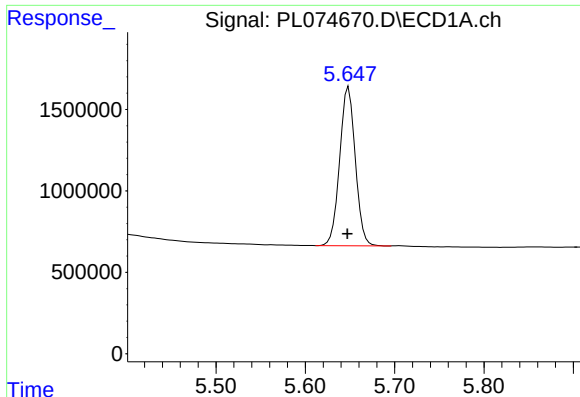

#1 Tetrachloro-m-xylene


R.T.: 5.649 min
Delta R.T.: 0.002 min
Response: 11828715
Conc: 23.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

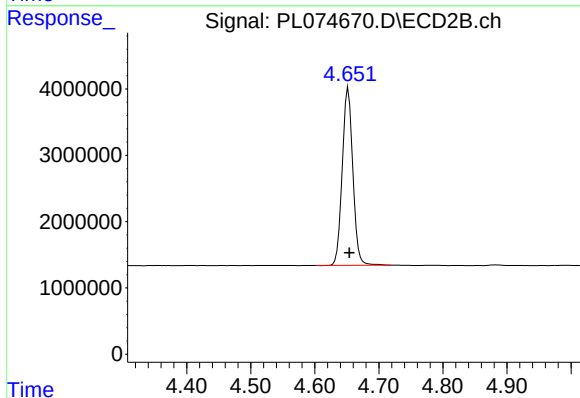


#1 Tetrachloro-m-xylene

R.T.: 4.652 min
Delta R.T.: -0.002 min
Response: 30662957
Conc: 22.34 ng/ml

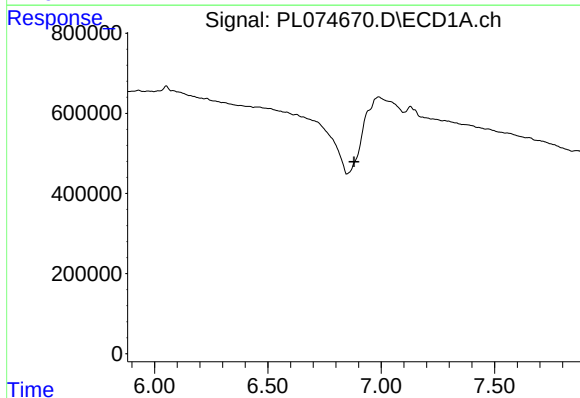


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.881 min
Response: 0
Conc: N.D.

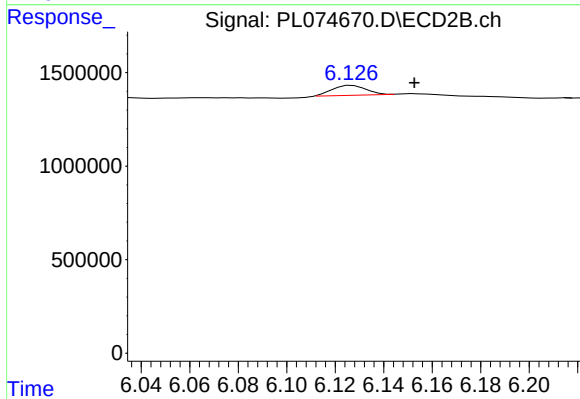

#6 beta-BHC


R.T.: 6.127 min
Delta R.T.: -0.026 min
Response: 514942
Conc: 0.65 ng/ml

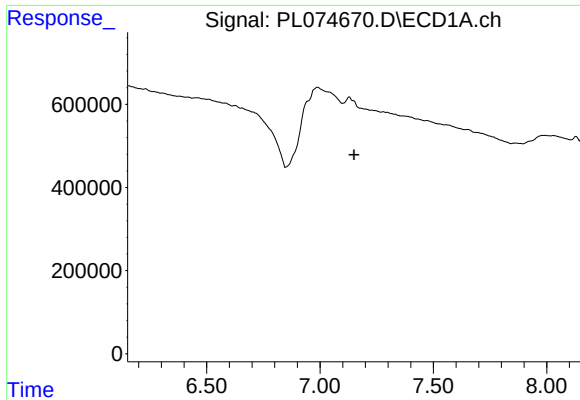

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

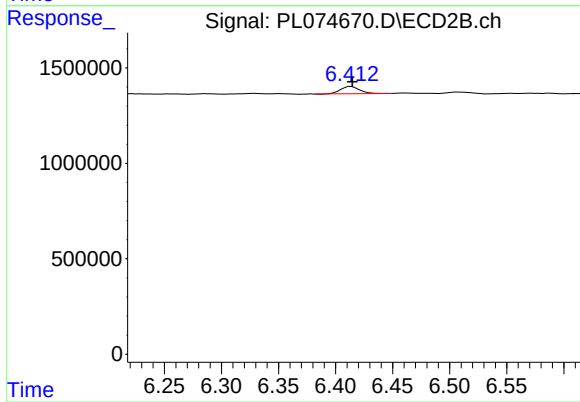


#7 delta-BHC

R.T.: 6.413 min
Delta R.T.: -0.001 min
Response: 438646
Conc: 0.28 ng/ml

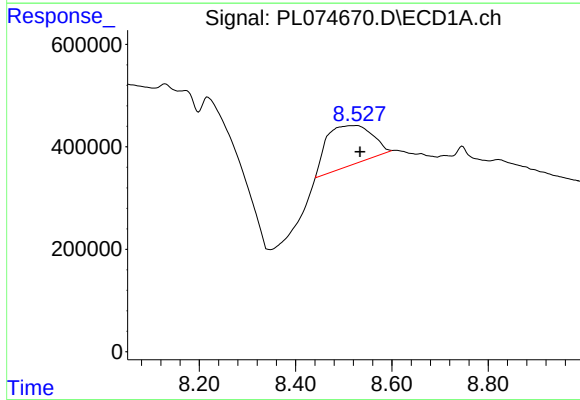


#9 Endosulfan I

R.T.: 8.528 min
Delta R.T.: -0.006 min
Response: 5192699
Conc: 9.01 ng/ml

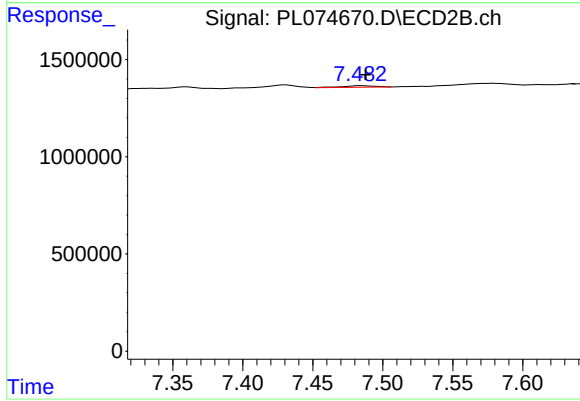

#9 Endosulfan I


R.T.: 7.484 min
Delta R.T.: -0.004 min
Response: 113685
Conc: 0.09 ng/ml

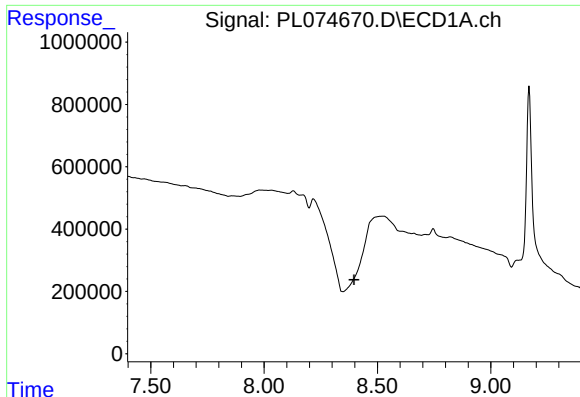

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

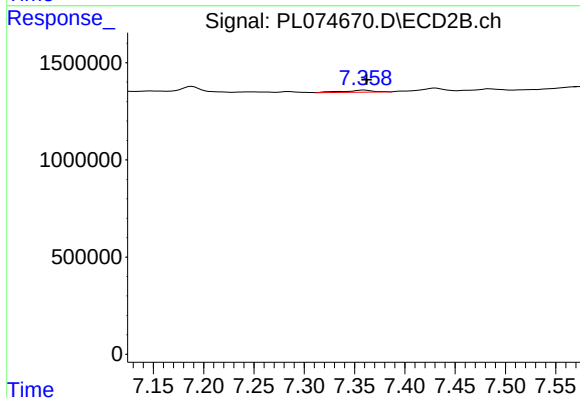


#10 gamma-Chlordane

R.T.: 7.360 min
Delta R.T.: -0.002 min
Response: 210224
Conc: 0.15 ng/ml

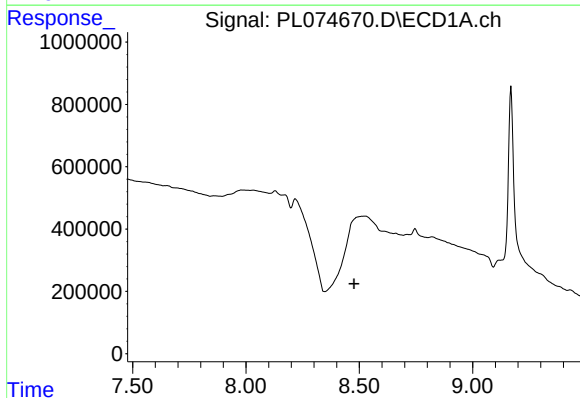


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 8.477 min
Response: 0
Conc: N.D.

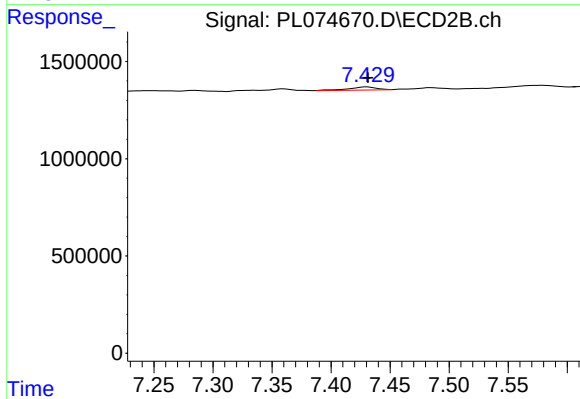

#11 alpha-Chlordane


R.T.: 7.430 min
Delta R.T.: 0.000 min
Response: 253184
Conc: 0.19 ng/ml

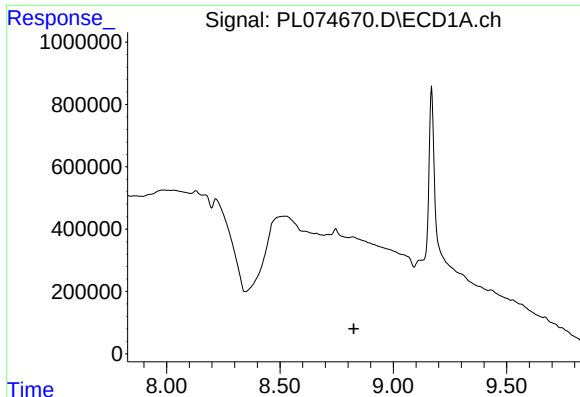

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 8.826 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

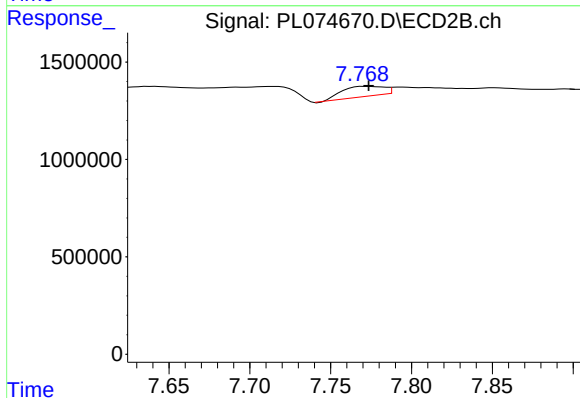


#13 Dieldrin

R.T.: 7.771 min
Delta R.T.: -0.002 min
Response: 917036
Conc: 0.72 ng/ml

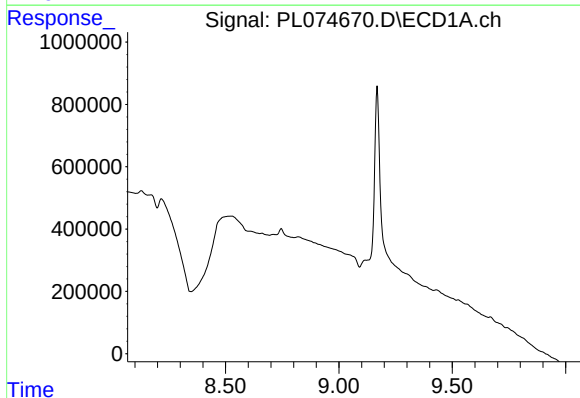


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.067 min
Response: 0
Conc: N.D.

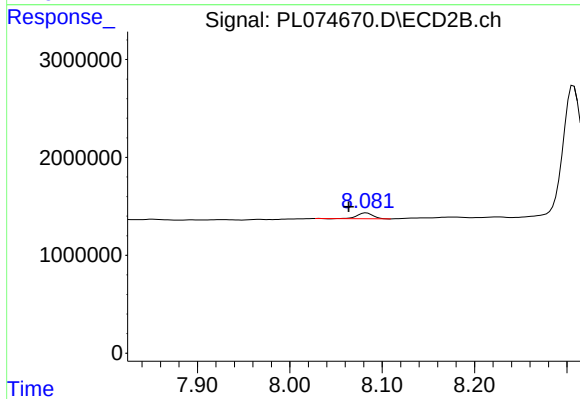

#14 Endrin


R.T.: 8.083 min
Delta R.T.: 0.019 min
Response: 685693
Conc: 0.65 ng/ml

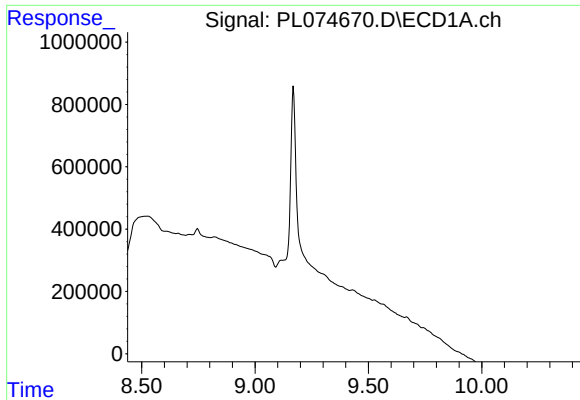

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 9.436 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

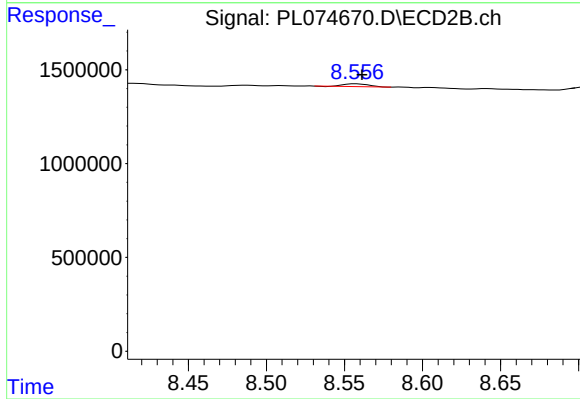


#18 Endrin aldehyde

R.T.: 8.558 min
Delta R.T.: -0.004 min
Response: 162098
Conc: 0.20 ng/ml

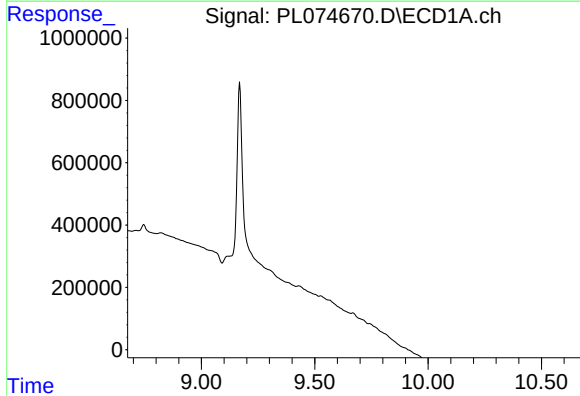


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.674 min
Response: 0
Conc: N.D.

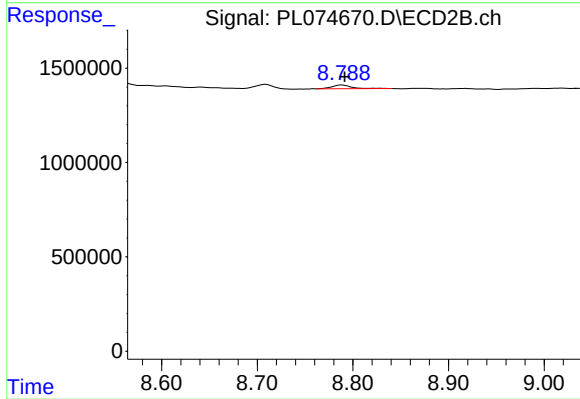

#19 Endosulfan Sulfate


R.T.: 8.789 min
Delta R.T.: -0.002 min
Response: 287160
Conc: 0.26 ng/ml

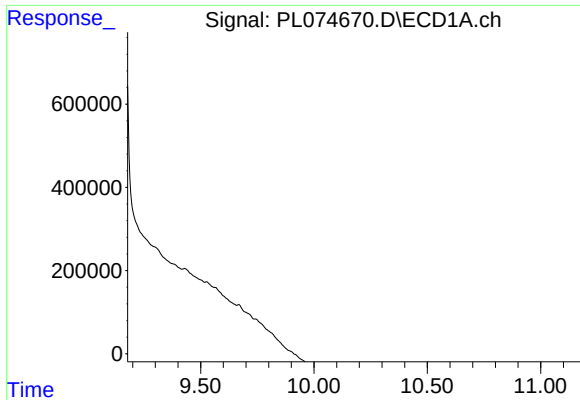

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 10.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

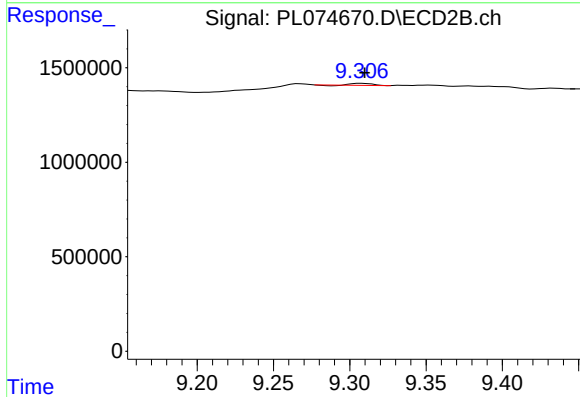


#21 Endrin ketone

R.T.: 9.308 min
Delta R.T.: -0.002 min
Response: 84605
Conc: 0.08 ng/ml

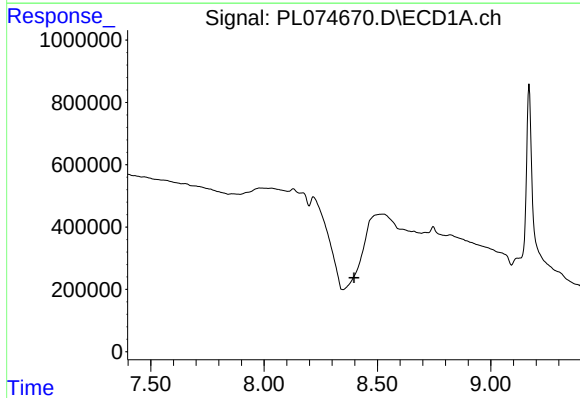


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

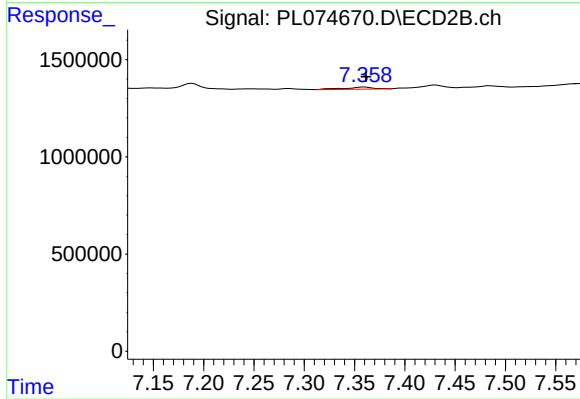

#25 Chlordane-3


R.T.: 7.360 min
Delta R.T.: -0.002 min
Response: 210224
Conc: 1.62 ng/ml

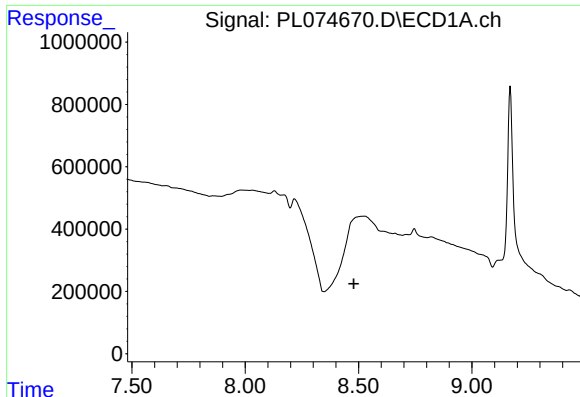

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

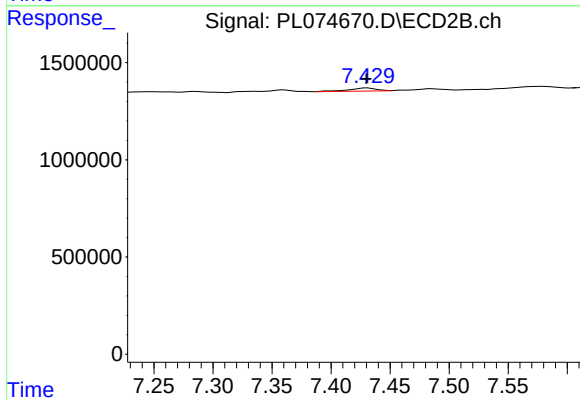


#26 Chlordane-4

R.T.: 7.430 min
Delta R.T.: 0.000 min
Response: 253184
Conc: 1.85 ng/ml

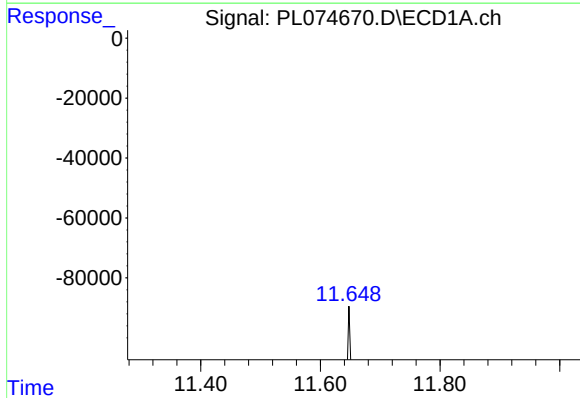

#28 Decachlorobiphenyl

R.T.: 11.649 min
Delta R.T.: 0.000 min
Response: 11748837
Conc: 26.31 ng/ml

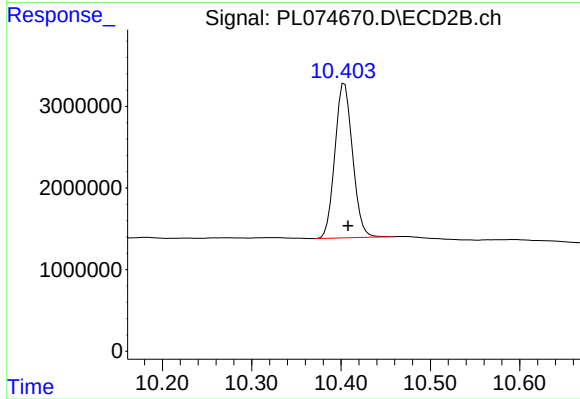

#28 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.004 min
Response: 25951724
Conc: 25.28 ng/ml