

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051222\
 Data File : PL074680.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2022 01:13
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 03:12:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 16:19:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.647	4.653	11627592	28841430	22.901	21.014
28)	SA Decachlor...	11.647	10.404	11230165	23927078	25.147	23.311
Target Compounds							
4)	MA Heptachlor	0.000	6.164f	0	205745	N.D.	0.136 #
6)	B beta-BHC	0.000	6.164	0	205745	N.D.	0.259 #
9)	A Endosulfan I	8.507f	0.000	5127211	0	8.894	N.D. #
13)	MA Dieldrin	0.000	7.793f	0	1349947	N.D.	1.060 #
14)	MA Endrin	0.000	8.083f	0	1772799	N.D.	1.678 #
26)	Chlordane-4	8.507f	0.000	5127211	0	53.220	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051222\
Data File : PL074680.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2022 01:13
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 03:12:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 16:19:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

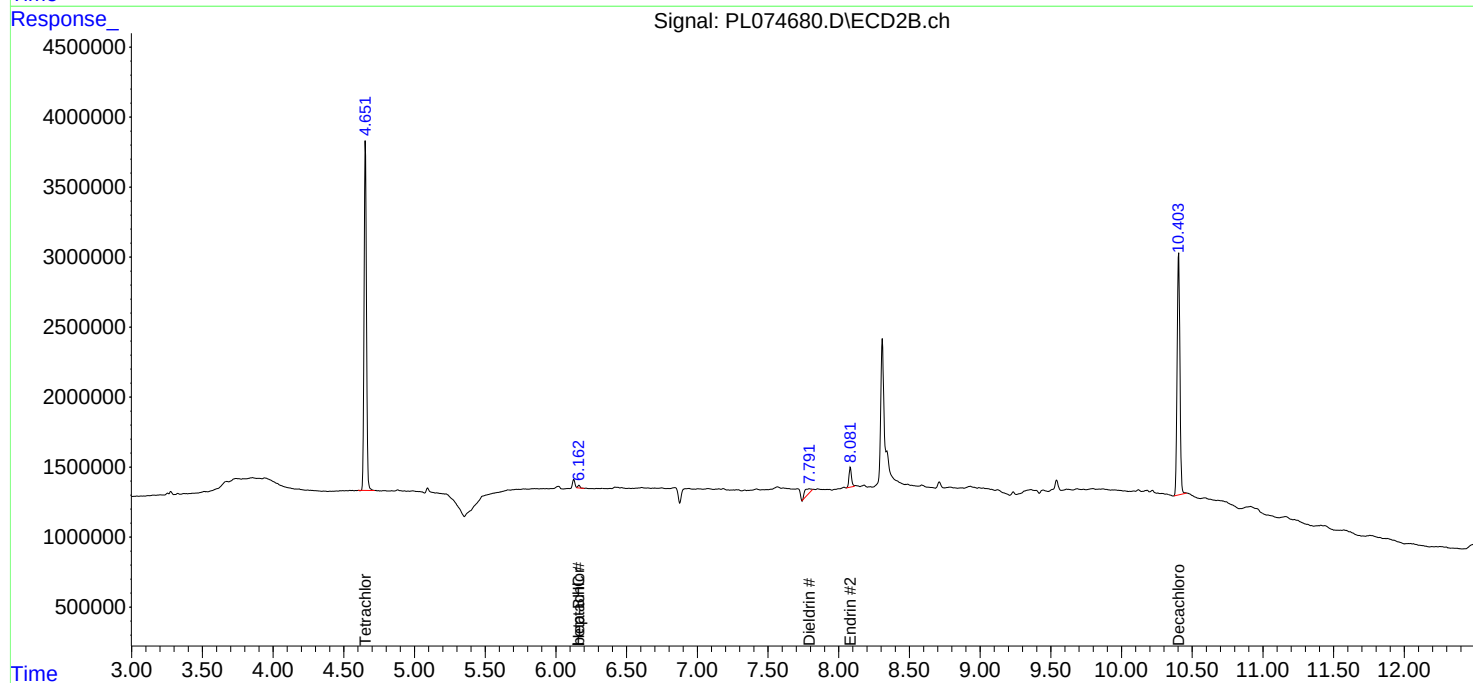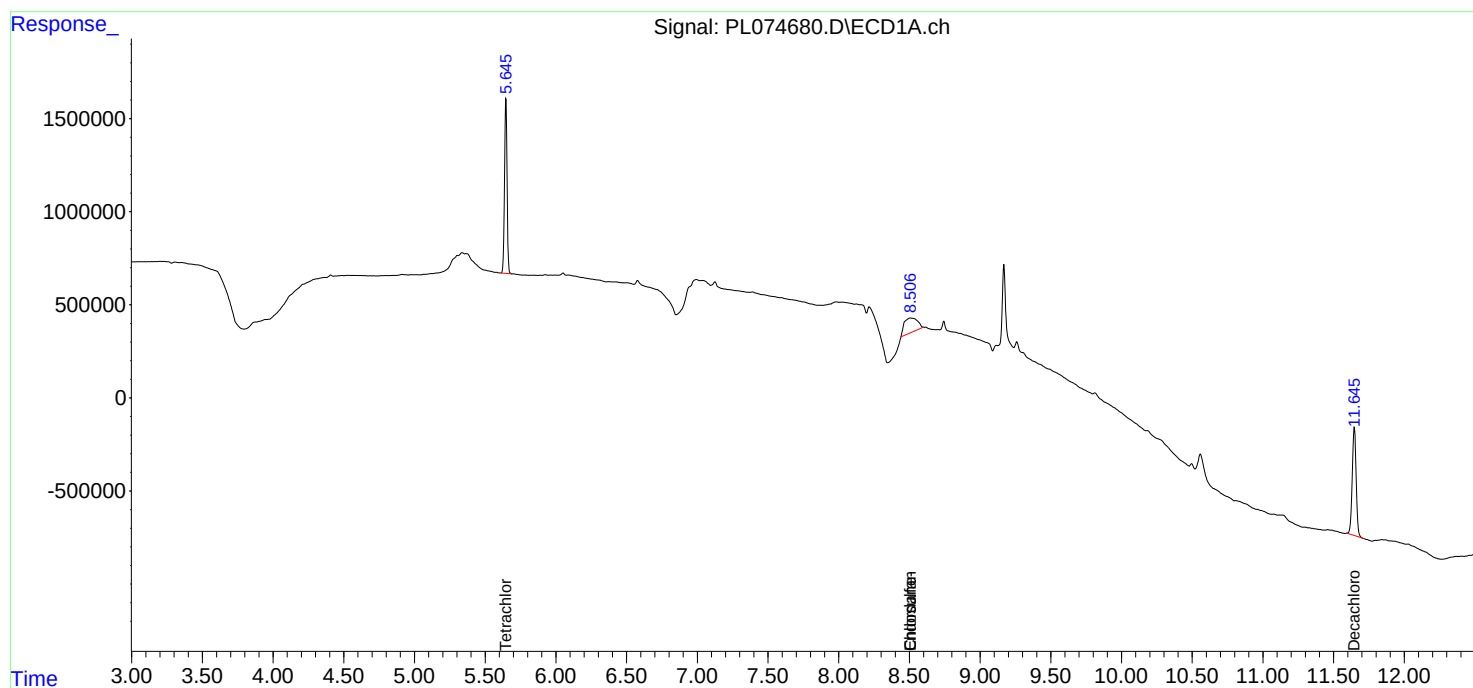


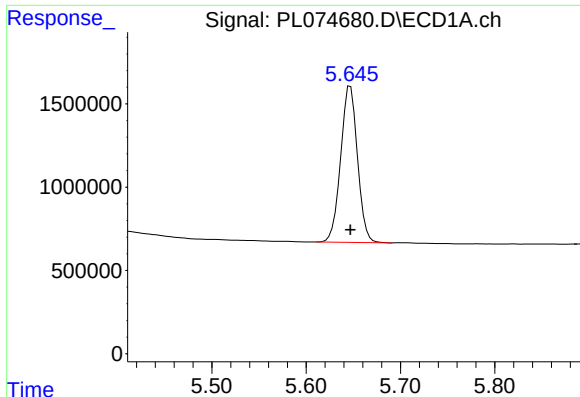

#1 Tetrachloro-m-xylene


R.T.: 5.647 min
Delta R.T.: 0.000 min
Response: 11627592
Conc: 22.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

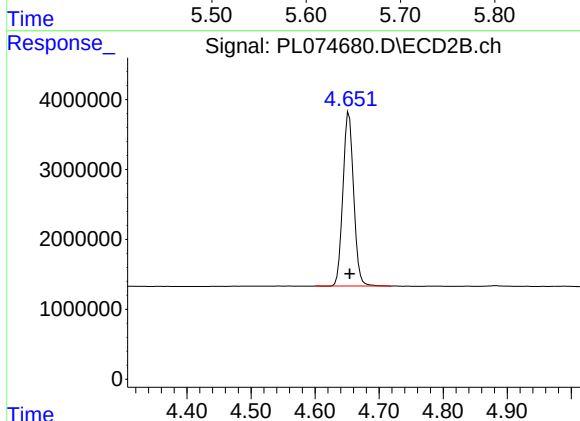


#1 Tetrachloro-m-xylene

R.T.: 4.653 min
Delta R.T.: -0.001 min
Response: 28841430
Conc: 21.01 ng/ml

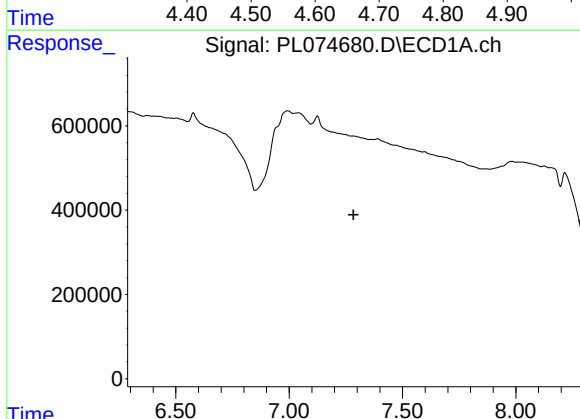


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.284 min
Response: 0
Conc: N.D.

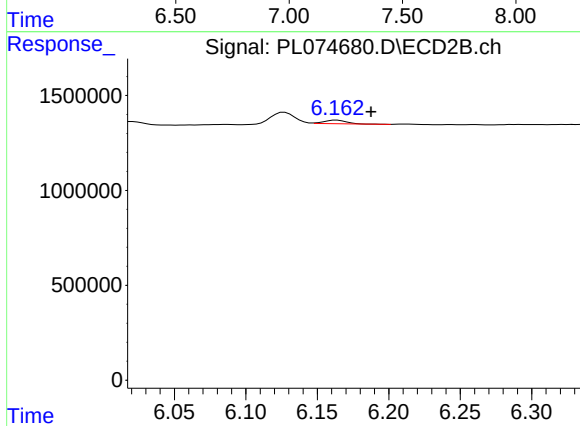

#4 Heptachlor


R.T.: 6.164 min
Delta R.T.: -0.024 min
Response: 205745
Conc: 0.14 ng/ml

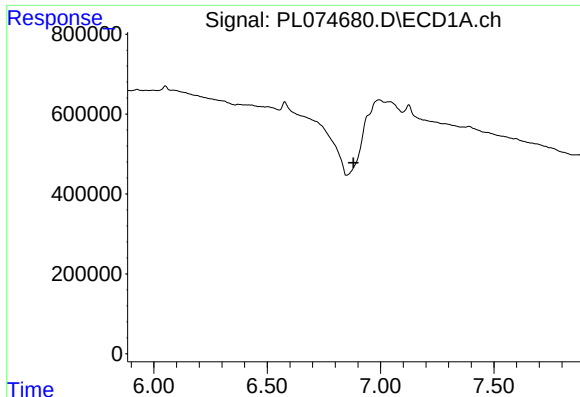

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.881 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

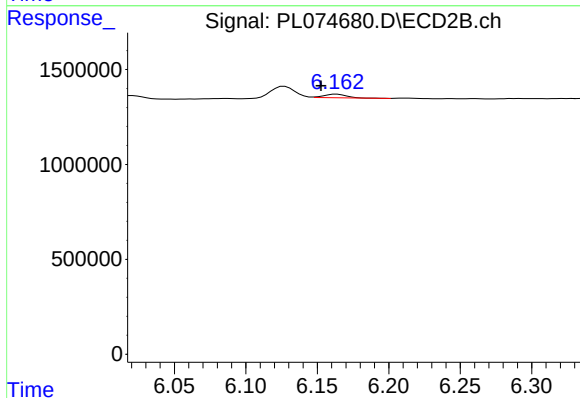


#6 beta-BHC

R.T.: 6.164 min
Delta R.T.: 0.011 min
Response: 205745
Conc: 0.26 ng/ml

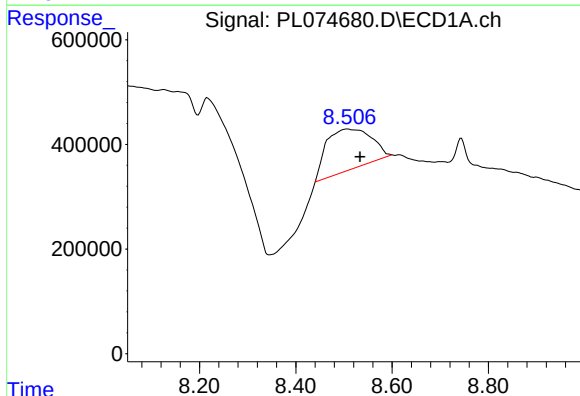


#9 Endosulfan I

R.T.: 8.507 min
Delta R.T.: -0.026 min
Response: 5127211
Conc: 8.89 ng/ml

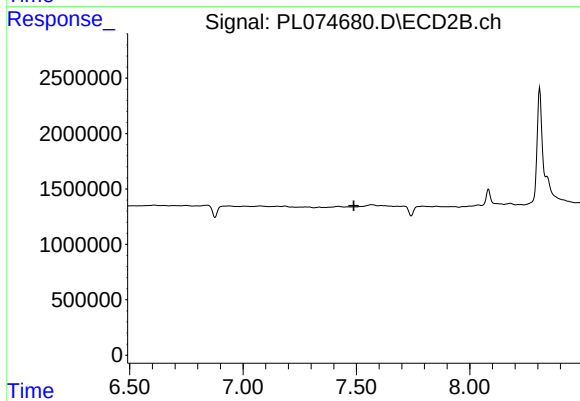

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.488 min
Response: 0
Conc: N.D.

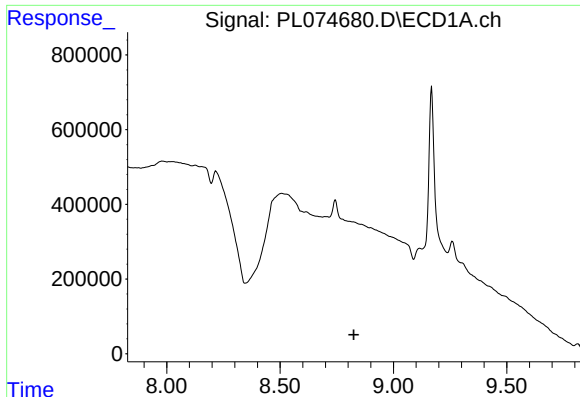

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.826 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

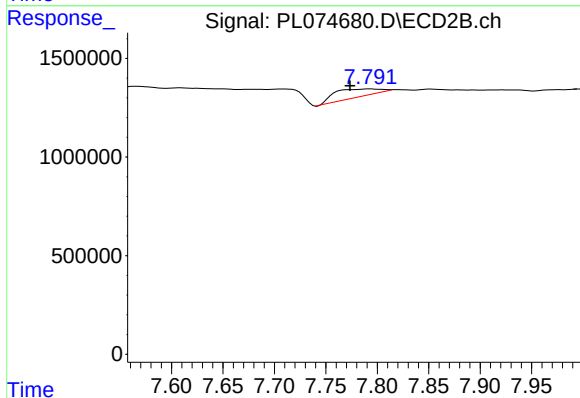


#13 Dieldrin

R.T.: 7.793 min
Delta R.T.: 0.019 min
Response: 1349947
Conc: 1.06 ng/ml

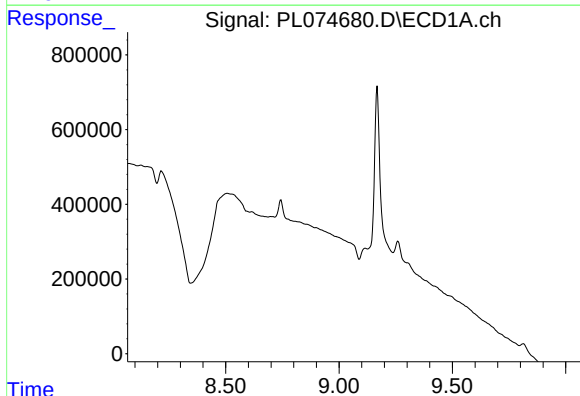


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.067 min
Response: 0
Conc: N.D.

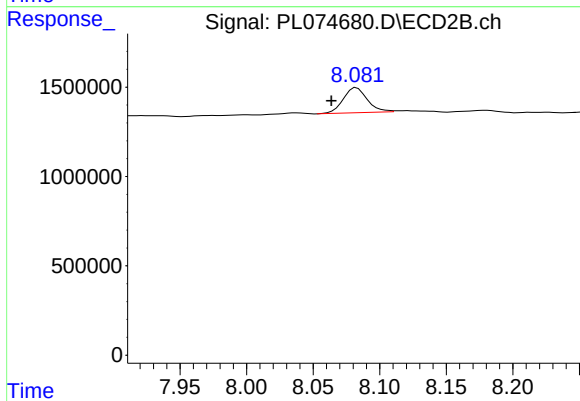

#14 Endrin


R.T.: 8.083 min
Delta R.T.: 0.019 min
Response: 1772799
Conc: 1.68 ng/ml

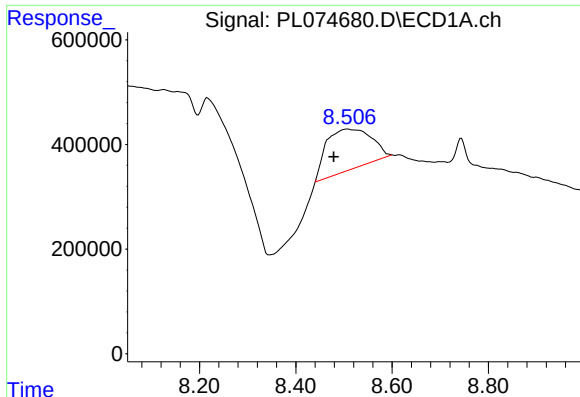

#26 Chlordane-4


R.T.: 8.507 min
Delta R.T.: 0.029 min
Response: 5127211
Conc: 53.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

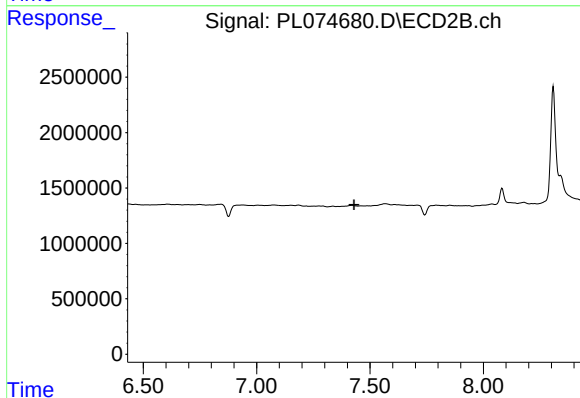


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.430 min
Response: 0
Conc: N.D.

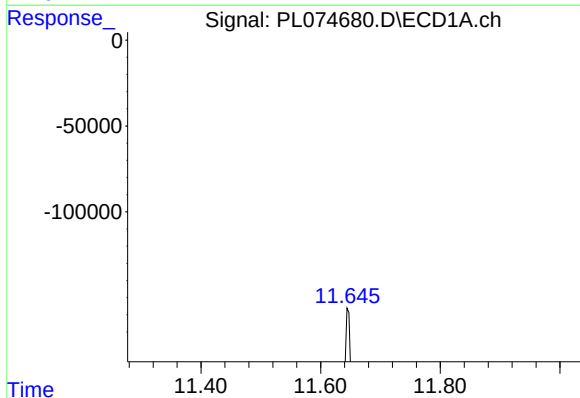

#28 Decachlorobiphenyl

R.T.: 11.647 min
Delta R.T.: -0.003 min
Response: 11230165
Conc: 25.15 ng/ml

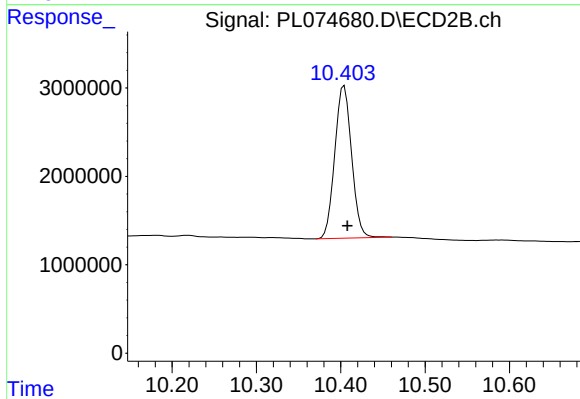

#28 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.004 min
Response: 23927078
Conc: 23.31 ng/ml