

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051222\
 Data File : PL074665.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2022 13:39
 Operator : AR\AJ
 Sample : N2756-02RE
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HP-640RE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/13/2022
 Supervised By : mohammad ahmed 05/16/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 03:08:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 16:19:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.647	4.652	10100810	10362105	19.894m	7.550 #
28) SA Decachlor...	11.647	10.405	2365151	4510677	5.296	4.395

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051222\
Data File : PL074665.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2022 13:39
Operator : AR\AJ
Sample : N2756-02RE
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HP-640RE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/13/2022
Supervised By : mohammad ahmed 05/16/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 03:08:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 16:19:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

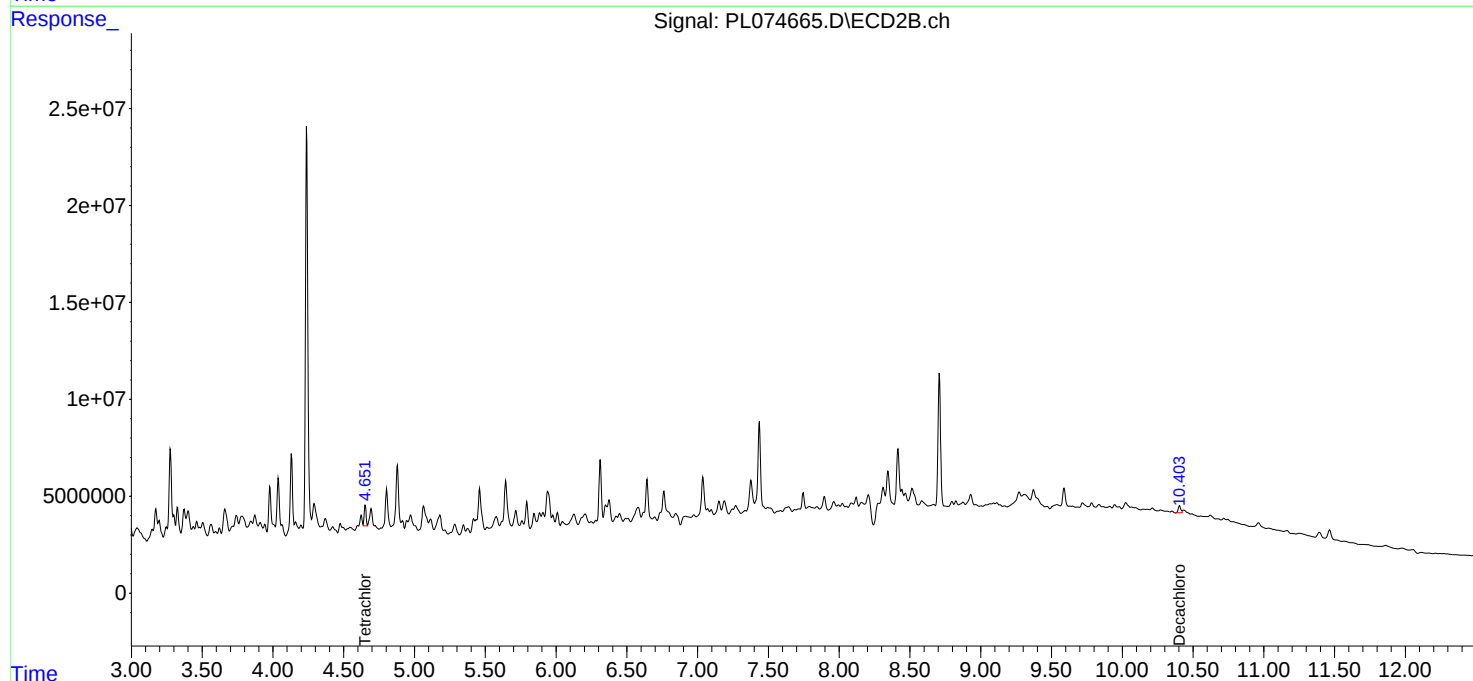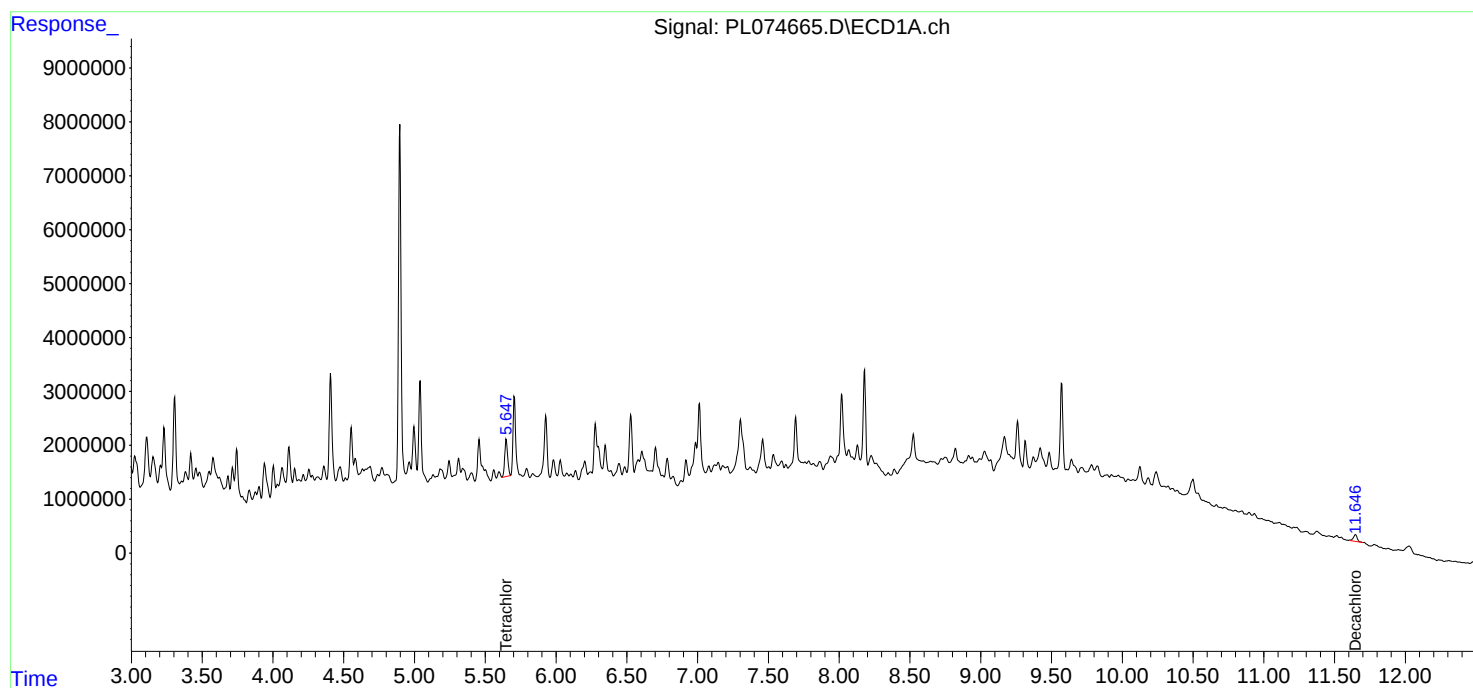

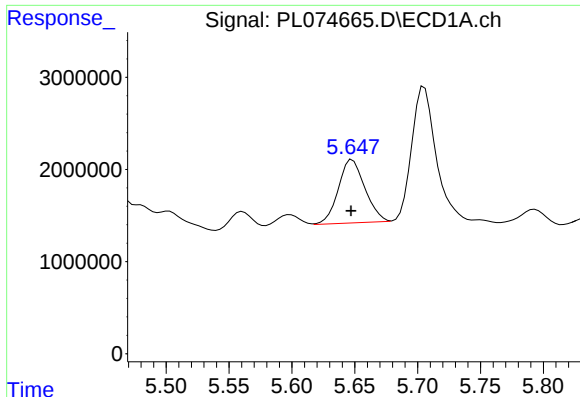


#1 Tetrachloro-m-xylene

R.T.: 5.647 min
Delta R.T.: 0.000 min
Response: 10100810
Conc: 19.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
HP-640RE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/13/2022
Supervised By :mohammad ahmed 05/16/2022

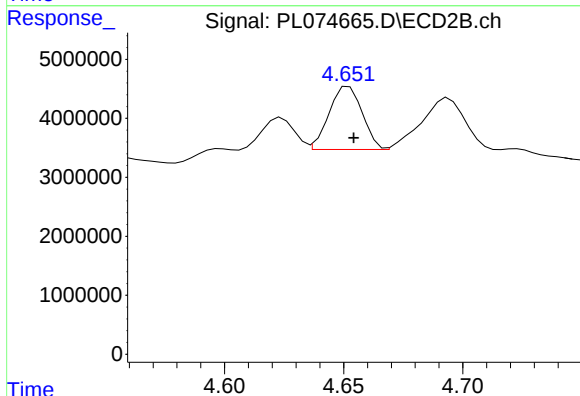


#1 Tetrachloro-m-xylene

R.T.: 4.652 min
Delta R.T.: -0.002 min
Response: 10362105
Conc: 7.55 ng/ml

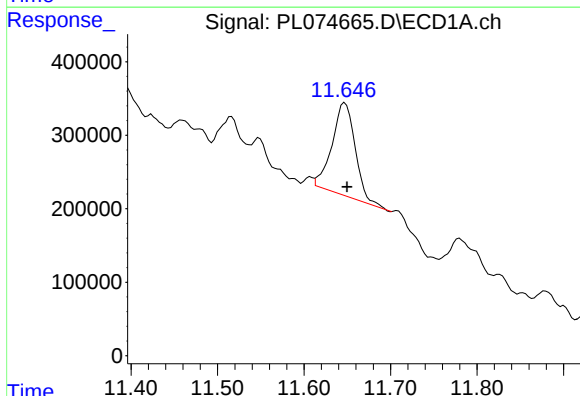

#28 Decachlorobiphenyl

R.T.: 11.647 min
Delta R.T.: -0.003 min
Response: 2365151
Conc: 5.30 ng/ml

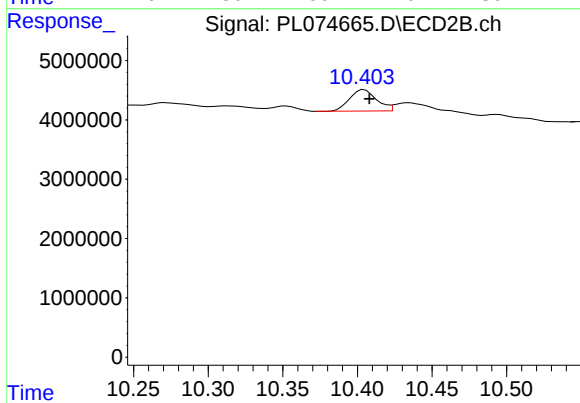

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.003 min
Response: 4510677
Conc: 4.39 ng/ml