

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051223\
 Data File : PL082697.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2023 16:11
 Operator : AR\AJ
 Sample : 02760-01 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HR-2-051123

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/15/2023
 Supervised By : Ankita Jodhani 05/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 23:24:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.318	2.641	5326318	4438693	1.994	1.916
2) SA Decachlor...	8.734	7.748	4266575	4245201	2.235	1.860
Target Compounds						
18) B Endrin al...	6.674	5.975	1032475	2215947	0.548	1.184m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051223\
Data File : PL082697.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2023 16:11
Operator : AR\AJ
Sample : 02760-01 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HR-2-051123


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/15/2023
Supervised By : Ankita Jodhani 05/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 23:24:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

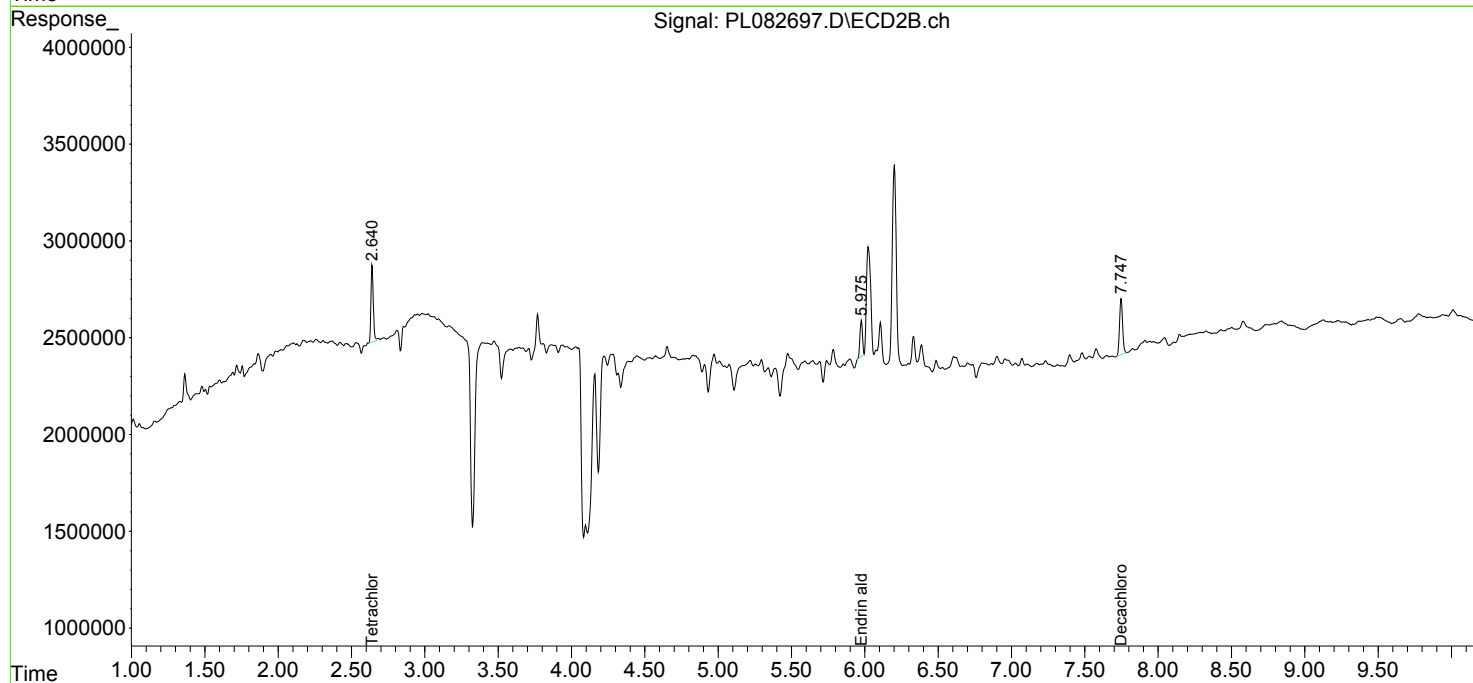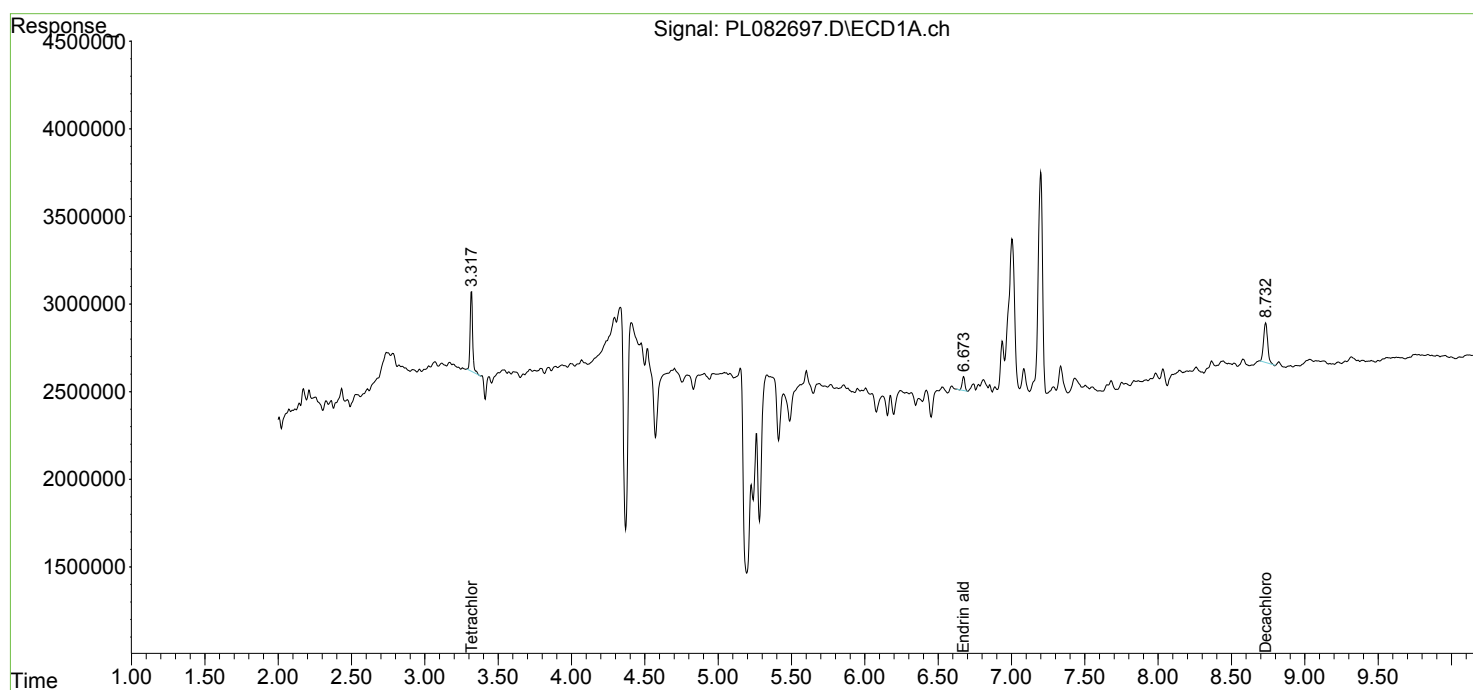

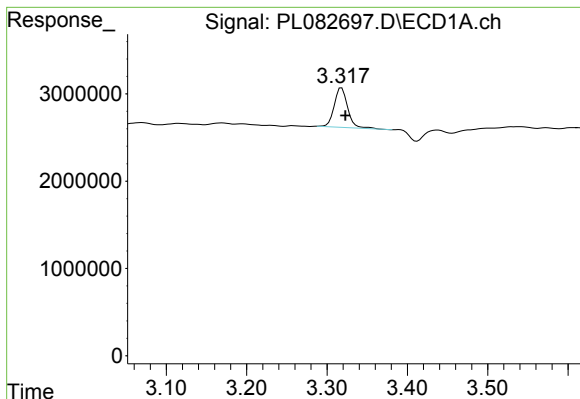


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: -0.005 min
Response: 5326318
Conc: 1.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-2-051123


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/15/2023
Supervised By :Ankita Jodhani 05/16/2023

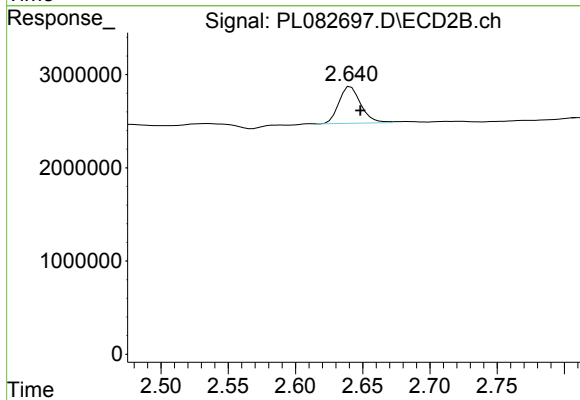


#1 Tetrachloro-m-xylene

R.T.: 2.641 min
Delta R.T.: -0.007 min
Response: 4438693
Conc: 1.92 ng/ml

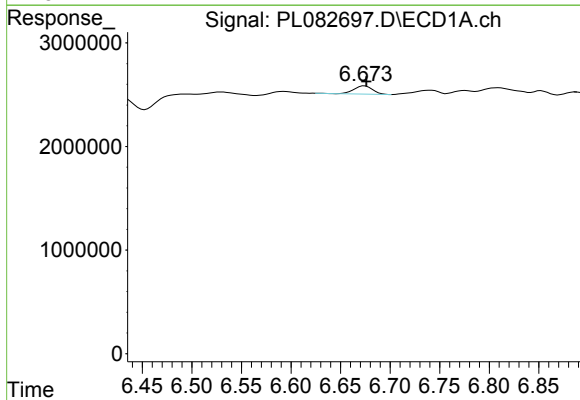


#18 Endrin aldehyde

R.T.: 6.674 min
Delta R.T.: -0.002 min
Response: 1032475
Conc: 0.55 ng/ml

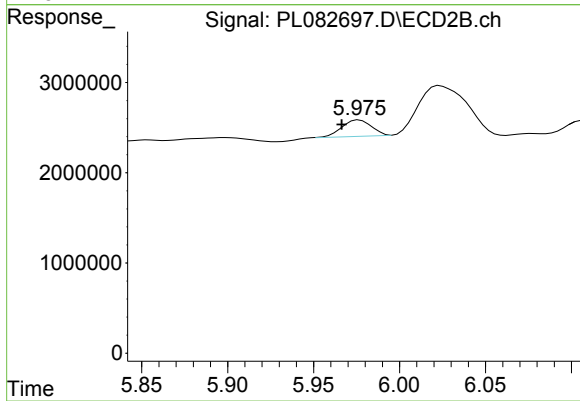

#18 Endrin aldehyde

R.T.: 5.975 min
Delta R.T.: 0.009 min
Response: 2215947
Conc: 1.18 ng/ml m

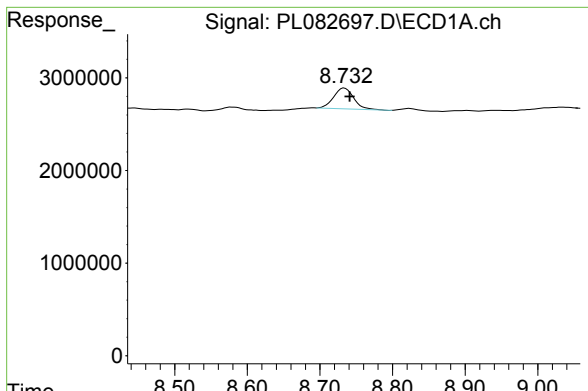


#28 Decachlorobiphenyl

R.T.: 8.734 min
Delta R.T.: -0.007 min
Response: 4266575
Conc: 2.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-2-051123

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/15/2023
Supervised By :Ankita Jodhani 05/16/2023

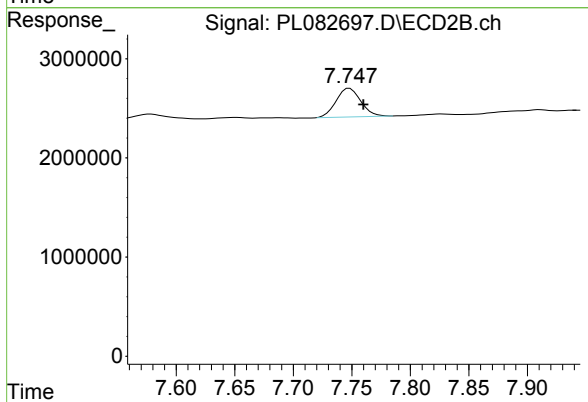

#28 Decachlorobiphenyl

R.T.: 7.748 min
Delta R.T.: -0.012 min
Response: 4245201
Conc: 1.86 ng/ml