

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051319\
 Data File : PL048481.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2019 12:37
 Operator : AJ\SJ
 Sample : K2692-12MSD
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 A5175MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 01:00:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 10 01:24:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.940	193.7E6	48810944	18.680	18.515
27)	SA Decachlor...	7.998	8.980	248.0E6	73284602	23.269	26.882
Target Compounds							
3)	MA gamma-BHC...	4.032	4.612	701.0E6	159.9E6	47.425	46.751
4)	MA Heptachlor	4.317	5.116	677.6E6	156.8E6	43.240	43.082
5)	MB Aldrin	4.556	5.419	630.5E6	139.8E6	42.313	42.396
13)	MA Dieldrin	5.563	6.418	1225.5E6	273.6E6	85.705	86.832
14)	MA Endrin	5.816	6.635	1109.8E6	234.4E6	88.922	89.126
17)	MA 4,4'-DDT	6.185	7.059	889.1E6	200.5E6	79.806	79.750

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051319\
Data File : PL048481.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2019 12:37
Operator : AJ\SJ
Sample : K2692-12MSD
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 01:00:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 10 01:24:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

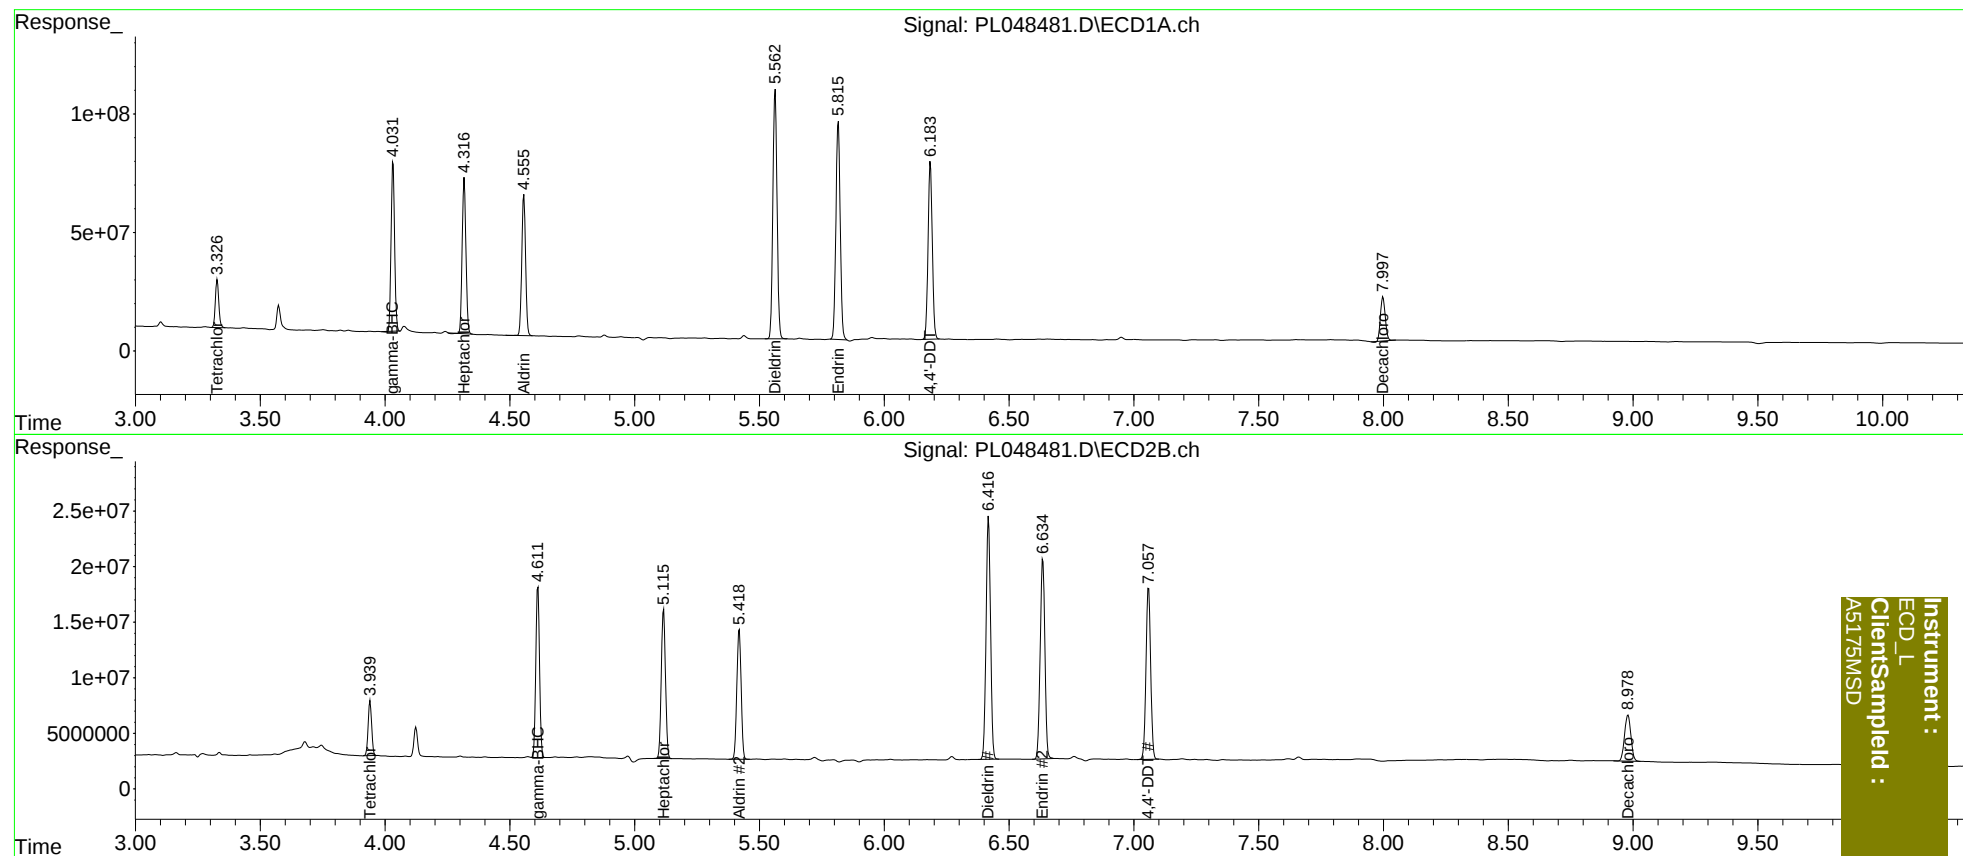

Instrument :
ECD_L
ClientSampled :
A5175MSD