

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051320\
 Data File : PL058669.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2020 08:47
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 01:51:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Wed May 13 09:14:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.532	4.076	38238152	51246303	23.276	23.675
28)	SA Decachlor...	8.321	9.189	32260454	44656115	24.706	25.268
Target Compounds							
7)	B delta-BHC	0.000	5.120f	0	905992	N.D.	0.319 #
8)	B Heptachlo...	0.000	5.958	0	9723615	N.D.	4.049 #
9)	A Endosulfan I	0.000	6.311f	0	1669883	N.D.	0.776 #
10)	B gamma-Chl...	0.000	6.175f	0	7965822	N.D.	3.391 #
14)	MA Endrin	0.000	6.785f	0	2008350	N.D.	1.107 #
15)	B Endosulfa...	0.000	7.013	0	960351	N.D.	0.481 #
16)	A 4,4'-DDD	0.000	6.950f	0	516624	N.D.	0.295 #
17)	MA 4,4'-DDT	0.000	7.224	0	1152135	N.D.	0.681 #
18)	B Endrin al...	0.000	7.128	0	381361	N.D.	0.223 #
25)	Chlordane-3	0.000	6.175f	0	7965822	N.D.	26.300 #
27)	Chlordane-5	0.000	7.082	0	243876	N.D.	3.906 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051320\
Data File : PL058669.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2020 08:47
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 01:51:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Wed May 13 09:14:54 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

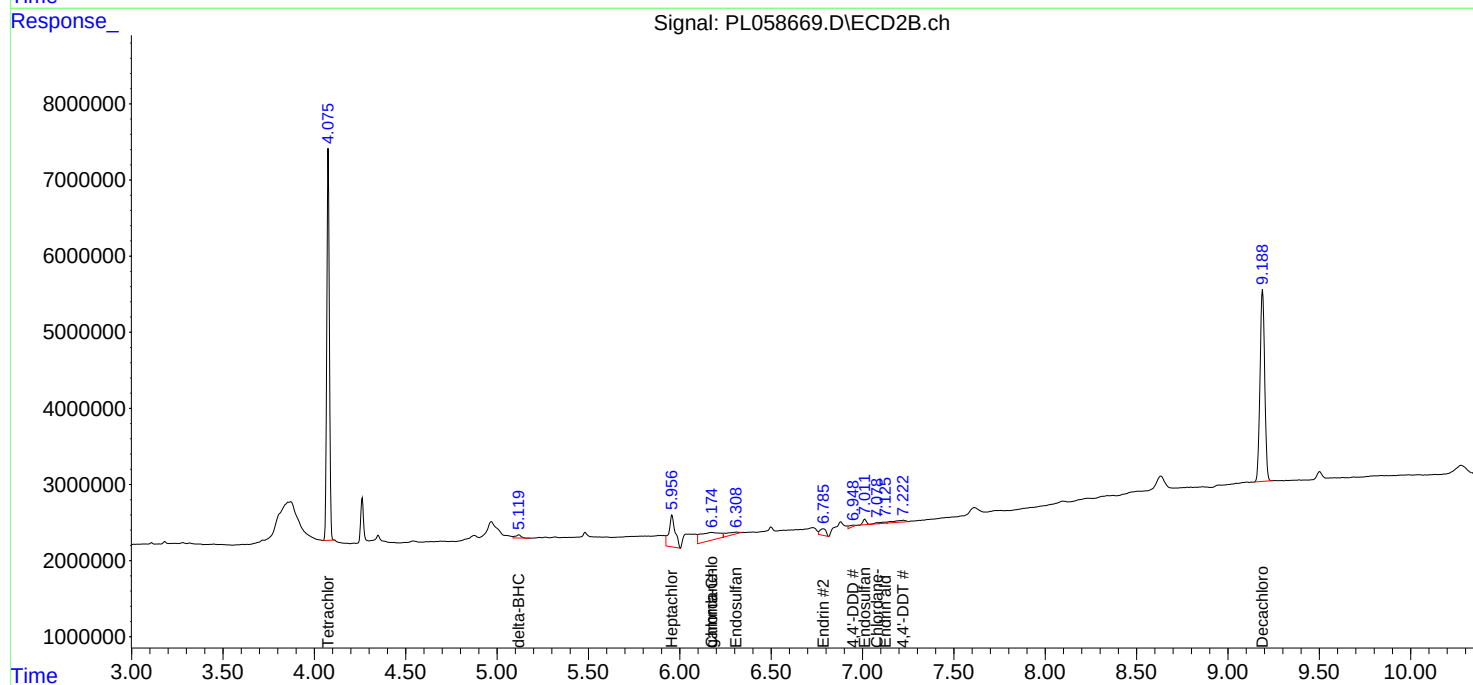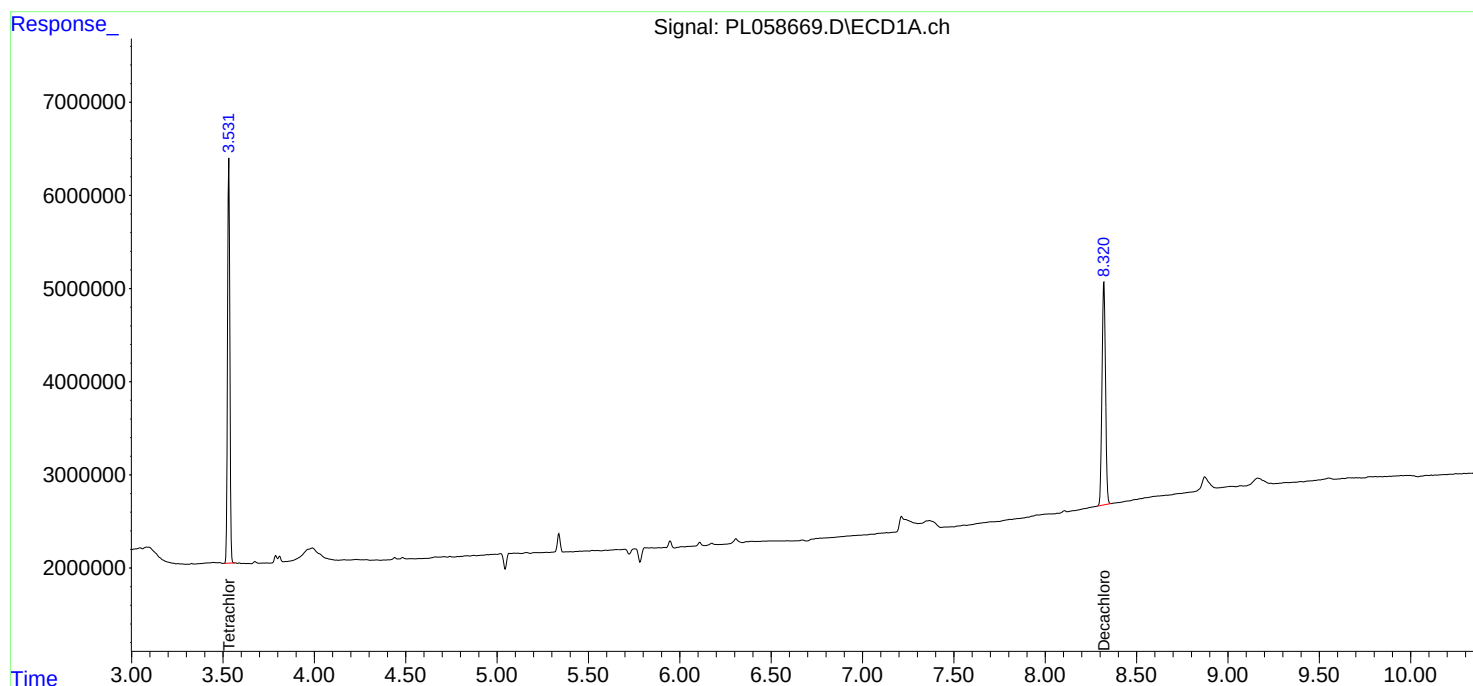


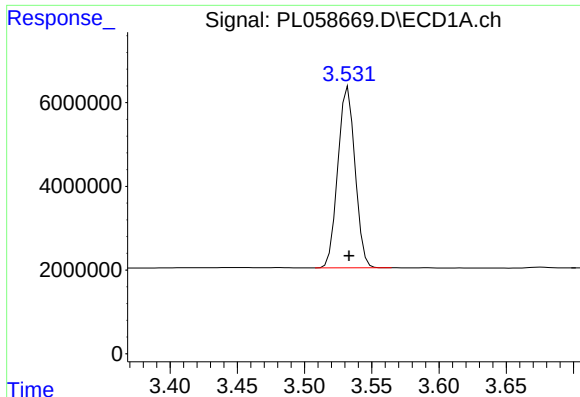

#1 Tetrachloro-m-xylene


R.T.: 3.532 min
Delta R.T.: 0.000 min
Response: 38238152
Conc: 23.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

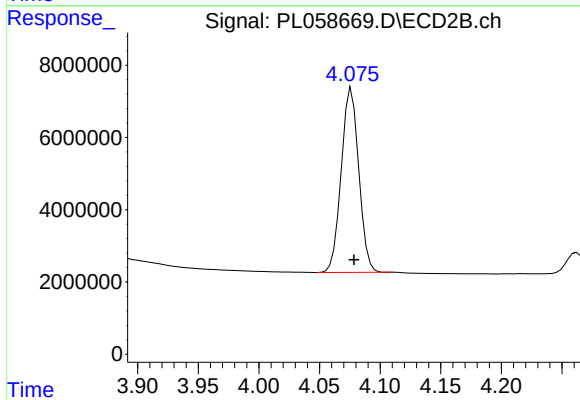


#1 Tetrachloro-m-xylene

R.T.: 4.076 min
Delta R.T.: -0.002 min
Response: 51246303
Conc: 23.67 ng/ml

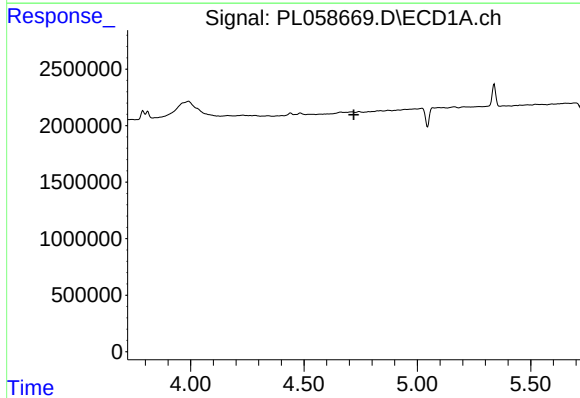


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.719 min
Response: 0
Conc: N.D.

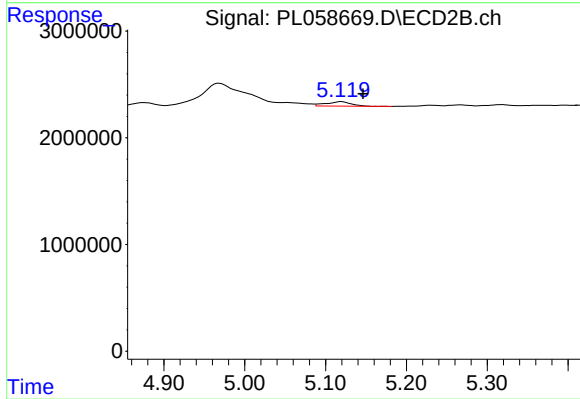

#7 delta-BHC


R.T.: 5.120 min
Delta R.T.: -0.027 min
Response: 905992
Conc: 0.32 ng/ml

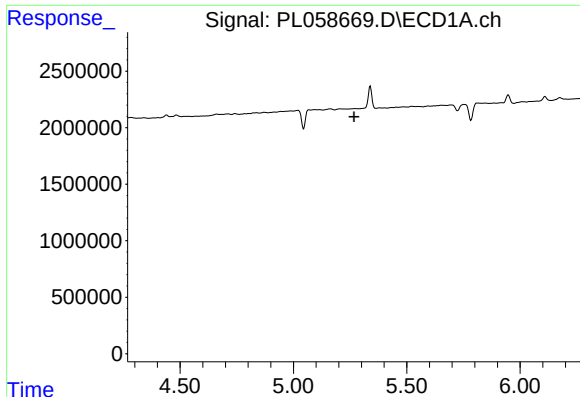

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

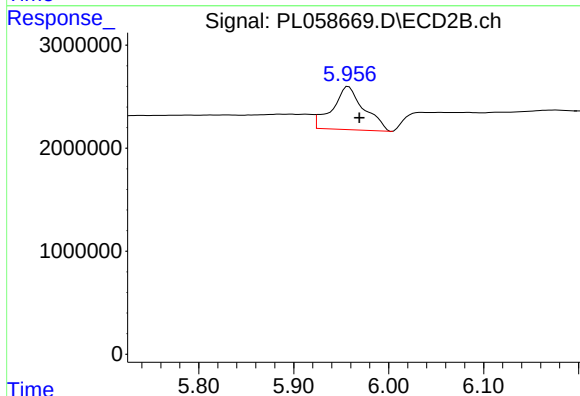


#8 Heptachlor epoxide

R.T.: 5.958 min
Delta R.T.: -0.011 min
Response: 9723615
Conc: 4.05 ng/ml

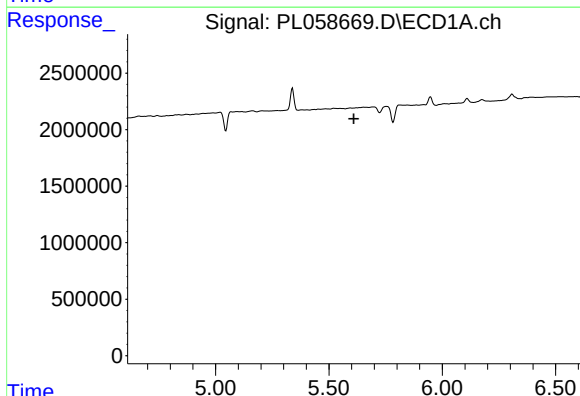


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.609 min
Response: 0
Conc: N.D.

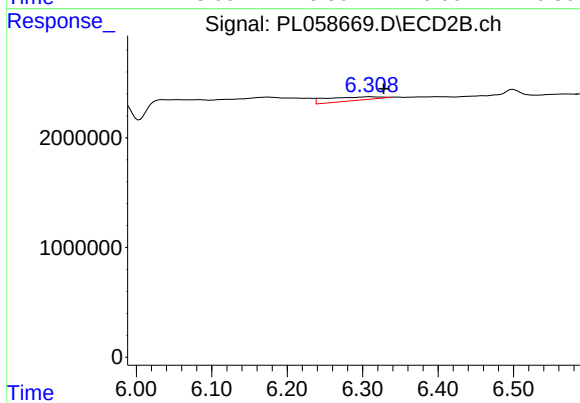

#9 Endosulfan I


R.T.: 6.311 min
Delta R.T.: -0.017 min
Response: 1669883
Conc: 0.78 ng/ml

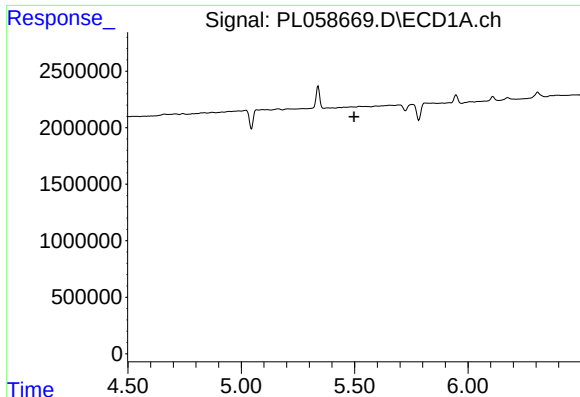

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

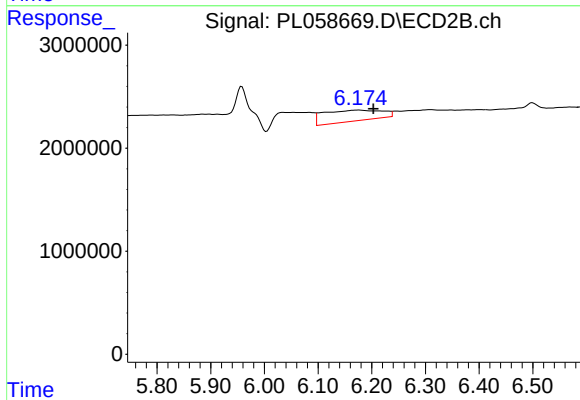


#10 gamma-Chlordane

R.T.: 6.175 min
Delta R.T.: -0.028 min
Response: 7965822
Conc: 3.39 ng/ml

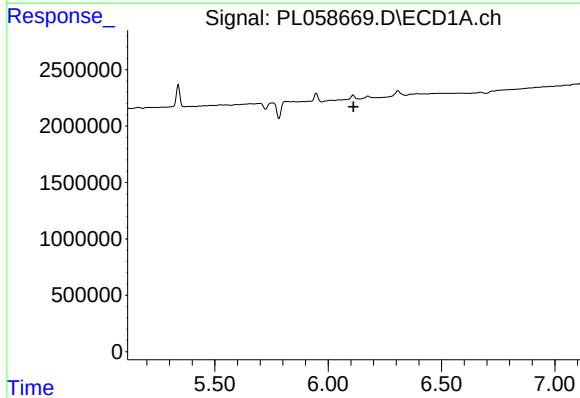


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

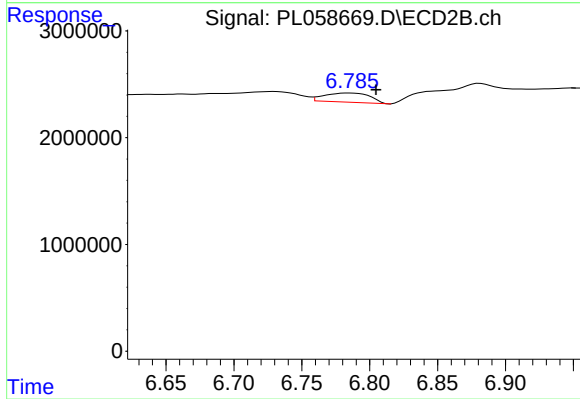

#14 Endrin


R.T.: 6.785 min
Delta R.T.: -0.020 min
Response: 2008350
Conc: 1.11 ng/ml

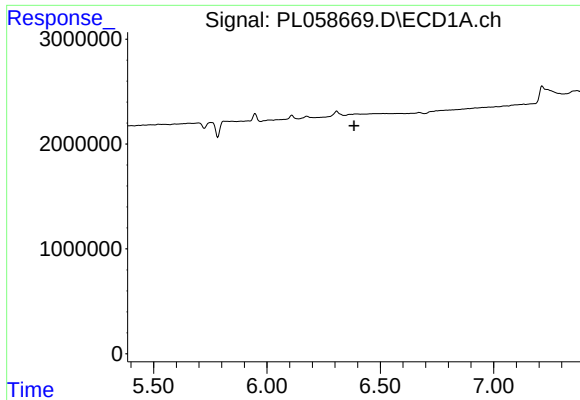

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.385 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

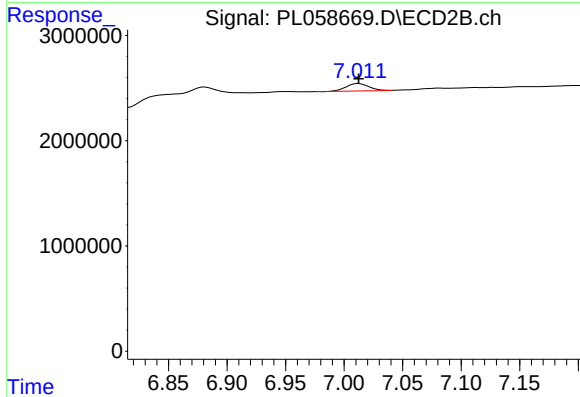


#15 Endosulfan II

R.T.: 7.013 min
Delta R.T.: 0.000 min
Response: 960351
Conc: 0.48 ng/ml

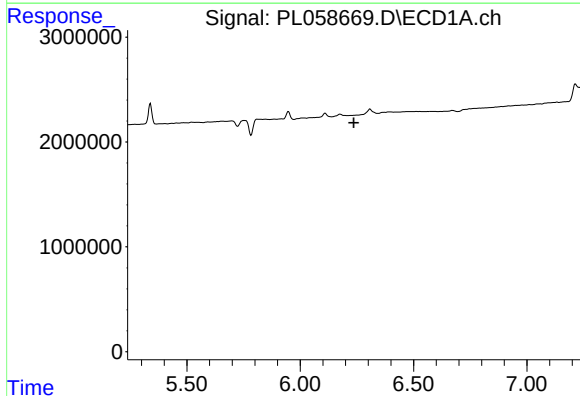


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.237 min
Response: 0
Conc: N.D.

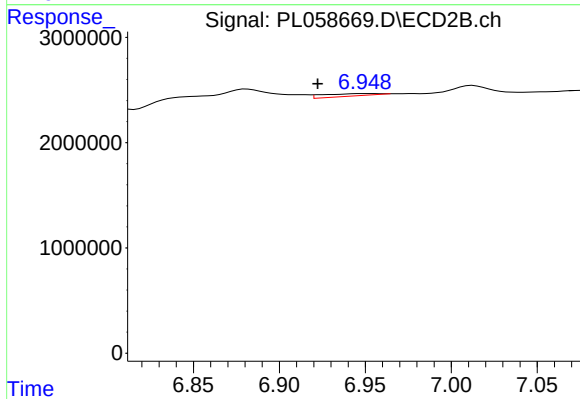

#16 4,4'-DDD


R.T.: 6.950 min
Delta R.T.: 0.027 min
Response: 516624
Conc: 0.30 ng/ml

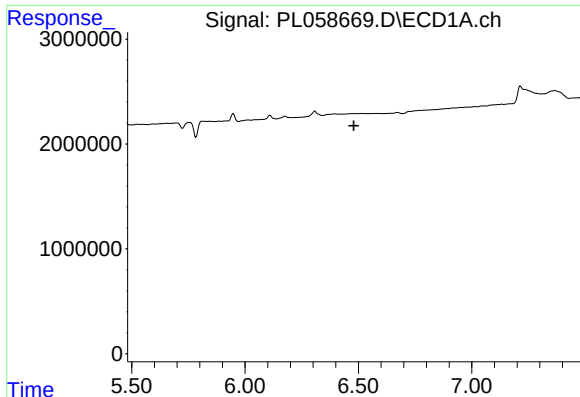

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.480 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

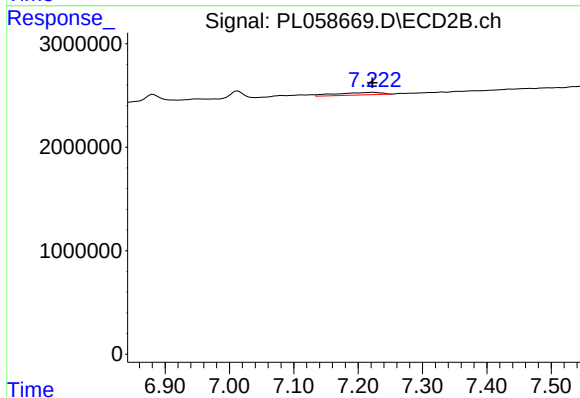


#17 4,4'-DDT

R.T.: 7.224 min
Delta R.T.: 0.001 min
Response: 1152135
Conc: 0.68 ng/ml

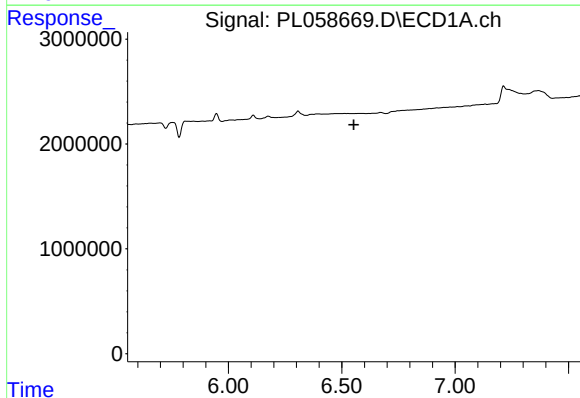


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.553 min
Response: 0
Conc: N.D.

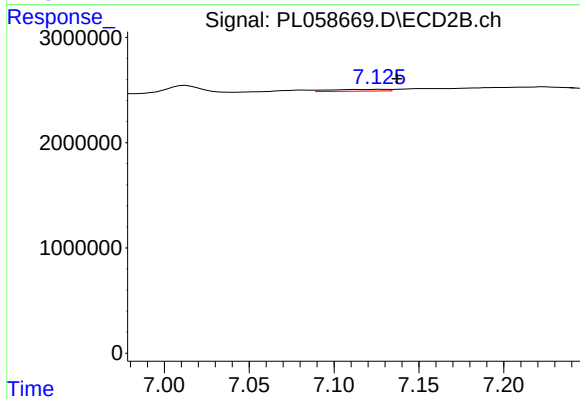

#18 Endrin aldehyde


R.T.: 7.128 min
Delta R.T.: -0.009 min
Response: 381361
Conc: 0.22 ng/ml

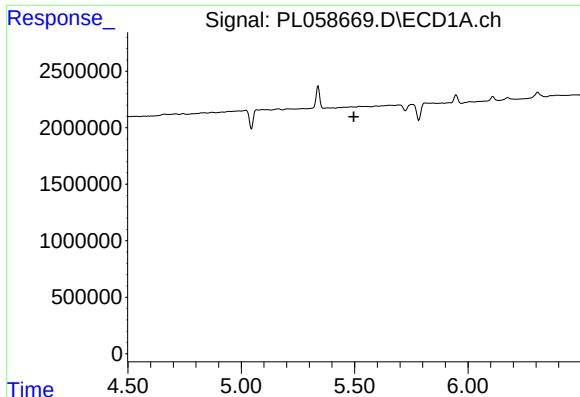

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

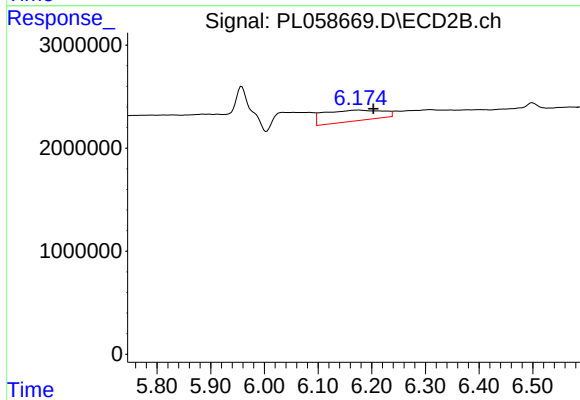


#25 Chlordane-3

R.T.: 6.175 min
Delta R.T.: -0.028 min
Response: 7965822
Conc: 26.30 ng/ml

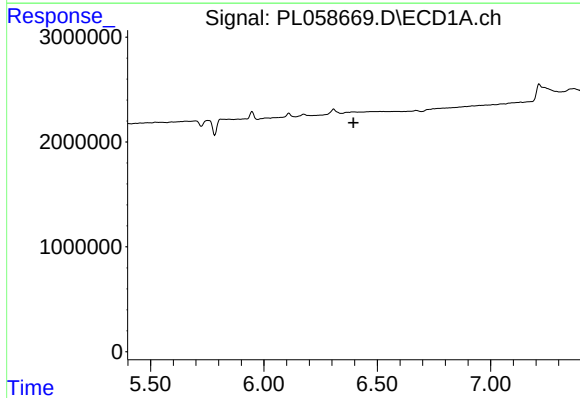


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

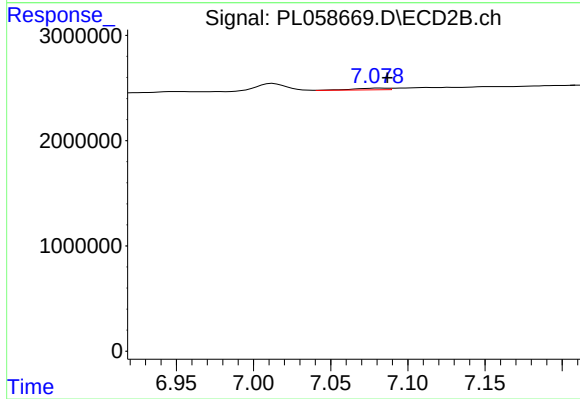

#27 Chlordane-5


R.T.: 7.082 min
Delta R.T.: -0.005 min
Response: 243876
Conc: 3.91 ng/ml

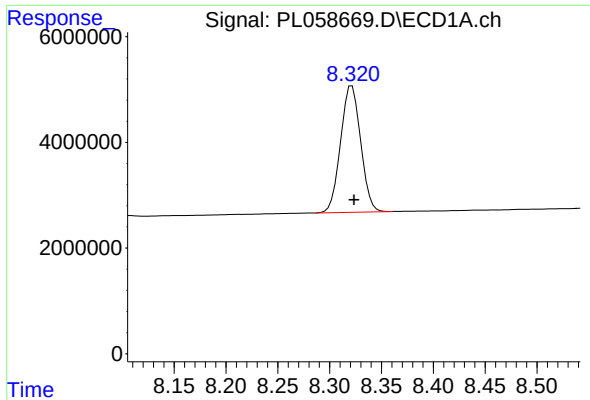

#28 Decachlorobiphenyl

R.T.: 8.321 min
Delta R.T.: -0.002 min
Response: 32260454
Conc: 24.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

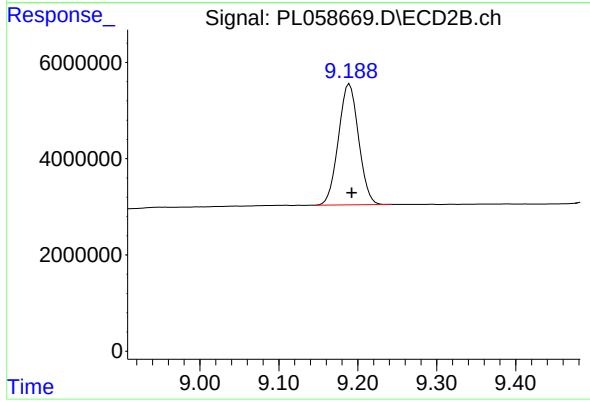

#28 Decachlorobiphenyl

R.T.: 9.189 min
Delta R.T.: -0.003 min
Response: 44656115
Conc: 25.27 ng/ml