

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051320\
 Data File : PL058674.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2020 10:41
 Operator : AJ\MA
 Sample : PB128769BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 01:53:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Wed May 13 09:14:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.532	4.078	36784978	50972894	22.391	23.548
28)	SA Decachlor...	8.320	9.189	32151872	46200790	24.623	26.142
Target Compounds							
7)	B delta-BHC	0.000	5.121f	0	1177352	N.D.	0.415 #
8)	B Heptachlo...	0.000	5.958	0	19805689	N.D.	8.248 #
9)	A Endosulfan I	0.000	6.307f	0	2862479	N.D.	1.330 #
10)	B gamma-Chl...	0.000	6.213	0	1781022	N.D.	0.758 #
13)	MA Dieldrin	5.849	0.000	4710674	0	3.163	N.D. #
14)	MA Endrin	6.108	6.787f	803056	4106346	0.618	2.264 #
15)	B Endosulfa...	0.000	7.013	0	1188057	N.D.	0.595 #
23)	Chlordane-1	0.000	5.055f	0	1027675	N.D.	12.842 #
25)	Chlordane-3	0.000	6.213	0	1781022	N.D.	5.880 #
26)	Chlordane-4	0.000	6.307f	0	2862479	N.D.	7.854 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051320\
Data File : PL058674.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2020 10:41
Operator : AJ\MA
Sample : PB128769BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 01:53:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Wed May 13 09:14:54 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

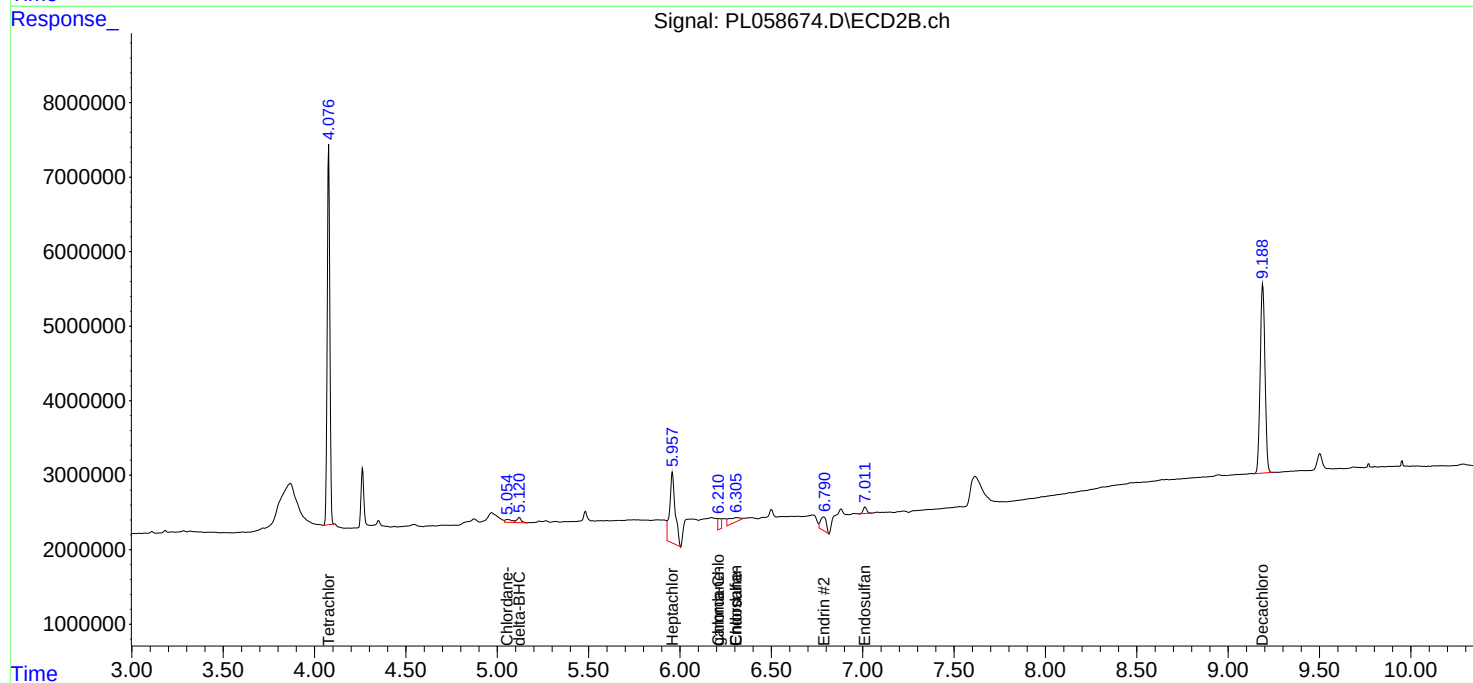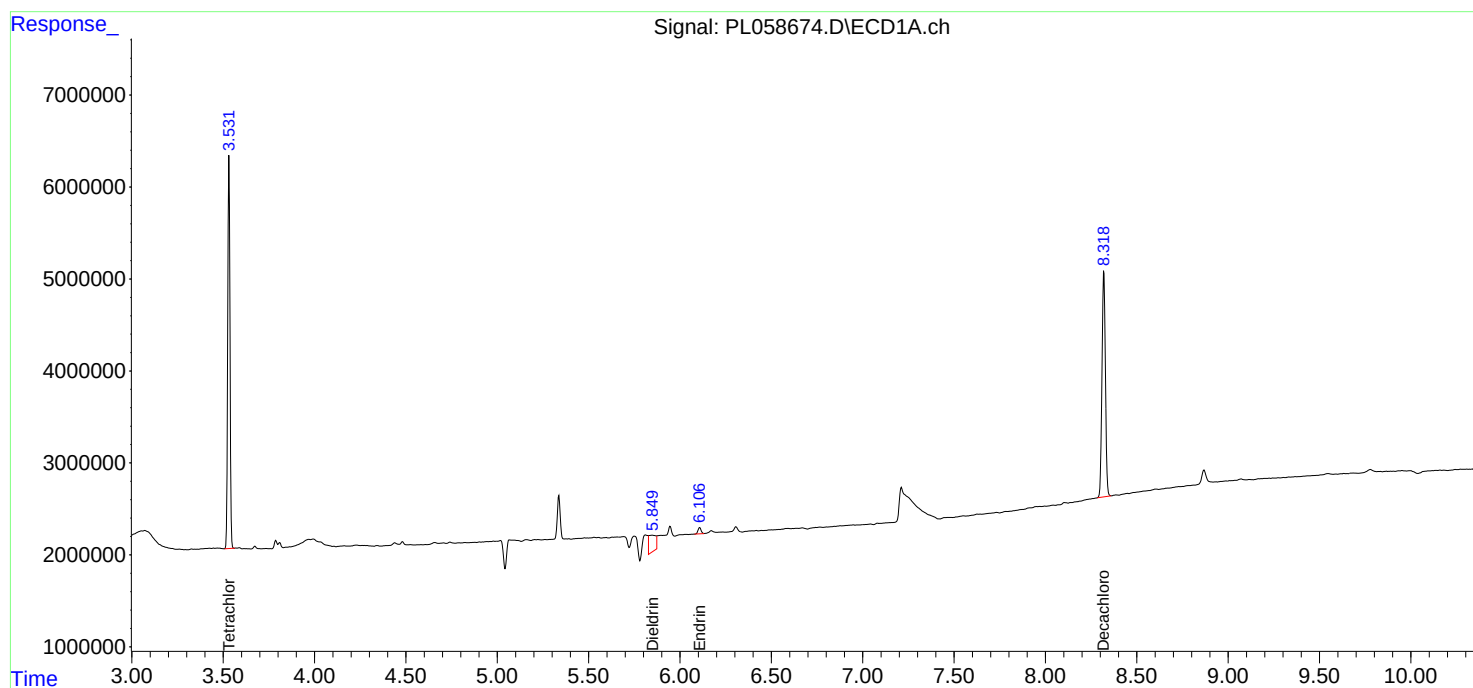


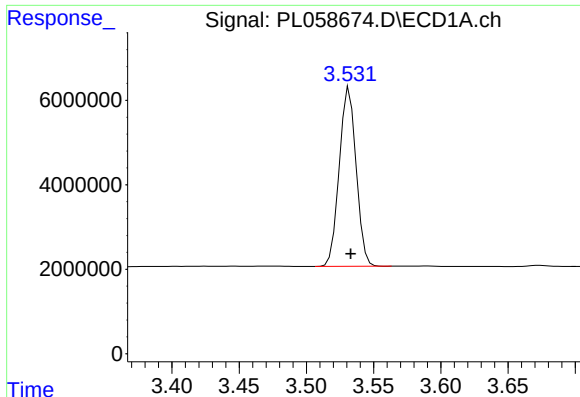

#1 Tetrachloro-m-xylene


R.T.: 3.532 min
Delta R.T.: -0.001 min
Response: 36784978
Conc: 22.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

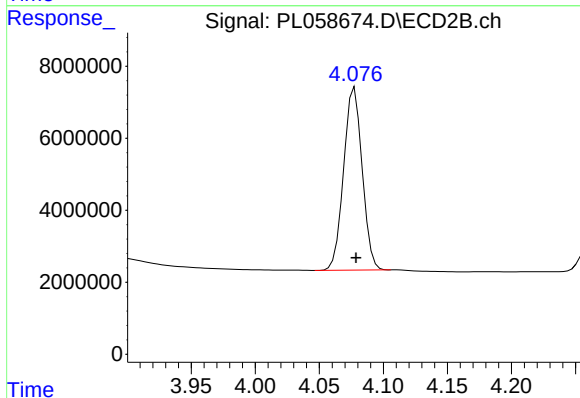


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: -0.001 min
Response: 50972894
Conc: 23.55 ng/ml

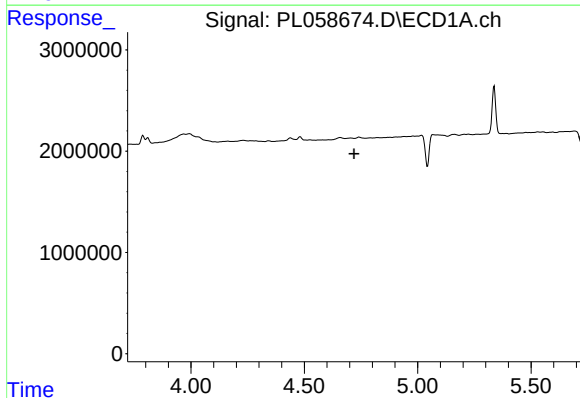


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.719 min
Response: 0
Conc: N.D.

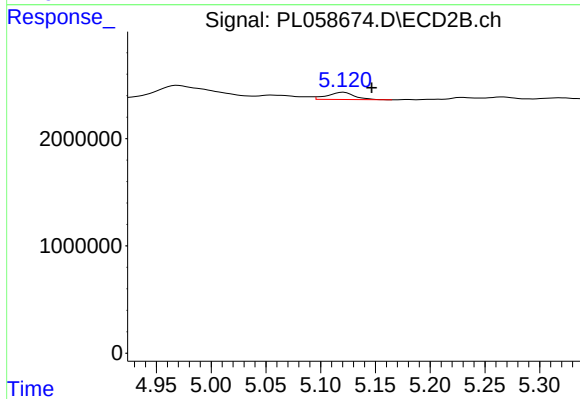

#7 delta-BHC


R.T.: 5.121 min
Delta R.T.: -0.025 min
Response: 1177352
Conc: 0.41 ng/ml

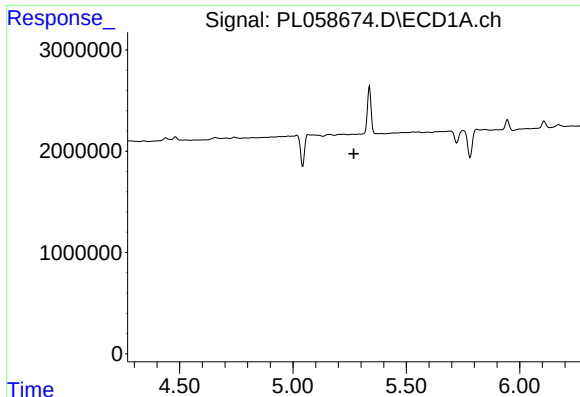

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

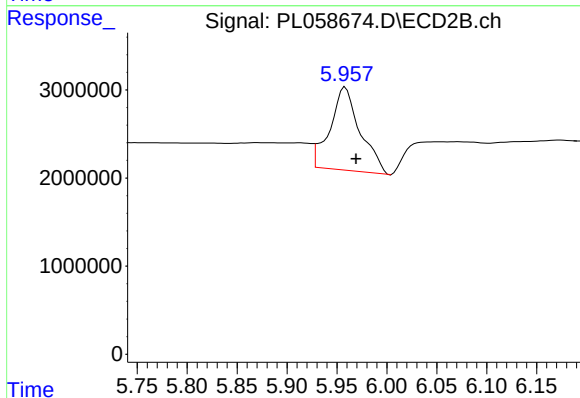


#8 Heptachlor epoxide

R.T.: 5.958 min
Delta R.T.: -0.011 min
Response: 19805689
Conc: 8.25 ng/ml

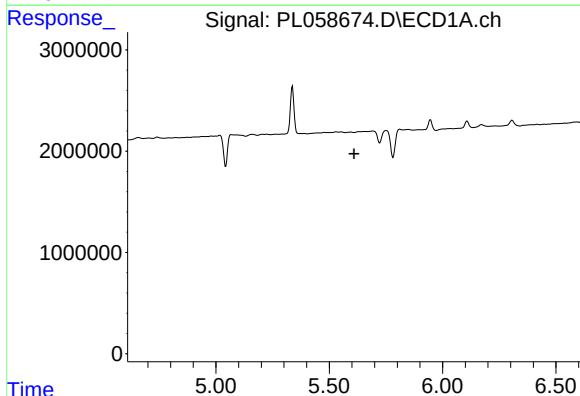


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.609 min
Response: 0
Conc: N.D.

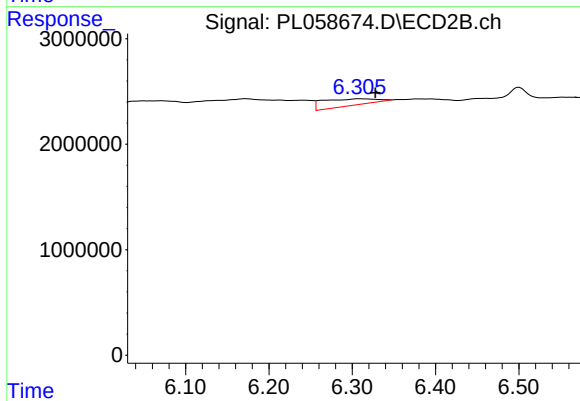

#9 Endosulfan I


R.T.: 6.307 min
Delta R.T.: -0.020 min
Response: 2862479
Conc: 1.33 ng/ml

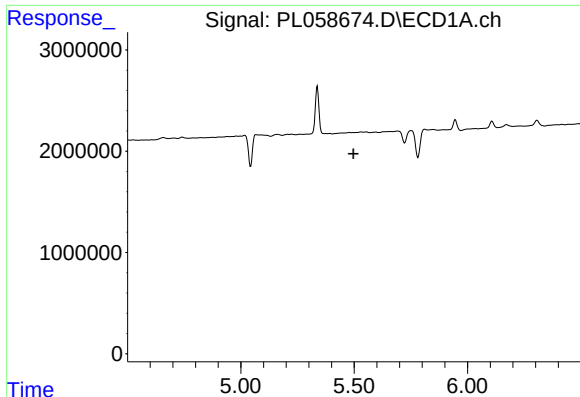

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

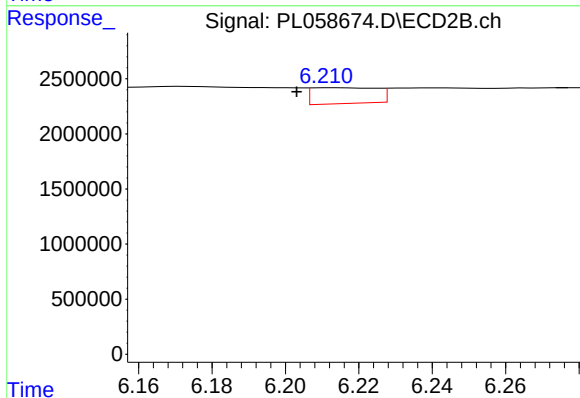


#10 gamma-Chlordane

R.T.: 6.213 min
Delta R.T.: 0.009 min
Response: 1781022
Conc: 0.76 ng/ml

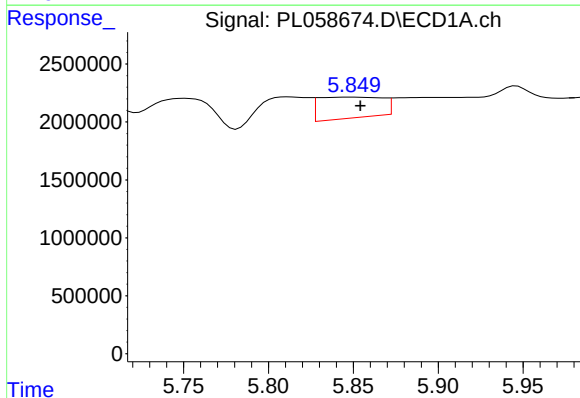


#13 Dieldrin

R.T.: 5.849 min
Delta R.T.: -0.006 min
Response: 4710674
Conc: 3.16 ng/ml

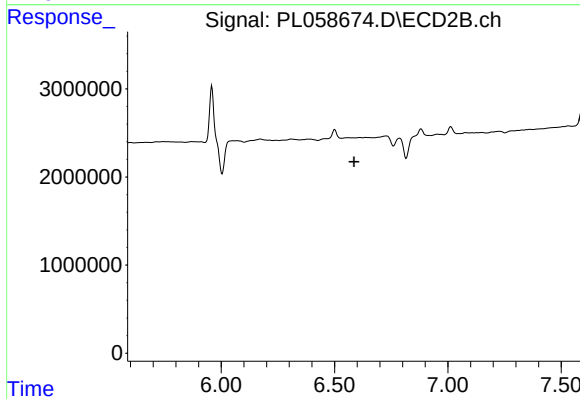

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.586 min
Response: 0
Conc: N.D.

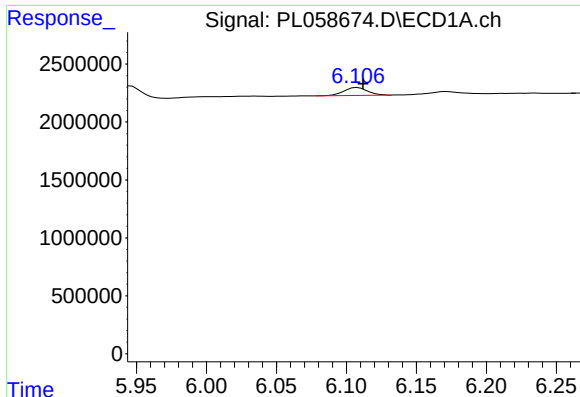

#14 Endrin


R.T.: 6.108 min
Delta R.T.: -0.004 min
Response: 803056
Conc: 0.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

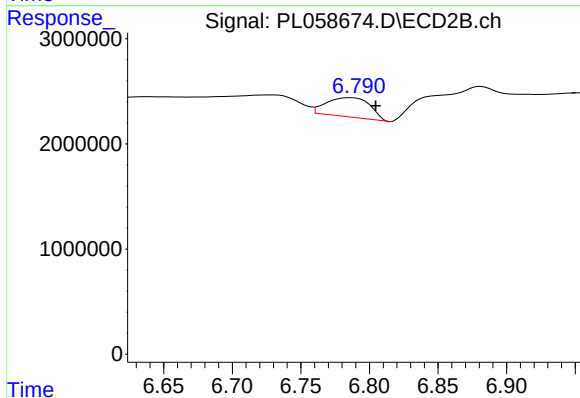


#14 Endrin

R.T.: 6.787 min
Delta R.T.: -0.018 min
Response: 4106346
Conc: 2.26 ng/ml

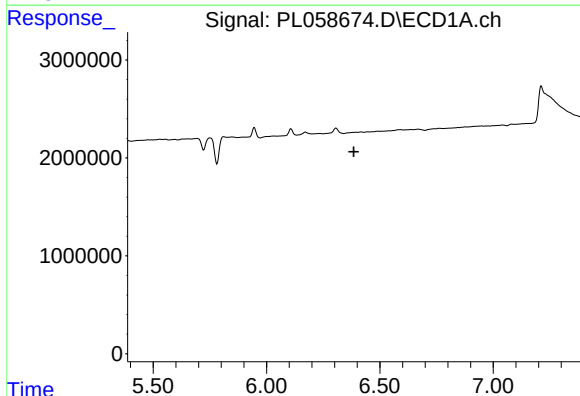


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.385 min
Response: 0
Conc: N.D.

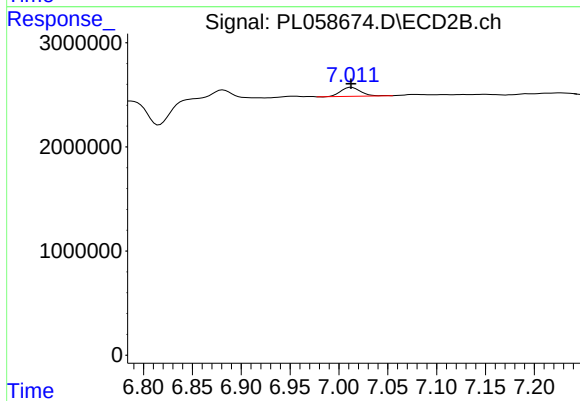

#15 Endosulfan II


R.T.: 7.013 min
Delta R.T.: 0.000 min
Response: 1188057
Conc: 0.59 ng/ml

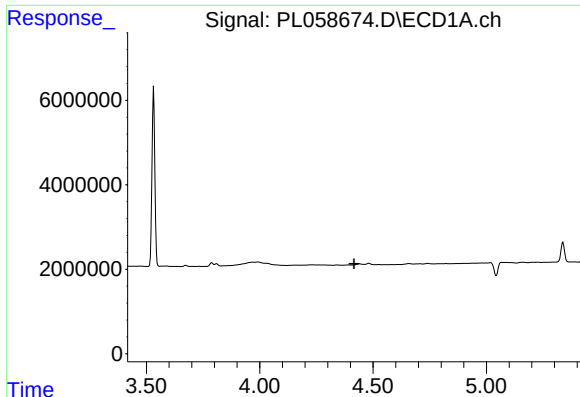

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

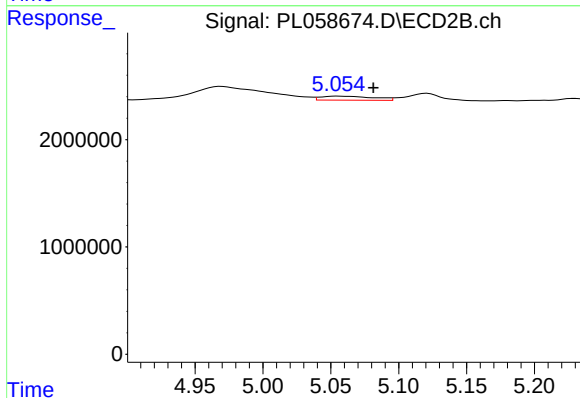


#23 Chlordane-1

R.T.: 5.055 min
Delta R.T.: -0.027 min
Response: 1027675
Conc: 12.84 ng/ml

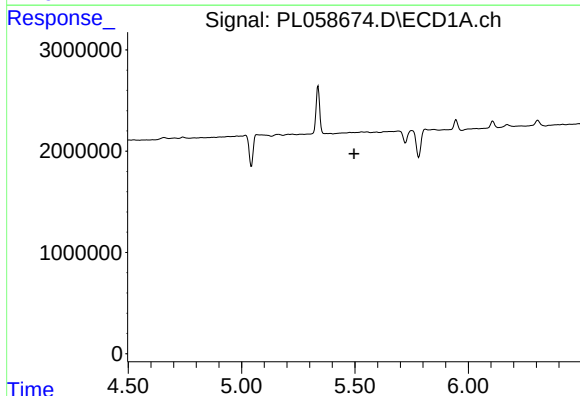


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

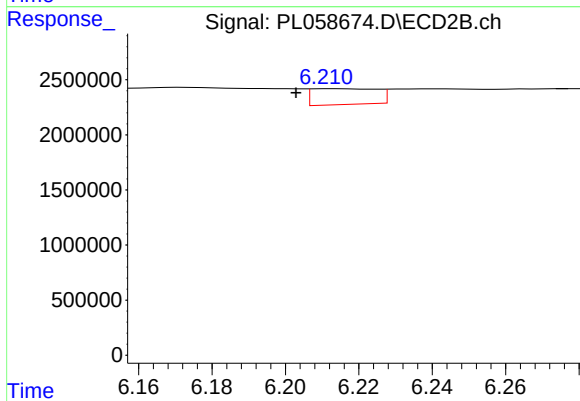

#25 Chlordane-3


R.T.: 6.213 min
Delta R.T.: 0.010 min
Response: 1781022
Conc: 5.88 ng/ml

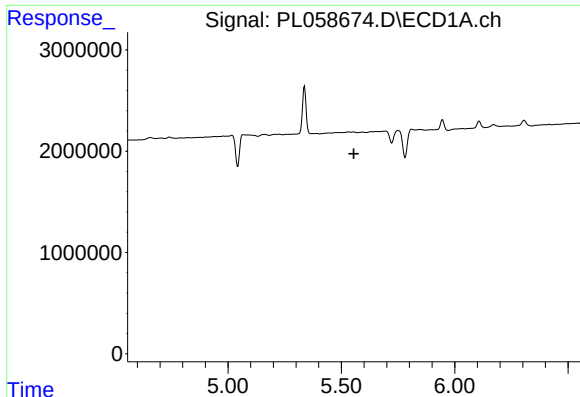

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.555 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

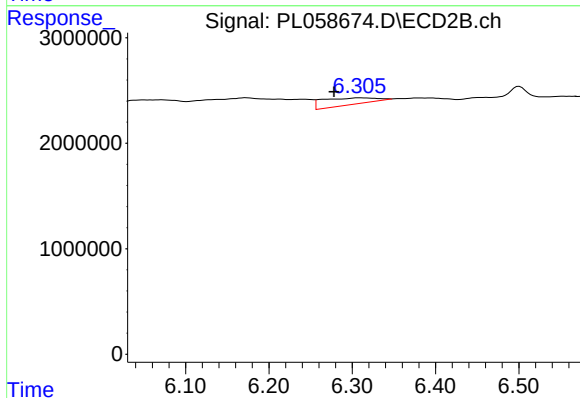


#26 Chlordane-4

R.T.: 6.307 min
Delta R.T.: 0.029 min
Response: 2862479
Conc: 7.85 ng/ml

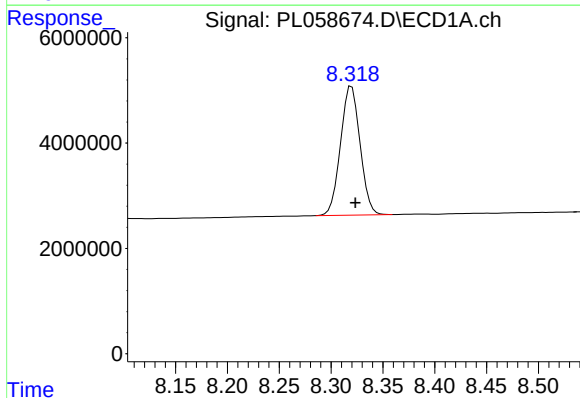

#28 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: -0.004 min
Response: 32151872
Conc: 24.62 ng/ml

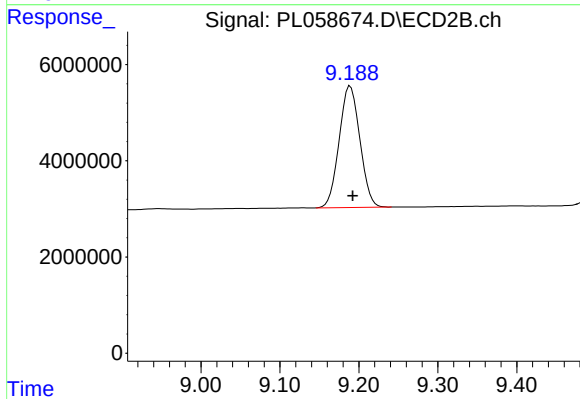

#28 Decachlorobiphenyl

R.T.: 9.189 min
Delta R.T.: -0.003 min
Response: 46200790
Conc: 26.14 ng/ml