

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051320\
 Data File : PL058676.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2020 11:09
 Operator : AJ\MA
 Sample : PB128770BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 01:53:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Wed May 13 09:14:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.532	4.077	36823081	51333380	22.414	23.715
28)	SA Decachlor...	8.319	9.190	32464285	47266583	24.862	26.745
Target Compounds							
7)	B delta-BHC	0.000	5.121f	0	1228706	N.D.	0.433 #
8)	B Heptachlo...	0.000	5.958	0	3436430	N.D.	1.431 #
9)	A Endosulfan I	0.000	6.314	0	541864	N.D.	0.252 #
10)	B gamma-Chl...	0.000	6.177f	0	1796191	N.D.	0.765 #
11)	B alpha-Chl...	0.000	6.249f	0	373867	N.D.	0.159 #
13)	MA Dieldrin	5.844	0.000	453913	0	0.305	N.D. #
14)	MA Endrin	0.000	6.796	0	2115735	N.D.	1.167 #
15)	B Endosulfa...	0.000	7.012	0	1220208	N.D.	0.611 #
16)	A 4,4'-DDD	0.000	6.949f	0	475109	N.D.	0.271 #
23)	Chlordane-1	0.000	5.059f	0	967436	N.D.	12.089 #
25)	Chlordane-3	0.000	6.177f	0	1796191	N.D.	5.930 #
26)	Chlordane-4	0.000	6.249f	0	373867	N.D.	1.026 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051320\
Data File : PL058676.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2020 11:09
Operator : AJ\MA
Sample : PB128770BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 01:53:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Wed May 13 09:14:54 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

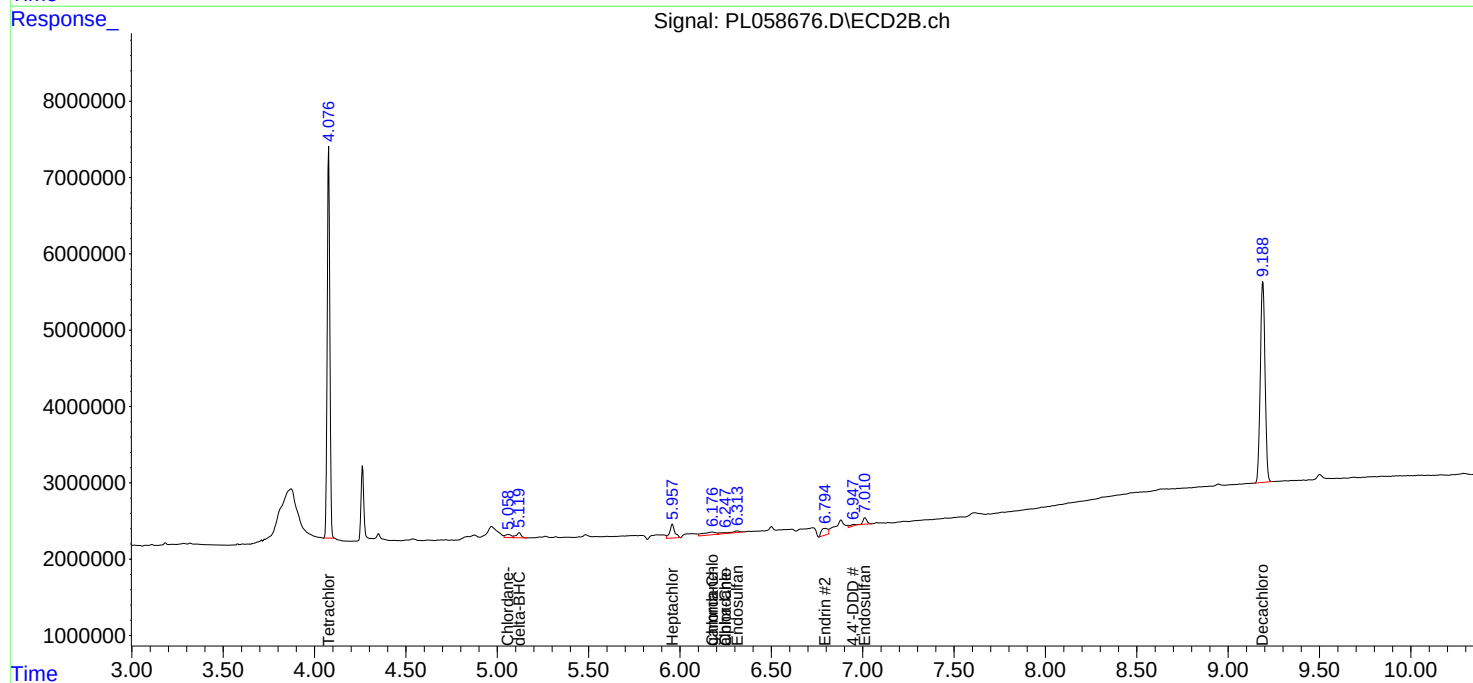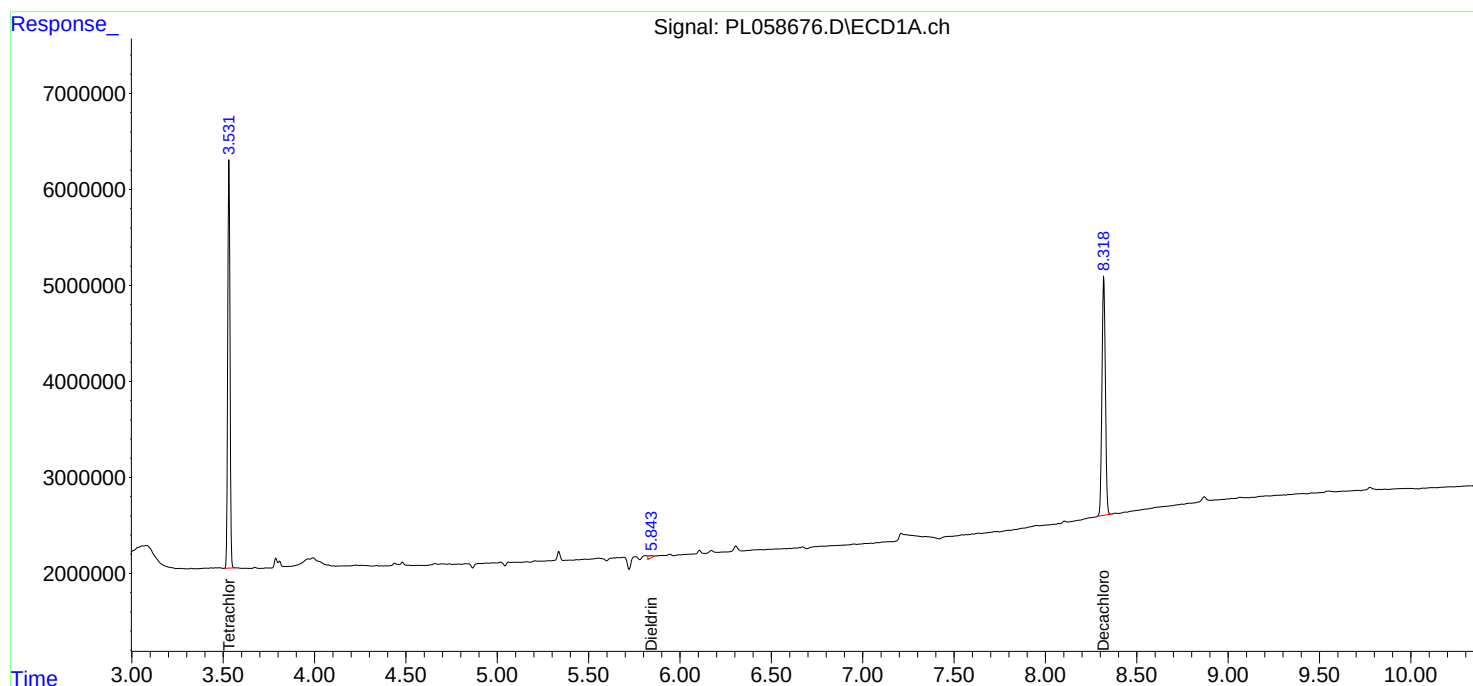


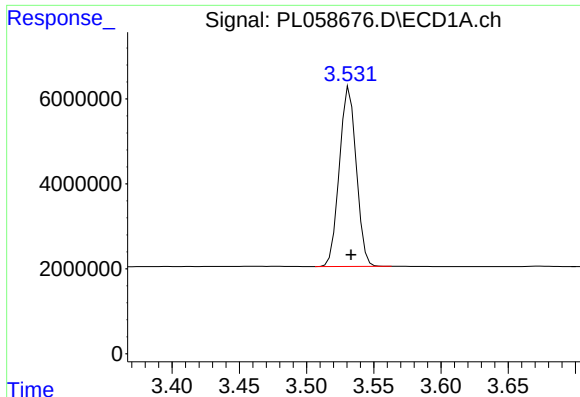

#1 Tetrachloro-m-xylene


R.T.: 3.532 min
Delta R.T.: -0.001 min
Response: 36823081
Conc: 22.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

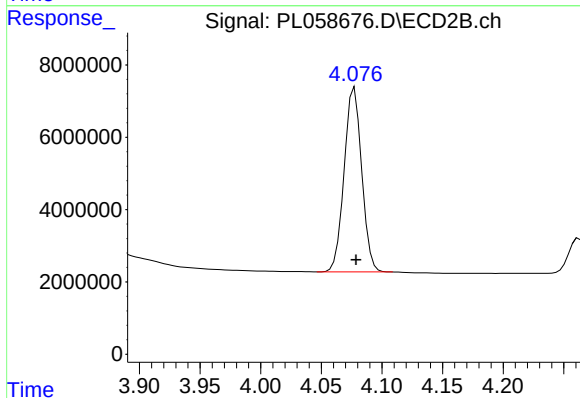


#1 Tetrachloro-m-xylene

R.T.: 4.077 min
Delta R.T.: -0.001 min
Response: 51333380
Conc: 23.71 ng/ml

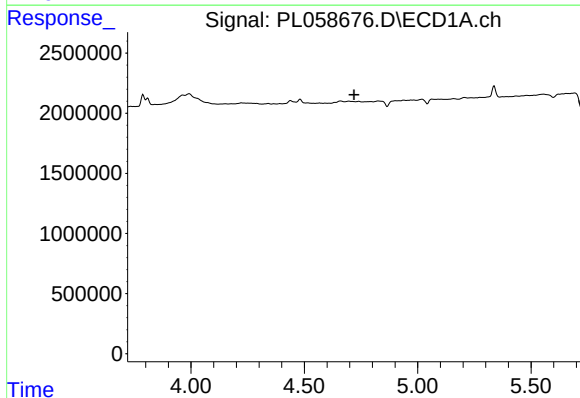


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.719 min
Response: 0
Conc: N.D.

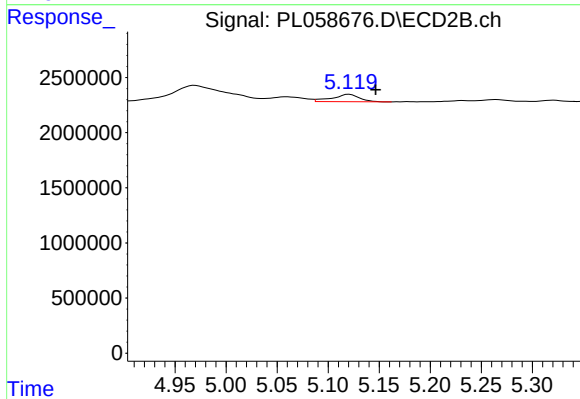

#7 delta-BHC


R.T.: 5.121 min
Delta R.T.: -0.026 min
Response: 1228706
Conc: 0.43 ng/ml

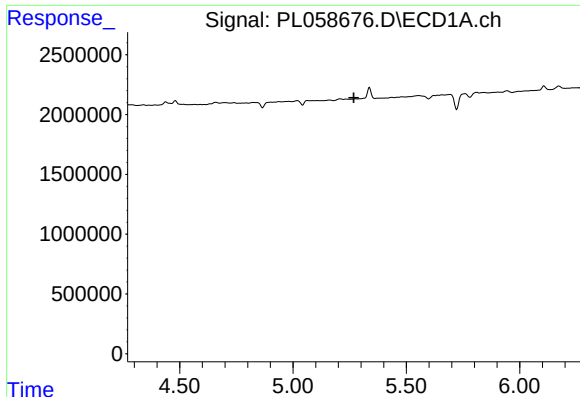

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

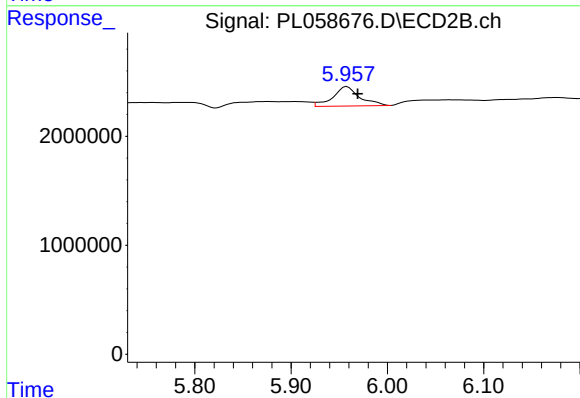


#8 Heptachlor epoxide

R.T.: 5.958 min
Delta R.T.: -0.011 min
Response: 3436430
Conc: 1.43 ng/ml

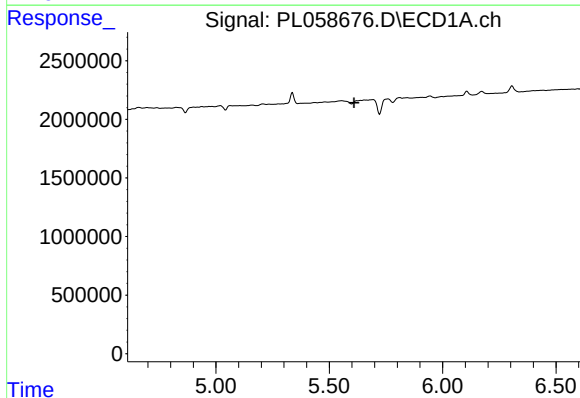


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.609 min
Response: 0
Conc: N.D.

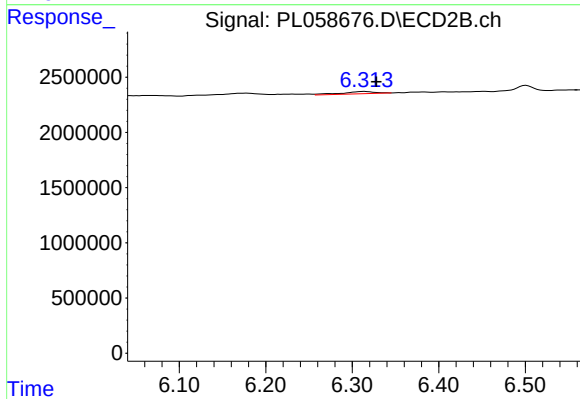

#9 Endosulfan I


R.T.: 6.314 min
Delta R.T.: -0.013 min
Response: 541864
Conc: 0.25 ng/ml

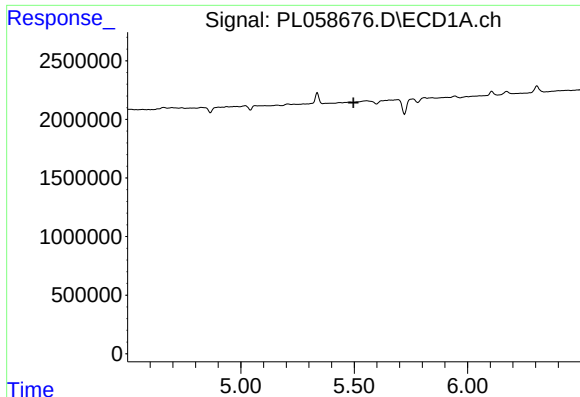

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

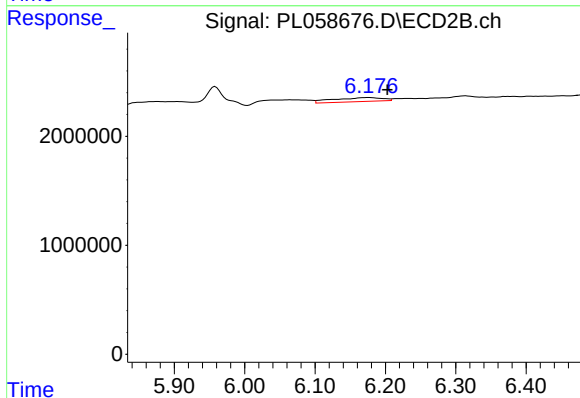


#10 gamma-Chlordane

R.T.: 6.177 min
Delta R.T.: -0.026 min
Response: 1796191
Conc: 0.76 ng/ml

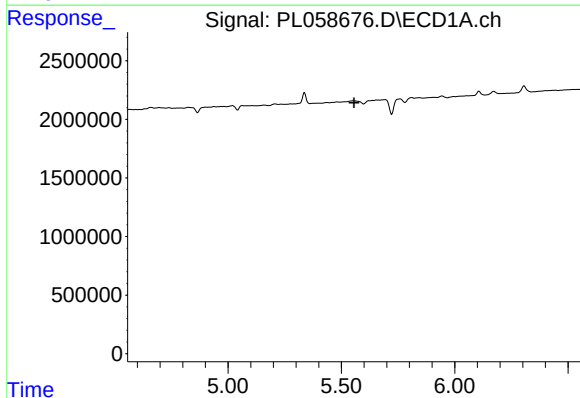


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.556 min
Response: 0
Conc: N.D.

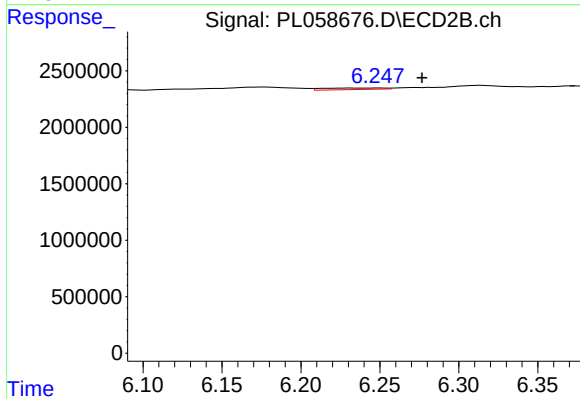

#11 alpha-Chlordane


R.T.: 6.249 min
Delta R.T.: -0.028 min
Response: 373867
Conc: 0.16 ng/ml

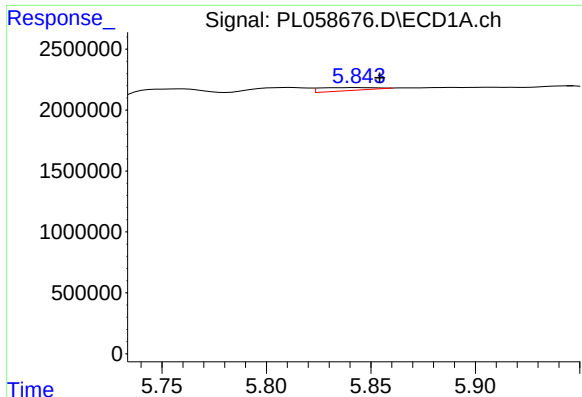

#13 Dieldrin


R.T.: 5.844 min
Delta R.T.: -0.010 min
Response: 453913
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

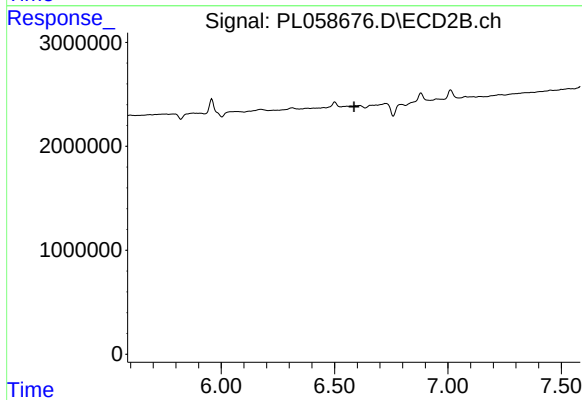


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.586 min
Response: 0
Conc: N.D.

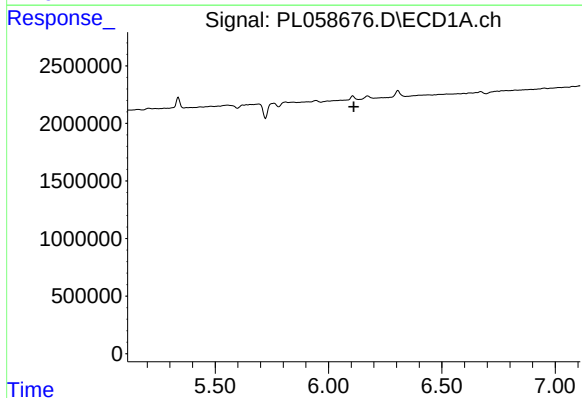


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

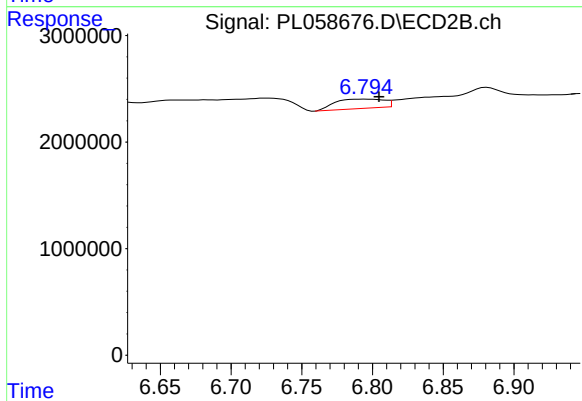

#14 Endrin


R.T.: 6.796 min
Delta R.T.: -0.009 min
Response: 2115735
Conc: 1.17 ng/ml

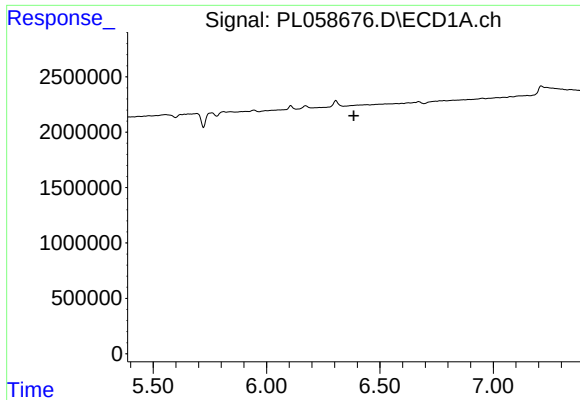

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.385 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

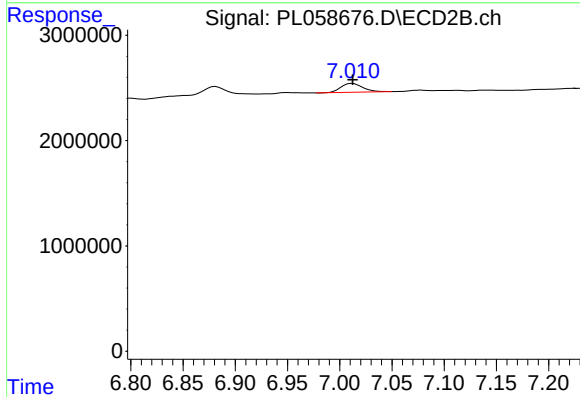


#15 Endosulfan II

R.T.: 7.012 min
Delta R.T.: 0.000 min
Response: 1220208
Conc: 0.61 ng/ml

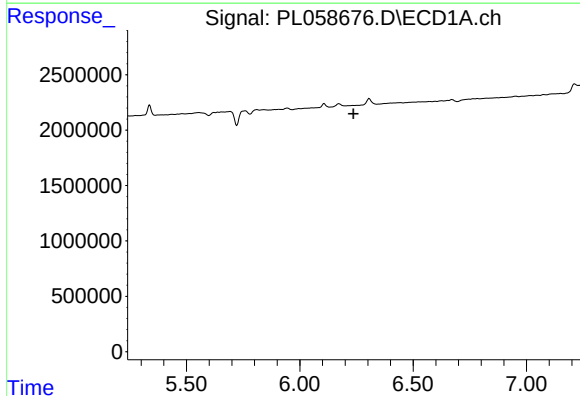


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.237 min
Response: 0
Conc: N.D.

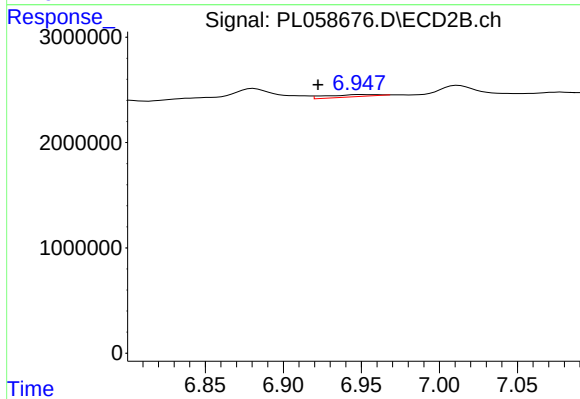

#16 4,4'-DDD


R.T.: 6.949 min
Delta R.T.: 0.027 min
Response: 475109
Conc: 0.27 ng/ml

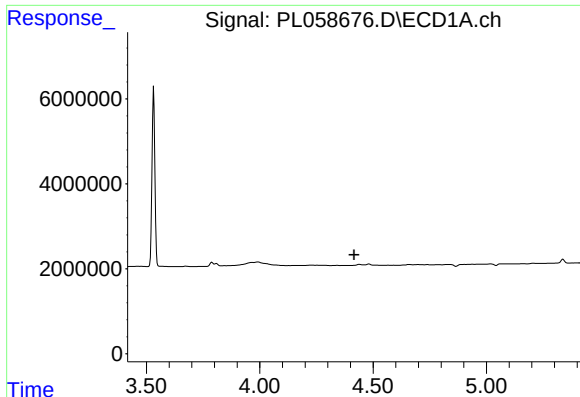

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

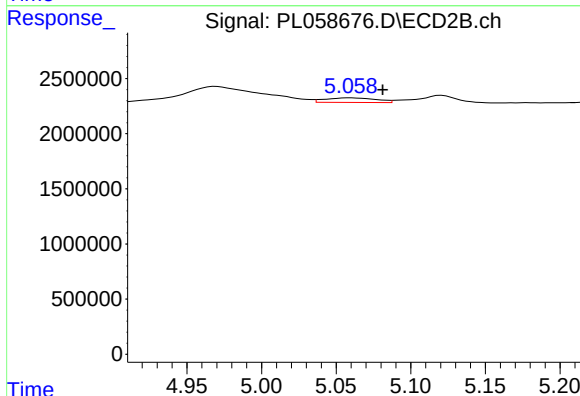


#23 Chlordane-1

R.T.: 5.059 min
Delta R.T.: -0.023 min
Response: 967436
Conc: 12.09 ng/ml

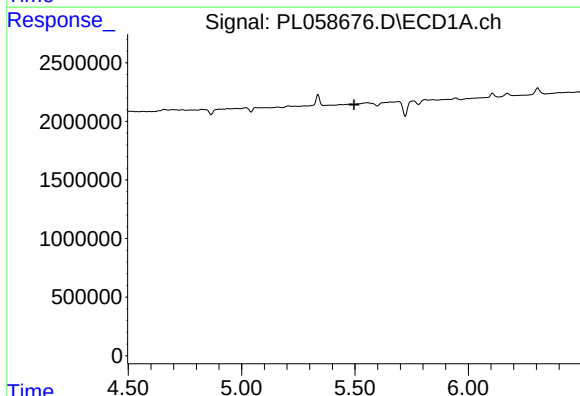


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

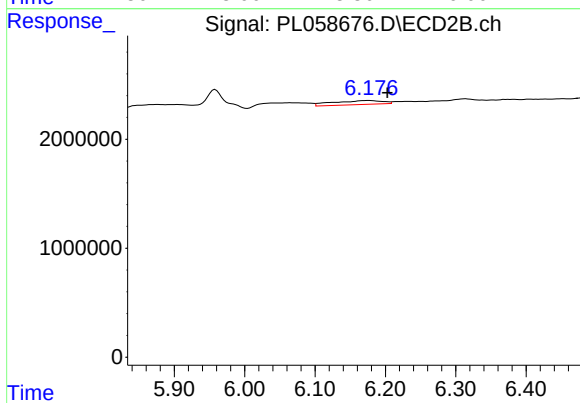

#25 Chlordane-3


R.T.: 6.177 min
Delta R.T.: -0.025 min
Response: 1796191
Conc: 5.93 ng/ml

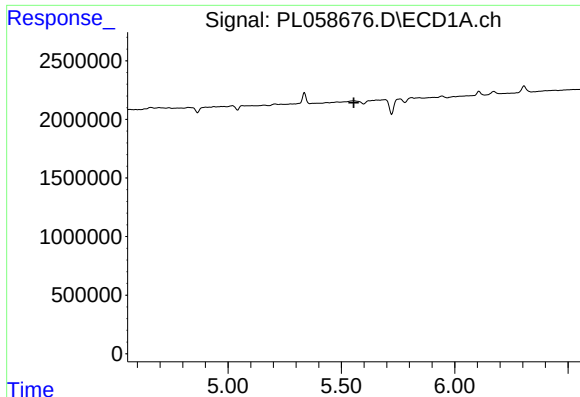

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.555 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

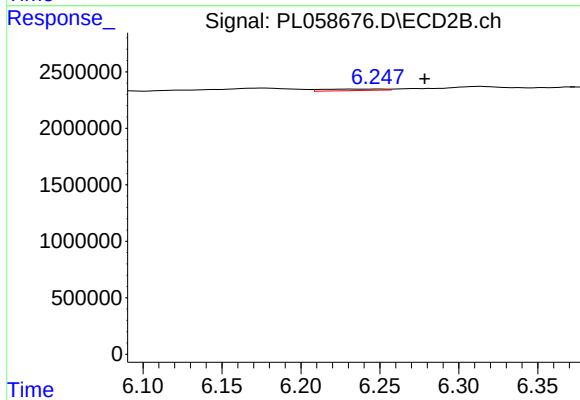


#26 Chlordane-4

R.T.: 6.249 min
Delta R.T.: -0.030 min
Response: 373867
Conc: 1.03 ng/ml

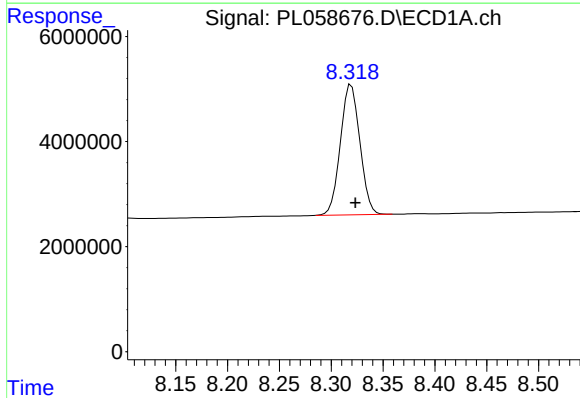

#28 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: -0.004 min
Response: 32464285
Conc: 24.86 ng/ml

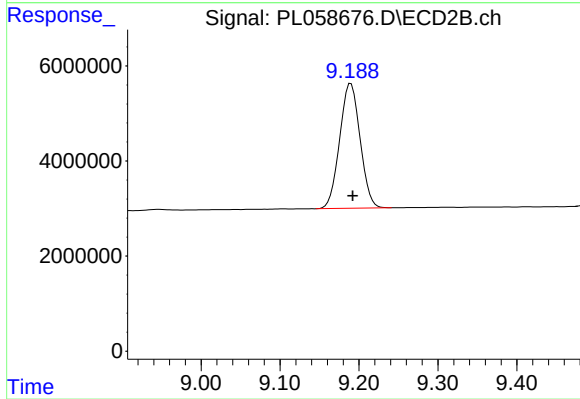

#28 Decachlorobiphenyl

R.T.: 9.190 min
Delta R.T.: -0.002 min
Response: 47266583
Conc: 26.75 ng/ml