

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051320\
 Data File : PL058696.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2020 18:44
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 01:59:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Wed May 13 09:14:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.532	4.078	35968804	50765829	21.894	23.453
28)	SA Decachlor...	8.320	9.192	31814944	46069827	24.365	26.068
Target Compounds							
7)	B delta-BHC	0.000	5.121f	0	1002060	N.D.	0.353 #
8)	B Heptachlo...	0.000	5.959	0	11262353	N.D.	4.690 #
9)	A Endosulfan I	0.000	6.311f	0	1964868	N.D.	0.913 #
10)	B gamma-Chl...	0.000	6.175f	0	5764811	N.D.	2.454 #
12)	B 4,4'-DDE	5.750f	0.000	2852662	0	2.047	N.D. #
14)	MA Endrin	0.000	6.786f	0	2711339	N.D.	1.495 #
15)	B Endosulfa...	0.000	7.014	0	1276798	N.D.	0.639 #
22)	Mirex	0.000	8.319f	0	119758	N.D.	0.076 #
25)	Chlordane-3	0.000	6.175f	0	5764811	N.D.	19.033 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051320\
Data File : PL058696.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2020 18:44
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 01:59:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Wed May 13 09:14:54 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

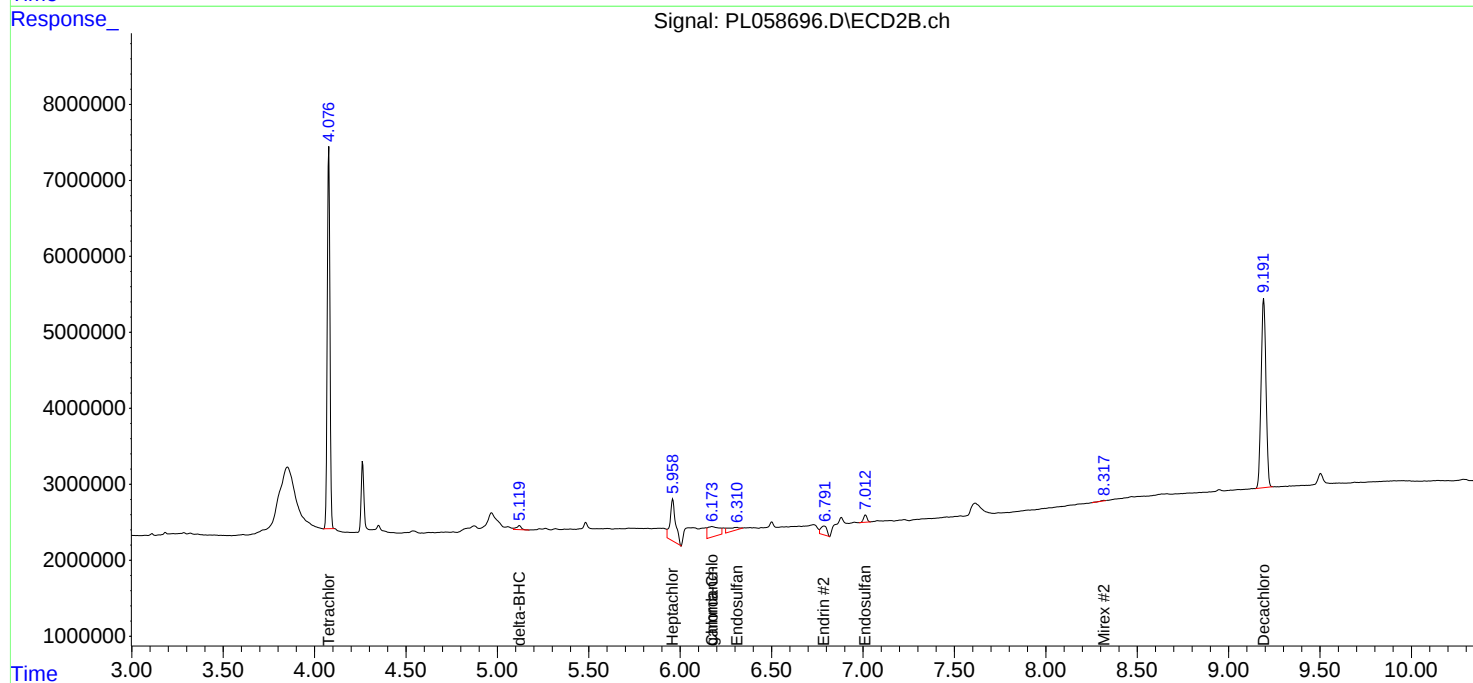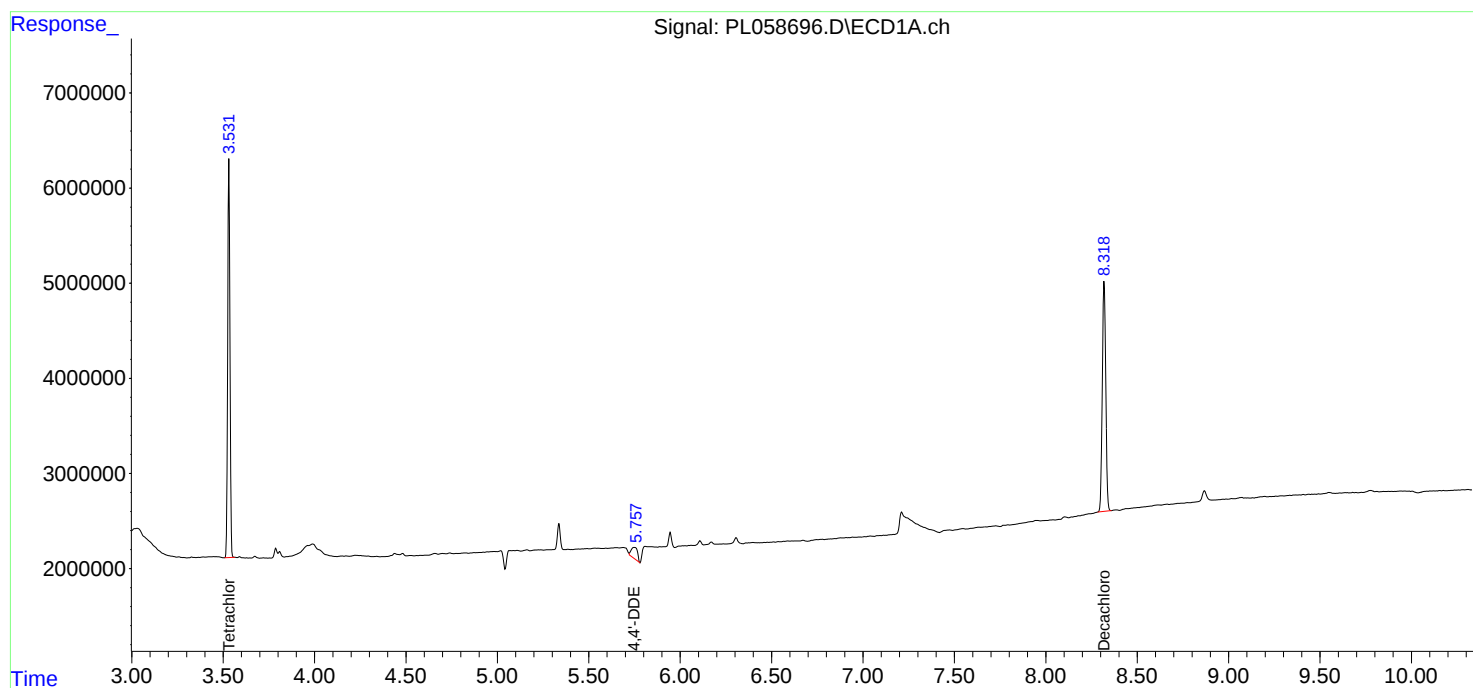


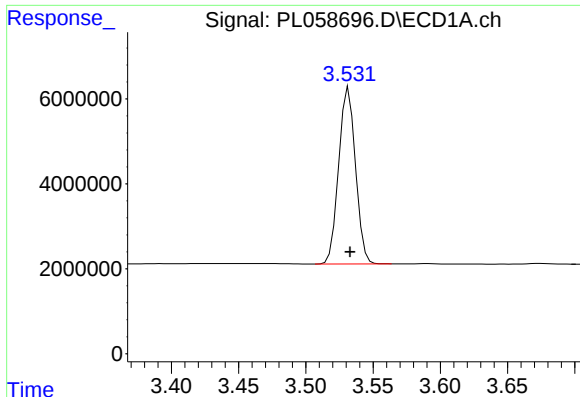

#1 Tetrachloro-m-xylene


R.T.: 3.532 min
Delta R.T.: -0.001 min
Response: 35968804
Conc: 21.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

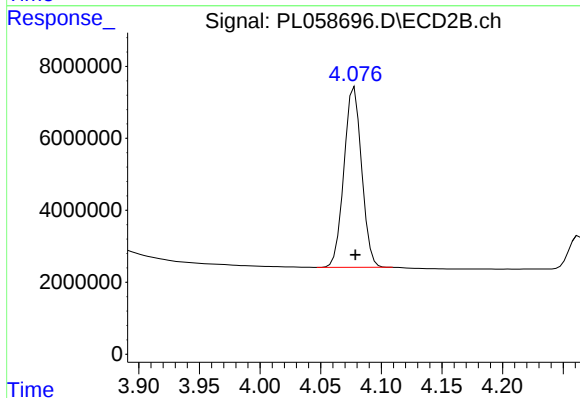


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 50765829
Conc: 23.45 ng/ml

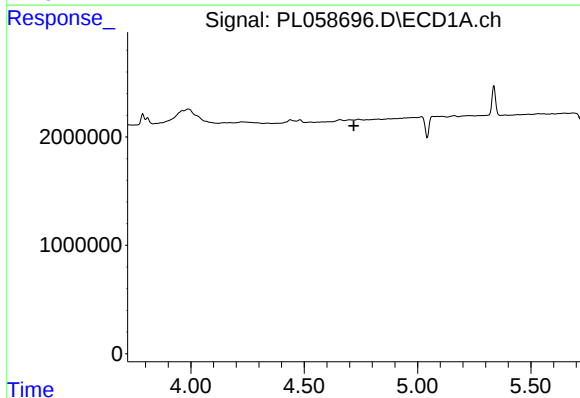


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.719 min
Response: 0
Conc: N.D.

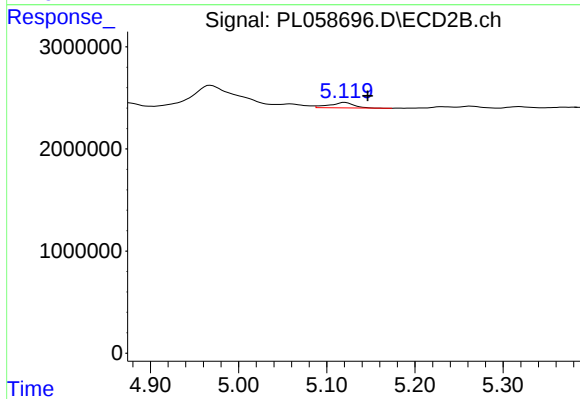

#7 delta-BHC


R.T.: 5.121 min
Delta R.T.: -0.026 min
Response: 1002060
Conc: 0.35 ng/ml

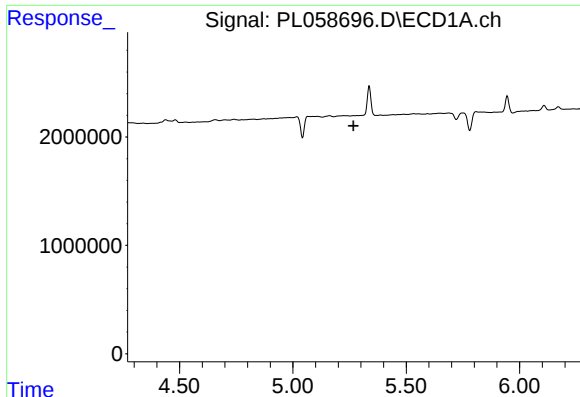

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

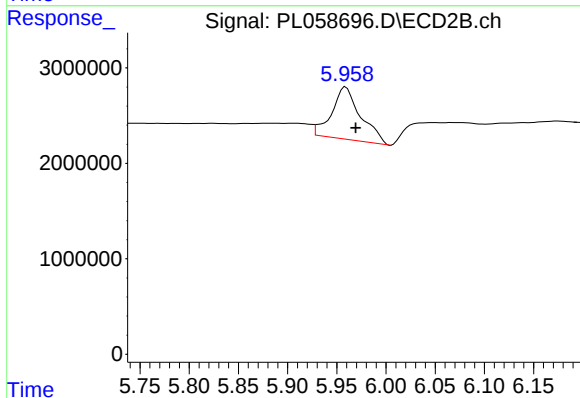


#8 Heptachlor epoxide

R.T.: 5.959 min
Delta R.T.: -0.010 min
Response: 11262353
Conc: 4.69 ng/ml

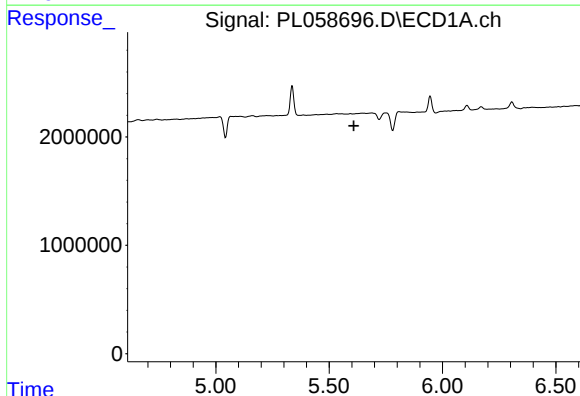


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.609 min
Response: 0
Conc: N.D.

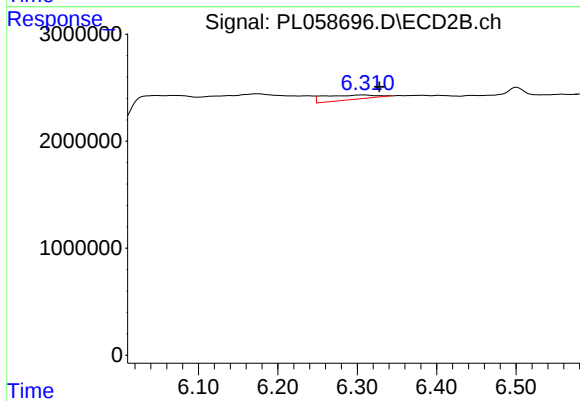

#9 Endosulfan I


R.T.: 6.311 min
Delta R.T.: -0.017 min
Response: 1964868
Conc: 0.91 ng/ml

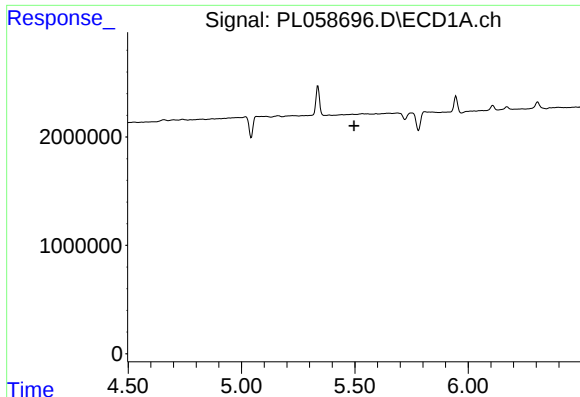

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

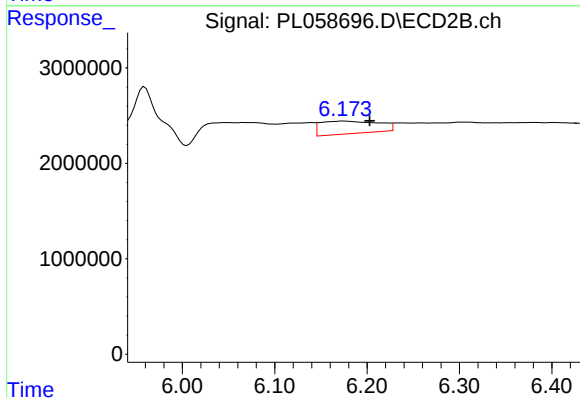


#10 gamma-Chlordane

R.T.: 6.175 min
Delta R.T.: -0.028 min
Response: 5764811
Conc: 2.45 ng/ml

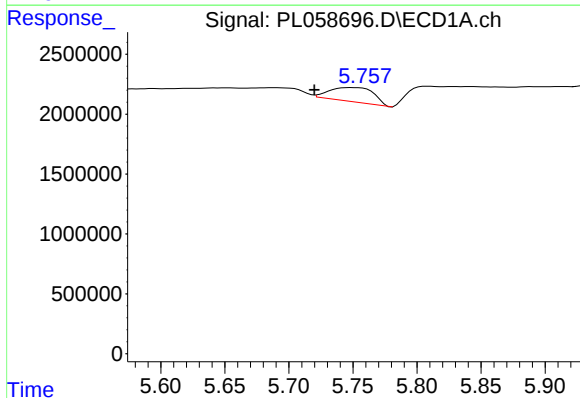


#12 4,4'-DDE

R.T.: 5.750 min
Delta R.T.: 0.030 min
Response: 2852662
Conc: 2.05 ng/ml

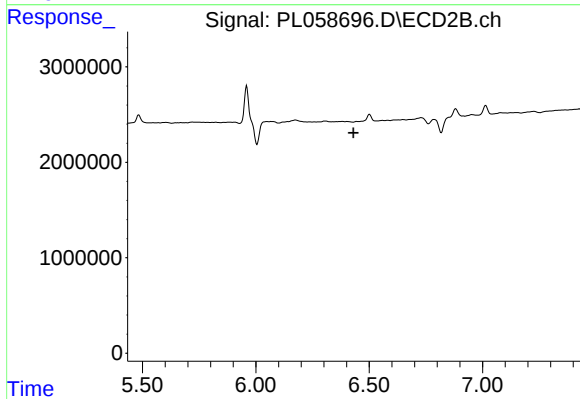

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.431 min
Response: 0
Conc: N.D.

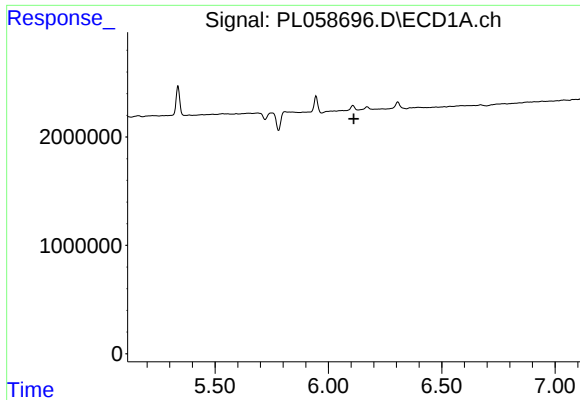

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

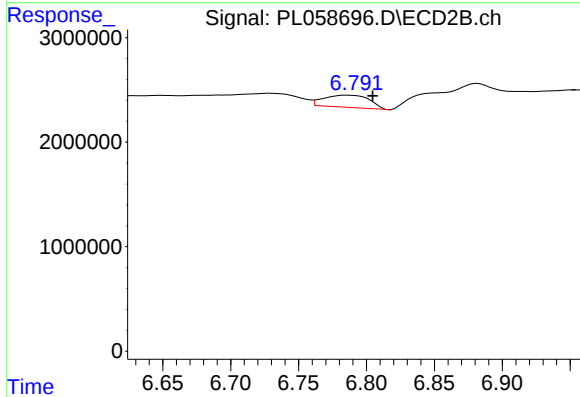


#14 Endrin

R.T.: 6.786 min
Delta R.T.: -0.018 min
Response: 2711339
Conc: 1.50 ng/ml

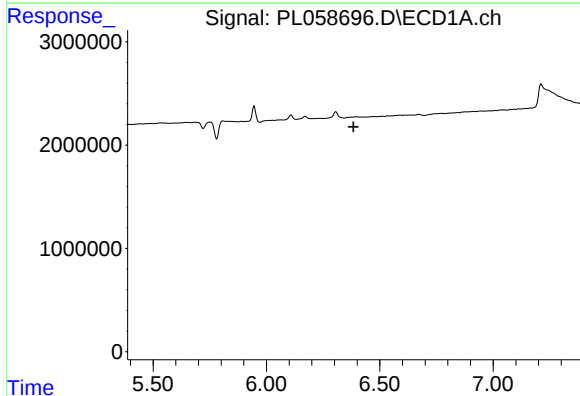


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.385 min
Response: 0
Conc: N.D.

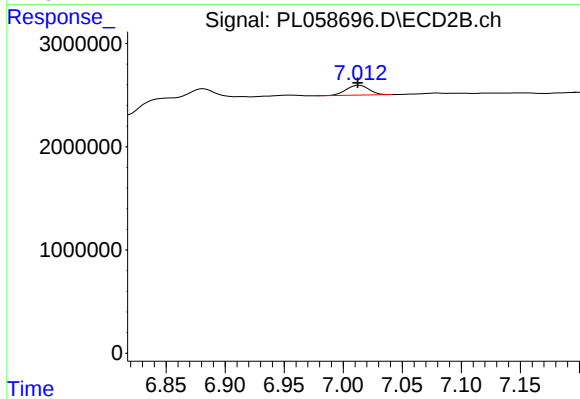

#15 Endosulfan II


R.T.: 7.014 min
Delta R.T.: 0.001 min
Response: 1276798
Conc: 0.64 ng/ml

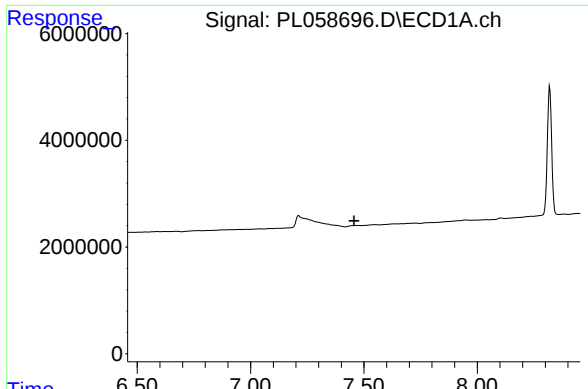

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

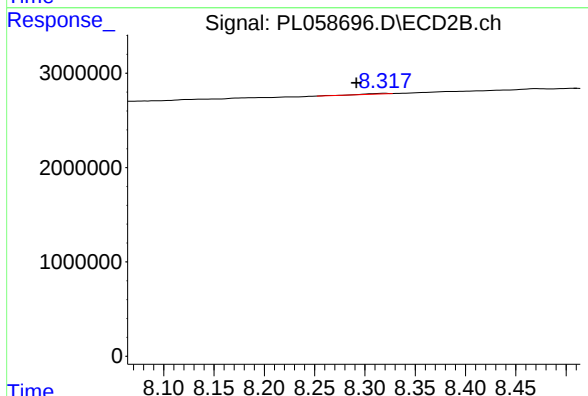


#22 Mirex

R.T.: 8.319 min
Delta R.T.: 0.028 min
Response: 119758
Conc: 0.08 ng/ml

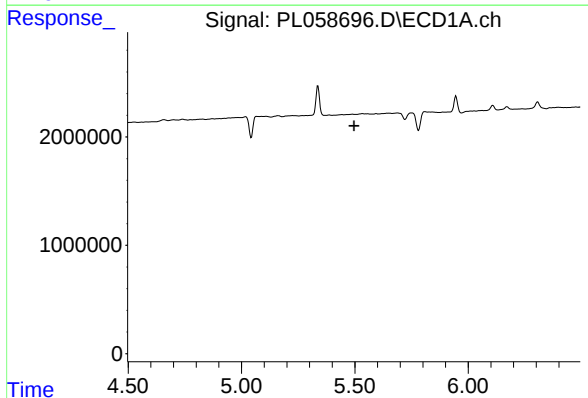


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

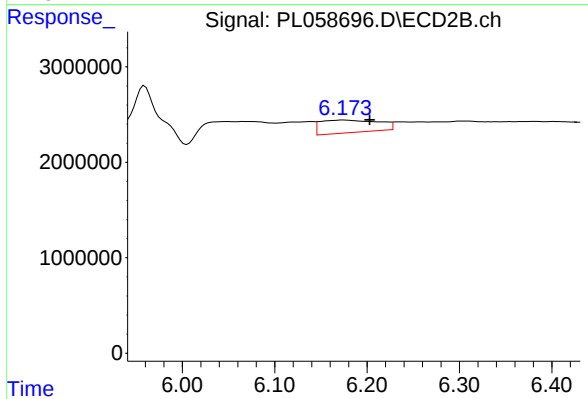

#25 Chlordane-3


R.T.: 6.175 min
Delta R.T.: -0.028 min
Response: 5764811
Conc: 19.03 ng/ml

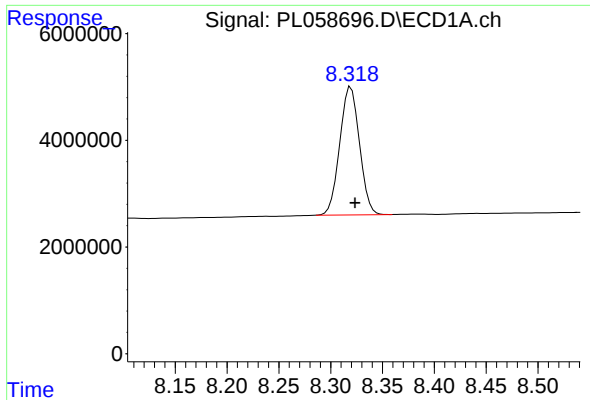

#28 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: -0.004 min
Response: 31814944
Conc: 24.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

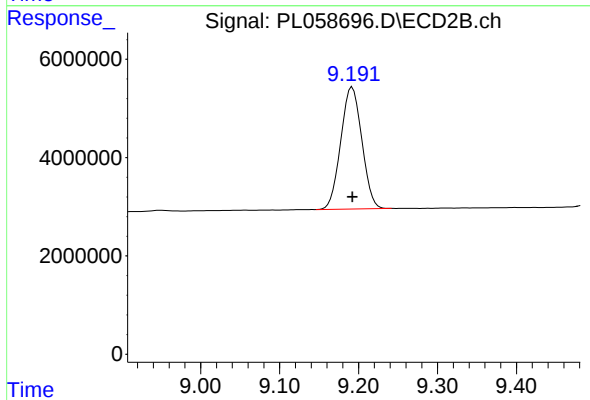

#28 Decachlorobiphenyl

R.T.: 9.192 min
Delta R.T.: 0.000 min
Response: 46069827
Conc: 26.07 ng/ml