

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051322\
 Data File : PL074682.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2022 09:07
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 23:13:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 16:19:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	0.000	10.417	0	590997	N.D.	0.576 #
Target Compounds							
5)	MB Aldrin	0.000	6.533f	0	207785	N.D.	0.138 #
6)	B beta-BHC	0.000	6.128f	0	270150	N.D.	0.340 #
8)	B Heptachlo...	8.130	0.000	7528675	0	13.237	N.D. #
9)	A Endosulfan I	8.512f	7.461f	5753064	2042766	9.979	1.633 #
10)	B gamma-Chl...	0.000	7.338f	0	1268072	N.D.	0.915 #
11)	B alpha-Chl...	0.000	7.411f	0	1382043	N.D.	1.022 #
14)	MA Endrin	0.000	8.084f	0	40525265	N.D.	38.365 #
15)	B Endosulfa...	0.000	8.374	0	817824	N.D.	0.724 #
17)	MA 4,4'-DDT	0.000	8.488	0	333370	N.D.	0.333 #
19)	B Endosulfa...	0.000	8.808f	0	257705	N.D.	0.237 #
22)	Mirex	10.673f	0.000	49602	0	0.123	N.D. #
25)	Chlordane-3	0.000	7.338f	0	1268072	N.D.	9.770 #
26)	Chlordane-4	0.000	7.411f	0	1382043	N.D.	10.081 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051322\
Data File : PL074682.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2022 09:07
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 23:13:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 16:19:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

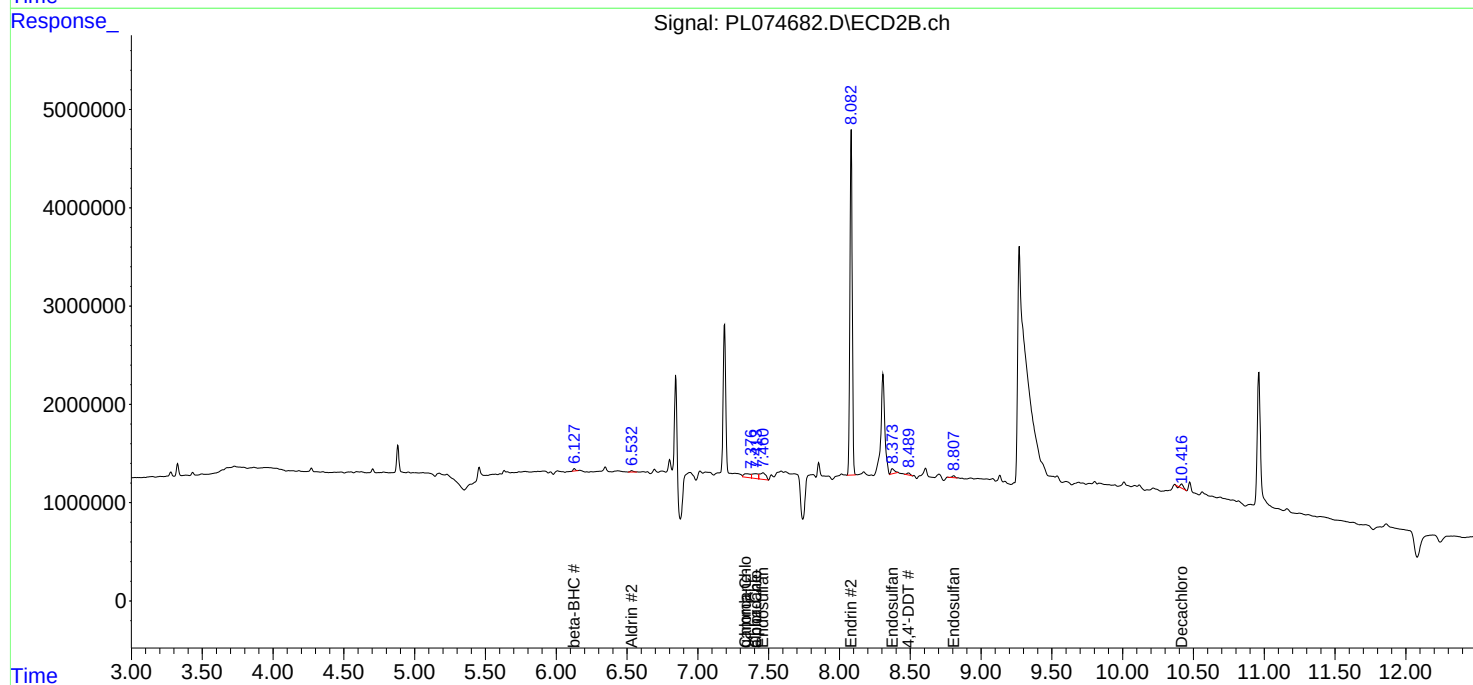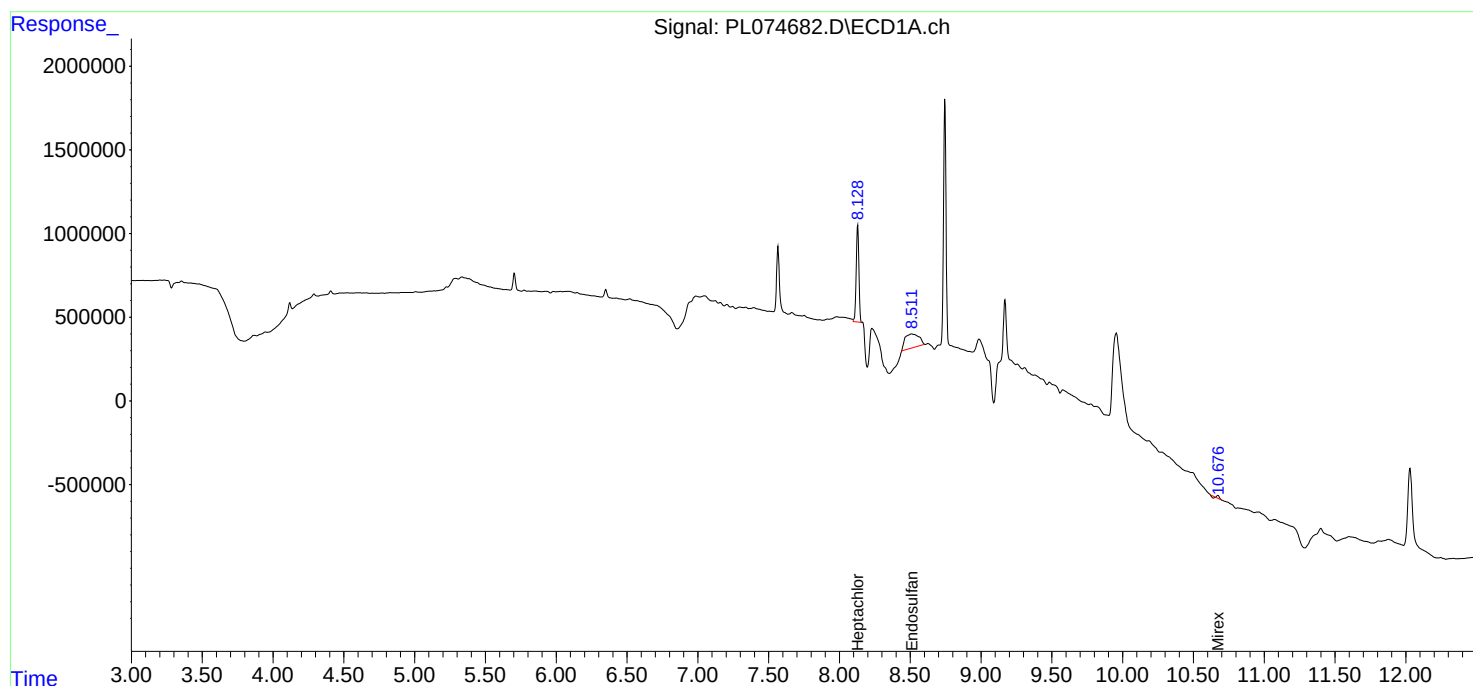


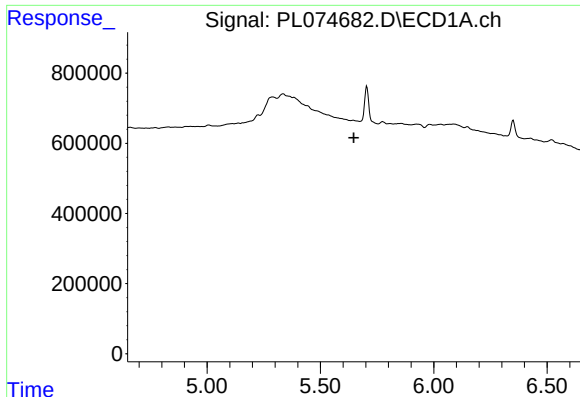

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 5.647 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

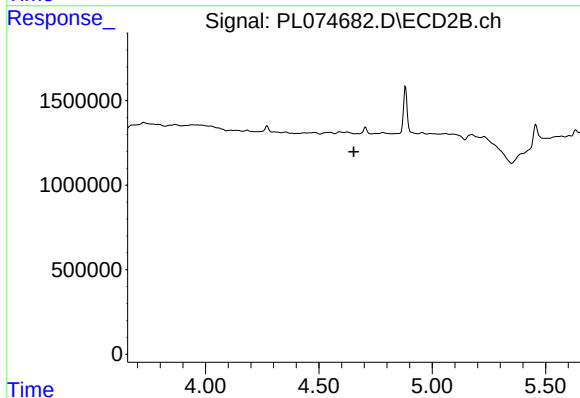


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.654 min
Response: 0
Conc: N.D.

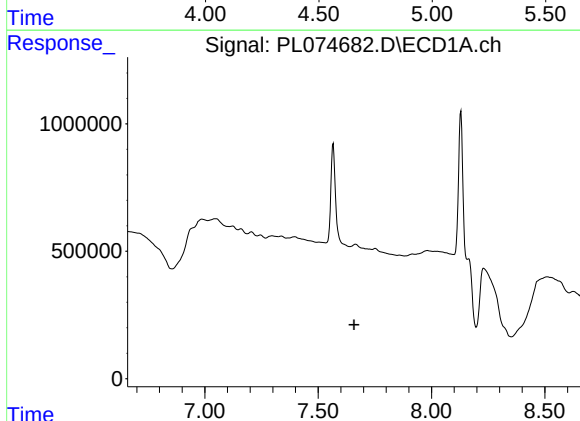


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.659 min
Response: 0
Conc: N.D.

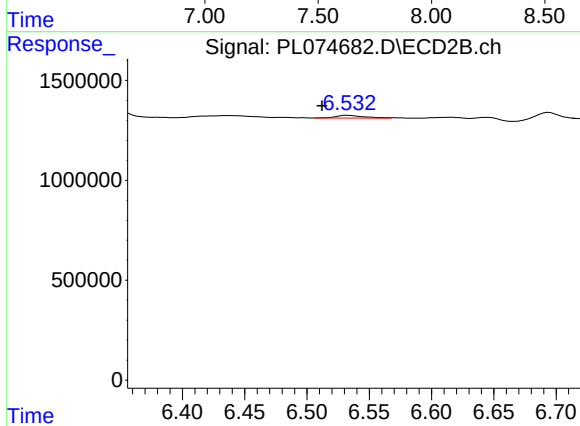

#5 Aldrin


R.T.: 6.533 min
Delta R.T.: 0.021 min
Response: 207785
Conc: 0.14 ng/ml

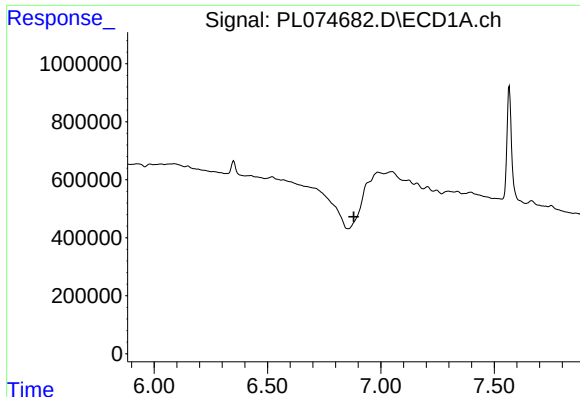

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.881 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

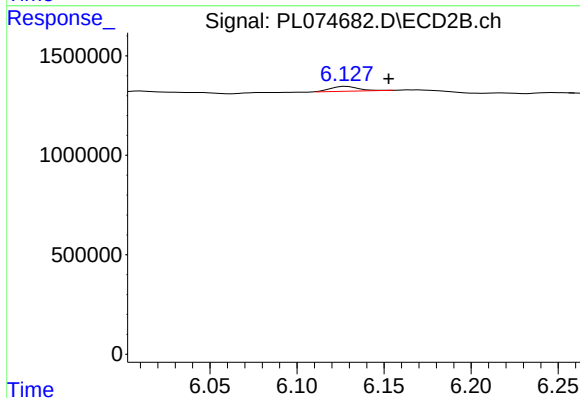


#6 beta-BHC

R.T.: 6.128 min
Delta R.T.: -0.024 min
Response: 270150
Conc: 0.34 ng/ml

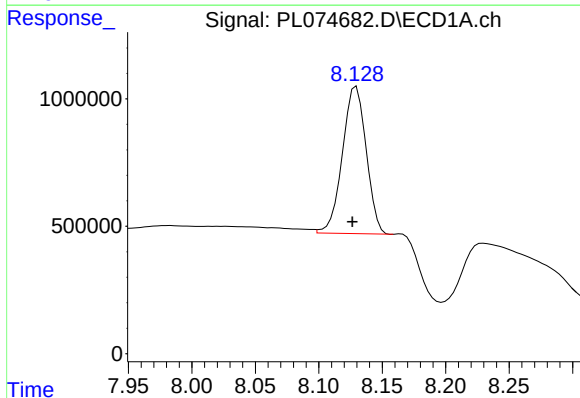


#8 Heptachlor epoxide

R.T.: 8.130 min
Delta R.T.: 0.003 min
Response: 7528675
Conc: 13.24 ng/ml

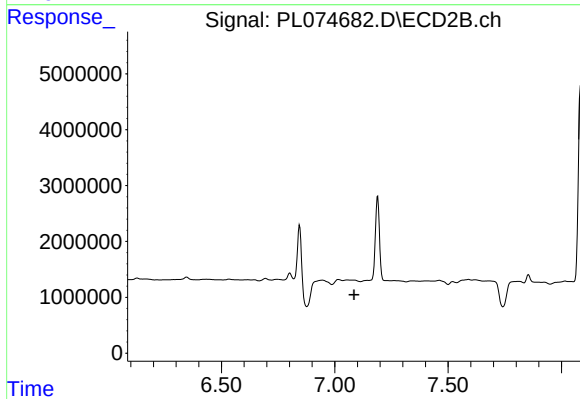

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.086 min
Response: 0
Conc: N.D.

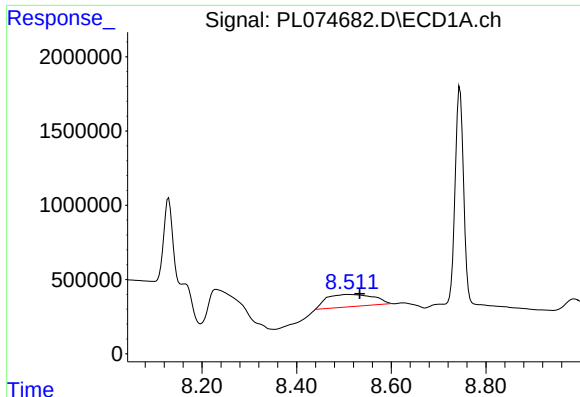

#9 Endosulfan I


R.T.: 8.512 min
Delta R.T.: -0.022 min
Response: 5753064
Conc: 9.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

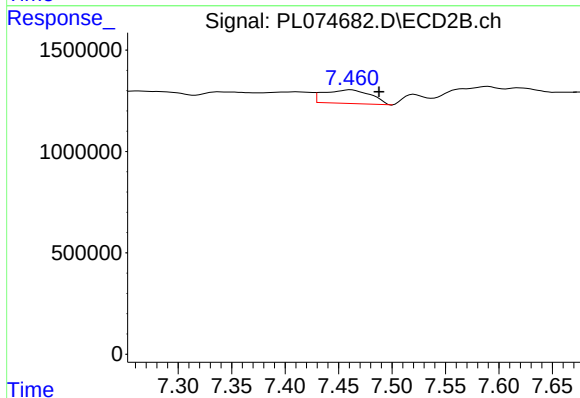


#9 Endosulfan I

R.T.: 7.461 min
Delta R.T.: -0.027 min
Response: 2042766
Conc: 1.63 ng/ml

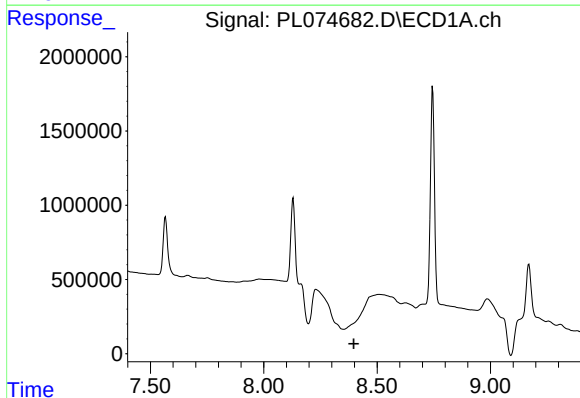


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.398 min
Response: 0
Conc: N.D.

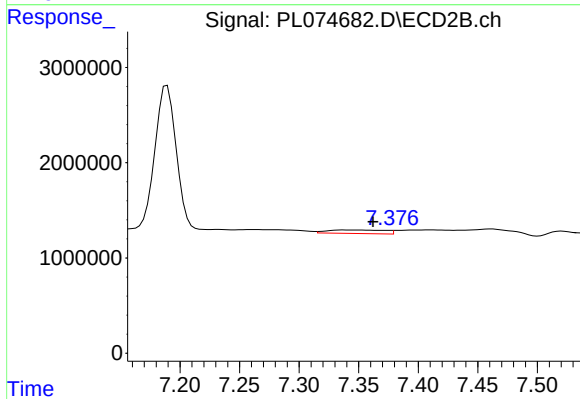

#10 gamma-Chlordane


R.T.: 7.338 min
Delta R.T.: -0.024 min
Response: 1268072
Conc: 0.92 ng/ml

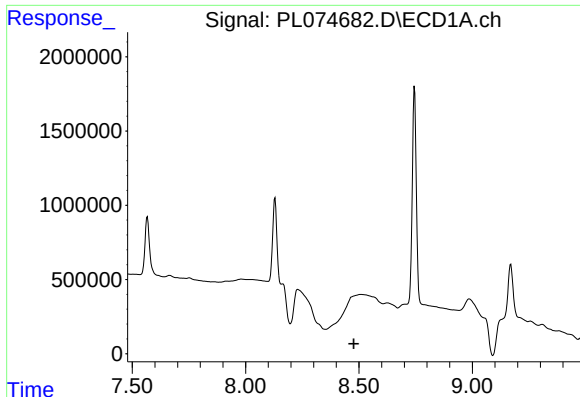

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

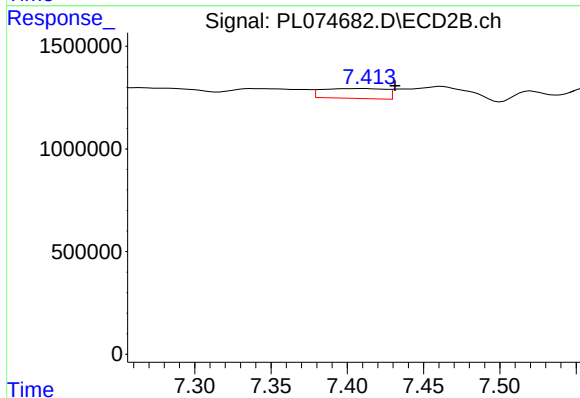


#11 alpha-Chlordane

R.T.: 7.411 min
Delta R.T.: -0.020 min
Response: 1382043
Conc: 1.02 ng/ml

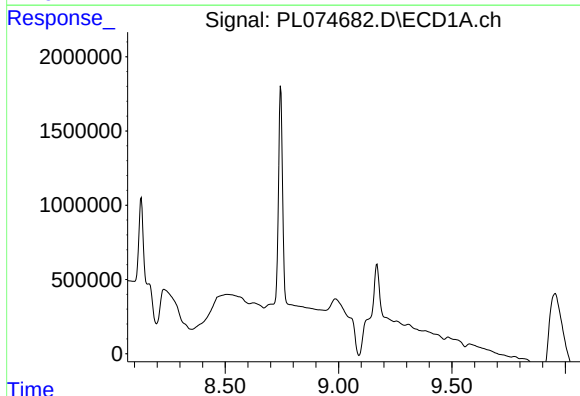


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.067 min
Response: 0
Conc: N.D.

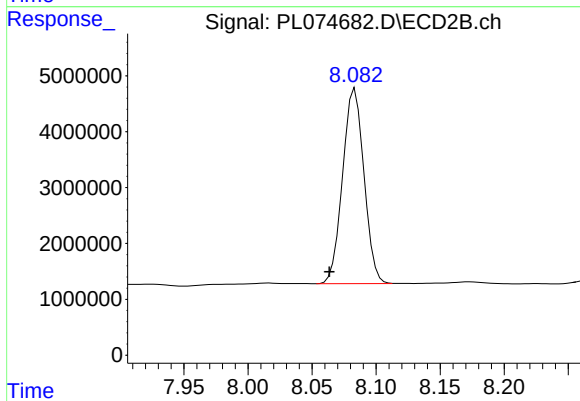

#14 Endrin


R.T.: 8.084 min
Delta R.T.: 0.020 min
Response: 40525265
Conc: 38.37 ng/ml

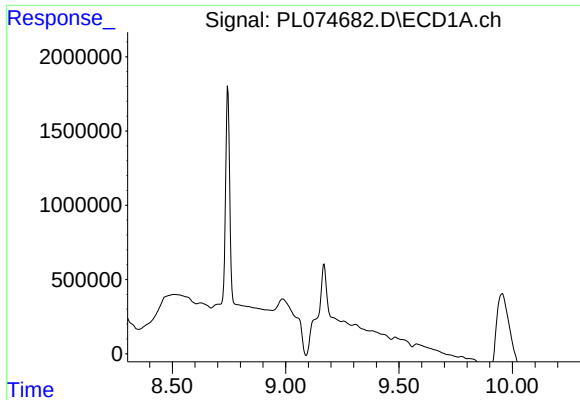

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 9.301 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

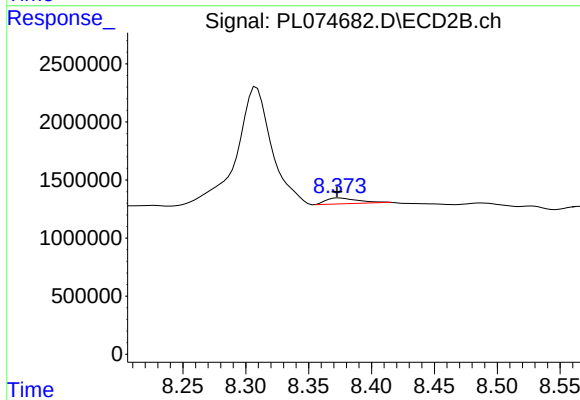


#15 Endosulfan II

R.T.: 8.374 min
Delta R.T.: 0.002 min
Response: 817824
Conc: 0.72 ng/ml

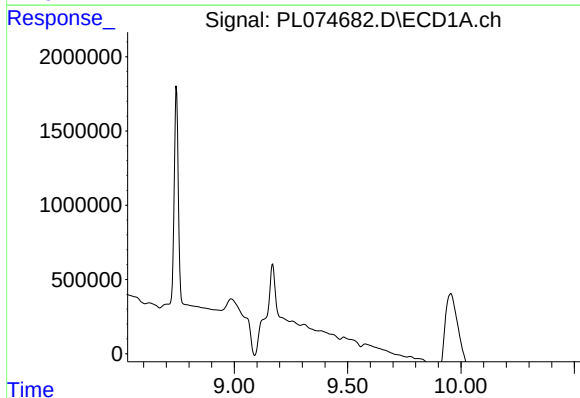


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 9.526 min
Response: 0
Conc: N.D.

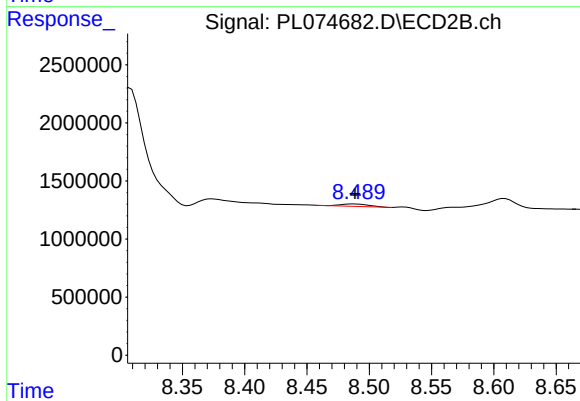

#17 4,4'-DDT


R.T.: 8.488 min
Delta R.T.: 0.000 min
Response: 333370
Conc: 0.33 ng/ml

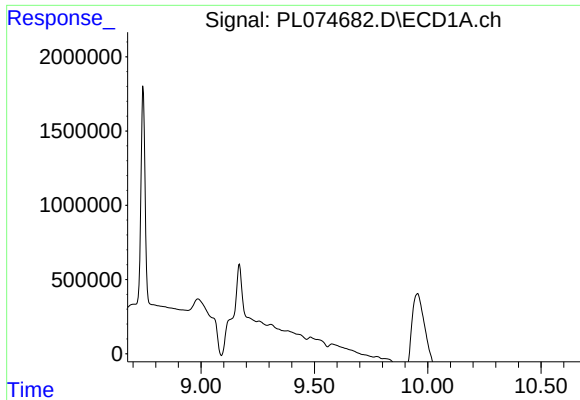

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

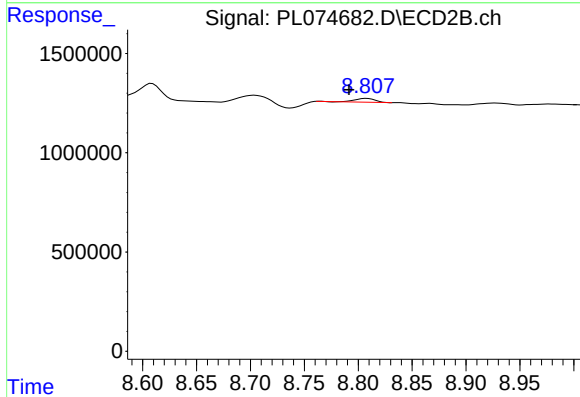


#19 Endosulfan Sulfate

R.T.: 8.808 min
Delta R.T.: 0.017 min
Response: 257705
Conc: 0.24 ng/ml

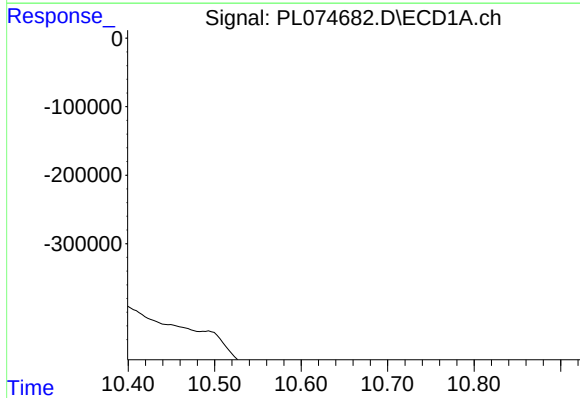


#22 Mirex

R.T.: 10.673 min
Delta R.T.: 0.024 min
Response: 49602
Conc: 0.12 ng/ml

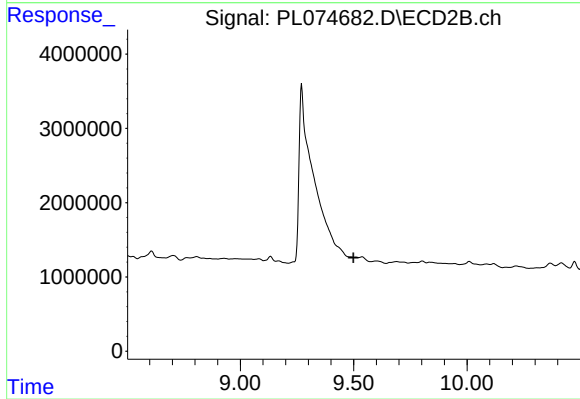

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.500 min
Response: 0
Conc: N.D.

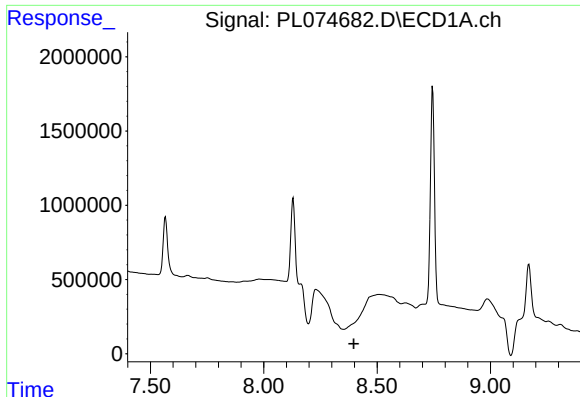

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

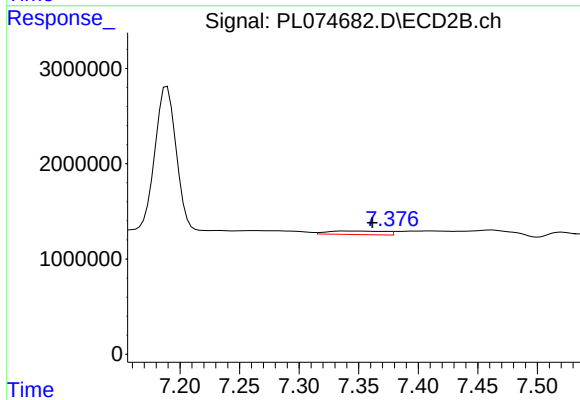


#25 Chlordane-3

R.T.: 7.338 min
Delta R.T.: -0.023 min
Response: 1268072
Conc: 9.77 ng/ml

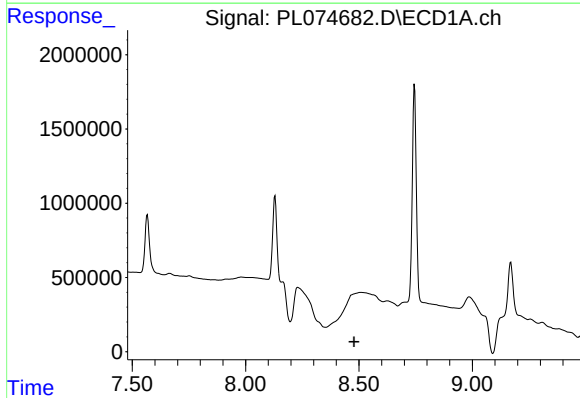


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 8.479 min
Response: 0
Conc: N.D.

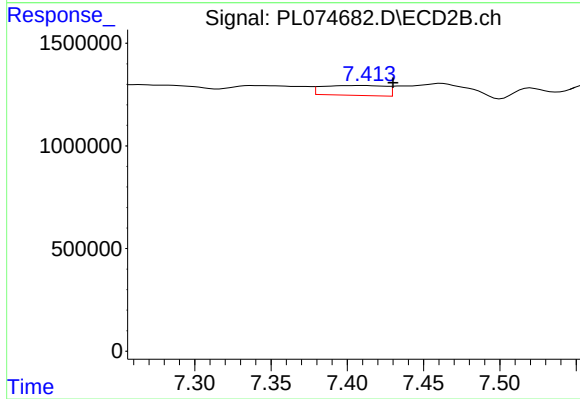

#26 Chlordane-4


R.T.: 7.411 min
Delta R.T.: -0.019 min
Response: 1382043
Conc: 10.08 ng/ml

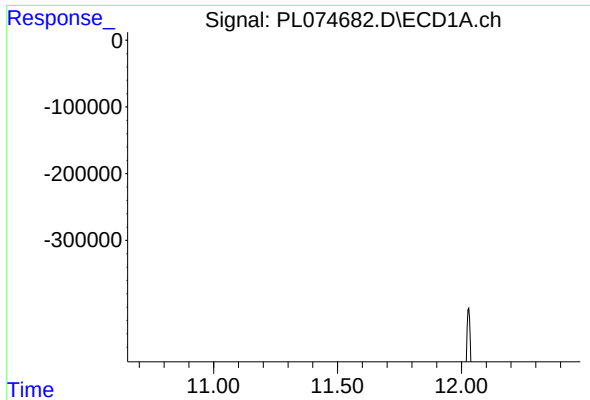

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 11.650 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

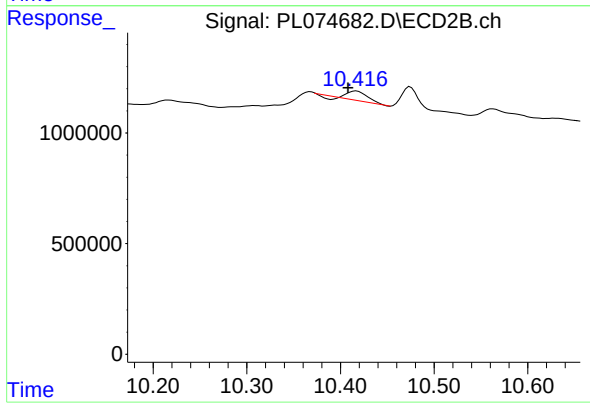

#28 Decachlorobiphenyl

R.T.: 10.417 min
Delta R.T.: 0.009 min
Response: 590997
Conc: 0.58 ng/ml