

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051322\
 Data File : PL074695.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2022 15:51
 Operator : AR\AJ
 Sample : N2809-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 23:17:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 16:19:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.652	4.654	3701193	8447127	7.290	6.154
28)	SA Decachlor...	11.652	10.408	4621776	9710996	10.349	9.461
Target Compounds							
6)	B beta-BHC	0.000	6.129f	0	610837	N.D.	0.769 #
9)	A Endosulfan I	8.530	0.000	1869191	0	3.242	N.D. #
11)	B alpha-Chl...	8.501f	0.000	3084037	0	4.787	N.D. #
23)	Chlordane-1	0.000	5.994f	0	141435	N.D.	3.121 #
26)	Chlordane-4	8.501f	0.000	3084037	0	32.012	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051322\
Data File : PL074695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2022 15:51
Operator : AR\AJ
Sample : N2809-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 23:17:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 16:19:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

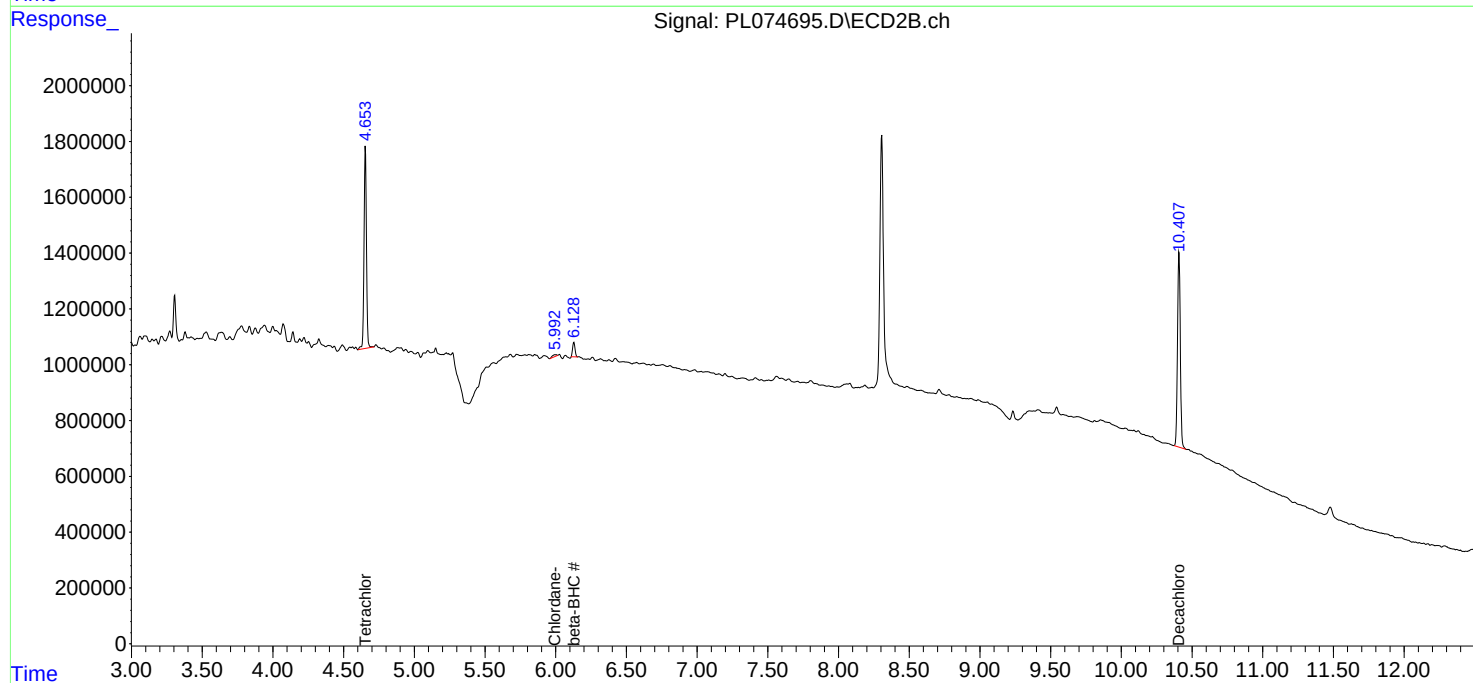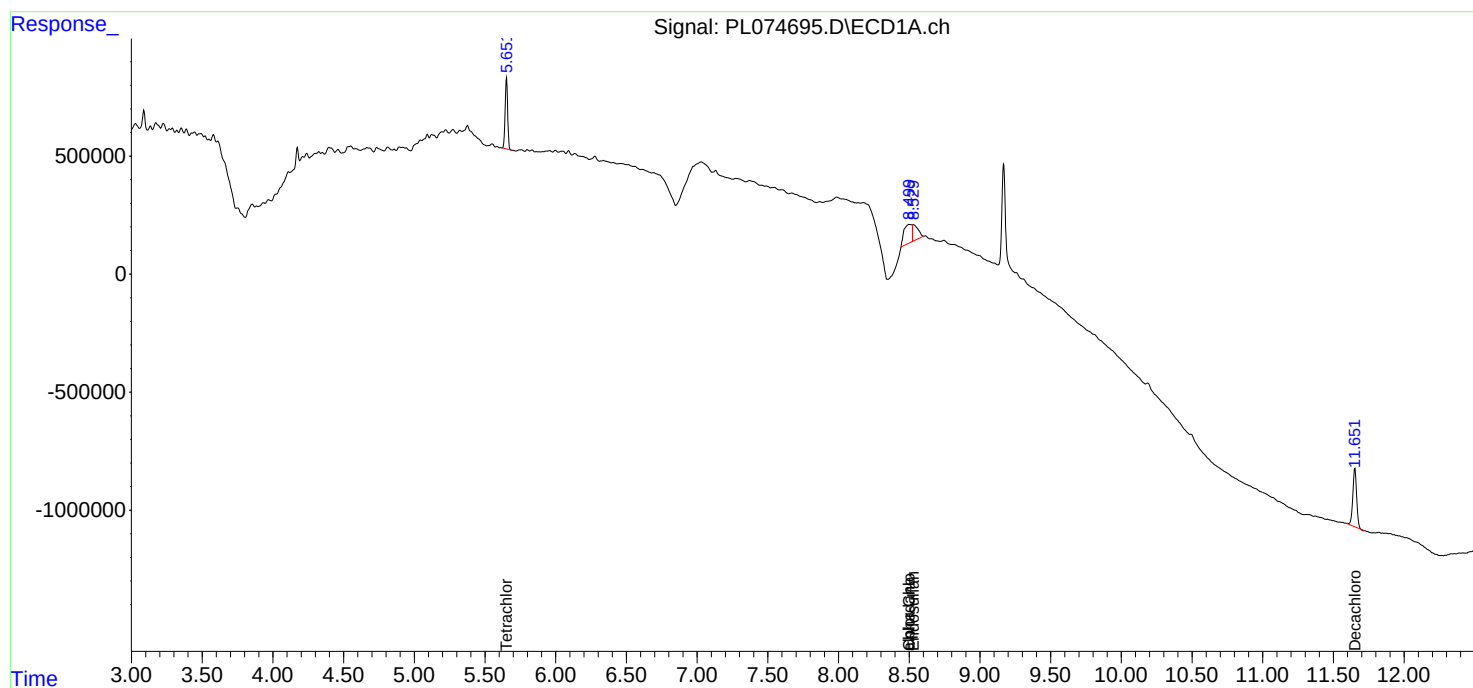


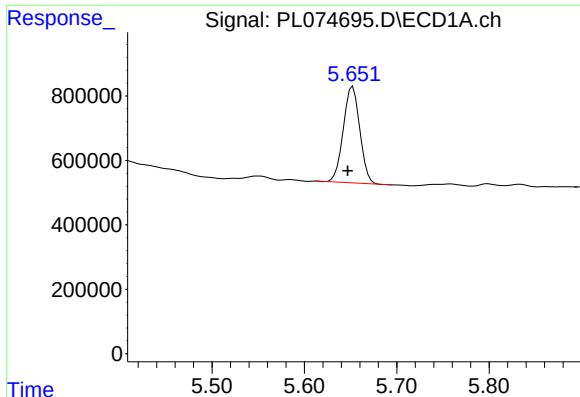

#1 Tetrachloro-m-xylene


R.T.: 5.652 min
Delta R.T.: 0.005 min
Response: 3701193
Conc: 7.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

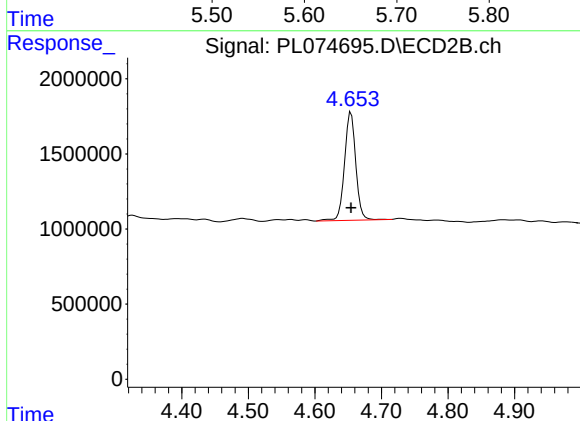


#1 Tetrachloro-m-xylene

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 8447127
Conc: 6.15 ng/ml

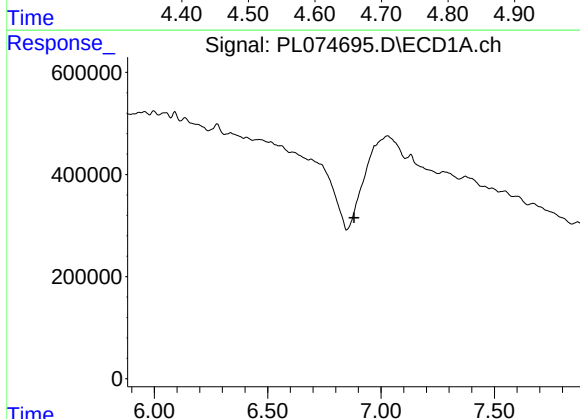


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.881 min
Response: 0
Conc: N.D.

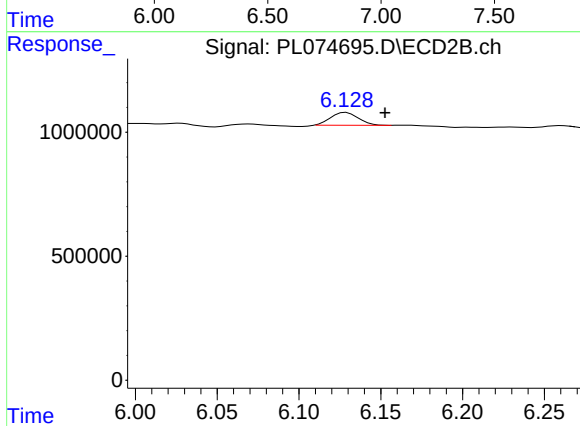

#6 beta-BHC


R.T.: 6.129 min
Delta R.T.: -0.024 min
Response: 610837
Conc: 0.77 ng/ml

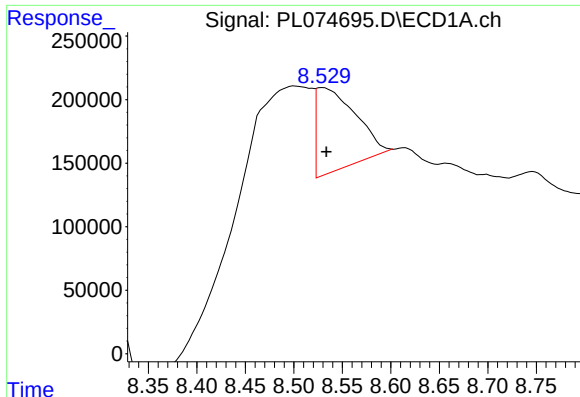

#9 Endosulfan I


R.T.: 8.530 min
Delta R.T.: -0.004 min
Response: 1869191
Conc: 3.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

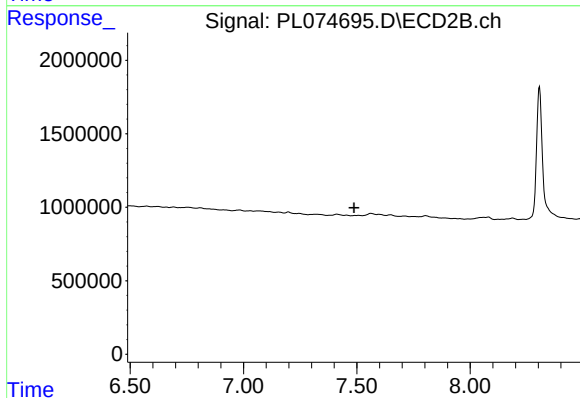


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.488 min
Response: 0
Conc: N.D.

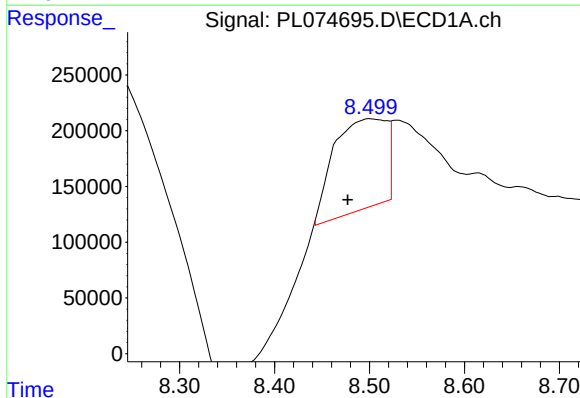


#11 alpha-Chlordane

R.T.: 8.501 min
Delta R.T.: 0.023 min
Response: 3084037
Conc: 4.79 ng/ml

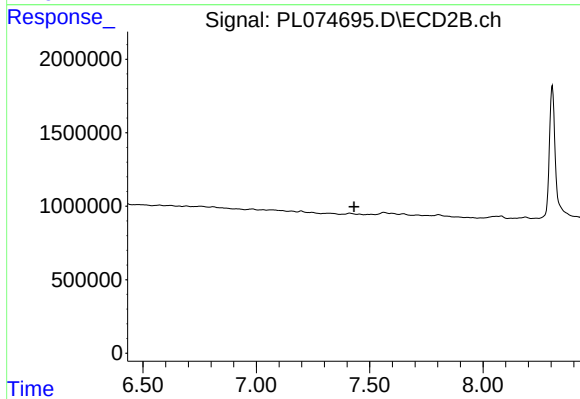

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.431 min
Response: 0
Conc: N.D.

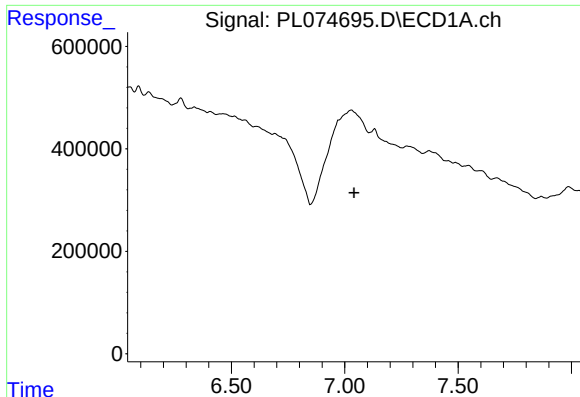

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 7.041 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

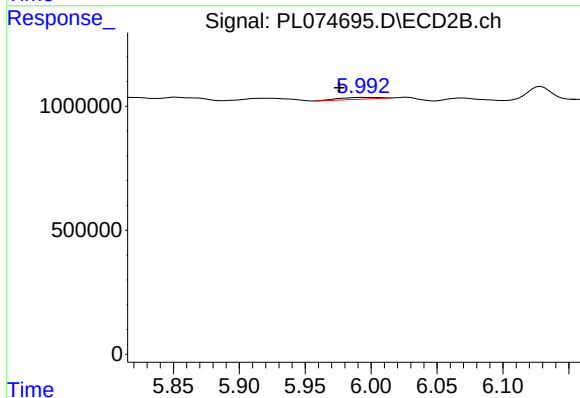


#23 Chlordane-1

R.T.: 5.994 min
Delta R.T.: 0.018 min
Response: 141435
Conc: 3.12 ng/ml

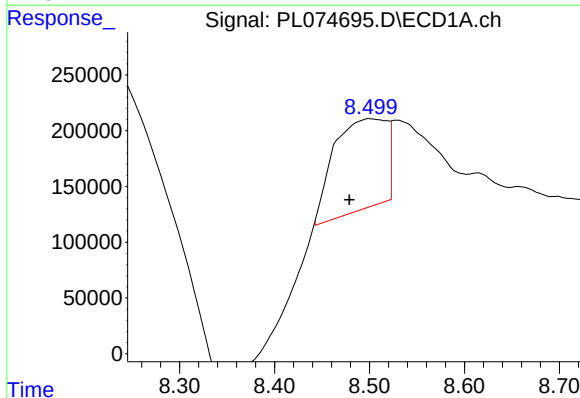


#26 Chlordane-4

R.T.: 8.501 min
Delta R.T.: 0.022 min
Response: 3084037
Conc: 32.01 ng/ml

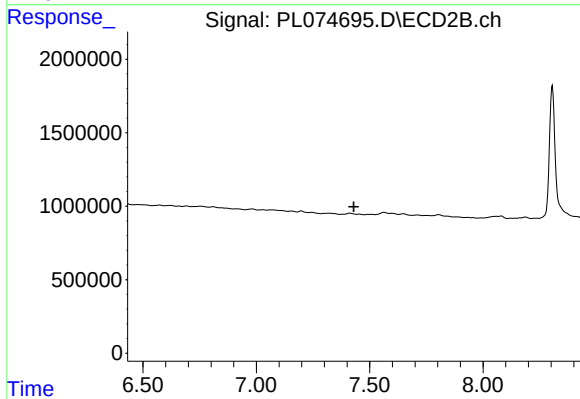

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

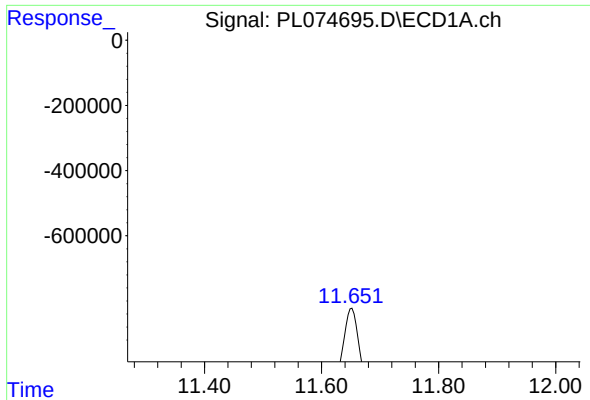

#28 Decachlorobiphenyl

R.T.: 11.652 min
Delta R.T.: 0.002 min
Response: 4621776
Conc: 10.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

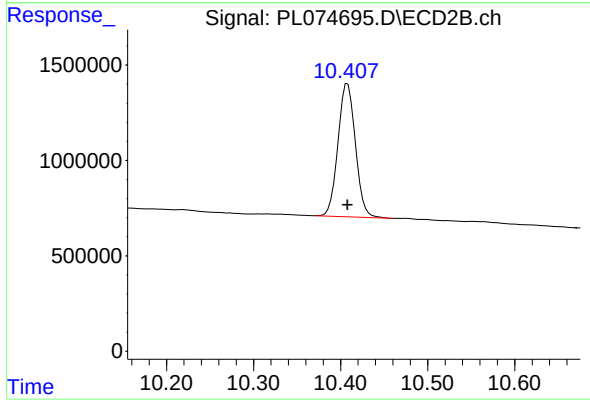

#28 Decachlorobiphenyl

R.T.: 10.408 min
Delta R.T.: 0.000 min
Response: 9710996
Conc: 9.46 ng/ml