

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051322\
 Data File : PL074701.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2022 17:30
 Operator : AR\AJ
 Sample : N2823-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 23:19:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 16:19:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.652	3897592	10427240	7.676	7.597
28)	SA Decachlor...	11.645	10.402	5483488	13326065	12.279	12.983
Target Compounds							
5)	MB Aldrin	0.000	6.501	0	396211	N.D.	0.264 #
6)	B beta-BHC	0.000	6.126f	0	734804	N.D.	0.925 #
7)	B delta-BHC	0.000	6.423	0	295402	N.D.	0.189 #
9)	A Endosulfan I	8.529	0.000	2209697	0	3.833	N.D. #
10)	B gamma-Chl...	0.000	7.339f	0	853480	N.D.	0.616 #
12)	B 4,4'-DDE	8.659	7.640	346108	1103498	0.748	0.938 #
14)	MA Endrin	0.000	8.052	0	547077	N.D.	0.518 #
17)	MA 4,4'-DDT	0.000	8.487	0	179063	N.D.	0.179 #
19)	B Endosulfa...	0.000	8.803	0	481829	N.D.	0.443 #
23)	Chlordane-1	0.000	5.962	0	3070836	N.D.	67.758 #
25)	Chlordane-3	0.000	7.339f	0	853480	N.D.	6.576 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051322\
Data File : PL074701.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2022 17:30
Operator : AR\AJ
Sample : N2823-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 23:19:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 16:19:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

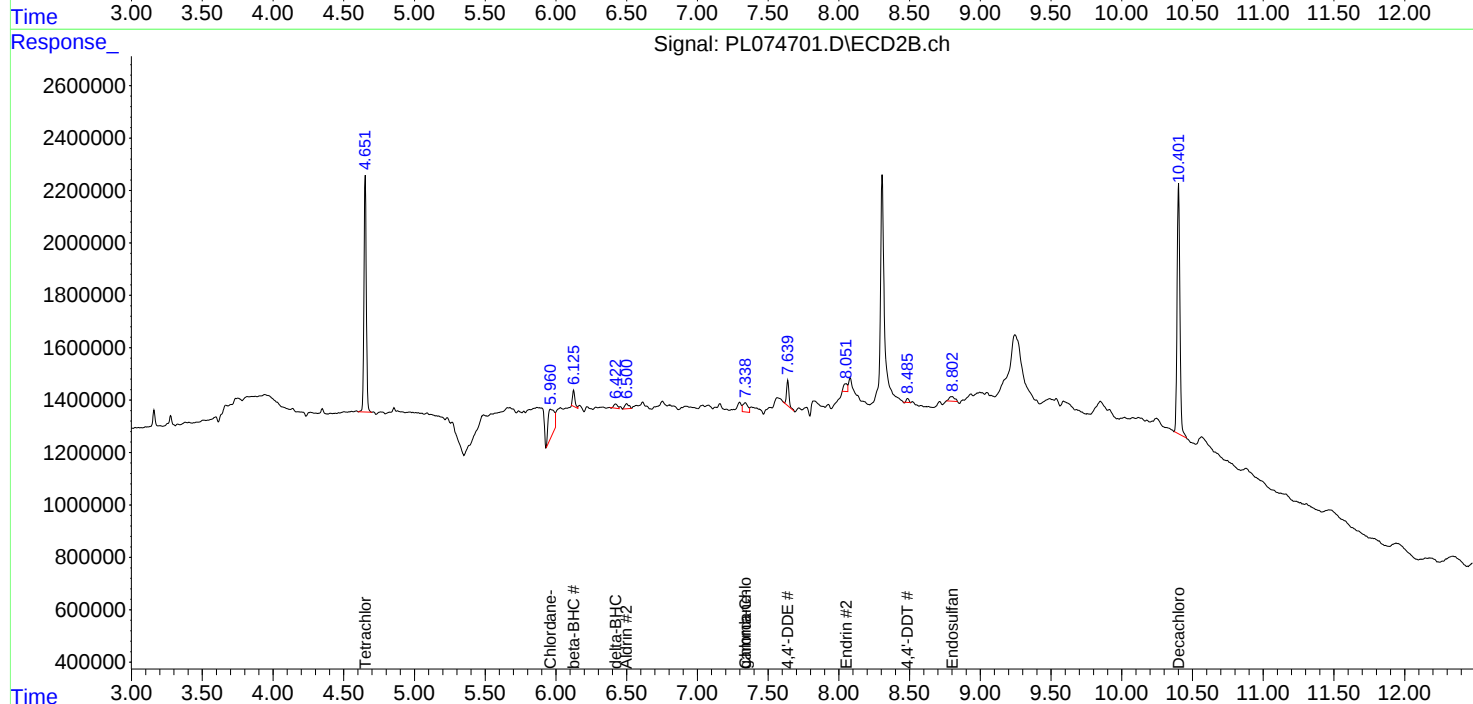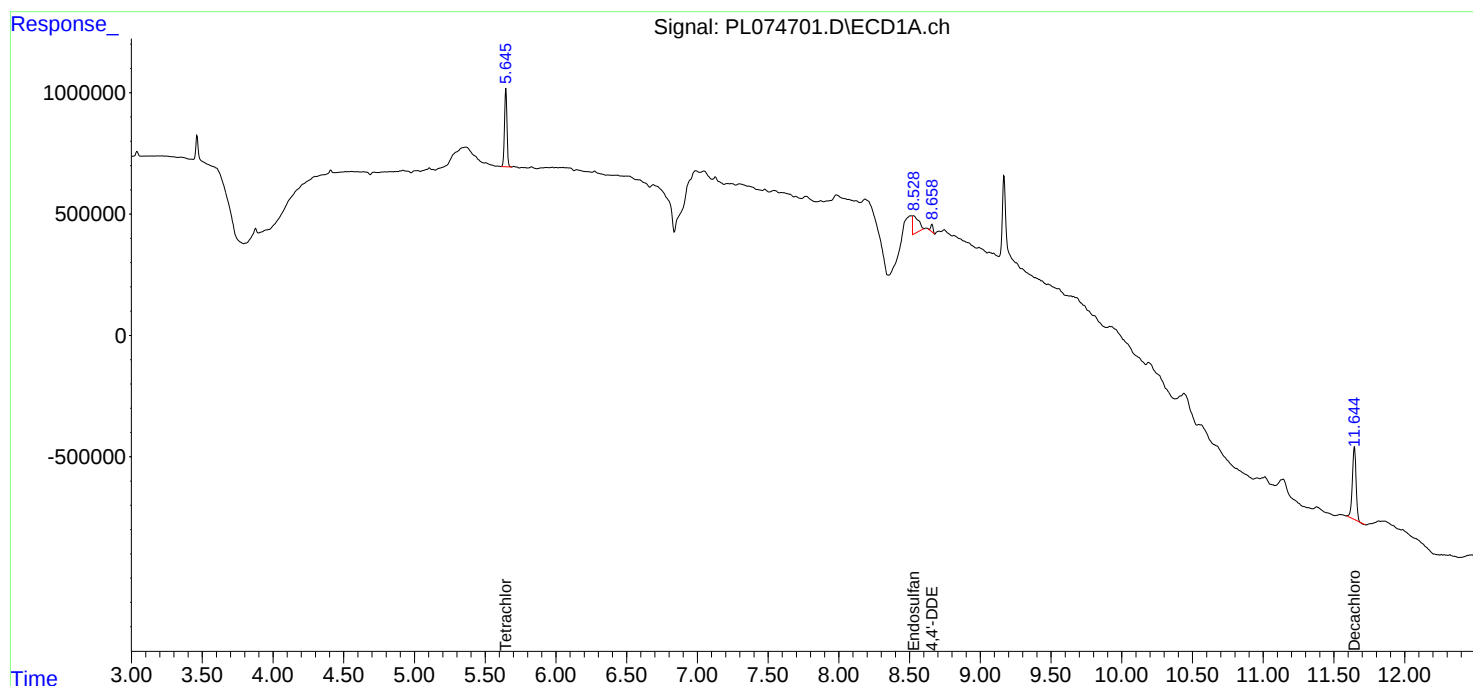


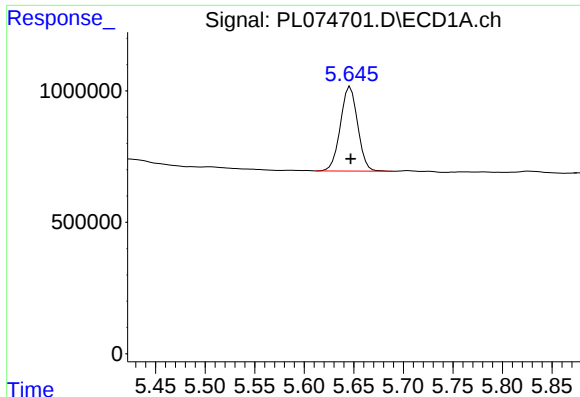

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: 0.000 min
Response: 3897592
Conc: 7.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

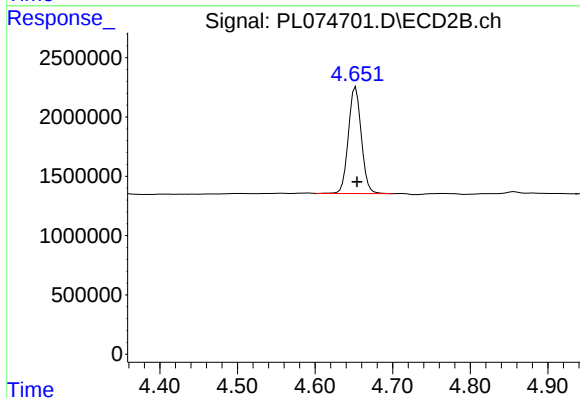


#1 Tetrachloro-m-xylene

R.T.: 4.652 min
Delta R.T.: -0.002 min
Response: 10427240
Conc: 7.60 ng/ml

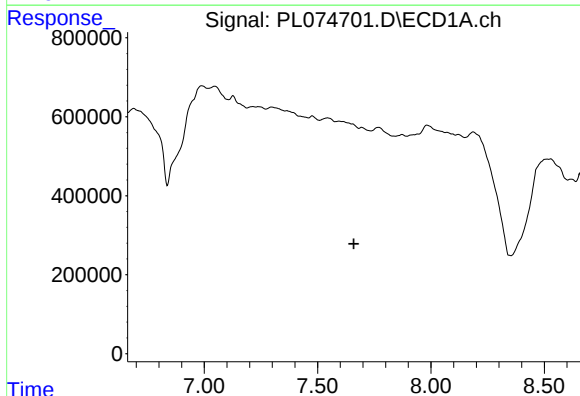


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.659 min
Response: 0
Conc: N.D.

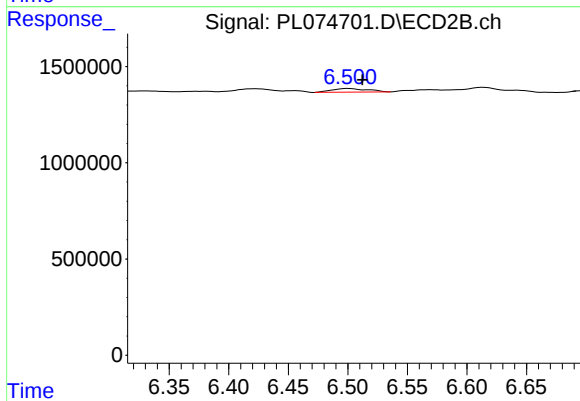

#5 Aldrin


R.T.: 6.501 min
Delta R.T.: -0.011 min
Response: 396211
Conc: 0.26 ng/ml

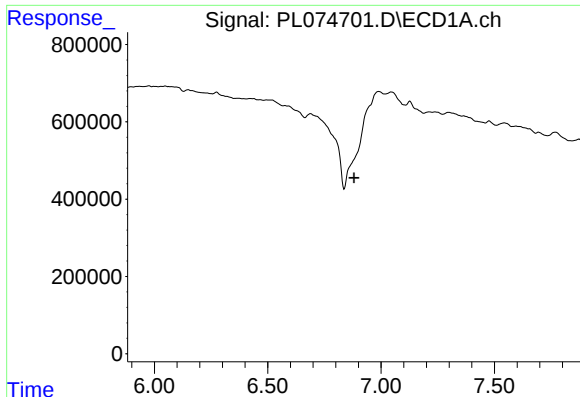

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.881 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

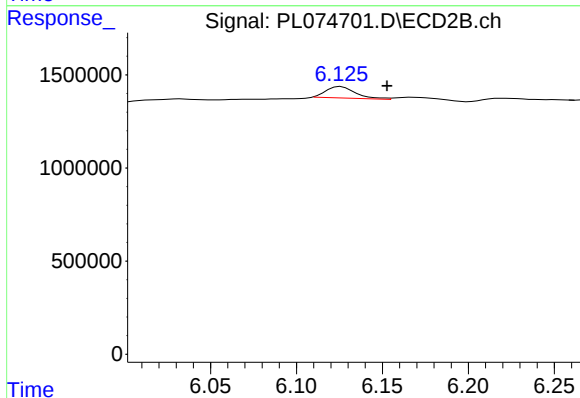


#6 beta-BHC

R.T.: 6.126 min
Delta R.T.: -0.027 min
Response: 734804
Conc: 0.93 ng/ml

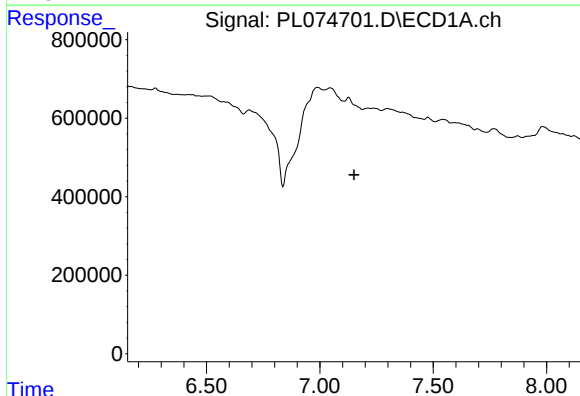


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 7.151 min
Response: 0
Conc: N.D.

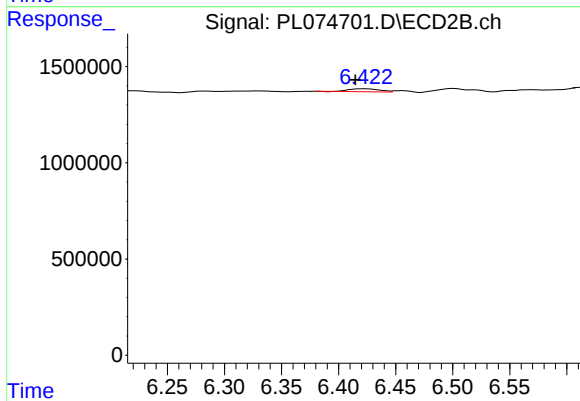

#7 delta-BHC


R.T.: 6.423 min
Delta R.T.: 0.008 min
Response: 295402
Conc: 0.19 ng/ml

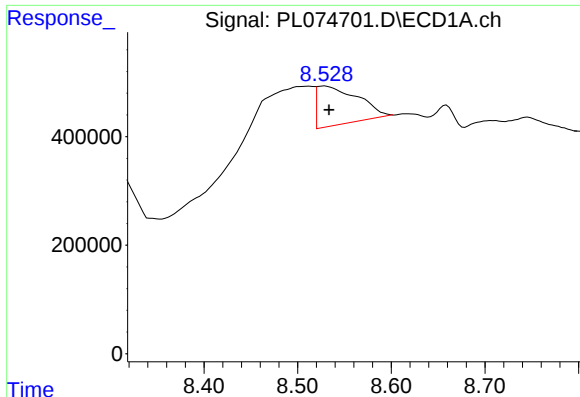

#9 Endosulfan I


R.T.: 8.529 min
Delta R.T.: -0.005 min
Response: 2209697
Conc: 3.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

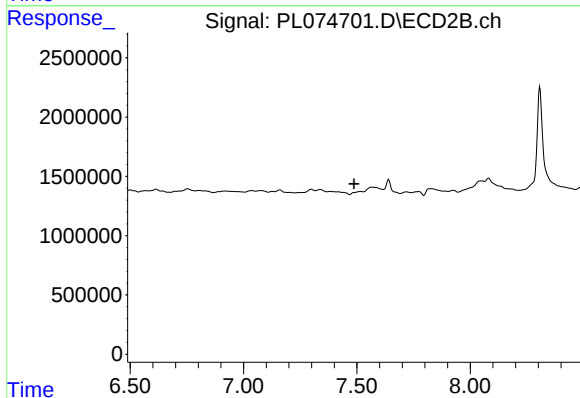


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.488 min
Response: 0
Conc: N.D.

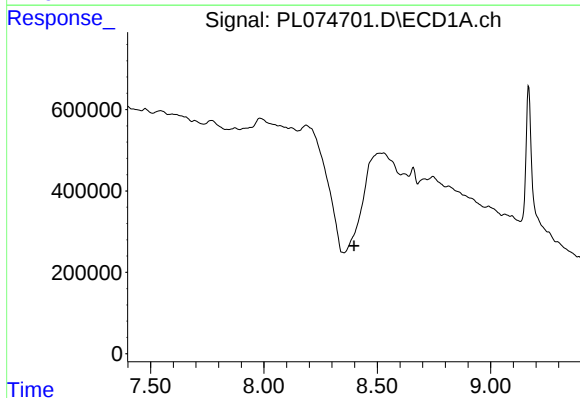


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.398 min
Response: 0
Conc: N.D.

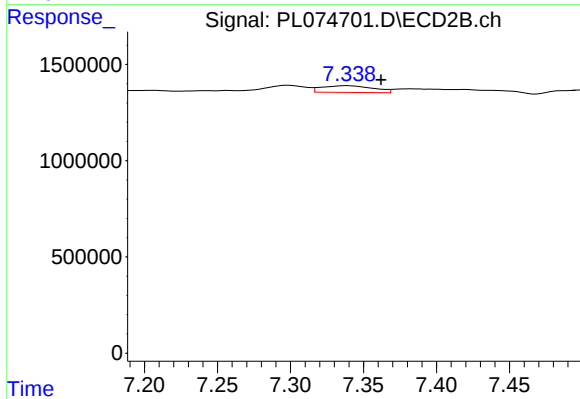

#10 gamma-Chlordane


R.T.: 7.339 min
Delta R.T.: -0.023 min
Response: 853480
Conc: 0.62 ng/ml

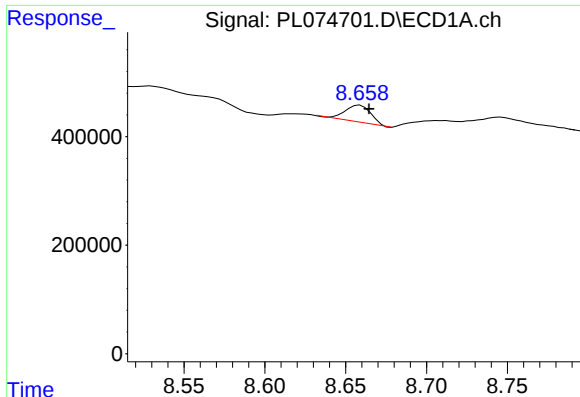

#12 4,4'-DDE


R.T.: 8.659 min
Delta R.T.: -0.006 min
Response: 346108
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

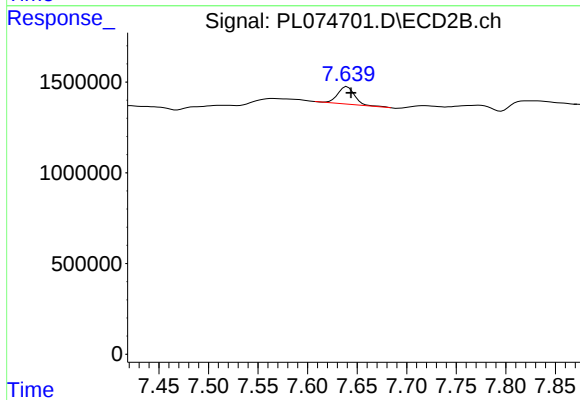


#12 4,4'-DDE

R.T.: 7.640 min
Delta R.T.: -0.004 min
Response: 1103498
Conc: 0.94 ng/ml

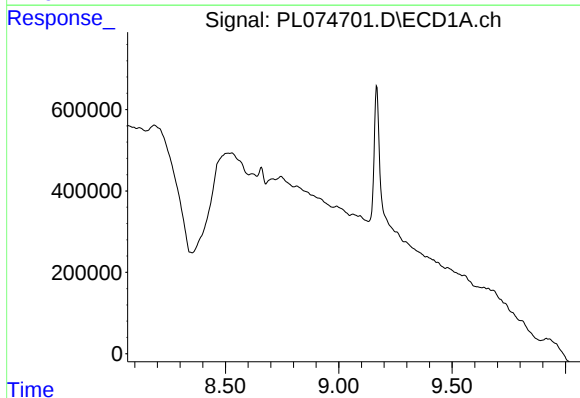


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.067 min
Response: 0
Conc: N.D.

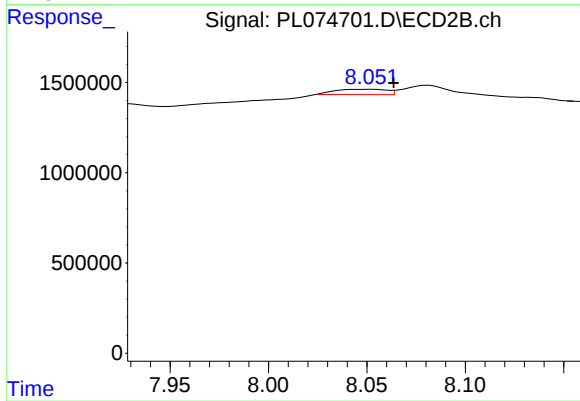

#14 Endrin


R.T.: 8.052 min
Delta R.T.: -0.011 min
Response: 547077
Conc: 0.52 ng/ml

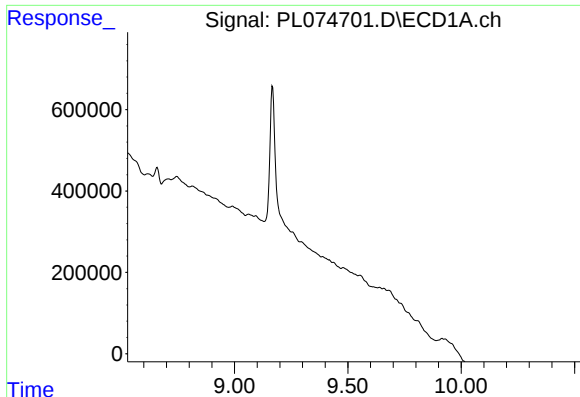

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.526 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

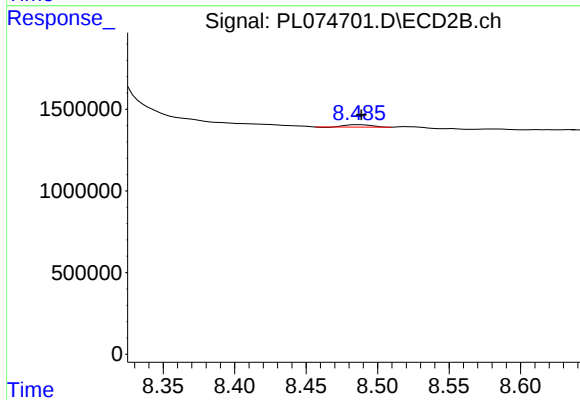


#17 4,4'-DDT

R.T.: 8.487 min
Delta R.T.: -0.002 min
Response: 179063
Conc: 0.18 ng/ml

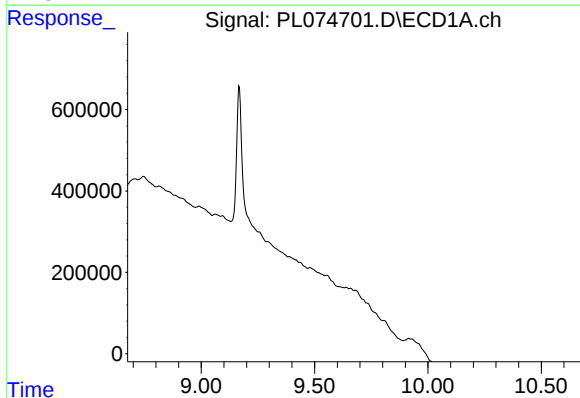


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 9.674 min
Response: 0
Conc: N.D.

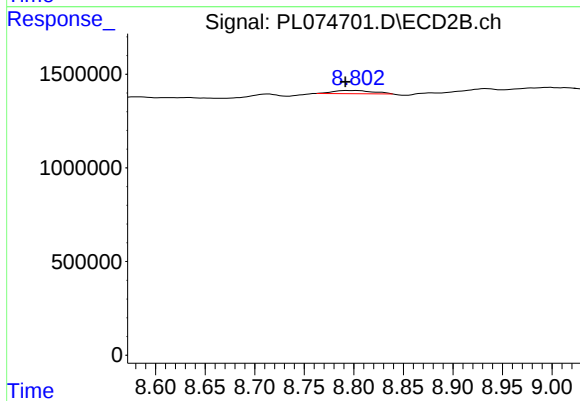

#19 Endosulfan Sulfate


R.T.: 8.803 min
Delta R.T.: 0.012 min
Response: 481829
Conc: 0.44 ng/ml

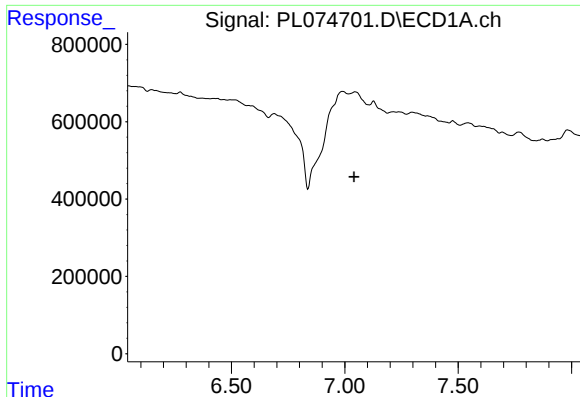

#23 Chlorine-1


R.T.: 0.000 min
Exp R.T.: 7.041 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

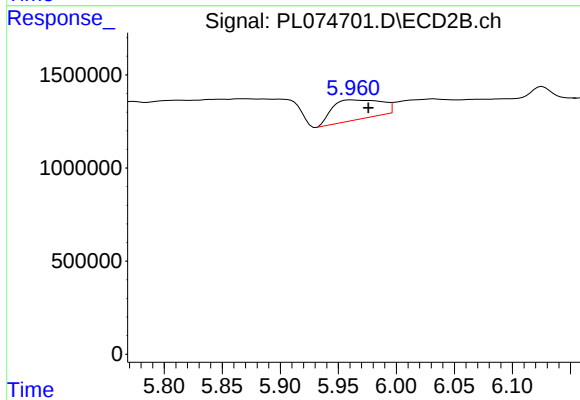


#23 Chlorine-1

R.T.: 5.962 min
Delta R.T.: -0.014 min
Response: 3070836
Conc: 67.76 ng/ml

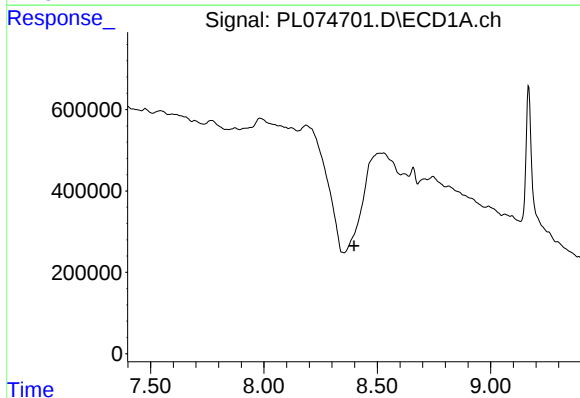


#25 Chlorine-3

R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

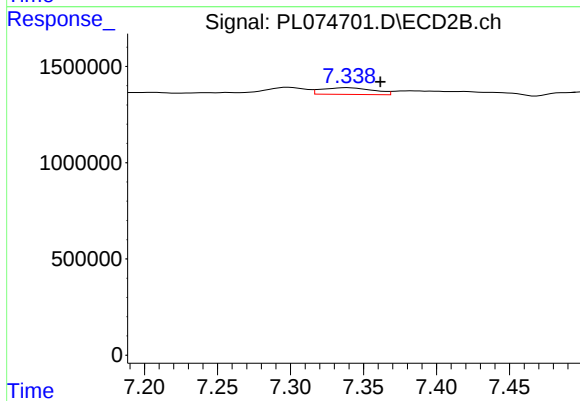

#25 Chlorine-3


R.T.: 7.339 min
Delta R.T.: -0.022 min
Response: 853480
Conc: 6.58 ng/ml

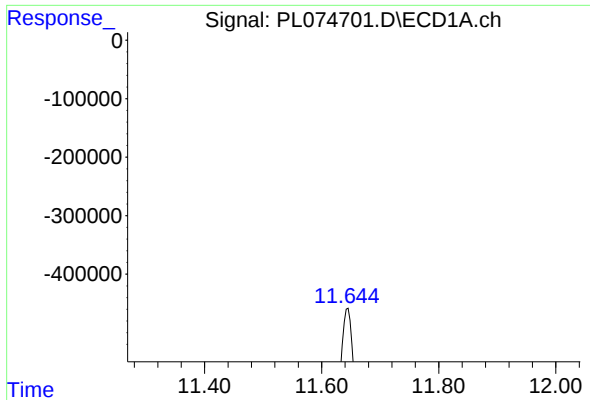

#28 Decachlorobiphenyl

R.T.: 11.645 min
Delta R.T.: -0.005 min
Response: 5483488
Conc: 12.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

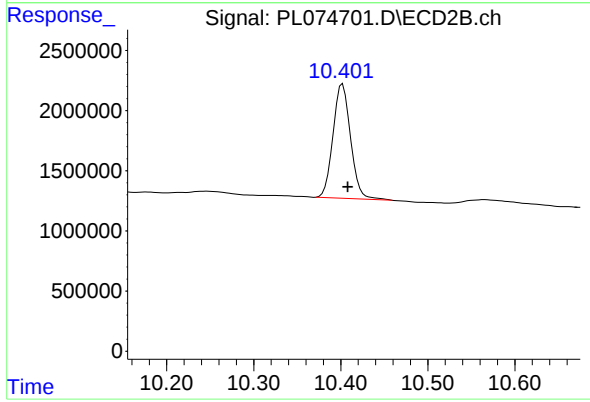

#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: -0.006 min
Response: 13326065
Conc: 12.98 ng/ml