

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051322\
 Data File : PL074706.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2022 18:53
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 23:20:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 16:19:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.647	4.652	10415667	26800442	20.514	19.527
28)	SA Decachlor...	11.645	10.403	8378156	22697885	18.761	22.114
Target Compounds							
4)	MA Heptachlor	0.000	6.163f	0	331745	N.D.	0.219 #
6)	B beta-BHC	0.000	6.163	0	331745	N.D.	0.418 #
8)	B Heptachlo...	8.128	0.000	439487	0	0.773	N.D. #
9)	A Endosulfan I	8.511f	7.481	5625090	1223458	9.757	0.978 #
11)	B alpha-Chl...	0.000	7.417	0	354883	N.D.	0.263 #
13)	MA Dieldrin	0.000	7.776	0	2897877	N.D.	2.275 #
14)	MA Endrin	0.000	8.082f	0	8170261	N.D.	7.735 #
19)	B Endosulfa...	0.000	8.808f	0	956027	N.D.	0.878 #
21)	B Endrin ke...	10.205f	0.000	841663	0	1.641	N.D. #
22)	Mirex	10.675f	0.000	3625357	0	8.985	N.D. #
26)	Chlordane-4	0.000	7.417	0	354883	N.D.	2.589 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051322\
Data File : PL074706.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2022 18:53
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 23:20:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 16:19:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

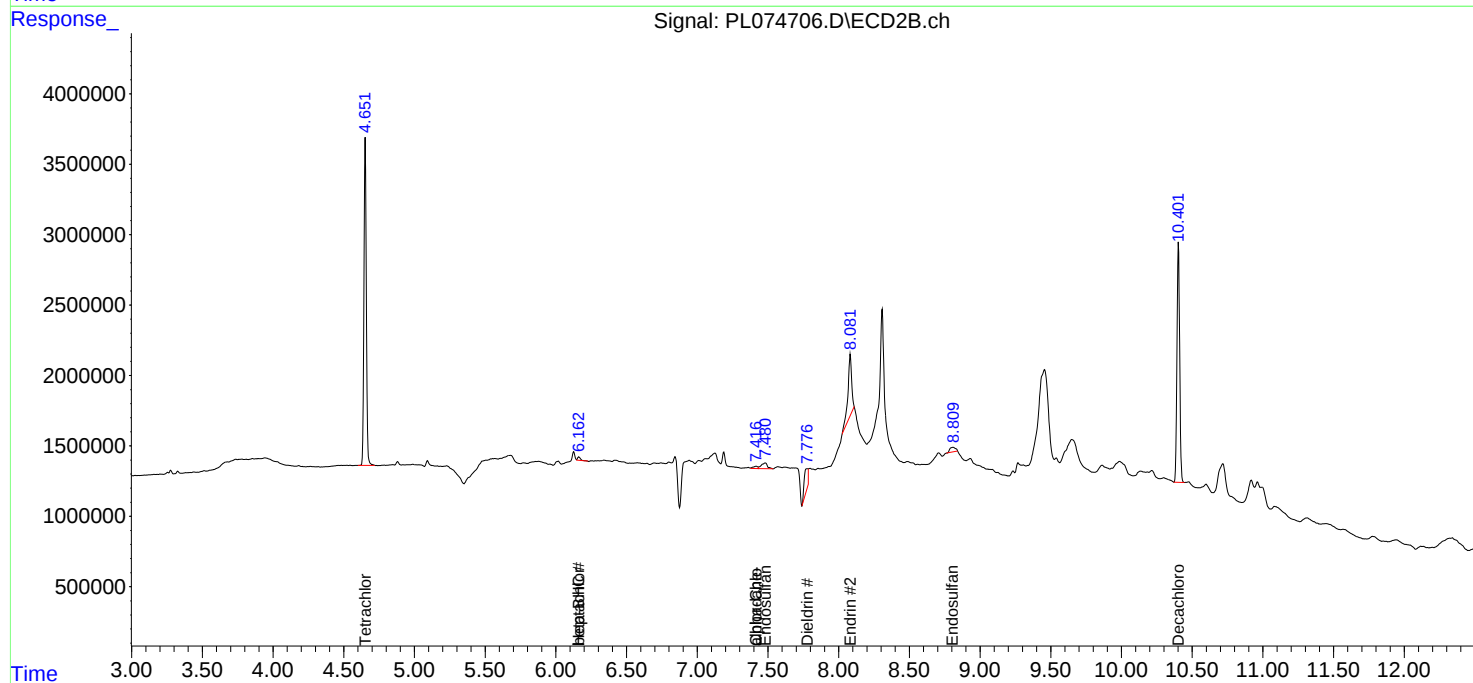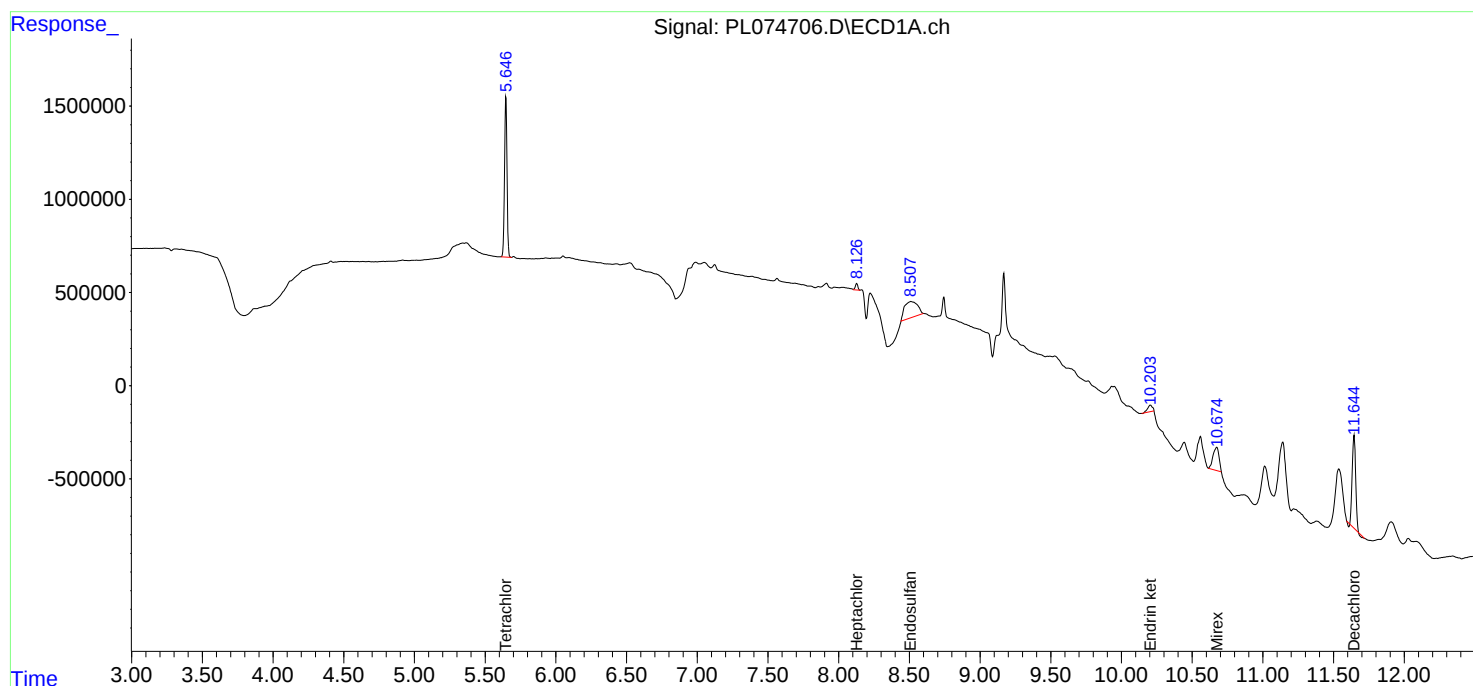


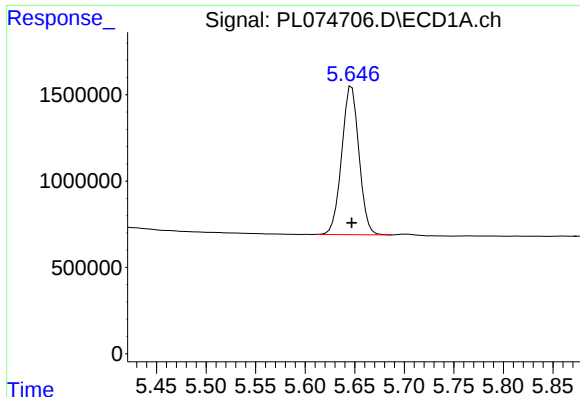

#1 Tetrachloro-m-xylene


R.T.: 5.647 min
Delta R.T.: 0.000 min
Response: 10415667
Conc: 20.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

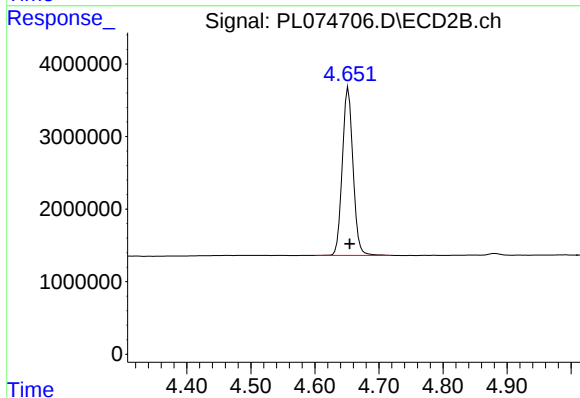


#1 Tetrachloro-m-xylene

R.T.: 4.652 min
Delta R.T.: -0.002 min
Response: 26800442
Conc: 19.53 ng/ml

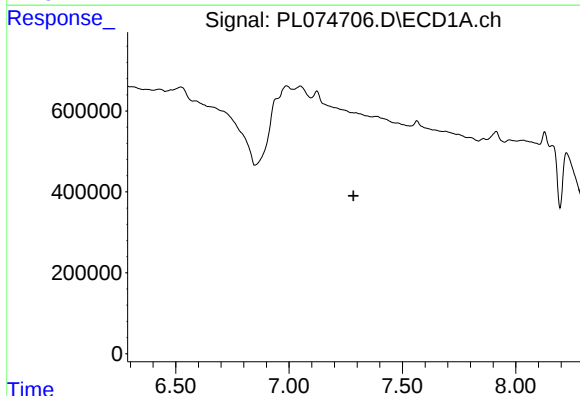


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.284 min
Response: 0
Conc: N.D.

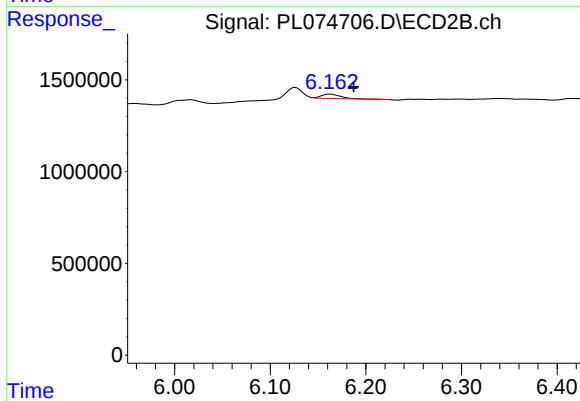

#4 Heptachlor


R.T.: 6.163 min
Delta R.T.: -0.025 min
Response: 331745
Conc: 0.22 ng/ml

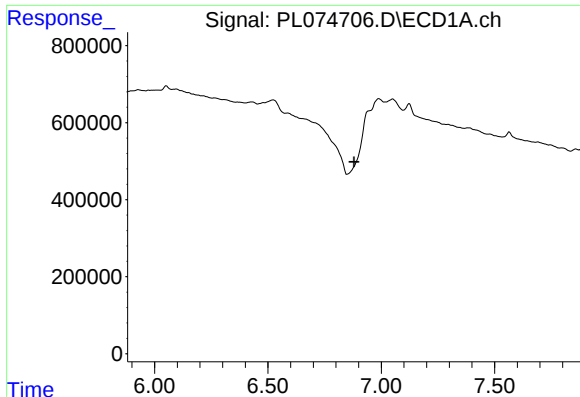

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.881 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

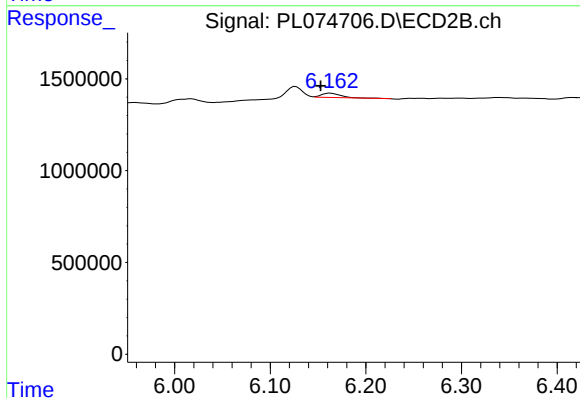


#6 beta-BHC

R.T.: 6.163 min
Delta R.T.: 0.010 min
Response: 331745
Conc: 0.42 ng/ml

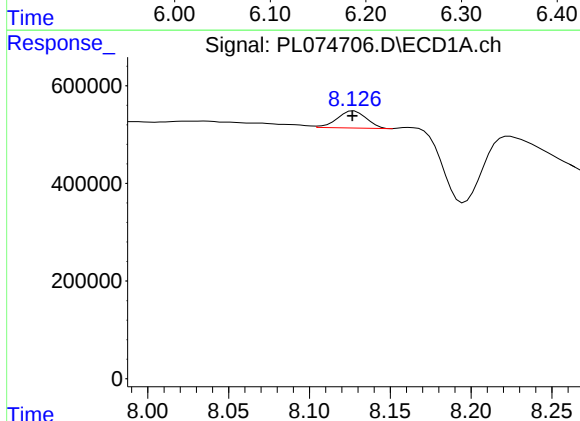


#8 Heptachlor epoxide

R.T.: 8.128 min
Delta R.T.: 0.001 min
Response: 439487
Conc: 0.77 ng/ml

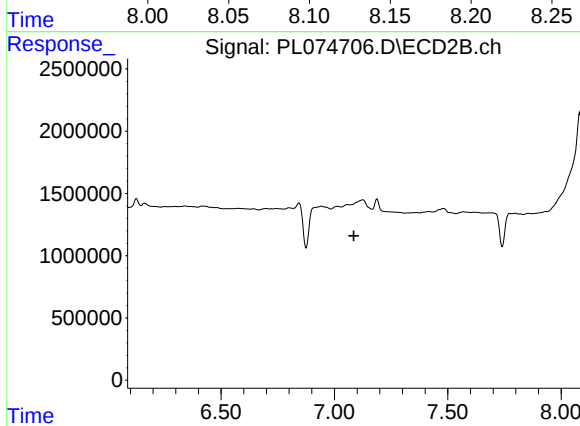

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.086 min
Response: 0
Conc: N.D.

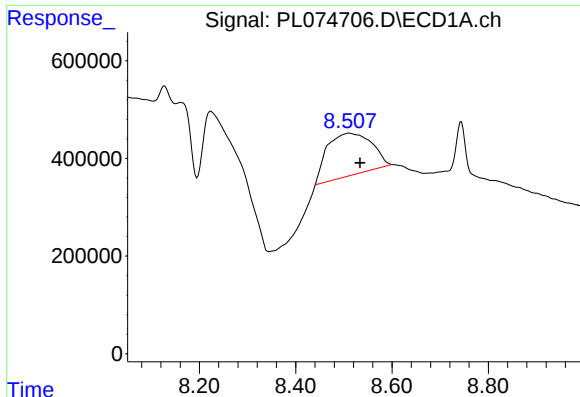

#9 Endosulfan I


R.T.: 8.511 min
Delta R.T.: -0.023 min
Response: 5625090
Conc: 9.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

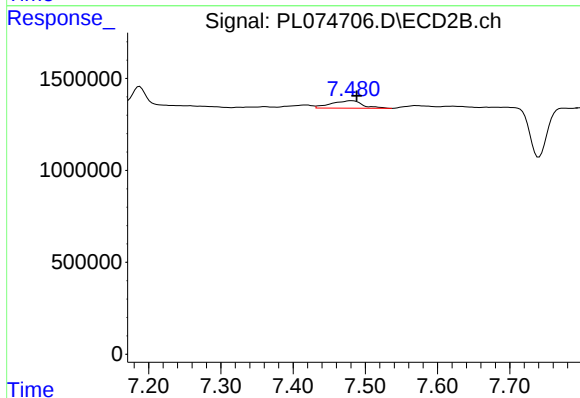


#9 Endosulfan I

R.T.: 7.481 min
Delta R.T.: -0.007 min
Response: 1223458
Conc: 0.98 ng/ml

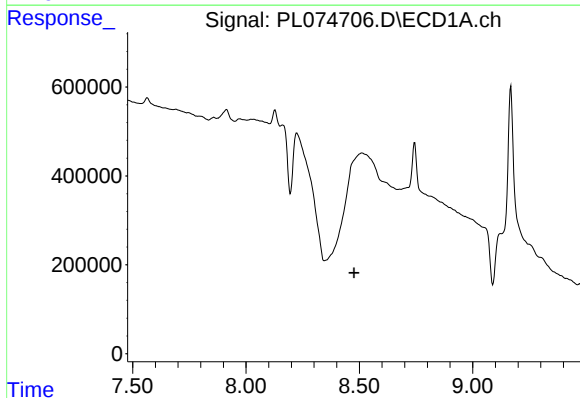


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.477 min
Response: 0
Conc: N.D.

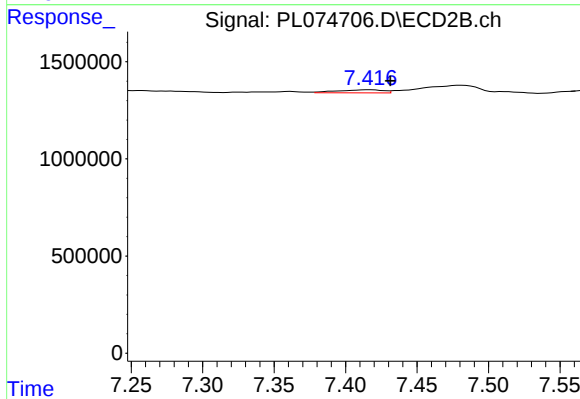

#11 alpha-Chlordane


R.T.: 7.417 min
Delta R.T.: -0.014 min
Response: 354883
Conc: 0.26 ng/ml

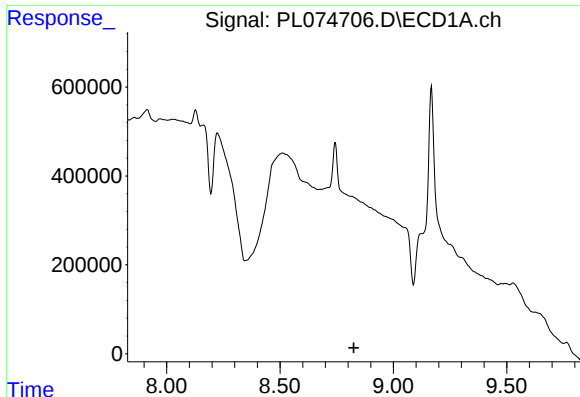

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.826 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

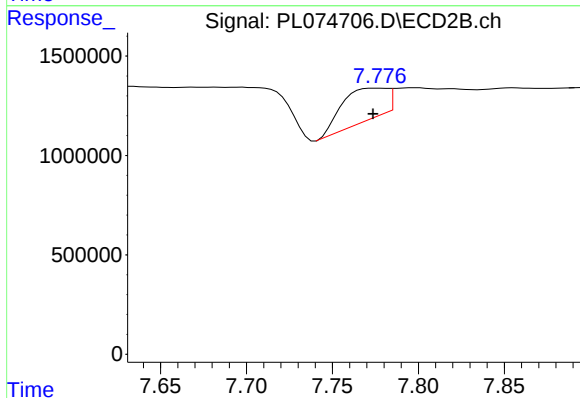


#13 Dieldrin

R.T.: 7.776 min
Delta R.T.: 0.003 min
Response: 2897877
Conc: 2.27 ng/ml

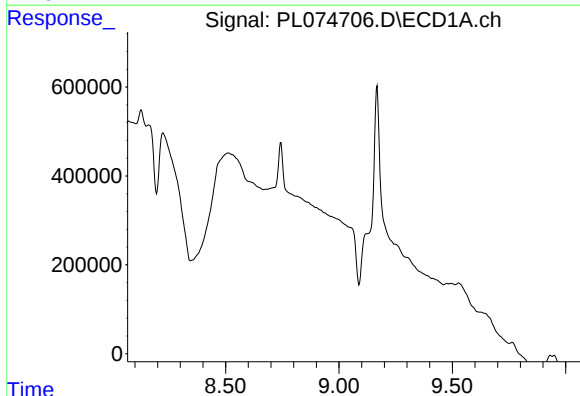


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.067 min
Response: 0
Conc: N.D.

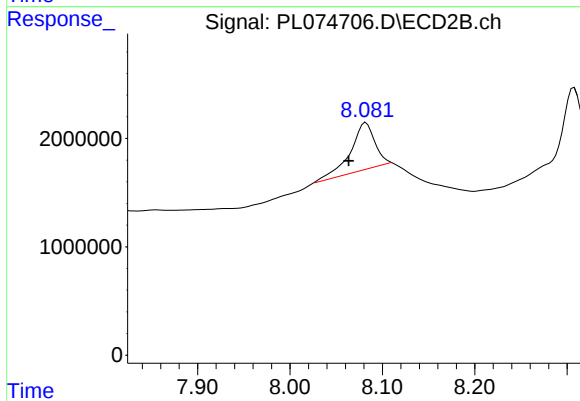

#14 Endrin


R.T.: 8.082 min
Delta R.T.: 0.019 min
Response: 8170261
Conc: 7.73 ng/ml

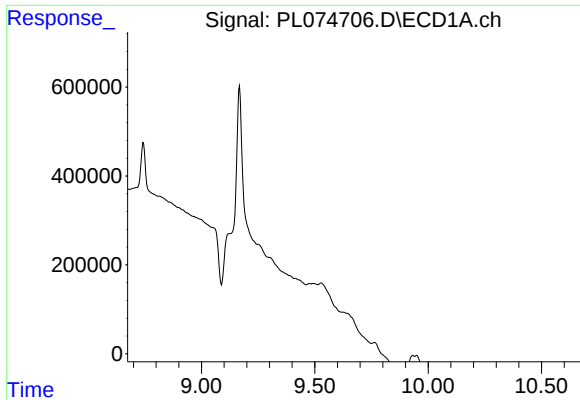

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

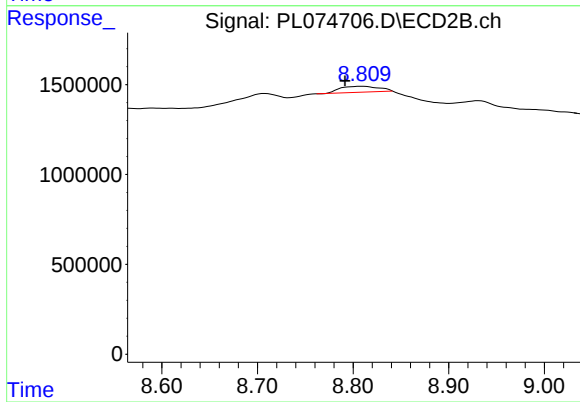


#19 Endosulfan Sulfate

R.T.: 8.808 min
Delta R.T.: 0.017 min
Response: 956027
Conc: 0.88 ng/ml

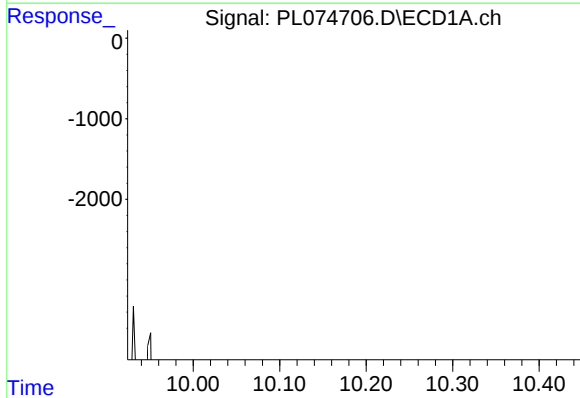


#21 Endrin ketone

R.T.: 10.205 min
Delta R.T.: 0.028 min
Response: 841663
Conc: 1.64 ng/ml

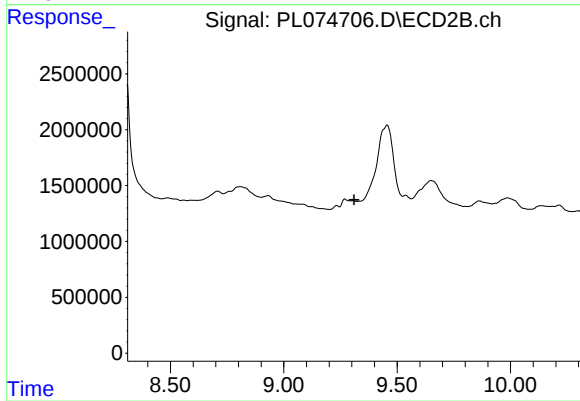

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.310 min
Response: 0
Conc: N.D.

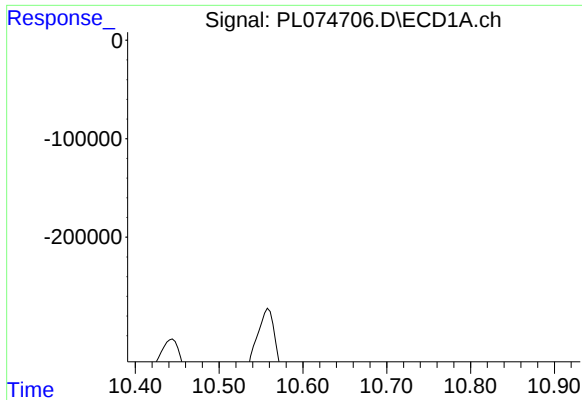

#22 Mirex


R.T.: 10.675 min
Delta R.T.: 0.025 min
Response: 3625357
Conc: 8.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

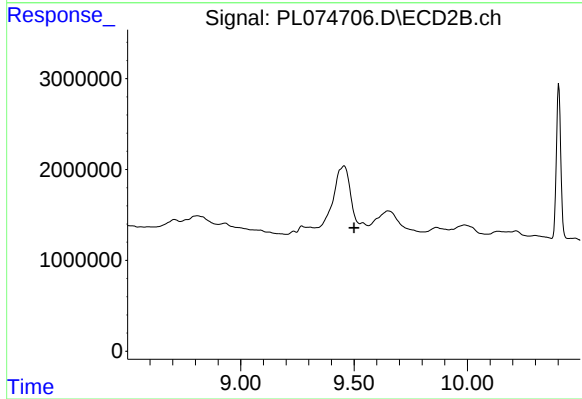


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.500 min
Response: 0
Conc: N.D.

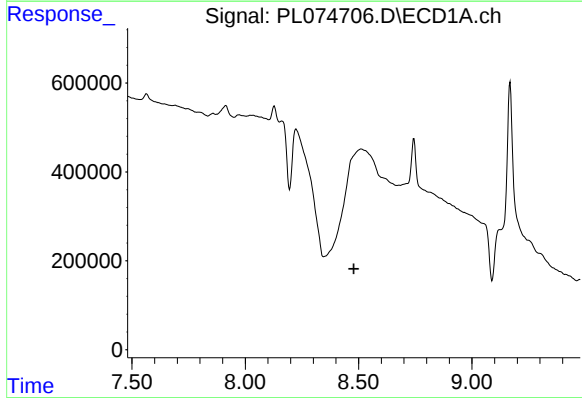


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.479 min
Response: 0
Conc: N.D.

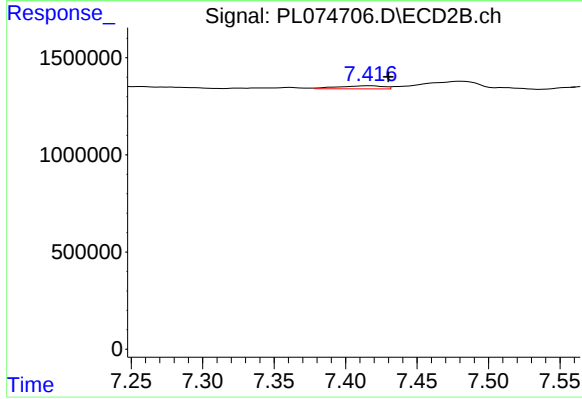

#26 Chlordane-4


R.T.: 7.417 min
Delta R.T.: -0.013 min
Response: 354883
Conc: 2.59 ng/ml

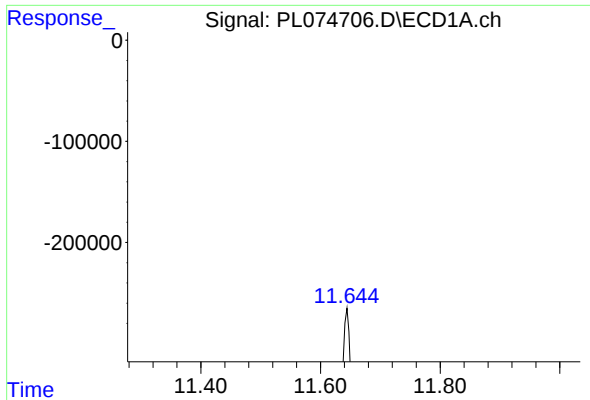

#28 Decachlorobiphenyl

R.T.: 11.645 min
Delta R.T.: -0.005 min
Response: 8378156
Conc: 18.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

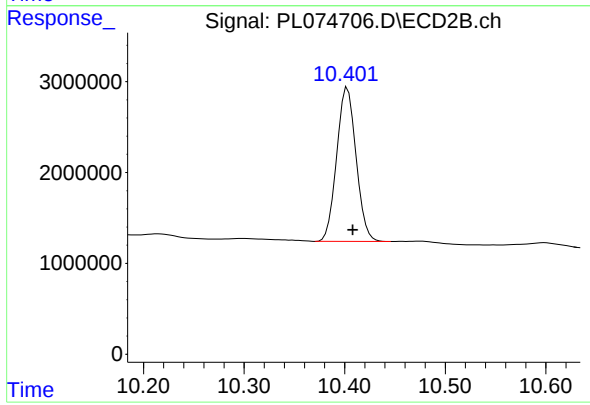

#28 Decachlorobiphenyl

R.T.: 10.403 min
Delta R.T.: -0.005 min
Response: 22697885
Conc: 22.11 ng/ml