

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051322\
 Data File : PL074701.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2022 17:30
 Operator : AR\AJ
 Sample : N2823-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SC-6

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/16/2022
 Supervised By : mohammad ahmed 05/16/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 23:19:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 16:19:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.646	4.652	3897592	10427240	7.676	7.597
28) SA Decachlor...	11.645	10.402	5483488	13326065	12.279	12.983
Target Compounds						
12) B 4,4'-DDE	8.658	7.640	348890	1103498	0.754m	0.938

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051322\
Data File : PL074701.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2022 17:30
Operator : AR\AJ
Sample : N2823-06
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SC-6


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/16/2022
Supervised By : mohammad ahmed 05/16/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 23:19:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 16:19:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

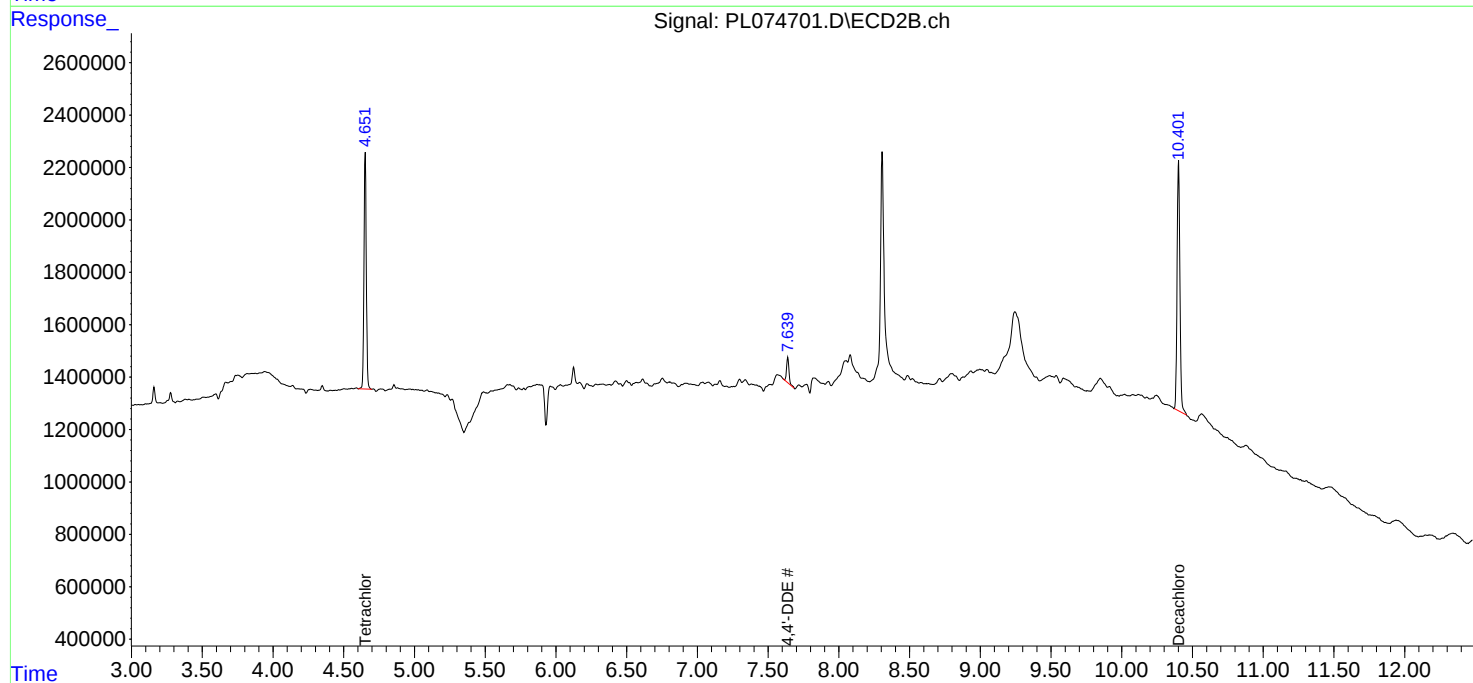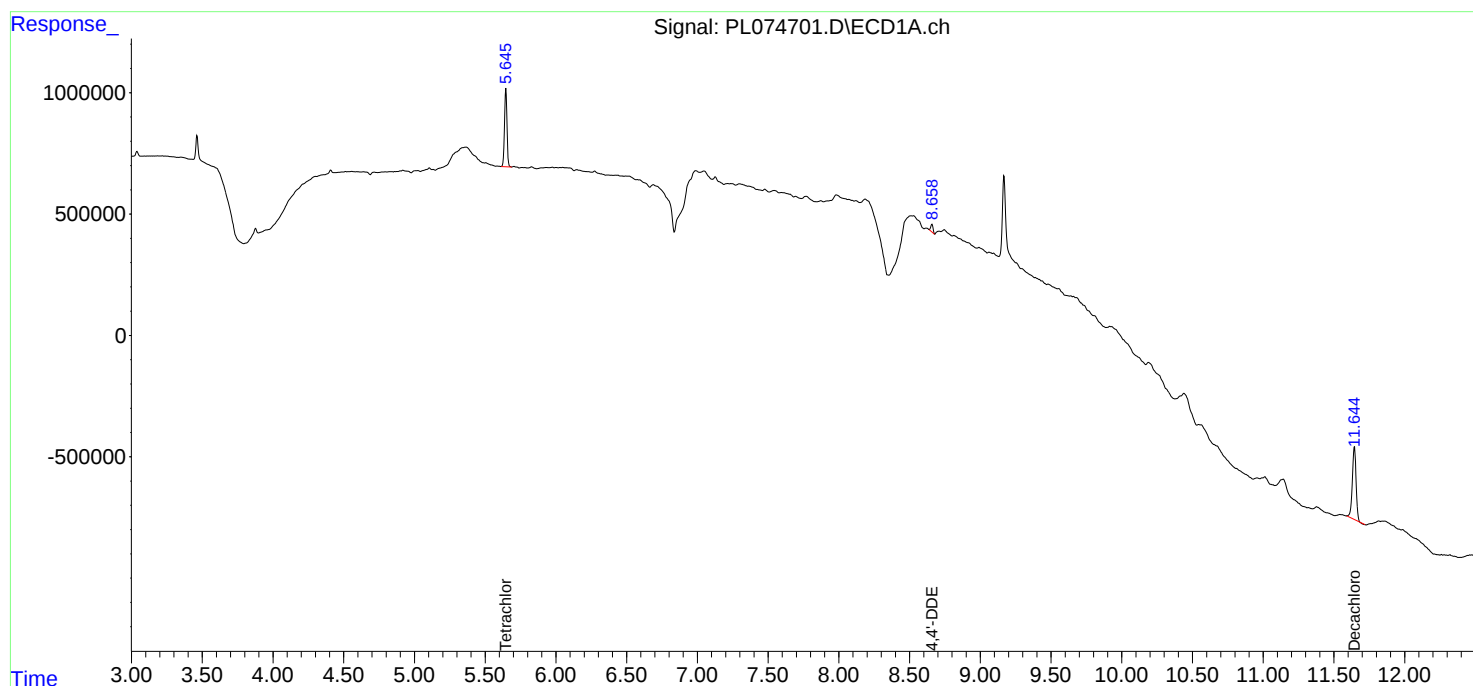

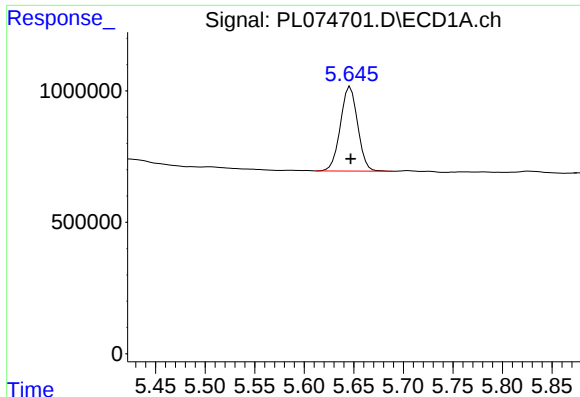


#1 Tetrachloro-m-xylene

R.T.: 5.646 min
Delta R.T.: 0.000 min
Response: 3897592
Conc: 7.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
SC-6


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/16/2022
Supervised By :mohammad ahmed 05/16/2022

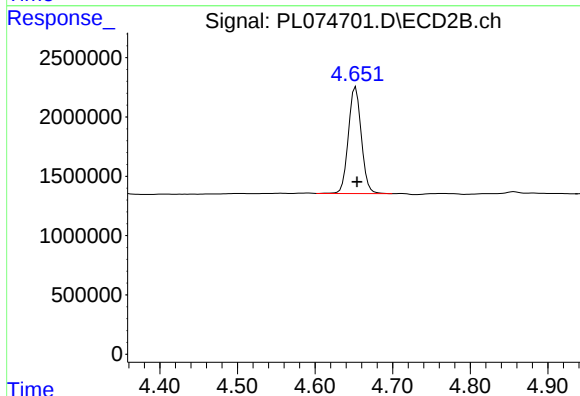


#1 Tetrachloro-m-xylene

R.T.: 4.652 min
Delta R.T.: -0.002 min
Response: 10427240
Conc: 7.60 ng/ml

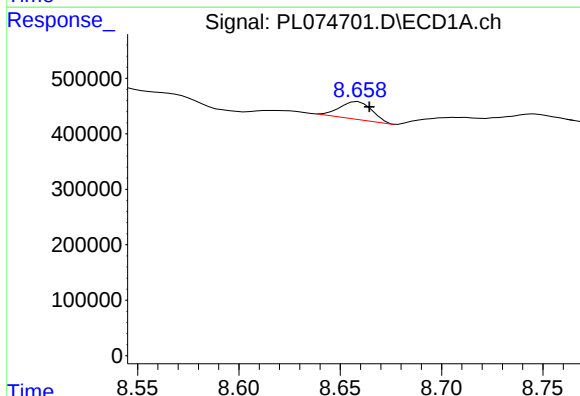


#12 4,4'-DDE

R.T.: 8.658 min
Delta R.T.: -0.006 min
Response: 348890
Conc: 0.75 ng/ml m

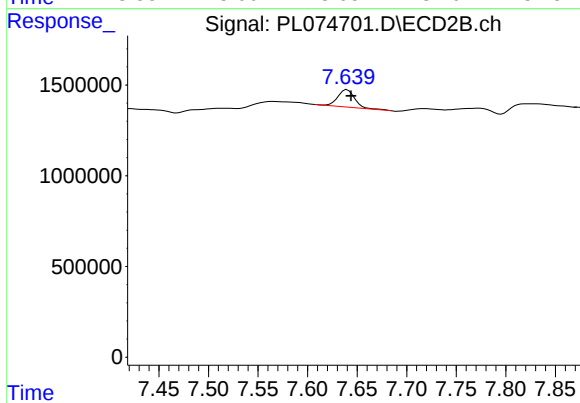

#12 4,4'-DDE

R.T.: 7.640 min
Delta R.T.: -0.004 min
Response: 1103498
Conc: 0.94 ng/ml

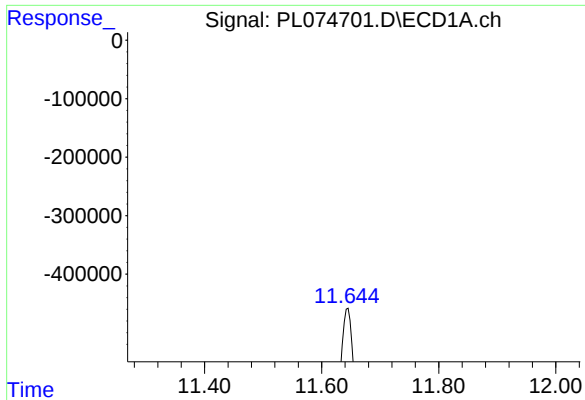


#28 Decachlorobiphenyl

R.T.: 11.645 min
Delta R.T.: -0.005 min
Response: 5483488
Conc: 12.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
SC-6

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/16/2022
Supervised By :mohammad ahmed 05/16/2022

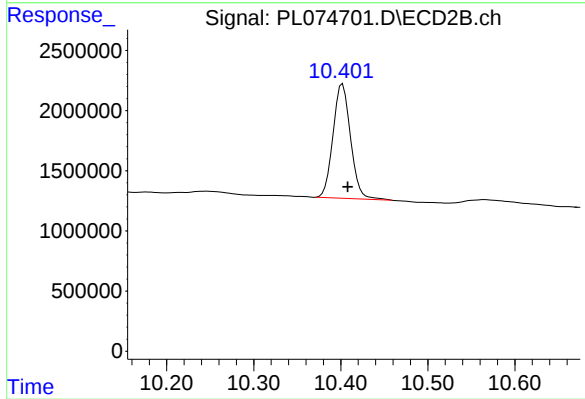

#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: -0.006 min
Response: 13326065
Conc: 12.98 ng/ml