

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051324\
 Data File : PL089510.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2024 15:32
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 04:36:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 26 19:27:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.796	85723533	72861039	42.571	56.788 #
28)	SA Decachlor...	9.064	7.946	58678160	60422390	41.942	44.917
Target Compounds							
23)	Chlordane-1	4.712	3.799	43657482	26032996	478.173m	529.107
24)	Chlordane-2	5.241	4.376	48322696	32002798	459.804m	503.069m
25)	Chlordane-3	5.950	5.008	154.8E6	90699795	468.635m	529.724
26)	Chlordane-4	6.033	5.070	182.2E6	81235219	447.085m	505.054m
27)	Chlordane-5	6.880	5.738	34903215	25518199	419.404m	498.617



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051324\
Data File : PL089510.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2024 15:32
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 04:36:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
Quant Title : GC Extractables
QLast Update : Fri Apr 26 19:27:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

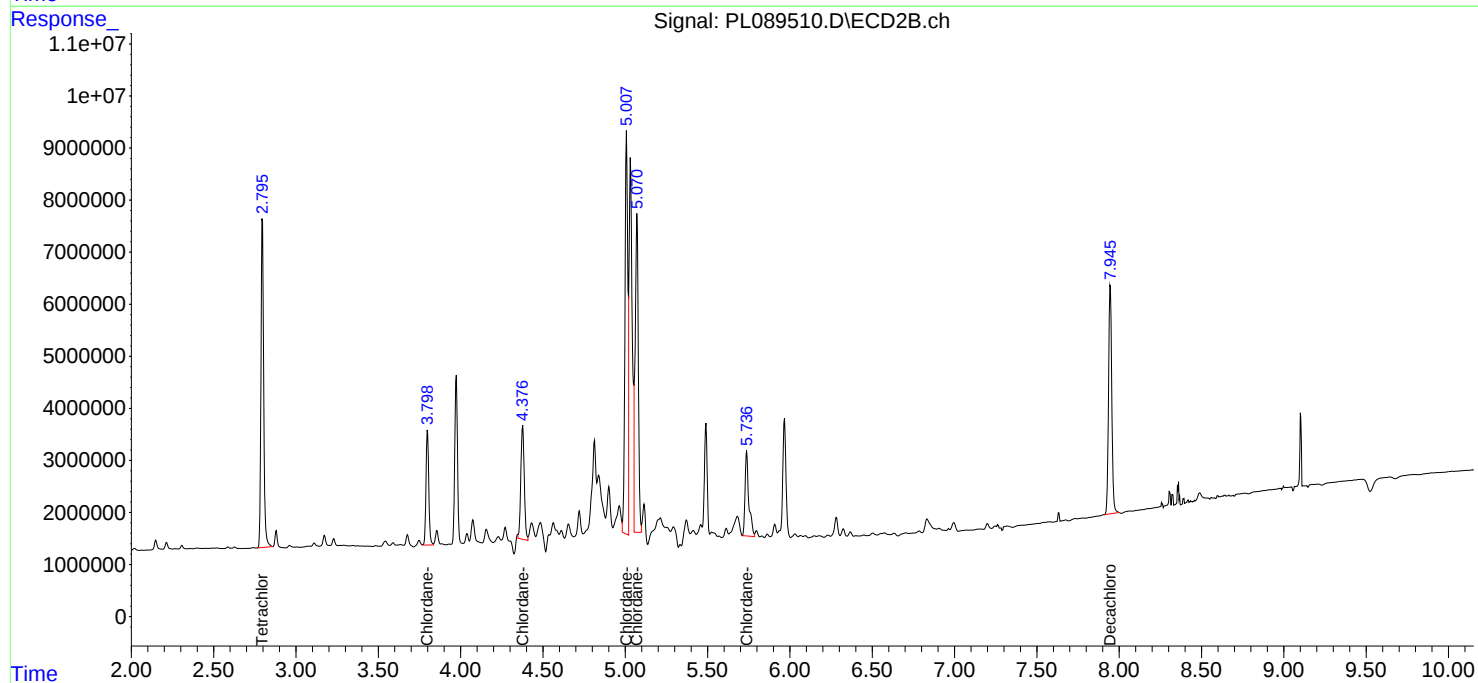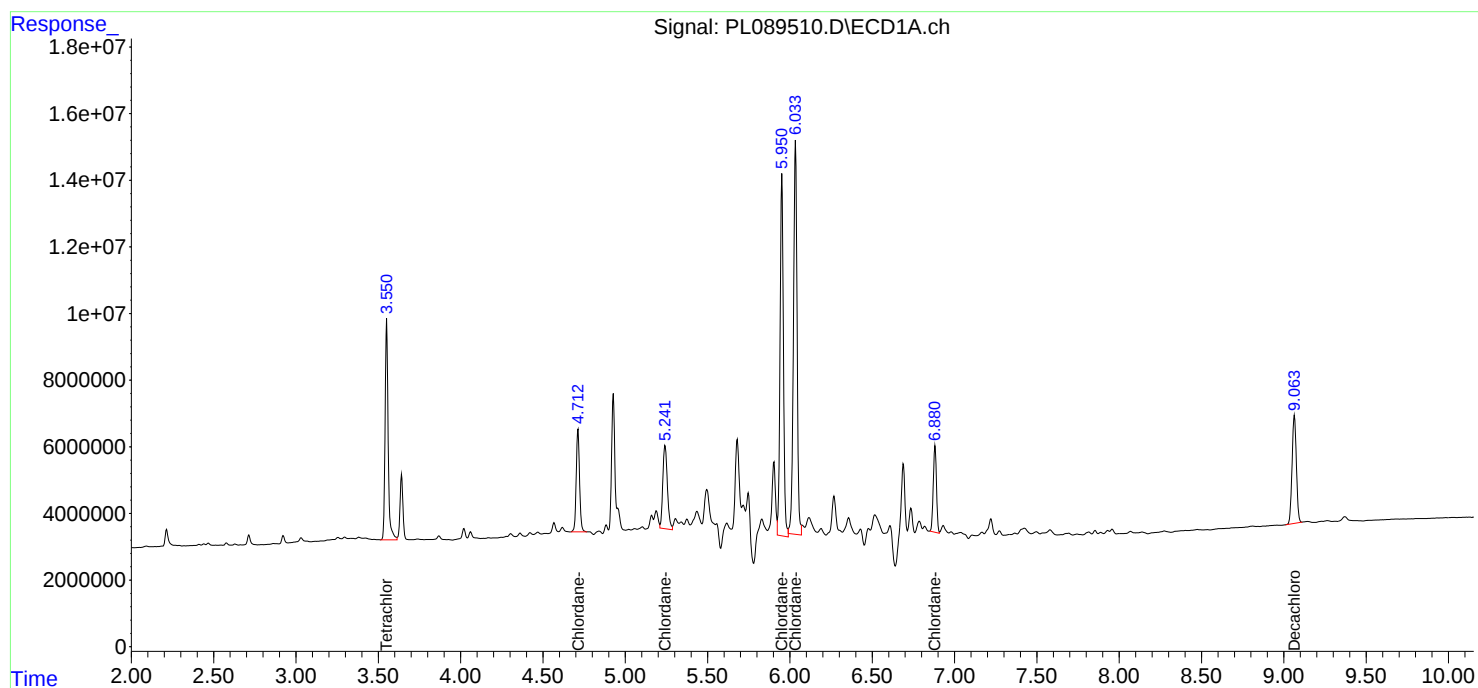


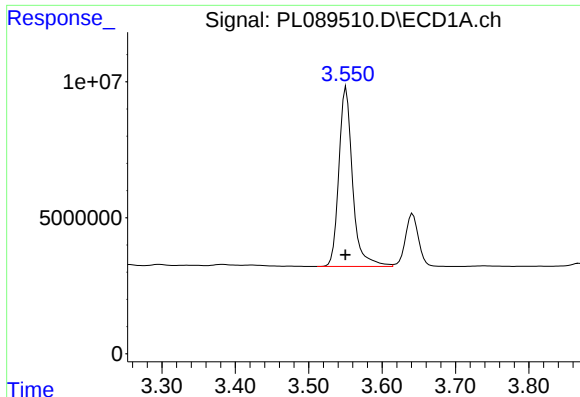

#1 Tetrachloro-m-xylene


R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 85723533
Conc: 42.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

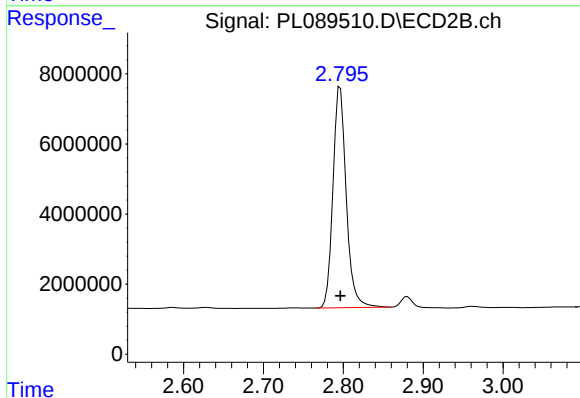


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 72861039
Conc: 56.79 ng/ml

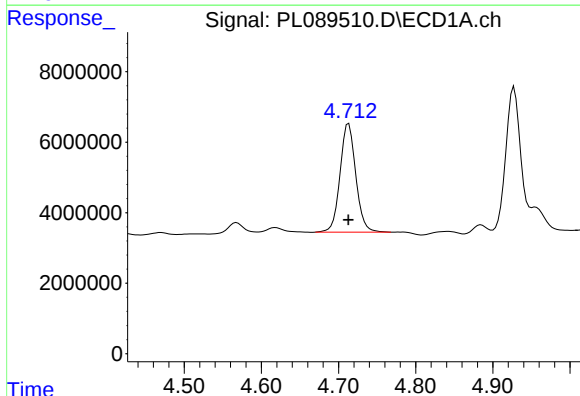


#23 Chlordane-1

R.T.: 4.712 min
Delta R.T.: 0.000 min
Response: 43657482
Conc: 478.17 ng/ml m

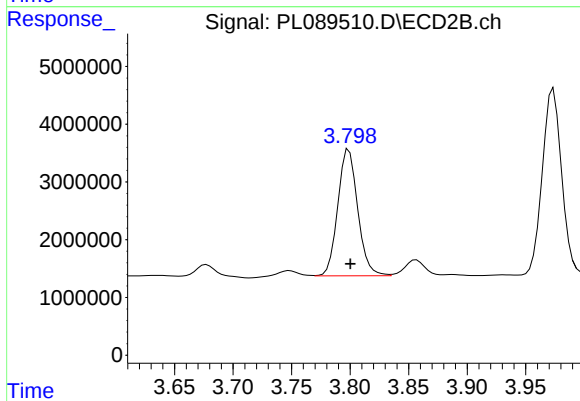

#23 Chlordane-1


R.T.: 3.799 min
Delta R.T.: -0.001 min
Response: 26032996
Conc: 529.11 ng/ml

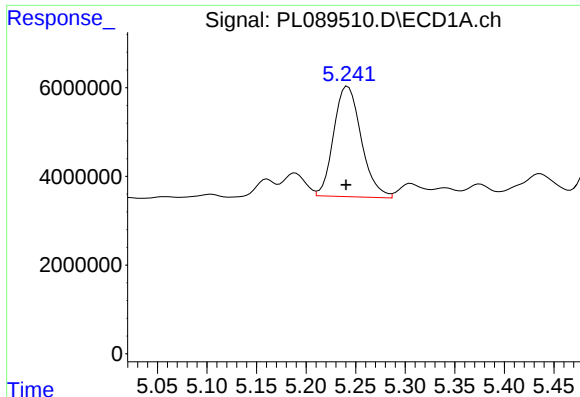

#24 Chlordane-2


R.T.: 5.241 min
Delta R.T.: 0.000 min
Response: 48322696
Conc: 459.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

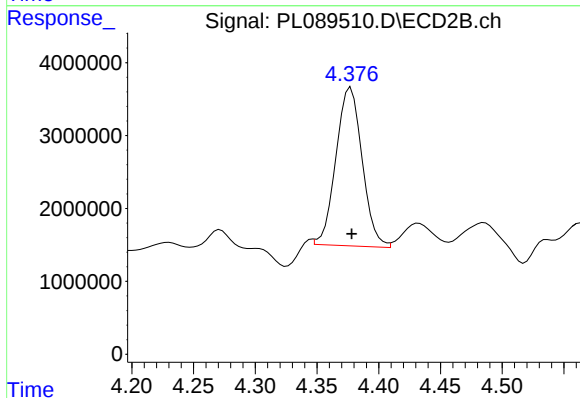


#24 Chlordane-2

R.T.: 4.376 min
Delta R.T.: -0.002 min
Response: 32002798
Conc: 503.07 ng/ml m

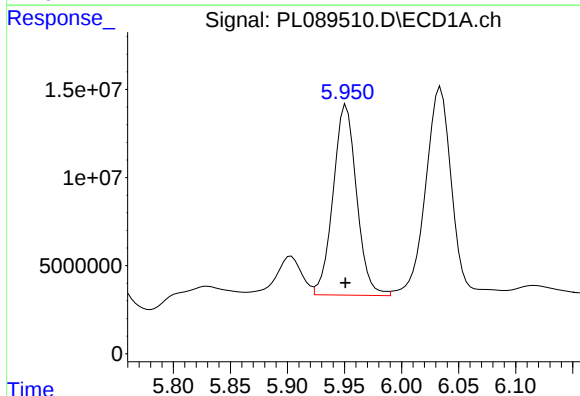


#25 Chlordane-3

R.T.: 5.950 min
Delta R.T.: 0.000 min
Response: 154770531
Conc: 468.64 ng/ml m

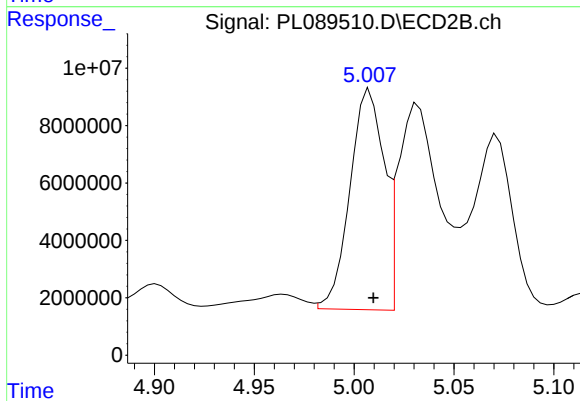

#25 Chlordane-3


R.T.: 5.008 min
Delta R.T.: -0.002 min
Response: 90699795
Conc: 529.72 ng/ml

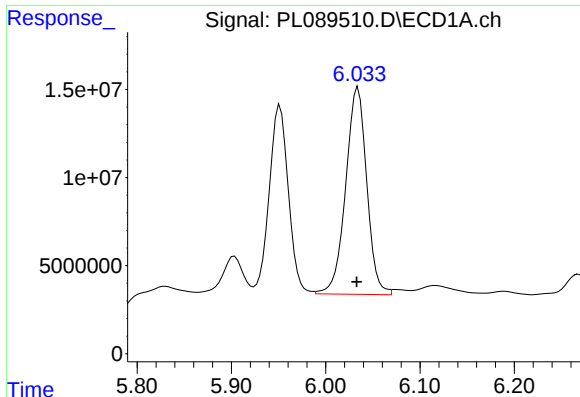

#26 Chlordane-4


R.T.: 6.033 min
Delta R.T.: 0.000 min
Response: 182243016
Conc: 447.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

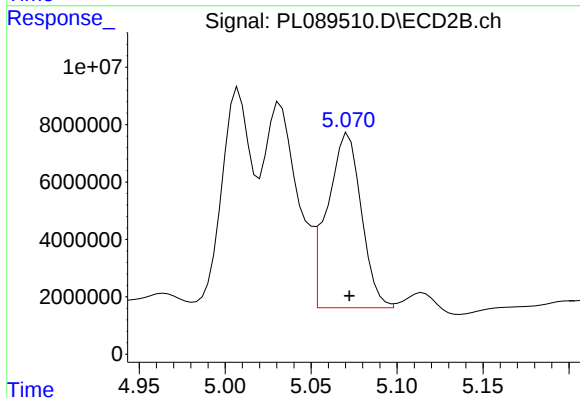


#26 Chlordane-4

R.T.: 5.070 min
Delta R.T.: -0.002 min
Response: 81235219
Conc: 505.05 ng/ml m

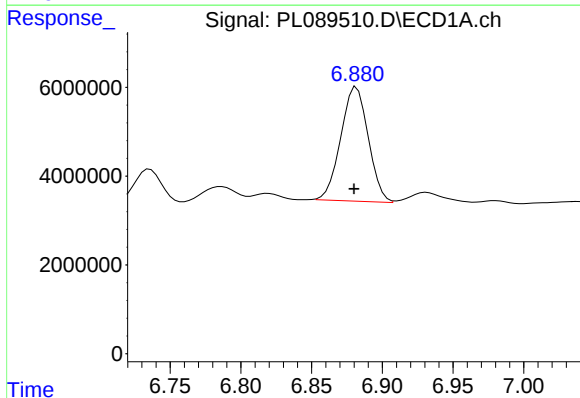


#27 Chlordane-5

R.T.: 6.880 min
Delta R.T.: 0.000 min
Response: 34903215
Conc: 419.40 ng/ml m

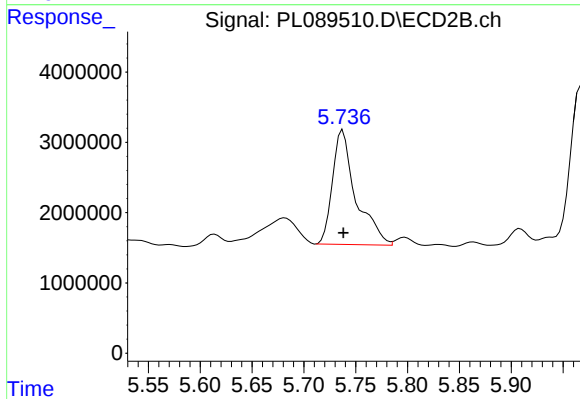

#27 Chlordane-5


R.T.: 5.738 min
Delta R.T.: 0.000 min
Response: 25518199
Conc: 498.62 ng/ml

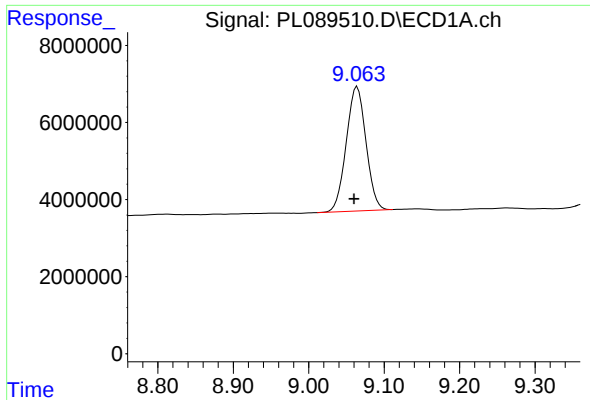

#28 Decachlorobiphenyl

R.T.: 9.064 min
Delta R.T.: 0.004 min
Response: 58678160
Conc: 41.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

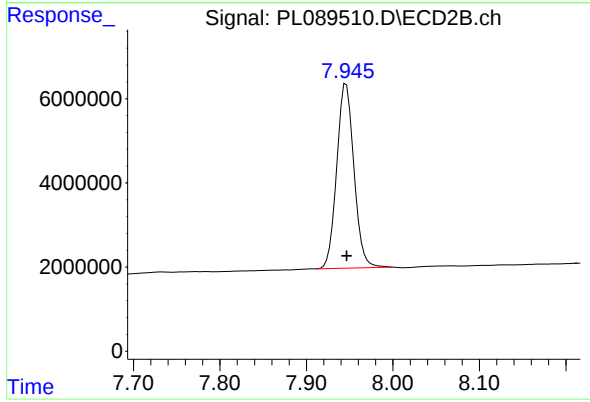

#28 Decachlorobiphenyl

R.T.: 7.946 min
Delta R.T.: 0.000 min
Response: 60422390
Conc: 44.92 ng/ml