

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051325\
 Data File : PL095640.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2025 13:59
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 14:09:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
 Quant Title : GC Extractables
 QLast Update : Tue May 13 14:09:36 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.593	2.911	186.5E6	272.6E6	50.000	50.000
28)	SA Decachlor...	9.115	8.088	157.5E6	194.2E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.758	3.930	111.0E6	112.5E6	500.000	500.000
24)	Chlordane-2	5.285	4.510	120.9E6	122.0E6	500.000	500.000
25)	Chlordane-3	5.990	5.148	464.1E6	356.2E6	500.000	500.000
26)	Chlordane-4	6.075	5.212	557.5E6	299.2E6	500.000	500.000
27)	Chlordane-5	6.915	6.108	91158414	135.2E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051325\
Data File : PL095640.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2025 13:59
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 14:09:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
Quant Title : GC Extractables
QLast Update : Tue May 13 14:09:36 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

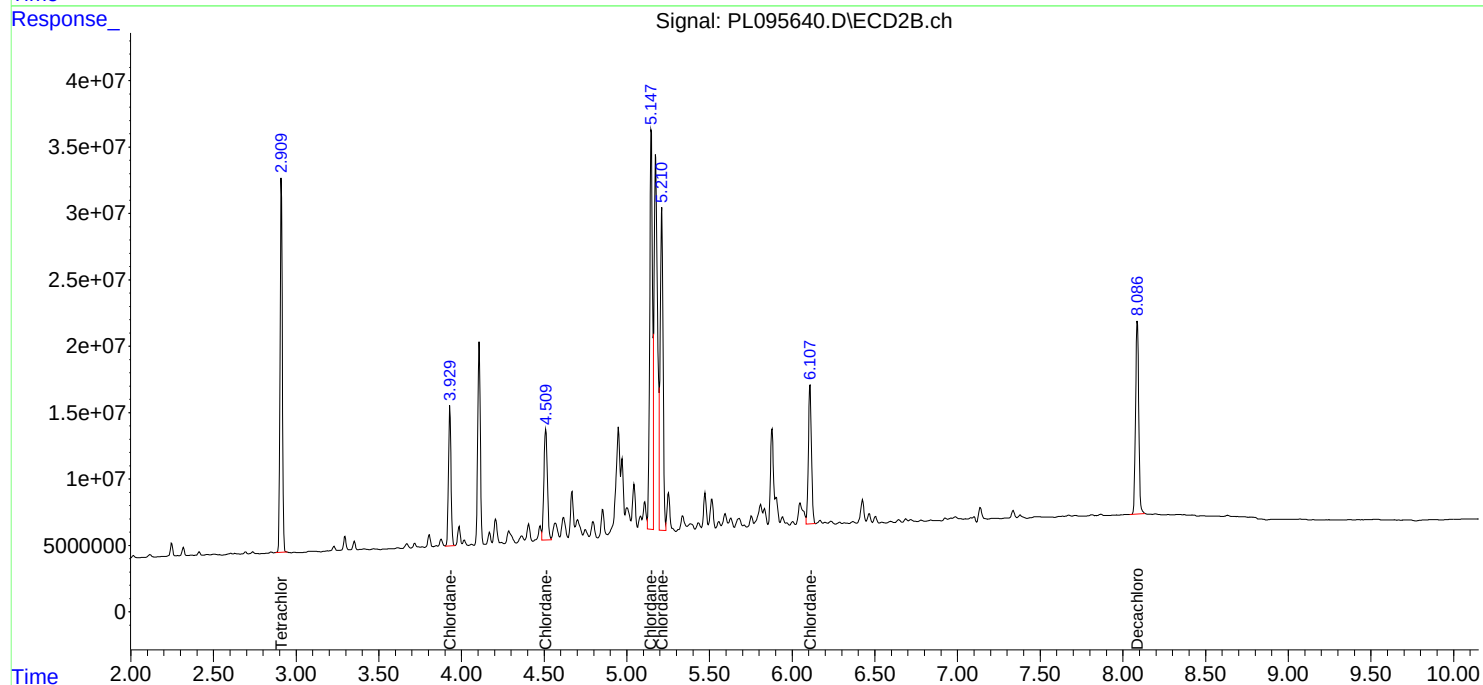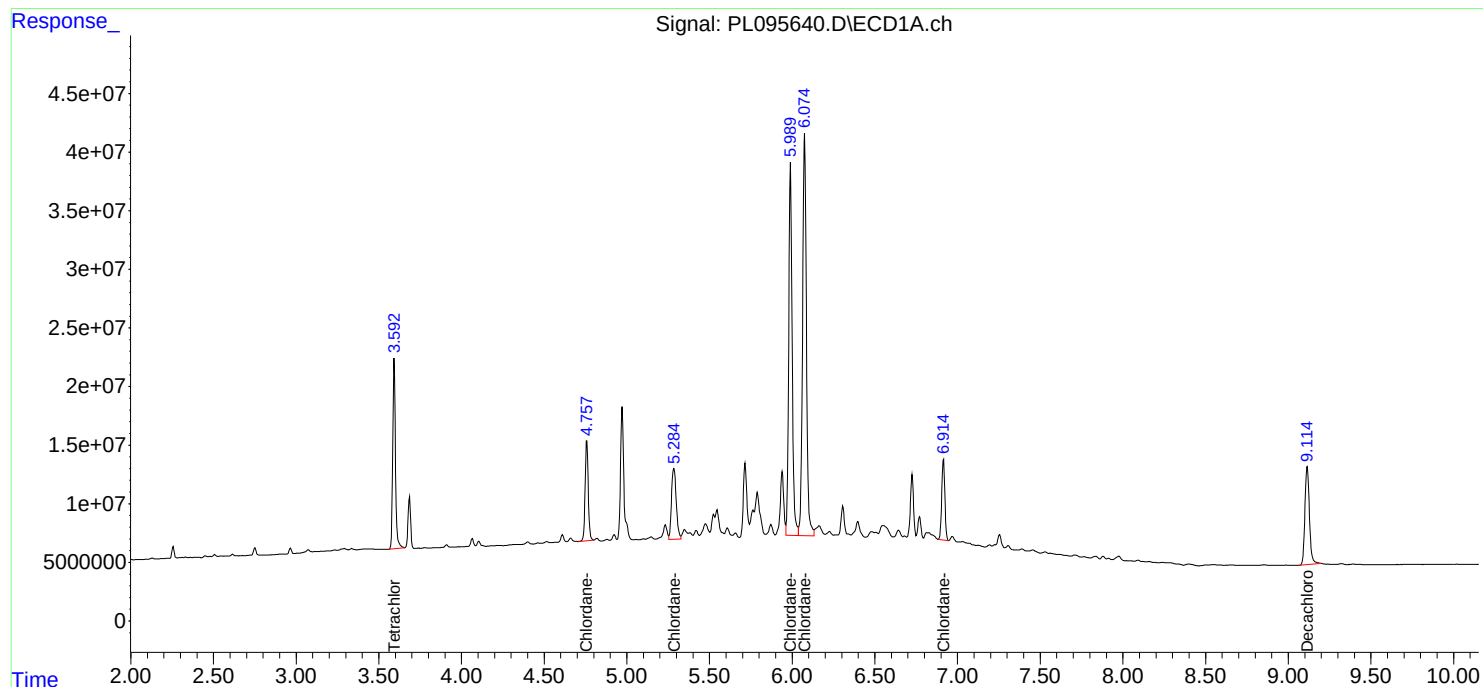


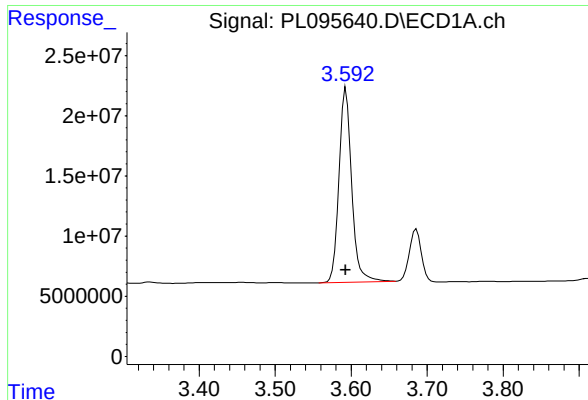

#1 Tetrachloro-m-xylene


R.T.: 3.593 min
Delta R.T.: 0.000 min
Response: 186500559
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

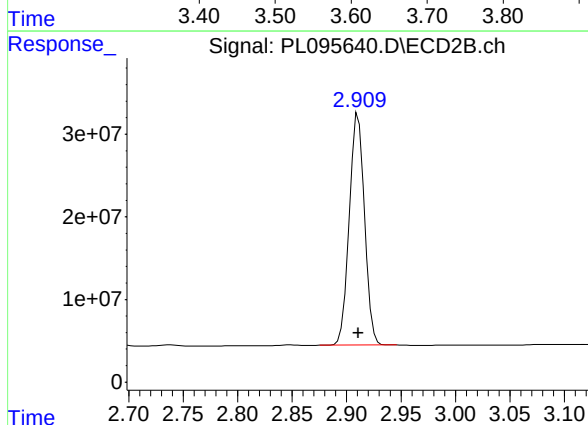


#1 Tetrachloro-m-xylene

R.T.: 2.911 min
Delta R.T.: 0.000 min
Response: 272604074
Conc: 50.00 ng/ml

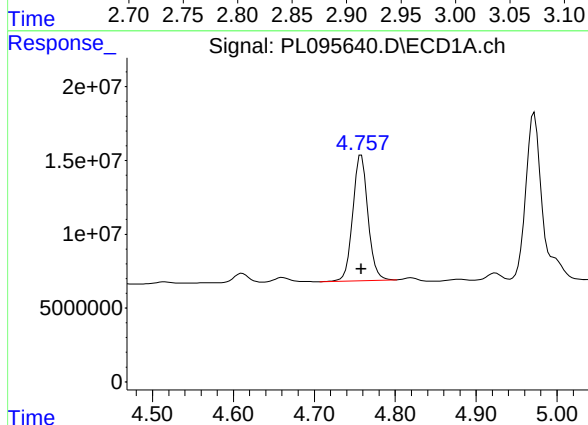


#23 Chlordane-1

R.T.: 4.758 min
Delta R.T.: 0.000 min
Response: 110973157
Conc: 500.00 ng/ml

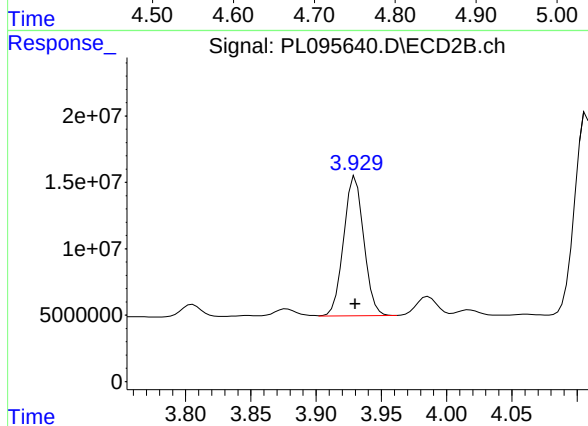

#23 Chlordane-1


R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 112480109
Conc: 500.00 ng/ml

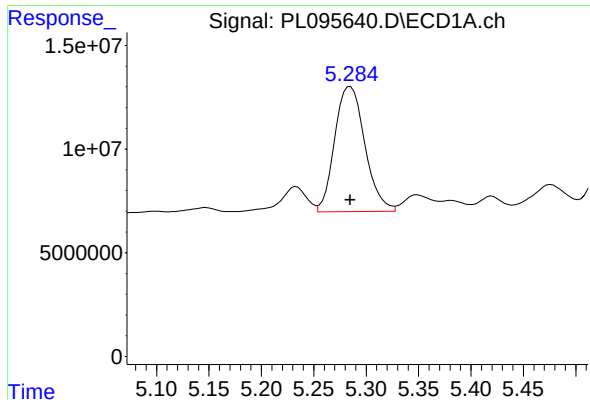

#24 Chlordane-2


R.T.: 5.285 min
Delta R.T.: 0.000 min
Response: 120893566
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

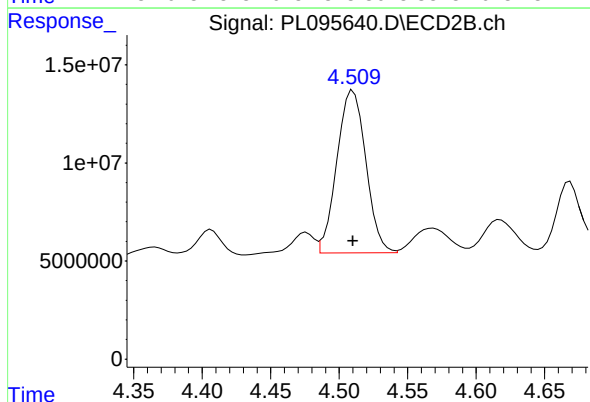


#24 Chlordane-2

R.T.: 4.510 min
Delta R.T.: 0.000 min
Response: 122033460
Conc: 500.00 ng/ml

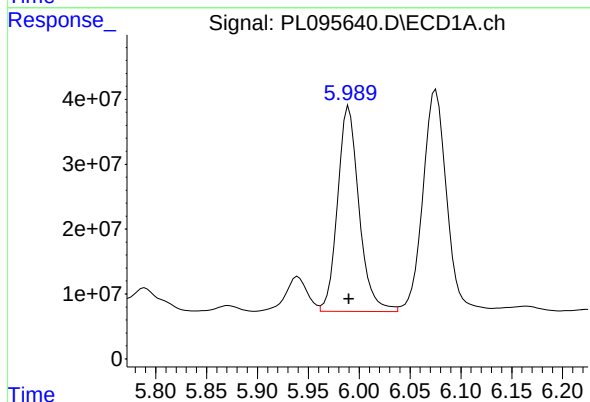


#25 Chlordane-3

R.T.: 5.990 min
Delta R.T.: 0.000 min
Response: 464097479
Conc: 500.00 ng/ml

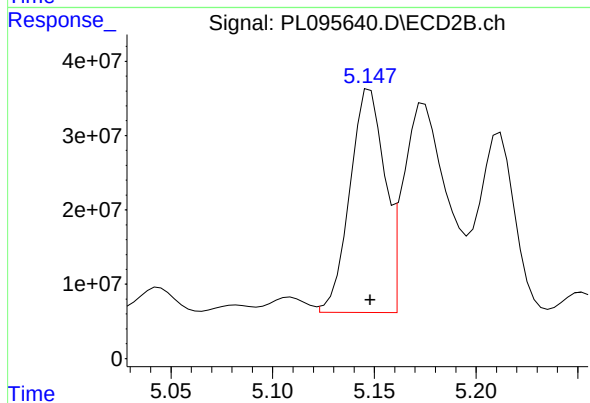

#25 Chlordane-3


R.T.: 5.148 min
Delta R.T.: 0.000 min
Response: 356151712
Conc: 500.00 ng/ml

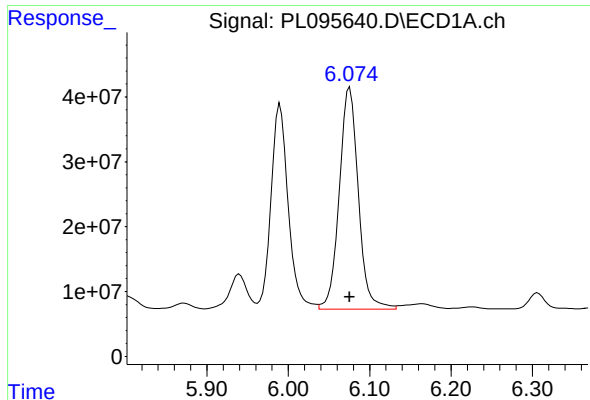

#26 Chlordane-4


R.T.: 6.075 min
Delta R.T.: 0.000 min
Response: 557487643
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

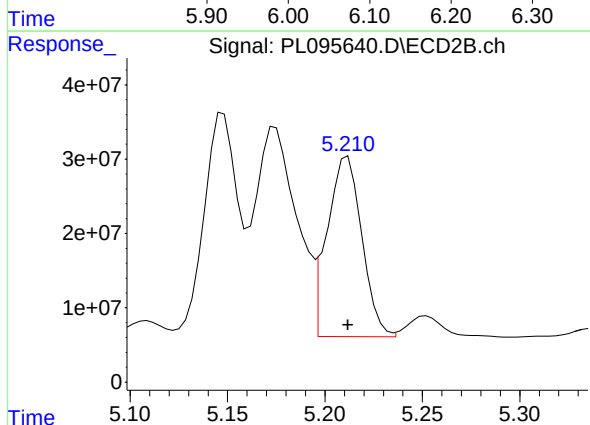


#26 Chlordane-4

R.T.: 5.212 min
Delta R.T.: 0.000 min
Response: 299194521
Conc: 500.00 ng/ml

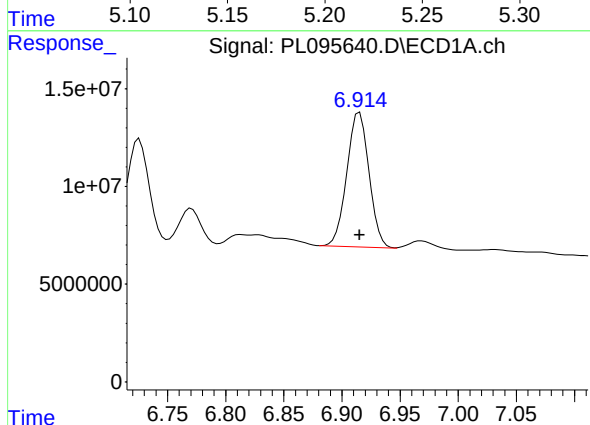


#27 Chlordane-5

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 91158414
Conc: 500.00 ng/ml

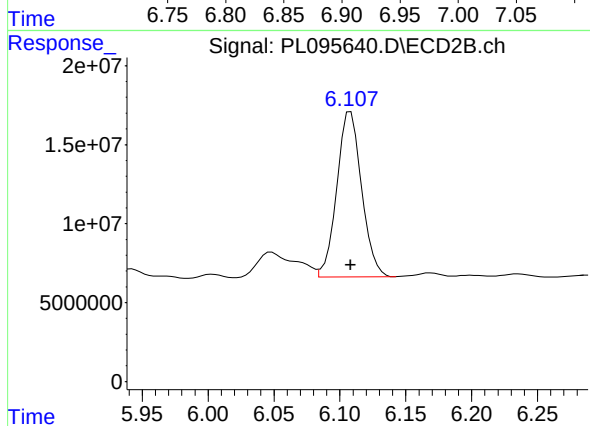

#27 Chlordane-5


R.T.: 6.108 min
Delta R.T.: 0.000 min
Response: 135186892
Conc: 500.00 ng/ml

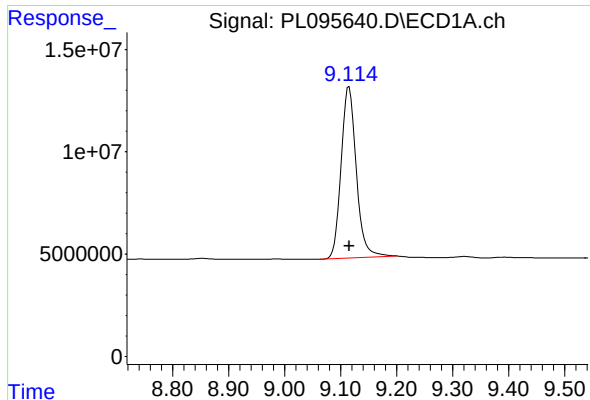

#28 Decachlorobiphenyl

R.T.: 9.115 min
Delta R.T.: 0.000 min
Response: 157521447
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

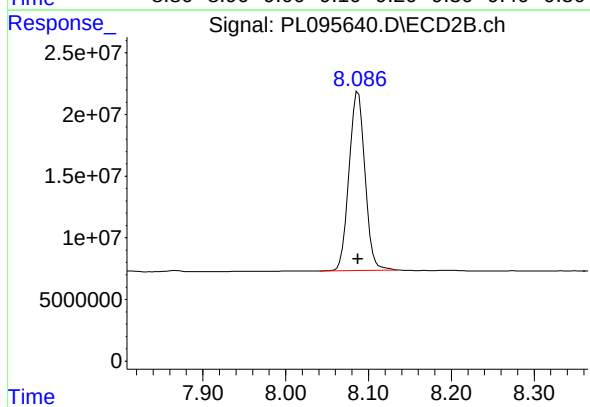

#28 Decachlorobiphenyl

R.T.: 8.088 min
Delta R.T.: 0.000 min
Response: 194157688
Conc: 50.00 ng/ml