

Data Path : \\74.0.250.170\terastorage\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051419\
 Data File : PL048517.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2019 13:38
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 01:00:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.940	155.4E6	42583766	16.044	17.096
28)	SA Decachlor...	7.996	8.978	143.5E6	80393270	14.275	30.288 #
Target Compounds							
9)	A Endosulfan I	5.331	6.164	-1277725	7630171	N.D.	2.699
13)	MA Dieldrin	5.576	0.000	97105537	0	7.458	N.D. #
14)	MA Endrin	5.831f	0.000	47701482	0	3.918	N.D. #
15)	B Endosulfa...	0.000	6.852	0	5683061	N.D.	2.107 #
18)	B Endrin al...	6.275f	0.000	110.7E6	0	11.387	N.D. #
20)	A Methoxychlor	6.706f	7.516	63169659	36849733	11.602	26.993 #
22)	Mirex	7.114	0.000	118.7E6	0	13.244	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\terastorage\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051419\
Data File : PL048517.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2019 13:38
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 01:00:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

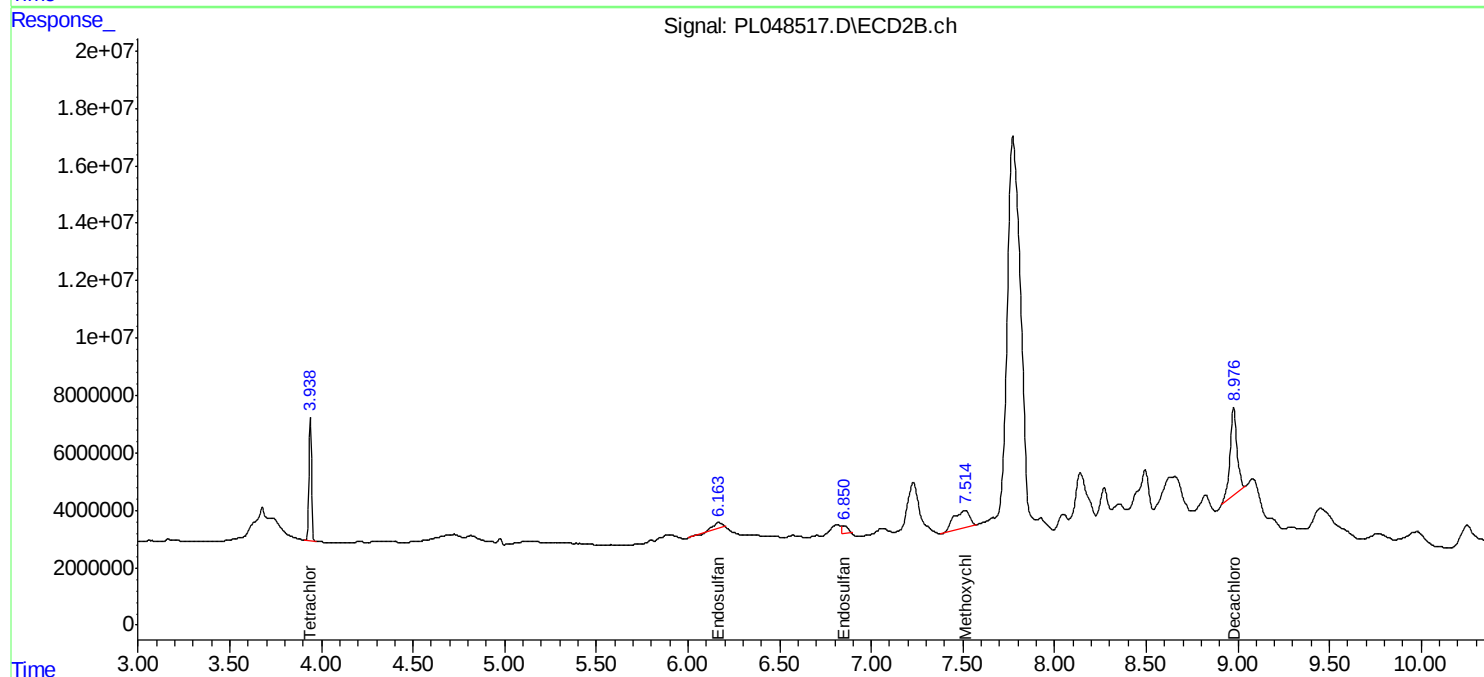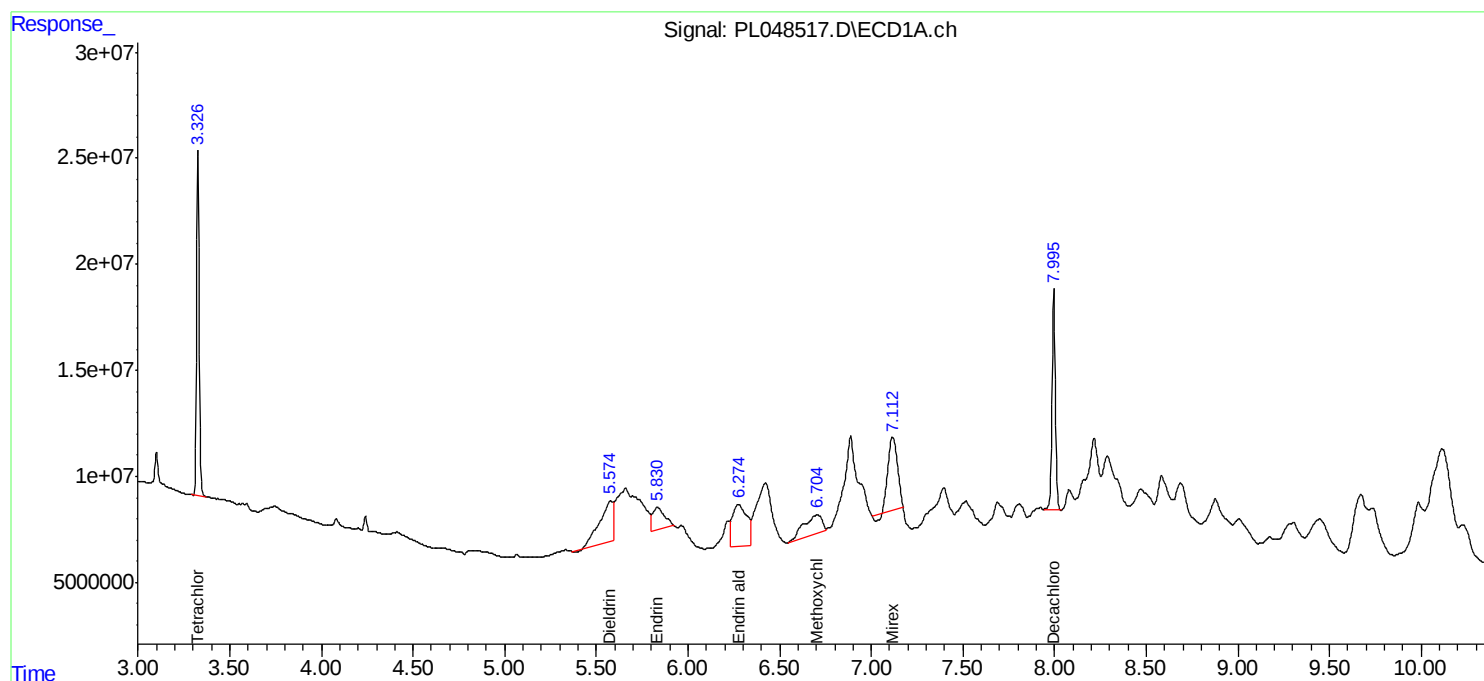


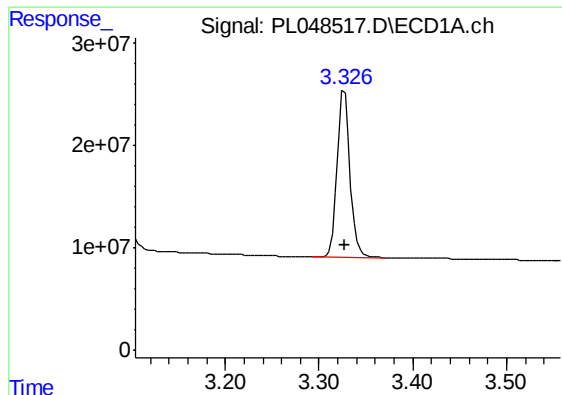

#1 Tetrachloro-m-xylene


R.T.: 3.327 min
Delta R.T.: 0.000 min
Response: 155417746
Conc: 16.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

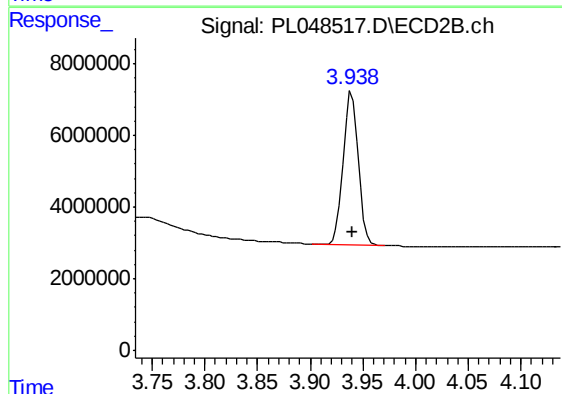


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 42583766
Conc: 17.10 ng/ml

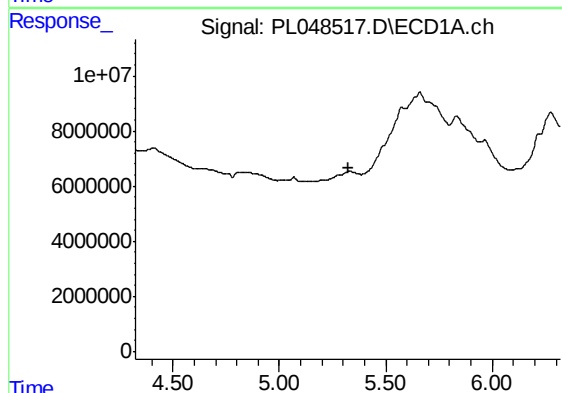


#9 Endosulfan I

R.T.: 5.331 min
Delta R.T.: 0.008 min
Response: -1277725
Conc: N.D.

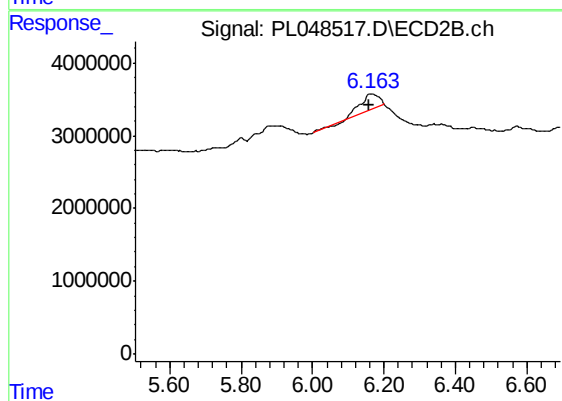

#9 Endosulfan I


R.T.: 6.164 min
Delta R.T.: 0.005 min
Response: 7630171
Conc: 2.70 ng/ml

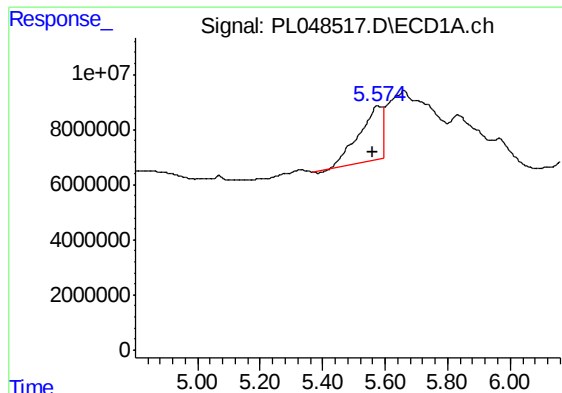

#13 Dieldrin


R.T.: 5.576 min
Delta R.T.: 0.014 min
Response: 97105537
Conc: 7.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

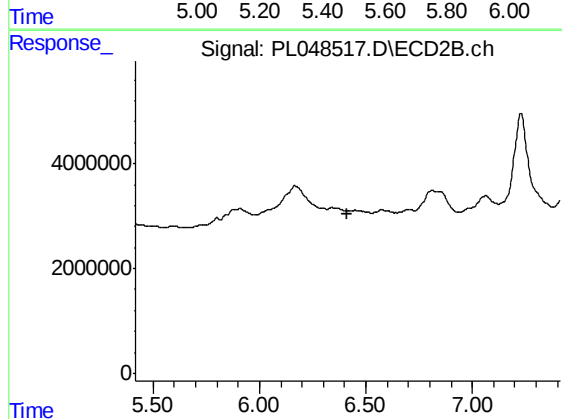


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

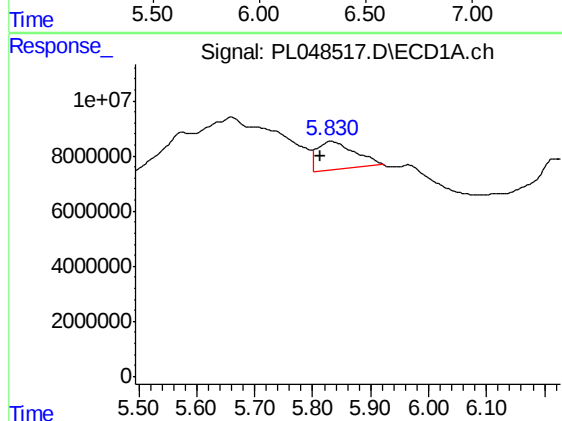


#14 Endrin

R.T.: 5.831 min
Delta R.T.: 0.017 min
Response: 47701482
Conc: 3.92 ng/ml

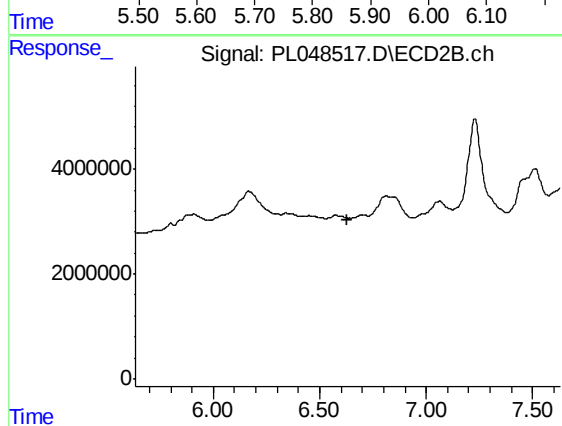

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.632 min
Response: 0
Conc: N.D.

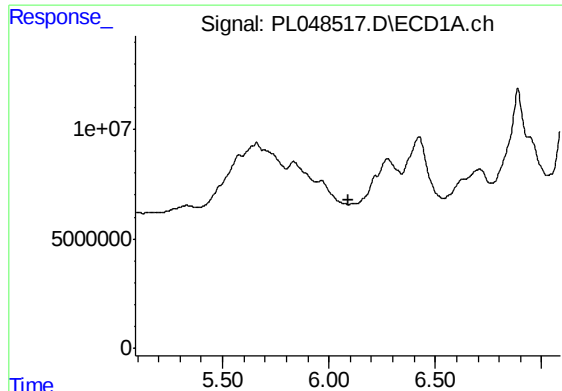

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

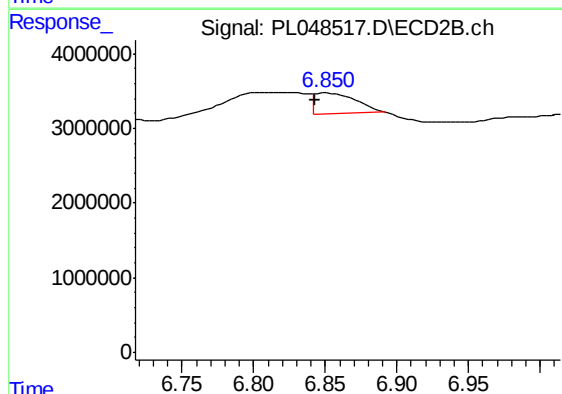


#15 Endosulfan II

R.T.: 6.852 min
Delta R.T.: 0.009 min
Response: 5683061
Conc: 2.11 ng/ml

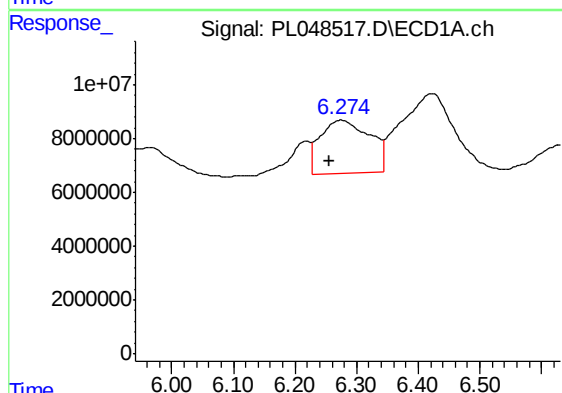


#18 Endrin aldehyde

R.T.: 6.275 min
Delta R.T.: 0.019 min
Response: 110659990
Conc: 11.39 ng/ml

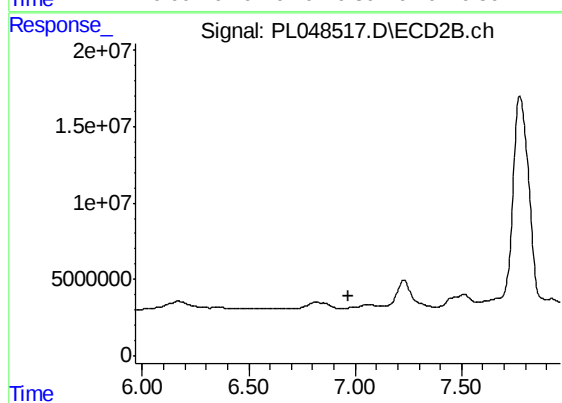

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.967 min
Response: 0
Conc: N.D.

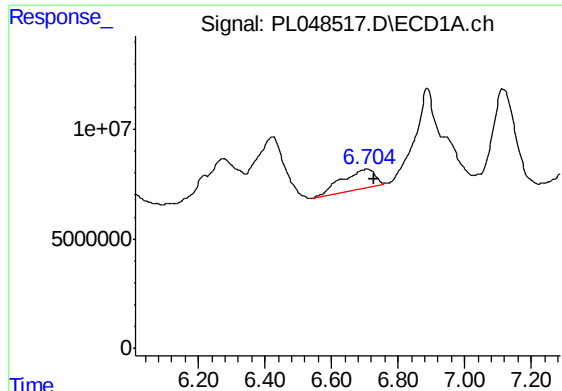

#20 Methoxychlor


R.T.: 6.706 min
Delta R.T.: -0.023 min
Response: 63169659
Conc: 11.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

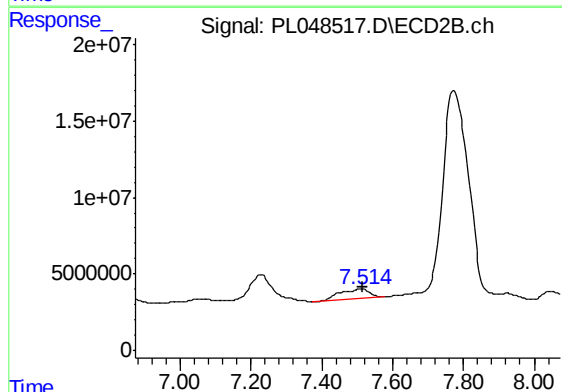


#20 Methoxychlor

R.T.: 7.516 min
Delta R.T.: 0.000 min
Response: 36849733
Conc: 26.99 ng/ml

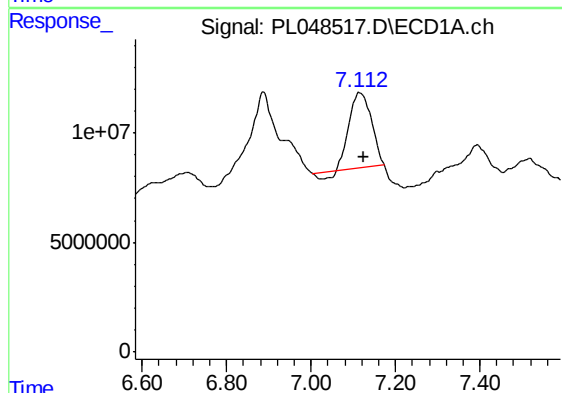


#22 Mirex

R.T.: 7.114 min
Delta R.T.: -0.010 min
Response: 118716826
Conc: 13.24 ng/ml

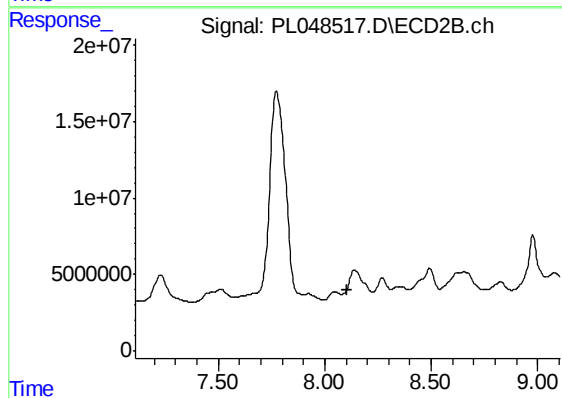

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.109 min
Response: 0
Conc: N.D.

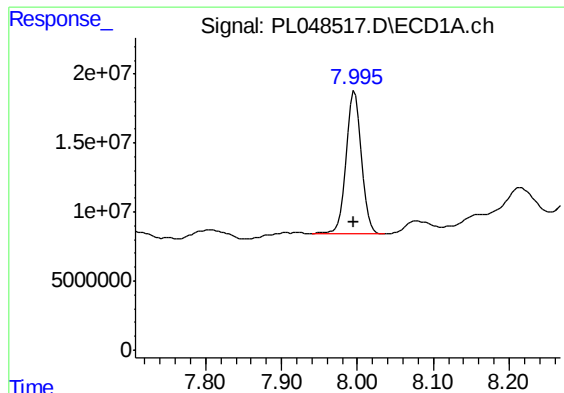

#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 143526242
Conc: 14.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

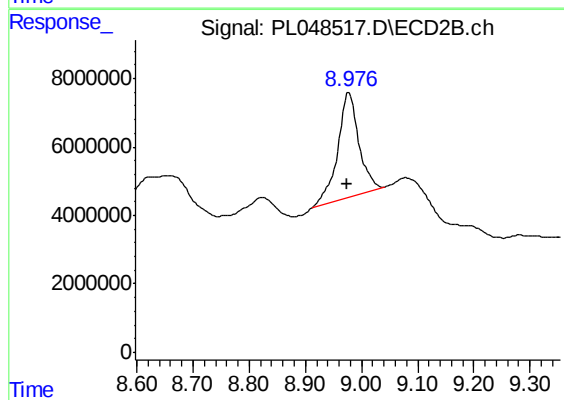

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: 0.003 min
Response: 80393270
Conc: 30.29 ng/ml