

Data Path : \\74.0.250.170\terastorage\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051419\
 Data File : PL048521.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2019 14:45
 Operator : AJ\SJ
 Sample : K2845-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FEBH-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 01:02:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.326	3.940	203.0E6	52608165	20.958	21.120
28)	SA Decachlor...	7.995	8.978	166.1E6	42228869	16.523	15.910
Target Compounds							
10)	B gamma-Chl...	5.237f	0.000	12922589	0	0.968	N.D. #
11)	B alpha-Chl...	5.280	0.000	4892503	0	0.374	N.D. #
22)	Mirex	7.153f	0.000	2921110	0	0.326	N.D. #
25)	Chlordane-3	5.237f	0.000	12922589	0	8.207	N.D. #
26)	Chlordane-4	5.280	0.000	4892503	0	3.370	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\terastorage\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051419\
Data File : PL048521.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2019 14:45
Operator : AJ\SJ
Sample : K2845-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
FEBH-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 01:02:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

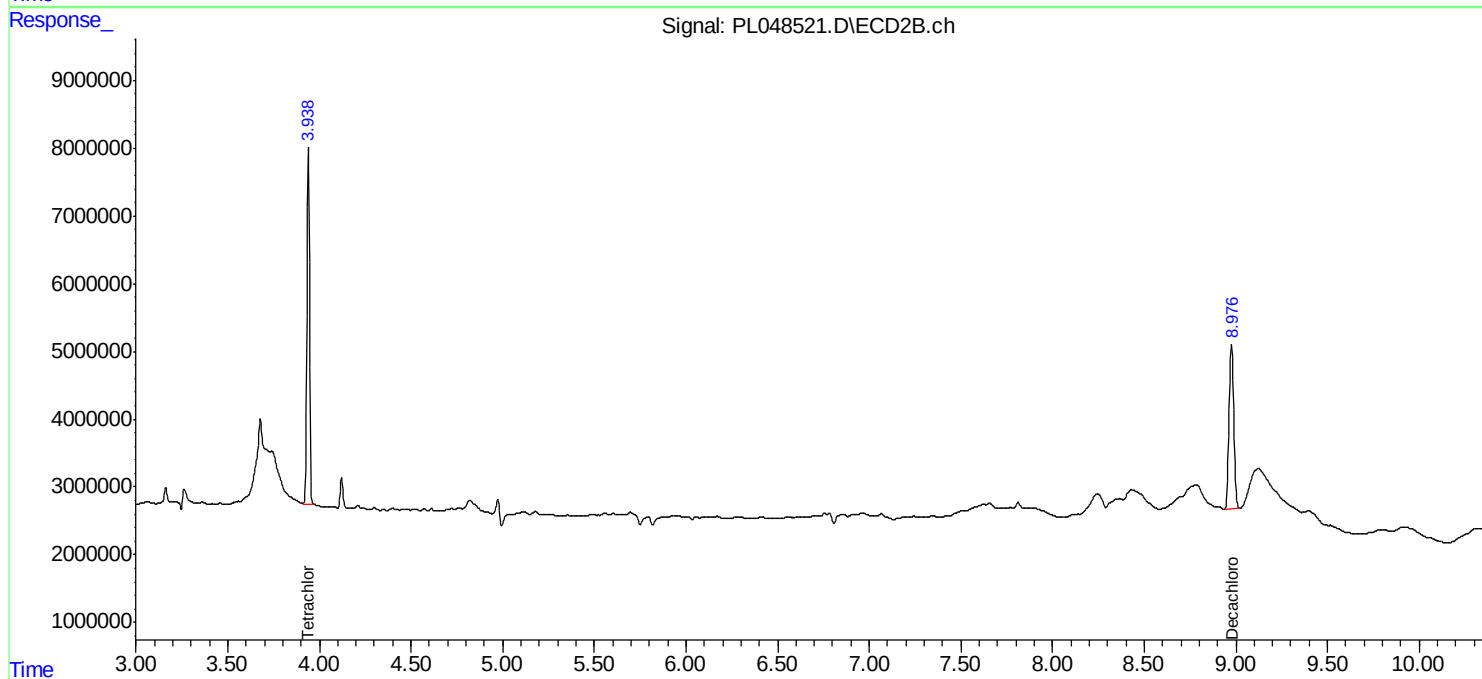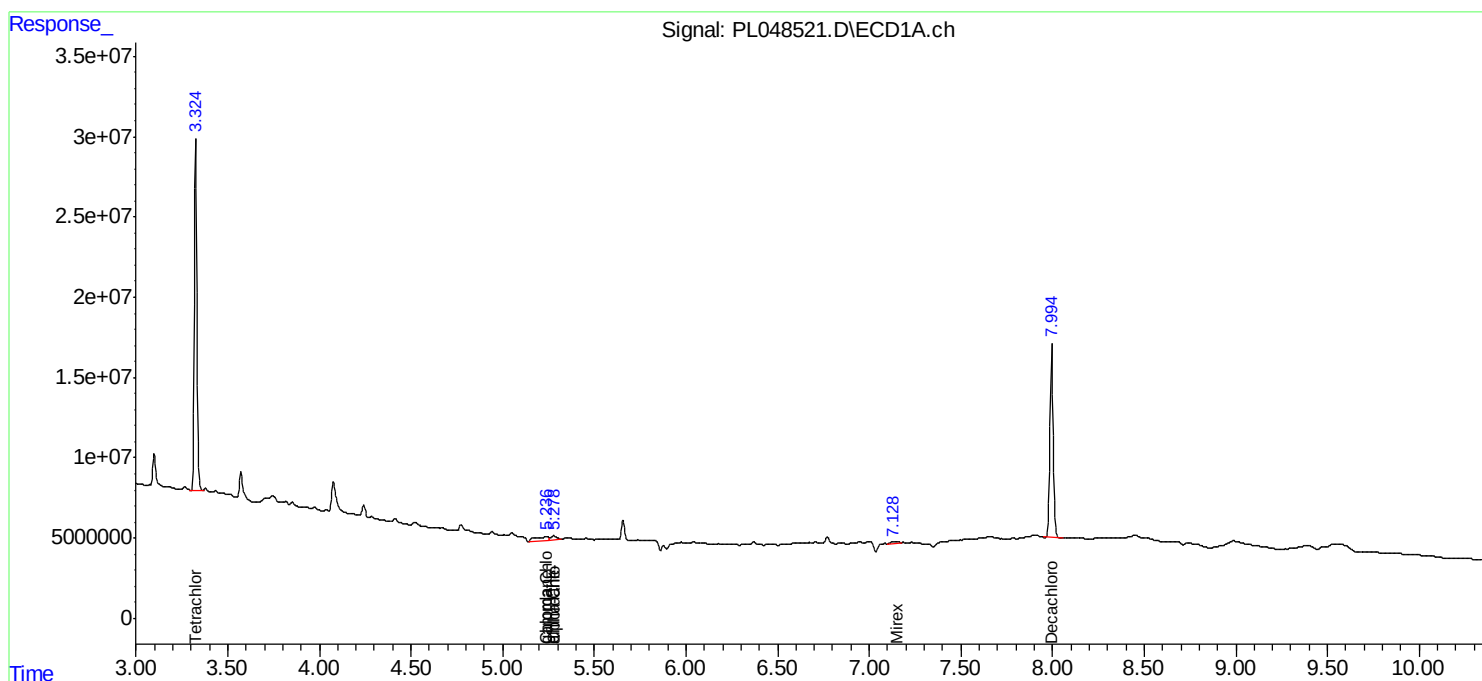


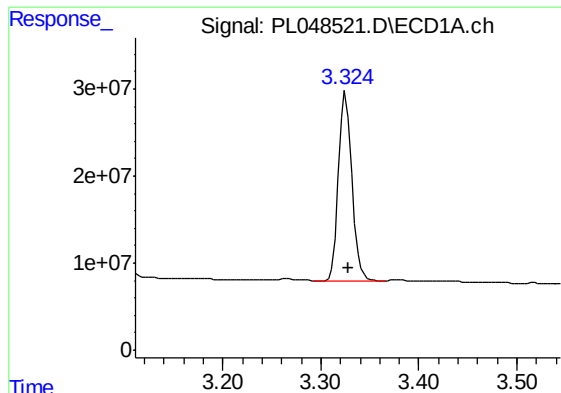

#1 Tetrachloro-m-xylene


R.T.: 3.326 min
Delta R.T.: -0.002 min
Response: 203018349
Conc: 20.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
FEBH-01

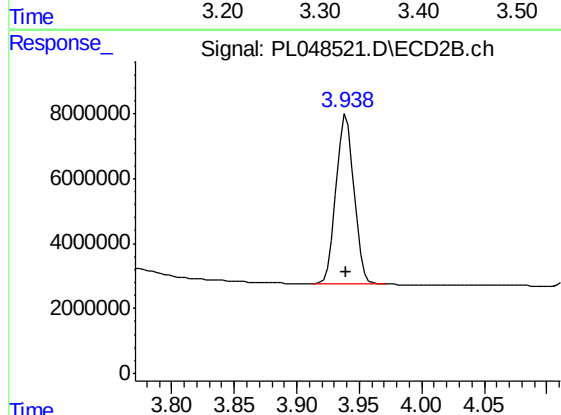


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 52608165
Conc: 21.12 ng/ml

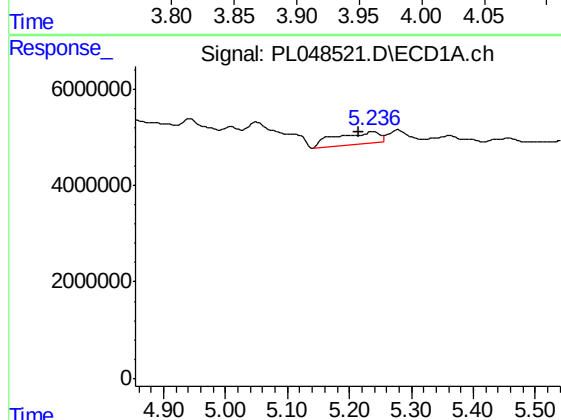


#10 gamma-Chlordane

R.T.: 5.237 min
Delta R.T.: 0.022 min
Response: 12922589
Conc: 0.97 ng/ml

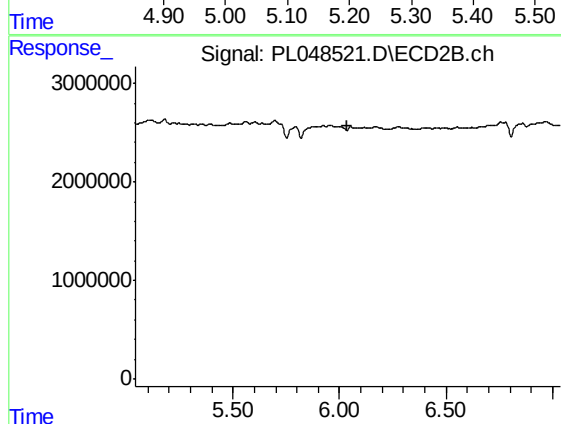

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

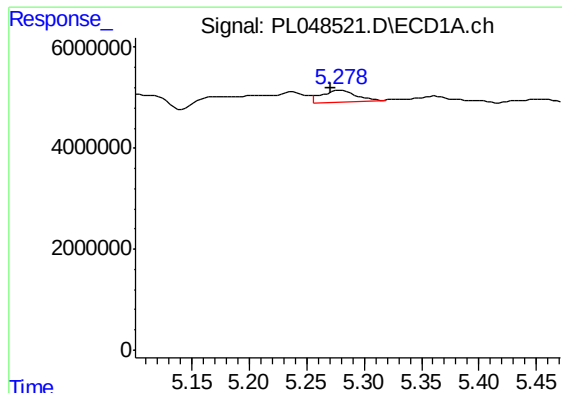

#11 alpha-Chlordane


R.T.: 5.280 min
Delta R.T.: 0.009 min
Response: 4892503
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
FEBH-01

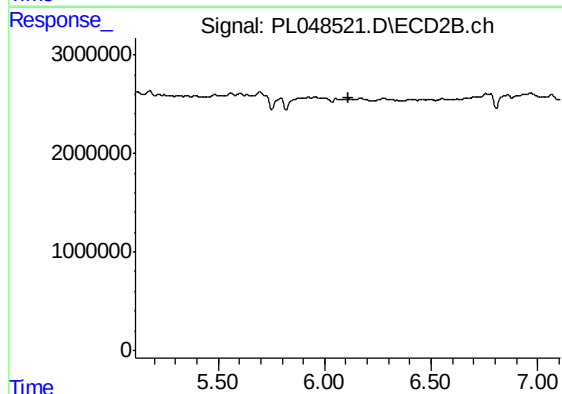


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.109 min
Response: 0
Conc: N.D.

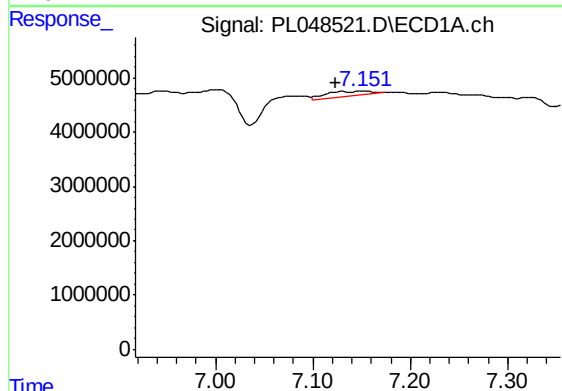


#22 Mirex

R.T.: 7.153 min
Delta R.T.: 0.029 min
Response: 2921110
Conc: 0.33 ng/ml

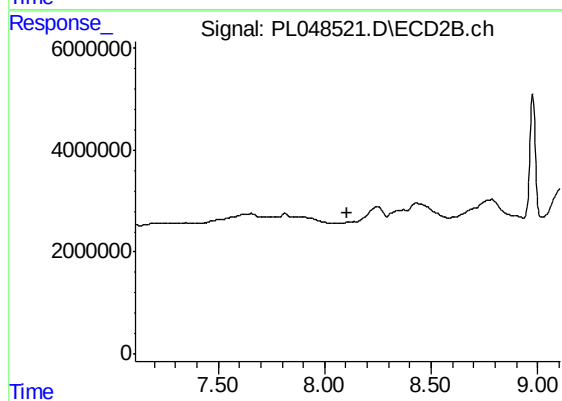

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.109 min
Response: 0
Conc: N.D.

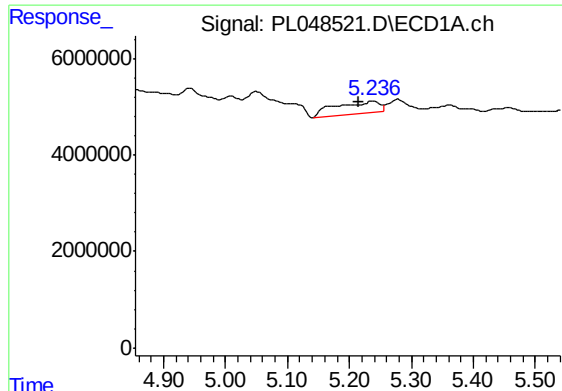

#25 Chlordane-3


R.T.: 5.237 min
Delta R.T.: 0.022 min
Response: 12922589
Conc: 8.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
FEBH-01

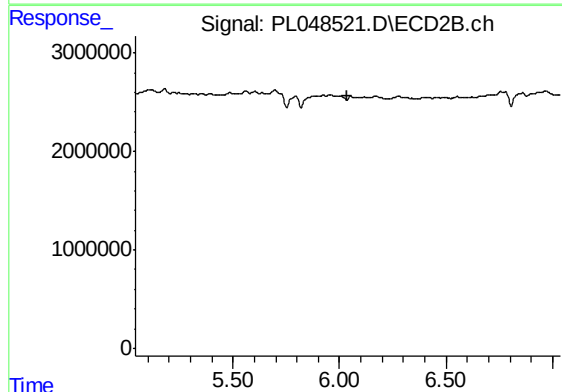


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

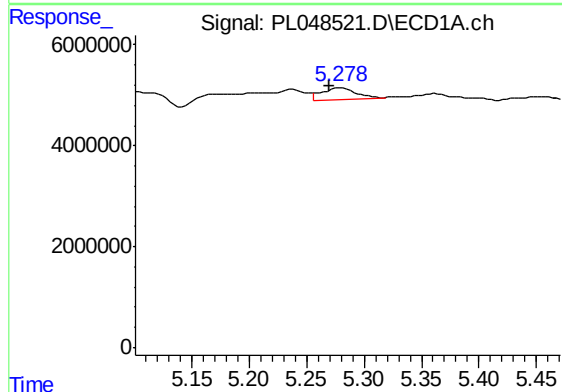


#26 Chlordane-4

R.T.: 5.280 min
Delta R.T.: 0.010 min
Response: 4892503
Conc: 3.37 ng/ml

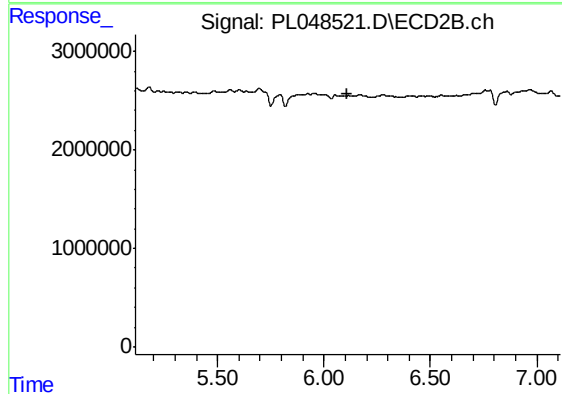

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.111 min
Response: 0
Conc: N.D.

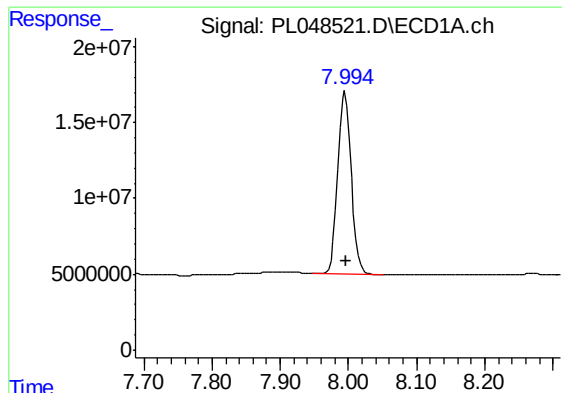

#28 Decachlorobiphenyl

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 166128170
Conc: 16.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
FEBH-01

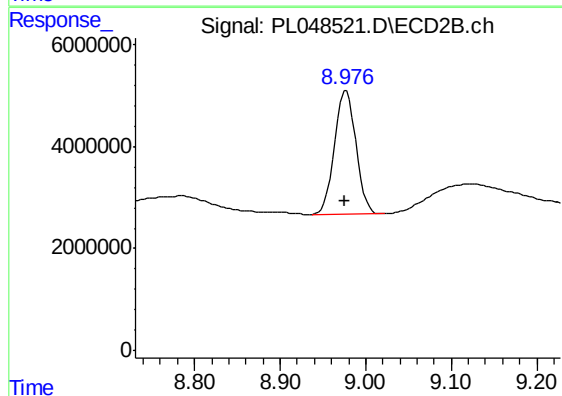

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: 0.003 min
Response: 42228869
Conc: 15.91 ng/ml