

Data Path : \\74.0.250.170\terastorage\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051419\
 Data File : PL048523.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2019 15:15
 Operator : AJ\SJ
 Sample : K2845-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FEBH-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 01:02:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.940	202.7E6	52081566	20.924	20.909
28)	SA Decachlor...	7.996	8.979	180.4E6	47315434	17.946	17.826
Target Compounds							
4)	MA Heptachlor	0.000	5.114	0	14898498	N.D.	4.304 #
8)	B Heptachlo...	0.000	5.790	0	6590773	N.D.	2.260 #
10)	B gamma-Chl...	5.206	0.000	10577493	0	0.792	N.D. #
11)	B alpha-Chl...	5.283	0.000	5655448	0	0.433	N.D. #
16)	A 4,4'-DDD	5.977f	0.000	2012243	0	0.207	N.D. #
25)	Chlordane-3	5.206	0.000	10577493	0	6.718	N.D. #
26)	Chlordane-4	5.283	0.000	5655448	0	3.895	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\terastorage\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051419\
Data File : PL048523.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2019 15:15
Operator : AJ\SJ
Sample : K2845-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
FEBH-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 01:02:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

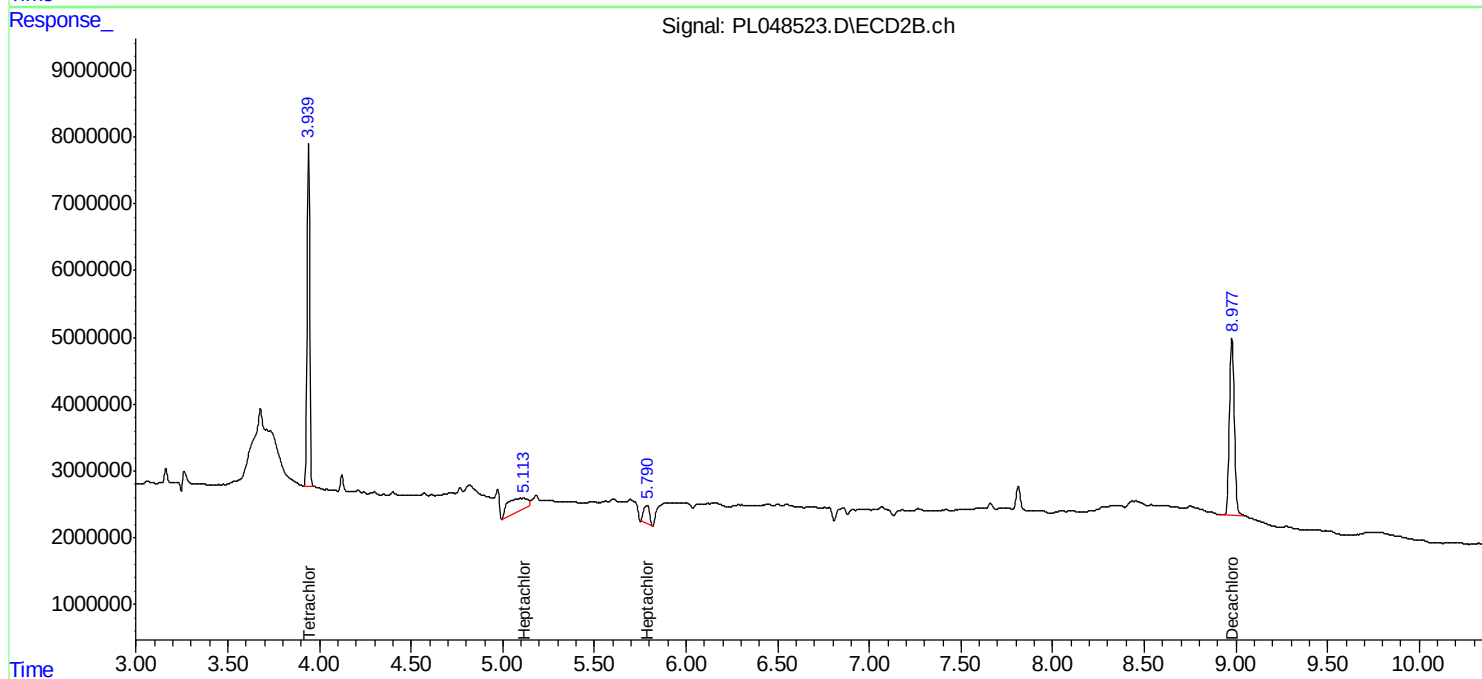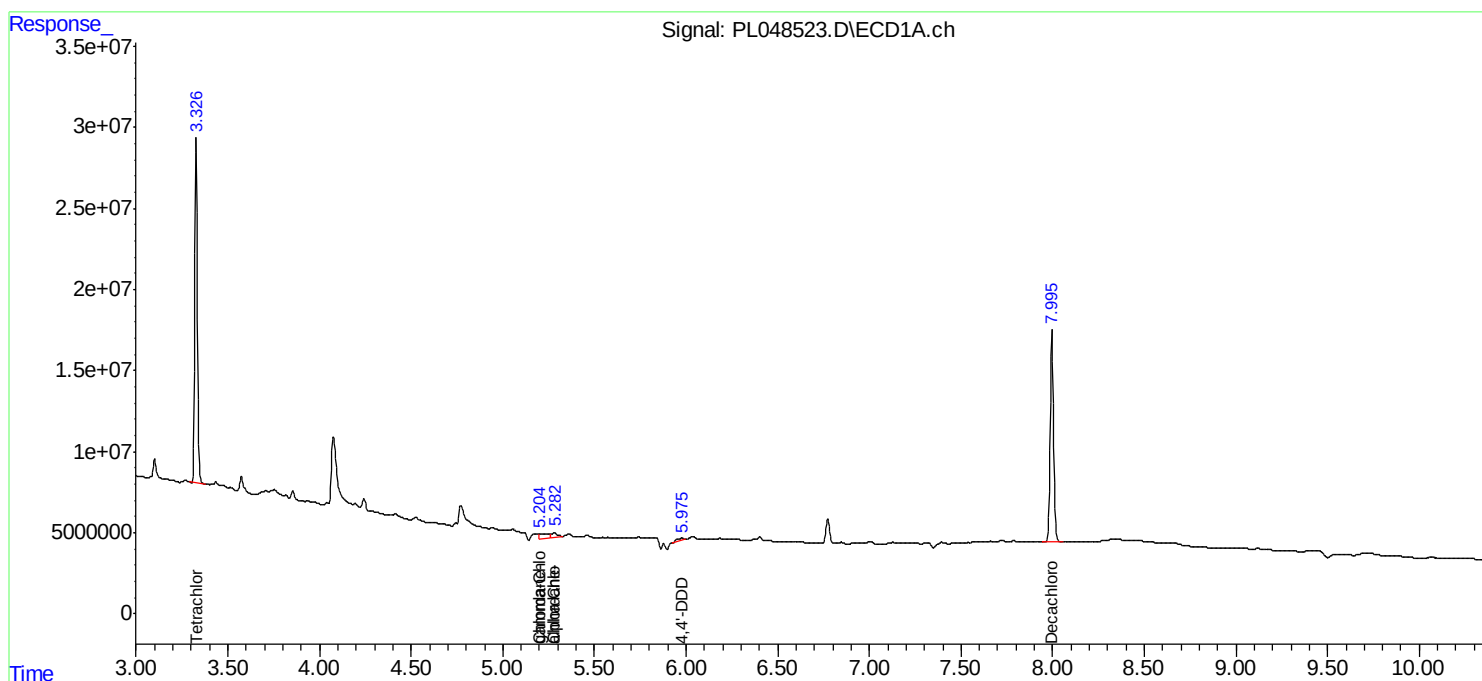


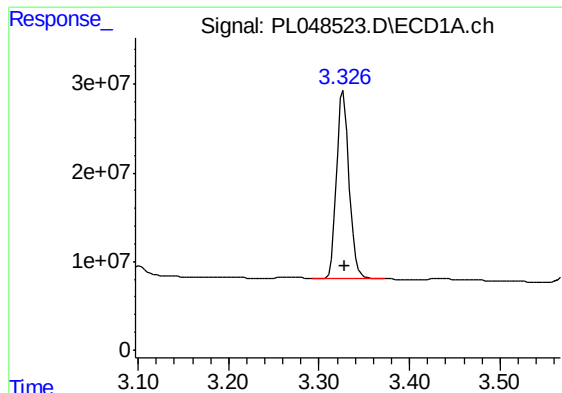

#1 Tetrachloro-m-xylene


R.T.: 3.327 min
Delta R.T.: 0.000 min
Response: 202689082
Conc: 20.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
FEBH-03

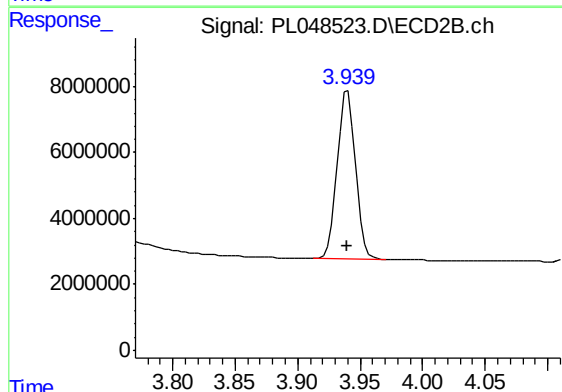


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 52081566
Conc: 20.91 ng/ml

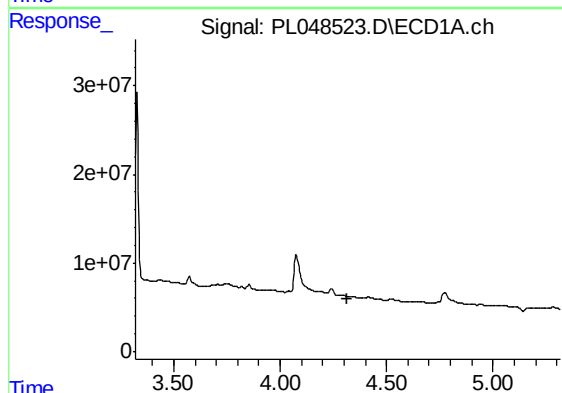


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

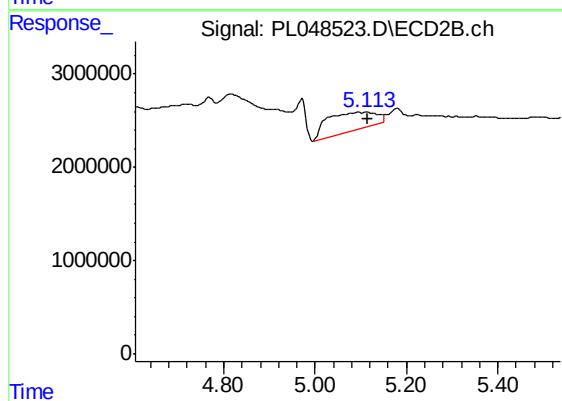

#4 Heptachlor


R.T.: 5.114 min
Delta R.T.: -0.001 min
Response: 14898498
Conc: 4.30 ng/ml

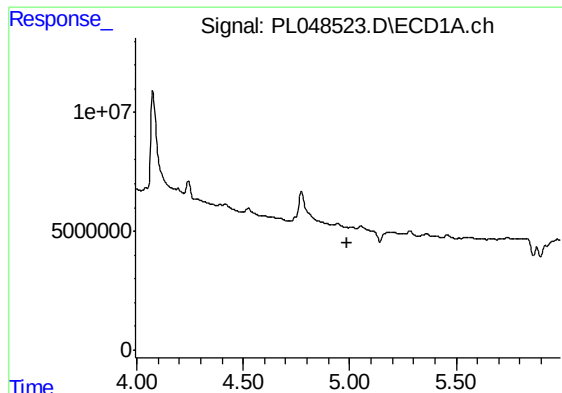

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FEBH-03

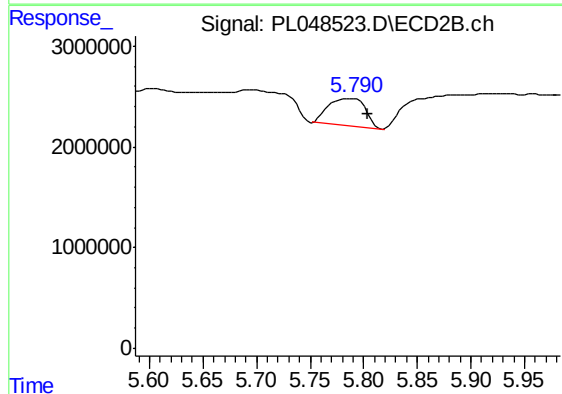


#8 Heptachlor epoxide

R.T.: 5.790 min
Delta R.T.: -0.014 min
Response: 6590773
Conc: 2.26 ng/ml

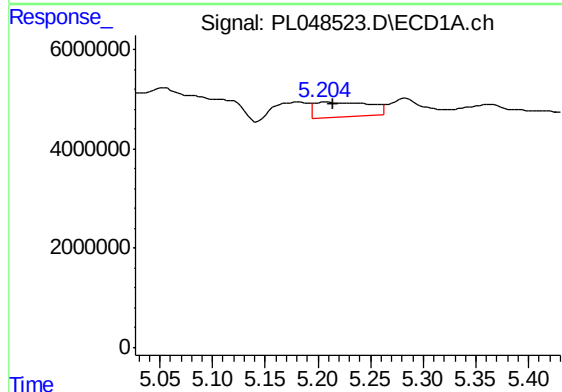


#10 gamma-Chlordane

R.T.: 5.206 min
Delta R.T.: -0.009 min
Response: 10577493
Conc: 0.79 ng/ml

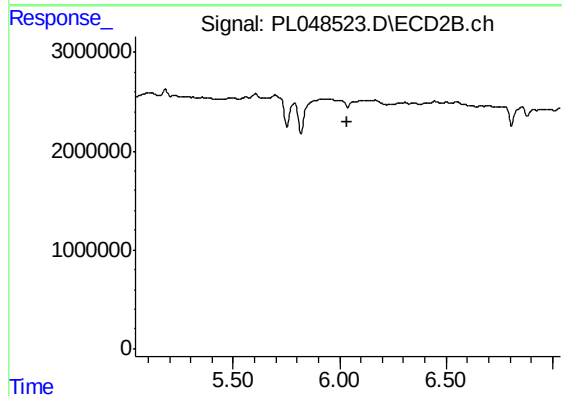

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

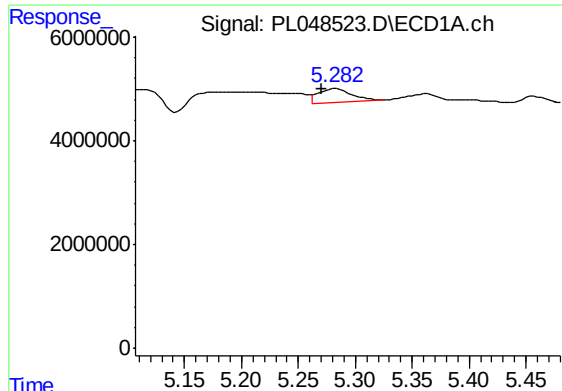

#11 alpha-Chlordane


R.T.: 5.283 min
Delta R.T.: 0.013 min
Response: 5655448
Conc: 0.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
FEBH-03

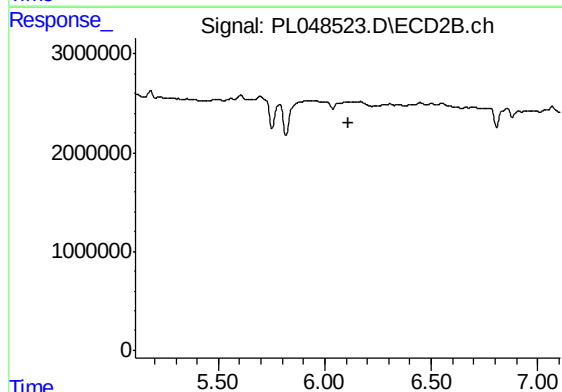


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.109 min
Response: 0
Conc: N.D.

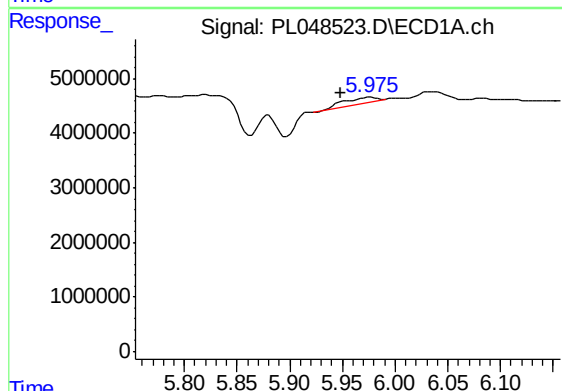


#16 4,4'-DDD

R.T.: 5.977 min
Delta R.T.: 0.028 min
Response: 2012243
Conc: 0.21 ng/ml

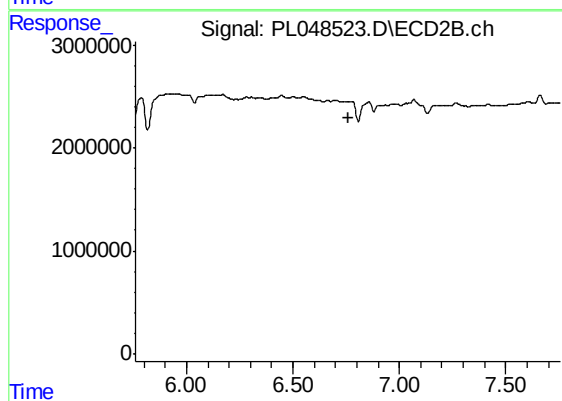

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.759 min
Response: 0
Conc: N.D.

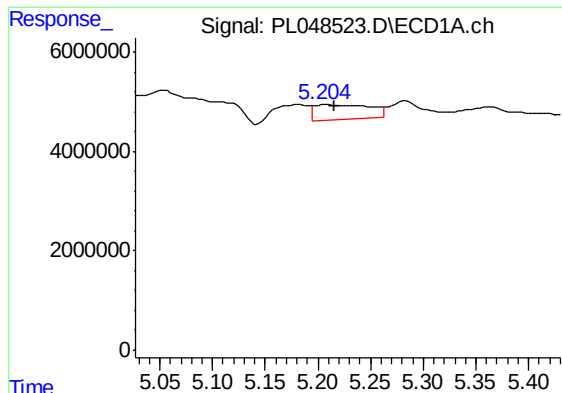

#25 Chlordane-3


R.T.: 5.206 min
Delta R.T.: -0.010 min
Response: 10577493
Conc: 6.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
FEBH-03

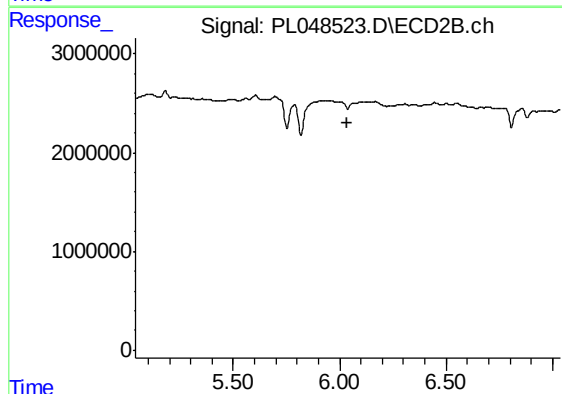


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

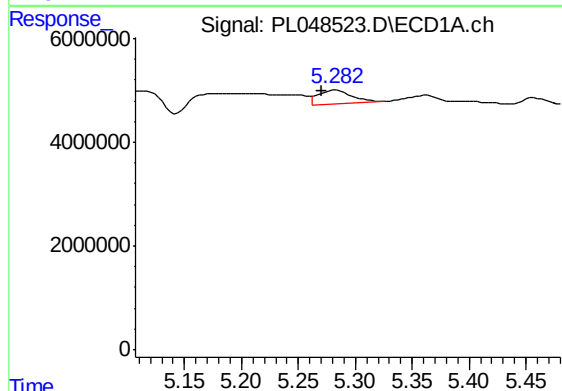


#26 Chlordane-4

R.T.: 5.283 min
Delta R.T.: 0.013 min
Response: 5655448
Conc: 3.90 ng/ml

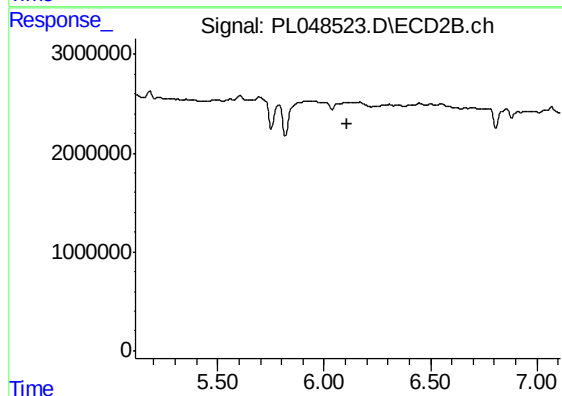

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.111 min
Response: 0
Conc: N.D.

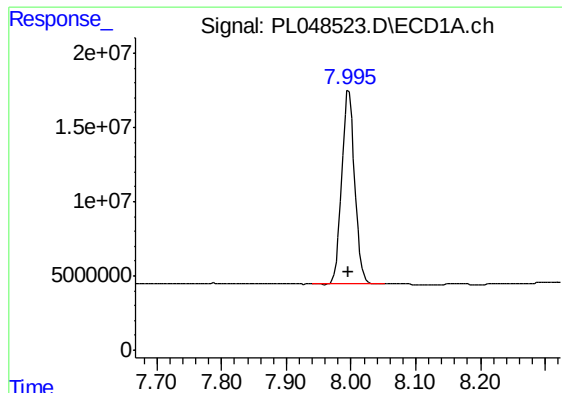

#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 180434512
Conc: 17.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
FEBH-03

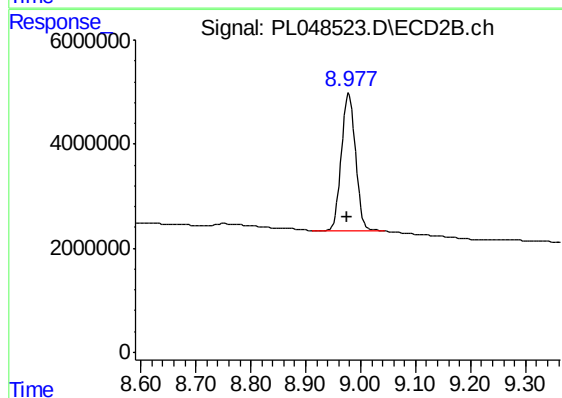

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: 0.004 min
Response: 47315434
Conc: 17.83 ng/ml