

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051420\
 Data File : PL058699.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2020 08:32
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 23:48:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Thu May 14 06:40:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.532	4.077	34955719	48791221	21.278	22.541
28)	SA Decachlor...	8.319	9.190	29977045	42744618	22.957	24.187
Target Compounds							
7)	B delta-BHC	0.000	5.120f	0	1139660	N.D.	0.402 #
8)	B Heptachlo...	0.000	5.958	0	4975696	N.D.	2.072 #
9)	A Endosulfan I	0.000	6.308f	0	744681	N.D.	0.346 #
11)	B alpha-Chl...	0.000	6.278	0	861085	N.D.	0.367 #
15)	B Endosulfa...	0.000	7.014	0	1232005	N.D.	0.617 #
18)	B Endrin al...	0.000	7.147	0	2428227	N.D.	1.423 #
20)	A Methoxychlor	0.000	7.697f	0	1246262	N.D.	1.269 #
23)	Chlordane-1	0.000	5.061f	0	974491	N.D.	12.177 #
26)	Chlordane-4	0.000	6.278	0	861085	N.D.	2.363 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051420\
Data File : PL058699.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2020 08:32
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 23:48:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Thu May 14 06:40:09 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

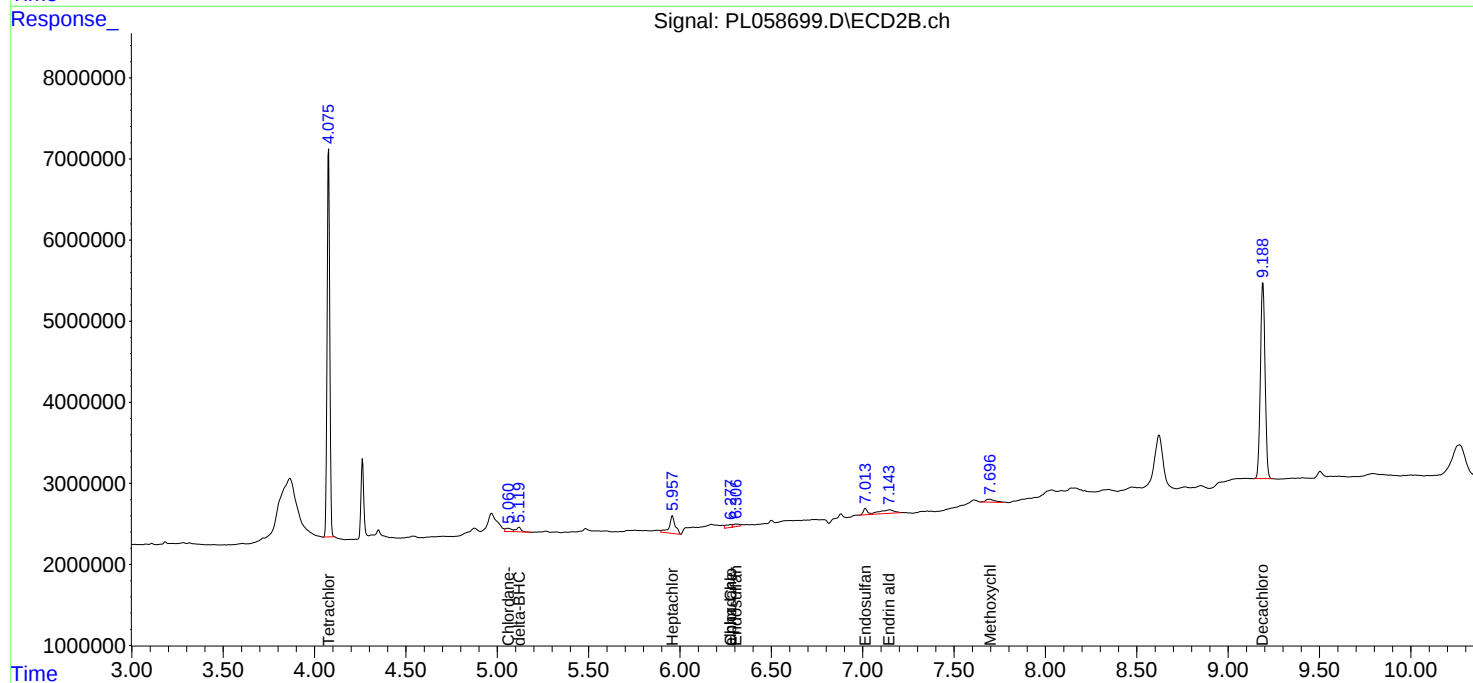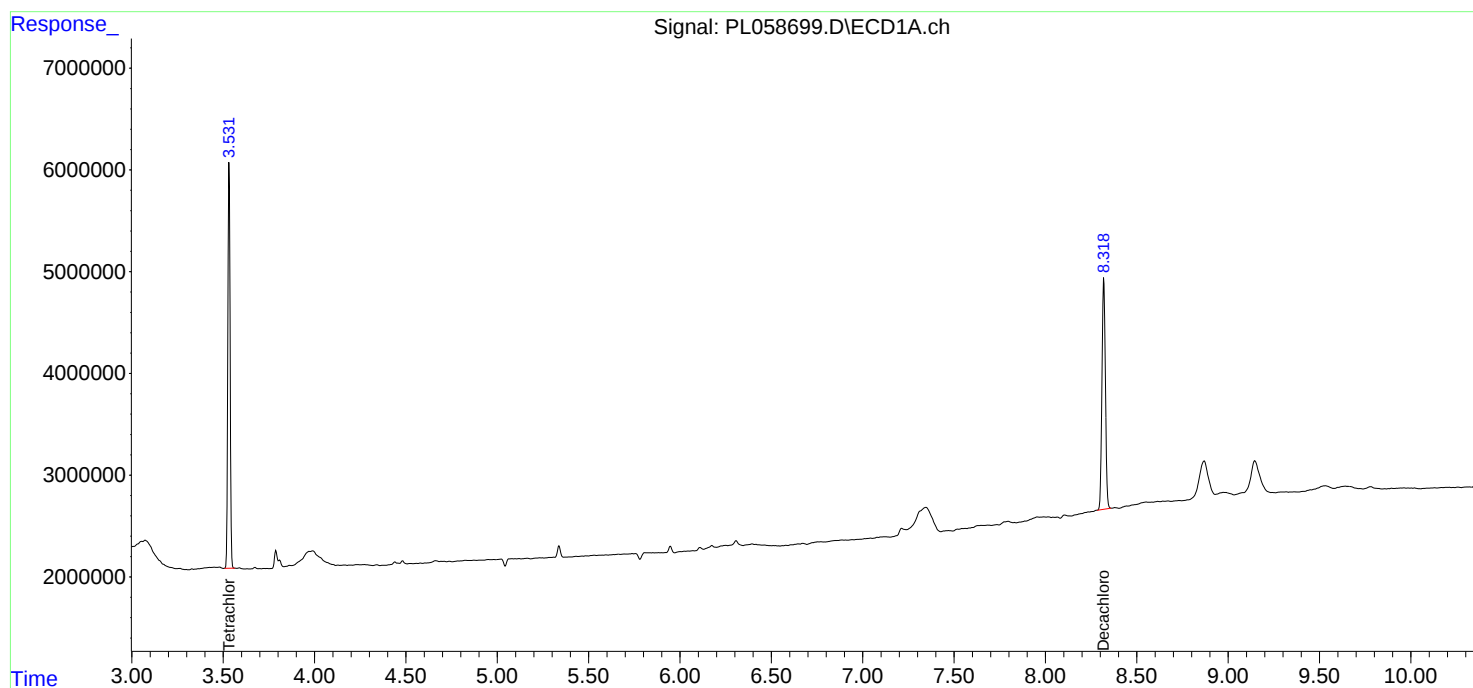


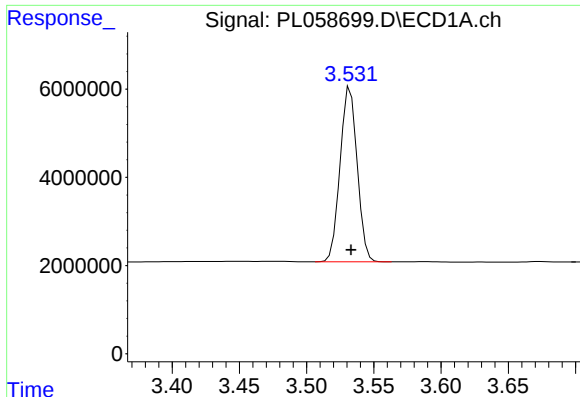

#1 Tetrachloro-m-xylene


R.T.: 3.532 min
Delta R.T.: 0.000 min
Response: 34955719
Conc: 21.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

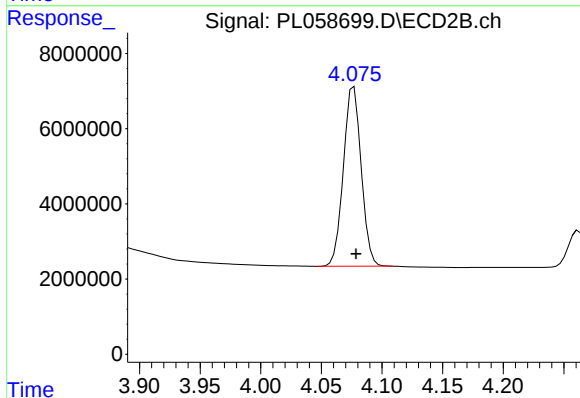


#1 Tetrachloro-m-xylene

R.T.: 4.077 min
Delta R.T.: -0.002 min
Response: 48791221
Conc: 22.54 ng/ml

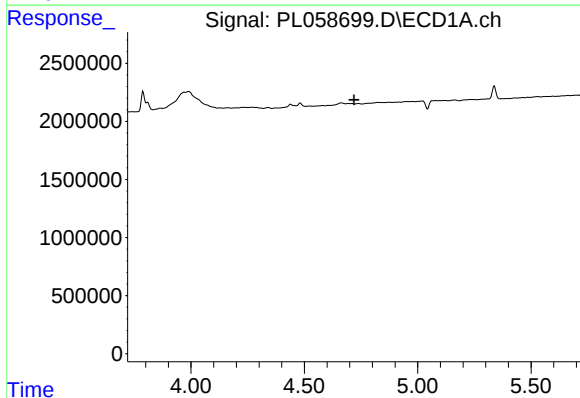


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.719 min
Response: 0
Conc: N.D.

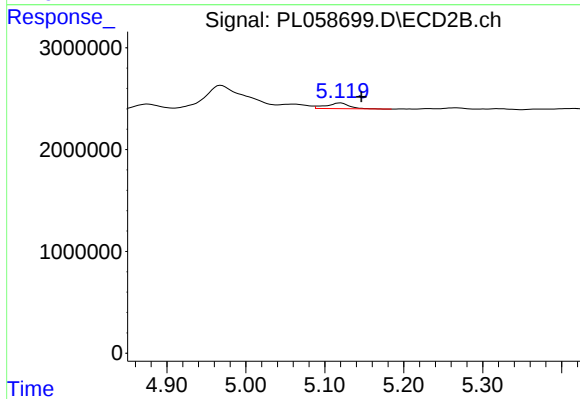

#7 delta-BHC


R.T.: 5.120 min
Delta R.T.: -0.026 min
Response: 1139660
Conc: 0.40 ng/ml

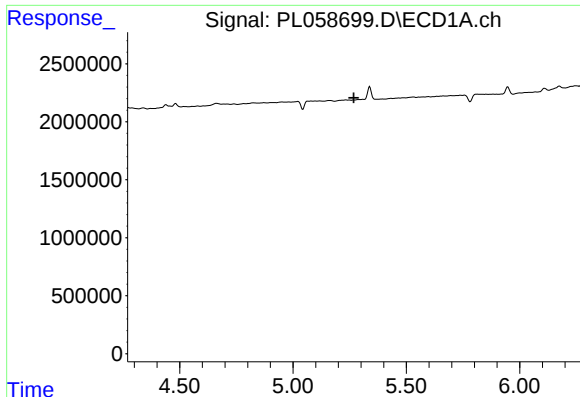

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

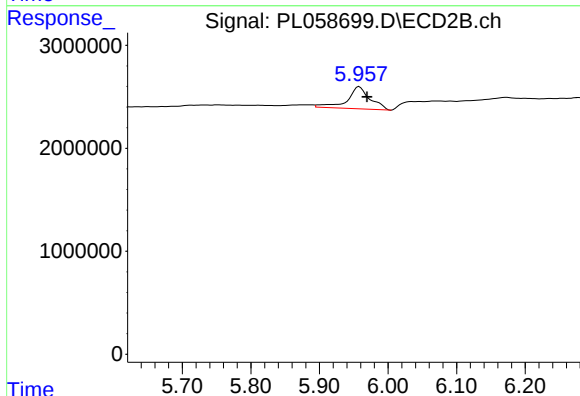


#8 Heptachlor epoxide

R.T.: 5.958 min
Delta R.T.: -0.011 min
Response: 4975696
Conc: 2.07 ng/ml

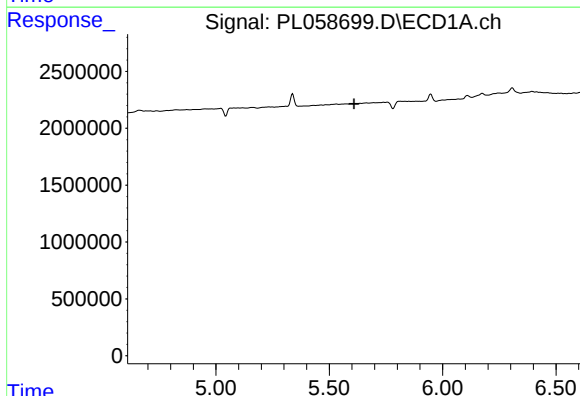


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.609 min
Response: 0
Conc: N.D.

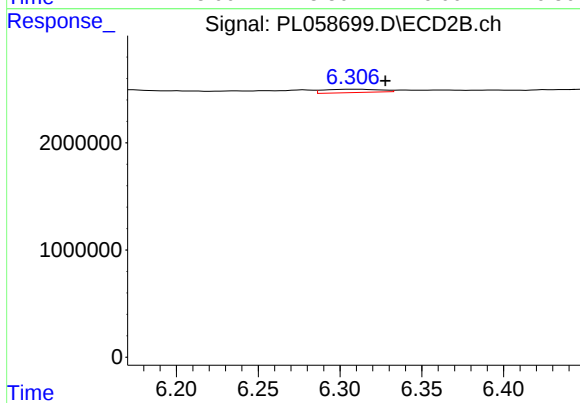

#9 Endosulfan I


R.T.: 6.308 min
Delta R.T.: -0.020 min
Response: 744681
Conc: 0.35 ng/ml

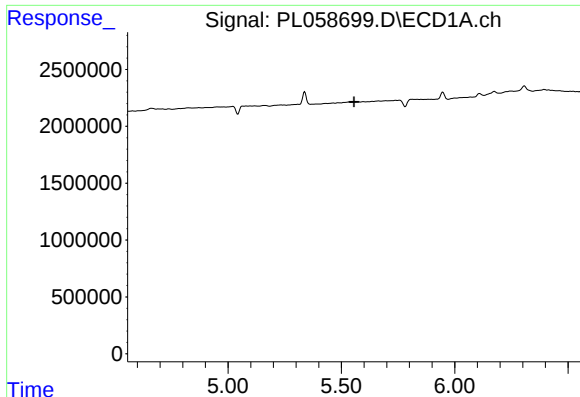

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.556 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

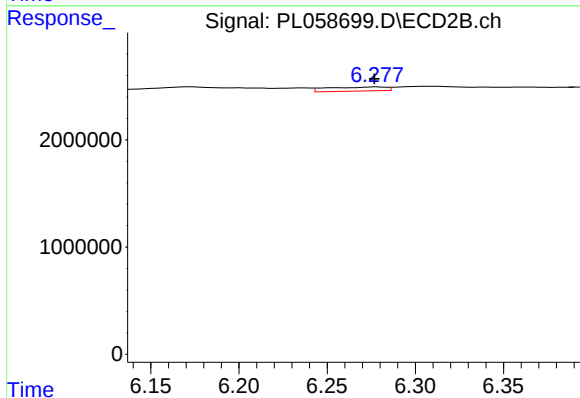


#11 alpha-Chlordane

R.T.: 6.278 min
Delta R.T.: 0.001 min
Response: 861085
Conc: 0.37 ng/ml

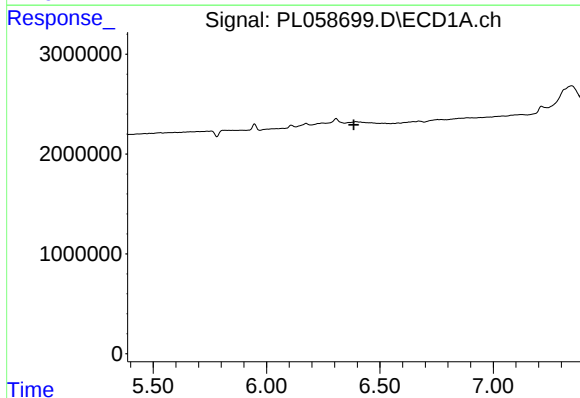


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.385 min
Response: 0
Conc: N.D.

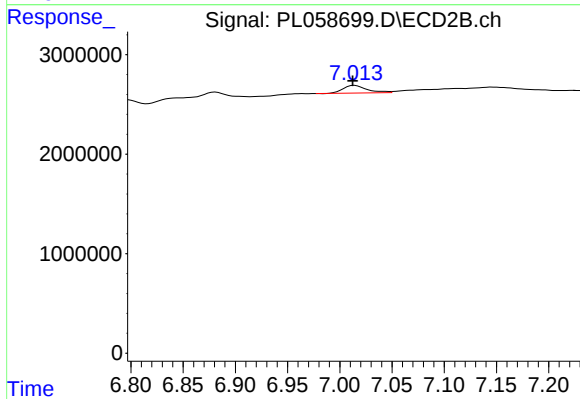

#15 Endosulfan II


R.T.: 7.014 min
Delta R.T.: 0.002 min
Response: 1232005
Conc: 0.62 ng/ml

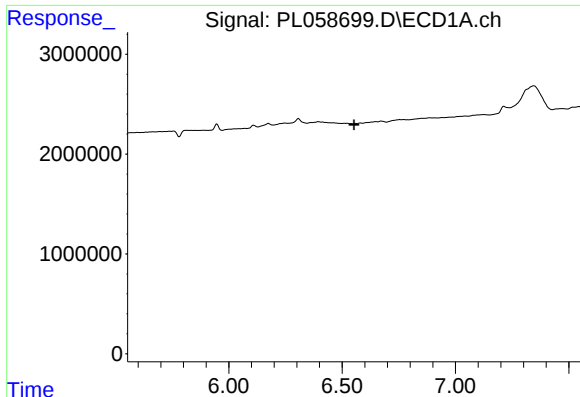

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.553 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

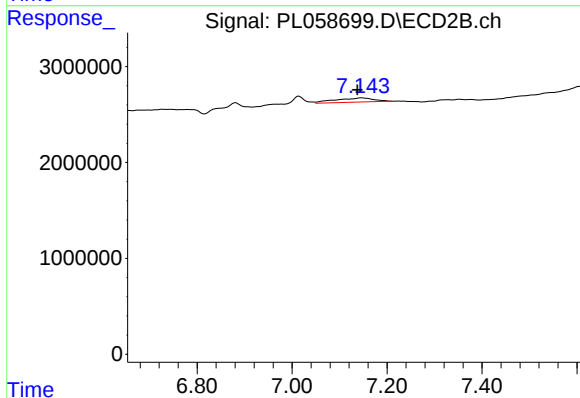


#18 Endrin aldehyde

R.T.: 7.147 min
Delta R.T.: 0.010 min
Response: 2428227
Conc: 1.42 ng/ml

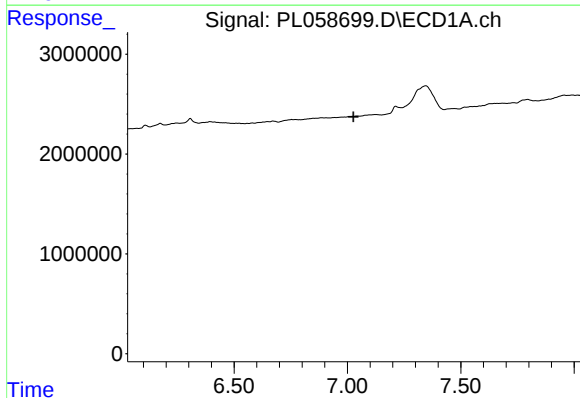


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.027 min
Response: 0
Conc: N.D.

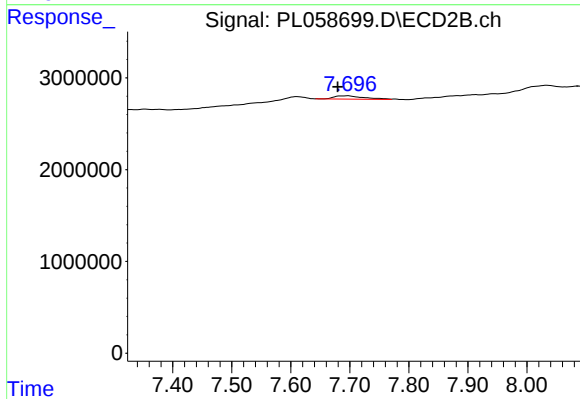

#20 Methoxychlor


R.T.: 7.697 min
Delta R.T.: 0.018 min
Response: 1246262
Conc: 1.27 ng/ml

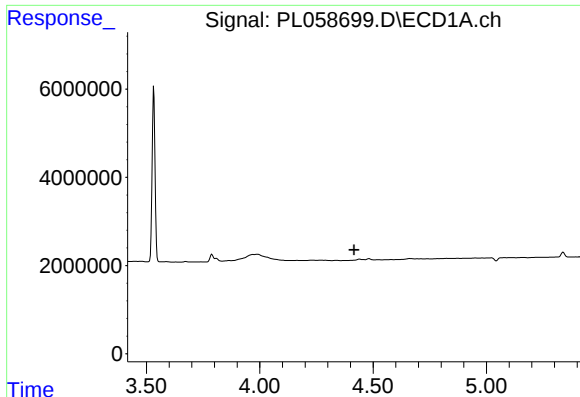

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

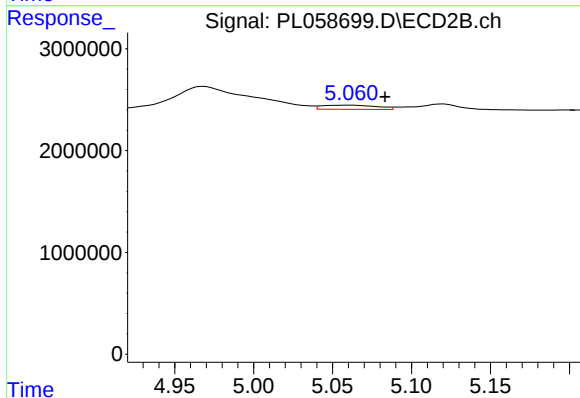


#23 Chlordane-1

R.T.: 5.061 min
Delta R.T.: -0.022 min
Response: 974491
Conc: 12.18 ng/ml

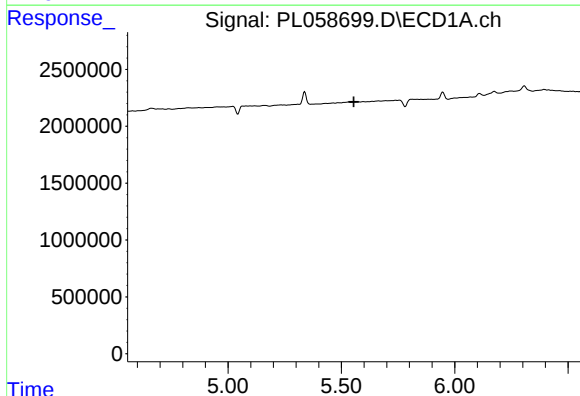


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.555 min
Response: 0
Conc: N.D.

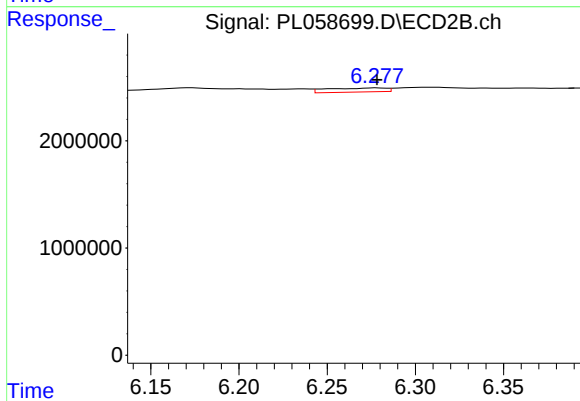

#26 Chlordane-4


R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 861085
Conc: 2.36 ng/ml

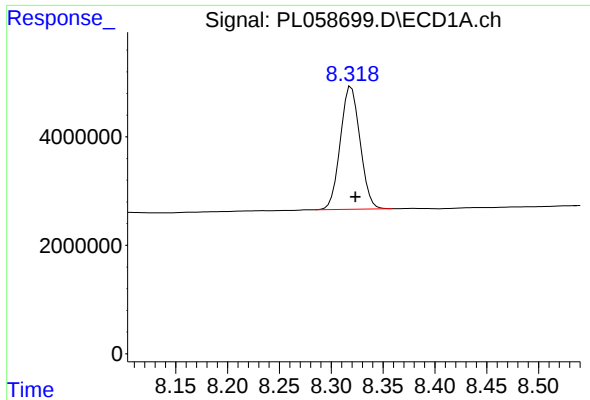

#28 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: -0.004 min
Response: 29977045
Conc: 22.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

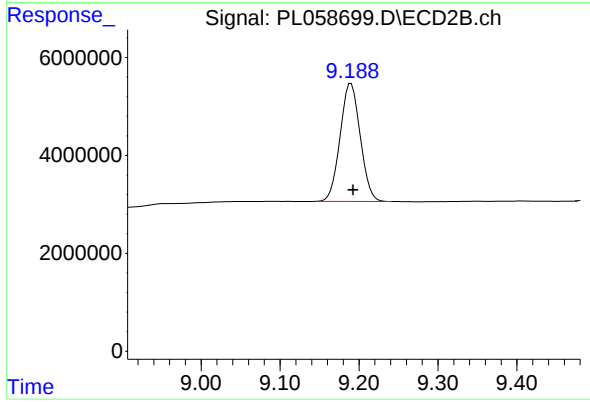

#28 Decachlorobiphenyl

R.T.: 9.190 min
Delta R.T.: -0.002 min
Response: 42744618
Conc: 24.19 ng/ml