

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051420\
 Data File : PL058712.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2020 12:46
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 23:52:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Thu May 14 06:40:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.531	4.077	35691801	50250142	21.726	23.215
28)	SA Decachlor...	8.318	9.190	31742856	45081712	24.310	25.509
Target Compounds							
7)	B delta-BHC	0.000	5.120f	0	1228864	N.D.	0.433 #
8)	B Heptachlo...	0.000	5.958	0	5120716	N.D.	2.132 #
9)	A Endosulfan I	0.000	6.306f	0	852588	N.D.	0.396 #
10)	B gamma-Chl...	0.000	6.175f	0	2165988	N.D.	0.922 #
11)	B alpha-Chl...	0.000	6.306f	0	852588	N.D.	0.364 #
13)	MA Dieldrin	5.857	0.000	1106913	0	0.743	N.D. #
15)	B Endosulfa...	0.000	7.013	0	1262202	N.D.	0.632 #
25)	Chlordane-3	0.000	6.175f	0	2165988	N.D.	7.151 #
26)	Chlordane-4	0.000	6.306f	0	852588	N.D.	2.339 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051420\
Data File : PL058712.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2020 12:46
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 23:52:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Thu May 14 06:40:09 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

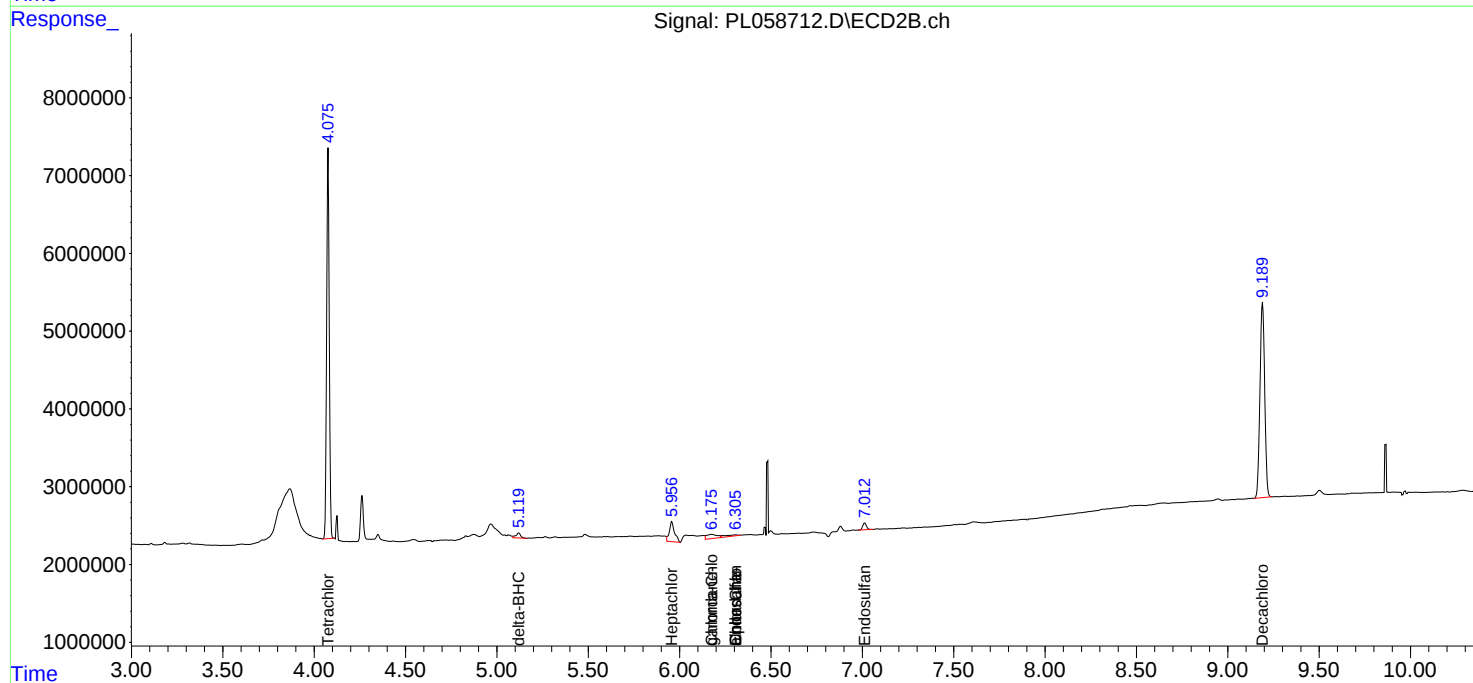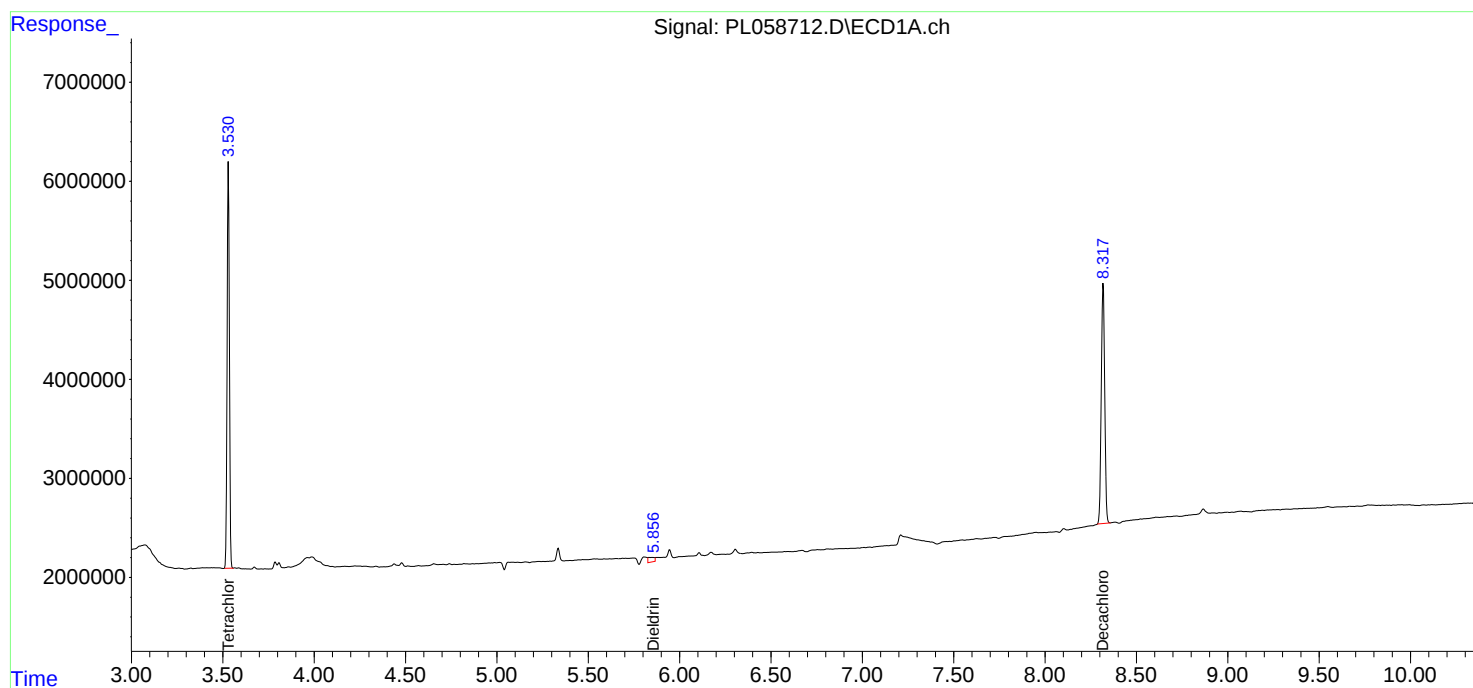


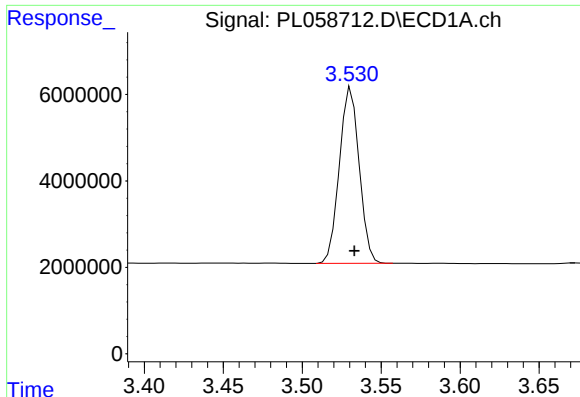

#1 Tetrachloro-m-xylene


R.T.: 3.531 min
Delta R.T.: -0.002 min
Response: 35691801
Conc: 21.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

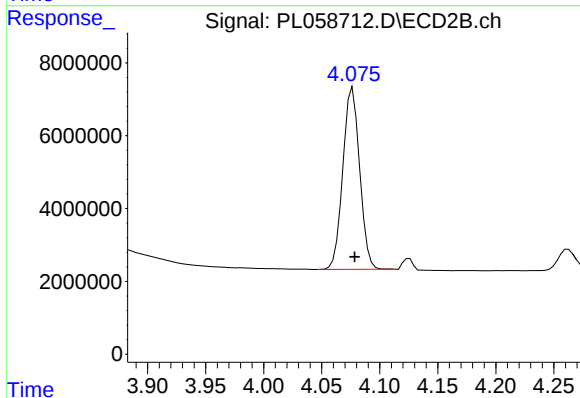


#1 Tetrachloro-m-xylene

R.T.: 4.077 min
Delta R.T.: -0.002 min
Response: 50250142
Conc: 23.21 ng/ml

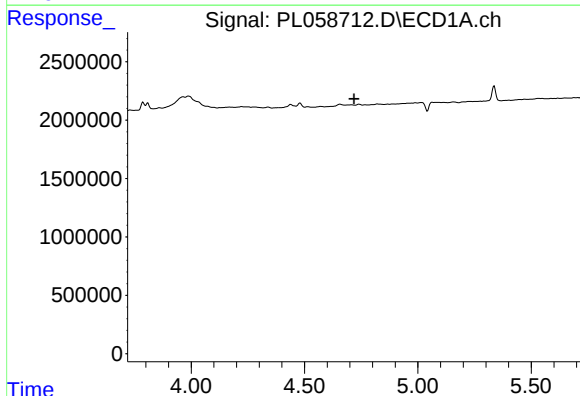


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.719 min
Response: 0
Conc: N.D.

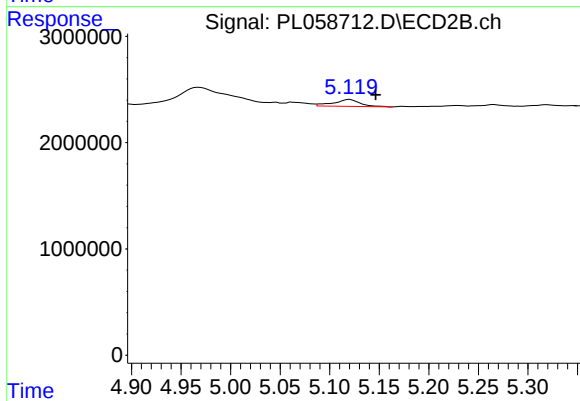

#7 delta-BHC


R.T.: 5.120 min
Delta R.T.: -0.026 min
Response: 1228864
Conc: 0.43 ng/ml

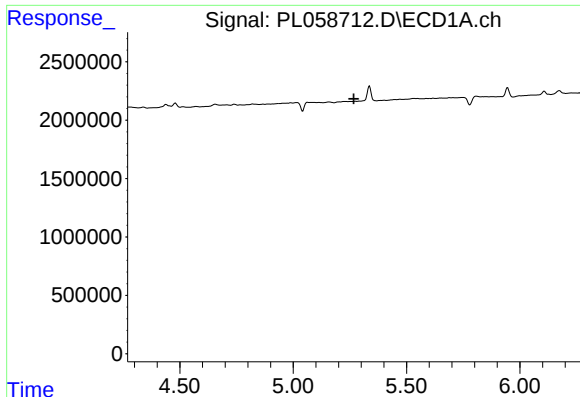

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

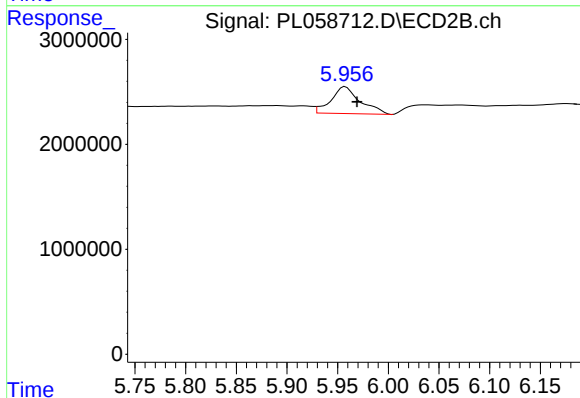


#8 Heptachlor epoxide

R.T.: 5.958 min
Delta R.T.: -0.011 min
Response: 5120716
Conc: 2.13 ng/ml

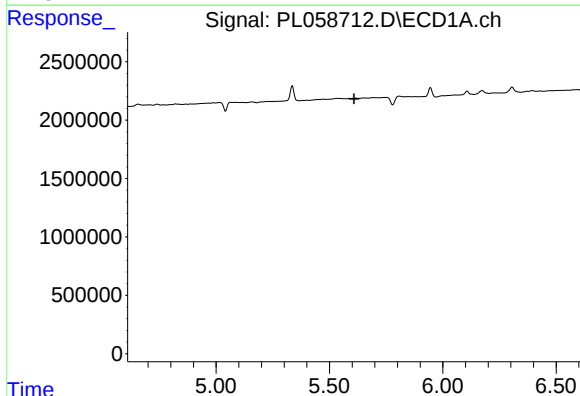


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.609 min
Response: 0
Conc: N.D.

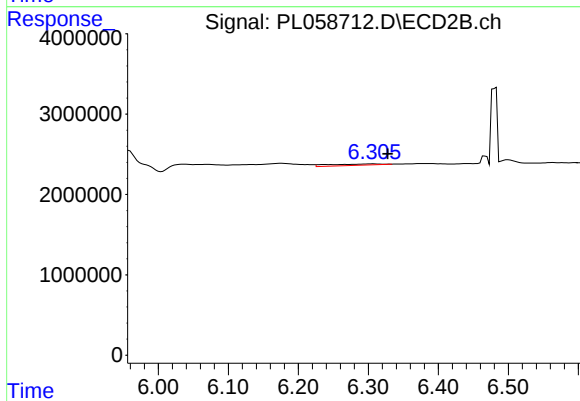

#9 Endosulfan I


R.T.: 6.306 min
Delta R.T.: -0.022 min
Response: 852588
Conc: 0.40 ng/ml

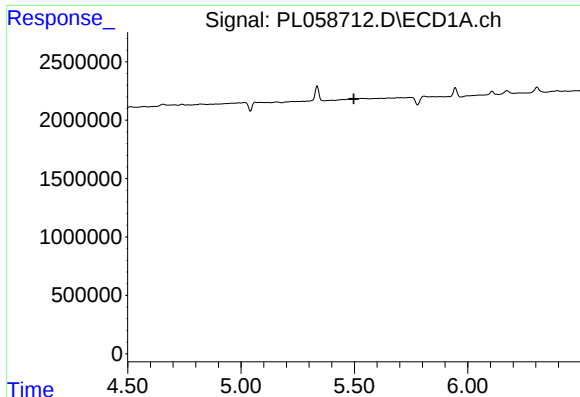

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

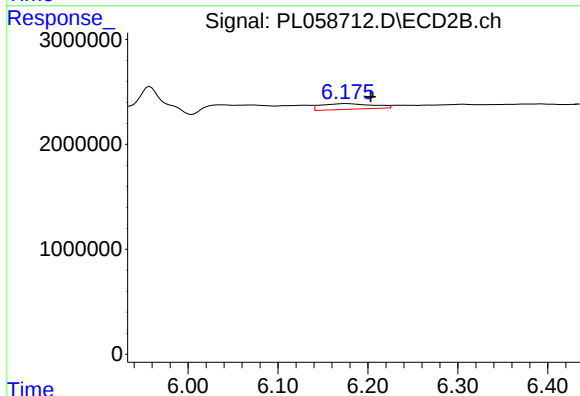


#10 gamma-Chlordane

R.T.: 6.175 min
Delta R.T.: -0.028 min
Response: 2165988
Conc: 0.92 ng/ml

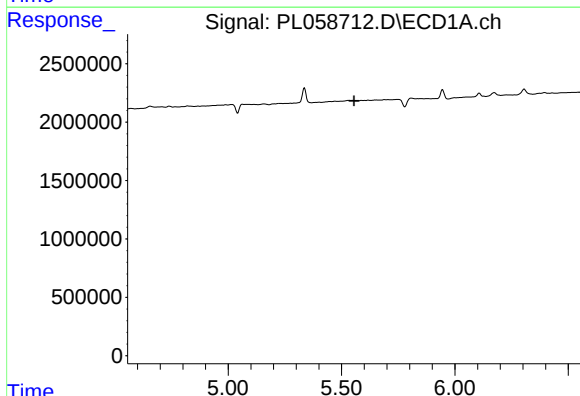


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.556 min
Response: 0
Conc: N.D.

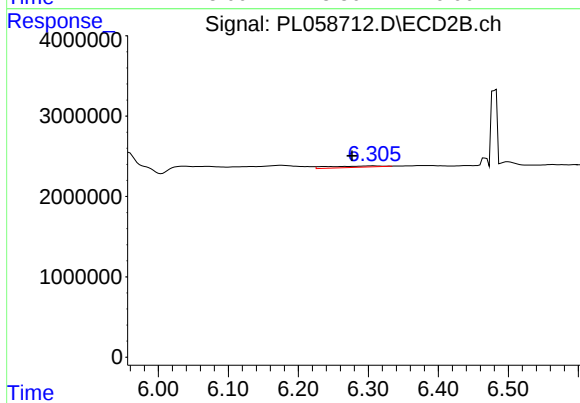

#11 alpha-Chlordane


R.T.: 6.306 min
Delta R.T.: 0.029 min
Response: 852588
Conc: 0.36 ng/ml

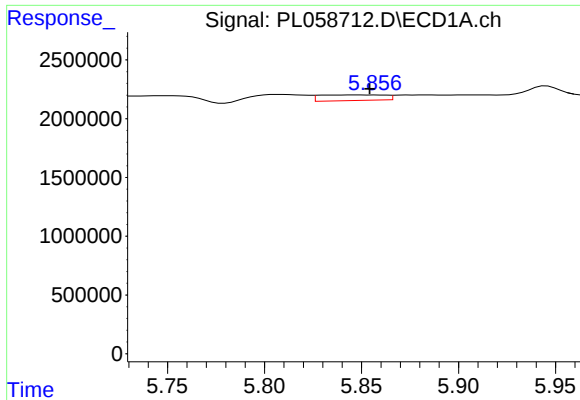

#13 Dieldrin


R.T.: 5.857 min
Delta R.T.: 0.003 min
Response: 1106913
Conc: 0.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

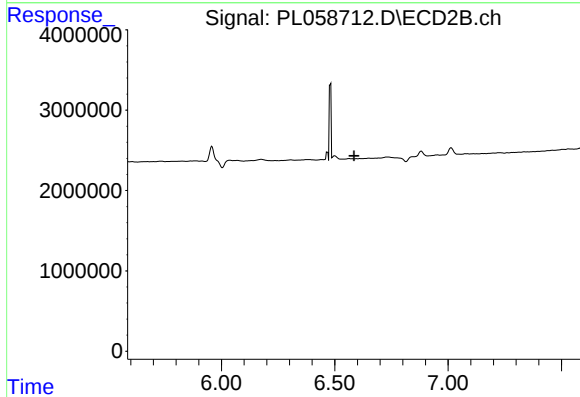


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.586 min
Response: 0
Conc: N.D.

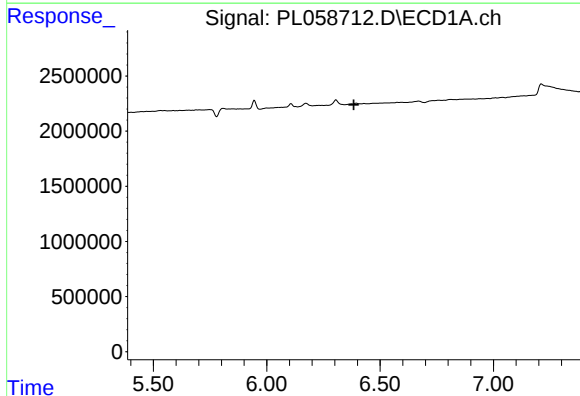


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.385 min
Response: 0
Conc: N.D.

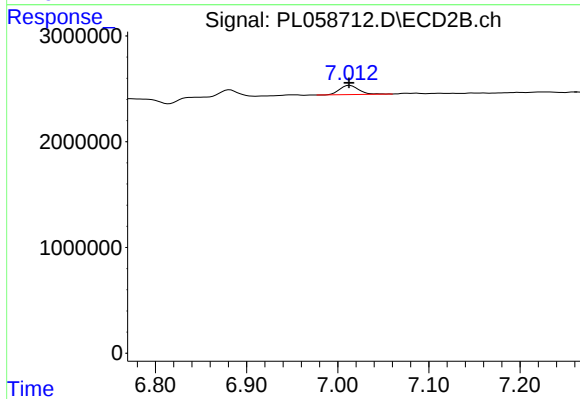

#15 Endosulfan II


R.T.: 7.013 min
Delta R.T.: 0.000 min
Response: 1262202
Conc: 0.63 ng/ml

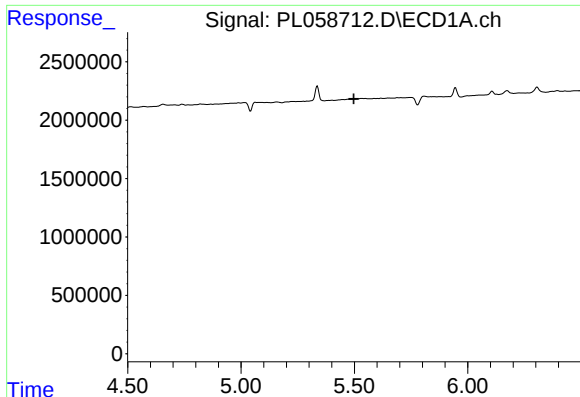

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

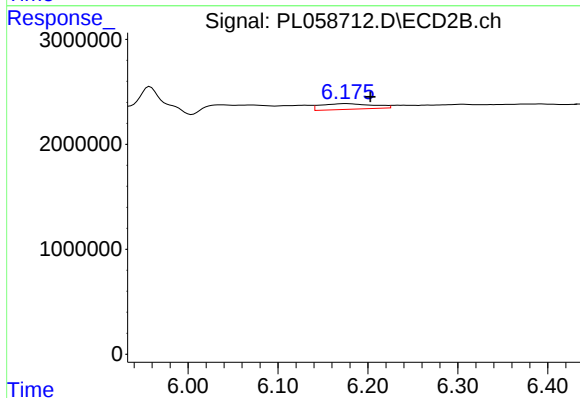


#25 Chlordane-3

R.T.: 6.175 min
Delta R.T.: -0.028 min
Response: 2165988
Conc: 7.15 ng/ml

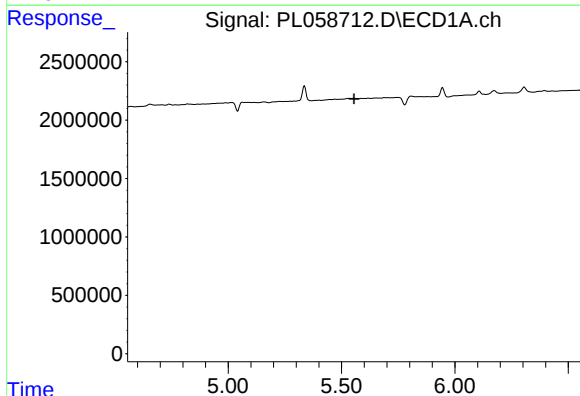


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.555 min
Response: 0
Conc: N.D.

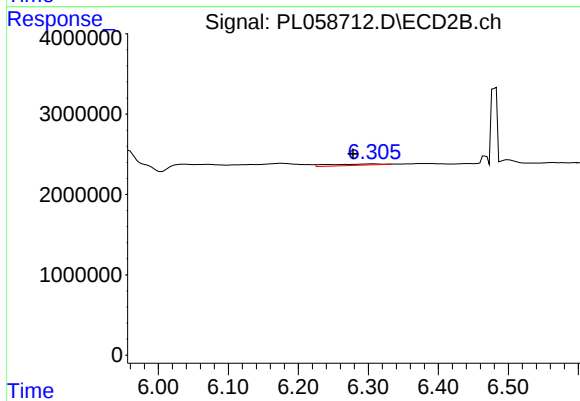

#26 Chlordane-4


R.T.: 6.306 min
Delta R.T.: 0.028 min
Response: 852588
Conc: 2.34 ng/ml

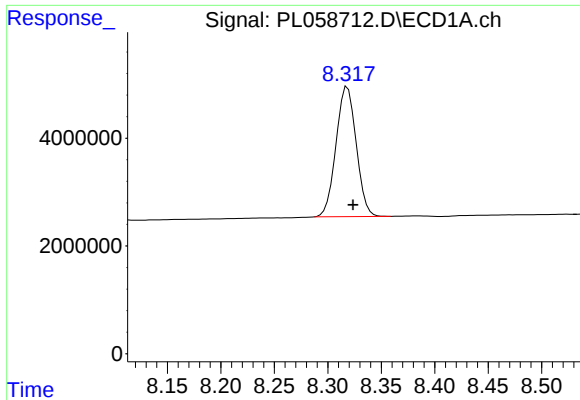

#28 Decachlorobiphenyl

R.T.: 8.318 min
Delta R.T.: -0.005 min
Response: 31742856
Conc: 24.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

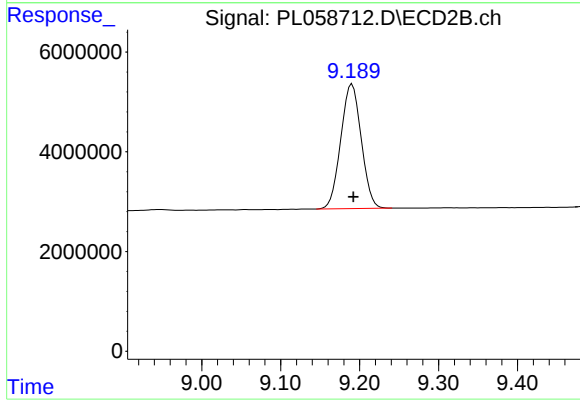

#28 Decachlorobiphenyl

R.T.: 9.190 min
Delta R.T.: -0.002 min
Response: 45081712
Conc: 25.51 ng/ml