

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051420\
 Data File : PL058717.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2020 13:58
 Operator : AJ\MA
 Sample : PB128877BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 23:53:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Thu May 14 06:40:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.534	4.078	33525418	47852738	20.407	22.107
28)	SA Decachlor...	8.321	9.192	31596190	44677610	24.197	25.280
Target Compounds							
7)	B delta-BHC	0.000	5.121f	0	1318255	N.D.	0.465 #
9)	A Endosulfan I	0.000	6.304f	0	294844	N.D.	0.137 #
10)	B gamma-Chl...	0.000	6.174f	0	1036706	N.D.	0.441 #
11)	B alpha-Chl...	0.000	6.276	0	98312	N.D.	0.042 #
14)	MA Endrin	0.000	6.822f	0	392116	N.D.	0.216 #
15)	B Endosulfa...	0.000	7.013	0	1754937	N.D.	0.879 #
16)	A 4,4'-DDD	0.000	6.950f	0	331282	N.D.	0.189 #
25)	Chlordane-3	0.000	6.174f	0	1036706	N.D.	3.423 #
26)	Chlordane-4	0.000	6.276	0	98312	N.D.	0.270 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051420\
Data File : PL058717.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2020 13:58
Operator : AJ\MA
Sample : PB128877BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 23:53:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Thu May 14 06:40:09 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

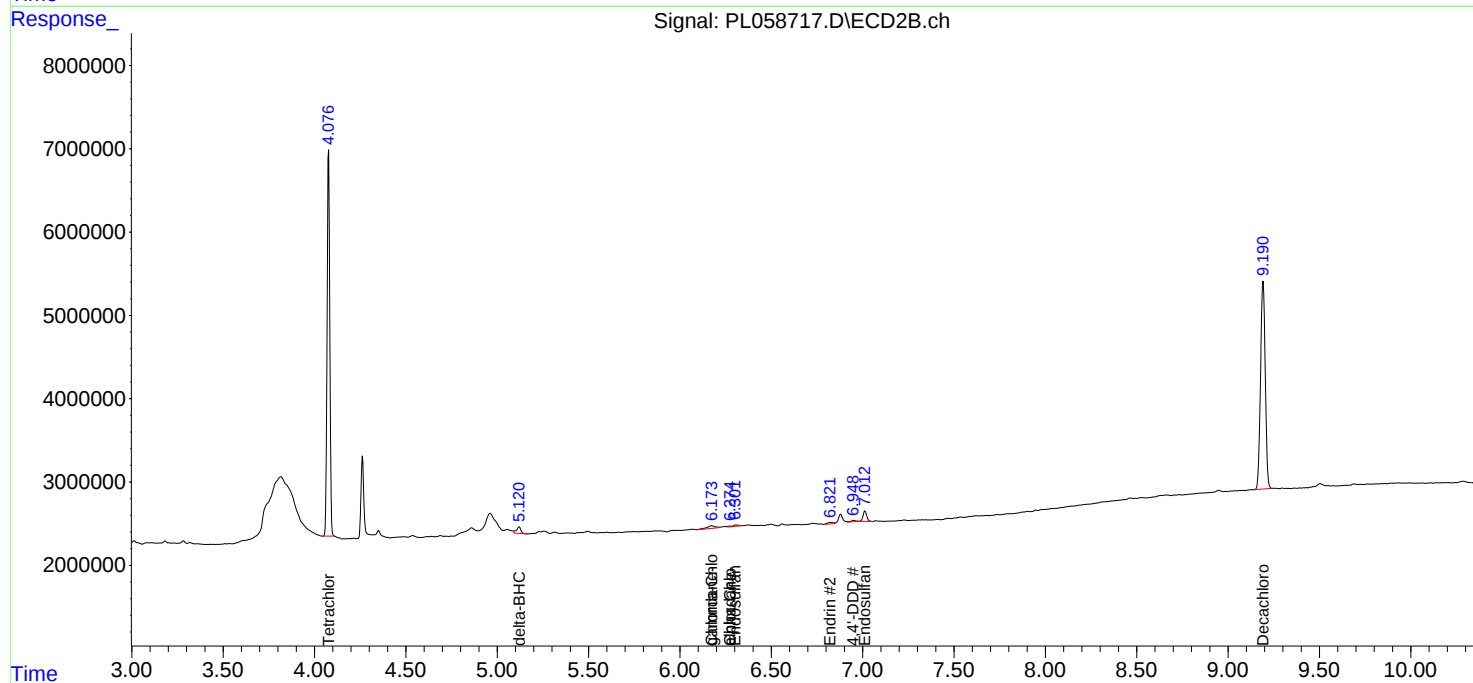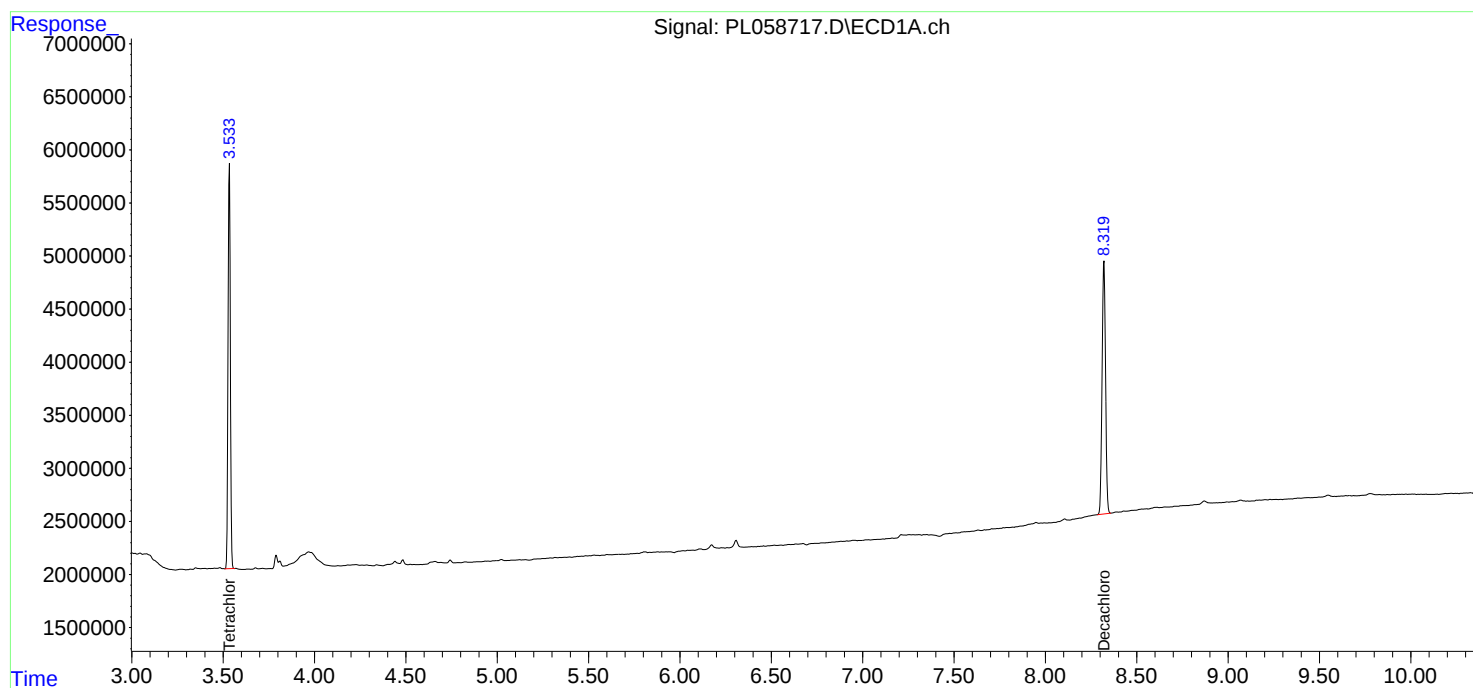


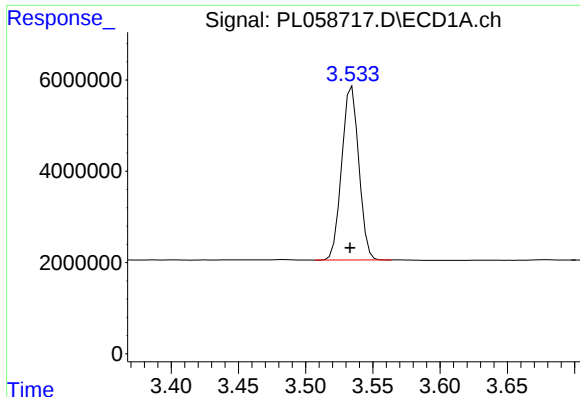

#1 Tetrachloro-m-xylene


R.T.: 3.534 min
Delta R.T.: 0.001 min
Response: 33525418
Conc: 20.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

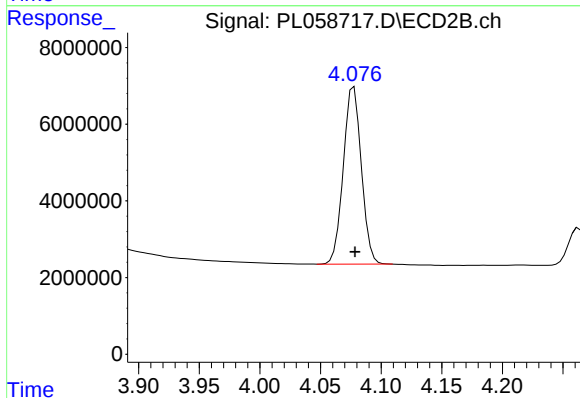


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: -0.001 min
Response: 47852738
Conc: 22.11 ng/ml

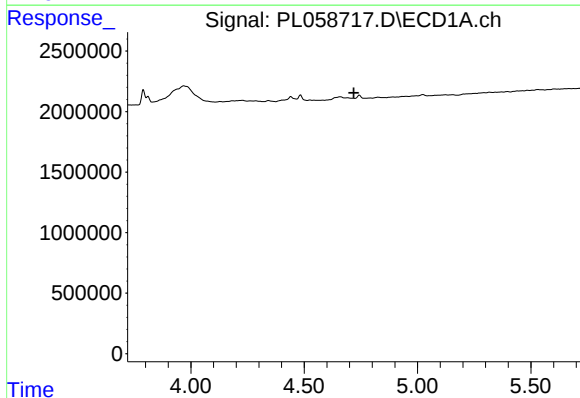


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.719 min
Response: 0
Conc: N.D.

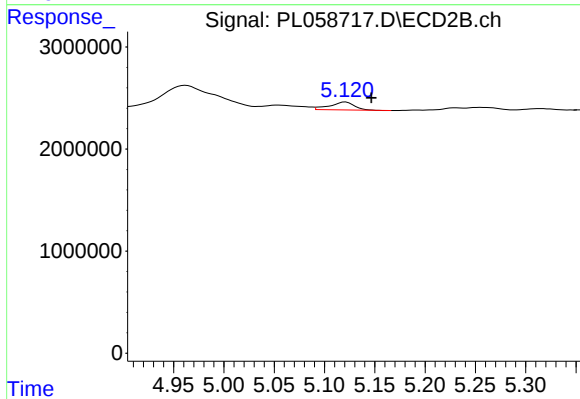

#7 delta-BHC


R.T.: 5.121 min
Delta R.T.: -0.025 min
Response: 1318255
Conc: 0.46 ng/ml

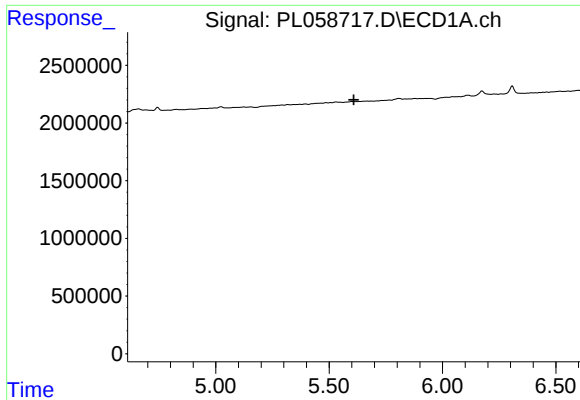

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.609 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

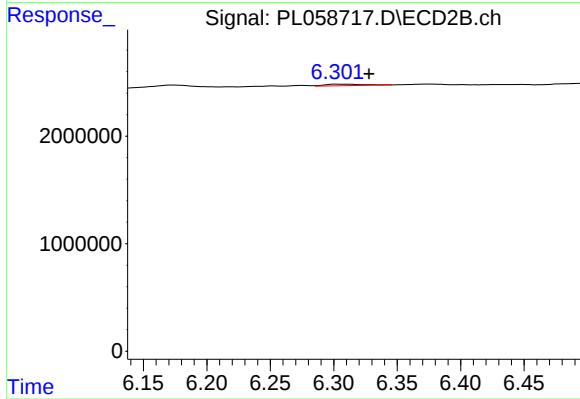


#9 Endosulfan I

R.T.: 6.304 min
Delta R.T.: -0.024 min
Response: 294844
Conc: 0.14 ng/ml

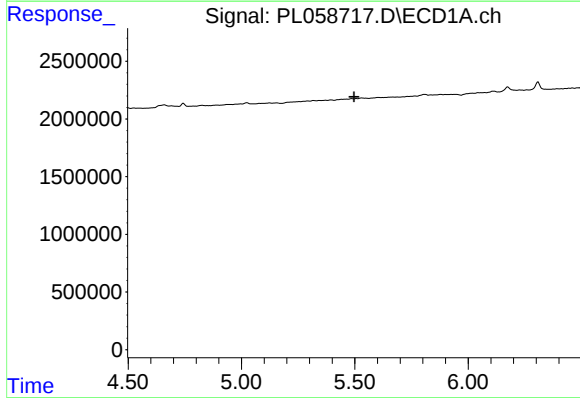


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

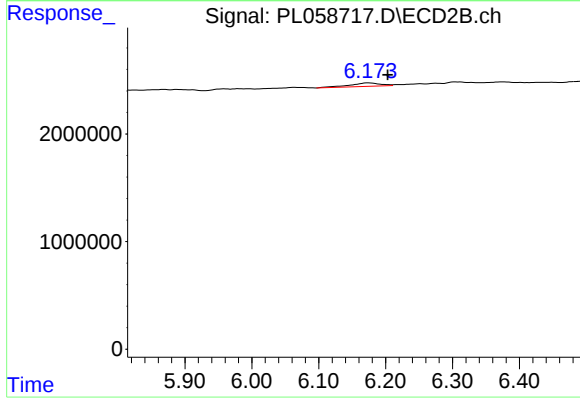

#10 gamma-Chlordane

R.T.: 6.174 min
Delta R.T.: -0.029 min
Response: 1036706
Conc: 0.44 ng/ml

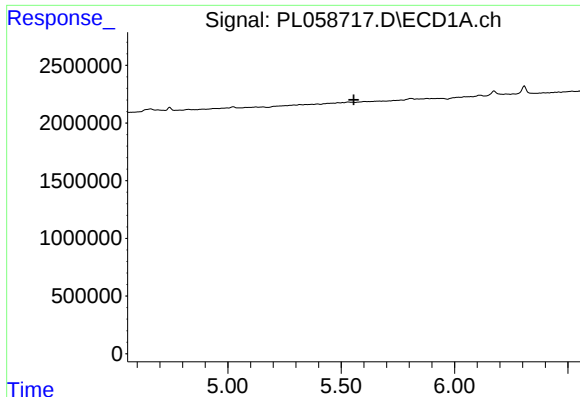

#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.556 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#11 alpha-Chlordane


R.T.: 6.276 min
Delta R.T.: -0.001 min
Response: 98312
Conc: 0.04 ng/ml

#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

#14 Endrin


R.T.: 6.822 min
Delta R.T.: 0.017 min
Response: 392116
Conc: 0.22 ng/ml

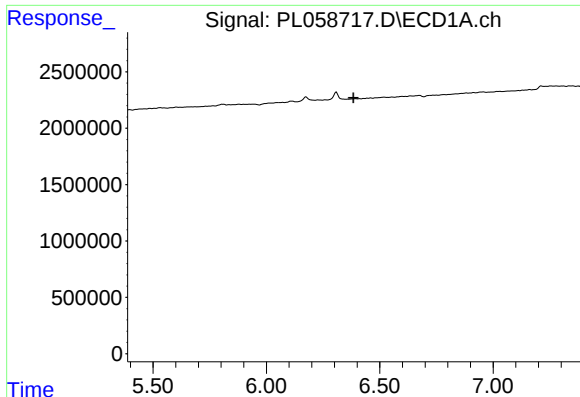

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.385 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

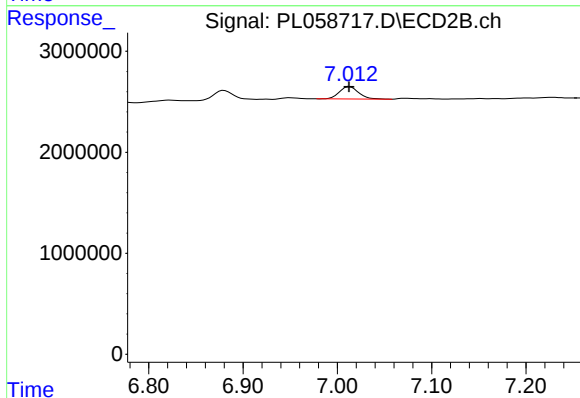


#15 Endosulfan II

R.T.: 7.013 min
Delta R.T.: 0.000 min
Response: 1754937
Conc: 0.88 ng/ml

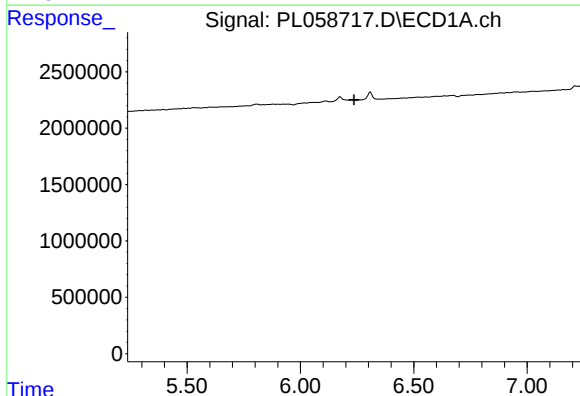


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.237 min
Response: 0
Conc: N.D.

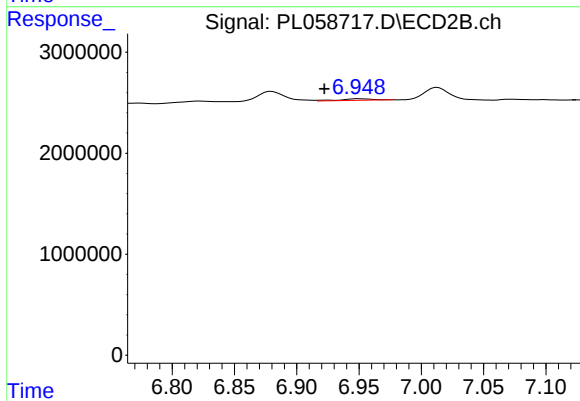

#16 4,4'-DDD


R.T.: 6.950 min
Delta R.T.: 0.028 min
Response: 331282
Conc: 0.19 ng/ml

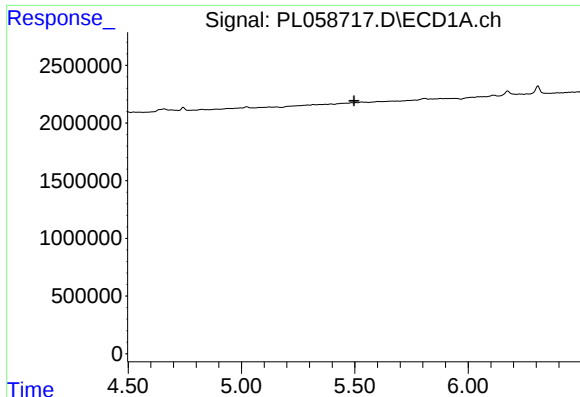

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

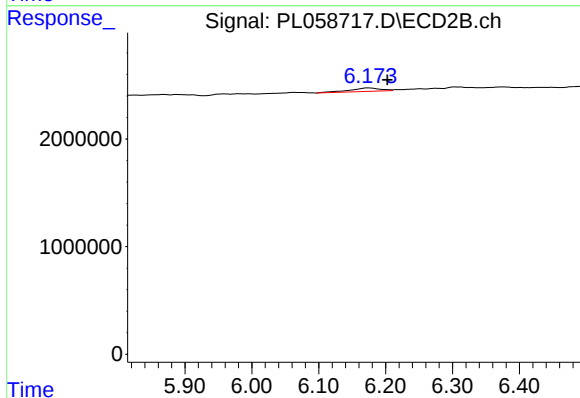


#25 Chlordane-3

R.T.: 6.174 min
Delta R.T.: -0.028 min
Response: 1036706
Conc: 3.42 ng/ml

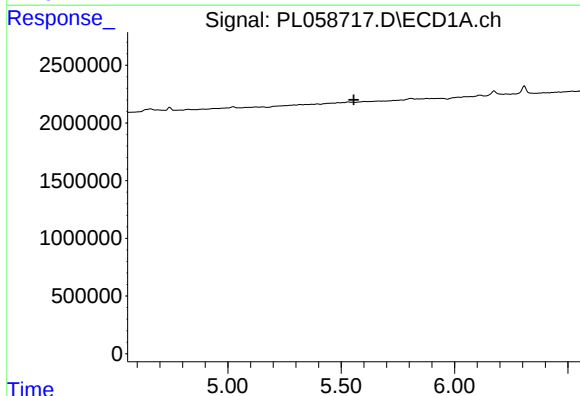


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.555 min
Response: 0
Conc: N.D.

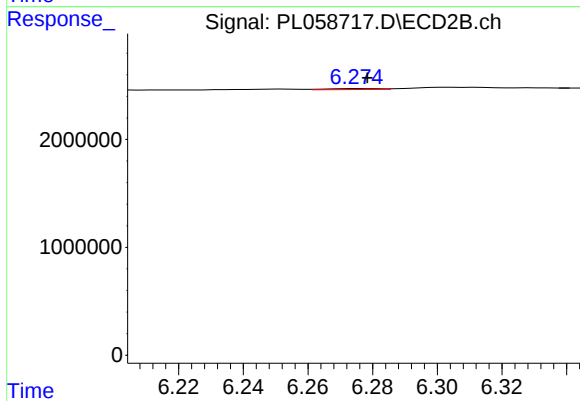

#26 Chlordane-4


R.T.: 6.276 min
Delta R.T.: -0.003 min
Response: 98312
Conc: 0.27 ng/ml

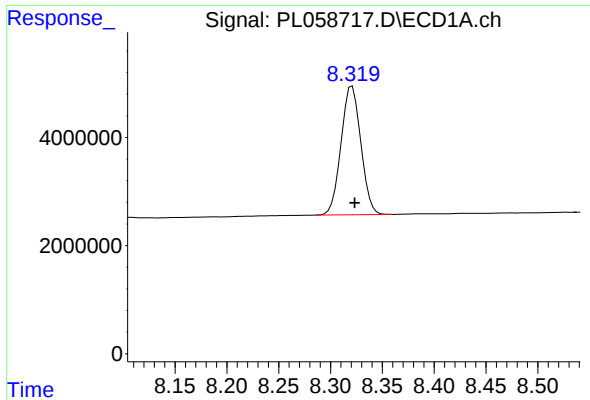

#28 Decachlorobiphenyl

R.T.: 8.321 min
Delta R.T.: -0.003 min
Response: 31596190
Conc: 24.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

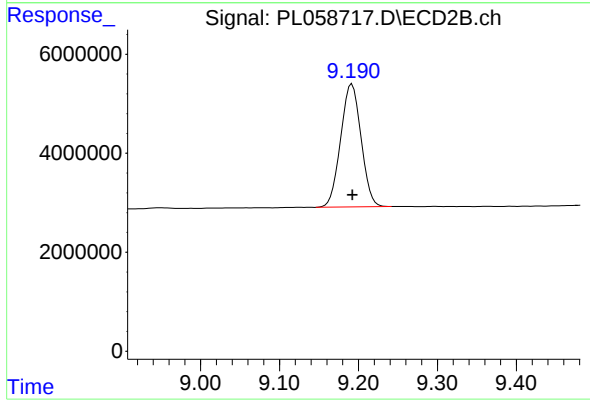

#28 Decachlorobiphenyl

R.T.: 9.192 min
Delta R.T.: 0.000 min
Response: 44677610
Conc: 25.28 ng/ml