

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051420\
 Data File : PL058726.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2020 16:48
 Operator : AJ\MA
 Sample : PB128892TB
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 23:56:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Thu May 14 06:40:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.531	4.077	32373969	46511312	19.706	21.487
28)	SA Decachlor...	8.318	9.191	29195473	42660597	22.359	24.139
Target Compounds							
4)	MA Heptachlor	0.000	5.265	0	729740	N.D.	0.260 #
7)	B delta-BHC	0.000	5.120f	0	1062175	N.D.	0.374 #
10)	B gamma-Chl...	0.000	6.178f	0	487128	N.D.	0.207 #
15)	B Endosulfa...	0.000	7.013	0	1350987	N.D.	0.676 #
16)	A 4,4'-DDD	0.000	6.951f	0	183763	N.D.	0.105 #
22)	Mirex	0.000	8.299	0	512914	N.D.	0.326 #
23)	Chlordane-1	0.000	5.059f	0	924095	N.D.	11.547 #
25)	Chlordane-3	0.000	6.178f	0	487128	N.D.	1.608 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051420\
Data File : PL058726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2020 16:48
Operator : AJ\MA
Sample : PB128892TB
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 23:56:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Thu May 14 06:40:09 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

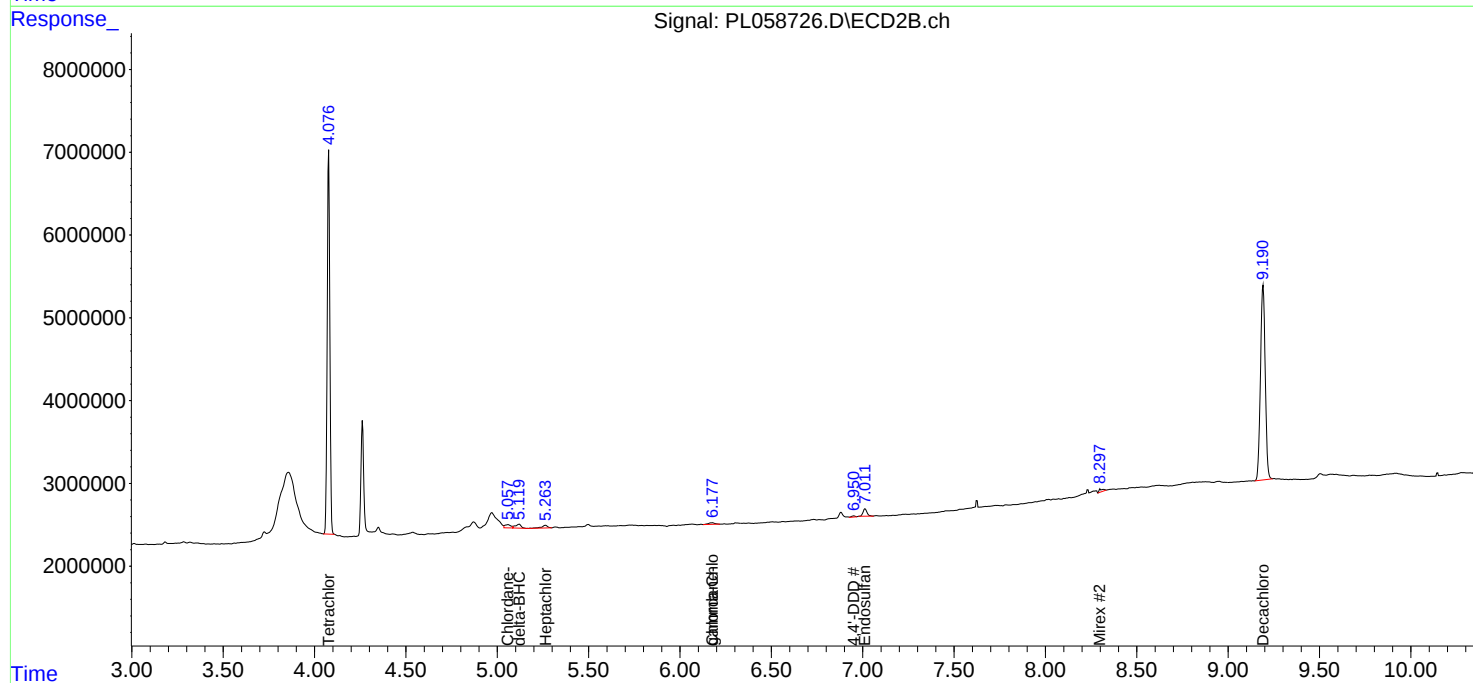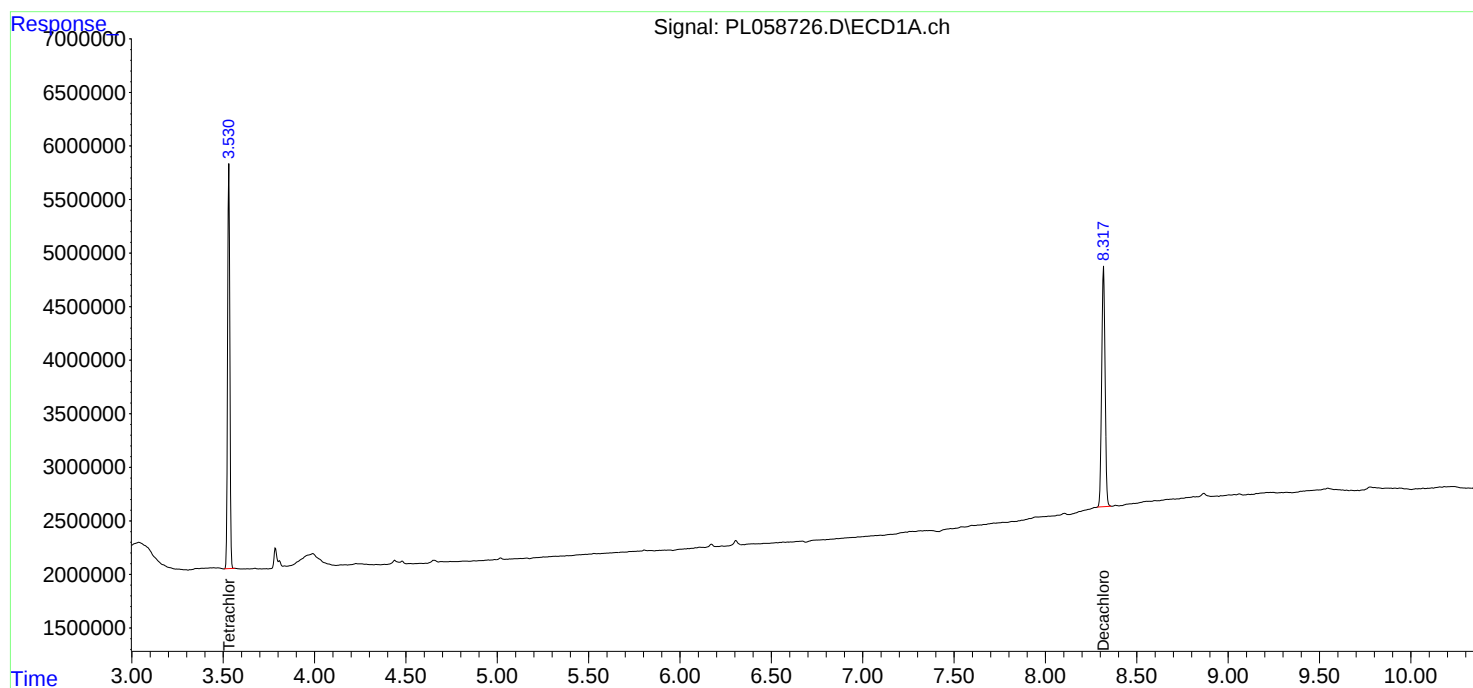


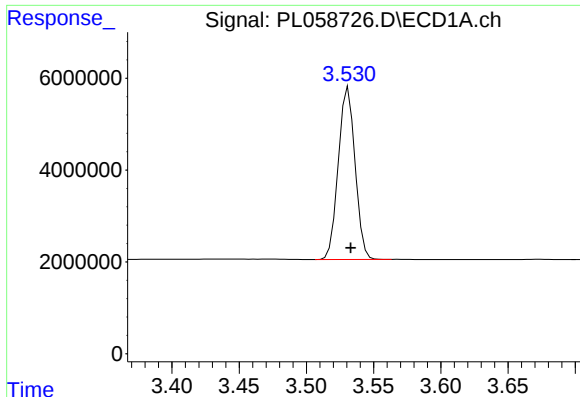

#1 Tetrachloro-m-xylene


R.T.: 3.531 min
Delta R.T.: -0.002 min
Response: 32373969
Conc: 19.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

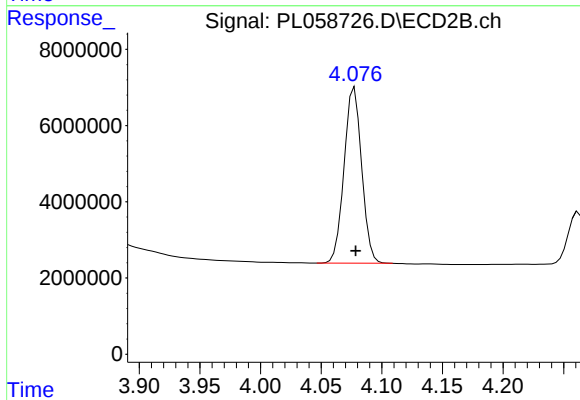


#1 Tetrachloro-m-xylene

R.T.: 4.077 min
Delta R.T.: -0.001 min
Response: 46511312
Conc: 21.49 ng/ml

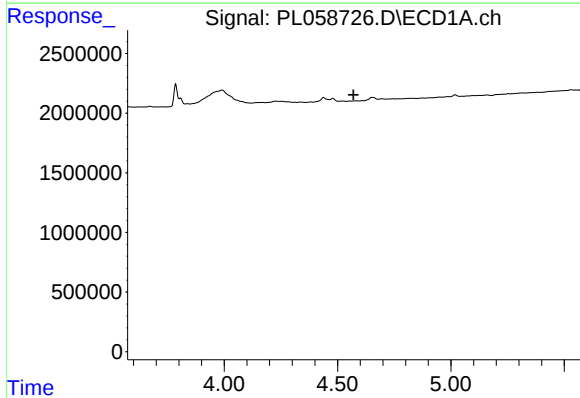


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.571 min
Response: 0
Conc: N.D.

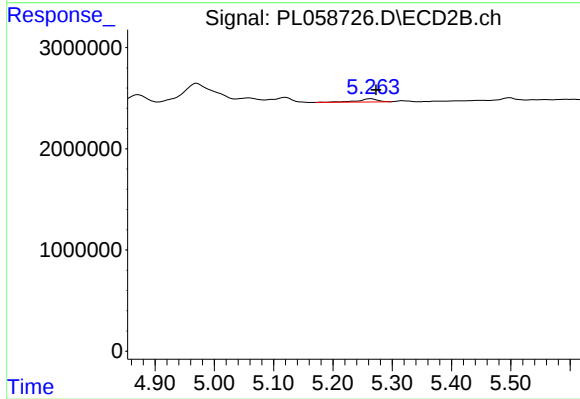

#4 Heptachlor


R.T.: 5.265 min
Delta R.T.: -0.008 min
Response: 729740
Conc: 0.26 ng/ml

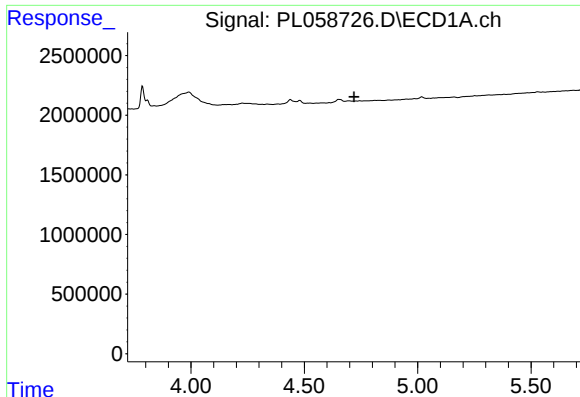

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.719 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

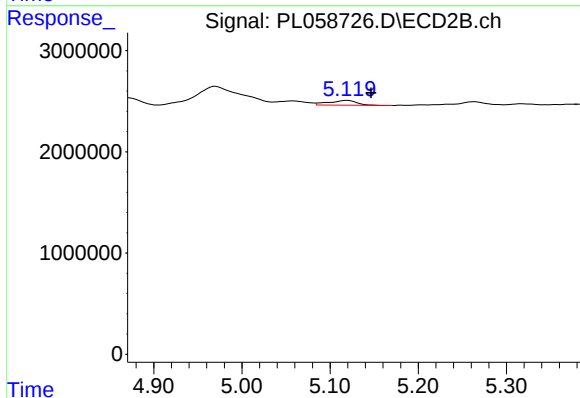


#7 delta-BHC

R.T.: 5.120 min
Delta R.T.: -0.027 min
Response: 1062175
Conc: 0.37 ng/ml

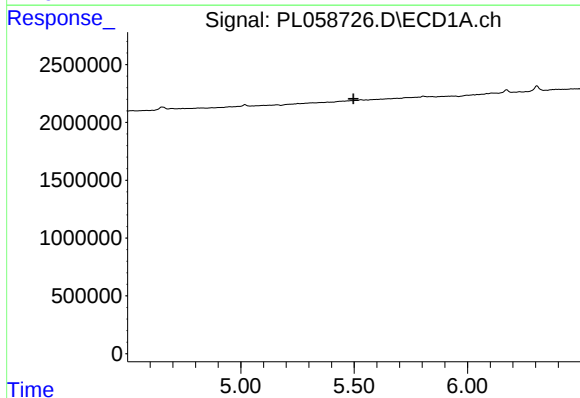


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

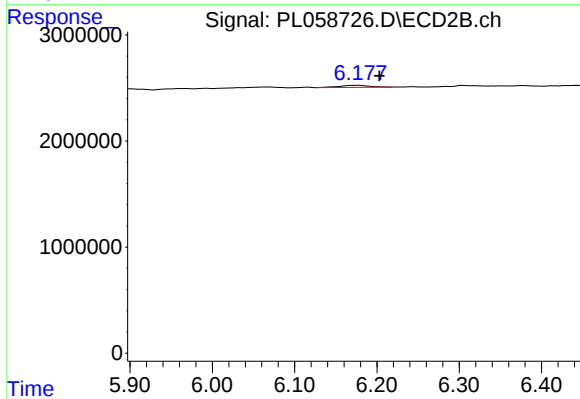

#10 gamma-Chlordane


R.T.: 6.178 min
Delta R.T.: -0.025 min
Response: 487128
Conc: 0.21 ng/ml

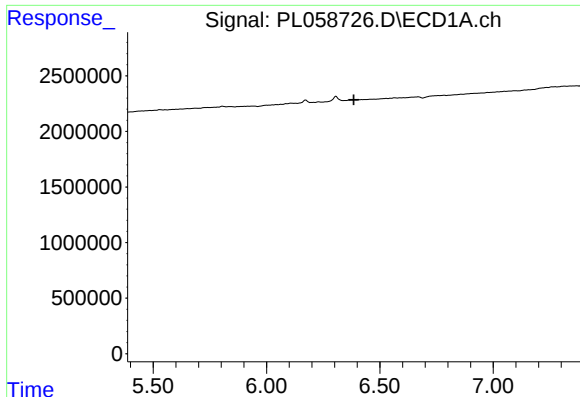

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.385 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

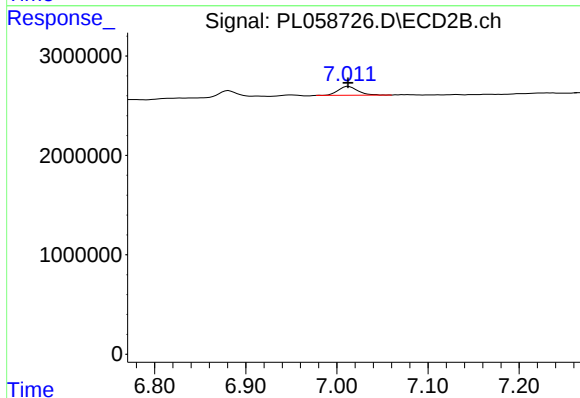


#15 Endosulfan II

R.T.: 7.013 min
Delta R.T.: 0.000 min
Response: 1350987
Conc: 0.68 ng/ml

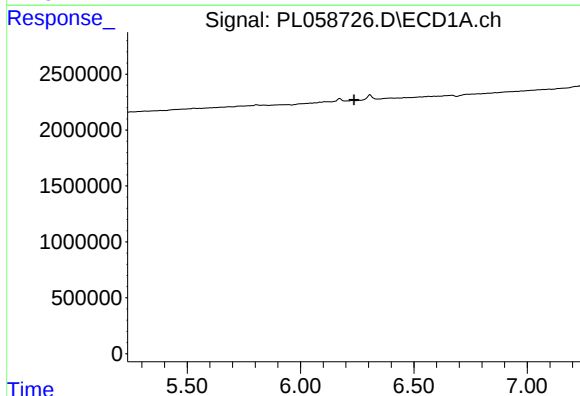


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.237 min
Response: 0
Conc: N.D.

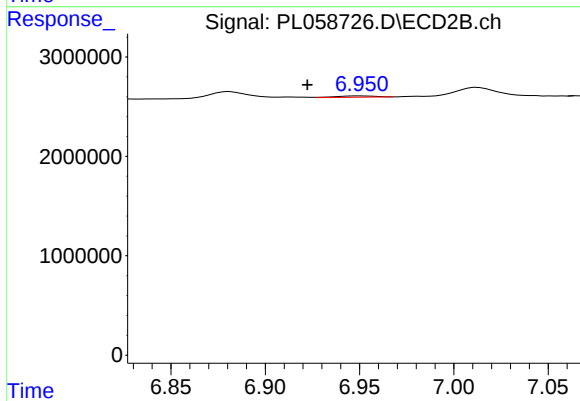

#16 4,4'-DDD


R.T.: 6.951 min
Delta R.T.: 0.029 min
Response: 183763
Conc: 0.11 ng/ml

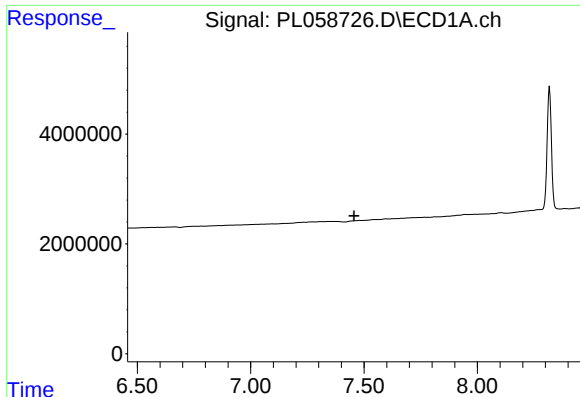

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

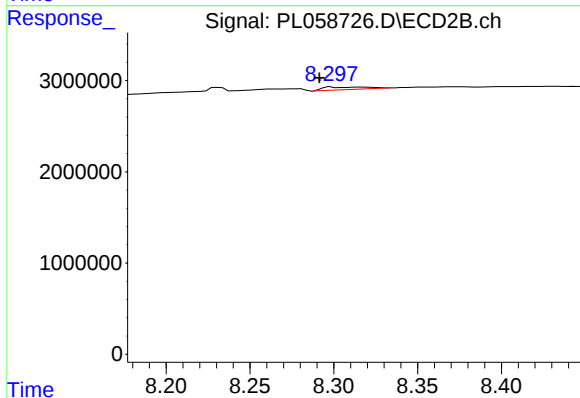


#22 Mirex

R.T.: 8.299 min
Delta R.T.: 0.007 min
Response: 512914
Conc: 0.33 ng/ml

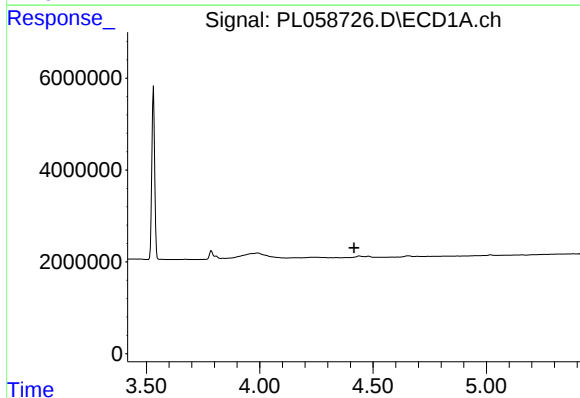


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.416 min
Response: 0
Conc: N.D.

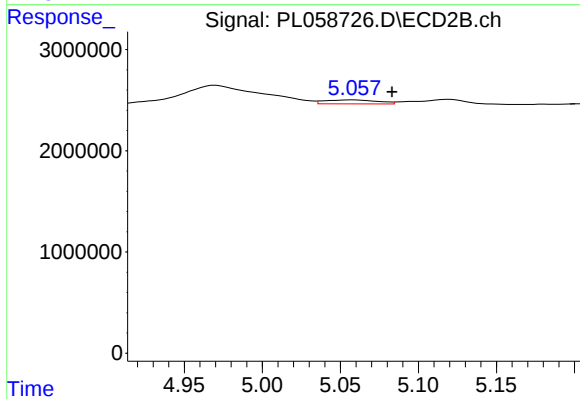

#23 Chlordane-1


R.T.: 5.059 min
Delta R.T.: -0.024 min
Response: 924095
Conc: 11.55 ng/ml

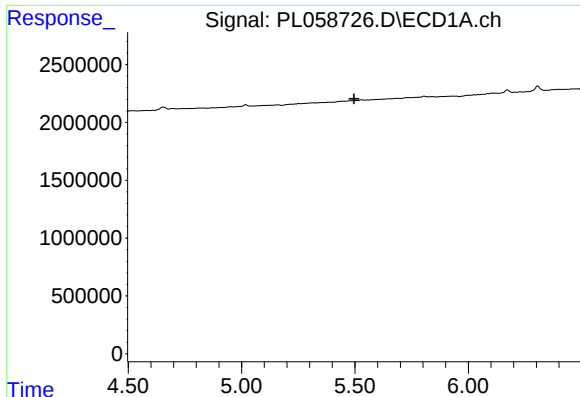

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

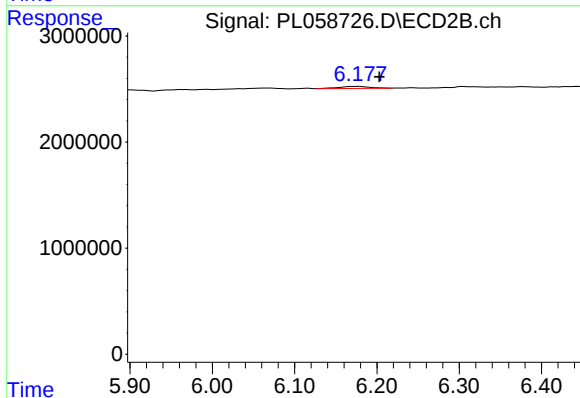


#25 Chlordane-3

R.T.: 6.178 min
Delta R.T.: -0.025 min
Response: 487128
Conc: 1.61 ng/ml

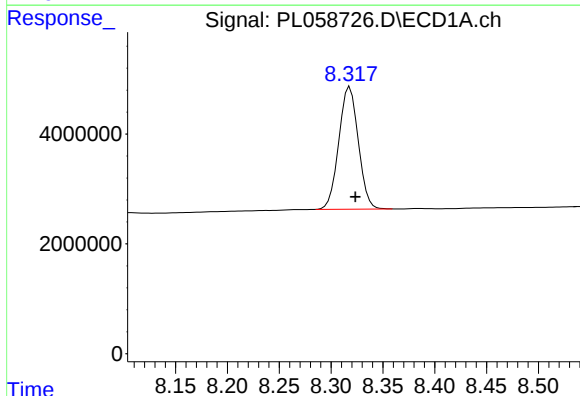

#28 Decachlorobiphenyl

R.T.: 8.318 min
Delta R.T.: -0.005 min
Response: 29195473
Conc: 22.36 ng/ml

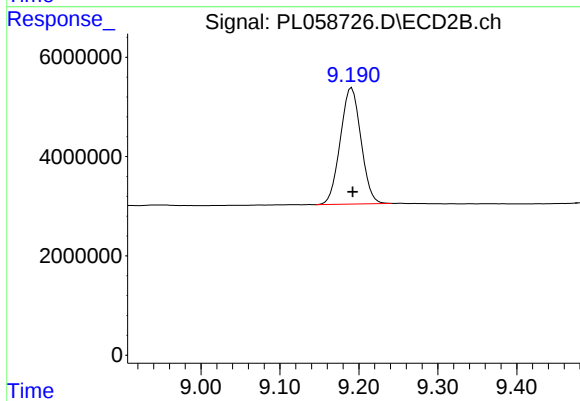

#28 Decachlorobiphenyl

R.T.: 9.191 min
Delta R.T.: -0.001 min
Response: 42660597
Conc: 24.14 ng/ml