

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051420\
 Data File : PL058734.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2020 18:41
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 23:58:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Thu May 14 06:40:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.532	4.078	32648976	49346590	19.873	22.797
28)	SA Decachlor...	8.319	9.192	32837232	47545802	25.148	26.903
Target Compounds							
2)	A alpha-BHC	3.988	0.000	1269348	0	0.551	N.D. #
7)	B delta-BHC	0.000	5.121f	0	2005168	N.D.	0.707 #
8)	B Heptachlo...	0.000	5.959	0	422864	N.D.	0.176 #
10)	B gamma-Chl...	0.000	6.173f	0	464662	N.D.	0.198 #
14)	MA Endrin	0.000	6.824f	0	261028	N.D.	0.144 #
15)	B Endosulfa...	0.000	7.013	0	1387986	N.D.	0.695 #
17)	MA 4,4'-DDT	0.000	7.228	0	127080	N.D.	0.075 #
21)	B Endrin ke...	0.000	7.844	0	143677	N.D.	0.071 #
25)	Chlordane-3	0.000	6.173f	0	464662	N.D.	1.534 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051420\
Data File : PL058734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2020 18:41
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 23:58:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Thu May 14 06:40:09 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

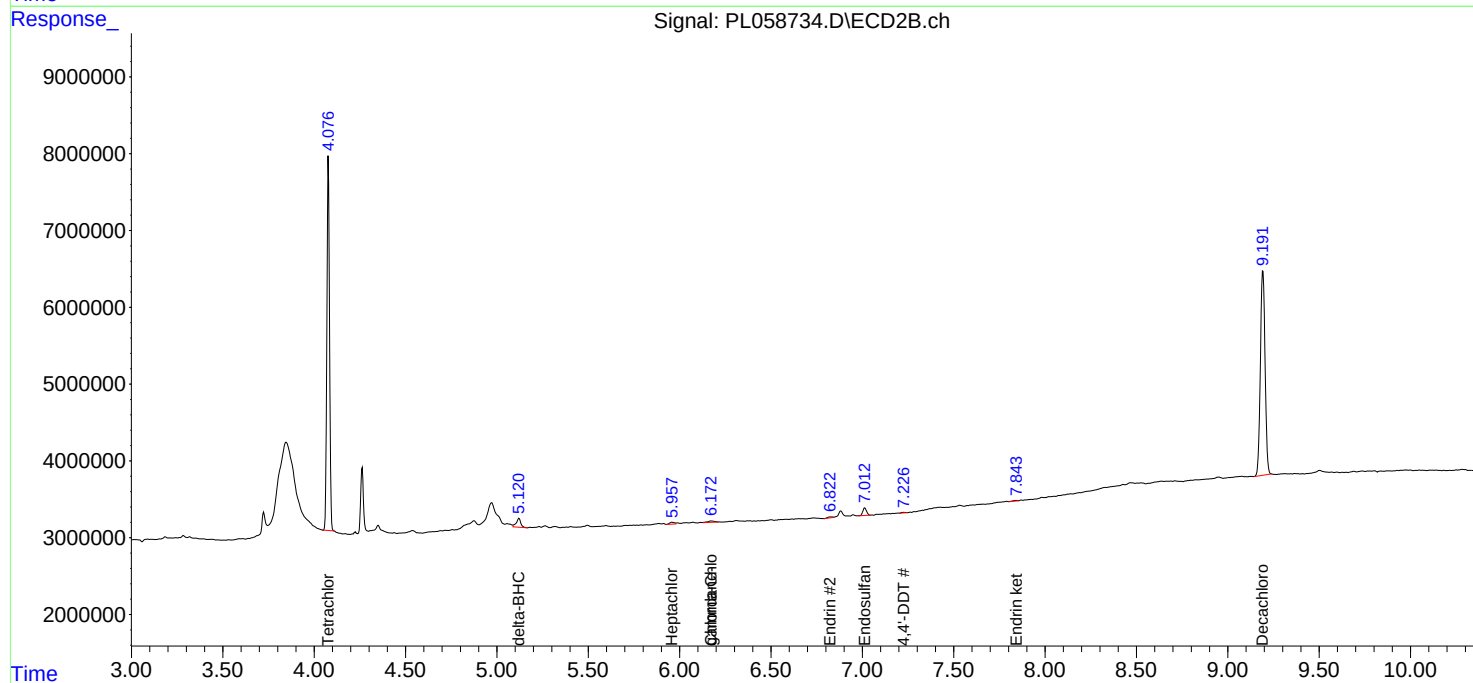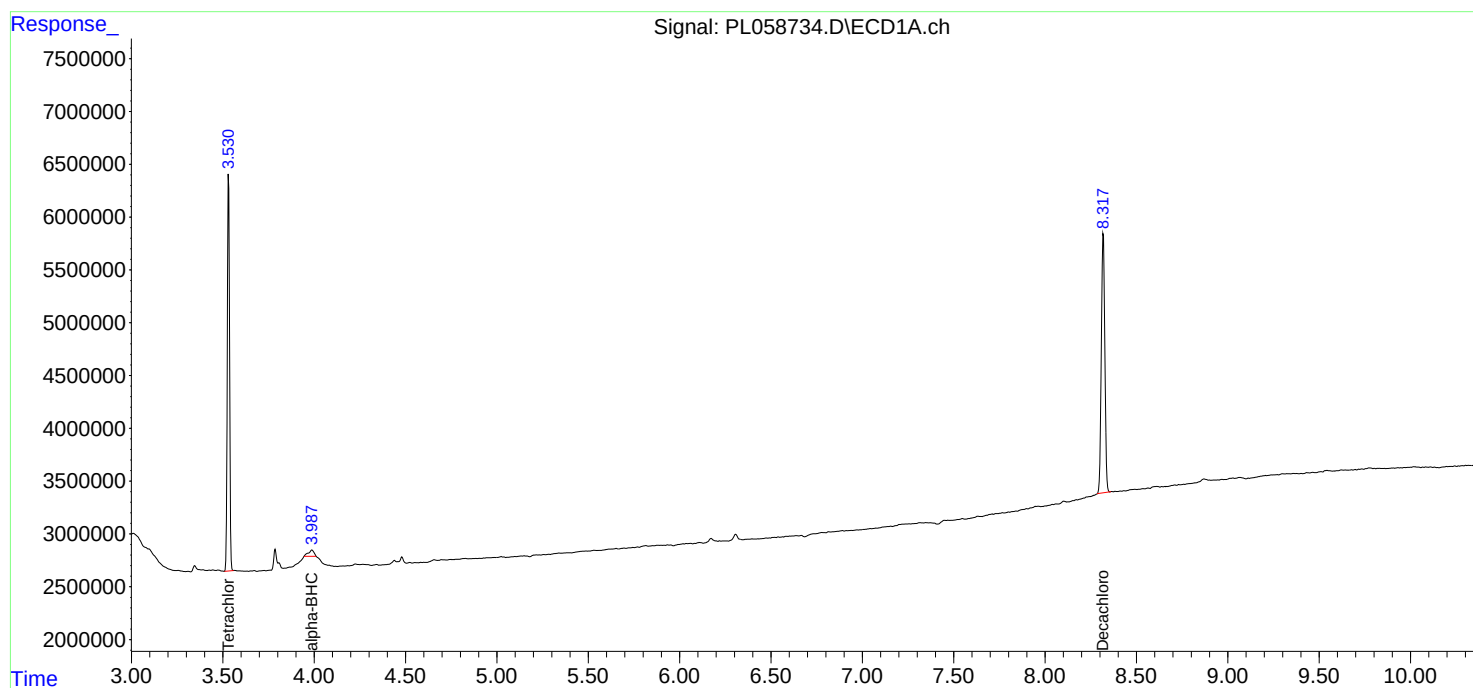


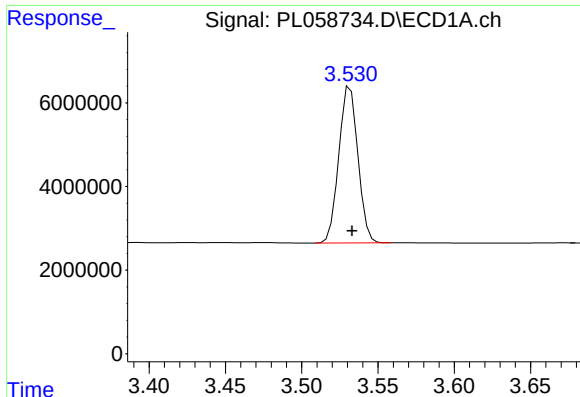

#1 Tetrachloro-m-xylene


R.T.: 3.532 min
Delta R.T.: -0.001 min
Response: 32648976
Conc: 19.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

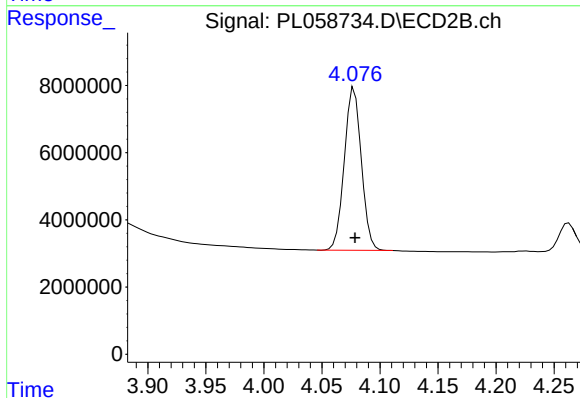


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 49346590
Conc: 22.80 ng/ml

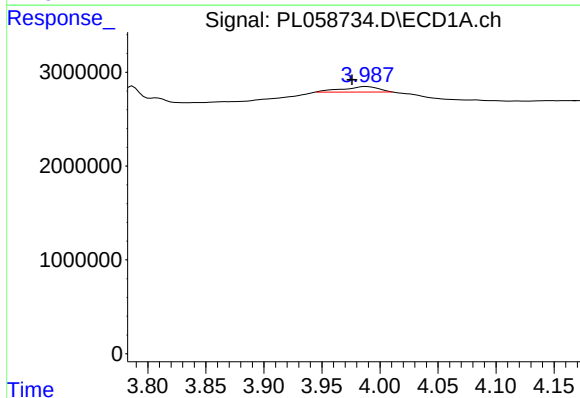


#2 alpha-BHC

R.T.: 3.988 min
Delta R.T.: 0.012 min
Response: 1269348
Conc: 0.55 ng/ml

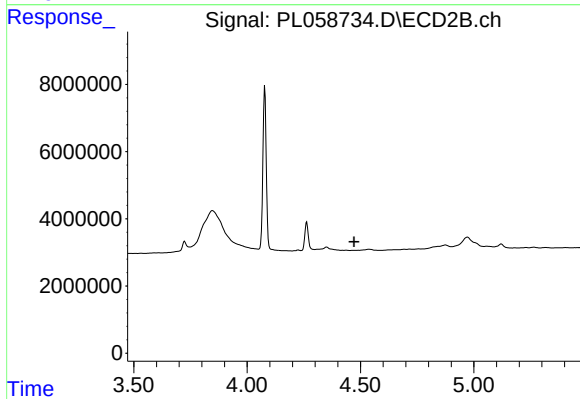

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.472 min
Response: 0
Conc: N.D.

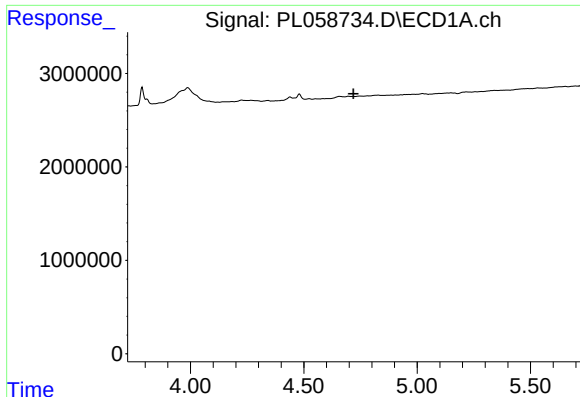

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.719 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

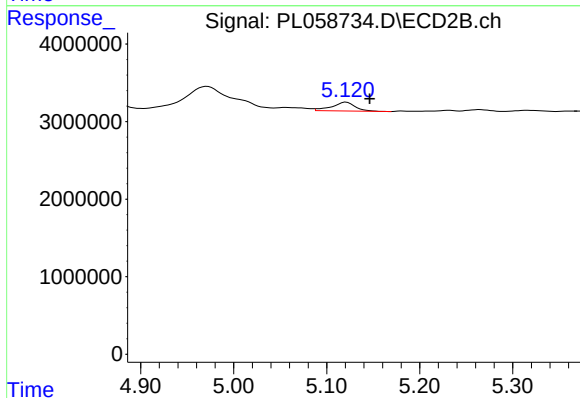


#7 delta-BHC

R.T.: 5.121 min
Delta R.T.: -0.025 min
Response: 2005168
Conc: 0.71 ng/ml

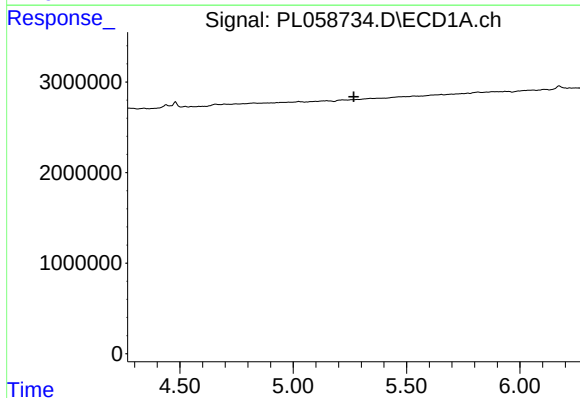


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.268 min
Response: 0
Conc: N.D.

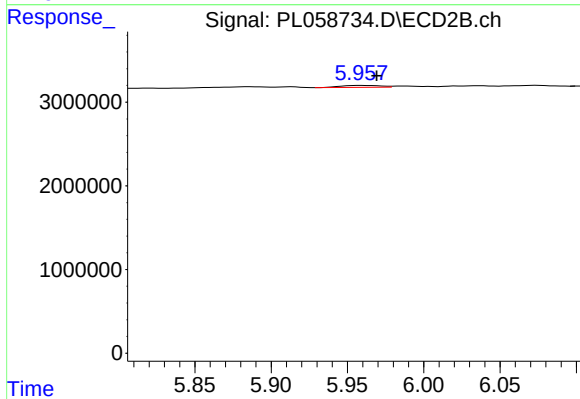

#8 Heptachlor epoxide


R.T.: 5.959 min
Delta R.T.: -0.011 min
Response: 422864
Conc: 0.18 ng/ml

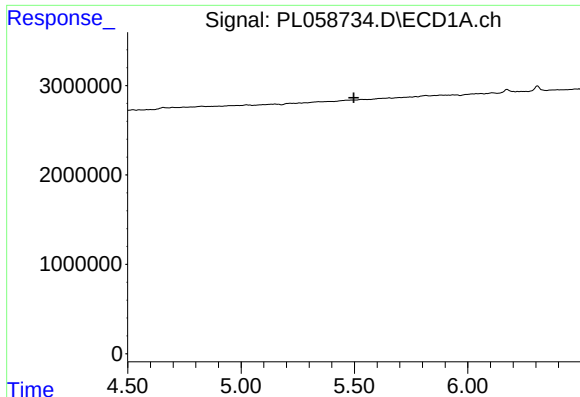

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

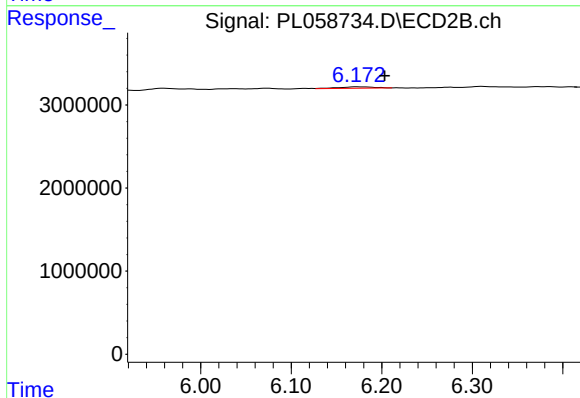


#10 gamma-Chlordane

R.T.: 6.173 min
Delta R.T.: -0.030 min
Response: 464662
Conc: 0.20 ng/ml

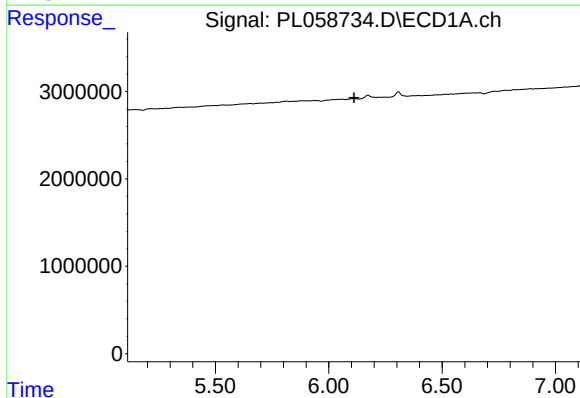


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

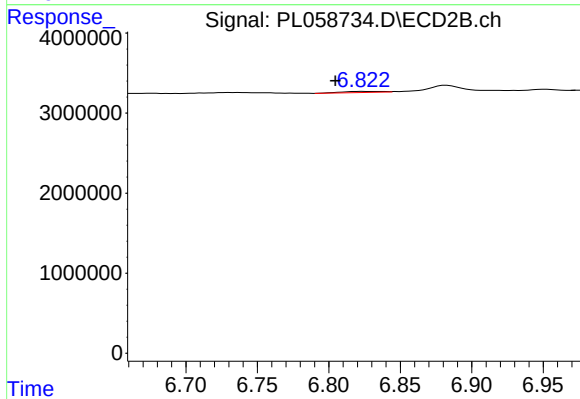

#14 Endrin


R.T.: 6.824 min
Delta R.T.: 0.019 min
Response: 261028
Conc: 0.14 ng/ml

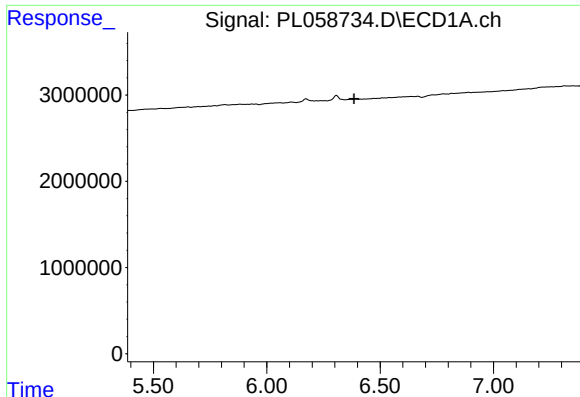

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.385 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

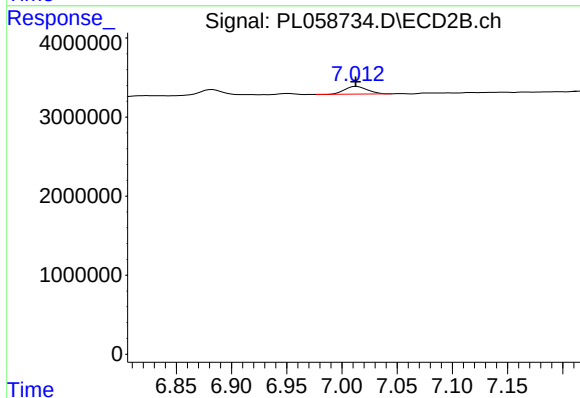


#15 Endosulfan II

R.T.: 7.013 min
Delta R.T.: 0.000 min
Response: 1387986
Conc: 0.70 ng/ml

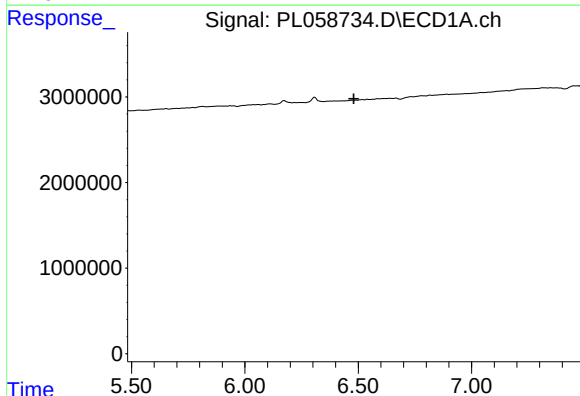


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.480 min
Response: 0
Conc: N.D.

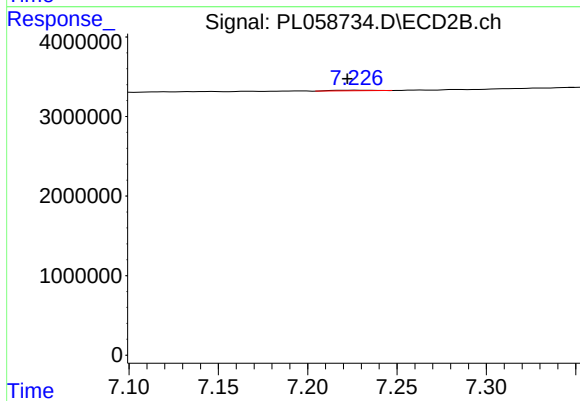

#17 4,4'-DDT


R.T.: 7.228 min
Delta R.T.: 0.006 min
Response: 127080
Conc: 0.08 ng/ml

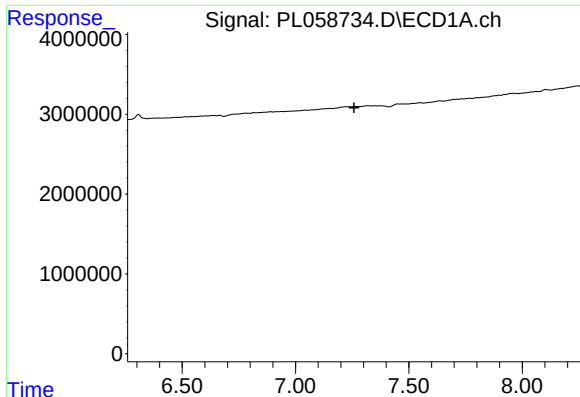

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.259 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

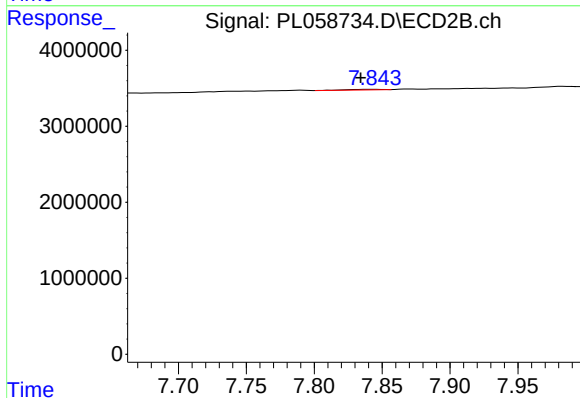


#21 Endrin ketone

R.T.: 7.844 min
Delta R.T.: 0.010 min
Response: 143677
Conc: 0.07 ng/ml

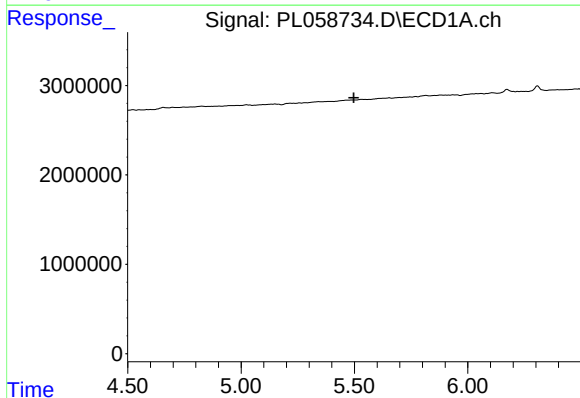


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

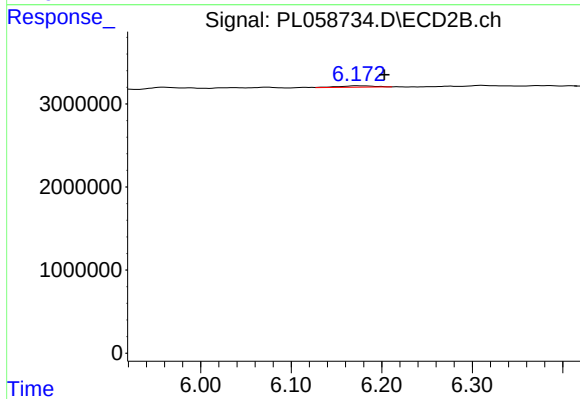

#25 Chlordane-3


R.T.: 6.173 min
Delta R.T.: -0.030 min
Response: 464662
Conc: 1.53 ng/ml

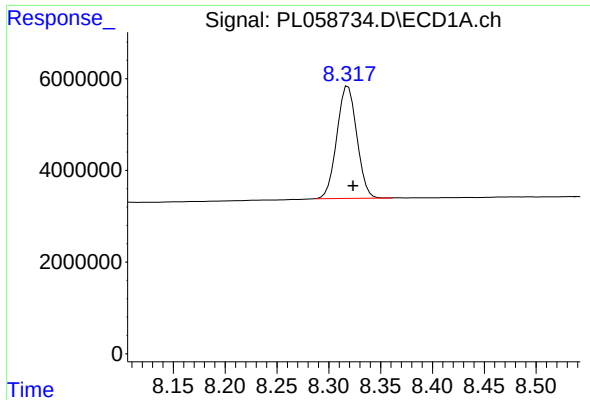

#28 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: -0.005 min
Response: 32837232
Conc: 25.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

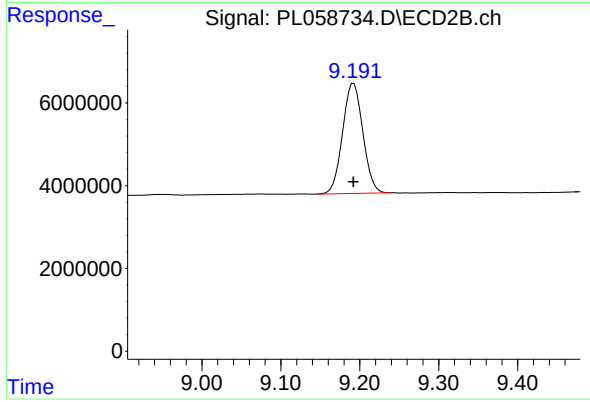

#28 Decachlorobiphenyl

R.T.: 9.192 min
Delta R.T.: 0.000 min
Response: 47545802
Conc: 26.90 ng/ml