

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051424\
 Data File : PL089522.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2024 16:54
 Operator : AR\AJ
 Sample : P2466-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-03-051324

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/15/2024
 Supervised By : Ankita Jodhani 05/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 00:45:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 26 19:27:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.551	2.800	26772633	17713372	13.295m	13.806
28) SA Decachlor...	9.064	7.946	18265467	17040280	13.056	12.668

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051424\
Data File : PL089522.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2024 16:54
Operator : AR\AJ
Sample : P2466-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-03-051324


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/15/2024
Supervised By : Ankita Jodhani 05/15/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 00:45:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
Quant Title : GC Extractables
QLast Update : Fri Apr 26 19:27:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

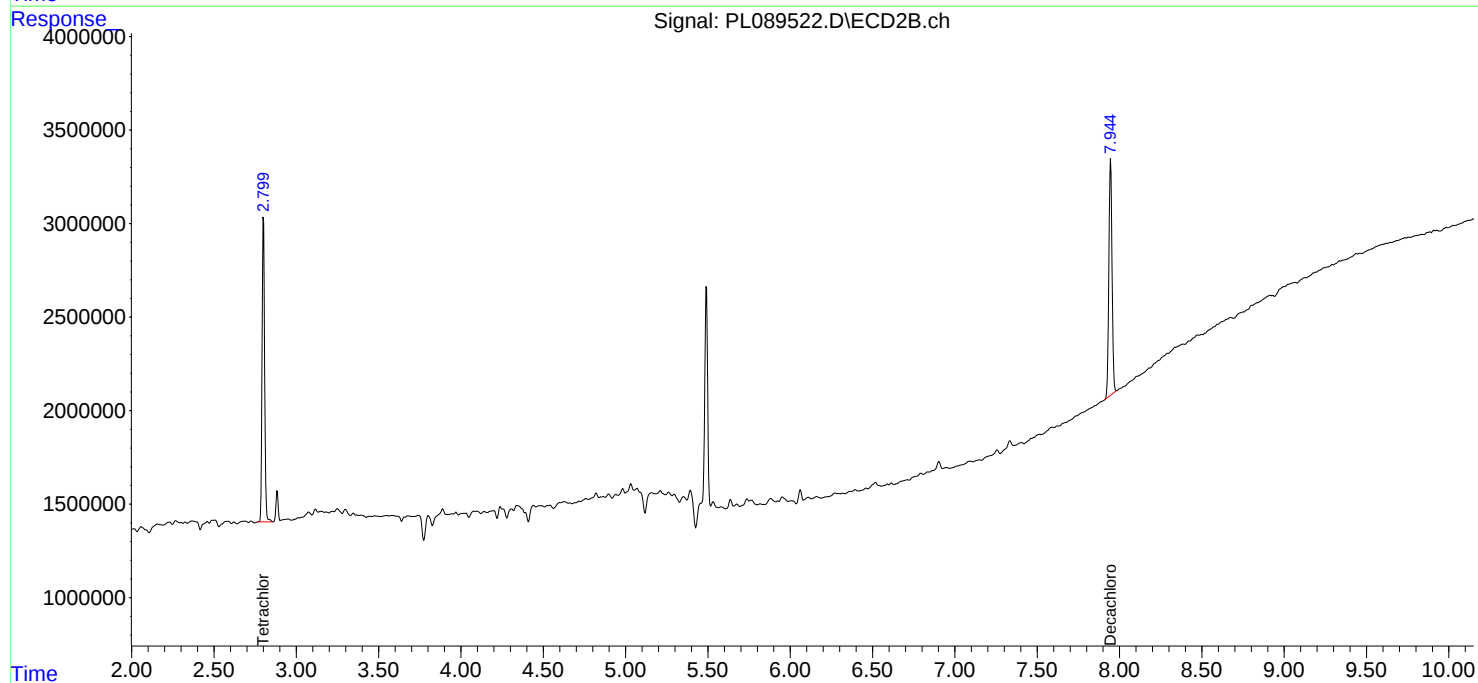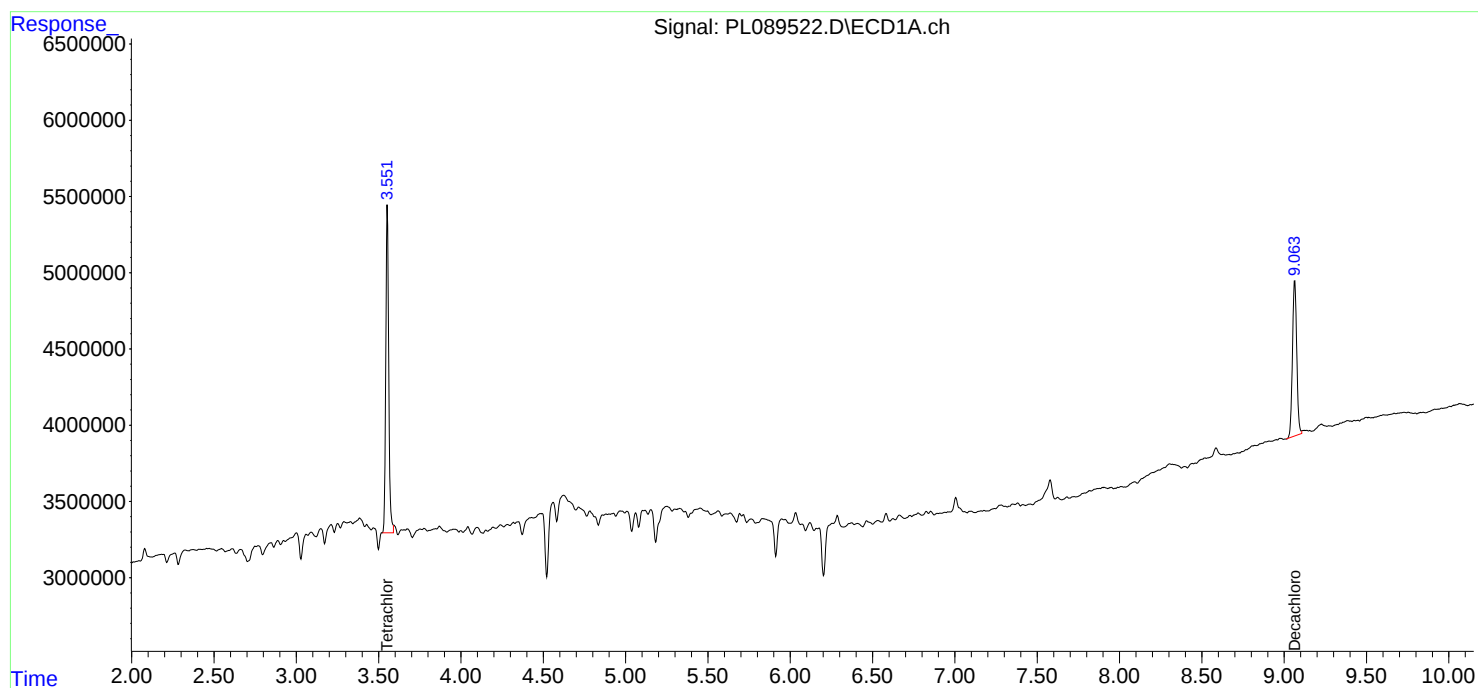

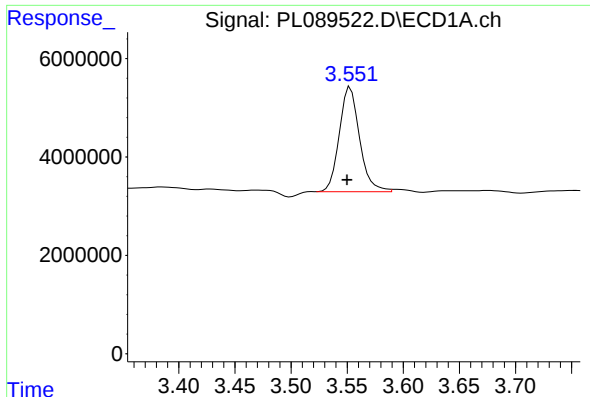


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: 0.001 min
Response: 26772633
Conc: 13.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-051324


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/15/2024
Supervised By :Ankita Jodhani 05/15/2024

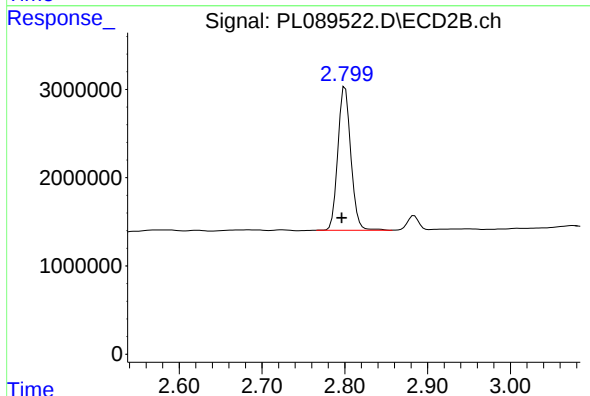


#1 Tetrachloro-m-xylene

R.T.: 2.800 min
Delta R.T.: 0.004 min
Response: 17713372
Conc: 13.81 ng/ml

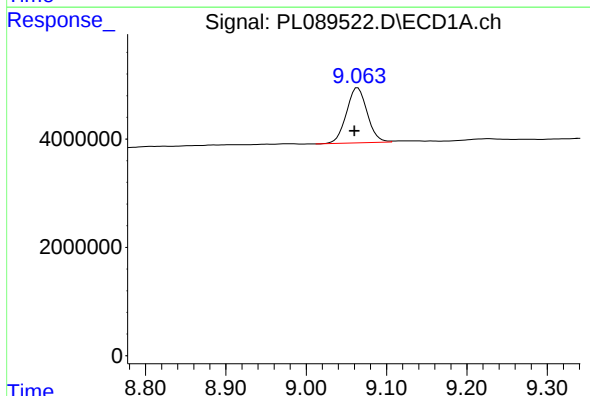

#28 Decachlorobiphenyl

R.T.: 9.064 min
Delta R.T.: 0.004 min
Response: 18265467
Conc: 13.06 ng/ml

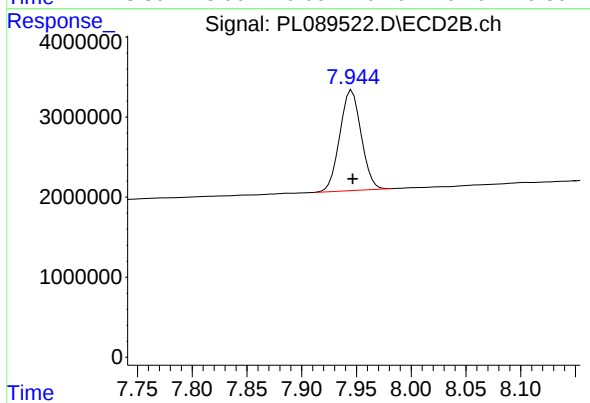

#28 Decachlorobiphenyl

R.T.: 7.946 min
Delta R.T.: 0.000 min
Response: 17040280
Conc: 12.67 ng/ml