

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051425\
 Data File : PL095679.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 19:12
 Operator : AR\AJ
 Sample : Q2022-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 02:12:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
 Quant Title : GC Extractables
 QLast Update : Tue May 13 14:38:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.591	2.906	117.1E6	99840911	28.670	21.315 #
28)	SA Decachlor...	9.113	8.082	68541421	80450230	20.204	19.504
Target Compounds							
7)	B delta-BHC	4.817	0.000	4981292	0	0.917	N.D. #
9)	A Endosulfan I	6.140f	5.281	19266871	11094740	3.936	2.145 #
13)	MA Dieldrin	0.000	5.526	0	14814998	N.D.	2.408 #
15)	B Endosulfa...	0.000	6.092	0	13501023	N.D.	2.465 #
16)	A 4,4'-DDD	6.744	0.000	10175011	0	2.619	N.D. #
17)	MA 4,4'-DDT	7.061	6.197	8706061	10497243	2.420	2.092
19)	B Endosulfa...	0.000	6.513	0	43569967	N.D.	8.763 #
20)	A Methoxychlor	0.000	6.800f	0	5803018	N.D.	2.145 #
24)	Chlordane-2	5.256f	0.000	6771803	0	24.549	N.D. #
27)	Chlordane-5	0.000	6.092	0	13501023	N.D.	47.005 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051425\
Data File : PL095679.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 19:12
Operator : AR\AJ
Sample : Q2022-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 02:12:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
Quant Title : GC Extractables
QLast Update : Tue May 13 14:38:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

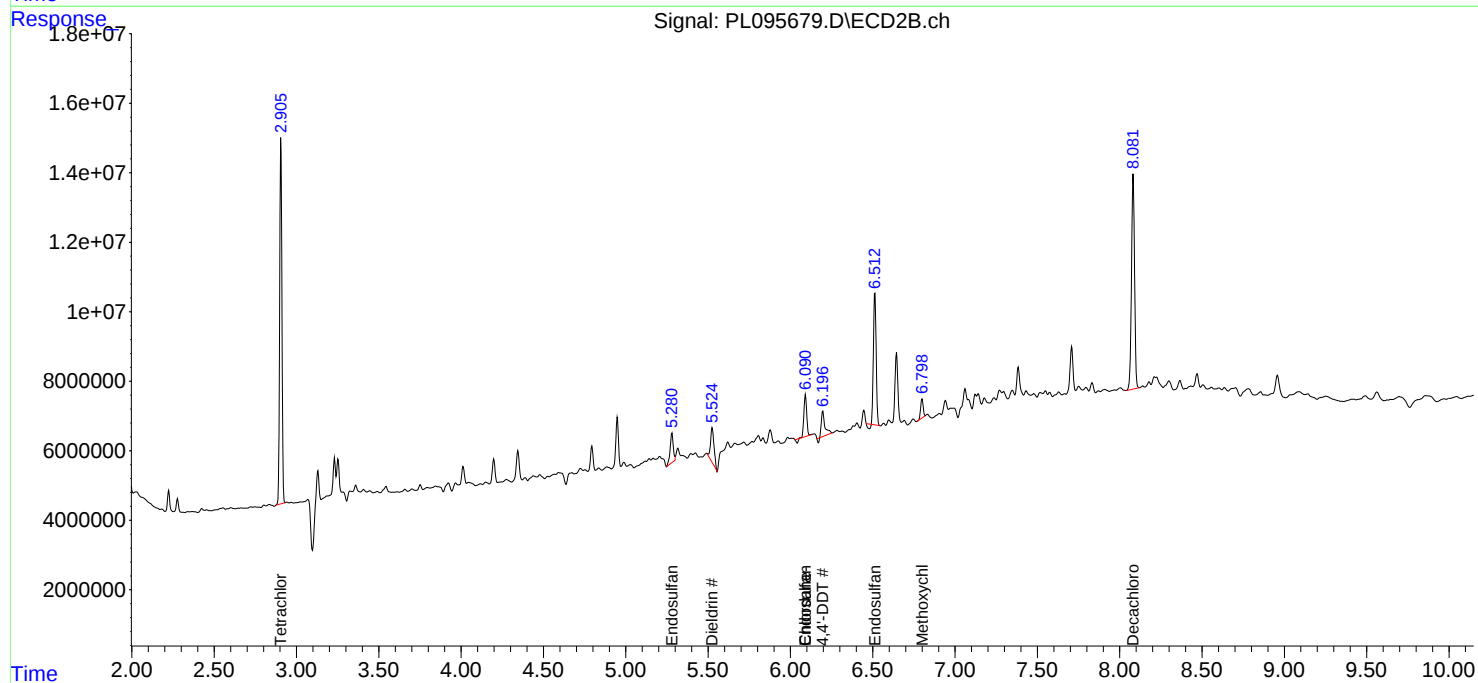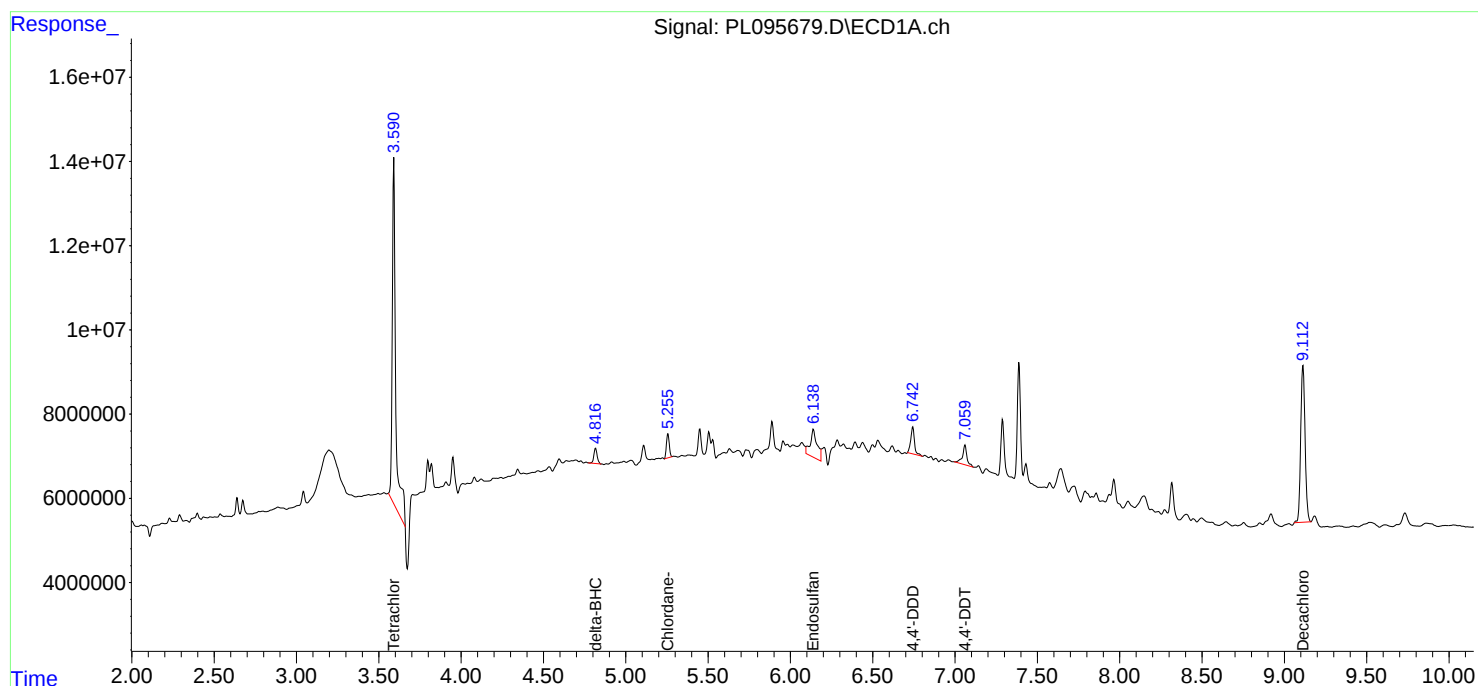


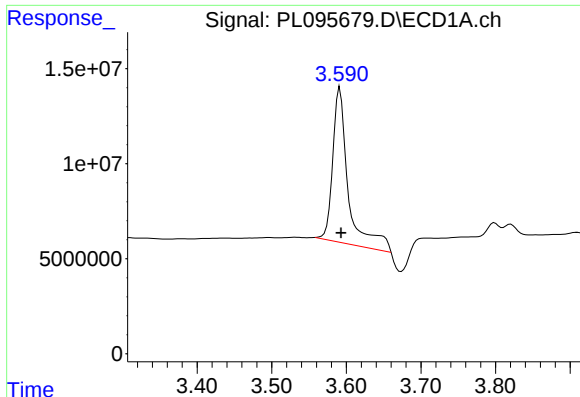

#1 Tetrachloro-m-xylene


R.T.: 3.591 min
Delta R.T.: -0.002 min
Response: 117146341
Conc: 28.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1

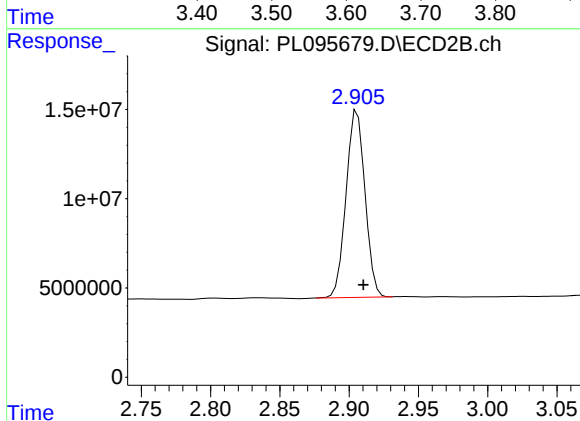


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: -0.004 min
Response: 99840911
Conc: 21.32 ng/ml

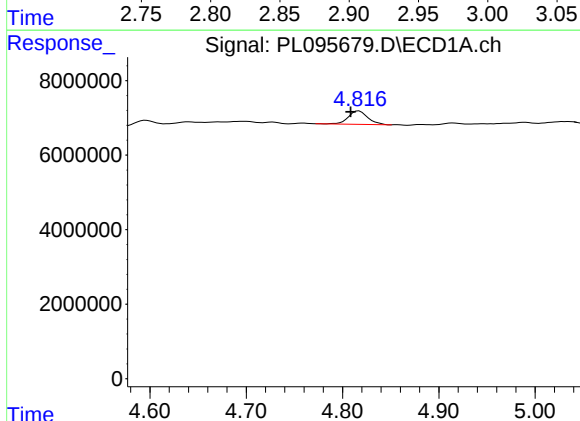


#7 delta-BHC

R.T.: 4.817 min
Delta R.T.: 0.008 min
Response: 4981292
Conc: 0.92 ng/ml

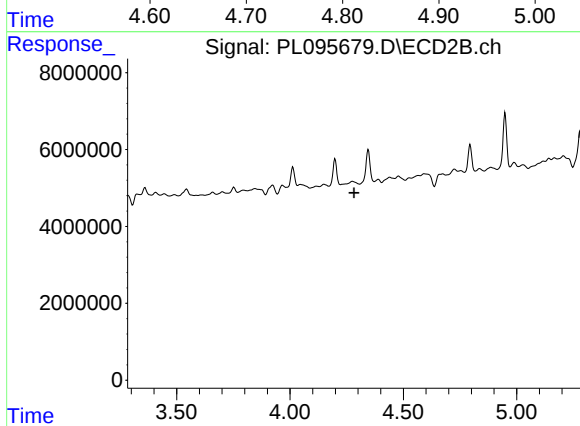

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.283 min
Response: 0
Conc: N.D.

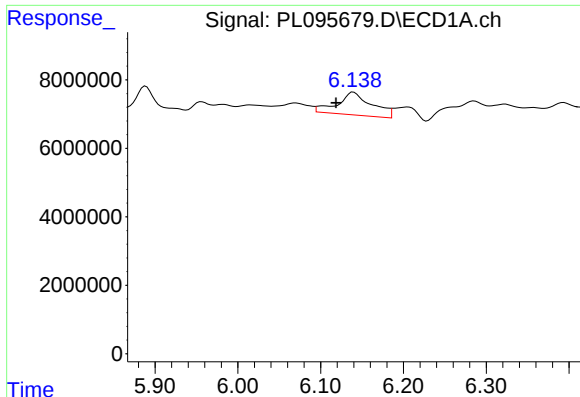

#9 Endosulfan I


R.T.: 6.140 min
Delta R.T.: 0.021 min
Response: 19266871
Conc: 3.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1

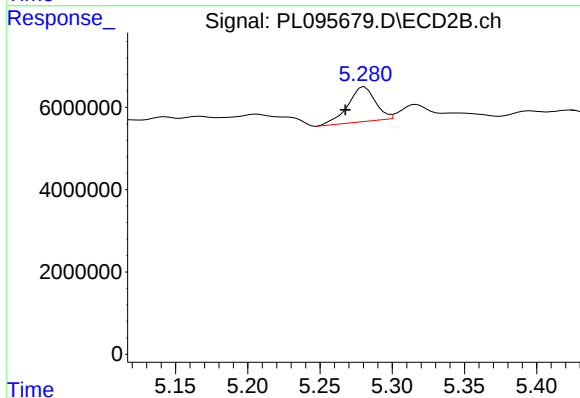


#9 Endosulfan I

R.T.: 5.281 min
Delta R.T.: 0.013 min
Response: 11094740
Conc: 2.15 ng/ml

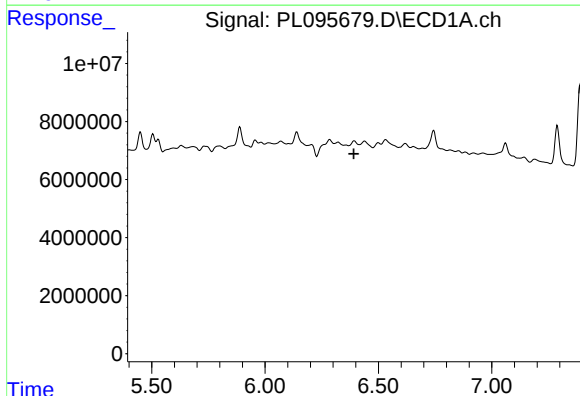


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.391 min
Response: 0
Conc: N.D.

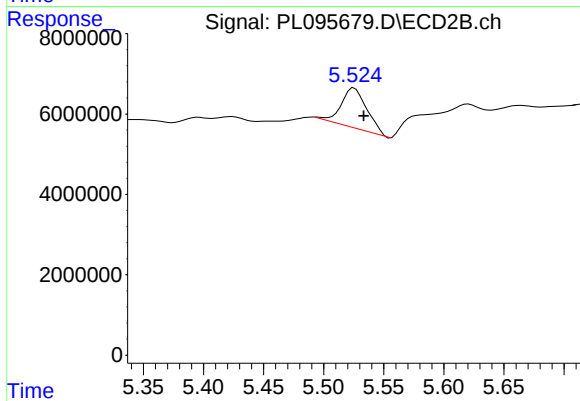

#13 Dieldrin


R.T.: 5.526 min
Delta R.T.: -0.008 min
Response: 14814998
Conc: 2.41 ng/ml

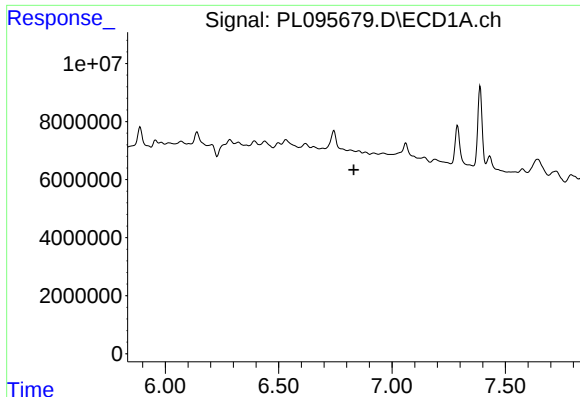

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.831 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-1

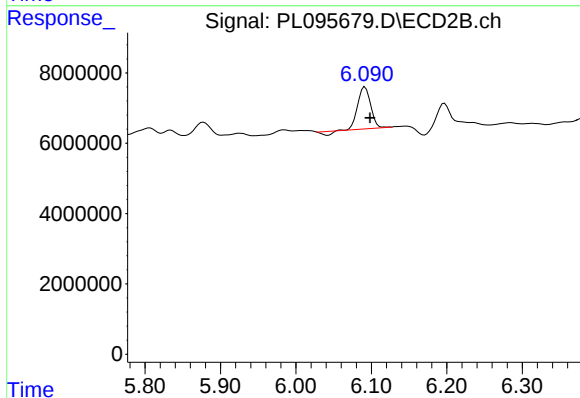


#15 Endosulfan II

R.T.: 6.092 min
Delta R.T.: -0.007 min
Response: 13501023
Conc: 2.47 ng/ml

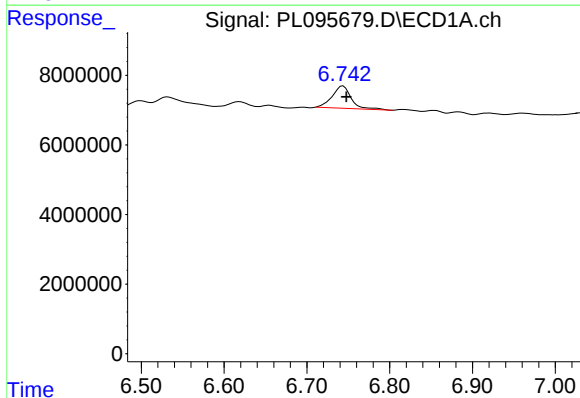


#16 4,4'-DDD

R.T.: 6.744 min
Delta R.T.: -0.004 min
Response: 10175011
Conc: 2.62 ng/ml

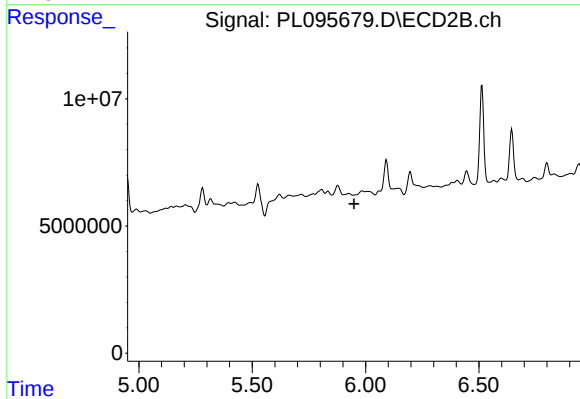

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.949 min
Response: 0
Conc: N.D.

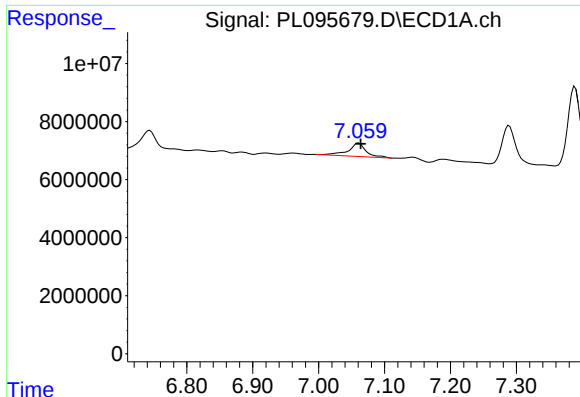

#17 4,4'-DDT


R.T.: 7.061 min
Delta R.T.: -0.003 min
Response: 8706061
Conc: 2.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1

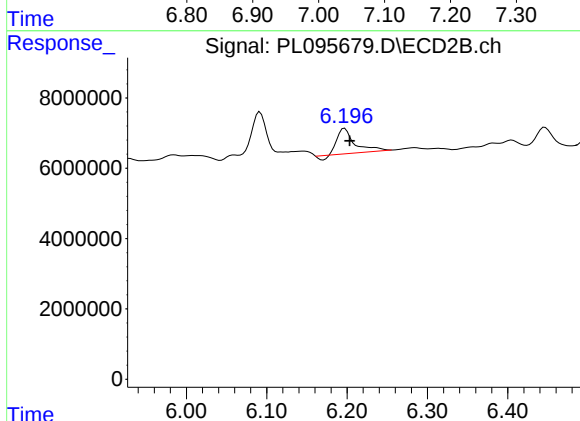


#17 4,4'-DDT

R.T.: 6.197 min
Delta R.T.: -0.006 min
Response: 10497243
Conc: 2.09 ng/ml

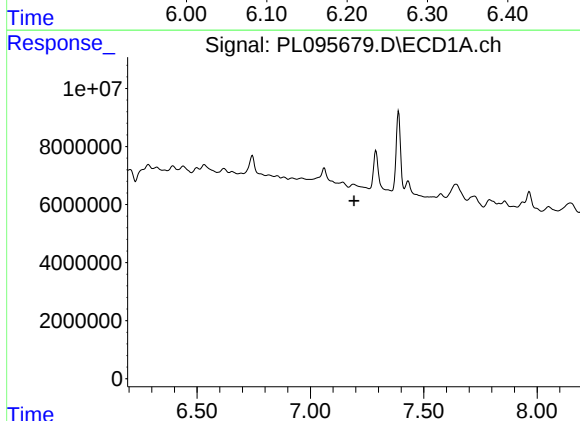


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.193 min
Response: 0
Conc: N.D.

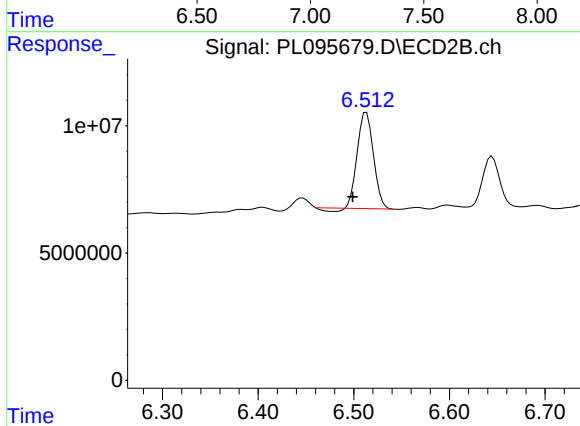

#19 Endosulfan Sulfate


R.T.: 6.513 min
Delta R.T.: 0.014 min
Response: 43569967
Conc: 8.76 ng/ml

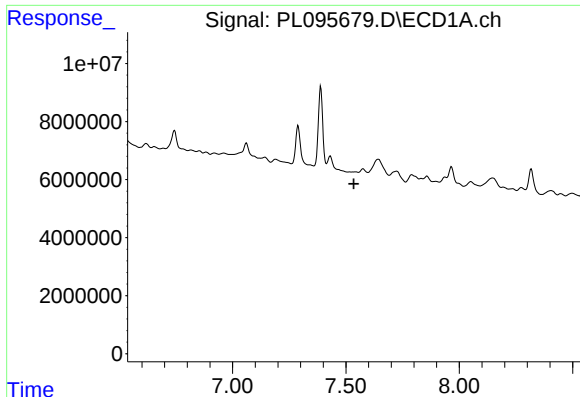

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.534 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-1

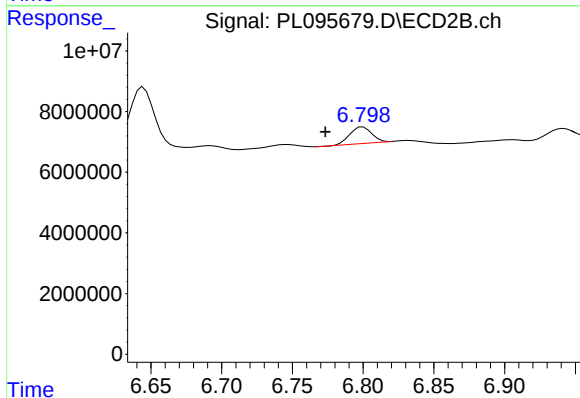


#20 Methoxychlor

R.T.: 6.800 min
Delta R.T.: 0.026 min
Response: 5803018
Conc: 2.14 ng/ml

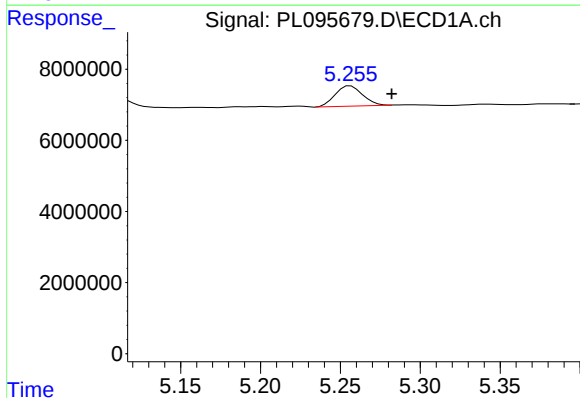


#24 Chlordane-2

R.T.: 5.256 min
Delta R.T.: -0.026 min
Response: 6771803
Conc: 24.55 ng/ml

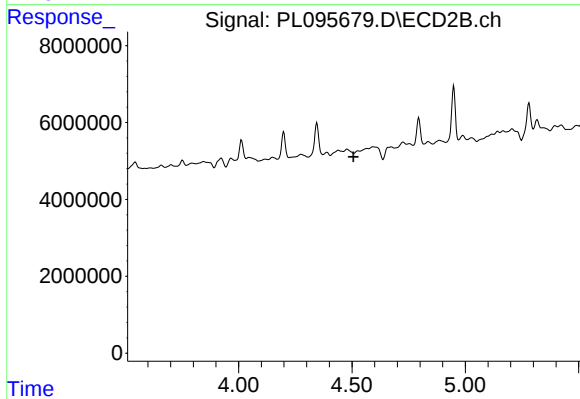

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.507 min
Response: 0
Conc: N.D.

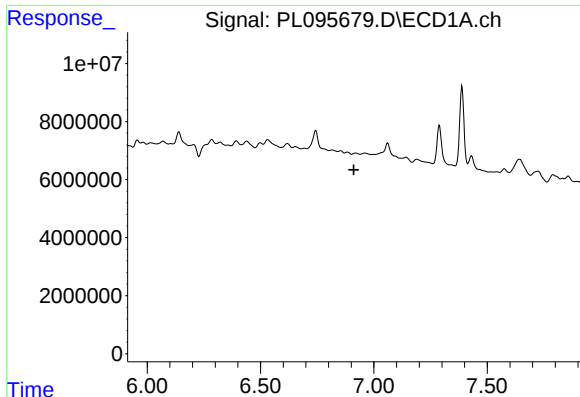

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.911 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-1

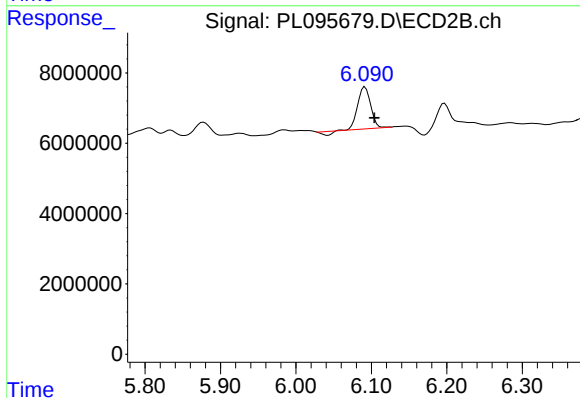


#27 Chlordane-5

R.T.: 6.092 min
Delta R.T.: -0.012 min
Response: 13501023
Conc: 47.00 ng/ml

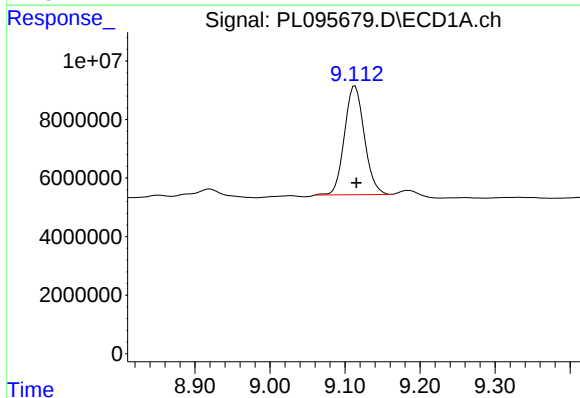

#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: -0.002 min
Response: 68541421
Conc: 20.20 ng/ml

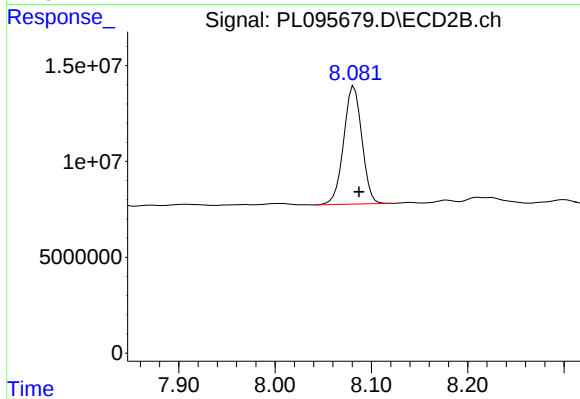

#28 Decachlorobiphenyl

R.T.: 8.082 min
Delta R.T.: -0.005 min
Response: 80450230
Conc: 19.50 ng/ml