

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051425\
 Data File : PL095680.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 19:26
 Operator : AR\AJ
 Sample : Q2022-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/15/2025
 Supervised By : mohammad ahmed 05/16/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 02:12:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
 Quant Title : GC Extractables
 QLast Update : Tue May 13 14:38:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.590	2.906	82730556	89291778	20.247m	19.063
28) SA Decachlor...	9.112	8.080	61559068	70292960	18.146	17.042m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051425\
Data File : PL095680.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 19:26
Operator : AR\AJ
Sample : Q2022-04
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/15/2025
Supervised By : mohammad ahmed 05/16/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 02:12:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
Quant Title : GC Extractables
QLast Update : Tue May 13 14:38:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

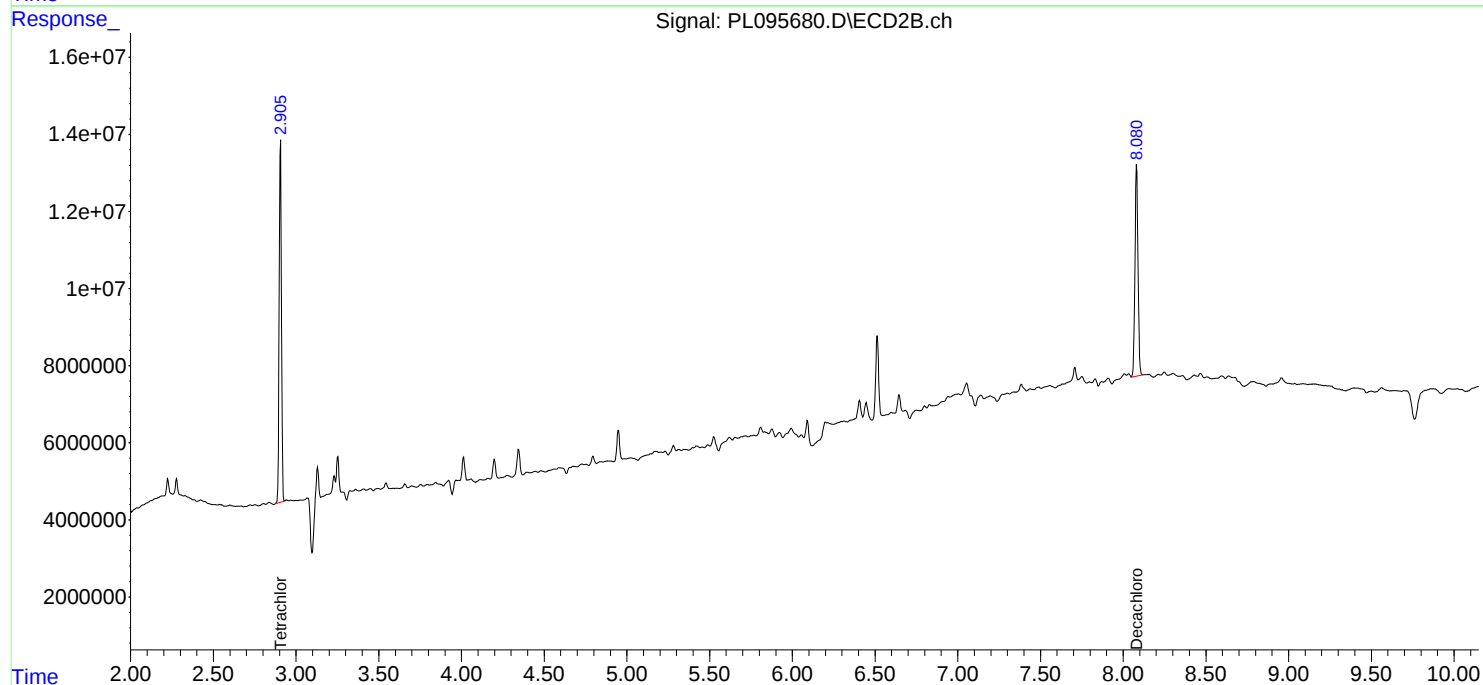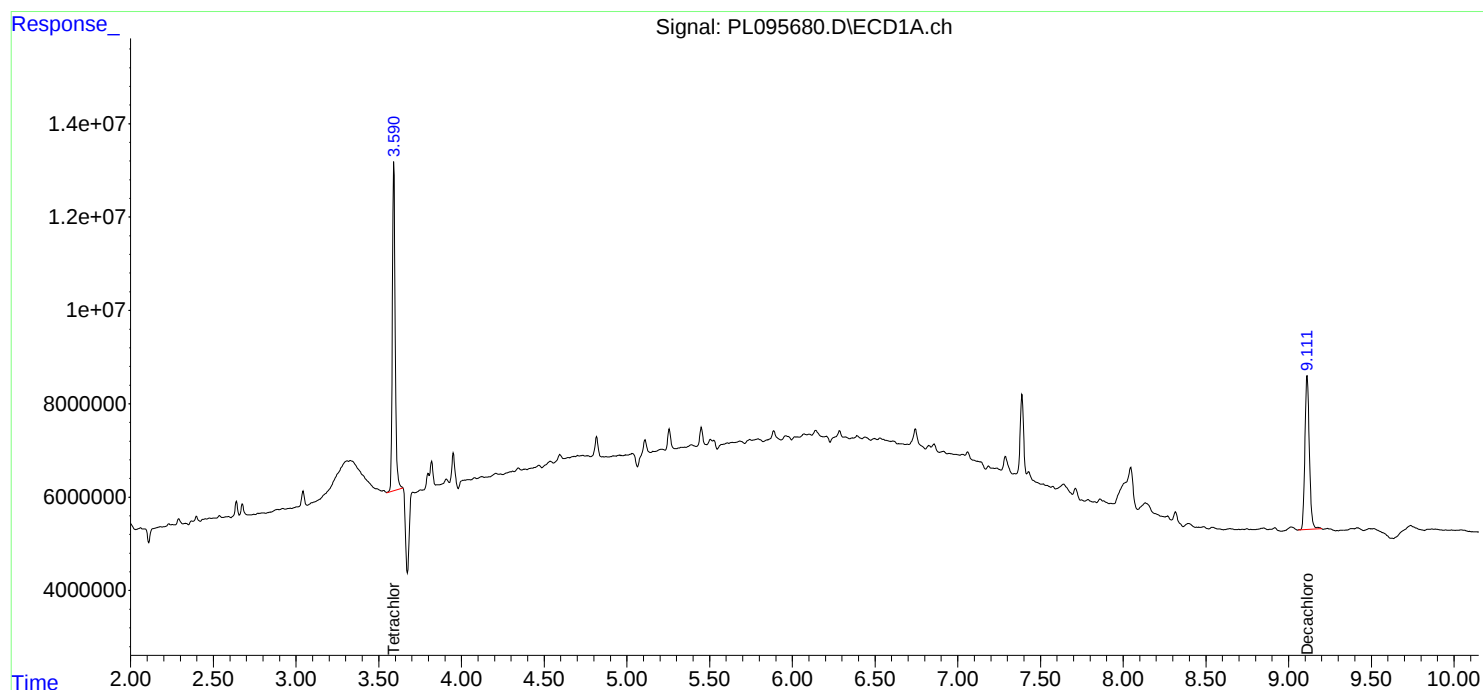

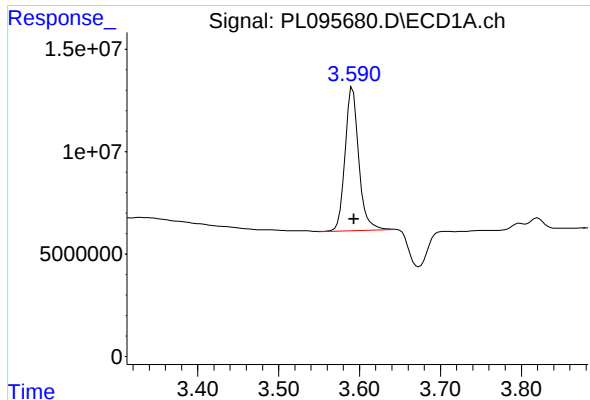


#1 Tetrachloro-m-xylene

R.T.: 3.590 min
Delta R.T.: -0.003 min
Response: 82730556
Conc: 20.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/15/2025
Supervised By :mohammad ahmed 05/16/2025

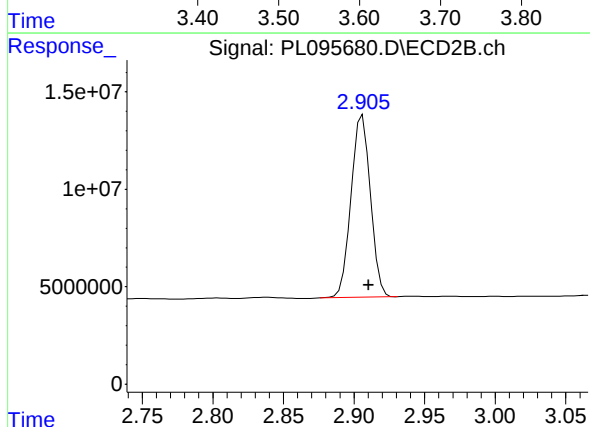


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: -0.004 min
Response: 89291778
Conc: 19.06 ng/ml

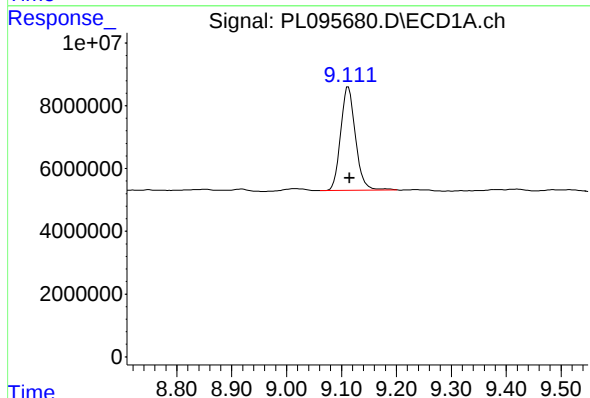

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: -0.003 min
Response: 61559068
Conc: 18.15 ng/ml

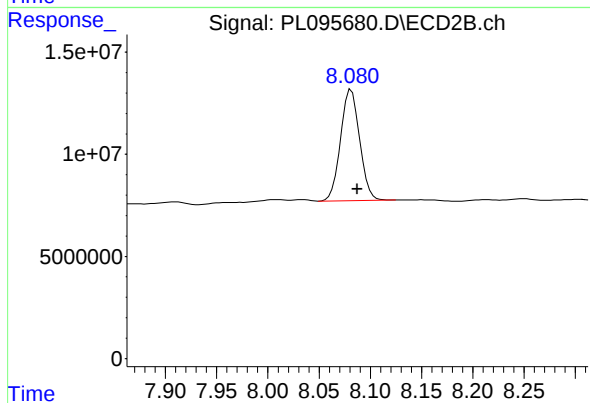

#28 Decachlorobiphenyl

R.T.: 8.080 min
Delta R.T.: -0.007 min
Response: 70292960
Conc: 17.04 ng/ml m