

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051519\
 Data File : PL048538.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2019 11:32
 Operator : AJ\SJ
 Sample : K2844-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HP-640

Manual Integrations
 APPROVED

Ankita
 5/16/2019 9:44:42 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 00:53:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.329	3.939	267.0E6	45874530	27.560m	18.417 #
28)	SA Decachlor...	7.995	8.977	117.0E6	40535306	11.637m	15.272 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051519\
Data File : PL048538.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2019 11:32
Operator : AJ\SJ
Sample : K2844-07
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HP-640


Manual Integrations
APPROVED

Ankita
5/16/2019 9:44:42 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 00:53:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

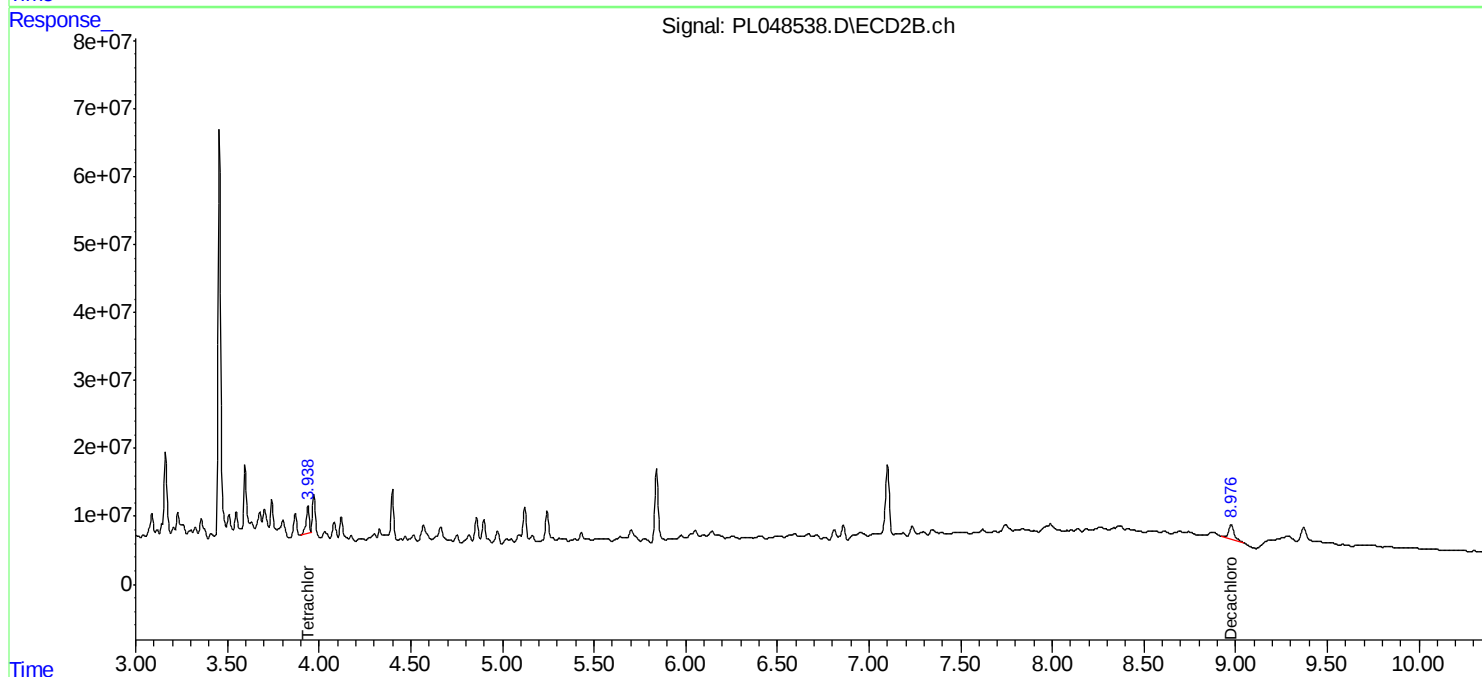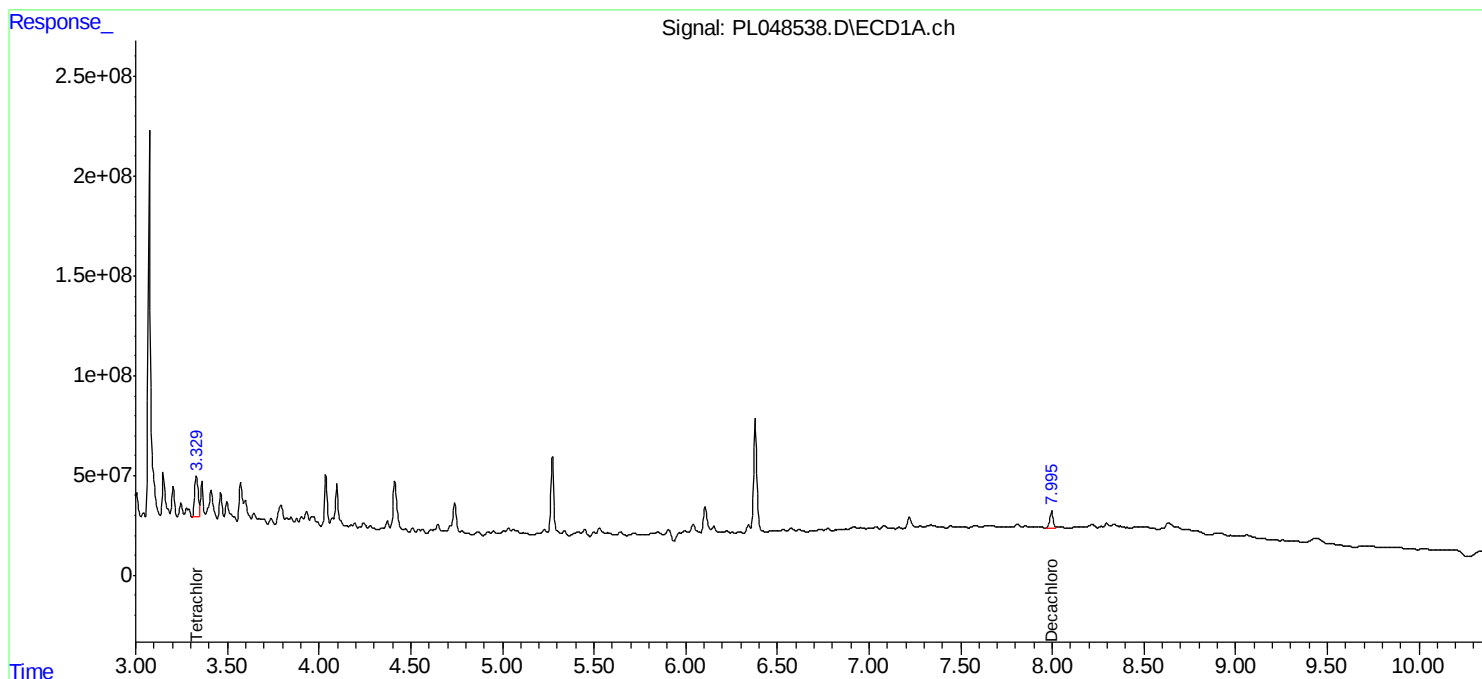

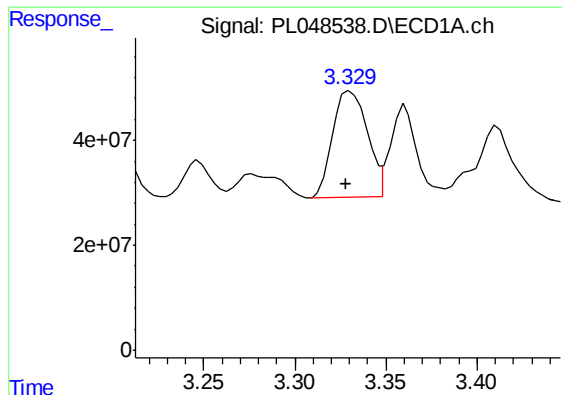


#1 Tetrachloro-m-xylene

R.T.: 3.329 min
Delta R.T.: 0.000 min
Response: 266968399
Conc: 27.56 ng/ml m

Instrument :
ECD_L
ClientSampleId :
HP-640


Manual Integrations
APPROVED

Ankita
5/16/2019 9:44:42 AM

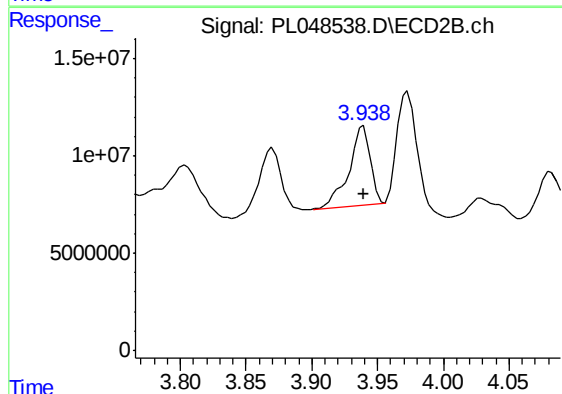


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 45874530
Conc: 18.42 ng/ml

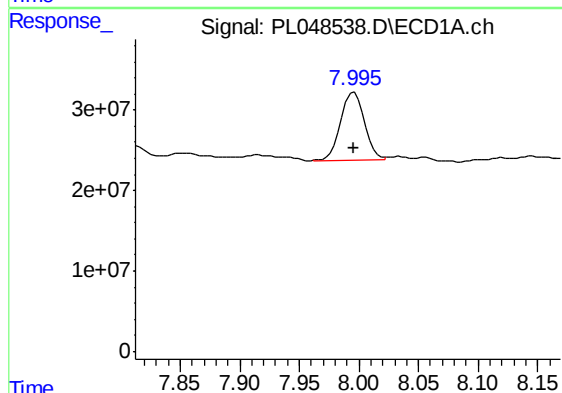

#28 Decachlorobiphenyl

R.T.: 7.995 min
Delta R.T.: -0.001 min
Response: 117004117
Conc: 11.64 ng/ml m

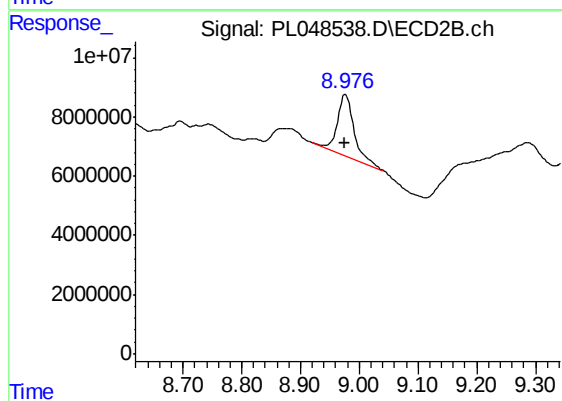

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: 0.002 min
Response: 40535306
Conc: 15.27 ng/ml