

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051520\
 Data File : PL058739.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2020 13:20
 Operator : AJ\MA
 Sample : PB128902BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 22:48:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Fri May 15 06:18:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	4.078	32418498	49959449	19.733	23.080
28)	SA Decachlor...	8.325	9.196	33954654	48735120	26.004	27.576
Target Compounds							
3)	MA gamma-BHC...	0.000	4.768	0	485638	N.D.	0.166 #
7)	B delta-BHC	0.000	5.121f	0	396874	N.D.	0.140 #
8)	B Heptachlo...	0.000	5.953f	0	1095417	N.D.	0.456 #
9)	A Endosulfan I	0.000	6.303f	0	82984	N.D.	0.039 #
11)	B alpha-Chl...	0.000	6.303f	0	82984	N.D.	0.035 #
15)	B Endosulfa...	0.000	7.013	0	5163318	N.D.	2.585 #
16)	A 4,4'-DDD	0.000	6.948f	0	844708	N.D.	0.483 #
17)	MA 4,4'-DDT	0.000	7.226	0	521460	N.D.	0.308 #
22)	Mirex	7.463	0.000	1365544	0	1.117	N.D. #
26)	Chlordane-4	0.000	6.303f	0	82984	N.D.	0.228 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051520\
Data File : PL058739.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2020 13:20
Operator : AJ\MA
Sample : PB128902BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 22:48:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Fri May 15 06:18:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

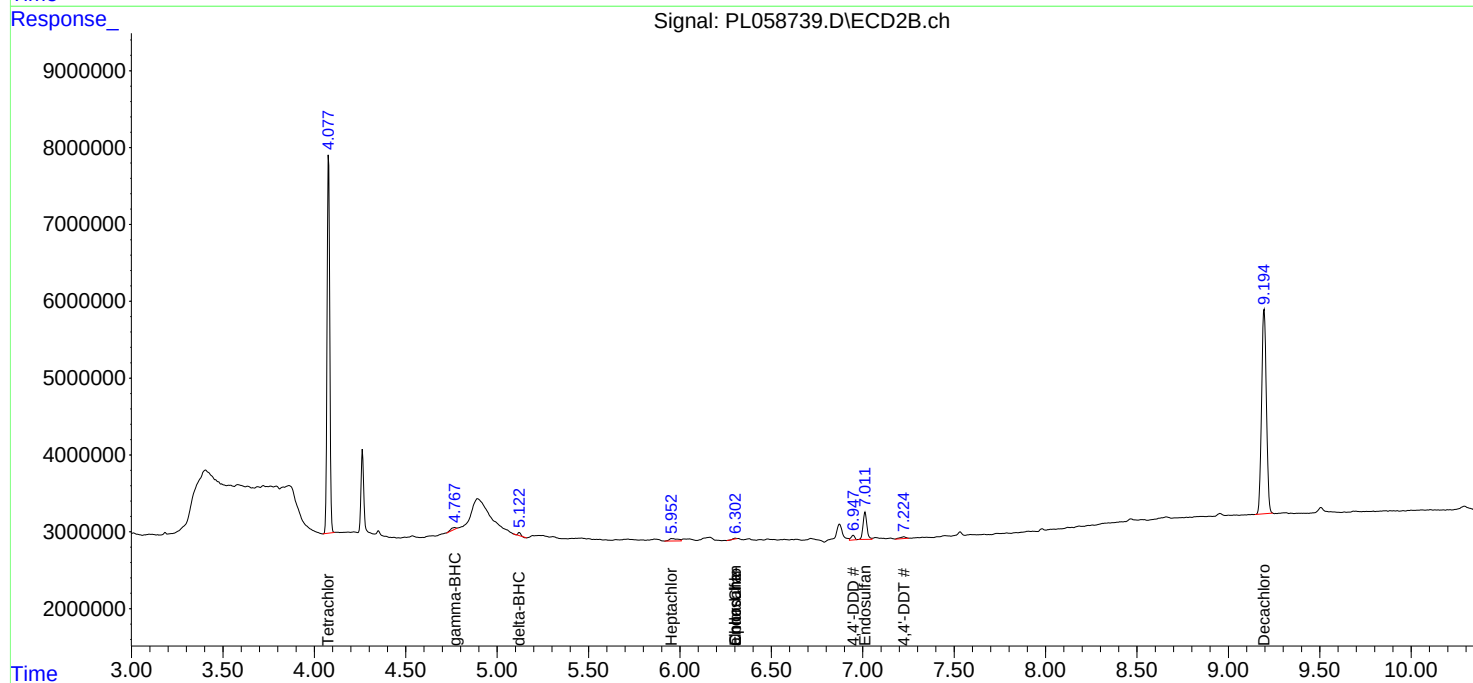


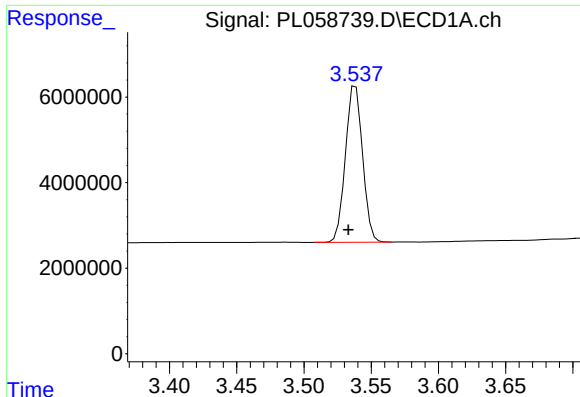

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.005 min
Response: 32418498
Conc: 19.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

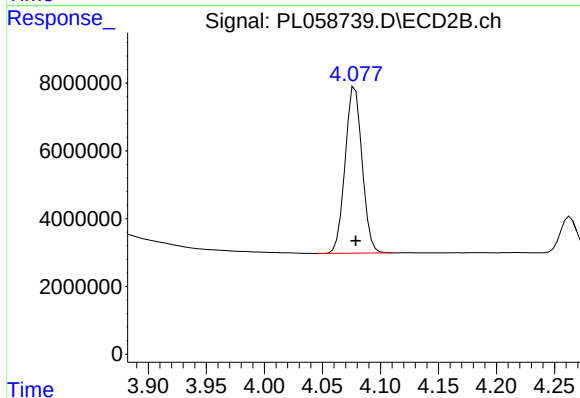


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 49959449
Conc: 23.08 ng/ml

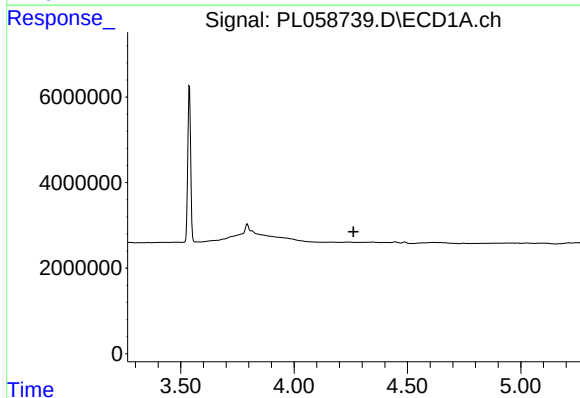


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.262 min
Response: 0
Conc: N.D.

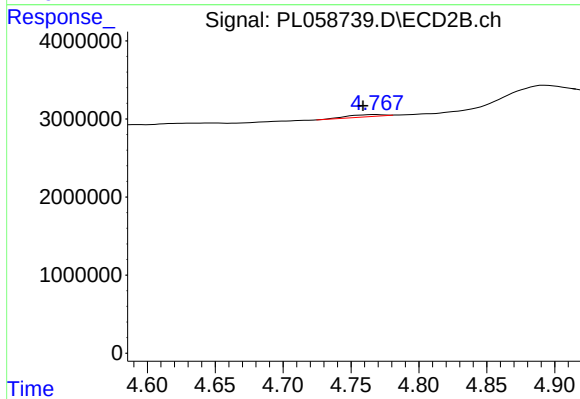

#3 gamma-BHC (Lindane)


R.T.: 4.768 min
Delta R.T.: 0.010 min
Response: 485638
Conc: 0.17 ng/ml

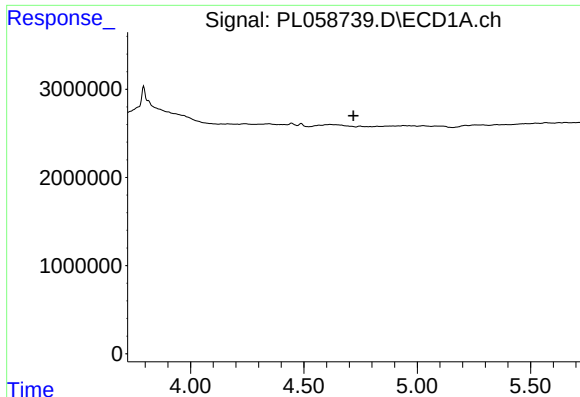

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.719 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

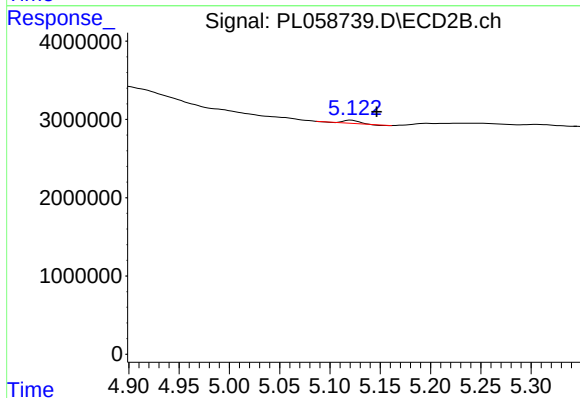


#7 delta-BHC

R.T.: 5.121 min
Delta R.T.: -0.025 min
Response: 396874
Conc: 0.14 ng/ml

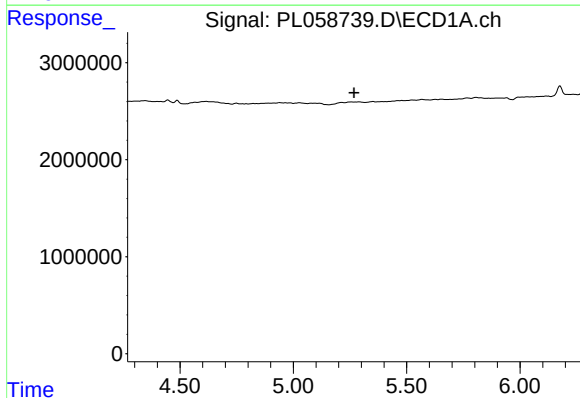


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.268 min
Response: 0
Conc: N.D.

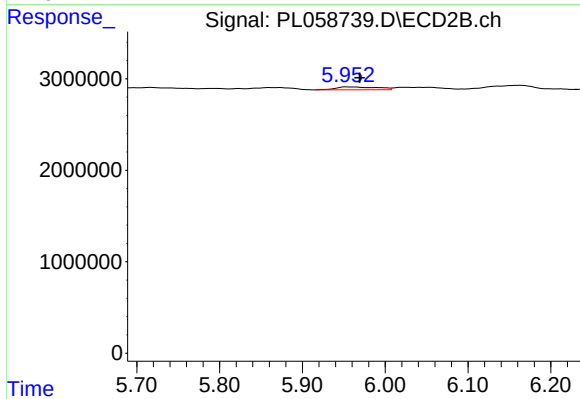

#8 Heptachlor epoxide


R.T.: 5.953 min
Delta R.T.: -0.016 min
Response: 1095417
Conc: 0.46 ng/ml

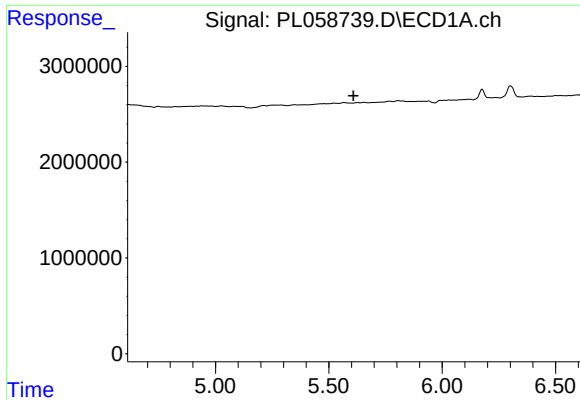

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.609 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

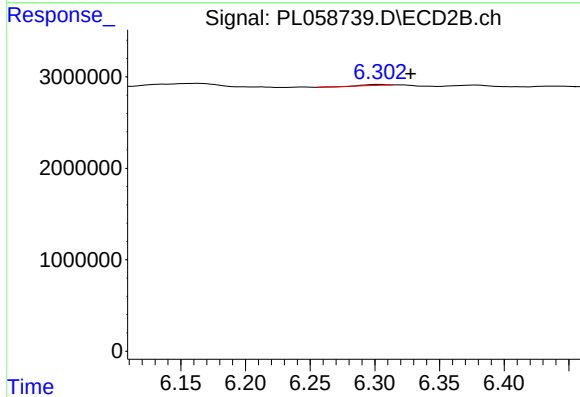


#9 Endosulfan I

R.T.: 6.303 min
Delta R.T.: -0.024 min
Response: 82984
Conc: 0.04 ng/ml

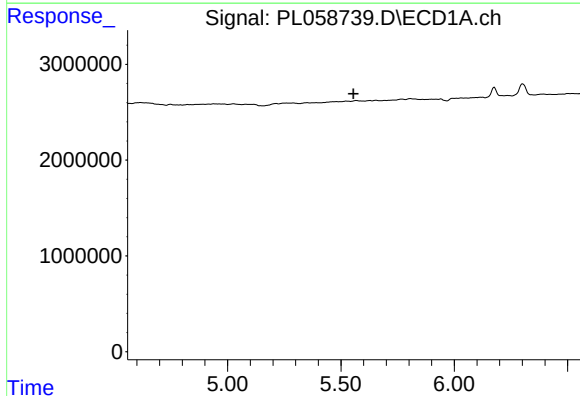


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.556 min
Response: 0
Conc: N.D.

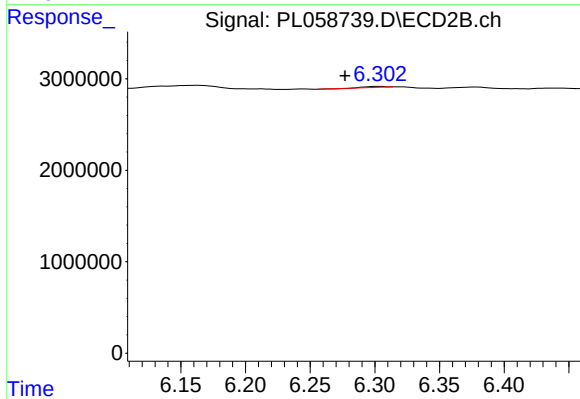

#11 alpha-Chlordane


R.T.: 6.303 min
Delta R.T.: 0.027 min
Response: 82984
Conc: 0.04 ng/ml

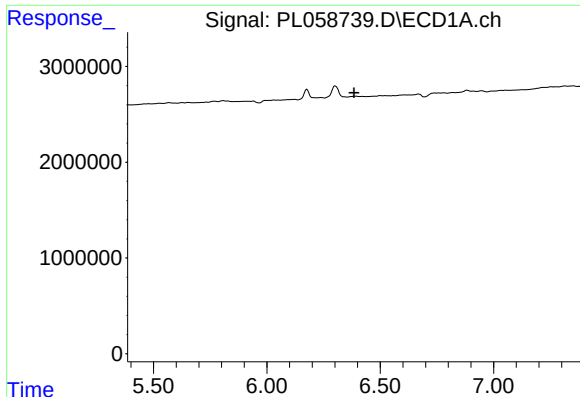

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.385 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

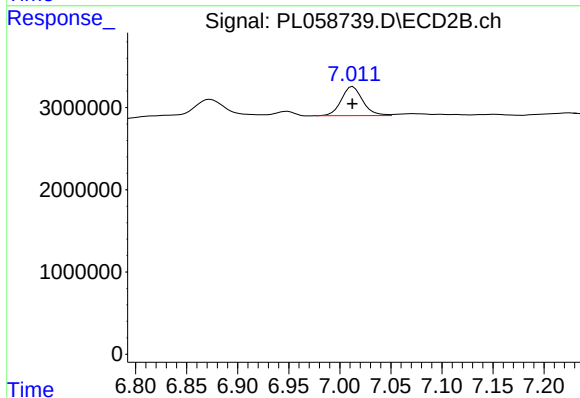


#15 Endosulfan II

R.T.: 7.013 min
Delta R.T.: 0.000 min
Response: 5163318
Conc: 2.59 ng/ml

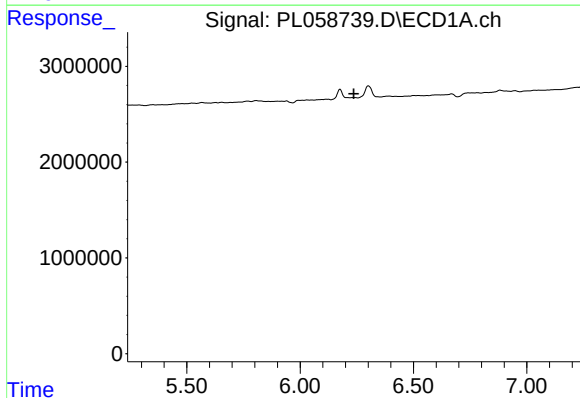


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.237 min
Response: 0
Conc: N.D.

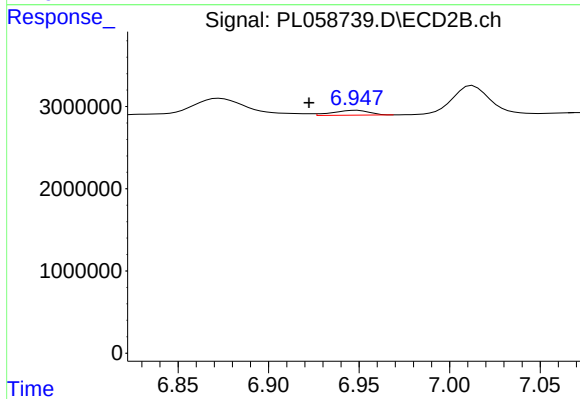

#16 4,4'-DDD


R.T.: 6.948 min
Delta R.T.: 0.026 min
Response: 844708
Conc: 0.48 ng/ml

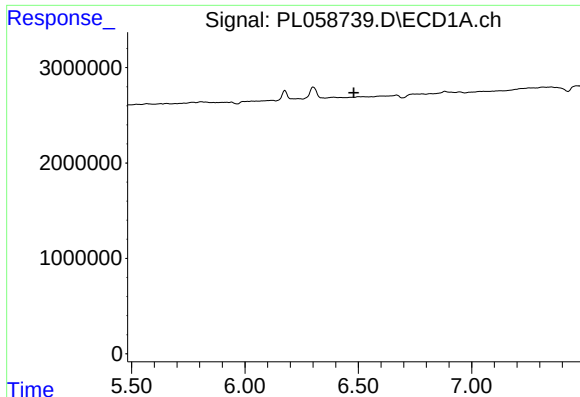

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.480 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

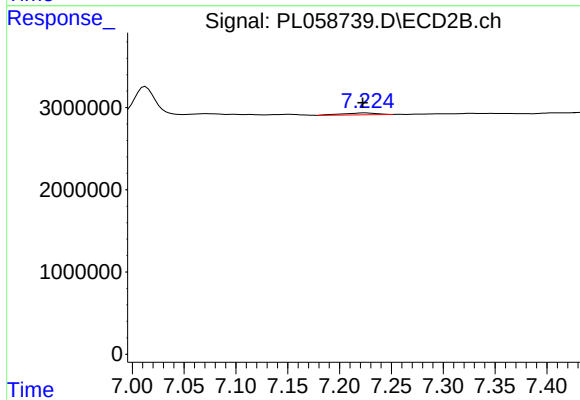


#17 4,4'-DDT

R.T.: 7.226 min
Delta R.T.: 0.003 min
Response: 521460
Conc: 0.31 ng/ml

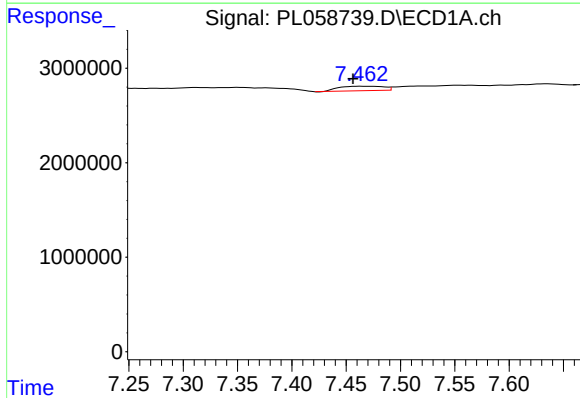


#22 Mirex

R.T.: 7.463 min
Delta R.T.: 0.007 min
Response: 1365544
Conc: 1.12 ng/ml

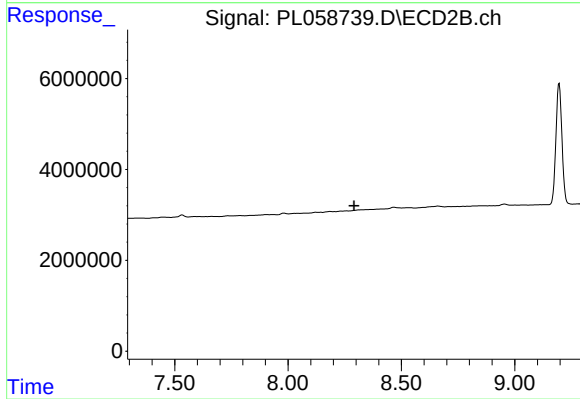

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

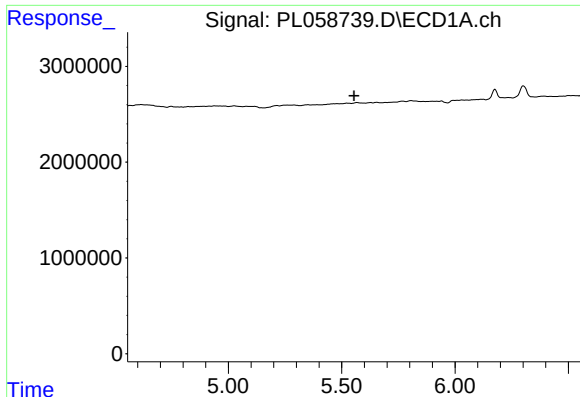

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.555 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

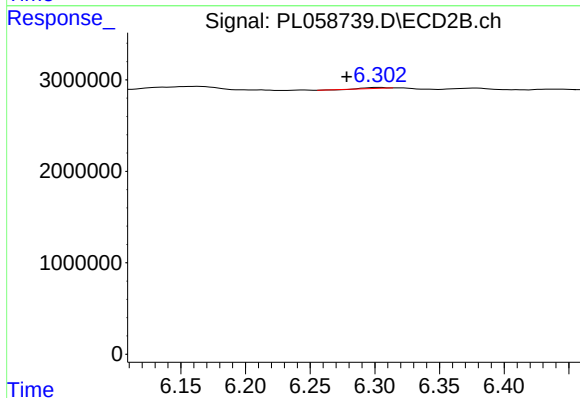


#26 Chlordane-4

R.T.: 6.303 min
Delta R.T.: 0.025 min
Response: 82984
Conc: 0.23 ng/ml

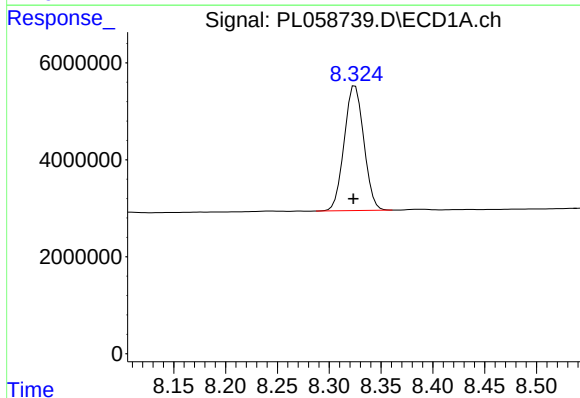

#28 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: 0.002 min
Response: 33954654
Conc: 26.00 ng/ml

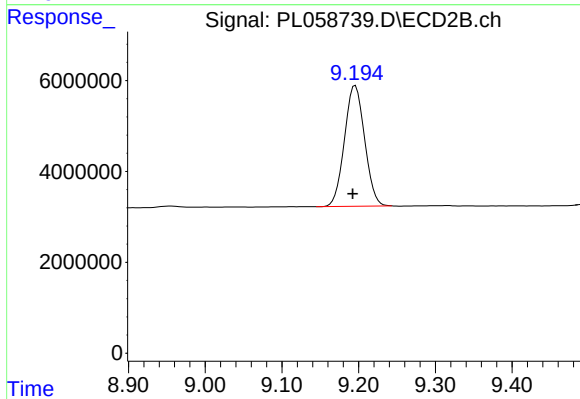

#28 Decachlorobiphenyl

R.T.: 9.196 min
Delta R.T.: 0.003 min
Response: 48735120
Conc: 27.58 ng/ml