

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051520\
 Data File : PL058757.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2020 18:09
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 22:52:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Fri May 15 06:18:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.531	4.078	33474886	49524572	20.376	22.879
28)	SA Decachlor...	8.318	9.193	29884427	44215812	22.887	25.019
Target Compounds							
7)	B delta-BHC	0.000	5.119f	0	1553769	N.D.	0.548 #
8)	B Heptachlo...	0.000	5.961	0	444546	N.D.	0.185 #
10)	B gamma-Chl...	0.000	6.173f	0	581323	N.D.	0.247 #
14)	MA Endrin	0.000	6.829f	0	4102594	N.D.	2.262 #
15)	B Endosulfa...	0.000	7.014	0	1412222	N.D.	0.707 #
25)	Chlordane-3	0.000	6.173f	0	581323	N.D.	1.919 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051520\
Data File : PL058757.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2020 18:09
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 22:52:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Fri May 15 06:18:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

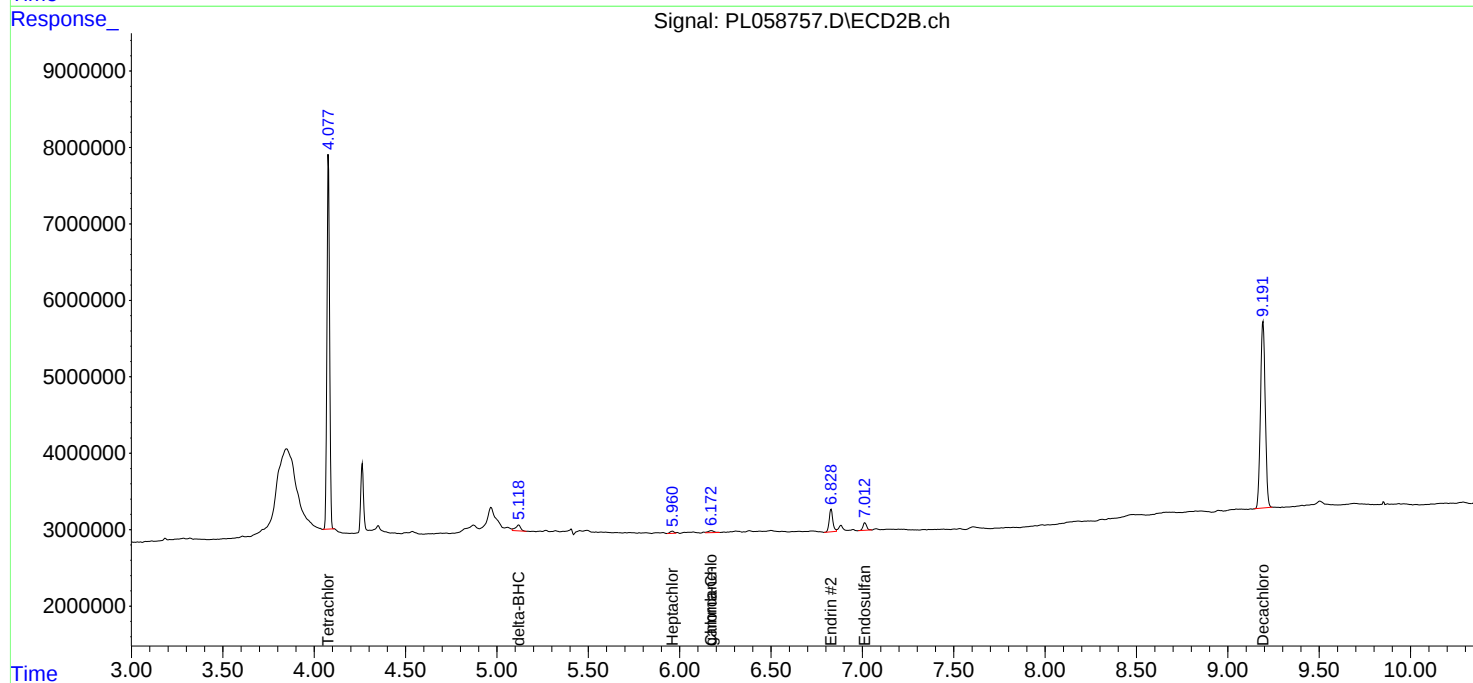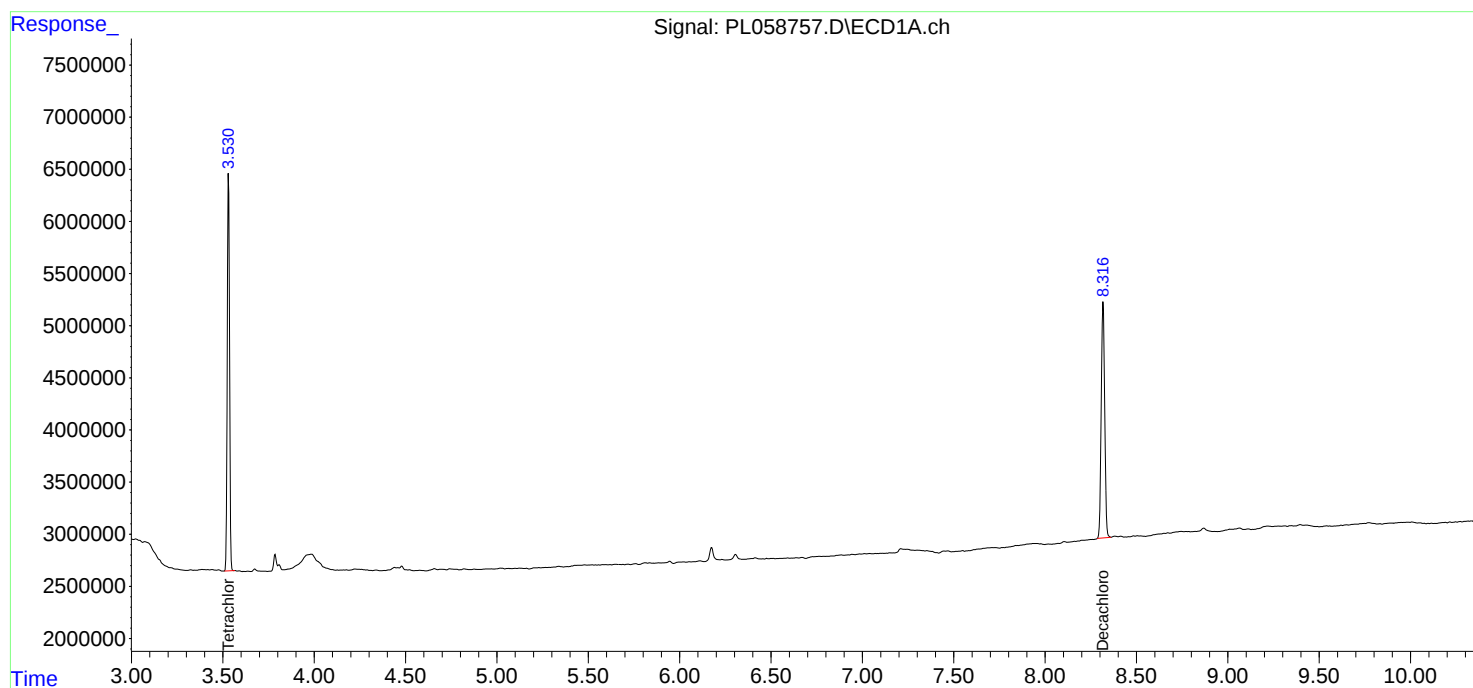


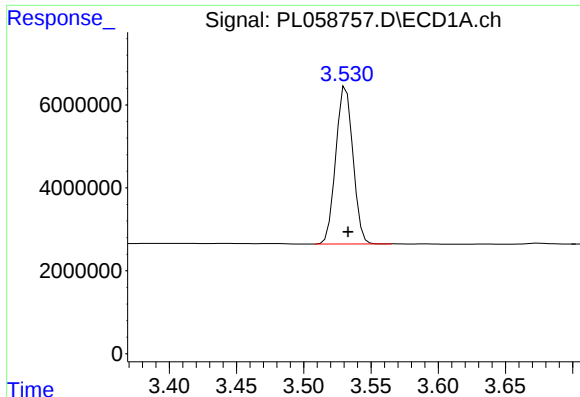

#1 Tetrachloro-m-xylene


R.T.: 3.531 min
Delta R.T.: -0.002 min
Response: 33474886
Conc: 20.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

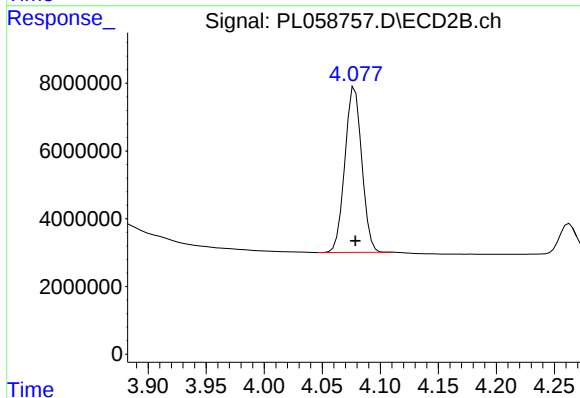


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 49524572
Conc: 22.88 ng/ml

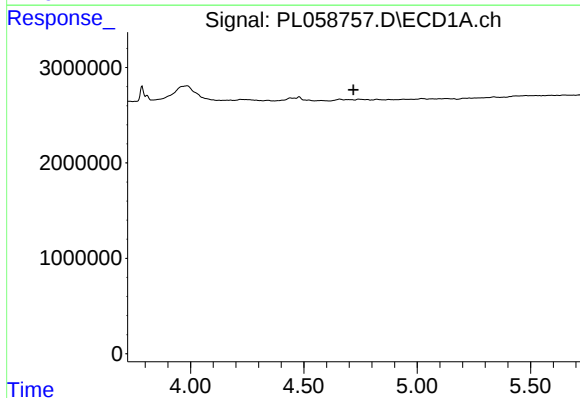


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.719 min
Response: 0
Conc: N.D.

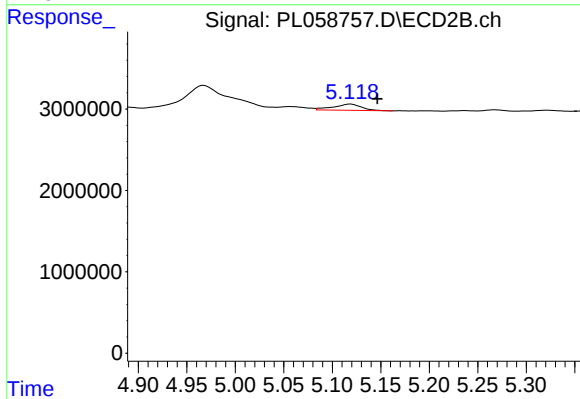

#7 delta-BHC


R.T.: 5.119 min
Delta R.T.: -0.027 min
Response: 1553769
Conc: 0.55 ng/ml

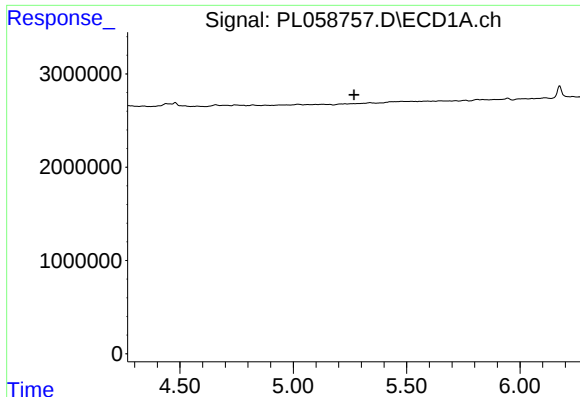

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

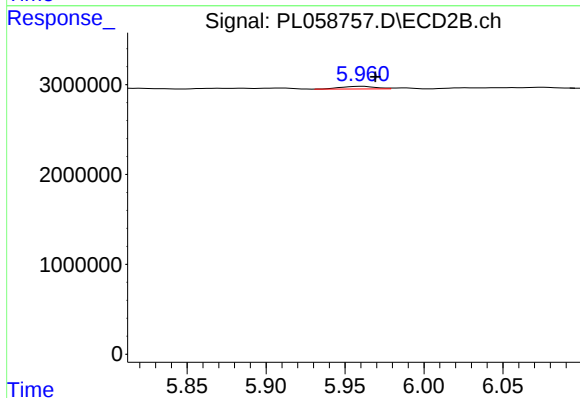


#8 Heptachlor epoxide

R.T.: 5.961 min
Delta R.T.: -0.008 min
Response: 444546
Conc: 0.19 ng/ml

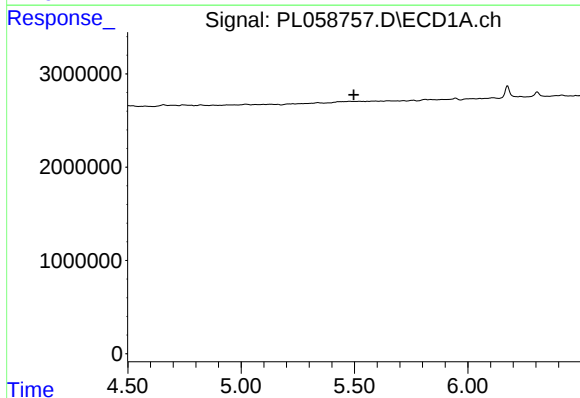


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

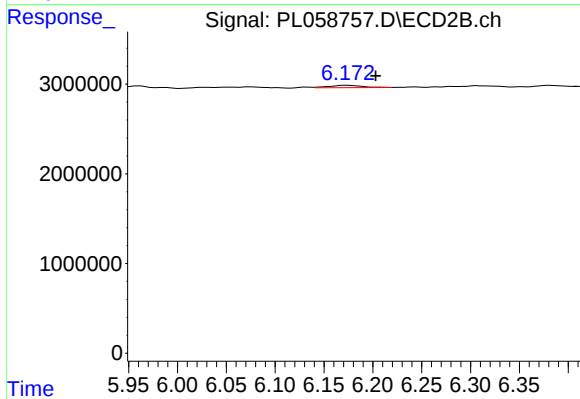

#10 gamma-Chlordane


R.T.: 6.173 min
Delta R.T.: -0.030 min
Response: 581323
Conc: 0.25 ng/ml

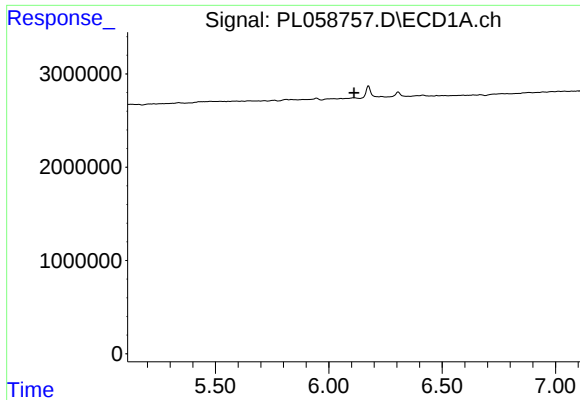

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

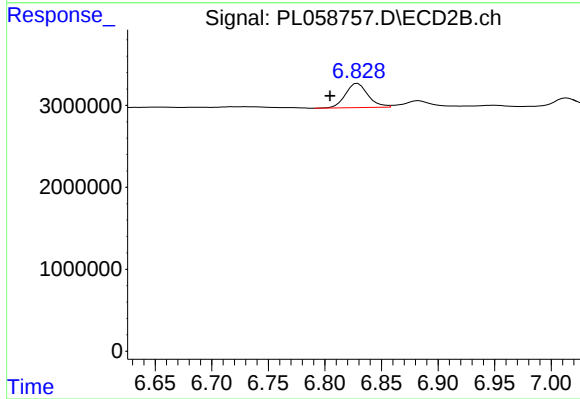


#14 Endrin

R.T.: 6.829 min
Delta R.T.: 0.024 min
Response: 4102594
Conc: 2.26 ng/ml

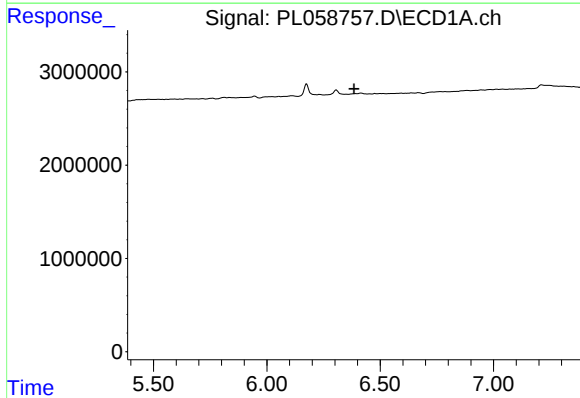


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.385 min
Response: 0
Conc: N.D.

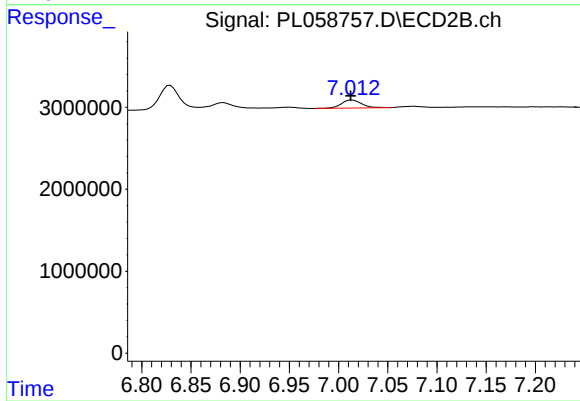

#15 Endosulfan II


R.T.: 7.014 min
Delta R.T.: 0.001 min
Response: 1412222
Conc: 0.71 ng/ml

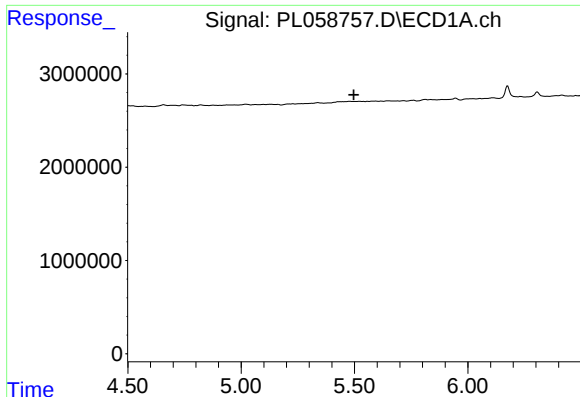

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

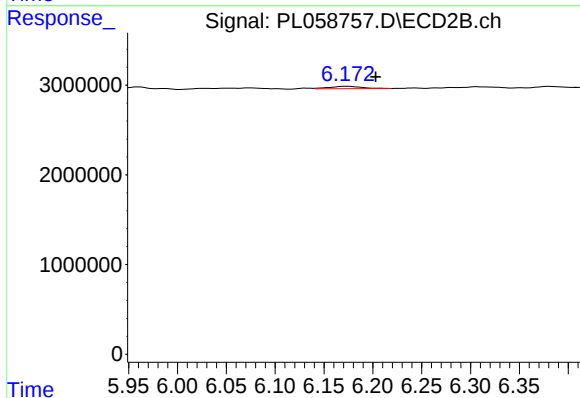


#25 Chlordane-3

R.T.: 6.173 min
Delta R.T.: -0.030 min
Response: 581323
Conc: 1.92 ng/ml

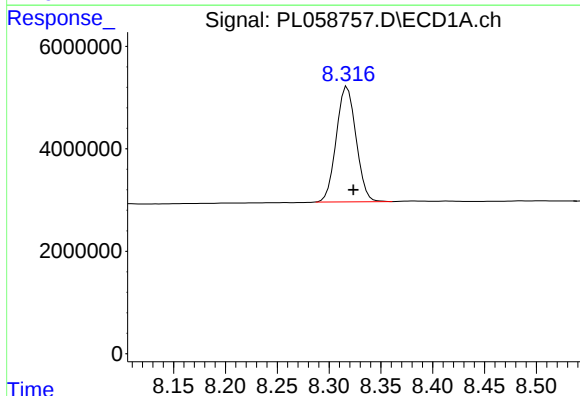

#28 Decachlorobiphenyl

R.T.: 8.318 min
Delta R.T.: -0.006 min
Response: 29884427
Conc: 22.89 ng/ml

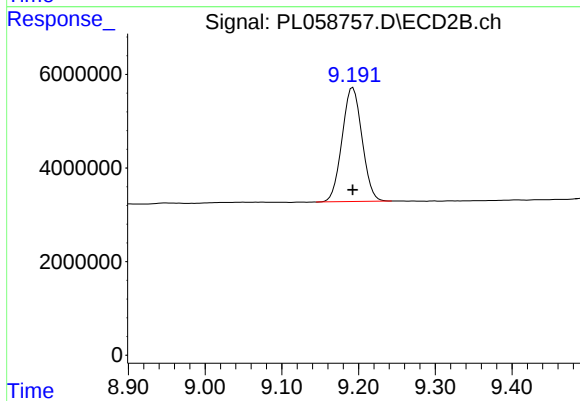

#28 Decachlorobiphenyl

R.T.: 9.193 min
Delta R.T.: 0.000 min
Response: 44215812
Conc: 25.02 ng/ml