

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051523\
 Data File : PL082716.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2023 13:35
 Operator : AR\AJ
 Sample : 02770-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-25990

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 21:59:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	2.644	18361396	16773498	6.874	7.240
28)	SA Decachlor...	8.742	7.752	26595137	27859460	13.931	12.206
Target Compounds							
11)	B alpha-Chl...	5.779	4.885	5376381	2094900	1.801	0.722 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051523\
Data File : PL082716.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2023 13:35
Operator : AR\AJ
Sample : 02770-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CHRT-25990

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 21:59:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

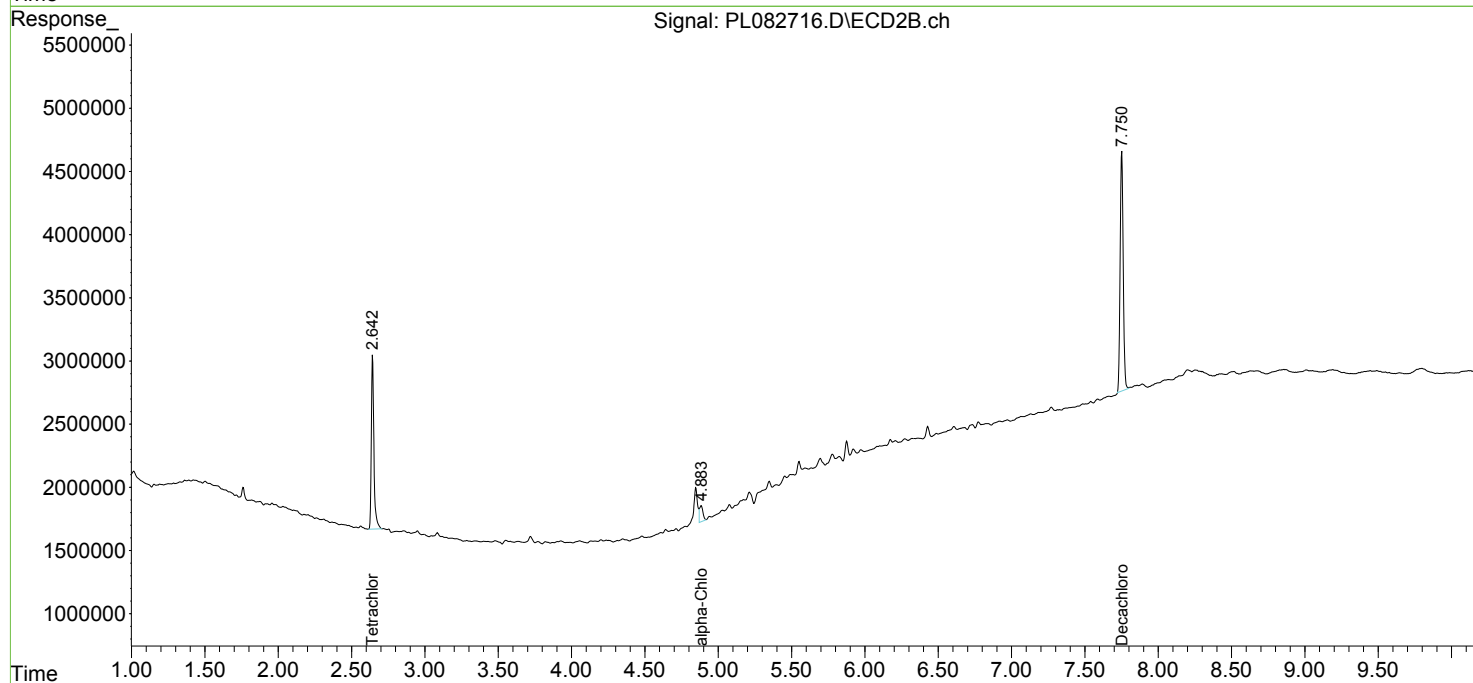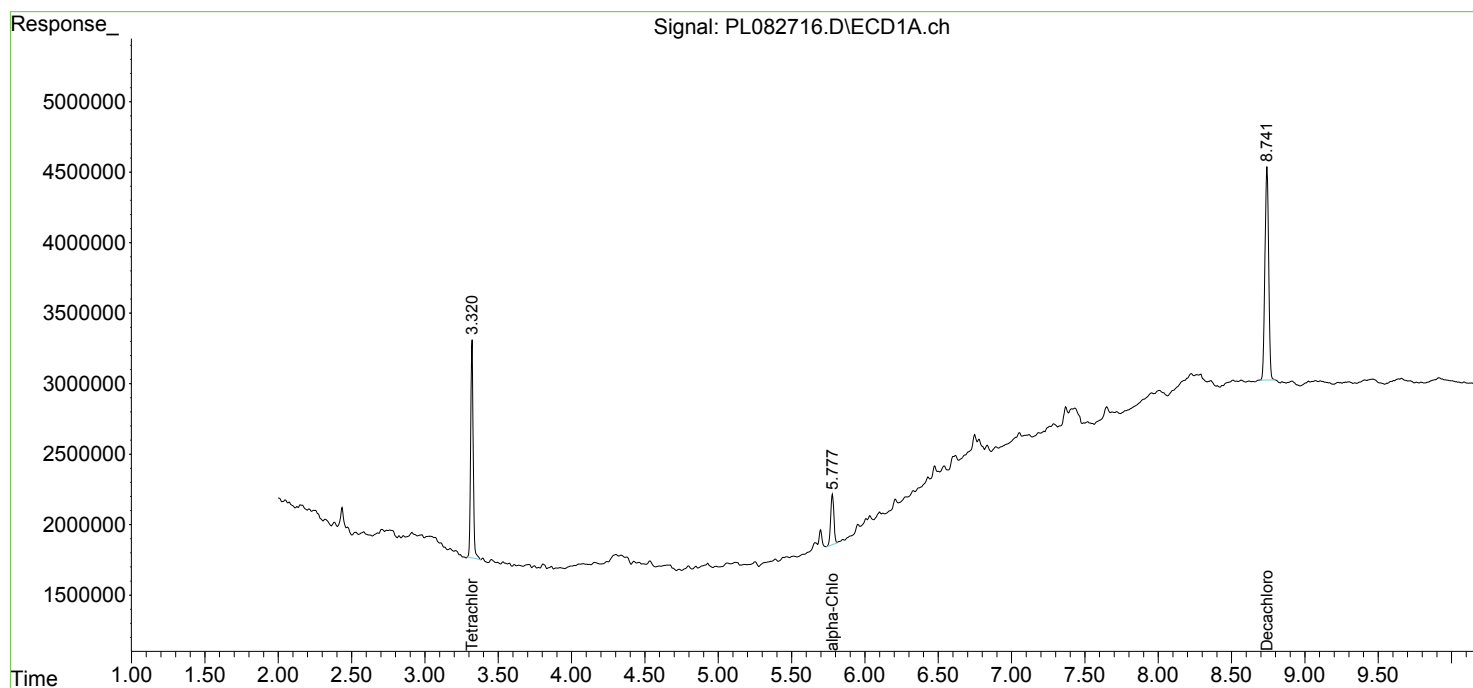


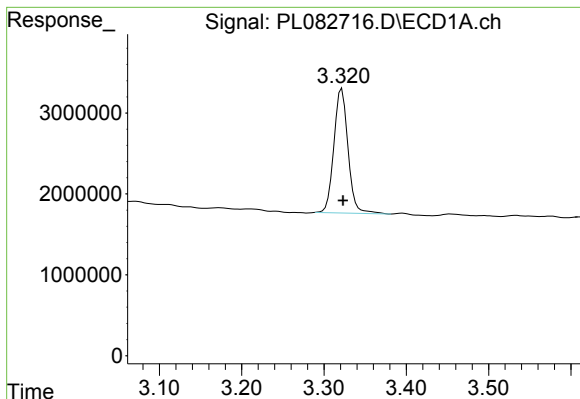

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: -0.001 min
Response: 18361396
Conc: 6.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-25990

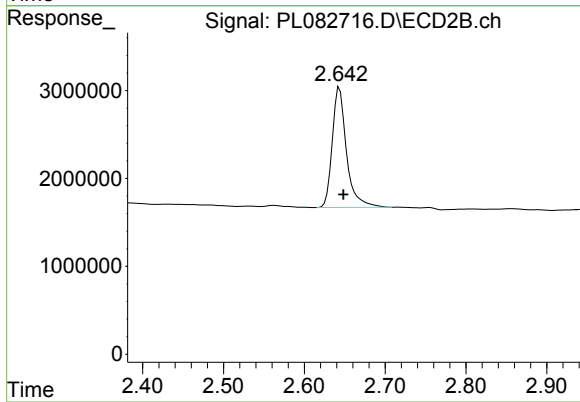


#1 Tetrachloro-m-xylene

R.T.: 2.644 min
Delta R.T.: -0.005 min
Response: 16773498
Conc: 7.24 ng/ml

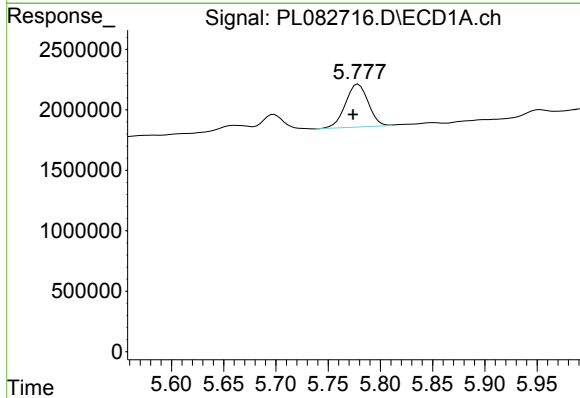


#11 alpha-Chlordane

R.T.: 5.779 min
Delta R.T.: 0.005 min
Response: 5376381
Conc: 1.80 ng/ml

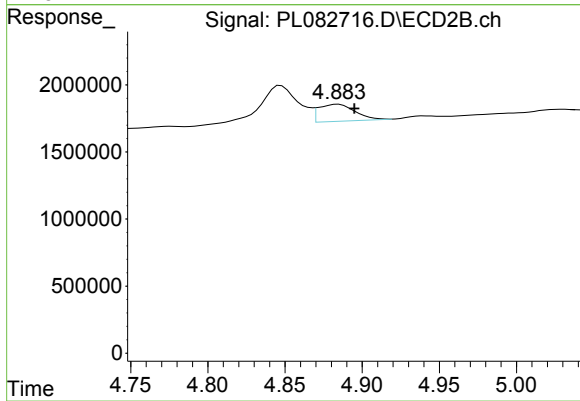

#11 alpha-Chlordane


R.T.: 4.885 min
Delta R.T.: -0.010 min
Response: 2094900
Conc: 0.72 ng/ml

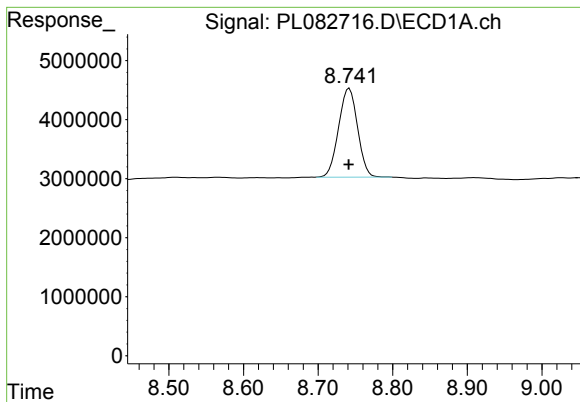

#28 Decachlorobiphenyl

R.T.: 8.742 min
Delta R.T.: 0.000 min
Response: 26595137
Conc: 13.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-25990

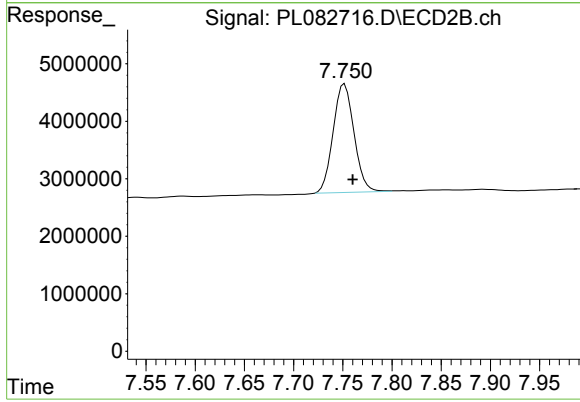

#28 Decachlorobiphenyl

R.T.: 7.752 min
Delta R.T.: -0.008 min
Response: 27859460
Conc: 12.21 ng/ml