

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051525\
 Data File : PL095684.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2025 08:06
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 14:14:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
 Quant Title : GC Extractables
 QLast Update : Tue May 13 14:38:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) B	Heptachlo...	5.733	0.000	25667113	0	4.953	N.D.	#
13) MA	Dieldrin	0.000	5.558f	0	11328548	N.D.	1.841	#
15) B	Endosulfa...	6.812f	0.000	8182079	0	1.963	N.D.	#
16) A	4,4'-DDD	6.742	0.000	22053348	0	5.676	N.D.	#
24)	Chlordane-2	0.000	4.501	0	9239587	N.D.	34.718	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051525\
Data File : PL095684.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2025 08:06
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 14:14:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
Quant Title : GC Extractables
QLast Update : Tue May 13 14:38:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

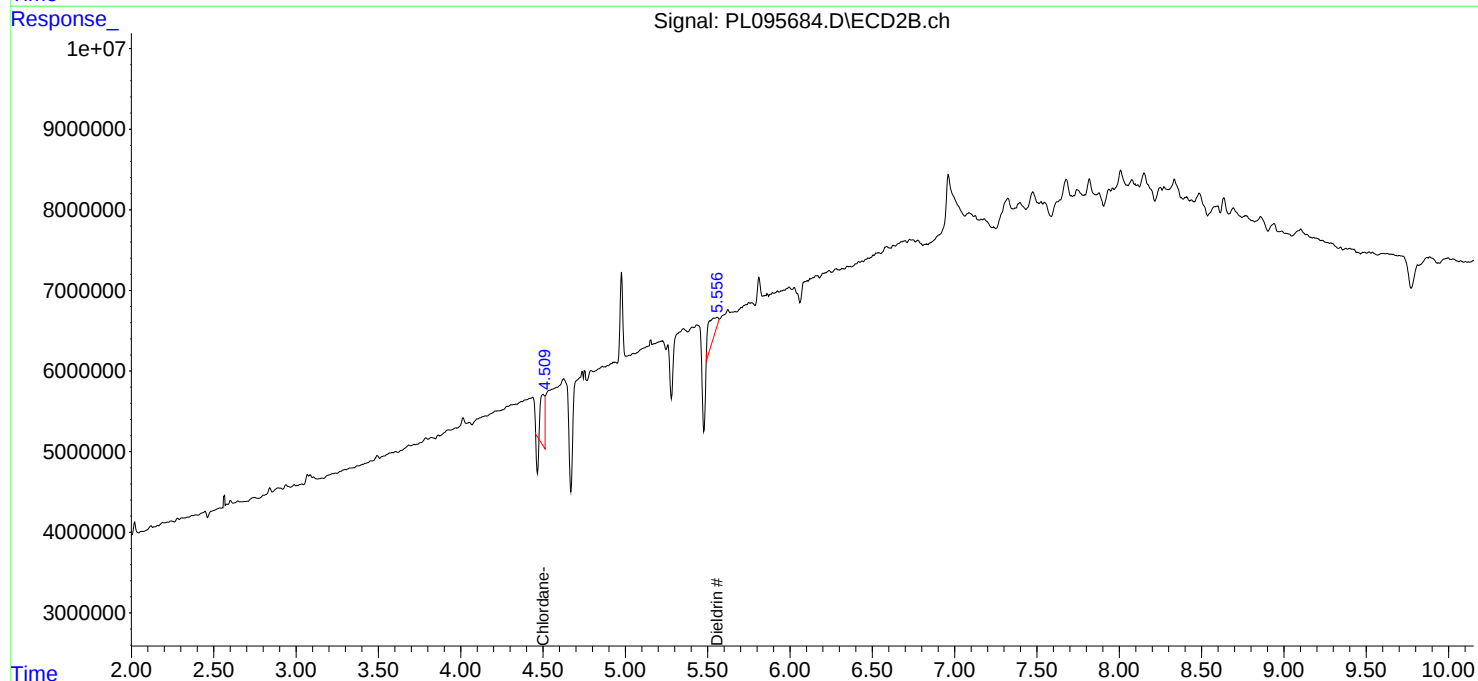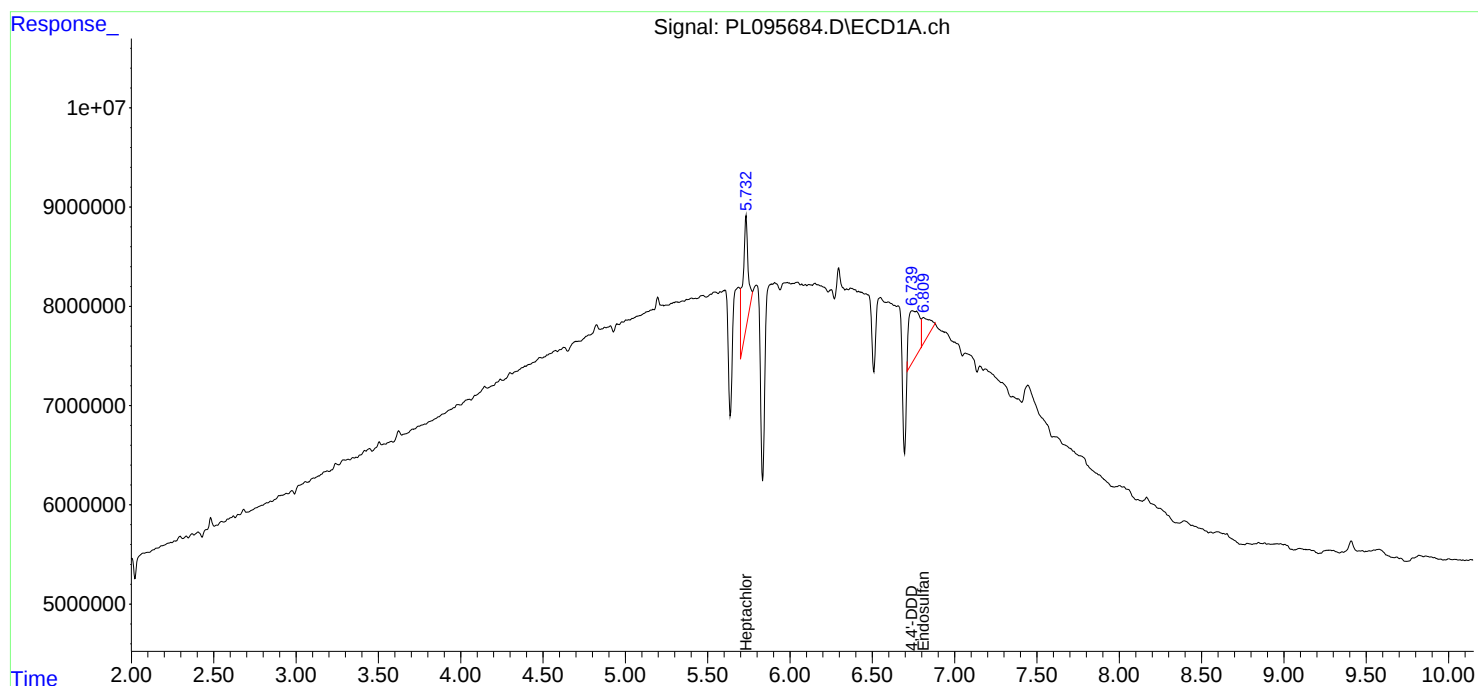


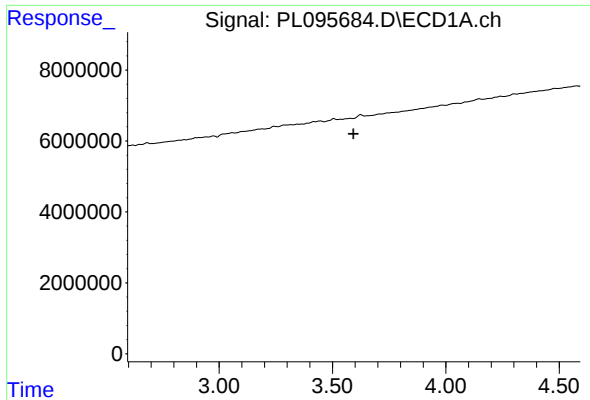

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.593 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

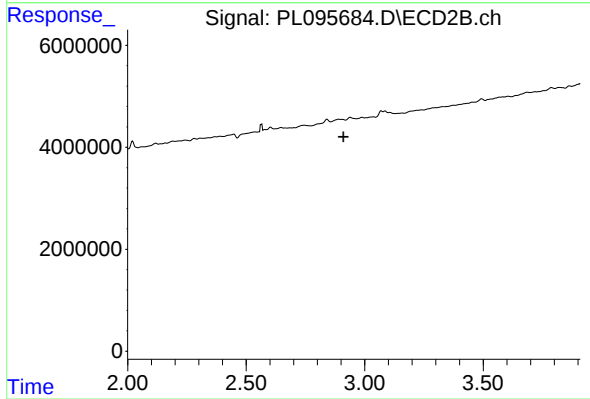


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.910 min
Response: 0
Conc: N.D.

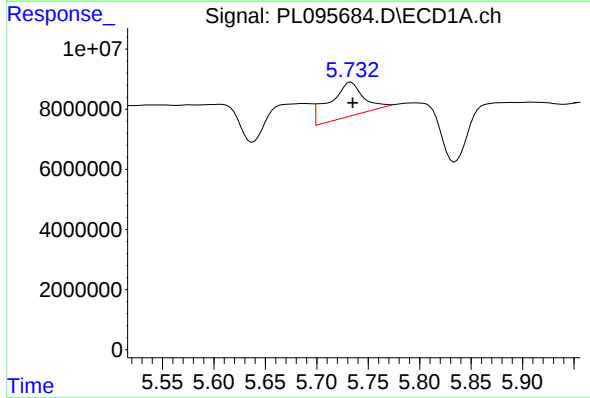


#8 Heptachlor epoxide

R.T.: 5.733 min
Delta R.T.: -0.001 min
Response: 25667113
Conc: 4.95 ng/ml

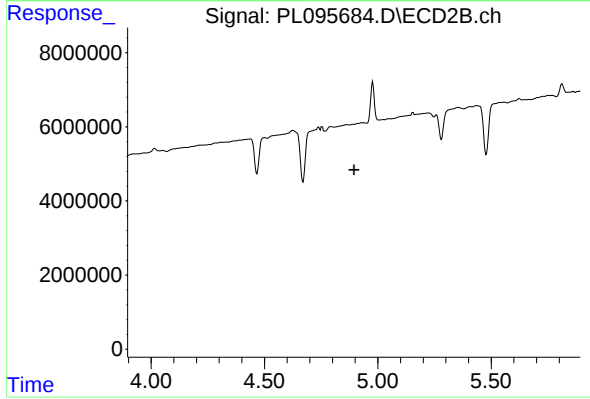

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.895 min
Response: 0
Conc: N.D.

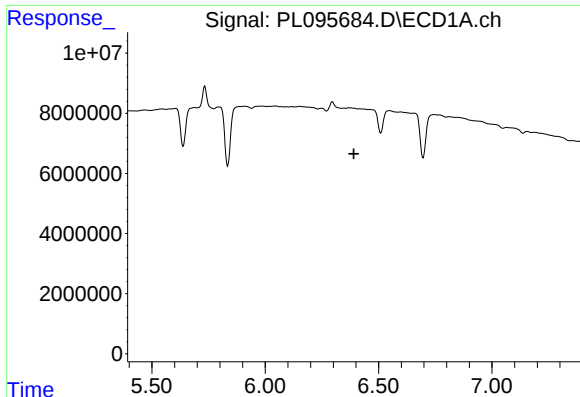

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

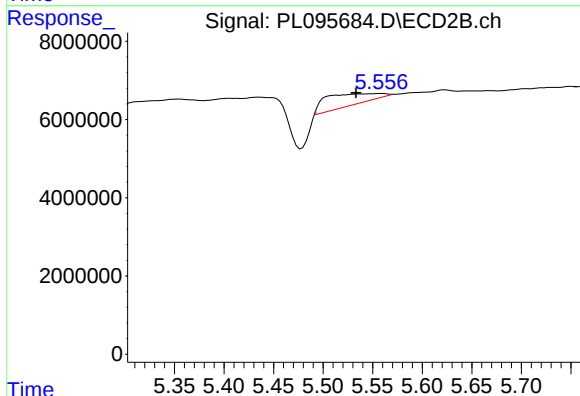


#13 Dieldrin

R.T.: 5.558 min
Delta R.T.: 0.025 min
Response: 11328548
Conc: 1.84 ng/ml

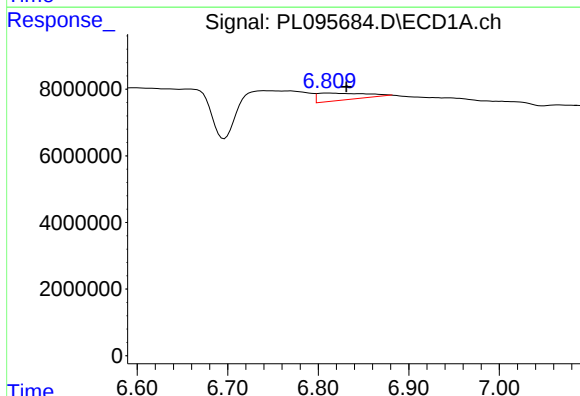


#15 Endosulfan II

R.T.: 6.812 min
Delta R.T.: -0.020 min
Response: 8182079
Conc: 1.96 ng/ml

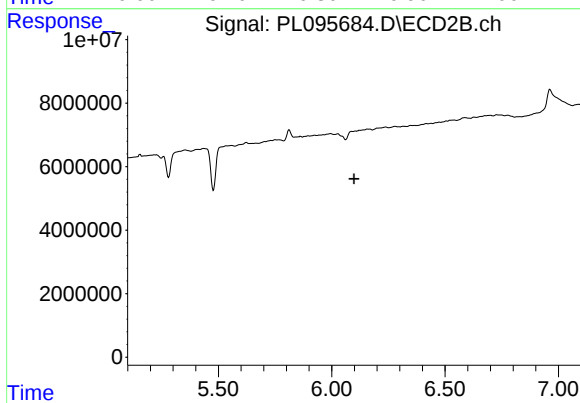

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.098 min
Response: 0
Conc: N.D.

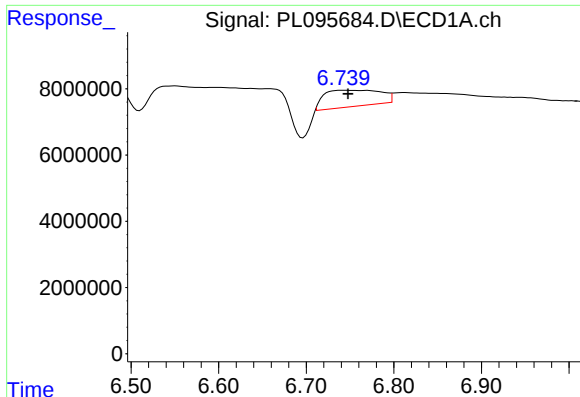

#16 4,4'-DDD


R.T.: 6.742 min
Delta R.T.: -0.005 min
Response: 22053348
Conc: 5.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

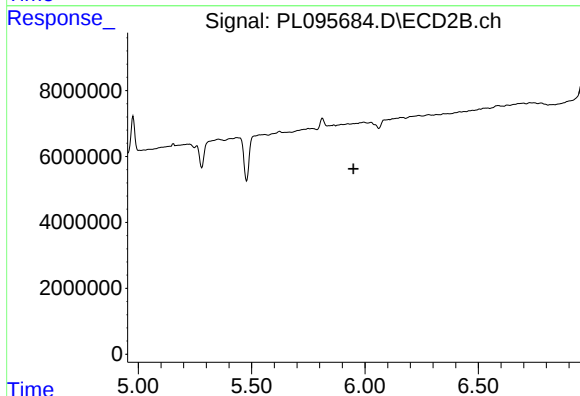


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

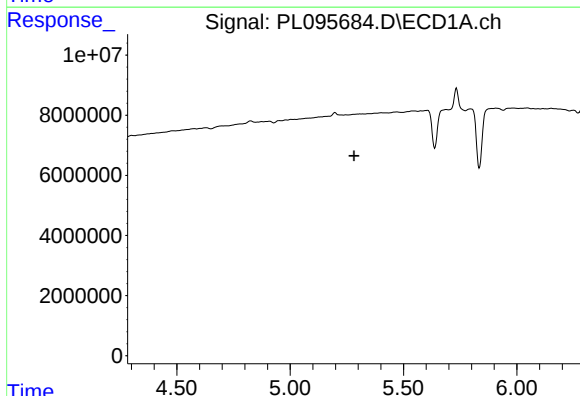


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.282 min
Response: 0
Conc: N.D.

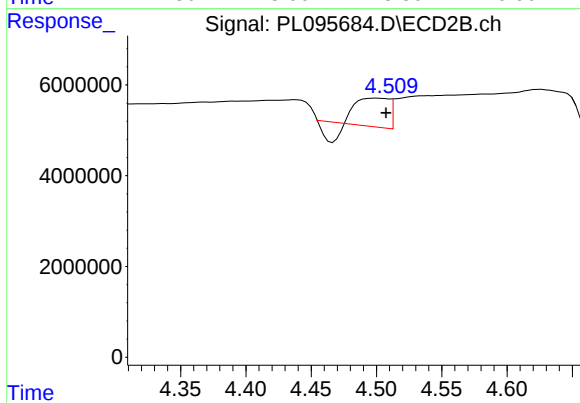

#24 Chlordane-2


R.T.: 4.501 min
Delta R.T.: -0.007 min
Response: 9239587
Conc: 34.72 ng/ml

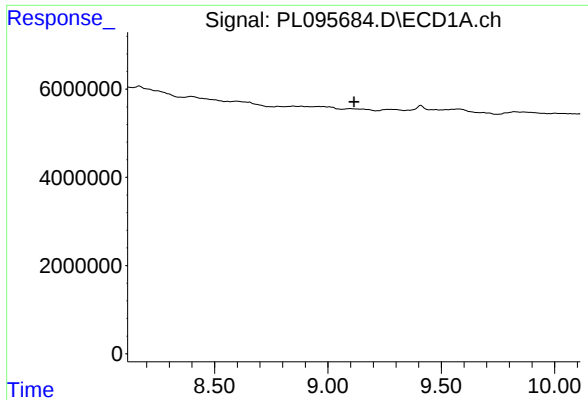

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.115 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

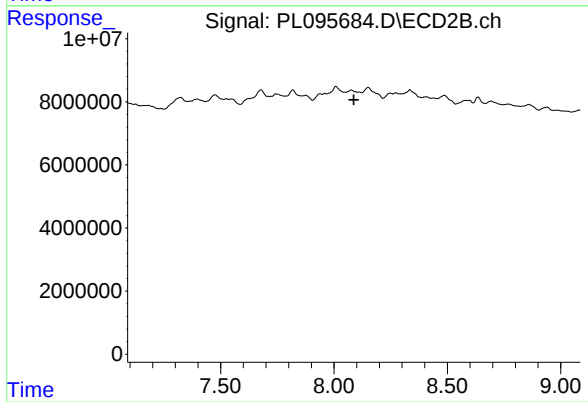

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.087 min
Response: 0
Conc: N.D.