

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051525\
 Data File : PL095695.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2025 16:42
 Operator : AR\AJ
 Sample : Q2034-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 L3-WC-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 04:04:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
 Quant Title : GC Extractables
 QLast Update : Tue May 13 14:38:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.591	2.906	88380049	70537291	21.630	15.059 #
28)	SA Decachlor...	9.113	8.082	32941920	41110901	9.710	9.967
Target Compounds							
7)	B delta-BHC	4.792f	0.000	5569609	0	1.025	N.D. #
9)	A Endosulfan I	0.000	5.282	0	8990603	N.D.	1.738 #
12)	B 4,4'-DDE	6.252	0.000	4960078	0	0.969	N.D. #
13)	MA Dieldrin	0.000	5.526	0	13589390	N.D.	2.209 #
15)	B Endosulfa...	6.808f	6.089	19442065	2870957	4.665	0.524 #
16)	A 4,4'-DDD	6.760	0.000	6638280	0	1.708	N.D. #
19)	B Endosulfa...	0.000	6.483f	0	4332941	N.D.	0.872 #
20)	A Methoxychlor	0.000	6.798f	0	6171118	N.D.	2.281 #
23)	Chlordane-1	0.000	3.926	0	7476353	N.D.	31.065 #
27)	Chlordane-5	0.000	6.089	0	2870957	N.D.	9.995 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051525\
Data File : PL095695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2025 16:42
Operator : AR\AJ
Sample : Q2034-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
L3-WC-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 04:04:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
Quant Title : GC Extractables
QLast Update : Tue May 13 14:38:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

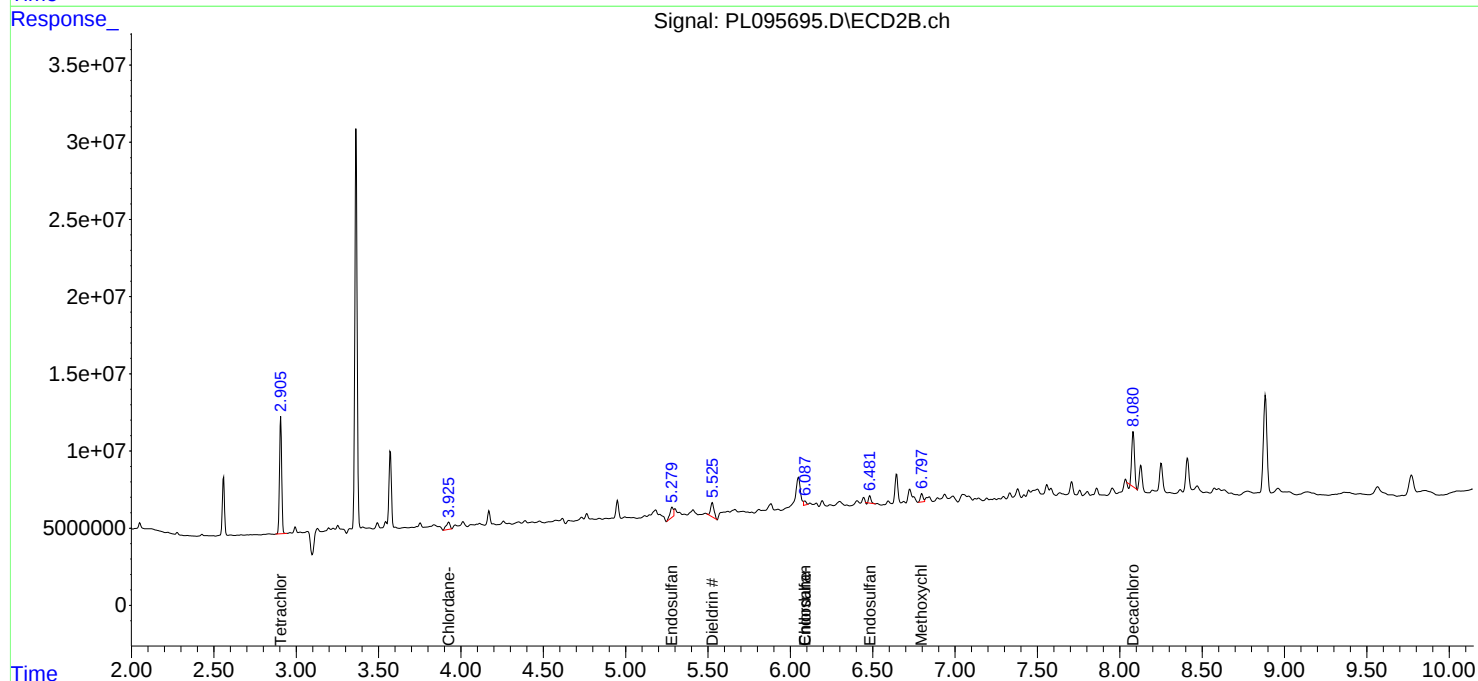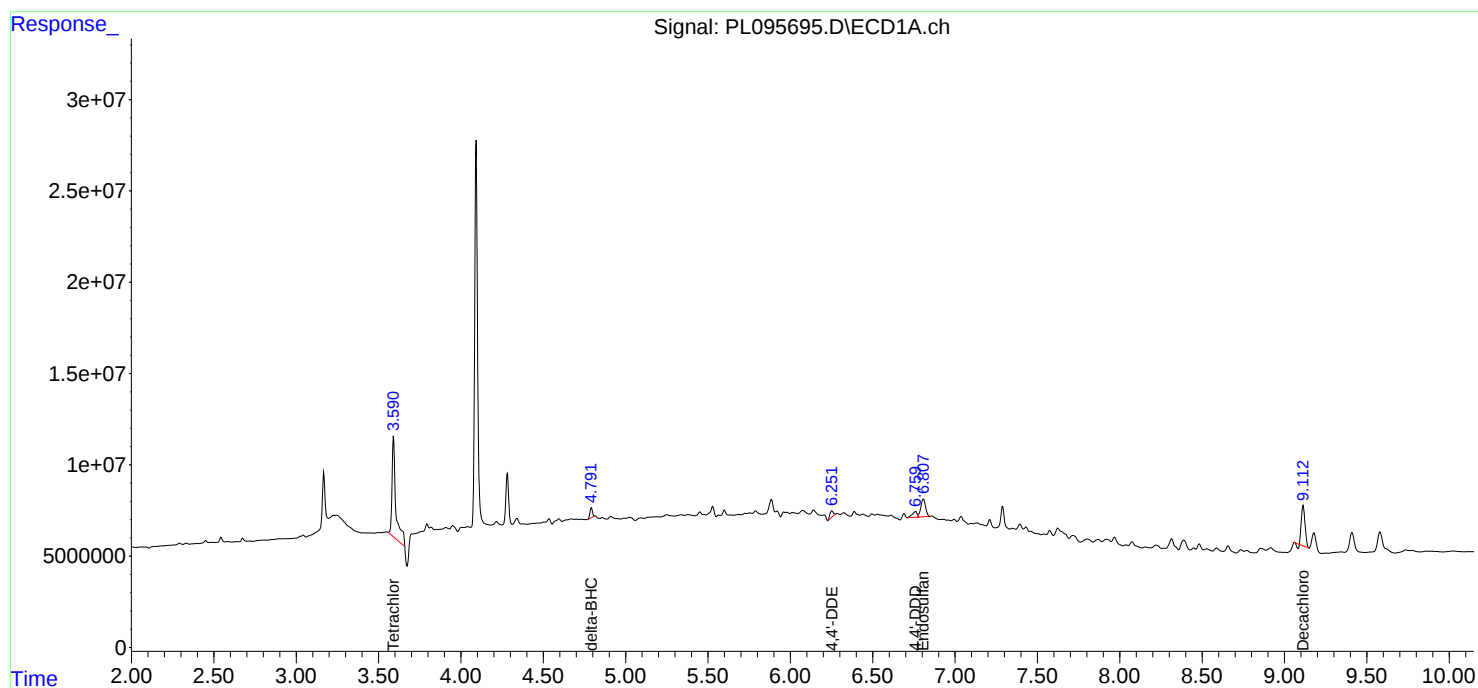


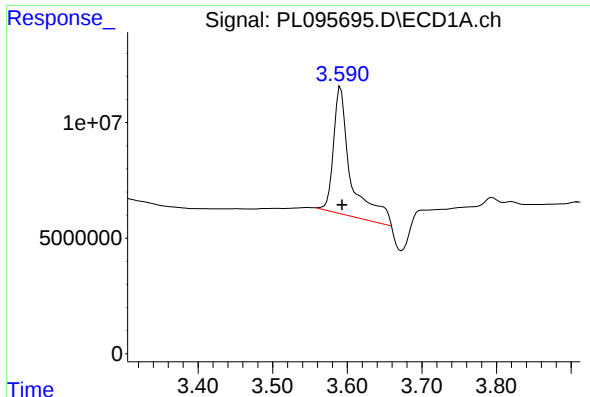

#1 Tetrachloro-m-xylene


R.T.: 3.591 min
Delta R.T.: -0.002 min
Response: 88380049
Conc: 21.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
L3-WC-2

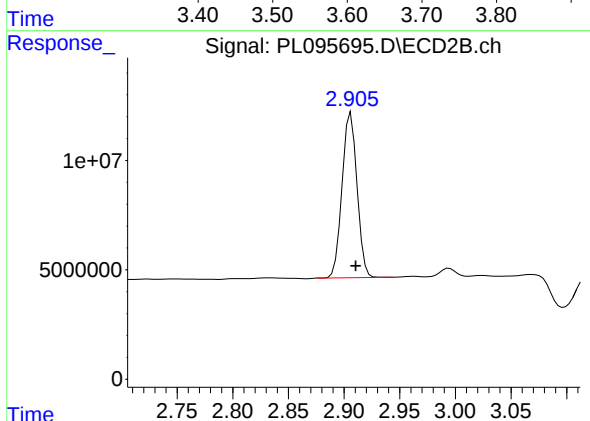


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: -0.004 min
Response: 70537291
Conc: 15.06 ng/ml

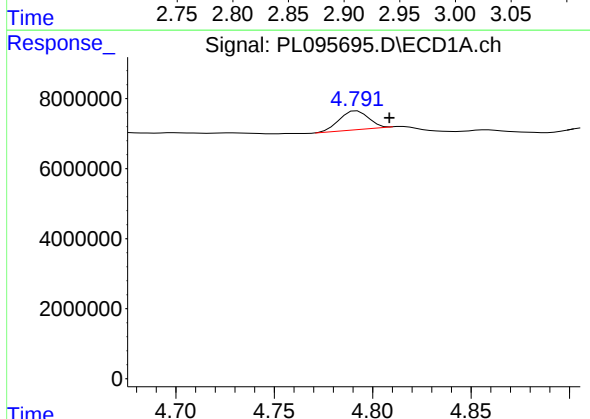


#7 delta-BHC

R.T.: 4.792 min
Delta R.T.: -0.016 min
Response: 5569609
Conc: 1.03 ng/ml

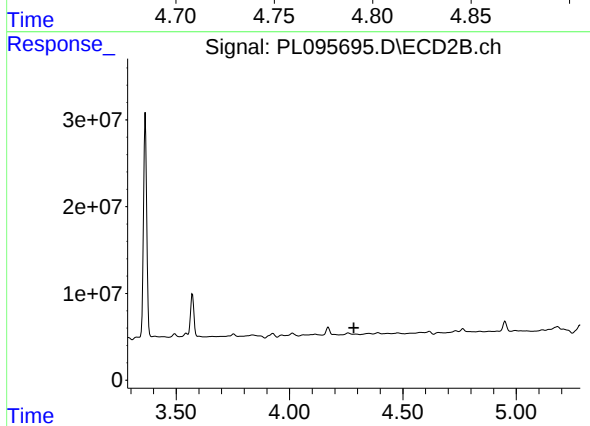

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.283 min
Response: 0
Conc: N.D.

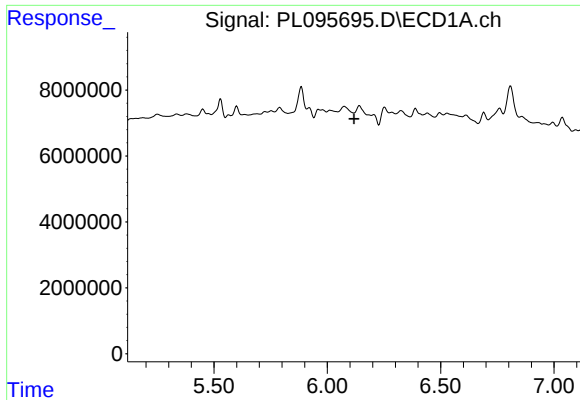

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
L3-WC-2

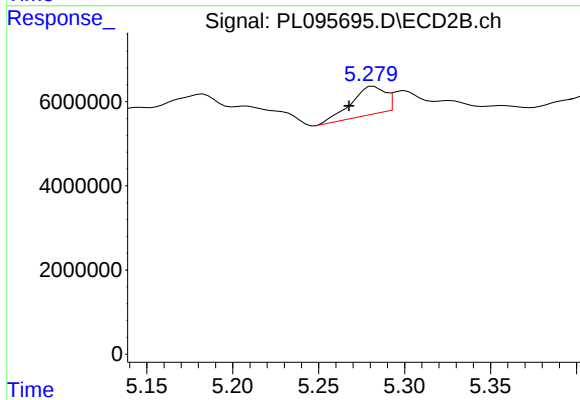


#9 Endosulfan I

R.T.: 5.282 min
Delta R.T.: 0.014 min
Response: 8990603
Conc: 1.74 ng/ml

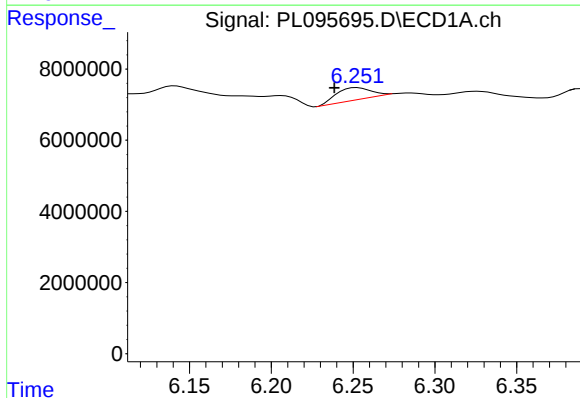


#12 4,4'-DDE

R.T.: 6.252 min
Delta R.T.: 0.014 min
Response: 4960078
Conc: 0.97 ng/ml

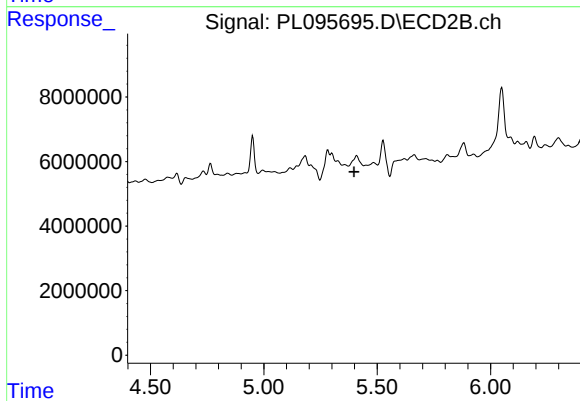

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.398 min
Response: 0
Conc: N.D.

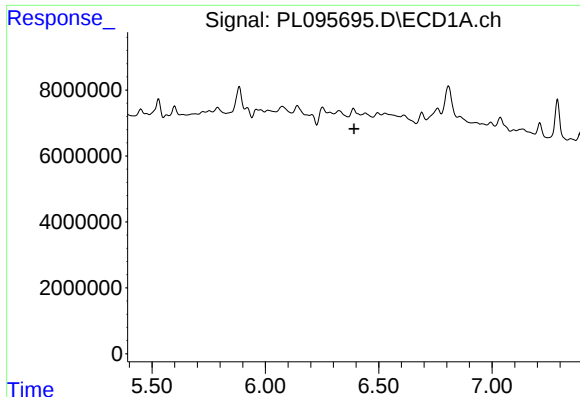

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
L3-WC-2

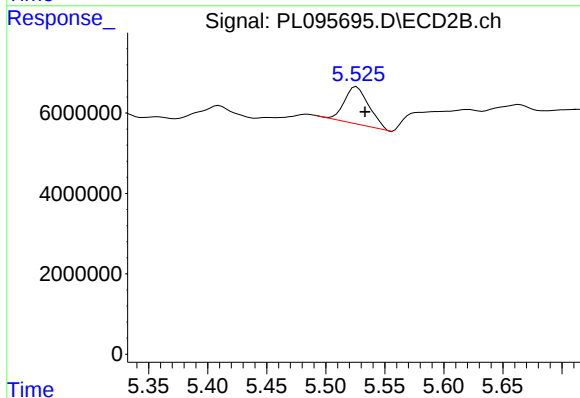


#13 Dieldrin

R.T.: 5.526 min
Delta R.T.: -0.007 min
Response: 13589390
Conc: 2.21 ng/ml

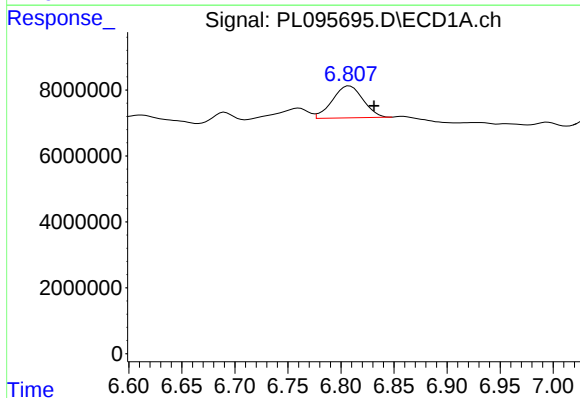


#15 Endosulfan II

R.T.: 6.808 min
Delta R.T.: -0.023 min
Response: 19442065
Conc: 4.66 ng/ml

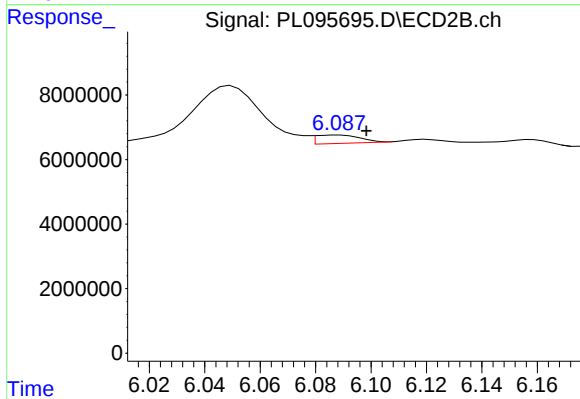

#15 Endosulfan II


R.T.: 6.089 min
Delta R.T.: -0.010 min
Response: 2870957
Conc: 0.52 ng/ml

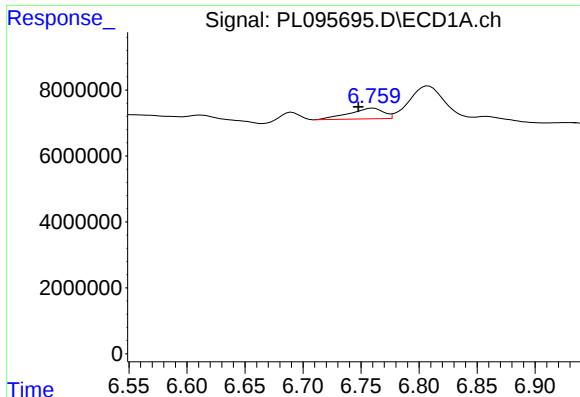

#16 4,4'-DDD


R.T.: 6.760 min
Delta R.T.: 0.013 min
Response: 6638280
Conc: 1.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
L3-WC-2

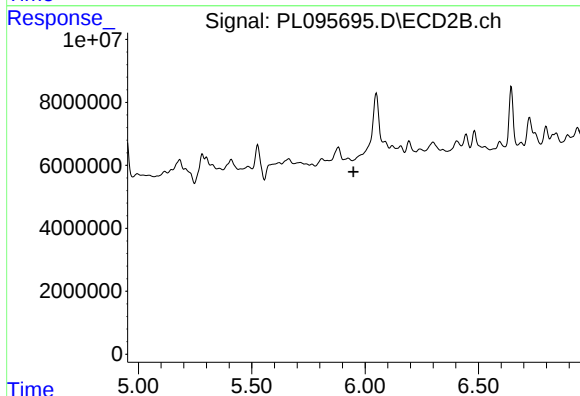


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

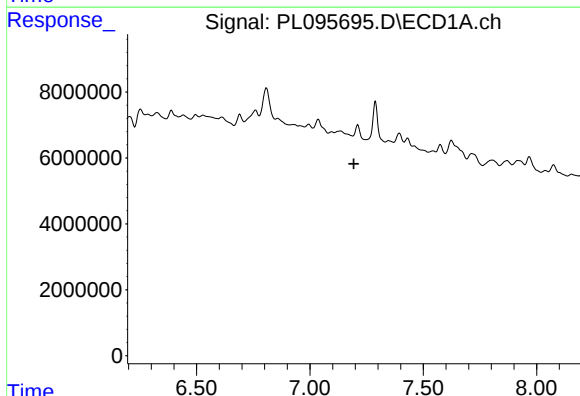


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.193 min
Response: 0
Conc: N.D.

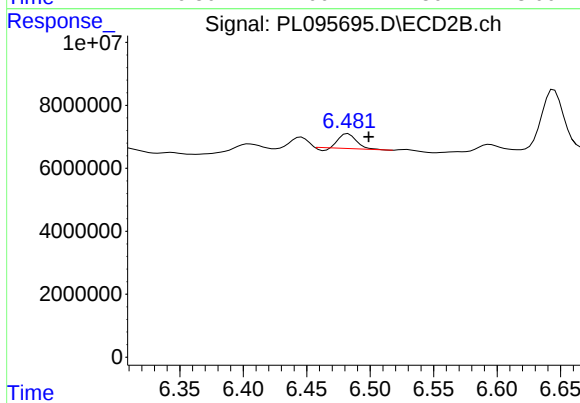

#19 Endosulfan Sulfate


R.T.: 6.483 min
Delta R.T.: -0.016 min
Response: 4332941
Conc: 0.87 ng/ml

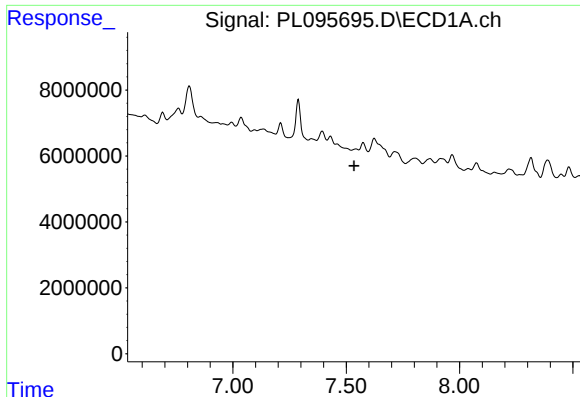

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.534 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
L3-WC-2

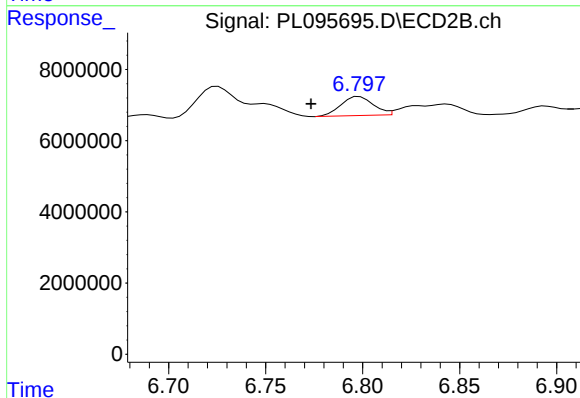


#20 Methoxychlor

R.T.: 6.798 min
Delta R.T.: 0.025 min
Response: 6171118
Conc: 2.28 ng/ml

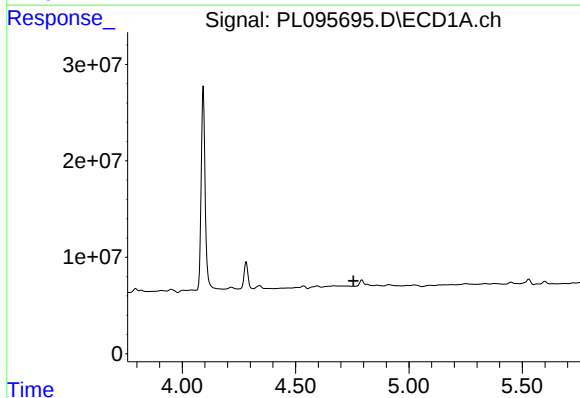


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.756 min
Response: 0
Conc: N.D.

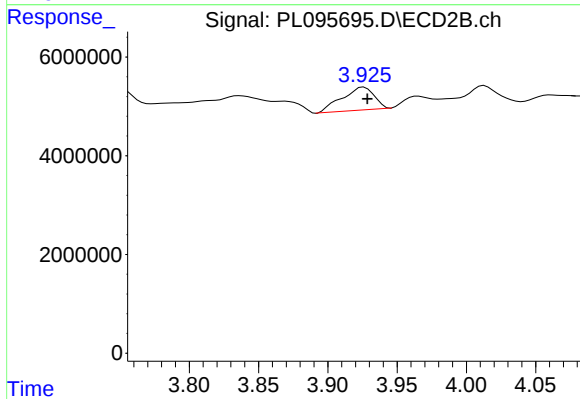

#23 Chlordane-1


R.T.: 3.926 min
Delta R.T.: -0.003 min
Response: 7476353
Conc: 31.07 ng/ml

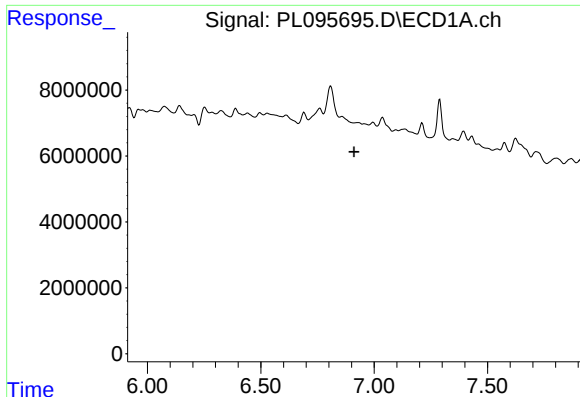

#27 Chlorine-5


R.T.: 0.000 min
Exp R.T.: 6.911 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
L3-WC-2

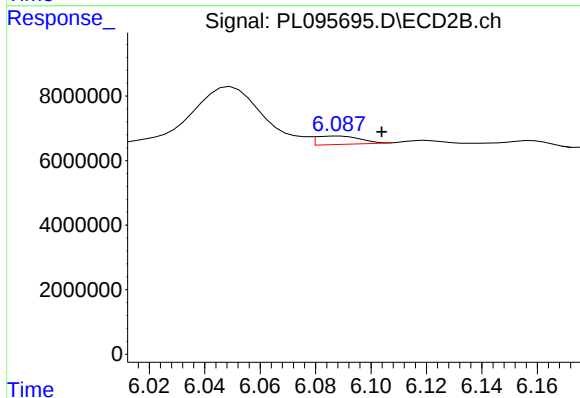


#27 Chlorine-5

R.T.: 6.089 min
Delta R.T.: -0.015 min
Response: 2870957
Conc: 10.00 ng/ml

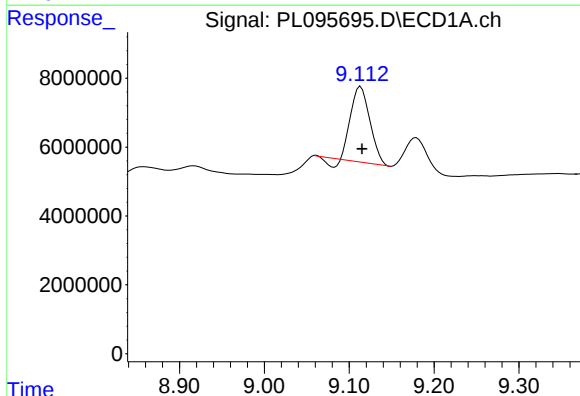

#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: -0.002 min
Response: 32941920
Conc: 9.71 ng/ml

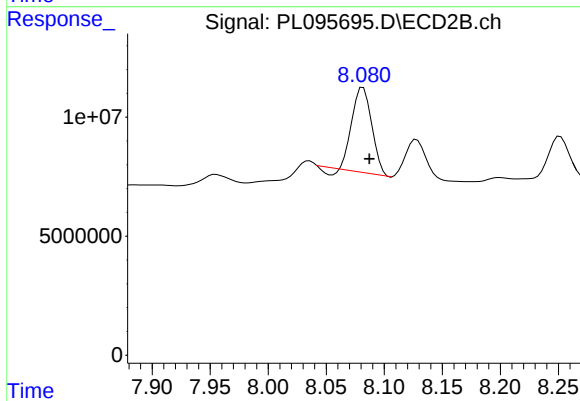

#28 Decachlorobiphenyl

R.T.: 8.082 min
Delta R.T.: -0.005 min
Response: 41110901
Conc: 9.97 ng/ml