

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051525\
 Data File : PL095703.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2025 18:33
 Operator : AR\AJ
 Sample : Q2034-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 L3-WC-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 04:05:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
 Quant Title : GC Extractables
 QLast Update : Tue May 13 14:38:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.591	2.907	107.9E6	84304210	26.406	17.998 #
28)	SA Decachlor...	9.113	8.083	58546353	70144617	17.258	17.006
Target Compounds							
10)	B gamma-Chl...	0.000	5.171f	0	8682219	N.D.	1.458 #
11)	B alpha-Chl...	6.074	0.000	9978769	0	1.920	N.D. #
15)	B Endosulfa...	6.807f	0.000	11570984	0	2.776	N.D. #
22)	Mirex	8.138f	0.000	9610400	0	3.157	N.D. #
25)	Chlordane-3	0.000	5.171f	0	8682219	N.D.	11.218 #
26)	Chlordane-4	6.074	0.000	9978769	0	8.597	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051525\
Data File : PL095703.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2025 18:33
Operator : AR\AJ
Sample : Q2034-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
L3-WC-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 04:05:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
Quant Title : GC Extractables
QLast Update : Tue May 13 14:38:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

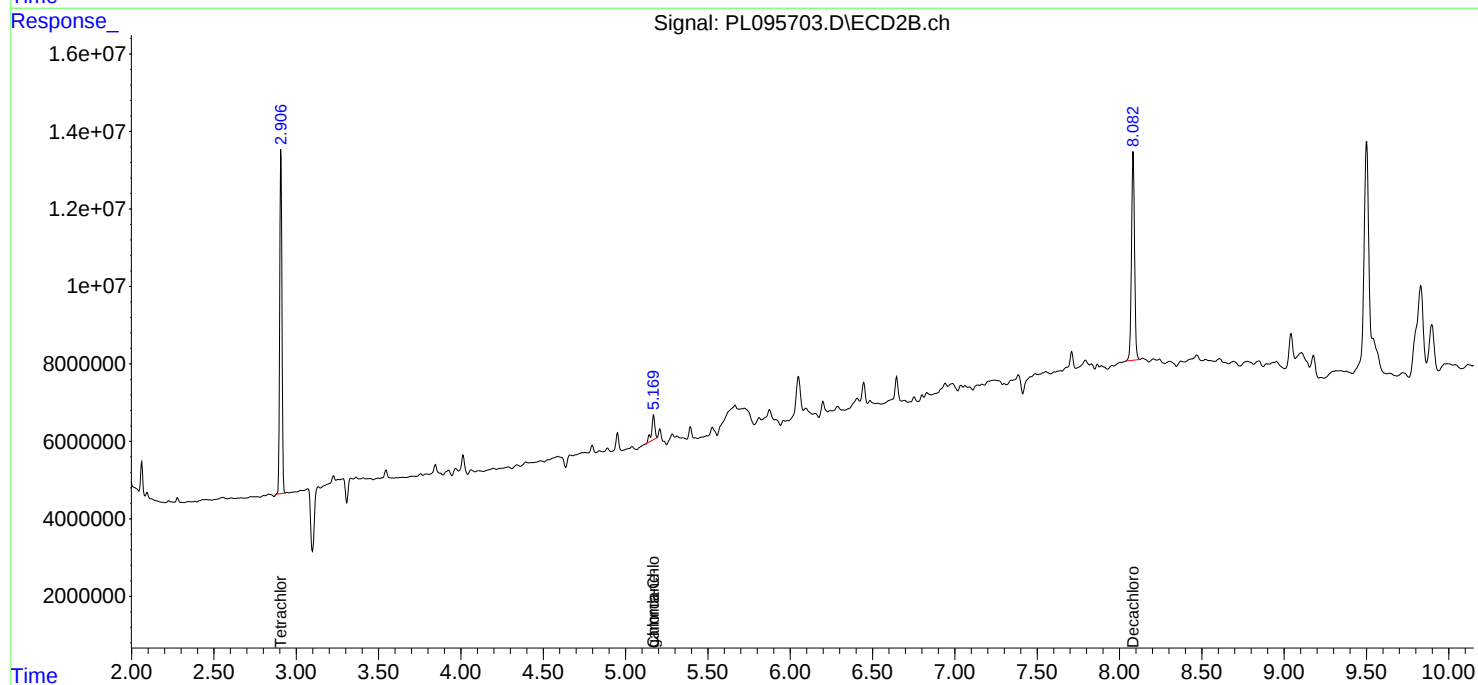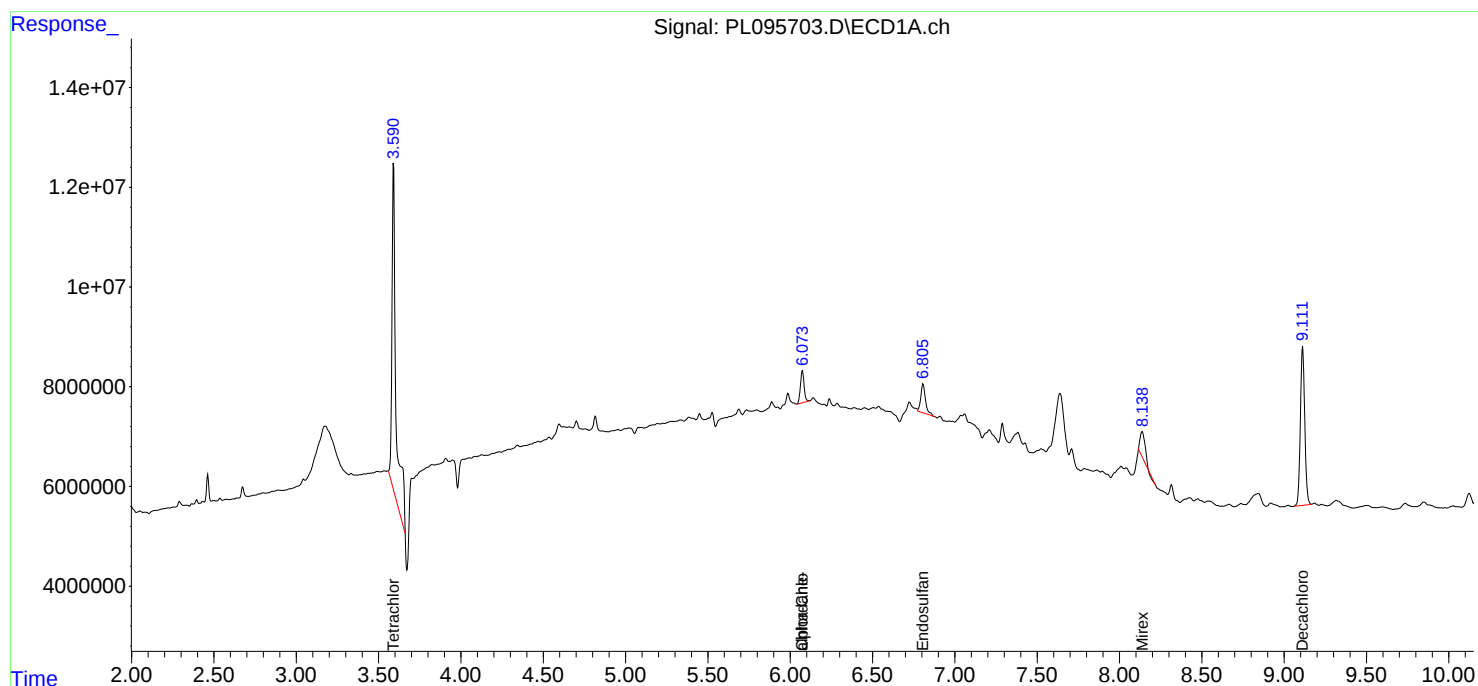


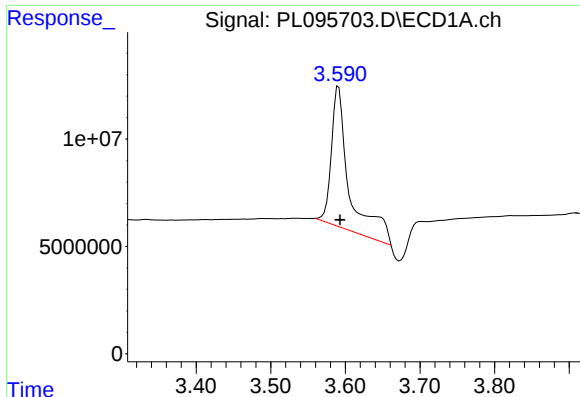

#1 Tetrachloro-m-xylene


R.T.: 3.591 min
Delta R.T.: -0.002 min
Response: 107893478
Conc: 26.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
L3-WC-6

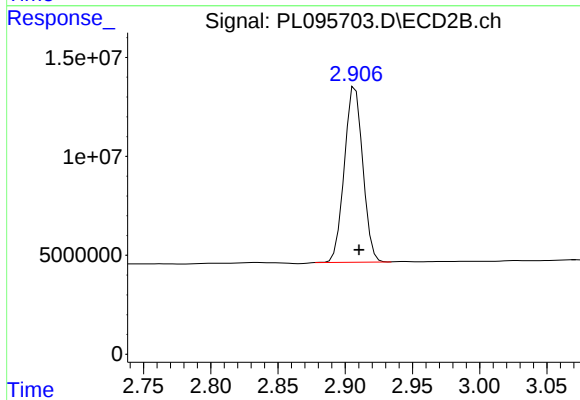


#1 Tetrachloro-m-xylene

R.T.: 2.907 min
Delta R.T.: -0.003 min
Response: 84304210
Conc: 18.00 ng/ml

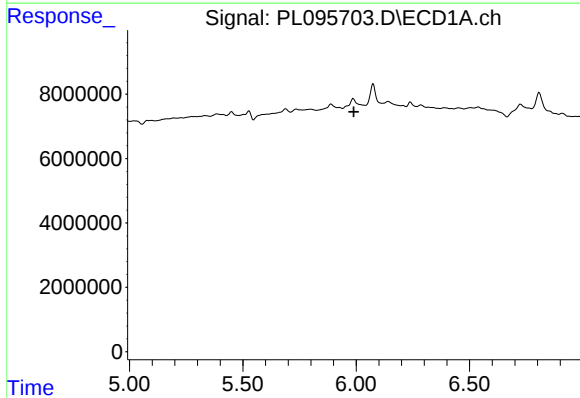


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.990 min
Response: 0
Conc: N.D.

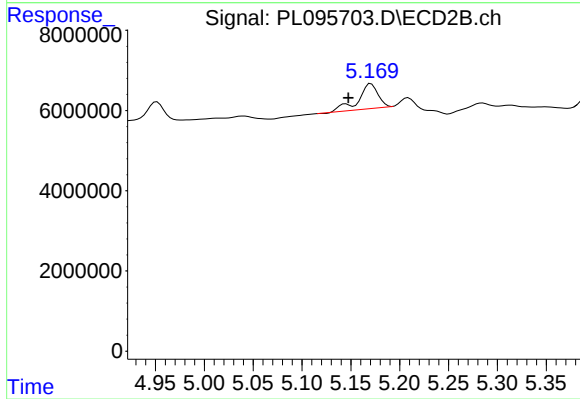

#10 gamma-Chlordane


R.T.: 5.171 min
Delta R.T.: 0.023 min
Response: 8682219
Conc: 1.46 ng/ml

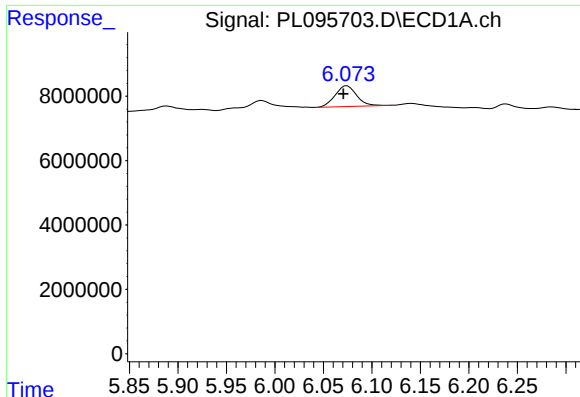

#11 alpha-Chlordane


R.T.: 6.074 min
Delta R.T.: 0.004 min
Response: 9978769
Conc: 1.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
L3-WC-6

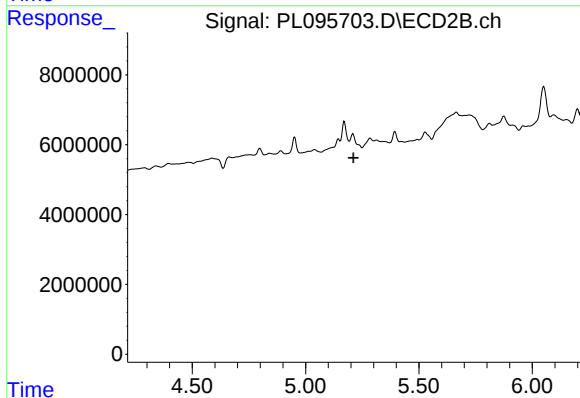


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.212 min
Response: 0
Conc: N.D.

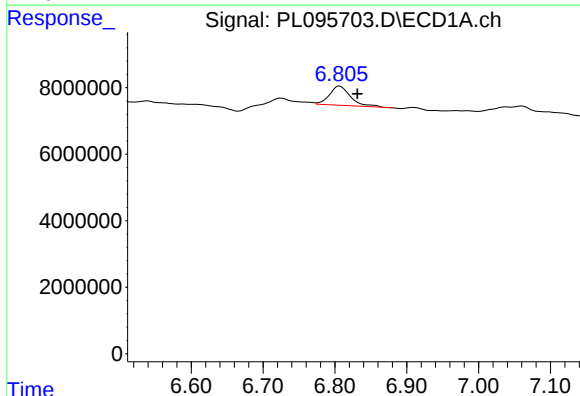


#15 Endosulfan II

R.T.: 6.807 min
Delta R.T.: -0.024 min
Response: 11570984
Conc: 2.78 ng/ml

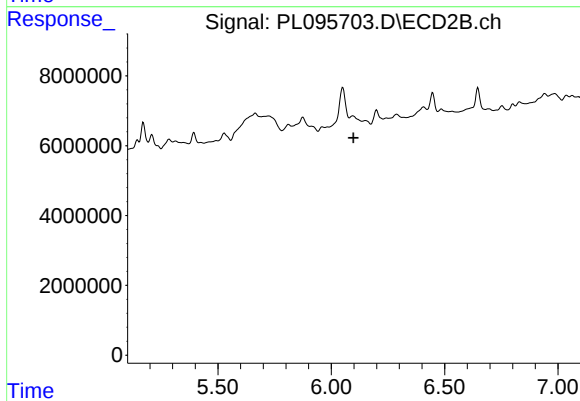

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

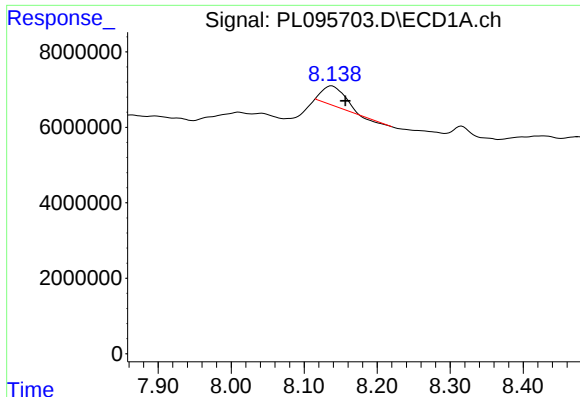

#22 Mirex


R.T.: 8.138 min
Delta R.T.: -0.018 min
Response: 9610400
Conc: 3.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
L3-WC-6

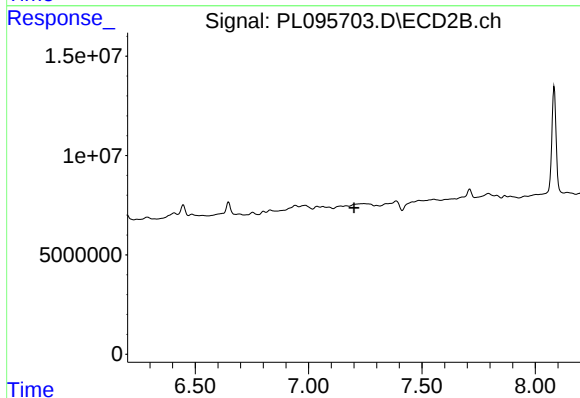


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.201 min
Response: 0
Conc: N.D.

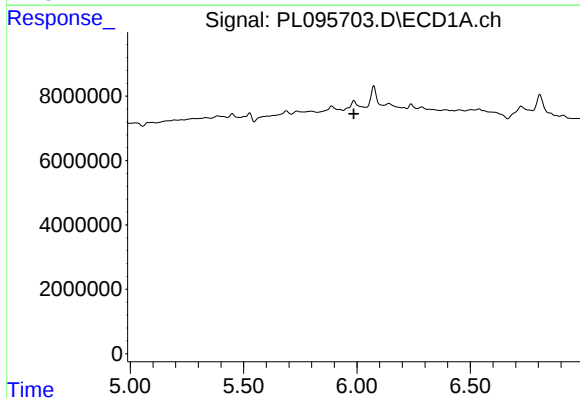


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.987 min
Response: 0
Conc: N.D.

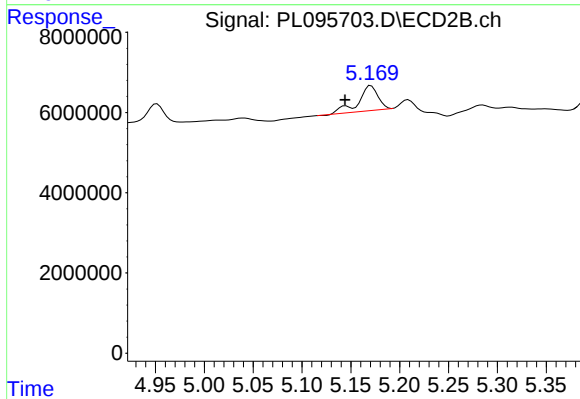

#25 Chlordane-3


R.T.: 5.171 min
Delta R.T.: 0.026 min
Response: 8682219
Conc: 11.22 ng/ml

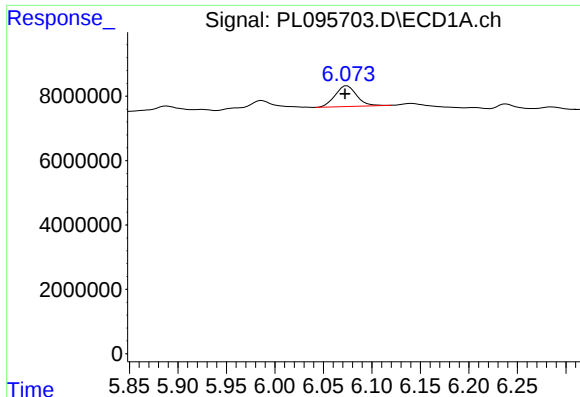

#26 Chlordane-4


R.T.: 6.074 min
Delta R.T.: 0.002 min
Response: 9978769
Conc: 8.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
L3-WC-6

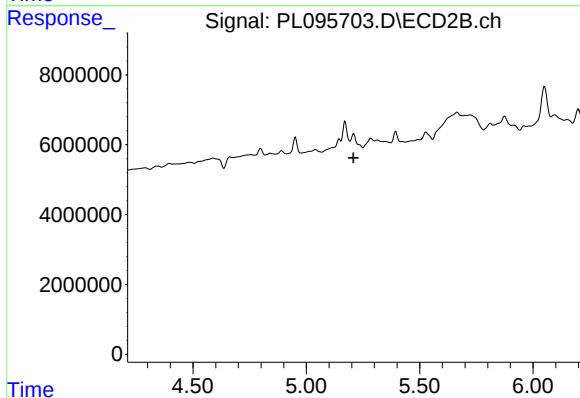


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.208 min
Response: 0
Conc: N.D.

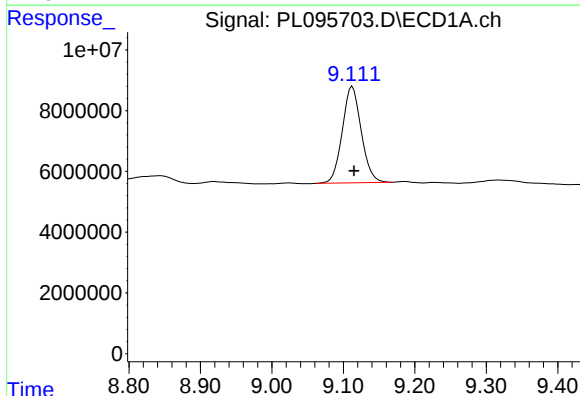

#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: -0.003 min
Response: 58546353
Conc: 17.26 ng/ml

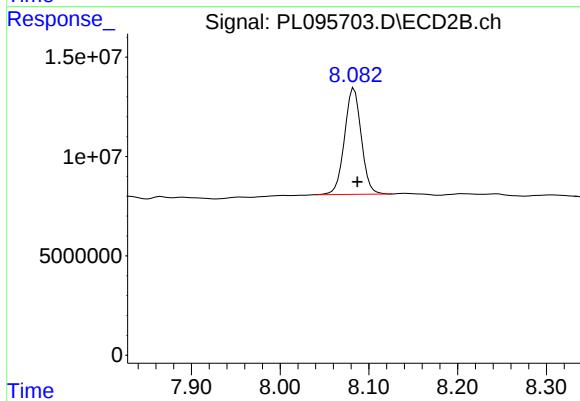

#28 Decachlorobiphenyl

R.T.: 8.083 min
Delta R.T.: -0.004 min
Response: 70144617
Conc: 17.01 ng/ml