

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051622\
 Data File : PL074738.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2022 19:55
 Operator : AR\AJ
 Sample : N2856-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 00:52:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.647	4.652	3769053	10419199	7.423	7.591
28)	SA Decachlor...	11.648	10.405	5416279	13550127	12.128	13.201
Target Compounds							
5)	MB Aldrin	0.000	6.501	0	212202	N.D.	0.141 #
6)	B beta-BHC	0.000	6.126f	0	721652	N.D.	0.909 #
10)	B gamma-Chl...	0.000	7.343f	0	317960	N.D.	0.229 #
11)	B alpha-Chl...	8.484	0.000	5229693	0	8.566	N.D. #
12)	B 4,4'-DDE	8.663	7.641	280465	525024	0.606	0.446 #
13)	MA Dieldrin	0.000	7.778	0	334695	N.D.	0.263 #
14)	MA Endrin	0.000	8.081f	0	304513	N.D.	0.288 #
15)	B Endosulfa...	0.000	8.361	0	411044	N.D.	0.364 #
17)	MA 4,4'-DDT	0.000	8.481	0	814942	N.D.	0.815 #
19)	B Endosulfa...	0.000	8.790	0	213515	N.D.	0.196 #
25)	Chlordane-3	0.000	7.343f	0	317960	N.D.	2.450 #
26)	Chlordane-4	8.484	0.000	5229693	0	54.284	N.D. #
27)	Chlordane-5	0.000	8.141	0	519013	N.D.	14.037 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051622\
Data File : PL074738.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2022 19:55
Operator : AR\AJ
Sample : N2856-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 00:52:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

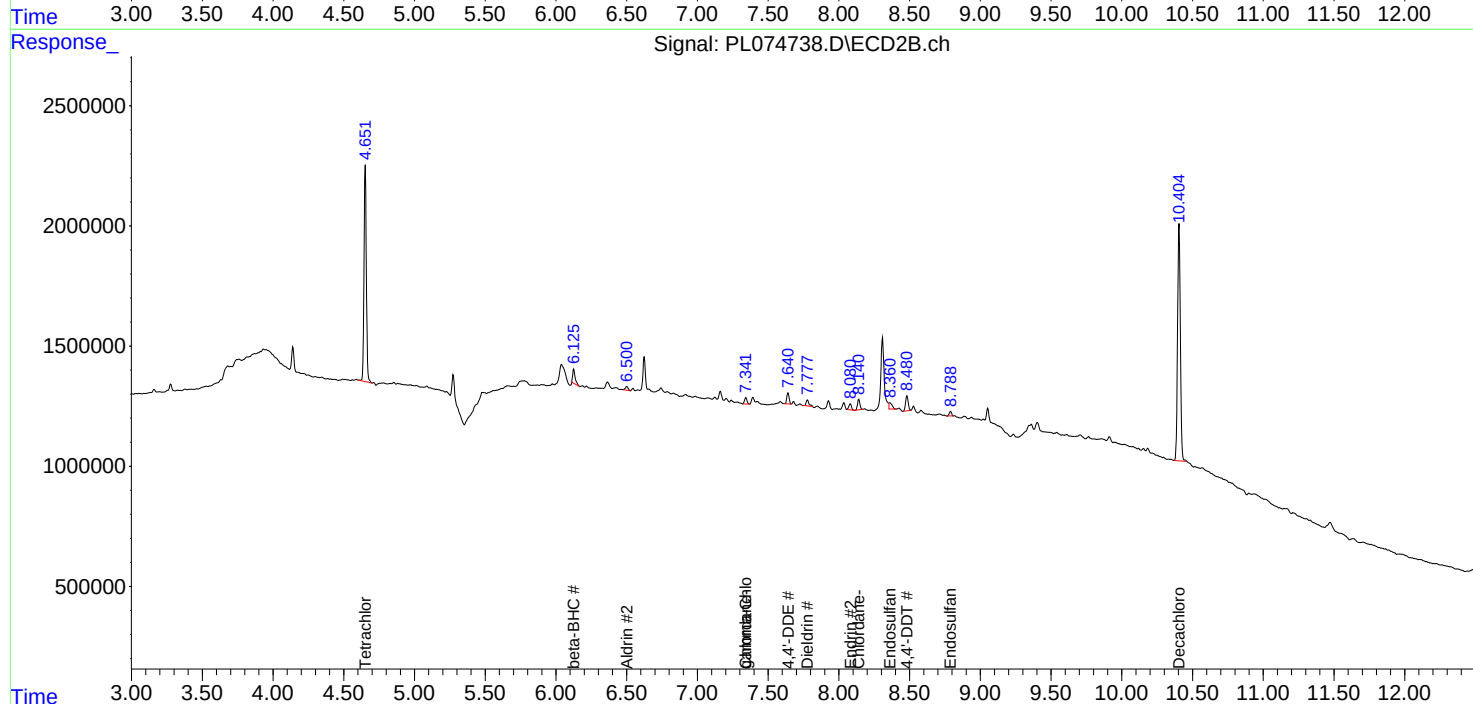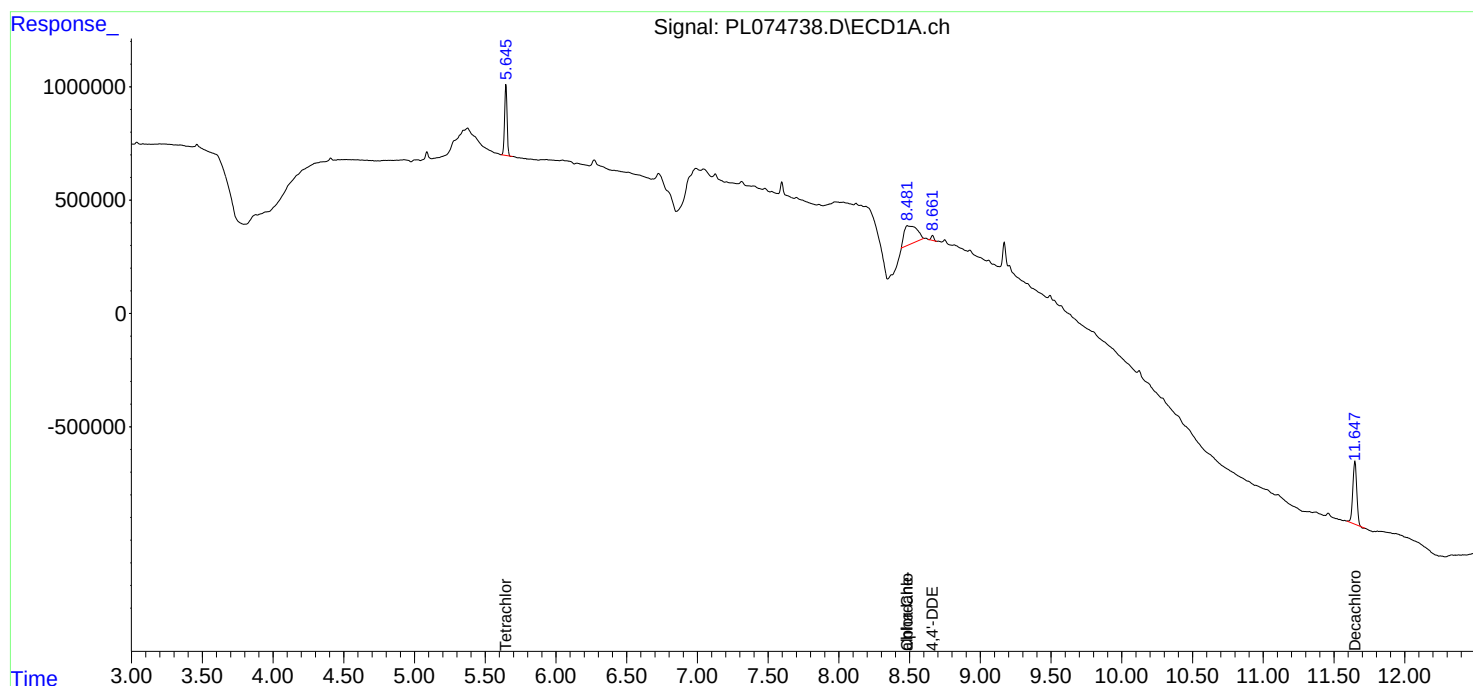


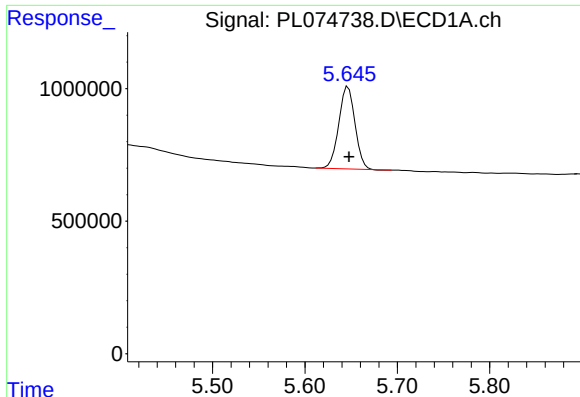

#1 Tetrachloro-m-xylene


R.T.: 5.647 min
Delta R.T.: -0.001 min
Response: 3769053
Conc: 7.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

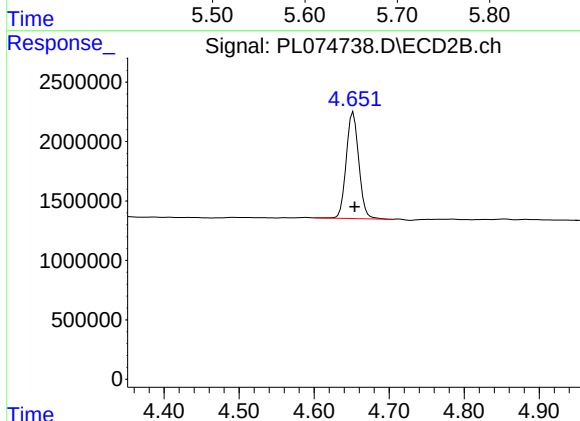


#1 Tetrachloro-m-xylene

R.T.: 4.652 min
Delta R.T.: -0.002 min
Response: 10419199
Conc: 7.59 ng/ml

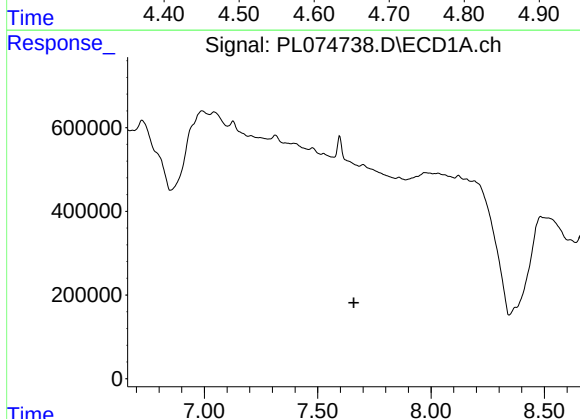


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.660 min
Response: 0
Conc: N.D.

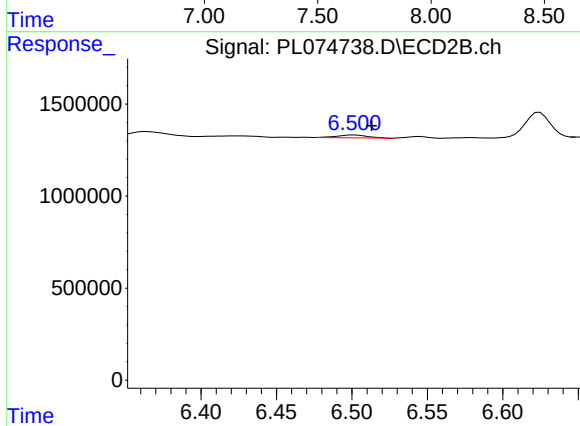

#5 Aldrin


R.T.: 6.501 min
Delta R.T.: -0.012 min
Response: 212202
Conc: 0.14 ng/ml

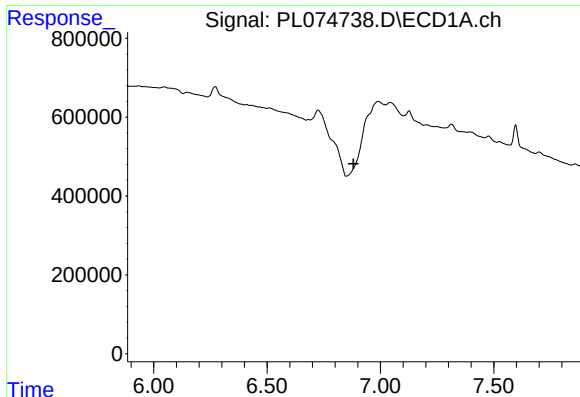

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.882 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

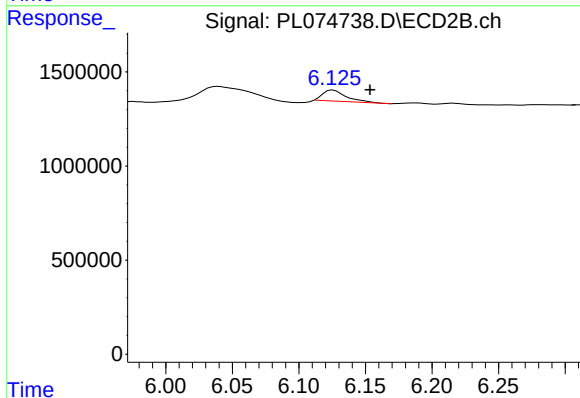


#6 beta-BHC

R.T.: 6.126 min
Delta R.T.: -0.028 min
Response: 721652
Conc: 0.91 ng/ml

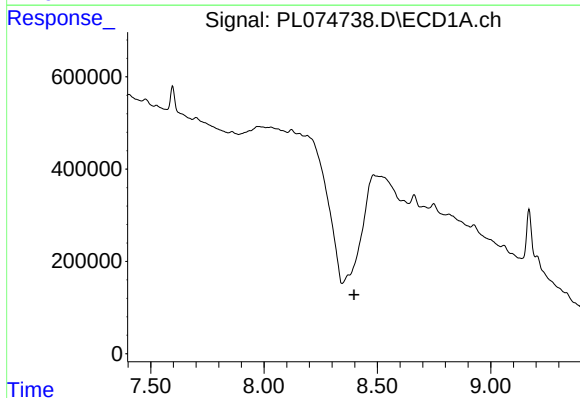


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

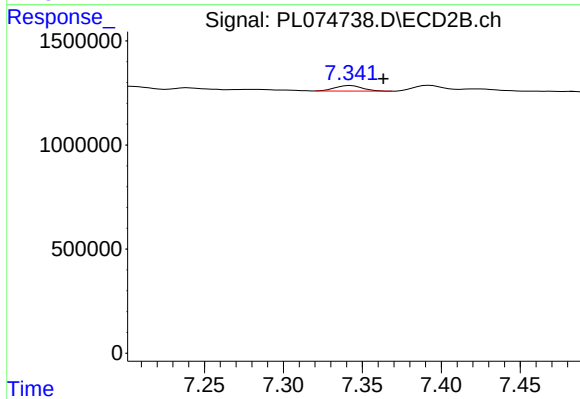

#10 gamma-Chlordane


R.T.: 7.343 min
Delta R.T.: -0.021 min
Response: 317960
Conc: 0.23 ng/ml

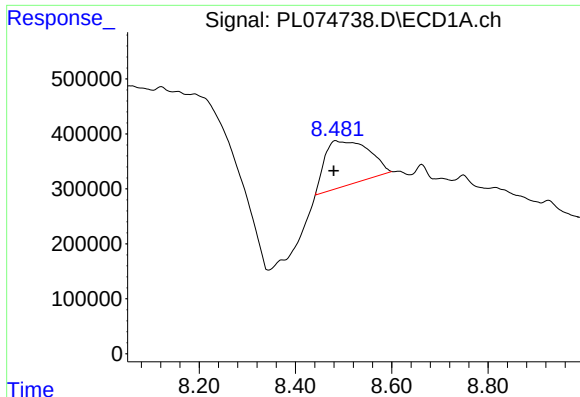

#11 alpha-Chlordane


R.T.: 8.484 min
Delta R.T.: 0.004 min
Response: 5229693
Conc: 8.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

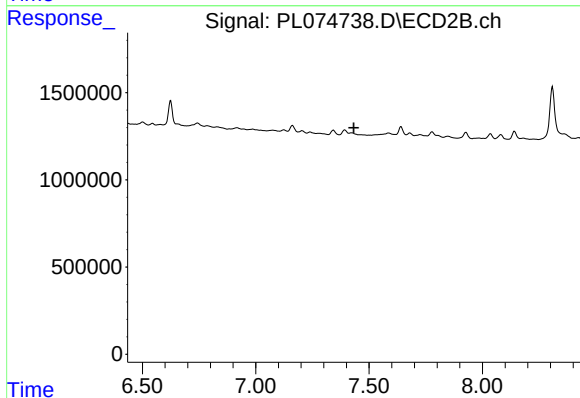


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.433 min
Response: 0
Conc: N.D.

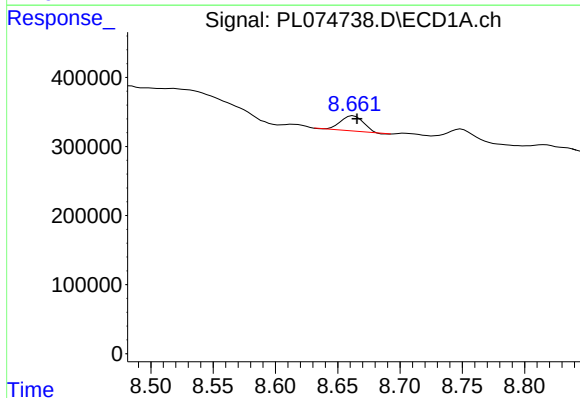


#12 4,4'-DDE

R.T.: 8.663 min
Delta R.T.: -0.003 min
Response: 280465
Conc: 0.61 ng/ml

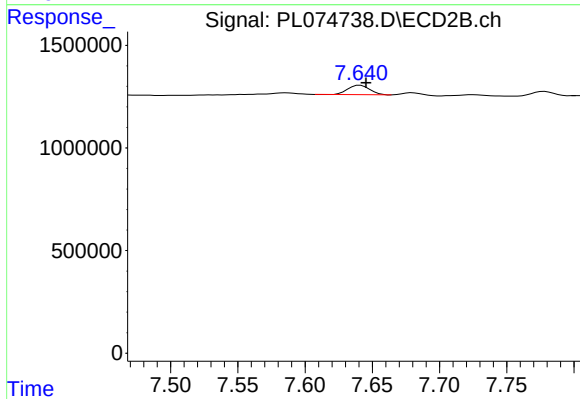

#12 4,4'-DDE


R.T.: 7.641 min
Delta R.T.: -0.004 min
Response: 525024
Conc: 0.45 ng/ml

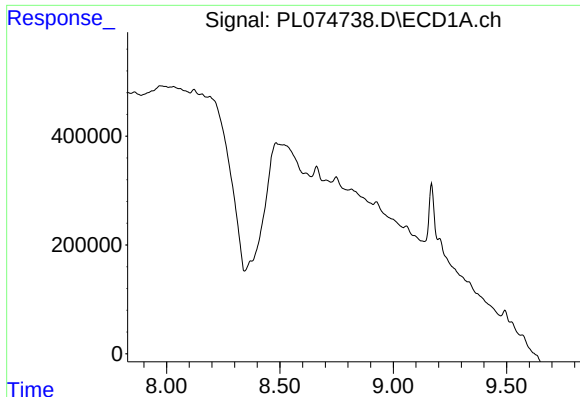

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.827 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

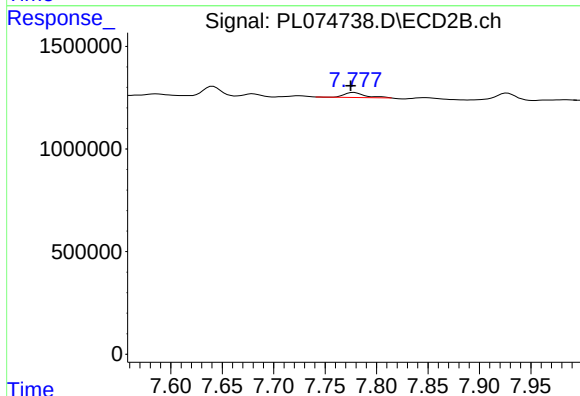


#13 Dieldrin

R.T.: 7.778 min
Delta R.T.: 0.003 min
Response: 334695
Conc: 0.26 ng/ml

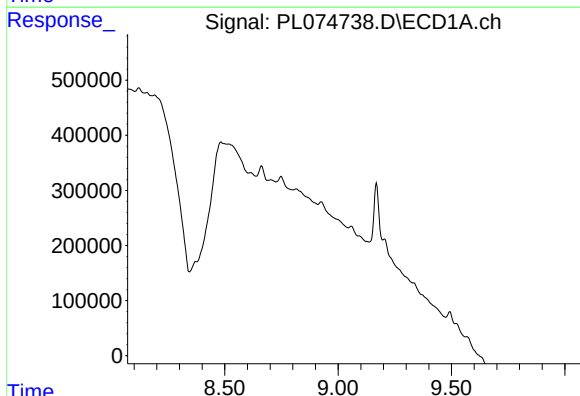


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.068 min
Response: 0
Conc: N.D.

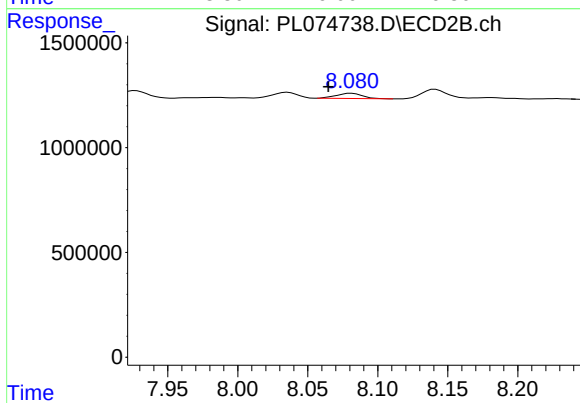

#14 Endrin


R.T.: 8.081 min
Delta R.T.: 0.017 min
Response: 304513
Conc: 0.29 ng/ml

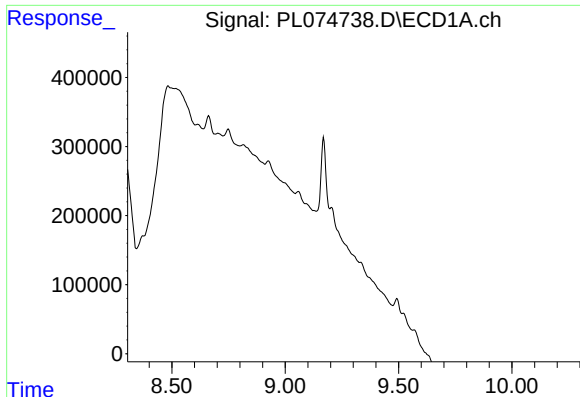

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 9.302 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

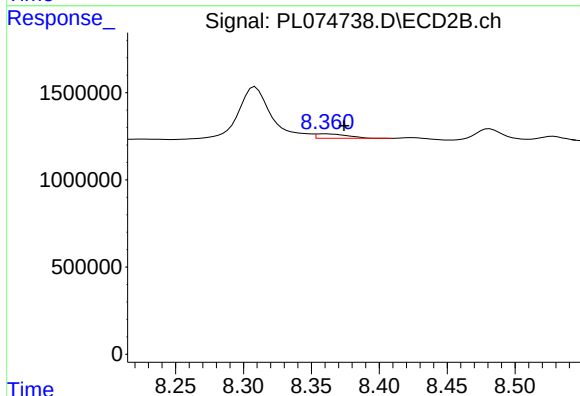


#15 Endosulfan II

R.T.: 8.361 min
Delta R.T.: -0.014 min
Response: 411044
Conc: 0.36 ng/ml

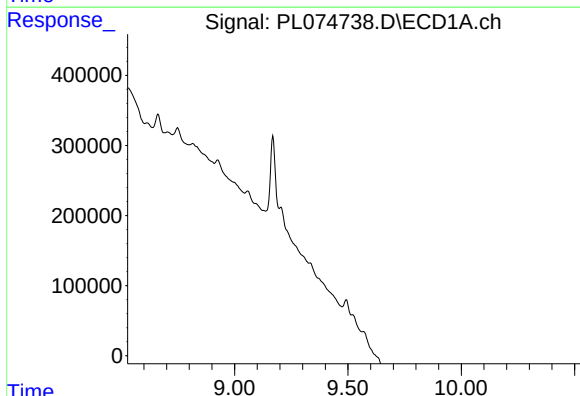


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 9.527 min
Response: 0
Conc: N.D.

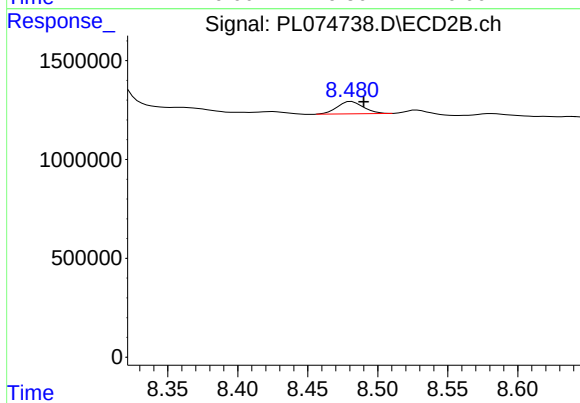

#17 4,4'-DDT


R.T.: 8.481 min
Delta R.T.: -0.009 min
Response: 814942
Conc: 0.81 ng/ml

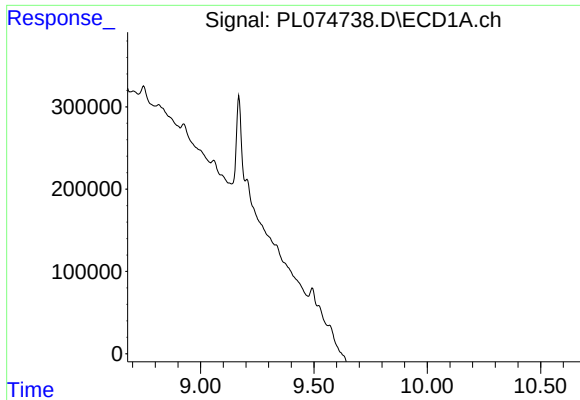

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

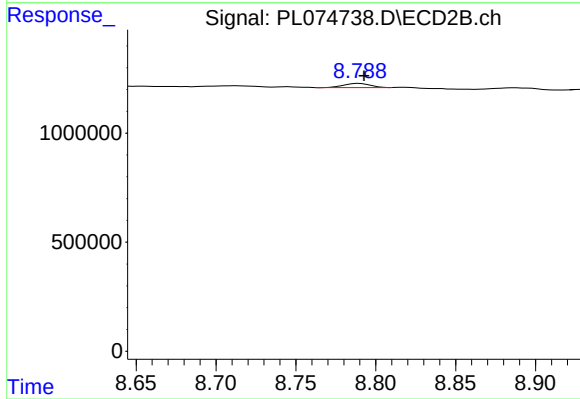


#19 Endosulfan Sulfate

R.T.: 8.790 min
Delta R.T.: -0.003 min
Response: 213515
Conc: 0.20 ng/ml

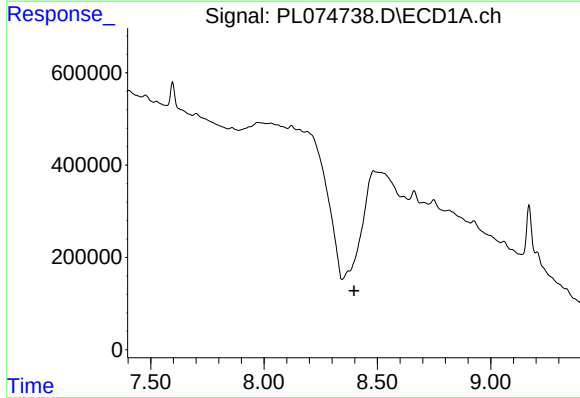


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

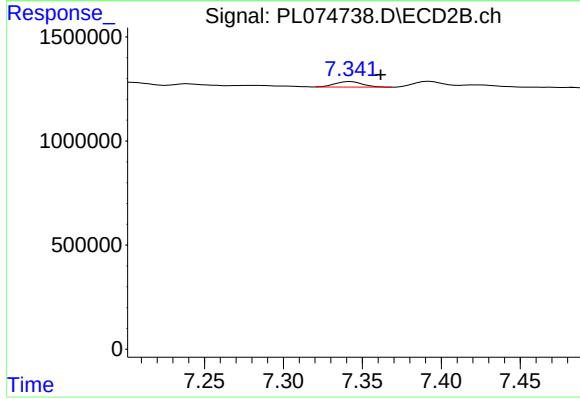

#25 Chlordane-3


R.T.: 7.343 min
Delta R.T.: -0.019 min
Response: 317960
Conc: 2.45 ng/ml

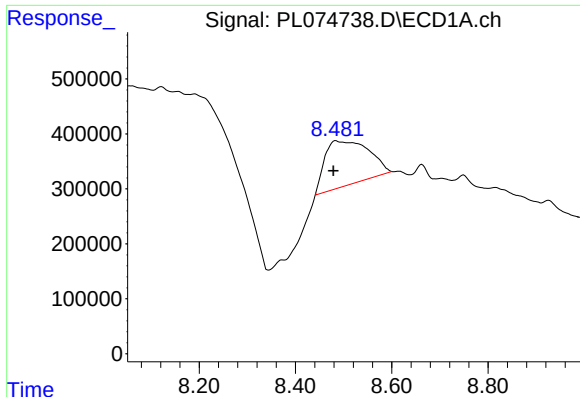

#26 Chlordane-4


R.T.: 8.484 min
Delta R.T.: 0.005 min
Response: 5229693
Conc: 54.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

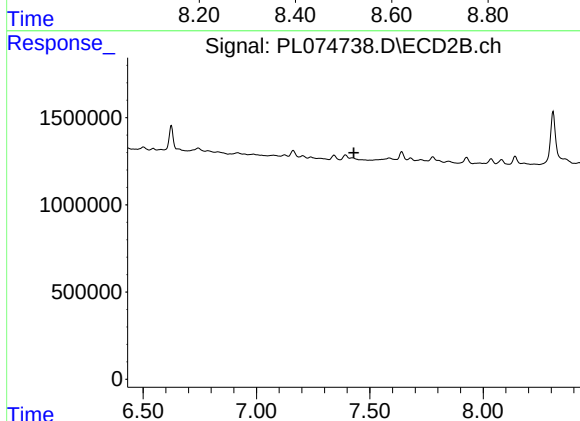


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.430 min
Response: 0
Conc: N.D.

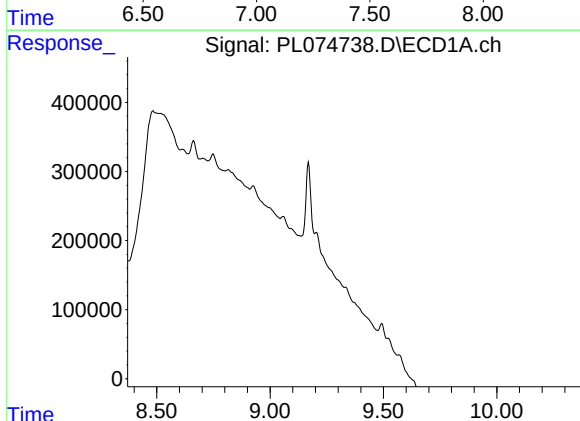


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.371 min
Response: 0
Conc: N.D.

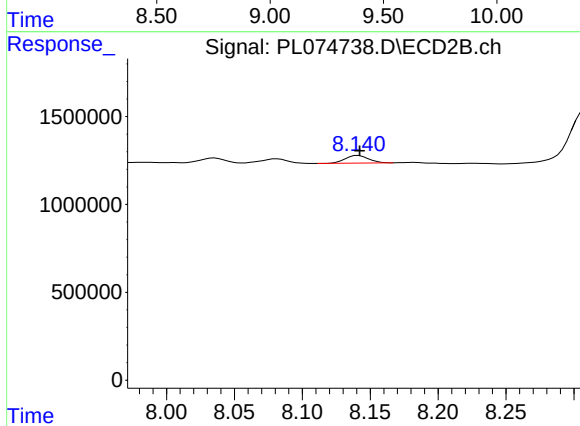

#27 Chlordane-5


R.T.: 8.141 min
Delta R.T.: -0.001 min
Response: 519013
Conc: 14.04 ng/ml

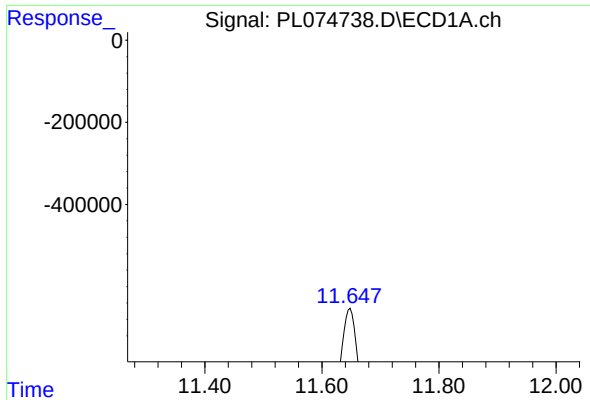

#28 Decachlorobiphenyl

R.T.: 11.648 min
Delta R.T.: -0.003 min
Response: 5416279
Conc: 12.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

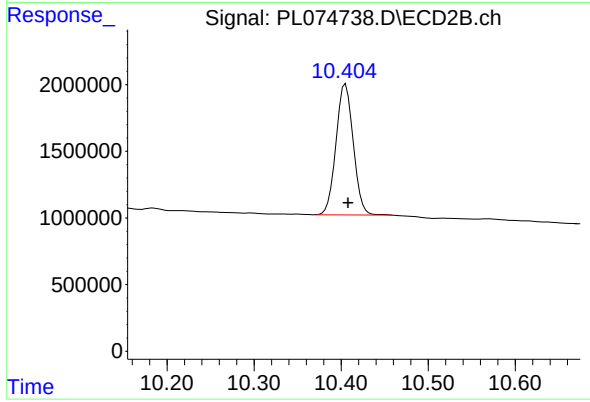

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.003 min
Response: 13550127
Conc: 13.20 ng/ml