

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051622\
 Data File : PL074739.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2022 20:11
 Operator : AR\AJ
 Sample : N2861-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 00:52:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.647	4.653	2274580	6357988	4.480	4.632
28)	SA Decachlor...	11.650	10.406	3525483	7535093	7.894	7.341
Target Compounds							
6)	B beta-BHC	0.000	6.125f	0	487916	N.D.	0.615 #
9)	A Endosulfan I	8.521	0.000	2914756	0	5.056	N.D. #
11)	B alpha-Chl...	8.489	0.000	2266427	0	3.712	N.D. #
12)	B 4,4'-DDE	0.000	7.643	0	475850	N.D.	0.404 #
14)	MA Endrin	0.000	8.084f	0	502547	N.D.	0.476 #
26)	Chlordane-4	8.489	0.000	2266427	0	23.525	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051622\
Data File : PL074739.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2022 20:11
Operator : AR\AJ
Sample : N2861-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 00:52:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

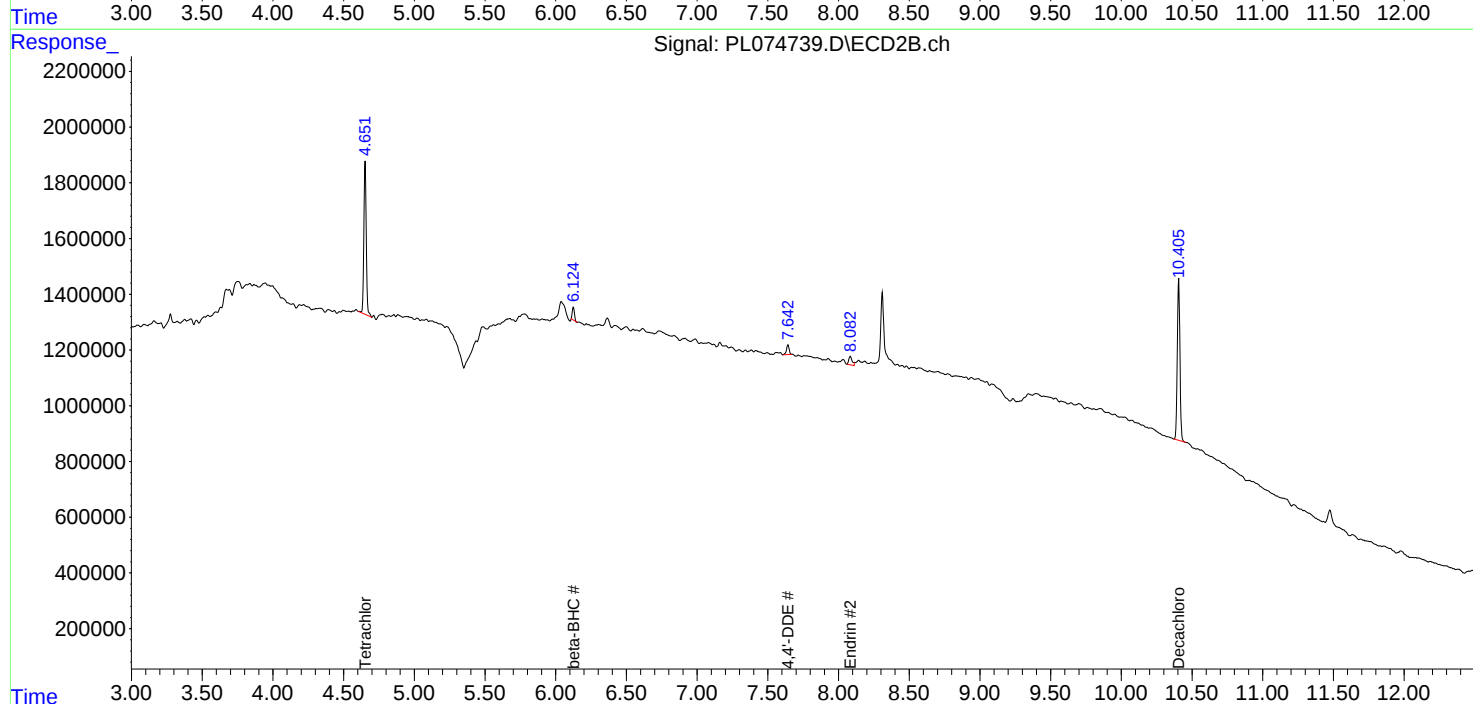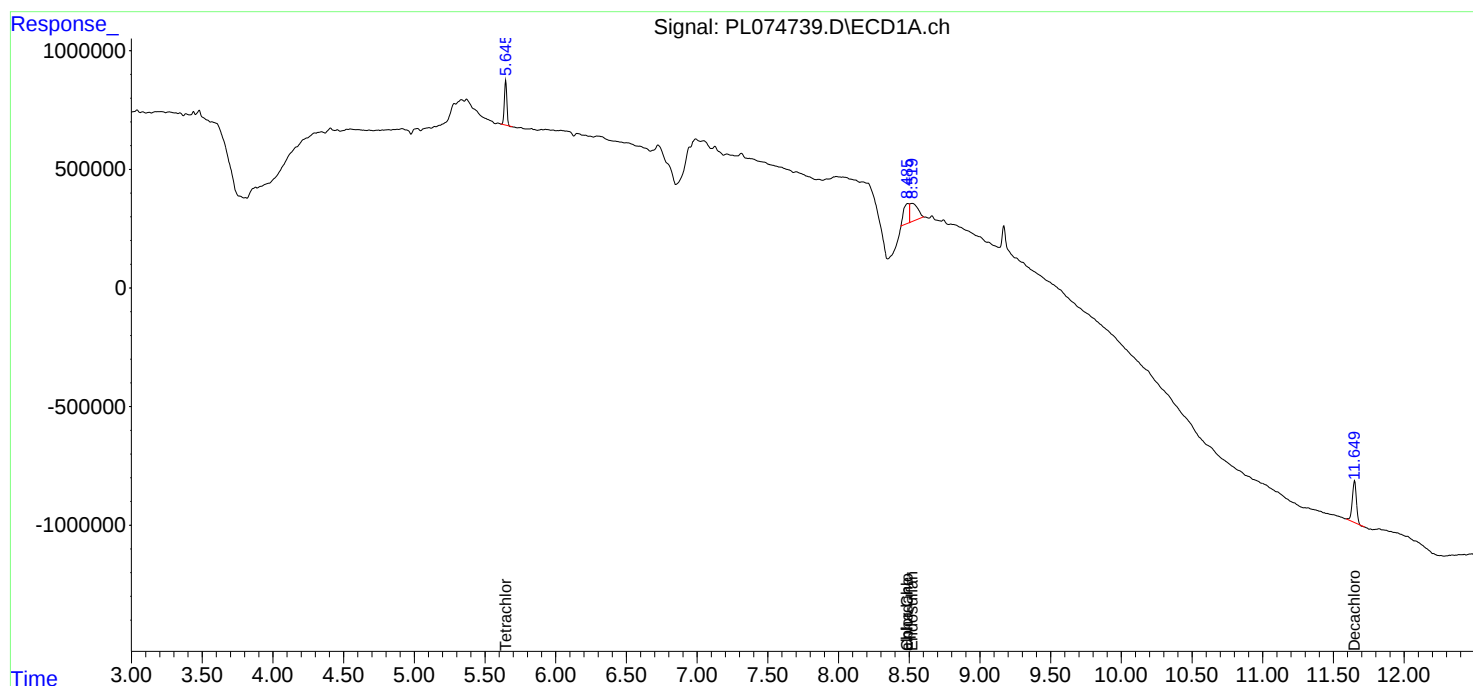


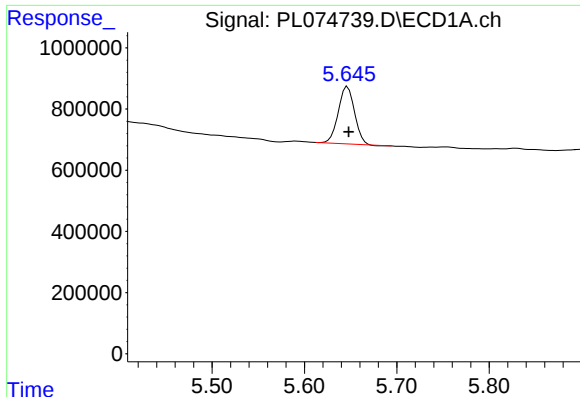

#1 Tetrachloro-m-xylene


R.T.: 5.647 min
Delta R.T.: -0.001 min
Response: 2274580
Conc: 4.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

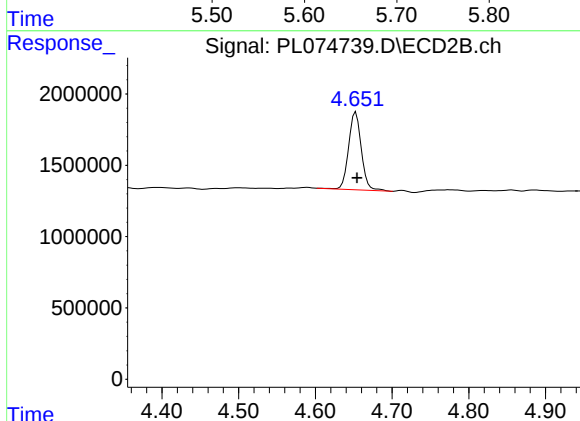


#1 Tetrachloro-m-xylene

R.T.: 4.653 min
Delta R.T.: -0.002 min
Response: 6357988
Conc: 4.63 ng/ml

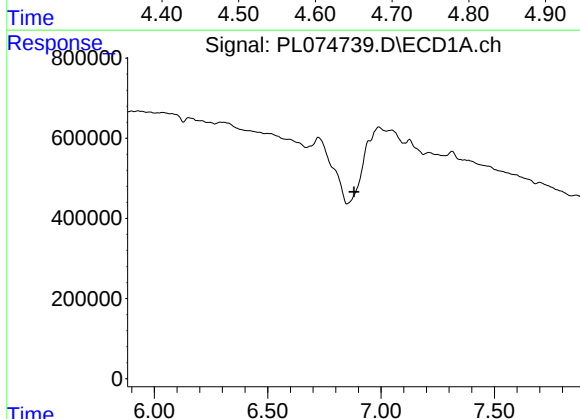


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.882 min
Response: 0
Conc: N.D.

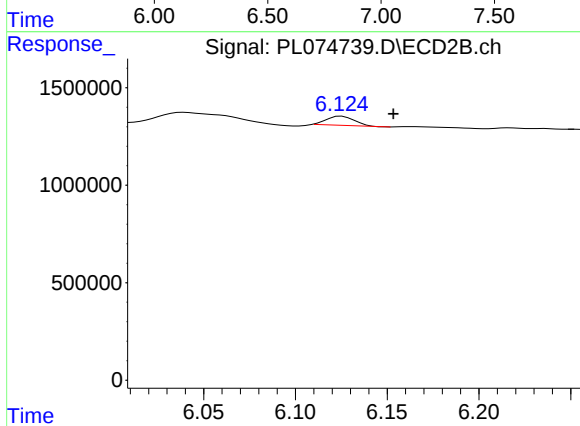

#6 beta-BHC


R.T.: 6.125 min
Delta R.T.: -0.028 min
Response: 487916
Conc: 0.61 ng/ml

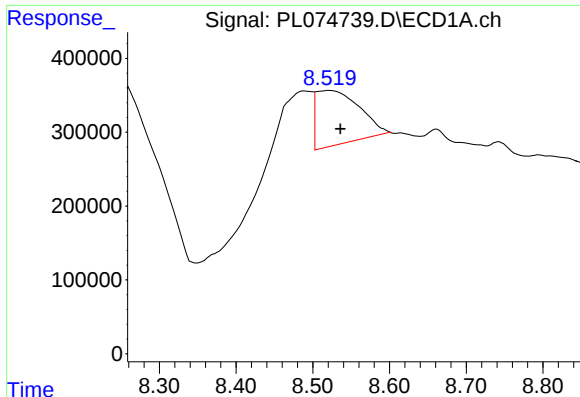

#9 Endosulfan I


R.T.: 8.521 min
Delta R.T.: -0.015 min
Response: 2914756
Conc: 5.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

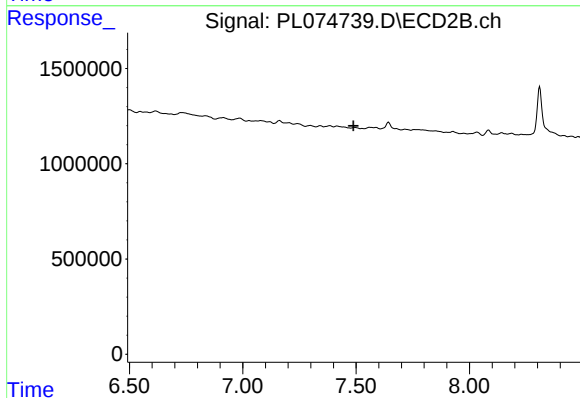


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.489 min
Response: 0
Conc: N.D.

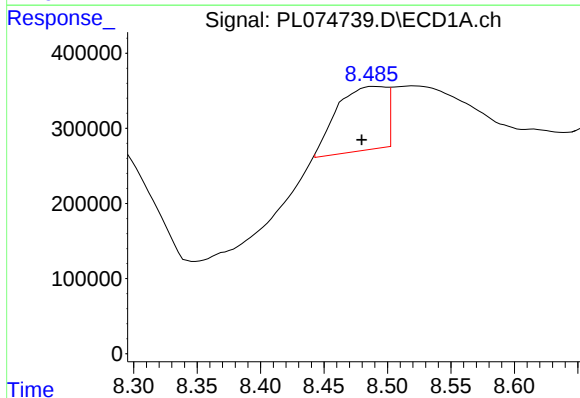


#11 alpha-Chlordane

R.T.: 8.489 min
Delta R.T.: 0.009 min
Response: 2266427
Conc: 3.71 ng/ml

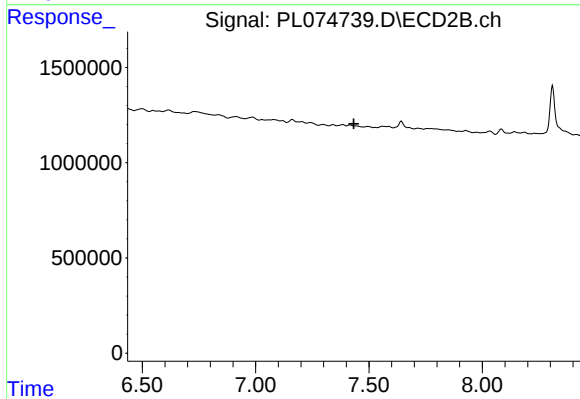

#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.433 min
Response: 0
Conc: N.D.

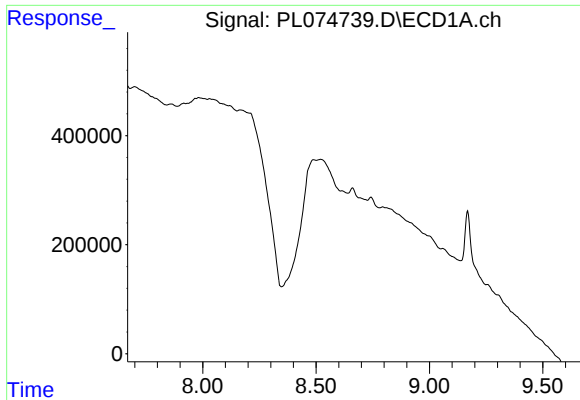

#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 8.665 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#12 4,4'-DDE


R.T.: 7.643 min
Delta R.T.: -0.002 min
Response: 475850
Conc: 0.40 ng/ml

#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.068 min
Response: 0
Conc: N.D.

#14 Endrin


R.T.: 8.084 min
Delta R.T.: 0.019 min
Response: 502547
Conc: 0.48 ng/ml

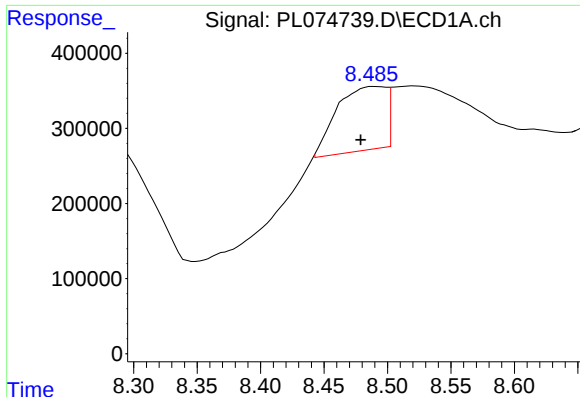

#26 Chlordane-4


R.T.: 8.489 min
Delta R.T.: 0.010 min
Response: 2266427
Conc: 23.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

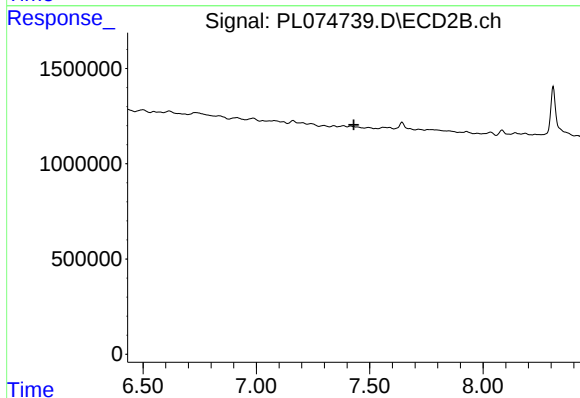


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.430 min
Response: 0
Conc: N.D.

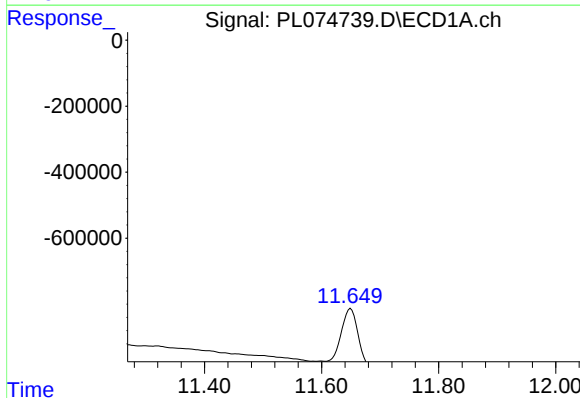

#28 Decachlorobiphenyl

R.T.: 11.650 min
Delta R.T.: -0.001 min
Response: 3525483
Conc: 7.89 ng/ml

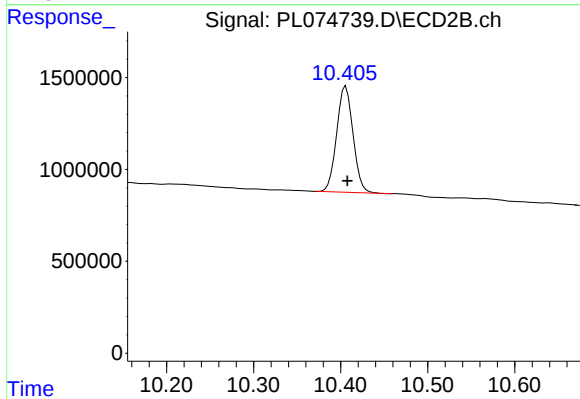

#28 Decachlorobiphenyl

R.T.: 10.406 min
Delta R.T.: -0.002 min
Response: 7535093
Conc: 7.34 ng/ml