

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051622\
 Data File : PL074724.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2022 12:33
 Operator : AR\AJ
 Sample : N2823-03DL 20X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SC-3DL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/17/2022
 Supervised By :mohammad ahmed 05/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 00:47:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.655	4.654	606943	1763086	1.195	1.285
28) SA Decachlor...	11.655	10.409	920440	1880802	2.061	1.832
Target Compounds						
12) B 4,4'-DDE	8.670	7.644	11644305	19637795	25.154	16.689m#
20) A Methoxychlor	10.015	9.081	439031	1390885	1.793m	2.380m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051622\
Data File : PL074724.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2022 12:33
Operator : AR\AJ
Sample : N2823-03DL 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleID :
SC-3DL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/17/2022
Supervised By : mohammad ahmed 05/17/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 00:47:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

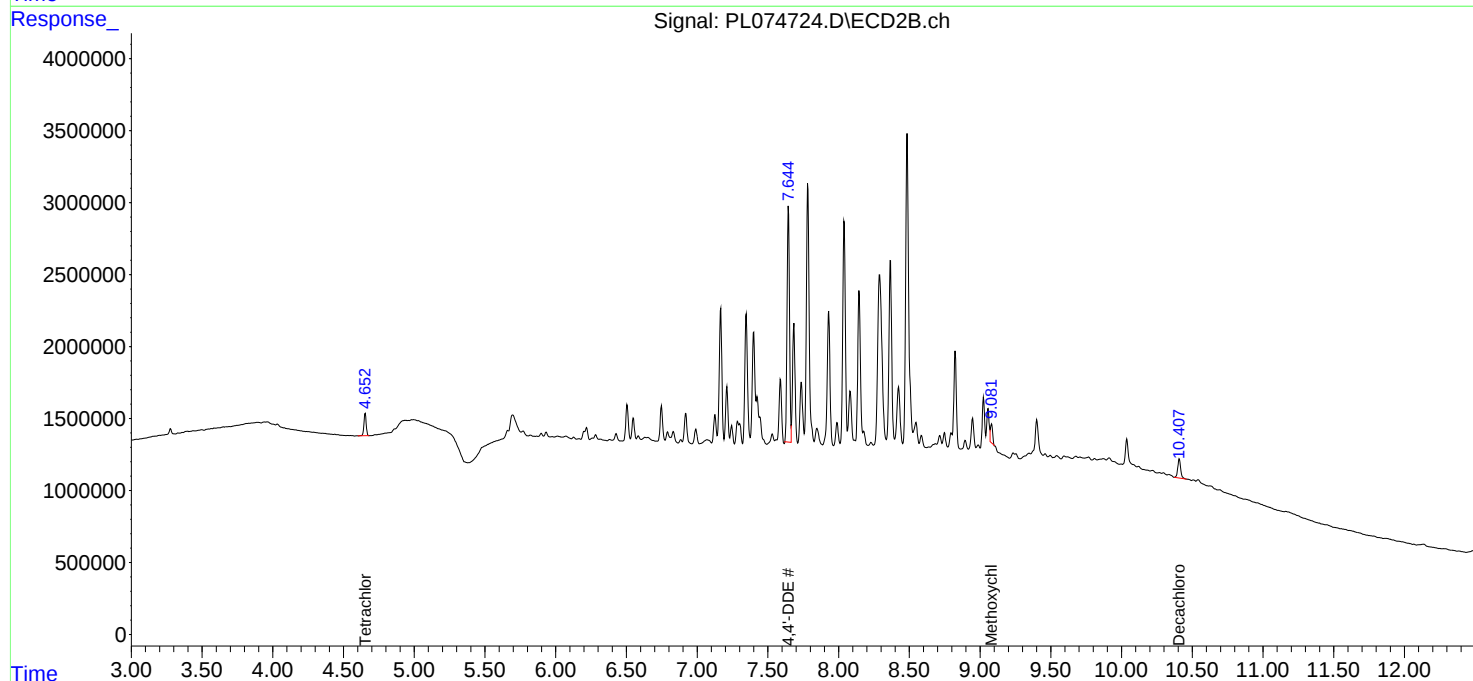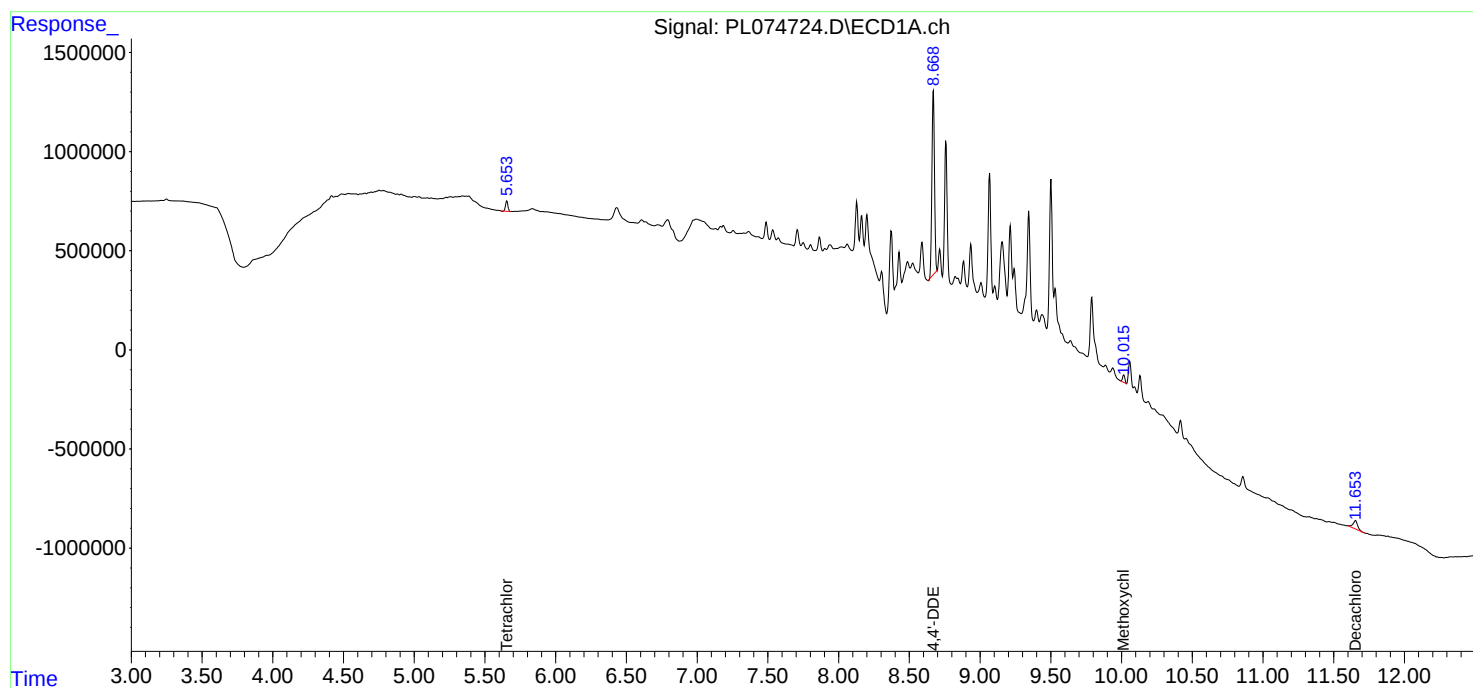

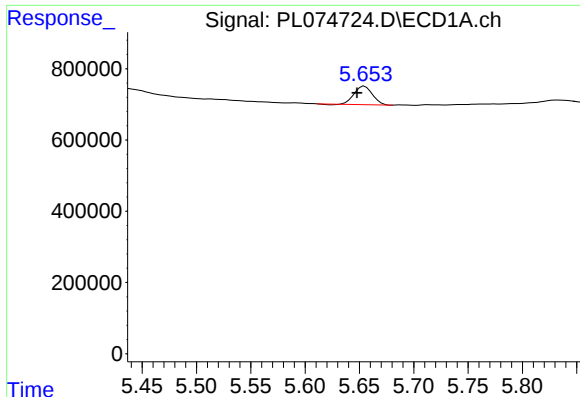


#1 Tetrachloro-m-xylene

R.T.: 5.655 min
Delta R.T.: 0.007 min
Response: 606943
Conc: 1.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
SC-3DL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/17/2022
Supervised By :mohammad ahmed 05/17/2022

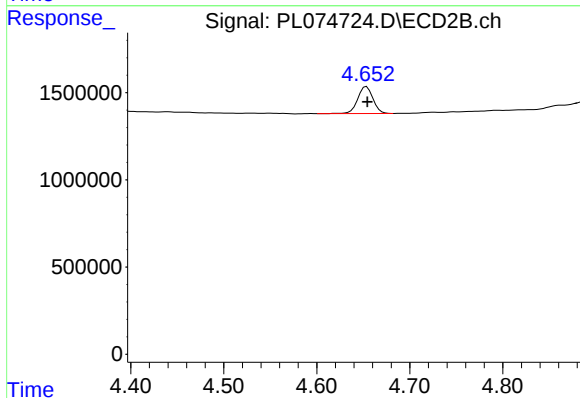


#1 Tetrachloro-m-xylene

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 1763086
Conc: 1.28 ng/ml

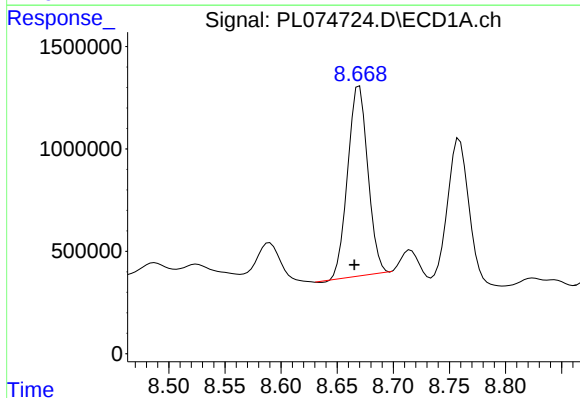


#12 4,4'-DDE

R.T.: 8.670 min
Delta R.T.: 0.004 min
Response: 11644305
Conc: 25.15 ng/ml

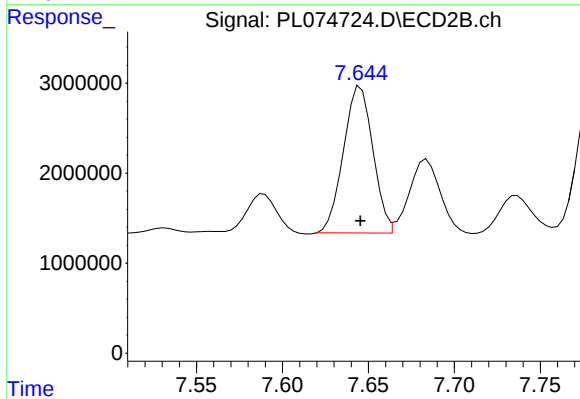

#12 4,4'-DDE

R.T.: 7.644 min
Delta R.T.: -0.001 min
Response: 19637795
Conc: 16.69 ng/ml m

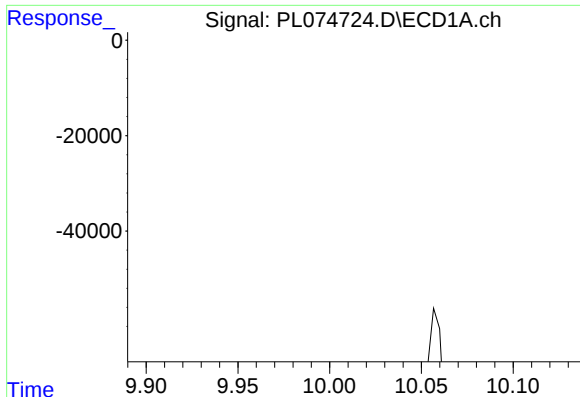


#20 Methoxychlor

R.T.: 10.015 min
Delta R.T.: 0.002 min
Response: 439031
Conc: 1.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
SC-3DL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/17/2022
Supervised By :mohammad ahmed 05/17/2022

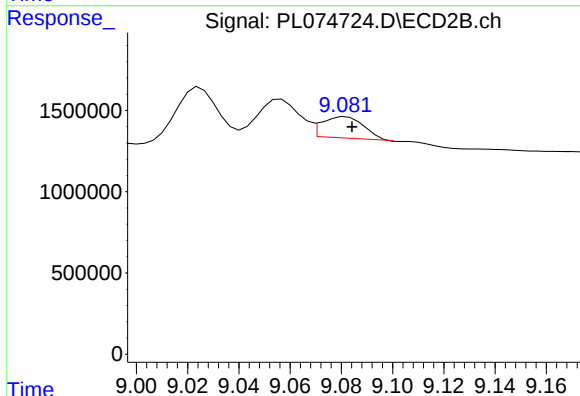


#20 Methoxychlor

R.T.: 9.081 min
Delta R.T.: -0.004 min
Response: 1390885
Conc: 2.38 ng/ml m

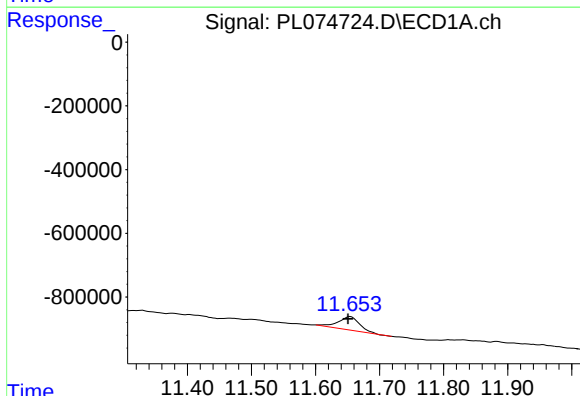

#28 Decachlorobiphenyl

R.T.: 11.655 min
Delta R.T.: 0.004 min
Response: 920440
Conc: 2.06 ng/ml

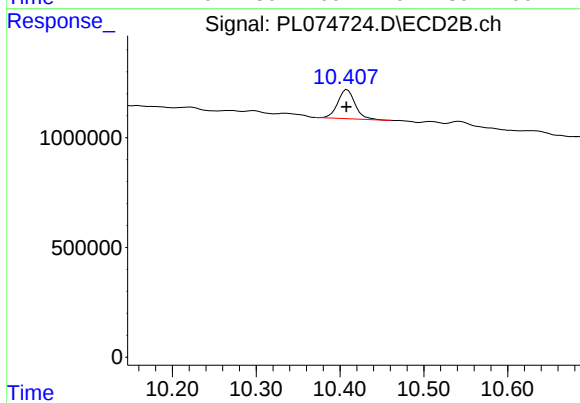

#28 Decachlorobiphenyl

R.T.: 10.409 min
Delta R.T.: 0.000 min
Response: 1880802
Conc: 1.83 ng/ml