

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051622\
 Data File : PL074726.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2022 13:06
 Operator : AR\AJ
 Sample : N2823-13DL 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SC-13DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 00:47:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.647	4.653	380164	847563	0.749	0.618
28)	SA Decachlor...	11.647	10.405	760590	1629381	1.703	1.587
Target Compounds							
12)	B 4,4'-DDE	8.664	7.643	12029088	29724432	25.985	25.261



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051622\
Data File : PL074726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2022 13:06
Operator : AR\AJ
Sample : N2823-13DL 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SC-13DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 00:47:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

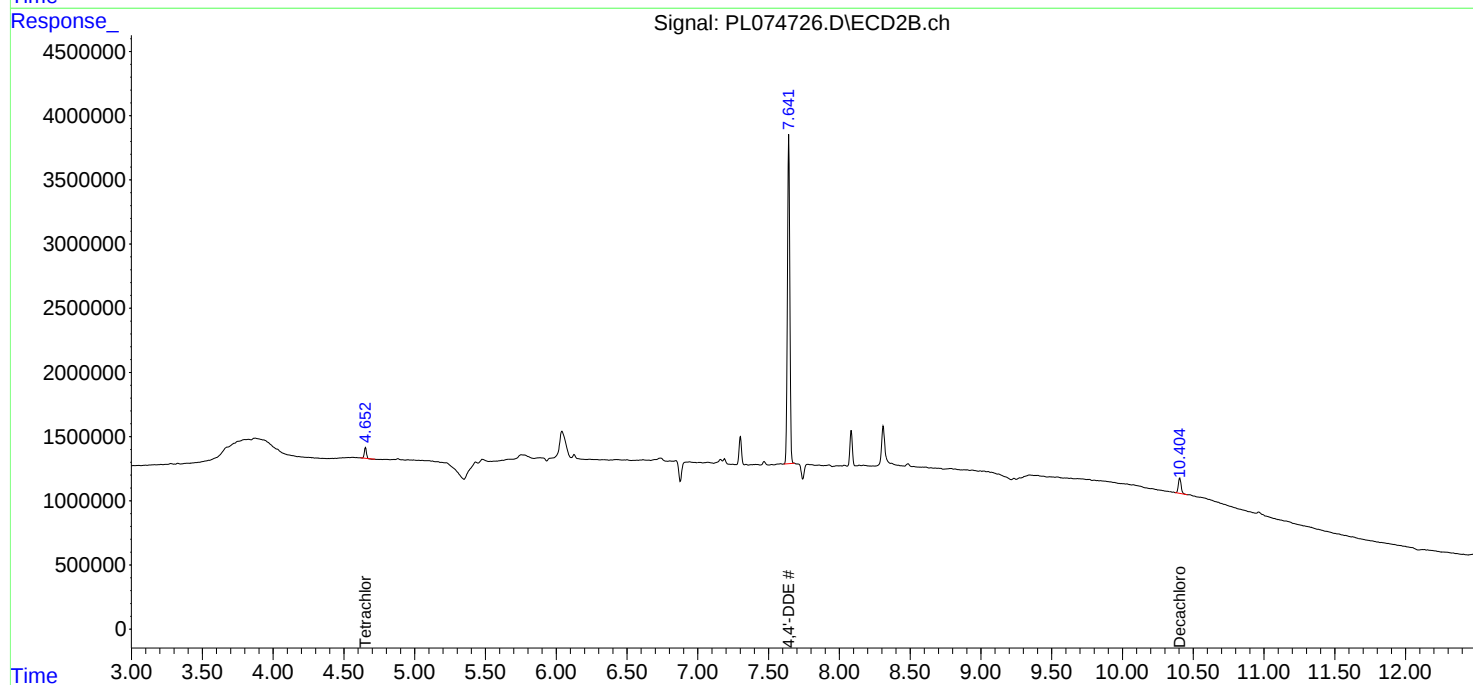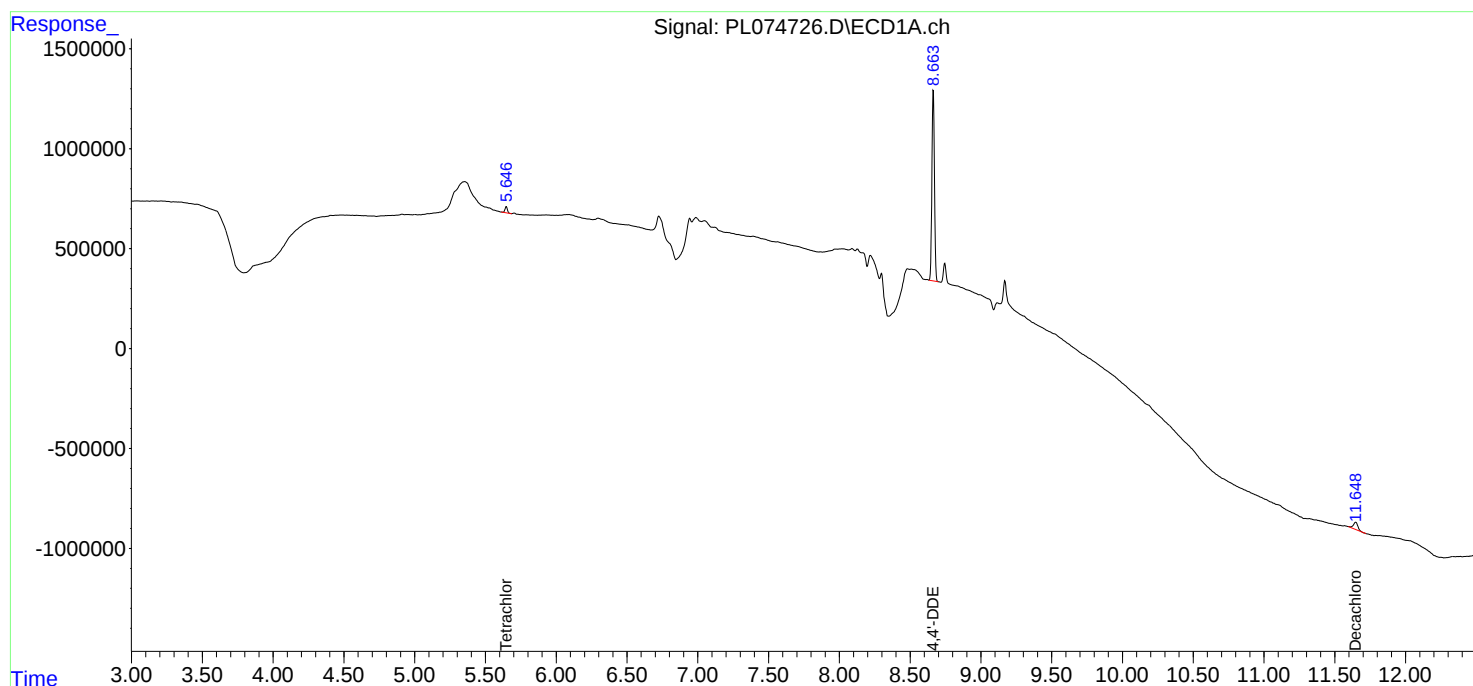


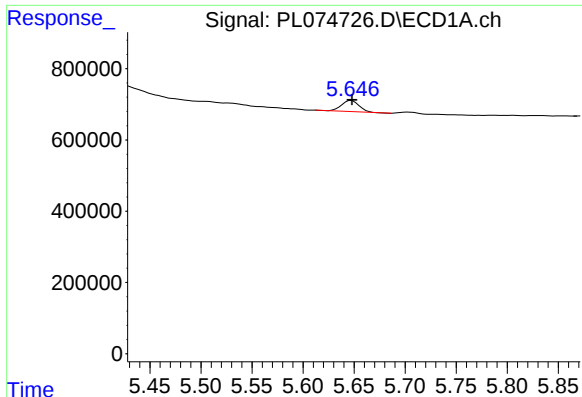

#1 Tetrachloro-m-xylene


R.T.: 5.647 min
Delta R.T.: 0.000 min
Response: 380164
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
SC-13DL

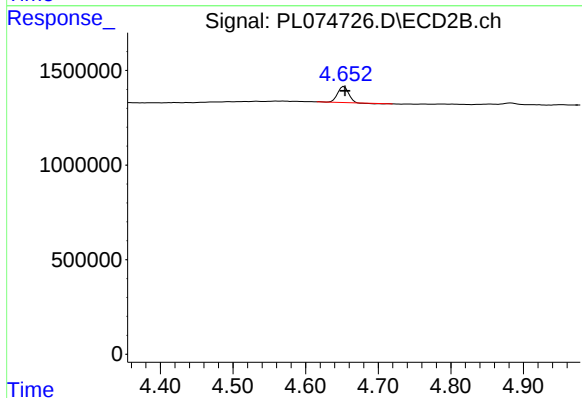


#1 Tetrachloro-m-xylene

R.T.: 4.653 min
Delta R.T.: -0.001 min
Response: 847563
Conc: 0.62 ng/ml

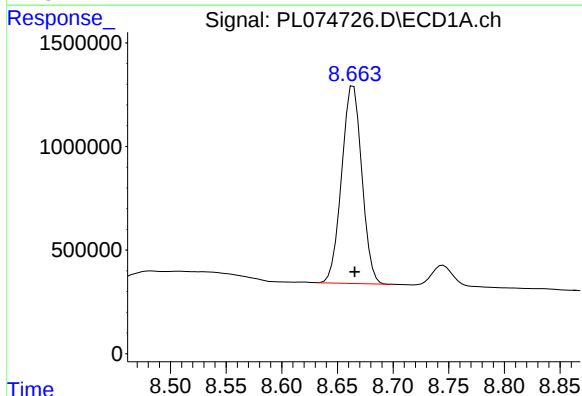


#12 4,4'-DDE

R.T.: 8.664 min
Delta R.T.: -0.001 min
Response: 12029088
Conc: 25.98 ng/ml

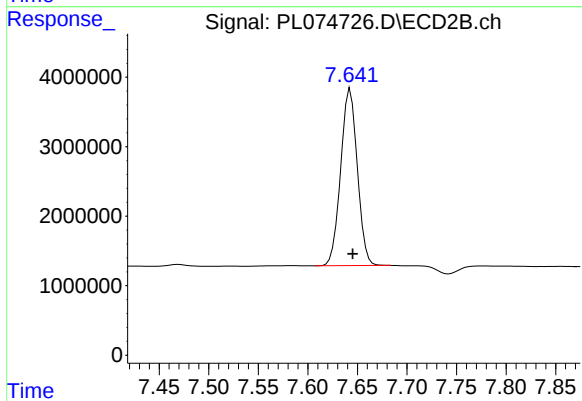

#12 4,4'-DDE


R.T.: 7.643 min
Delta R.T.: -0.002 min
Response: 29724432
Conc: 25.26 ng/ml

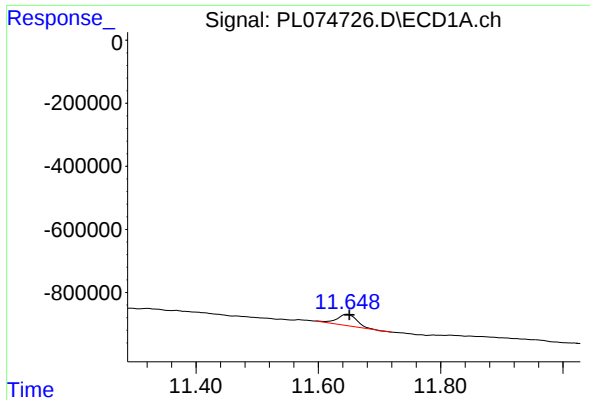

#28 Decachlorobiphenyl

R.T.: 11.647 min
Delta R.T.: -0.004 min
Response: 760590
Conc: 1.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
SC-13DL

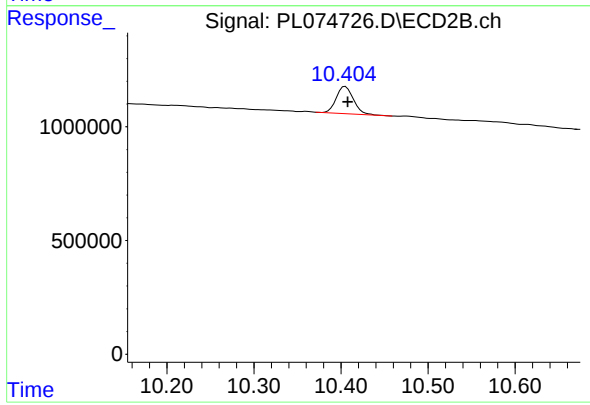

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.003 min
Response: 1629381
Conc: 1.59 ng/ml