

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051623\
 Data File : PL082743.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2023 19:23
 Operator : AR\AJ
 Sample : 02798-01MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 21:52:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm


	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	2.641	52430167	43589863	19.628	18.815
28)	SA Decachlor...	8.738	7.750	27357126	27616152	14.330	12.099
Target Compounds							
2)	A alpha-BHC	3.768	3.137	192.1E6	155.9E6	48.254	45.816
3)	MA gamma-BHC...	4.097	3.465	182.3E6	147.5E6	48.767	45.876
4)	MA Heptachlor	4.674	3.796	159.0E6	127.6E6	43.523	37.277
5)	MB Aldrin	5.011	4.072	165.7E6	147.8E6	50.249	46.913
6)	B beta-BHC	4.300	3.765	82899364	56632542	48.607	41.507
7)	B delta-BHC	4.541	3.990	161.8E6	132.2E6	44.962	43.106
8)	B Heptachlo...	5.437	4.573	143.6E6	130.6E6	47.066	45.348
9)	A Endosulfan I	5.818	4.941	131.8E6	114.7E6	47.518	42.961
10)	B gamma-Chl...	5.692	4.822	148.7E6	131.1E6	49.444	45.183
11)	B alpha-Chl...	5.770	4.885	144.0E6	129.5E6	48.247	44.626
12)	B 4,4'-DDE	5.949	5.076	126.0E6	111.3E6	49.564	48.405
13)	MA Dieldrin	6.093	5.205	140.1E6	121.6E6	50.781	45.041
14)	MA Endrin	6.320	5.479	119.8E6	103.2E6	49.422	42.186
15)	B Endosulfa...	6.542	5.776	111.5E6	106.5E6	45.816	47.236
16)	A 4,4'-DDD	6.465	5.630	102.1E6	91078907	50.357	48.695
17)	MA 4,4'-DDT	6.776	5.878	87096019	78696856	38.071	37.251
18)	B Endrin al...	6.672	5.956	56174311	49431581	29.814	26.415
19)	B Endosulfa...	6.907	6.178	106.8E6	93935757	45.035	39.900
20)	A Methoxychlor	7.257	6.458	44575358	42735504	36.527	35.265
21)	B Endrin ke...	7.387	6.683	105.8E6	93595852	44.181	36.875
22)	Mirex	7.850	6.854	90174262	83783212	46.094	36.360
23)	Chlordane-1	0.000	3.640	0	250492	N.D.	2.825 #
24)	Chlordane-2	5.011f	4.207	165.7E6	626763	1391.828	5.589 #
25)	Chlordane-3	5.692	4.822	148.7E6	131.1E6	344.385	461.487 #
26)	Chlordane-4	5.770	4.885	144.0E6	129.5E6	276.966	434.114 #
27)	Chlordane-5	0.000	5.776	0	106.5E6	N.D.	1078.646 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
ECD_L
ClientSampleId :

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

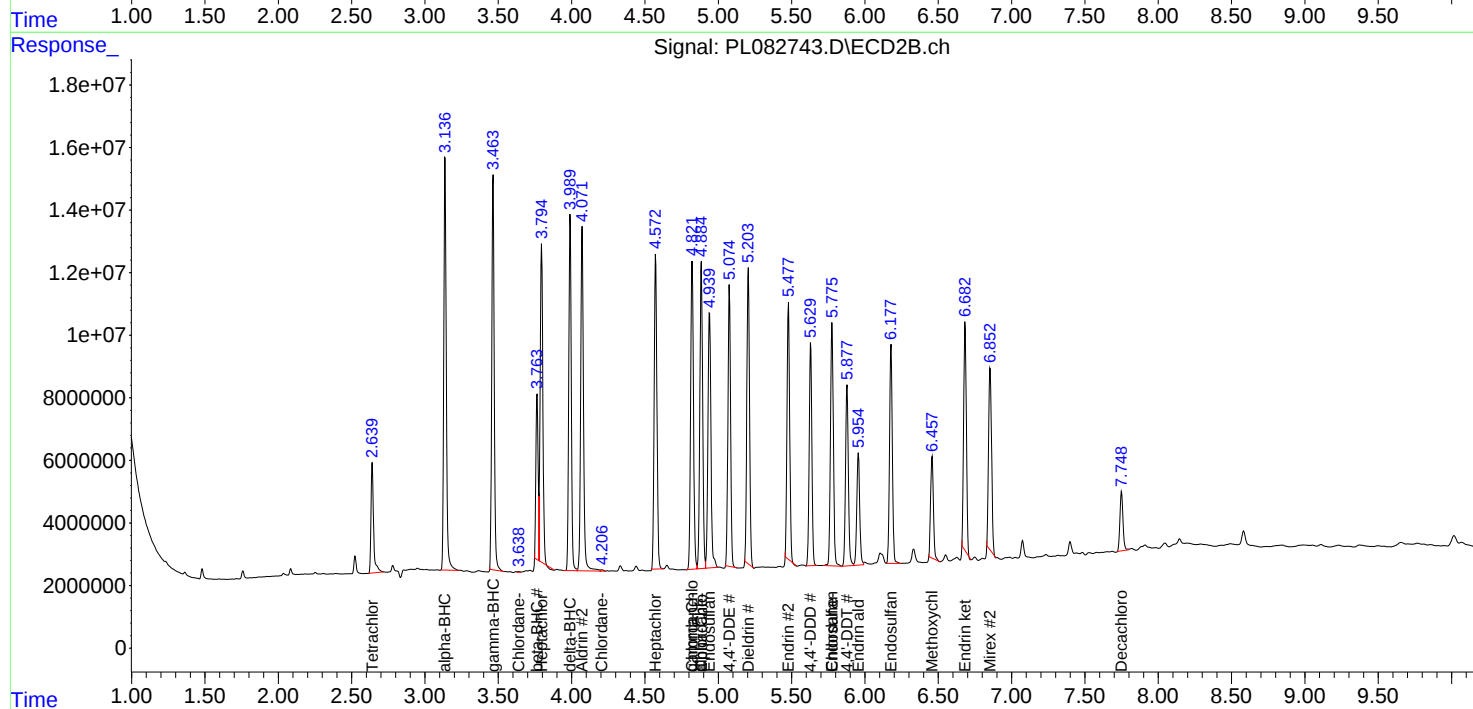


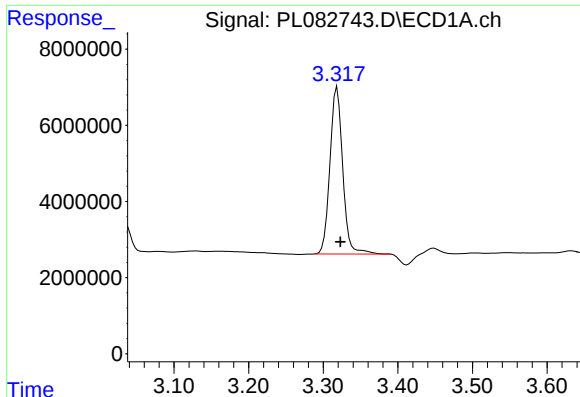

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: -0.004 min
Response: 52430167
Conc: 19.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

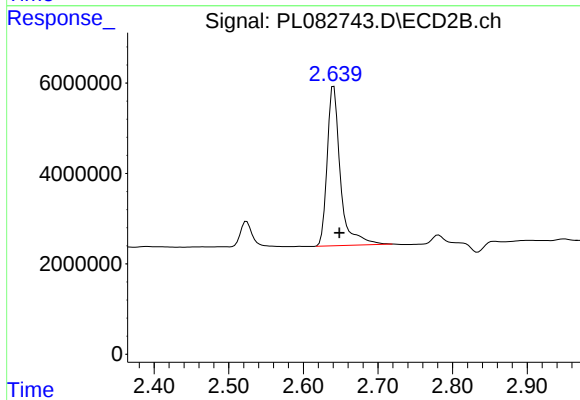


#1 Tetrachloro-m-xylene

R.T.: 2.641 min
Delta R.T.: -0.007 min
Response: 43589863
Conc: 18.82 ng/ml

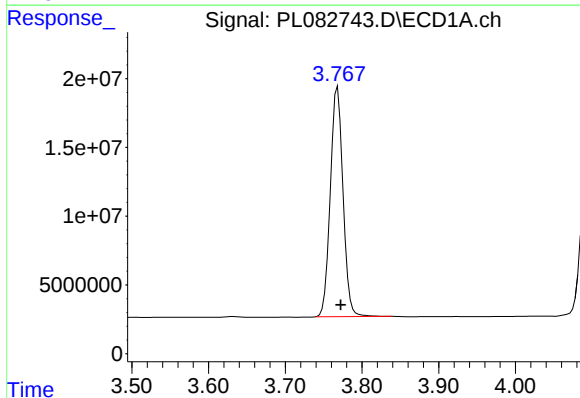


#2 alpha-BHC

R.T.: 3.768 min
Delta R.T.: -0.004 min
Response: 192063742
Conc: 48.25 ng/ml

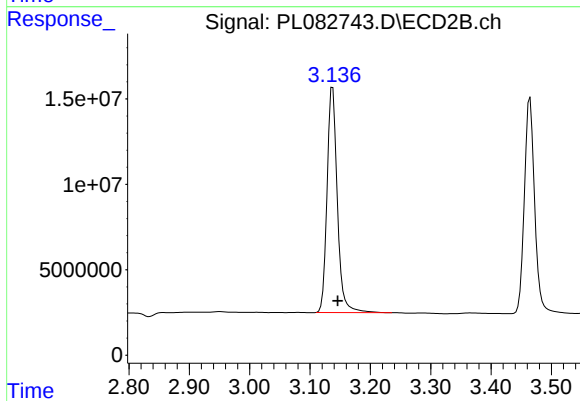

#2 alpha-BHC


R.T.: 3.137 min
Delta R.T.: -0.009 min
Response: 155933966
Conc: 45.82 ng/ml

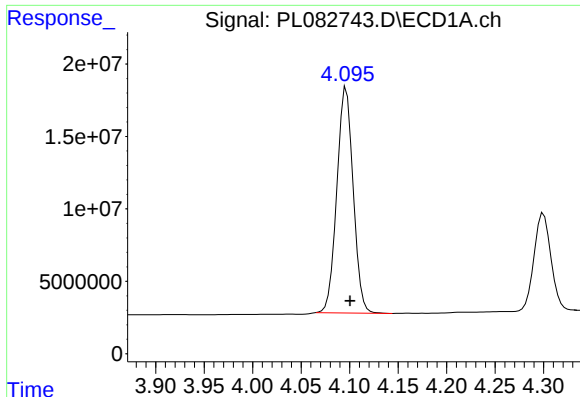

#3 gamma-BHC (Lindane)


R.T.: 4.097 min
Delta R.T.: -0.004 min
Response: 182336349
Conc: 48.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

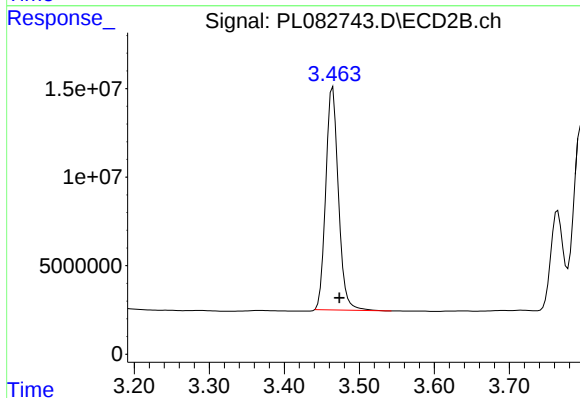


#3 gamma-BHC (Lindane)

R.T.: 3.465 min
Delta R.T.: -0.009 min
Response: 147505387
Conc: 45.88 ng/ml

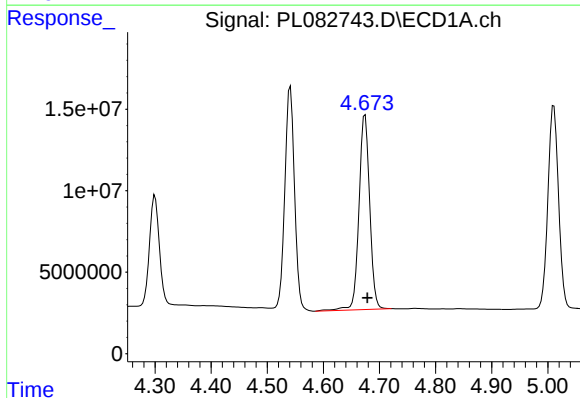


#4 Heptachlor

R.T.: 4.674 min
Delta R.T.: -0.004 min
Response: 159029652
Conc: 43.52 ng/ml

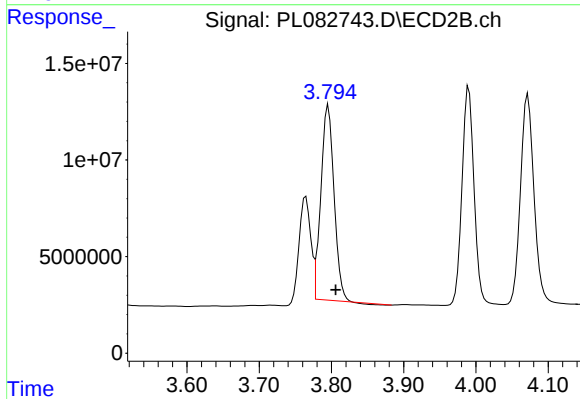

#4 Heptachlor


R.T.: 3.796 min
Delta R.T.: -0.010 min
Response: 127606687
Conc: 37.28 ng/ml

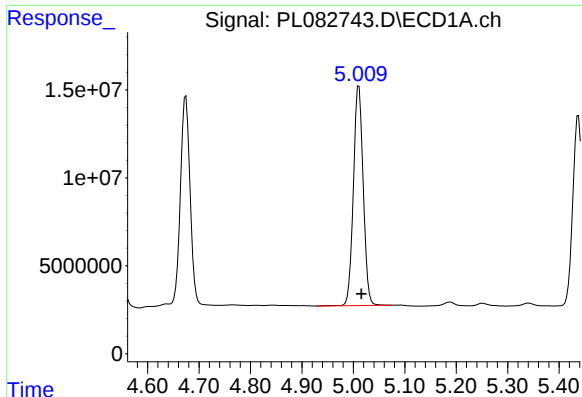

#5 Aldrin


R.T.: 5.011 min
Delta R.T.: -0.005 min
Response: 165700595
Conc: 50.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

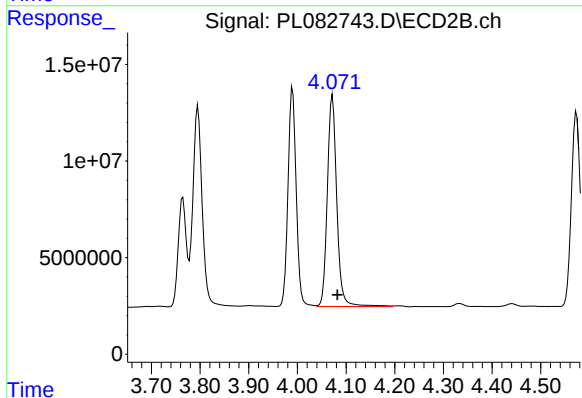


#5 Aldrin

R.T.: 4.072 min
Delta R.T.: -0.010 min
Response: 147770480
Conc: 46.91 ng/ml

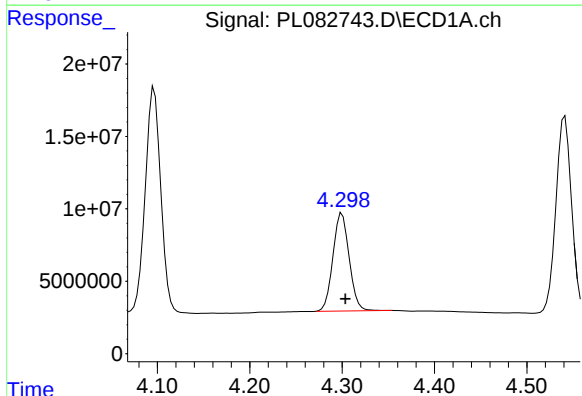


#6 beta-BHC

R.T.: 4.300 min
Delta R.T.: -0.004 min
Response: 82899364
Conc: 48.61 ng/ml

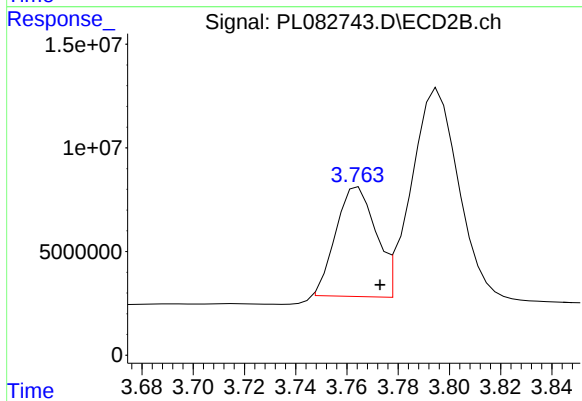

#6 beta-BHC


R.T.: 3.765 min
Delta R.T.: -0.008 min
Response: 56632542
Conc: 41.51 ng/ml

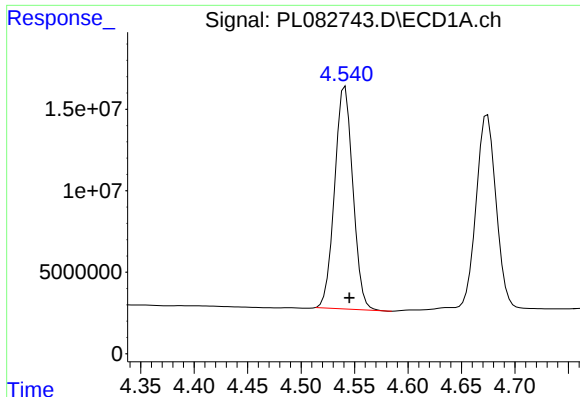

#7 delta-BHC


R.T.: 4.541 min
Delta R.T.: -0.004 min
Response: 161762171
Conc: 44.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

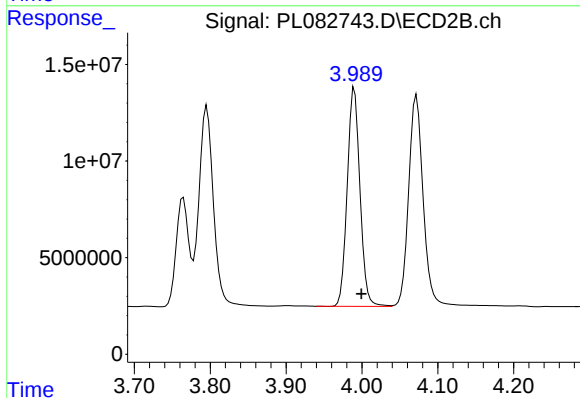


#7 delta-BHC

R.T.: 3.990 min
Delta R.T.: -0.009 min
Response: 132224457
Conc: 43.11 ng/ml

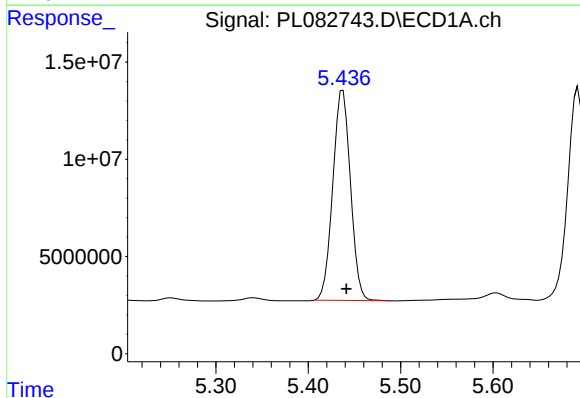


#8 Heptachlor epoxide

R.T.: 5.437 min
Delta R.T.: -0.004 min
Response: 143566481
Conc: 47.07 ng/ml

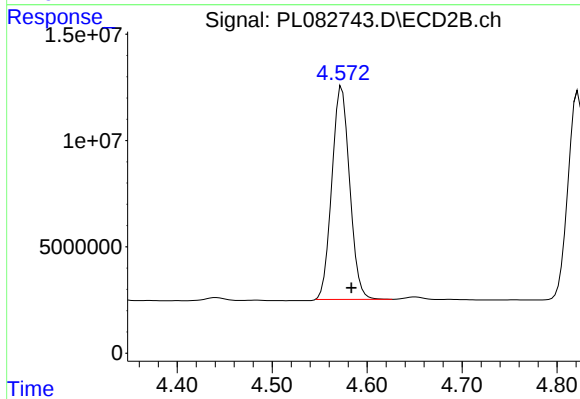

#8 Heptachlor epoxide


R.T.: 4.573 min
Delta R.T.: -0.010 min
Response: 130642847
Conc: 45.35 ng/ml

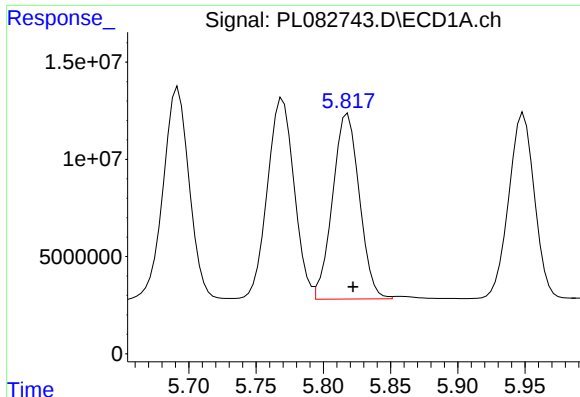

#9 Endosulfan I


R.T.: 5.818 min
Delta R.T.: -0.004 min
Response: 131755058
Conc: 47.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

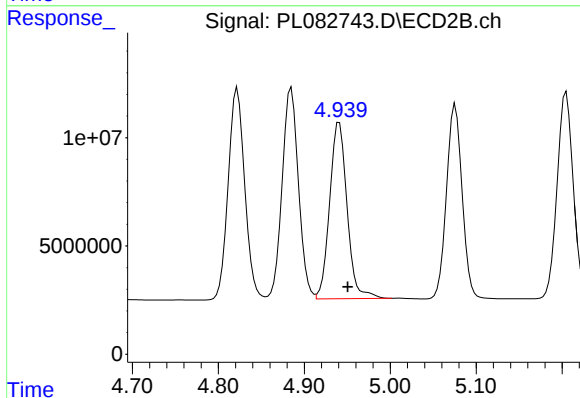


#9 Endosulfan I

R.T.: 4.941 min
Delta R.T.: -0.010 min
Response: 114682538
Conc: 42.96 ng/ml

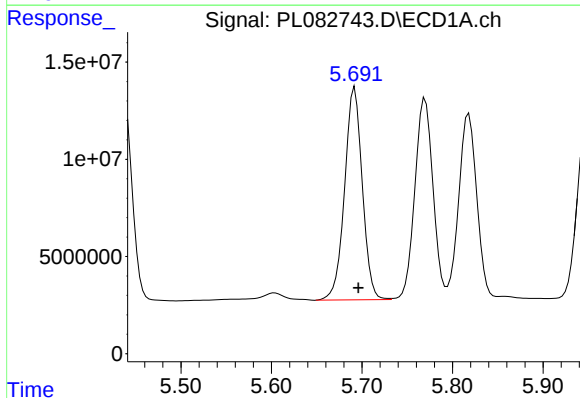


#10 gamma-Chlordane

R.T.: 5.692 min
Delta R.T.: -0.004 min
Response: 148672112
Conc: 49.44 ng/ml

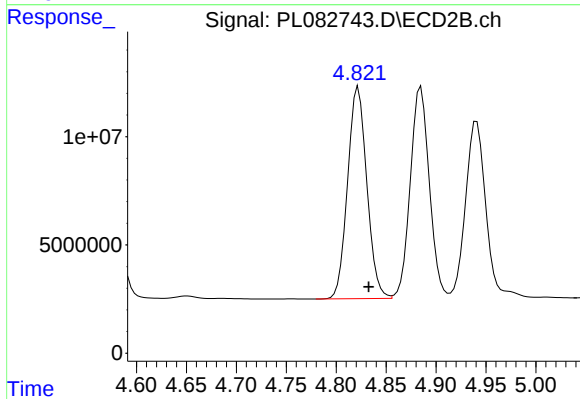

#10 gamma-Chlordane


R.T.: 4.822 min
Delta R.T.: -0.010 min
Response: 131112913
Conc: 45.18 ng/ml

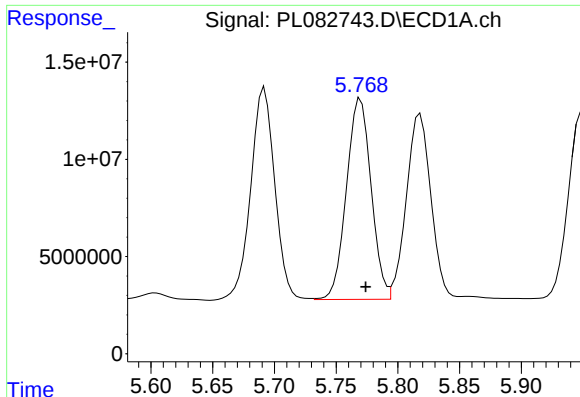

#11 alpha-Chlordane


R.T.: 5.770 min
Delta R.T.: -0.004 min
Response: 143998914
Conc: 48.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

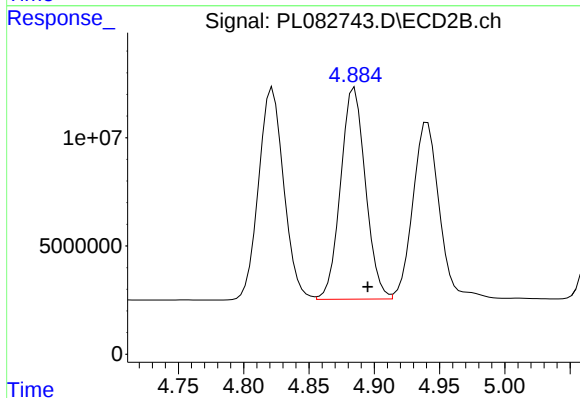


#11 alpha-Chlordane

R.T.: 4.885 min
Delta R.T.: -0.010 min
Response: 129542410
Conc: 44.63 ng/ml

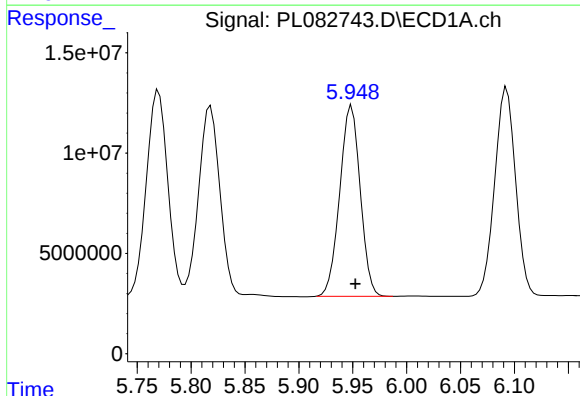


#12 4,4'-DDE

R.T.: 5.949 min
Delta R.T.: -0.003 min
Response: 125992708
Conc: 49.56 ng/ml

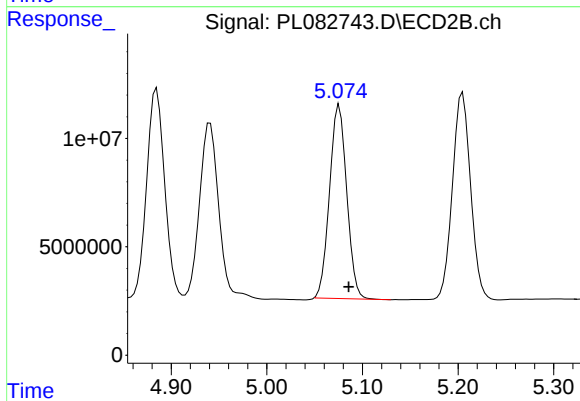

#12 4,4'-DDE


R.T.: 5.076 min
Delta R.T.: -0.010 min
Response: 111281754
Conc: 48.41 ng/ml

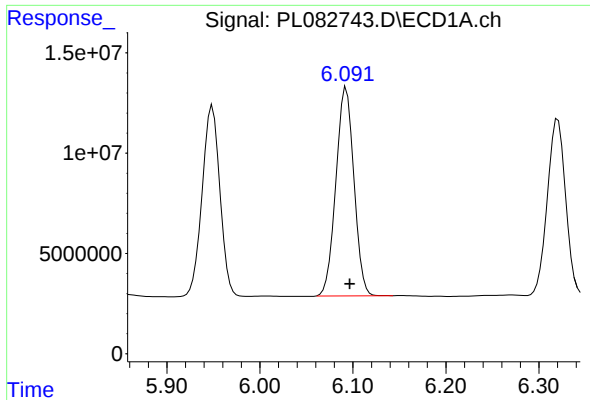

#13 Dieldrin


R.T.: 6.093 min
Delta R.T.: -0.004 min
Response: 140110901
Conc: 50.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

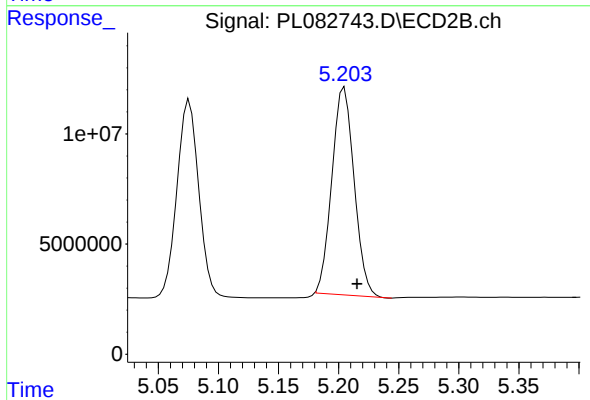


#13 Dieldrin

R.T.: 5.205 min
Delta R.T.: -0.011 min
Response: 121627538
Conc: 45.04 ng/ml

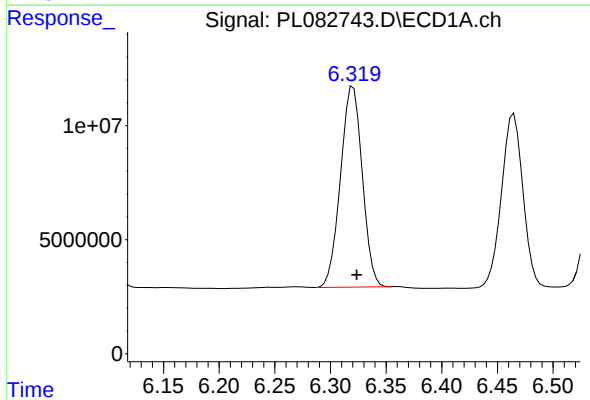


#14 Endrin

R.T.: 6.320 min
Delta R.T.: -0.003 min
Response: 119827362
Conc: 49.42 ng/ml

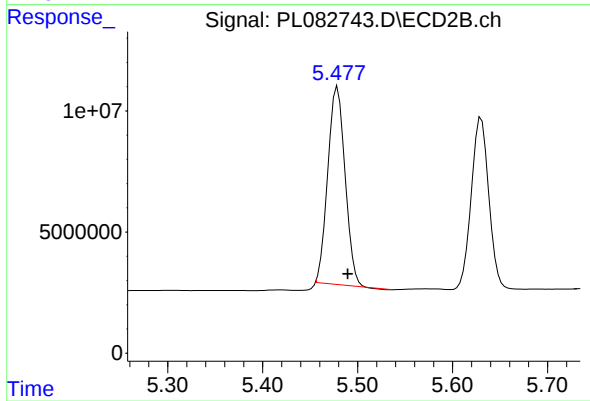

#14 Endrin


R.T.: 5.479 min
Delta R.T.: -0.011 min
Response: 103184846
Conc: 42.19 ng/ml

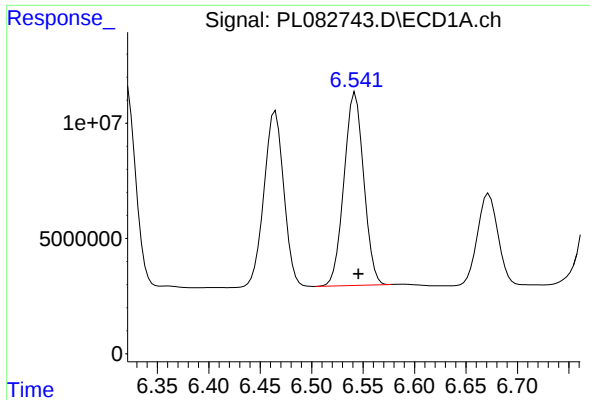

#15 Endosulfan II


R.T.: 6.542 min
Delta R.T.: -0.003 min
Response: 111541324
Conc: 45.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

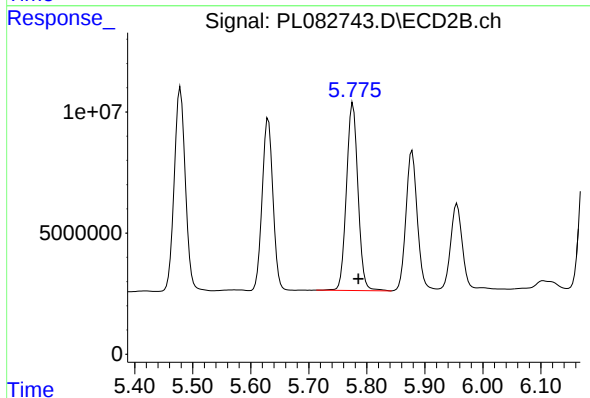


#15 Endosulfan II

R.T.: 5.776 min
Delta R.T.: -0.010 min
Response: 106475776
Conc: 47.24 ng/ml

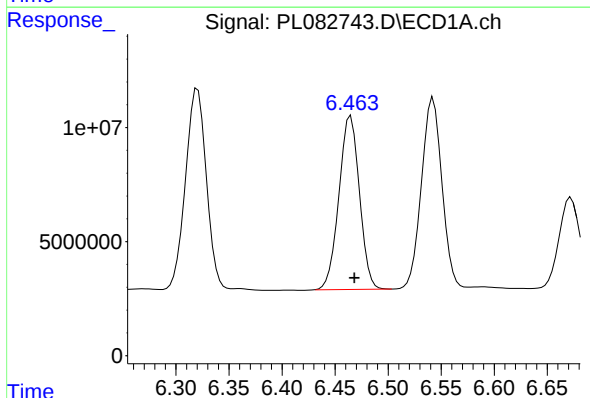


#16 4,4'-DDD

R.T.: 6.465 min
Delta R.T.: -0.003 min
Response: 102083303
Conc: 50.36 ng/ml

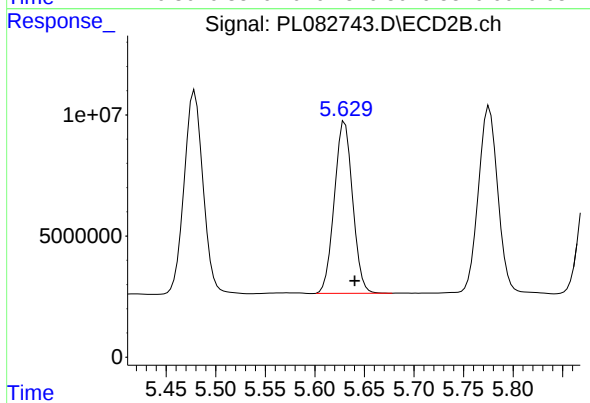

#16 4,4'-DDD


R.T.: 5.630 min
Delta R.T.: -0.010 min
Response: 91078907
Conc: 48.69 ng/ml

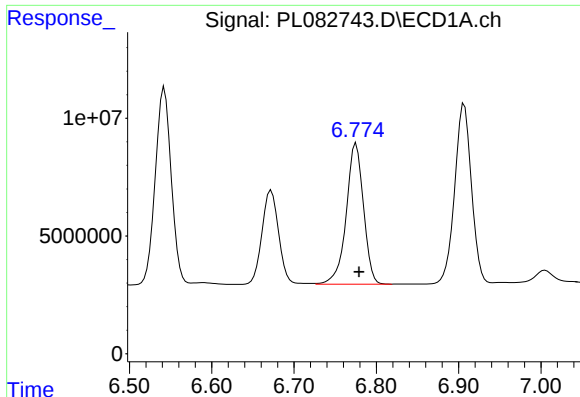

#17 4,4'-DDT


R.T.: 6.776 min
Delta R.T.: -0.003 min
Response: 87096019
Conc: 38.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

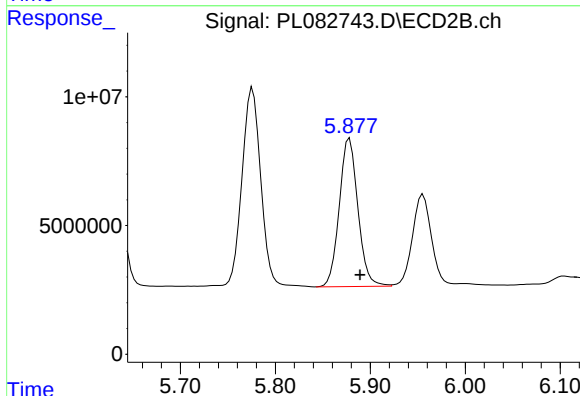


#17 4,4'-DDT

R.T.: 5.878 min
Delta R.T.: -0.011 min
Response: 78696856
Conc: 37.25 ng/ml

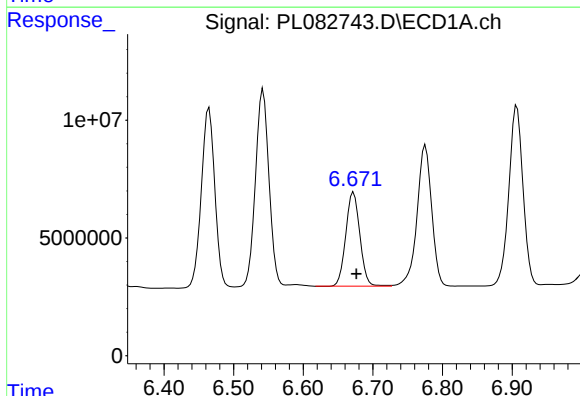


#18 Endrin aldehyde

R.T.: 6.672 min
Delta R.T.: -0.004 min
Response: 56174311
Conc: 29.81 ng/ml

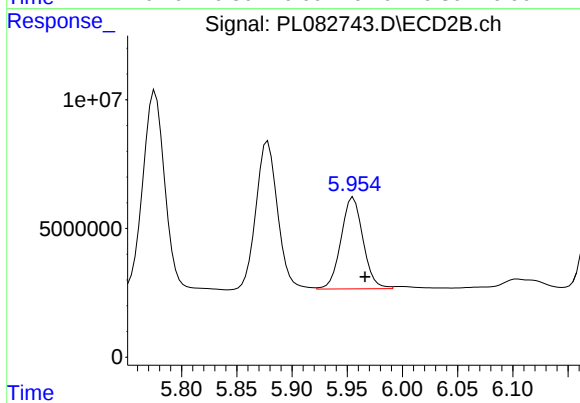

#18 Endrin aldehyde


R.T.: 5.956 min
Delta R.T.: -0.011 min
Response: 49431581
Conc: 26.41 ng/ml

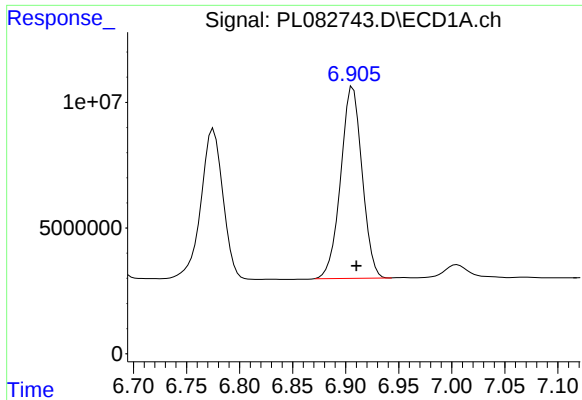

#19 Endosulfan Sulfate


R.T.: 6.907 min
Delta R.T.: -0.003 min
Response: 106802496
Conc: 45.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

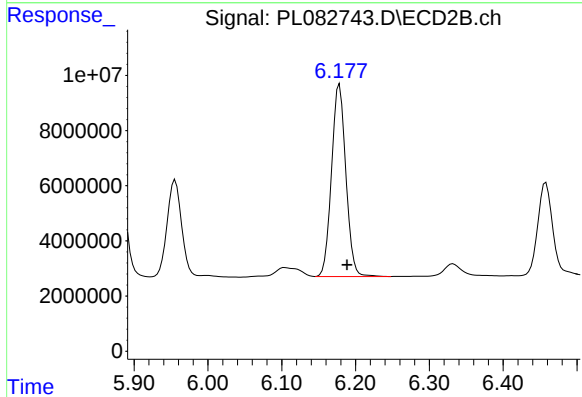


#19 Endosulfan Sulfate

R.T.: 6.178 min
Delta R.T.: -0.010 min
Response: 93935757
Conc: 39.90 ng/ml

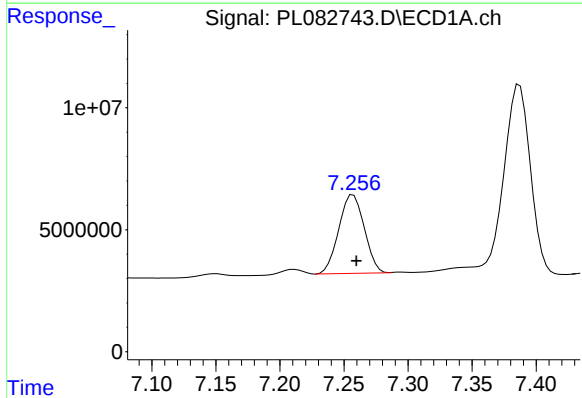


#20 Methoxychlor

R.T.: 7.257 min
Delta R.T.: -0.003 min
Response: 44575358
Conc: 36.53 ng/ml

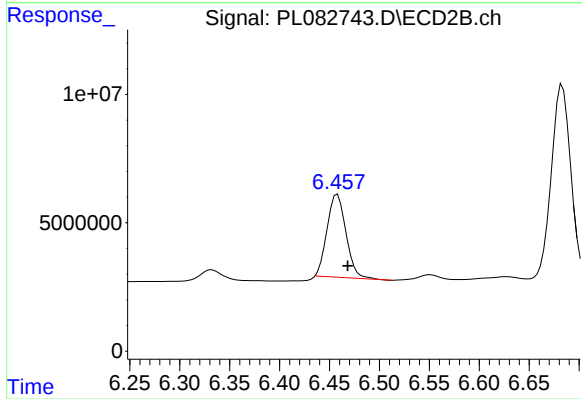

#20 Methoxychlor


R.T.: 6.458 min
Delta R.T.: -0.010 min
Response: 42735504
Conc: 35.27 ng/ml

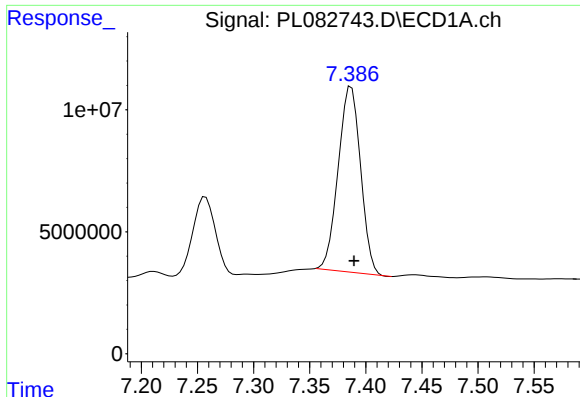

#21 Endrin ketone


R.T.: 7.387 min
Delta R.T.: -0.002 min
Response: 105787154
Conc: 44.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

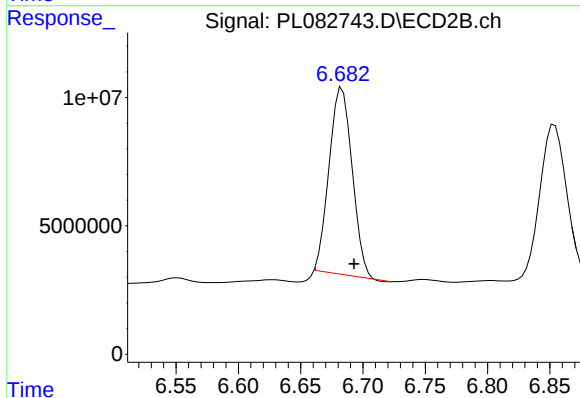


#21 Endrin ketone

R.T.: 6.683 min
Delta R.T.: -0.010 min
Response: 93595852
Conc: 36.88 ng/ml

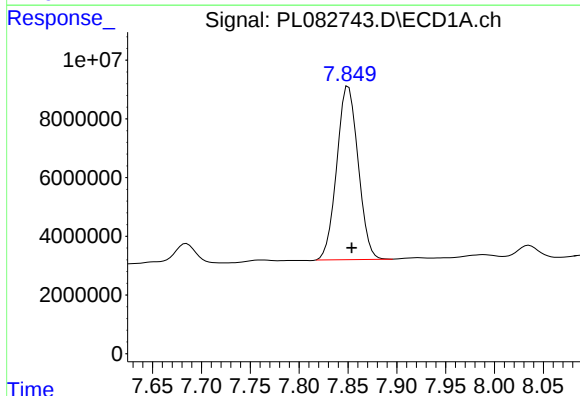


#22 Mirex

R.T.: 7.850 min
Delta R.T.: -0.003 min
Response: 90174262
Conc: 46.09 ng/ml

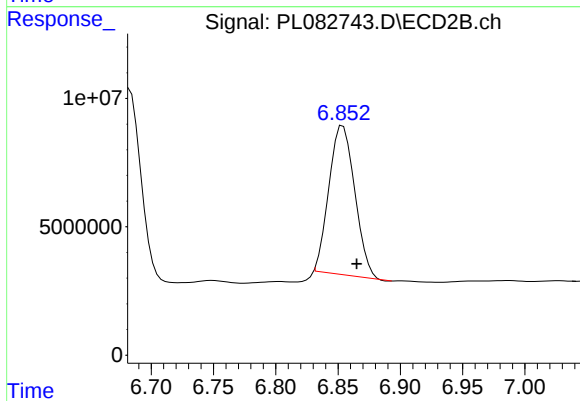

#22 Mirex


R.T.: 6.854 min
Delta R.T.: -0.011 min
Response: 83783212
Conc: 36.36 ng/ml

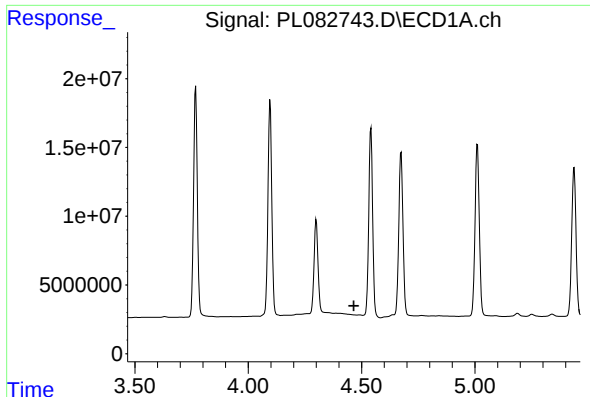

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.466 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

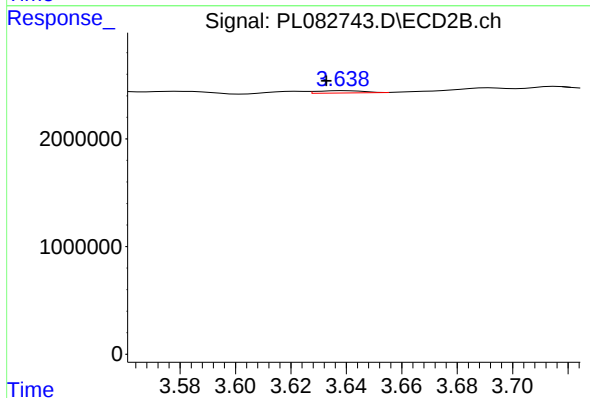


#23 Chlordane-1

R.T.: 3.640 min
Delta R.T.: 0.007 min
Response: 250492
Conc: 2.82 ng/ml

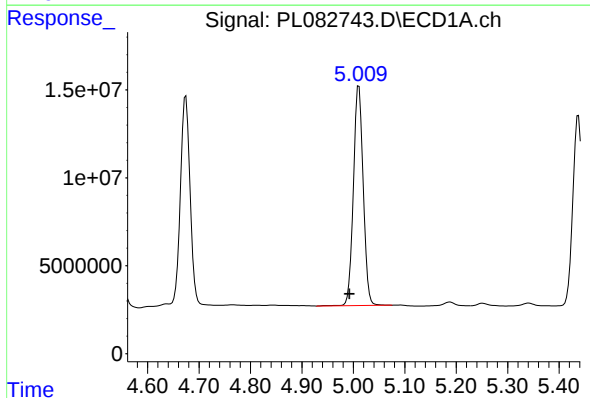


#24 Chlordane-2

R.T.: 5.011 min
Delta R.T.: 0.018 min
Response: 165700595
Conc: 1391.83 ng/ml

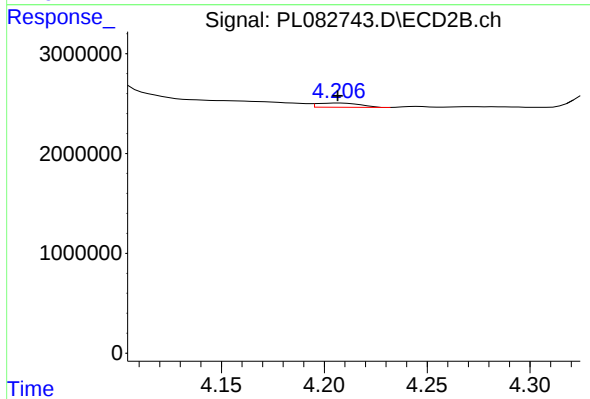

#24 Chlordane-2


R.T.: 4.207 min
Delta R.T.: 0.000 min
Response: 626763
Conc: 5.59 ng/ml

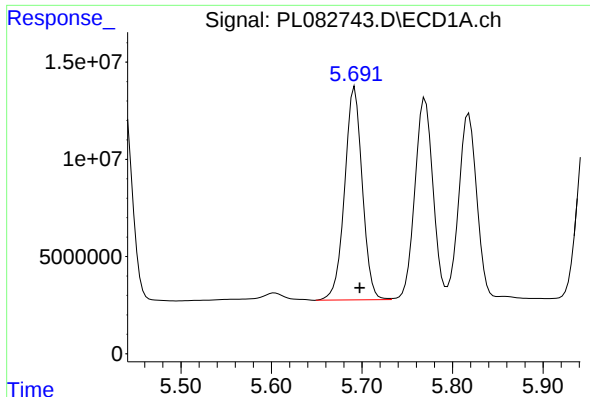

#25 Chlordane-3


R.T.: 5.692 min
Delta R.T.: -0.006 min
Response: 148672112
Conc: 344.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

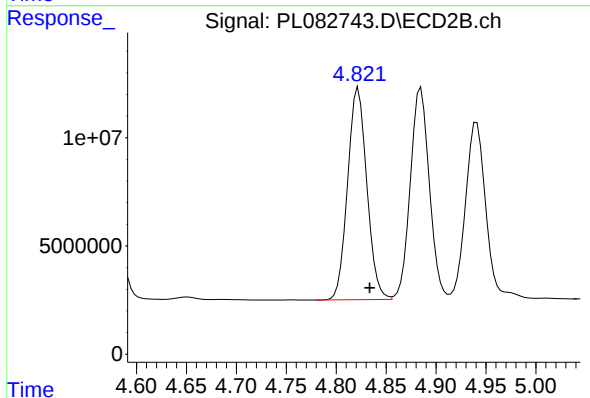


#25 Chlordane-3

R.T.: 4.822 min
Delta R.T.: -0.012 min
Response: 131112913
Conc: 461.49 ng/ml

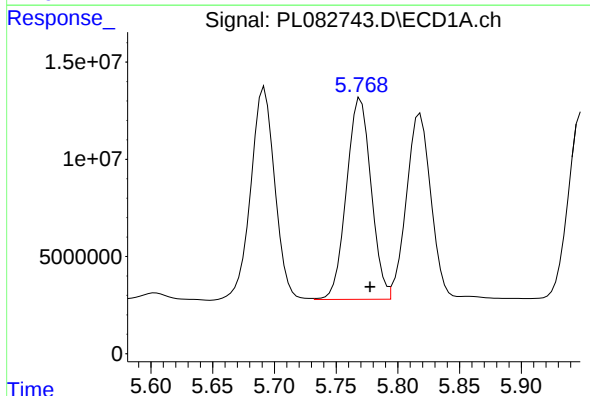


#26 Chlordane-4

R.T.: 5.770 min
Delta R.T.: -0.008 min
Response: 143998914
Conc: 276.97 ng/ml

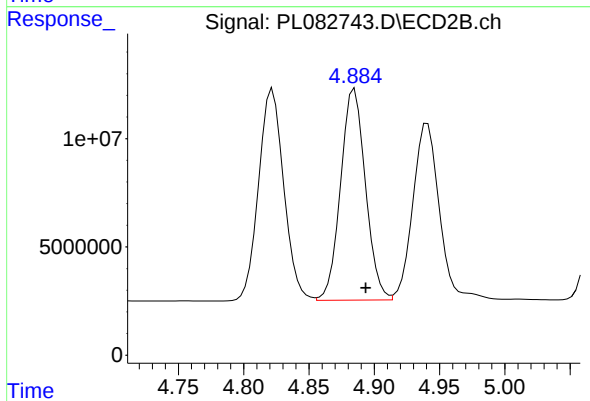

#26 Chlordane-4


R.T.: 4.885 min
Delta R.T.: -0.009 min
Response: 129542410
Conc: 434.11 ng/ml

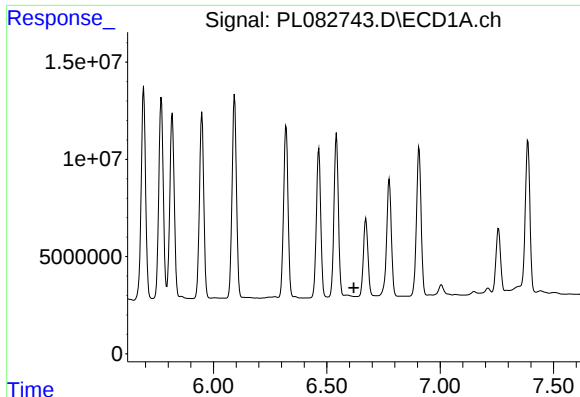

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.619 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

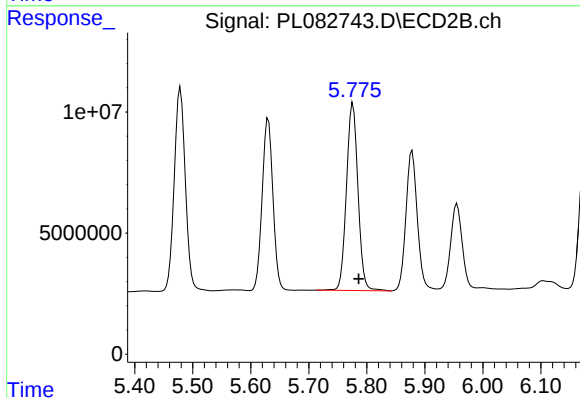


#27 Chlordane-5

R.T.: 5.776 min
Delta R.T.: -0.010 min
Response: 106475776
Conc: 1078.65 ng/ml

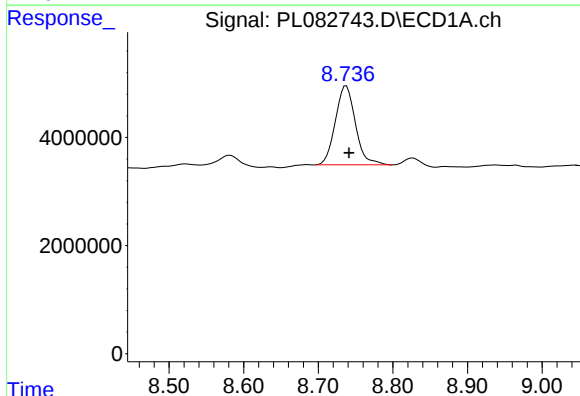

#28 Decachlorobiphenyl

R.T.: 8.738 min
Delta R.T.: -0.003 min
Response: 27357126
Conc: 14.33 ng/ml

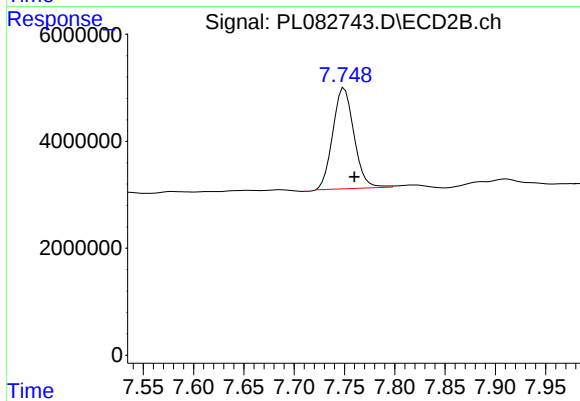

#28 Decachlorobiphenyl

R.T.: 7.750 min
Delta R.T.: -0.010 min
Response: 27616152
Conc: 12.10 ng/ml