

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051625\
 Data File : PL095712.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2025 09:58
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 01:54:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
 Quant Title : GC Extractables
 QLast Update : Tue May 13 14:38:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

5) MB Aldrin	5.297f	0.000	2769542	0	0.482	N.D. #
8) B Heptachlo...	5.749	0.000	222.1E6	0	42.854	N.D. #
13) MA Dieldrin	0.000	5.550f	0	38524755	N.D.	6.261 #
14) MA Endrin	0.000	5.813	0	8055839	N.D.	1.512 #
15) B Endosulfa...	0.000	6.097	0	6621488	N.D.	1.209 #
16) A 4,4'-DDD	6.765f	0.000	98902262	0	25.453	N.D. #
19) B Endosulfa...	7.198	0.000	9686117	0	2.639	N.D. #
24) Chlordane-2	5.297	4.498	2769542	-264032	10.040	N.D. #
27) Chlordane-5	0.000	6.097	0	6621488	N.D.	23.053 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051625\
Data File : PL095712.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2025 09:58
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 01:54:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
Quant Title : GC Extractables
QLast Update : Tue May 13 14:38:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

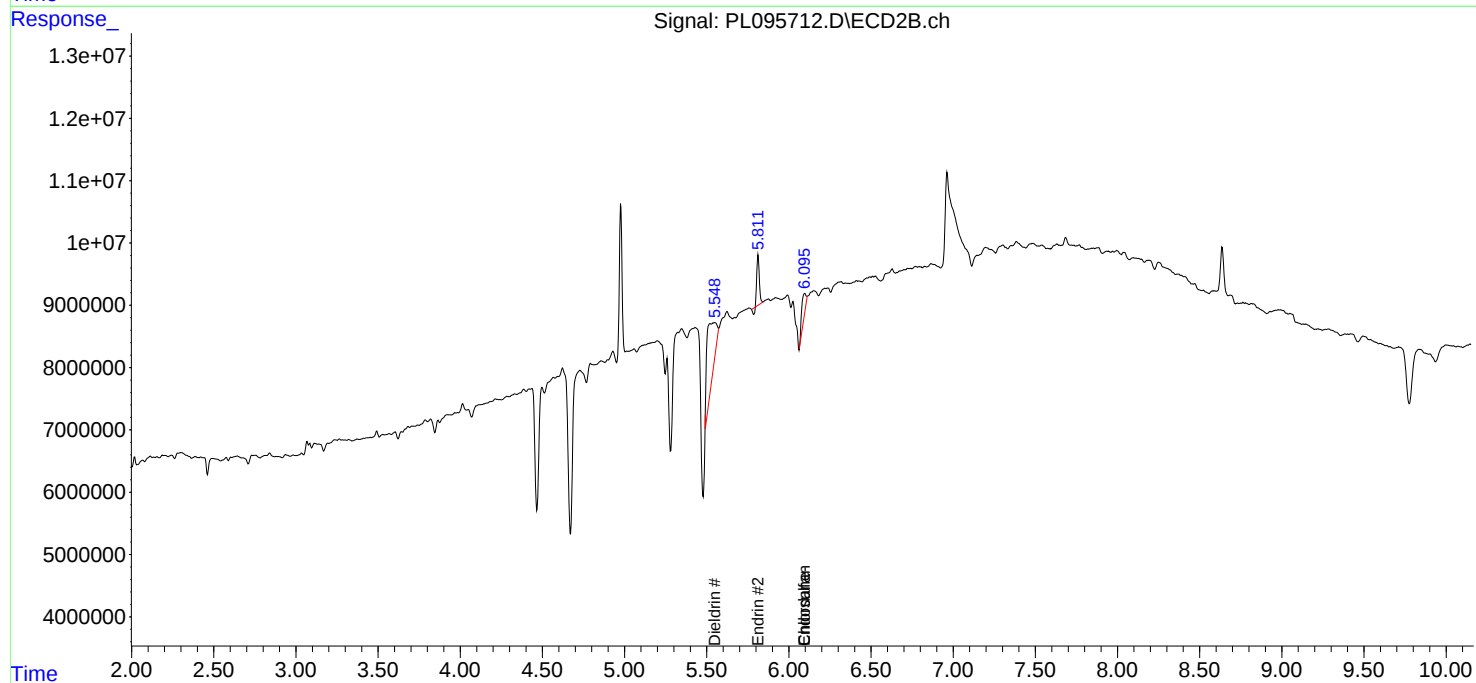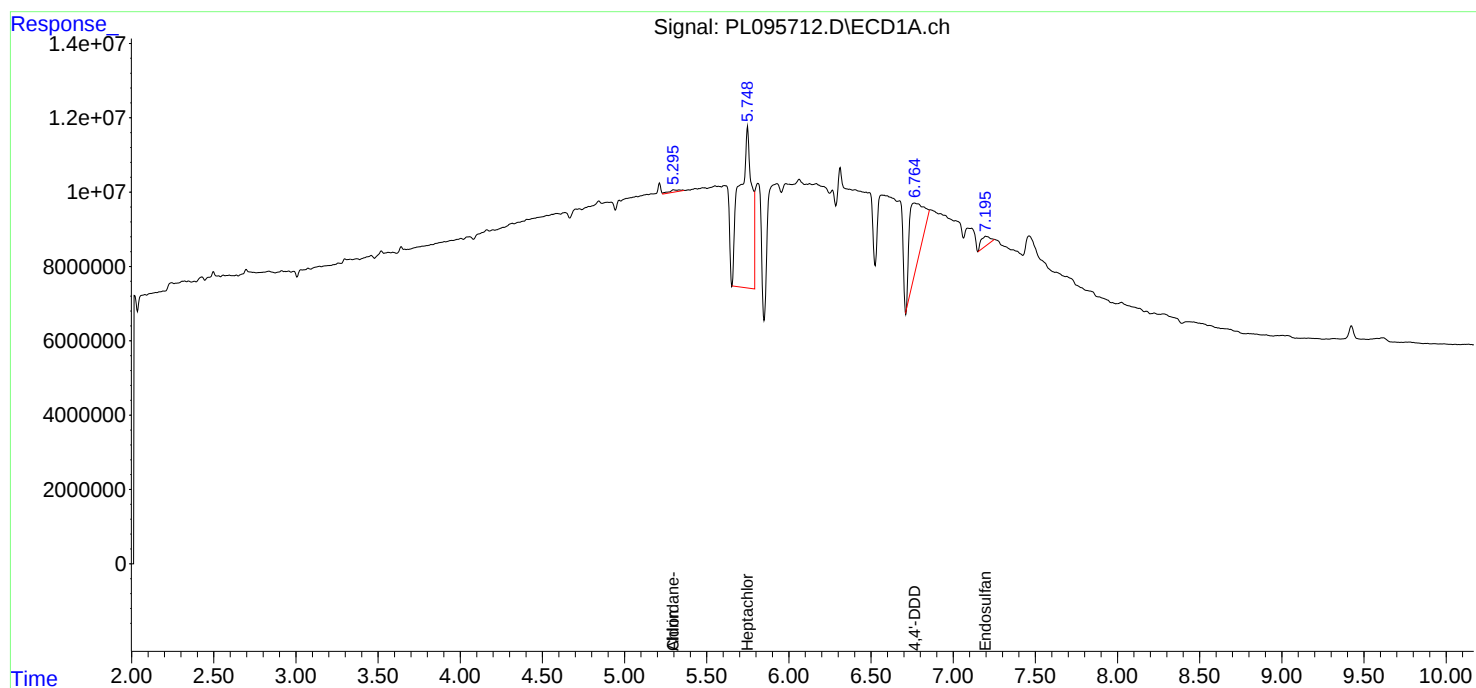


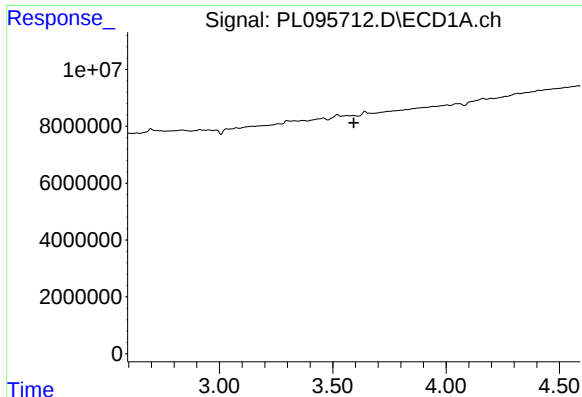

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.593 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

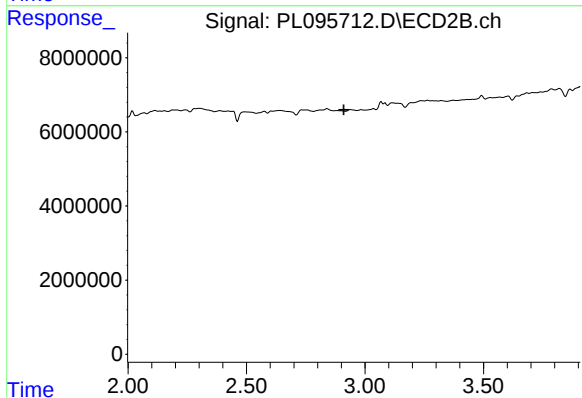


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.910 min
Response: 0
Conc: N.D.

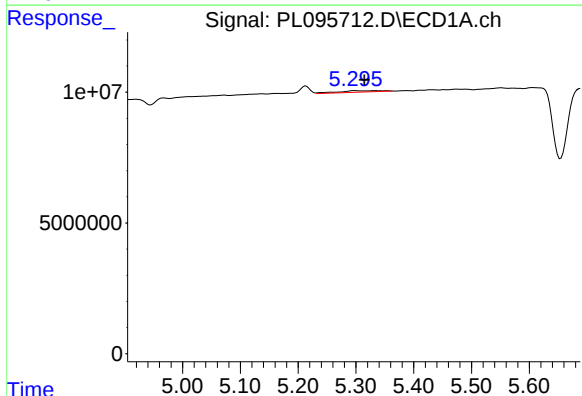


#5 Aldrin

R.T.: 5.297 min
Delta R.T.: -0.017 min
Response: 2769542
Conc: 0.48 ng/ml

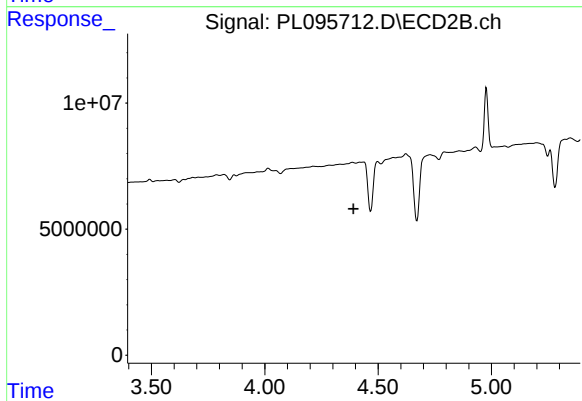

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.392 min
Response: 0
Conc: N.D.

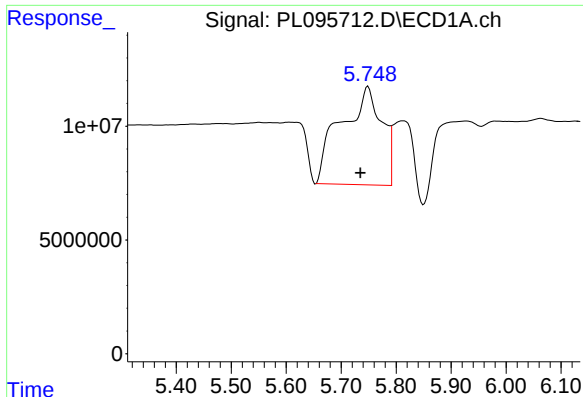

#8 Heptachlor epoxide


R.T.: 5.749 min
Delta R.T.: 0.014 min
Response: 222066433
Conc: 42.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

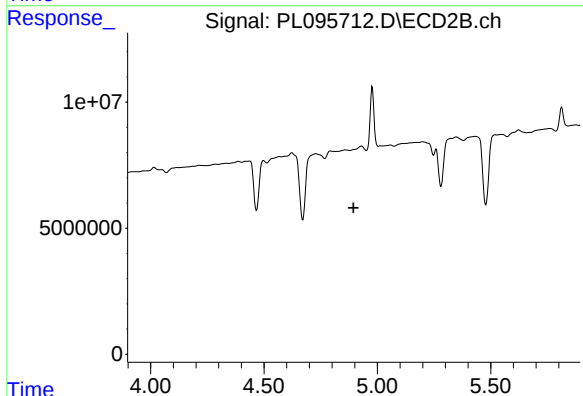


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.895 min
Response: 0
Conc: N.D.

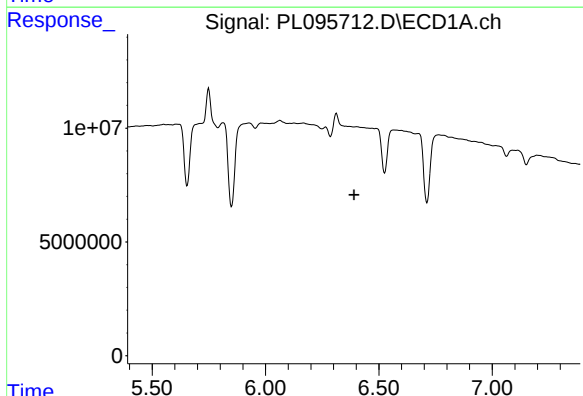


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.391 min
Response: 0
Conc: N.D.

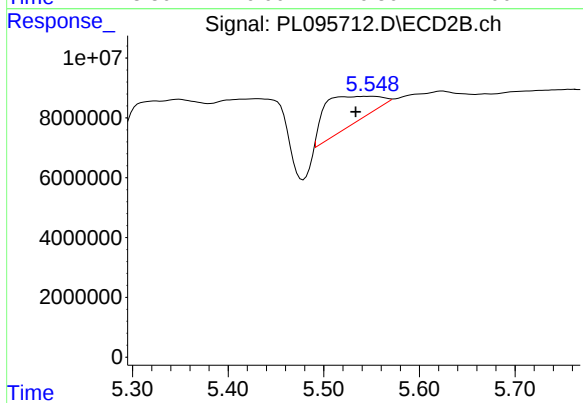

#13 Dieldrin


R.T.: 5.550 min
Delta R.T.: 0.017 min
Response: 38524755
Conc: 6.26 ng/ml

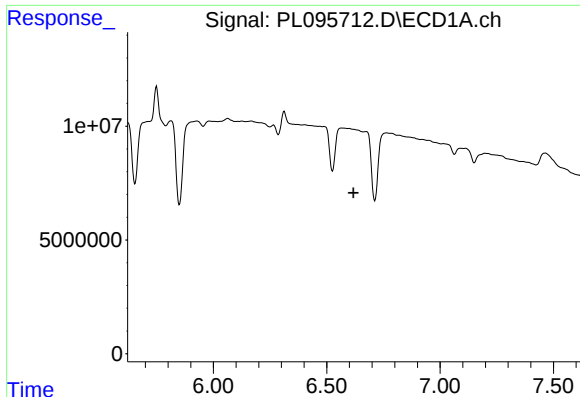

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.619 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

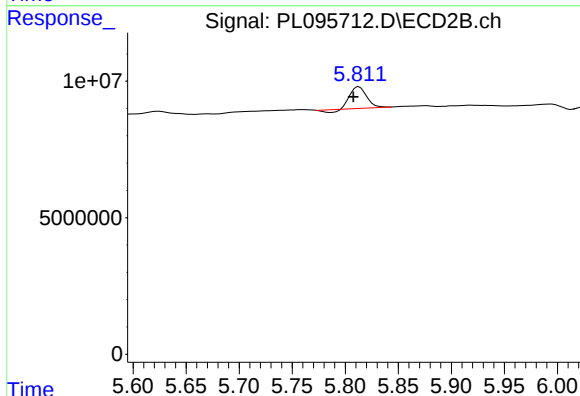


#14 Endrin

R.T.: 5.813 min
Delta R.T.: 0.005 min
Response: 8055839
Conc: 1.51 ng/ml

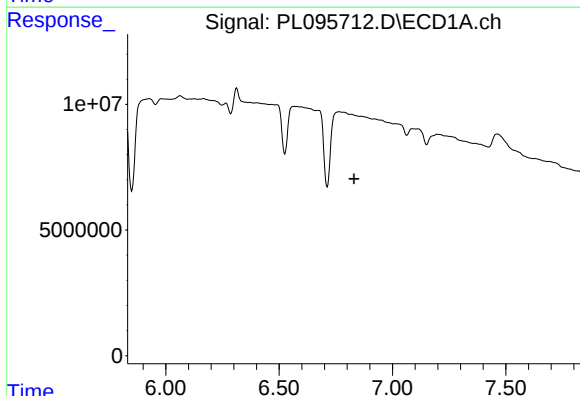


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.831 min
Response: 0
Conc: N.D.

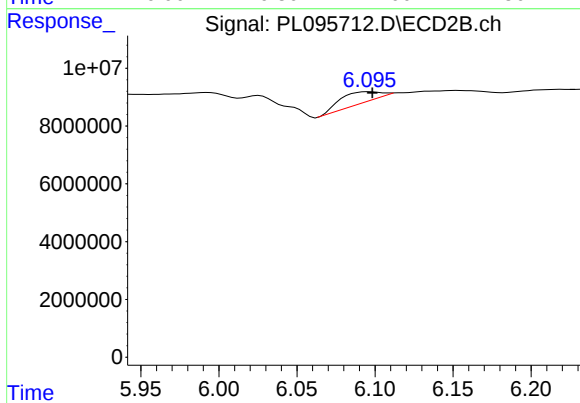

#15 Endosulfan II


R.T.: 6.097 min
Delta R.T.: -0.002 min
Response: 6621488
Conc: 1.21 ng/ml

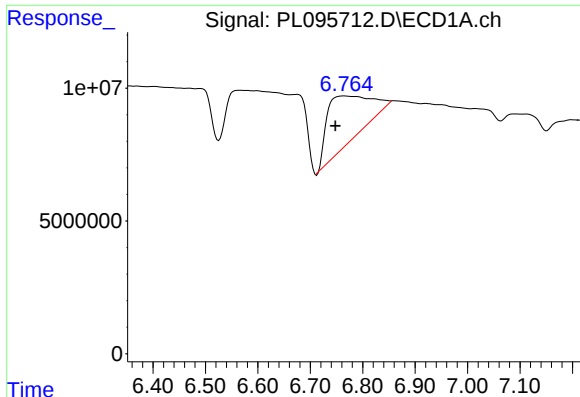

#16 4,4'-DDD


R.T.: 6.765 min
Delta R.T.: 0.018 min
Response: 98902262
Conc: 25.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

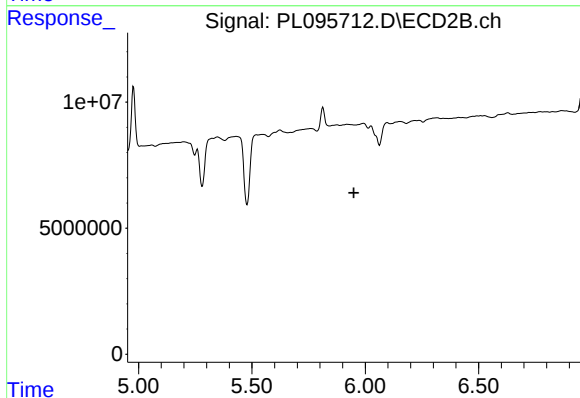


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

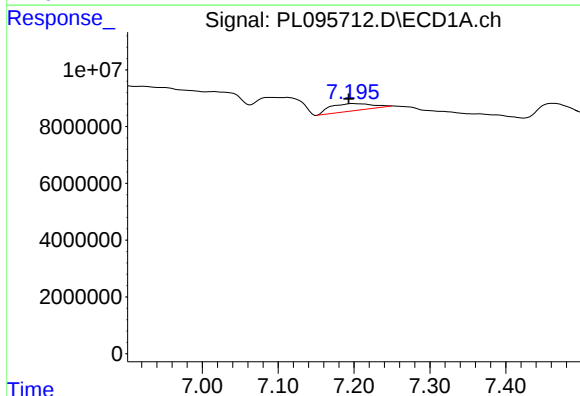


#19 Endosulfan Sulfate

R.T.: 7.198 min
Delta R.T.: 0.005 min
Response: 9686117
Conc: 2.64 ng/ml

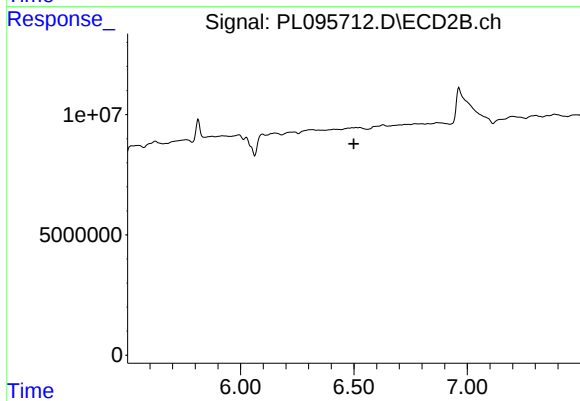

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.499 min
Response: 0
Conc: N.D.

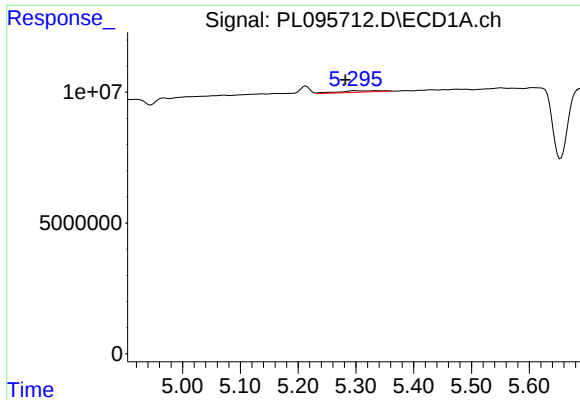

#24 Chlordane-2


R.T.: 5.297 min
Delta R.T.: 0.015 min
Response: 2769542
Conc: 10.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

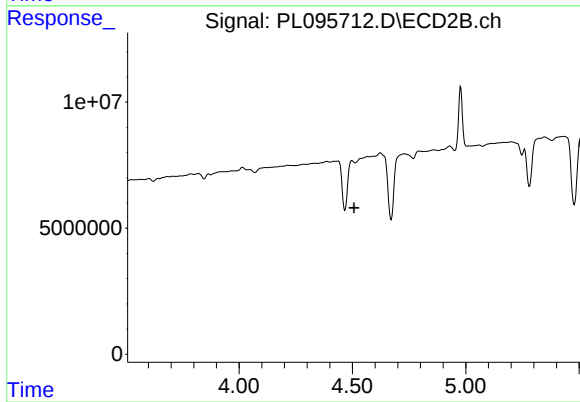


#24 Chlordane-2

R.T.: 4.498 min
Delta R.T.: -0.009 min
Response: -264032
Conc: N.D.

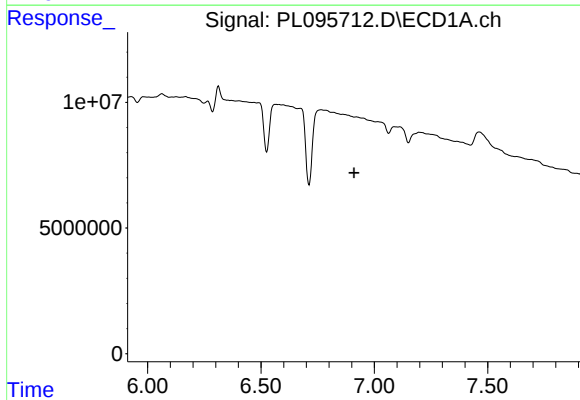


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.911 min
Response: 0
Conc: N.D.

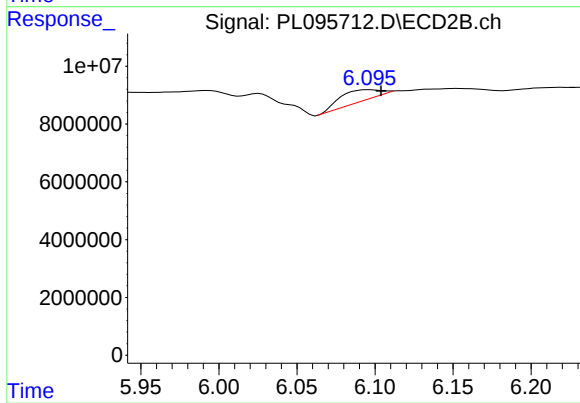

#27 Chlordane-5


R.T.: 6.097 min
Delta R.T.: -0.007 min
Response: 6621488
Conc: 23.05 ng/ml

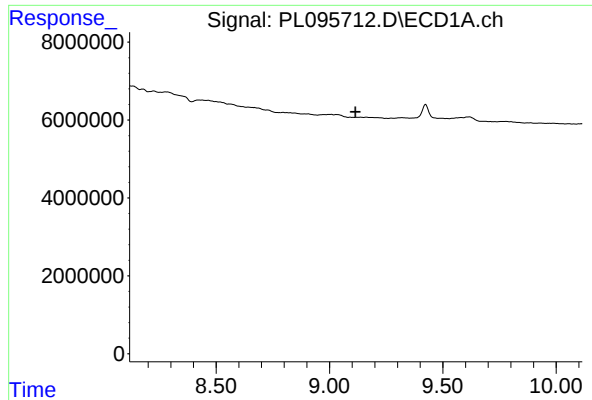

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.115 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

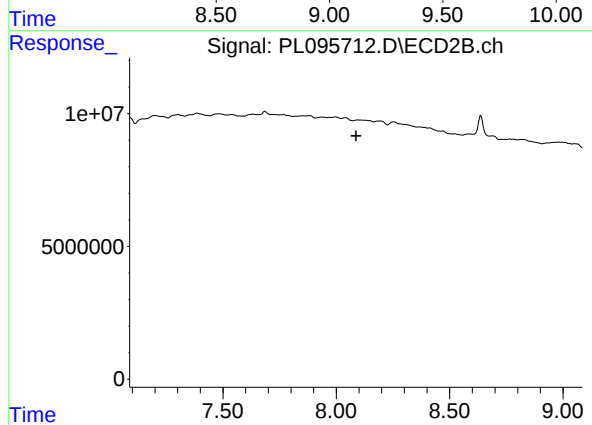

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.087 min
Response: 0
Conc: N.D.