

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051625\
 Data File : PL095713.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2025 10:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 01:54:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
 Quant Title : GC Extractables
 QLast Update : Tue May 13 14:38:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.593	2.909	77703479	79614973	19.017	16.997
28)	SA Decachlor...	9.118	8.087	73139401	80094870	21.560	19.418
Target Compounds							
5)	MB Aldrin	5.300	0.000	1943683	0	0.338	N.D. #
7)	B delta-BHC	4.818	0.000	4495213	0	0.827	N.D. #
8)	B Heptachlo...	5.726	0.000	112.5E6	0	21.717	N.D. #
13)	MA Dieldrin	0.000	5.553f	0	34217712	N.D.	5.561 #
14)	MA Endrin	0.000	5.812	0	19988077	N.D.	3.752 #
15)	B Endosulfa...	6.813f	6.093	8136439	8701360	1.952	1.589
16)	A 4,4'-DDD	6.738	0.000	19515114	0	5.022	N.D. #
27)	Chlordane-5	0.000	6.093	0	8701360	N.D.	30.294 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051625\
Data File : PL095713.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2025 10:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 01:54:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
Quant Title : GC Extractables
QLast Update : Tue May 13 14:38:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

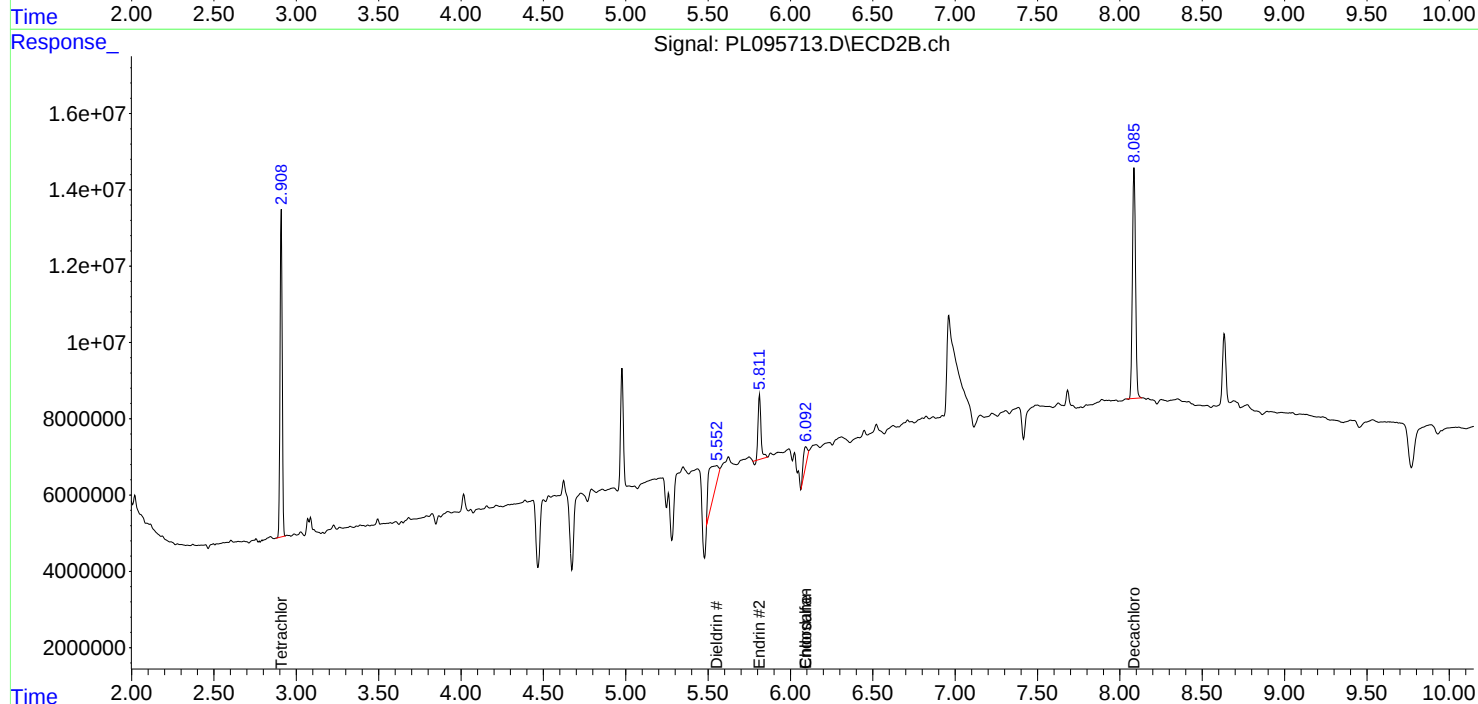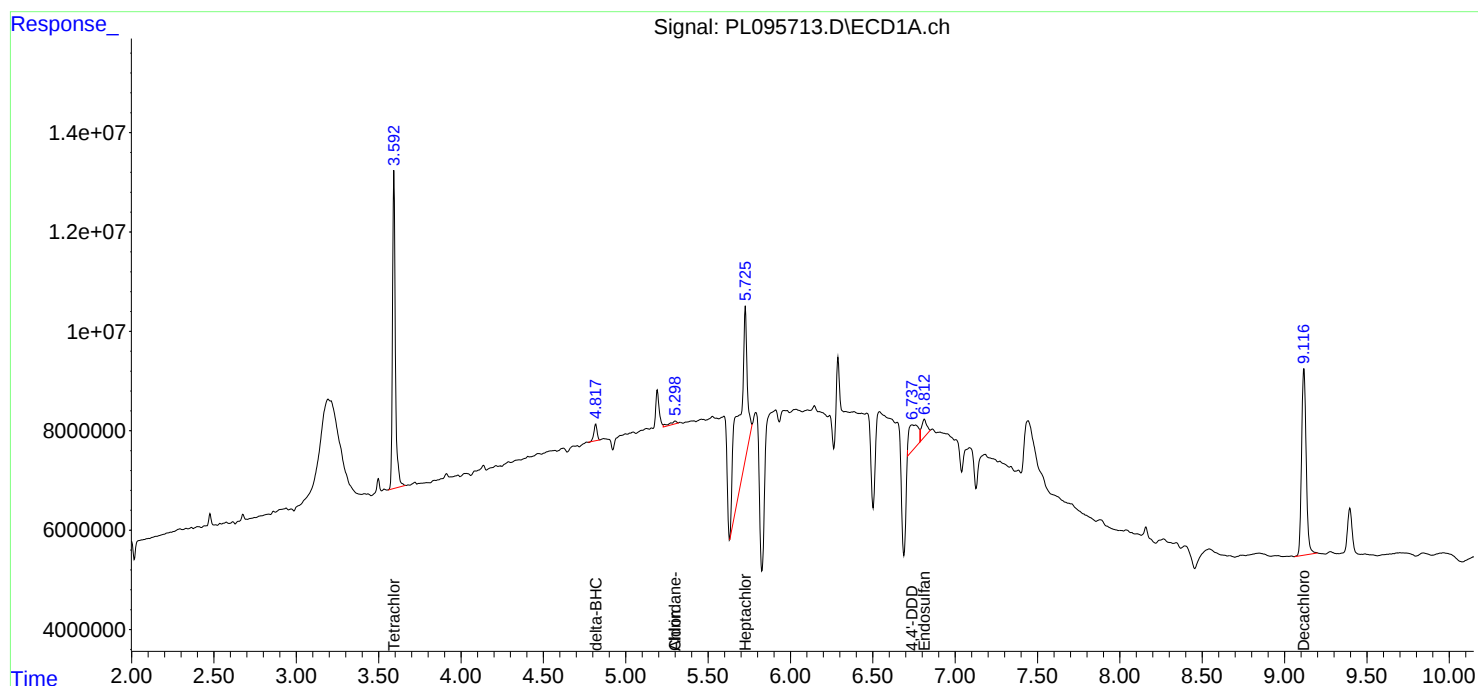


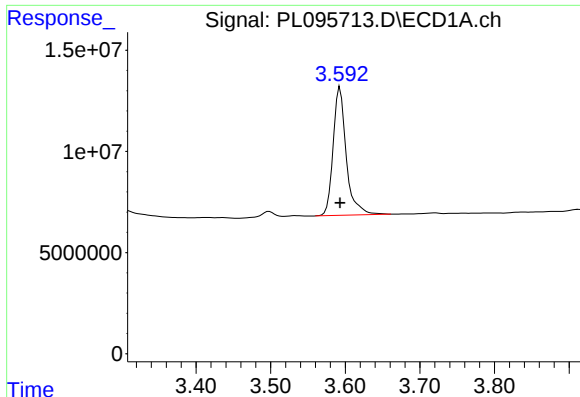

#1 Tetrachloro-m-xylene


R.T.: 3.593 min
Delta R.T.: 0.000 min
Response: 77703479
Conc: 19.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

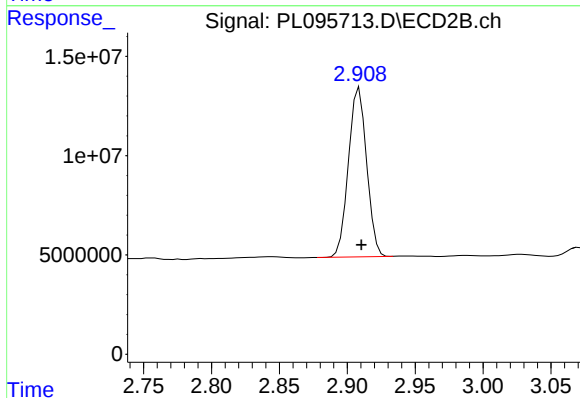


#1 Tetrachloro-m-xylene

R.T.: 2.909 min
Delta R.T.: -0.002 min
Response: 79614973
Conc: 17.00 ng/ml

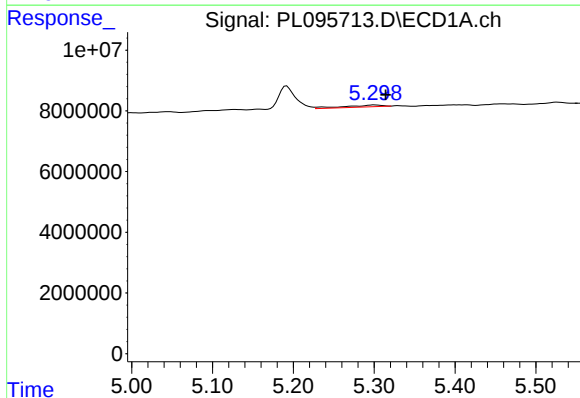


#5 Aldrin

R.T.: 5.300 min
Delta R.T.: -0.014 min
Response: 1943683
Conc: 0.34 ng/ml

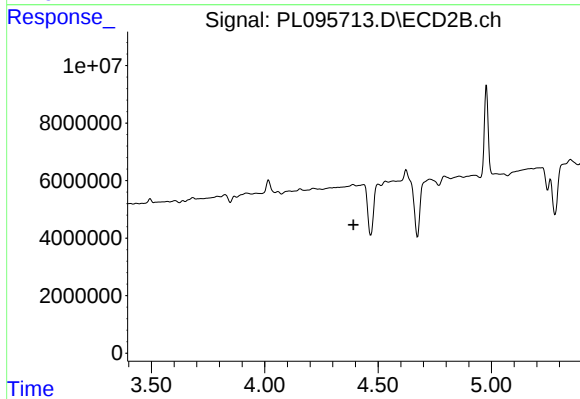

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 4.392 min
Response: 0
Conc: N.D.

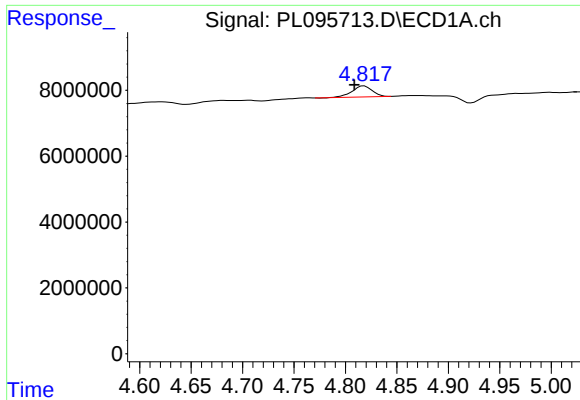

#7 delta-BHC


R.T.: 4.818 min
Delta R.T.: 0.010 min
Response: 4495213
Conc: 0.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

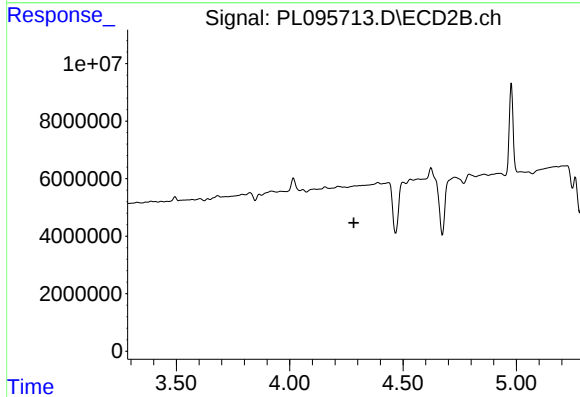


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.283 min
Response: 0
Conc: N.D.

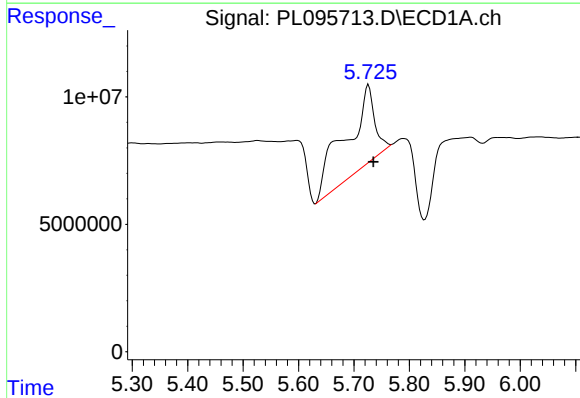


#8 Heptachlor epoxide

R.T.: 5.726 min
Delta R.T.: -0.009 min
Response: 112536264
Conc: 21.72 ng/ml

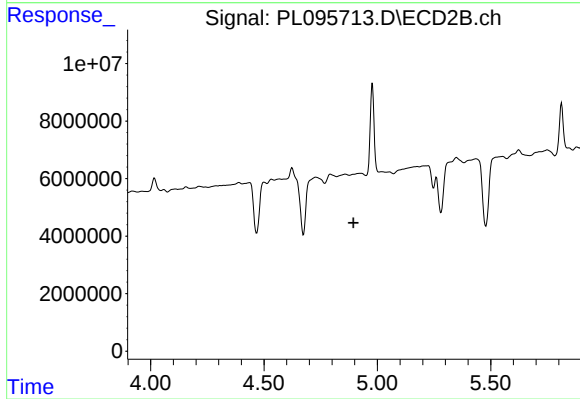

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.895 min
Response: 0
Conc: N.D.

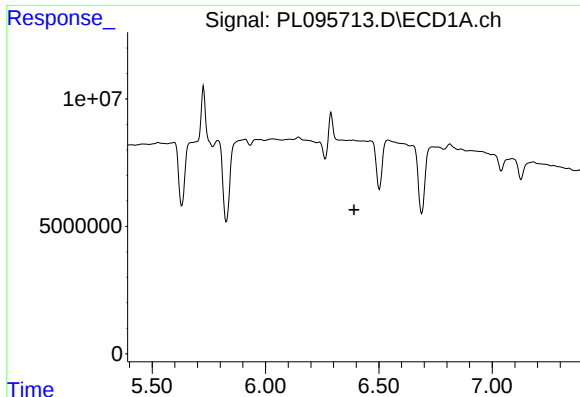

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

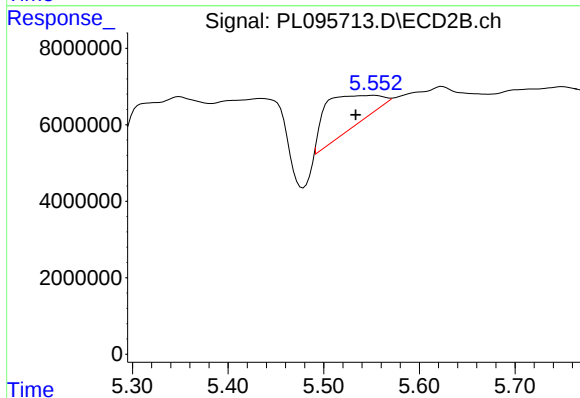


#13 Dieldrin

R.T.: 5.553 min
Delta R.T.: 0.020 min
Response: 34217712
Conc: 5.56 ng/ml

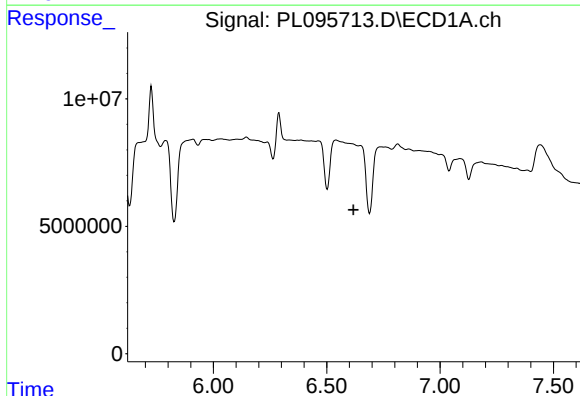


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.619 min
Response: 0
Conc: N.D.

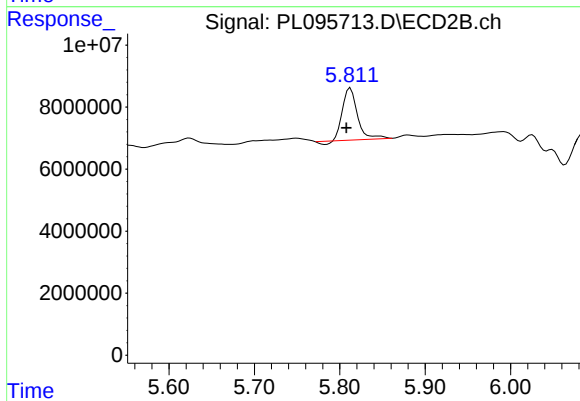

#14 Endrin


R.T.: 5.812 min
Delta R.T.: 0.005 min
Response: 19988077
Conc: 3.75 ng/ml

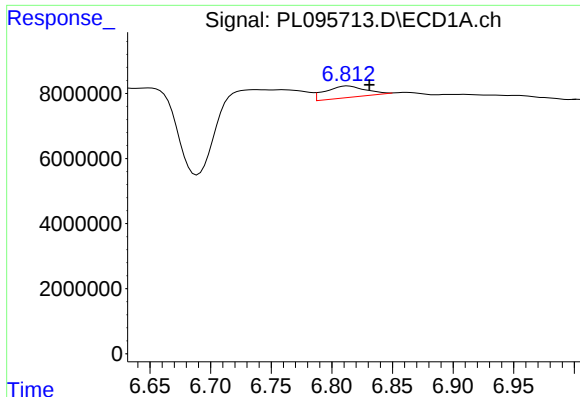

#15 Endosulfan II


R.T.: 6.813 min
Delta R.T.: -0.018 min
Response: 8136439
Conc: 1.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

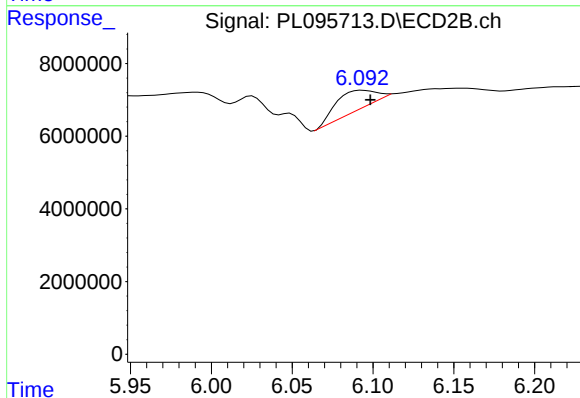


#15 Endosulfan II

R.T.: 6.093 min
Delta R.T.: -0.005 min
Response: 8701360
Conc: 1.59 ng/ml

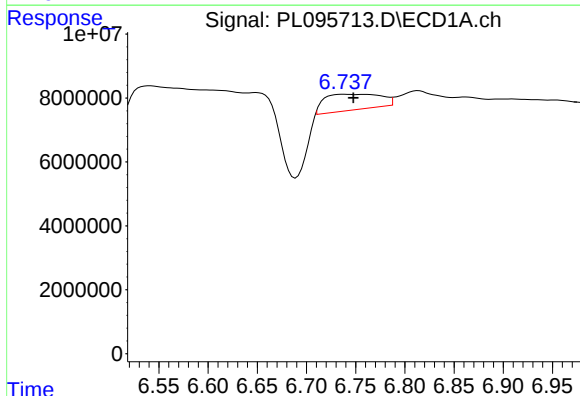


#16 4,4'-DDD

R.T.: 6.738 min
Delta R.T.: -0.010 min
Response: 19515114
Conc: 5.02 ng/ml

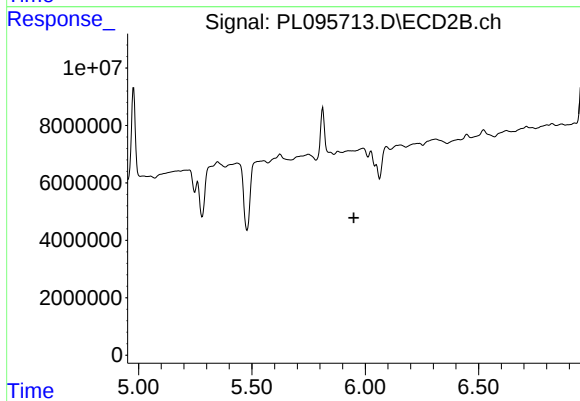

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.949 min
Response: 0
Conc: N.D.

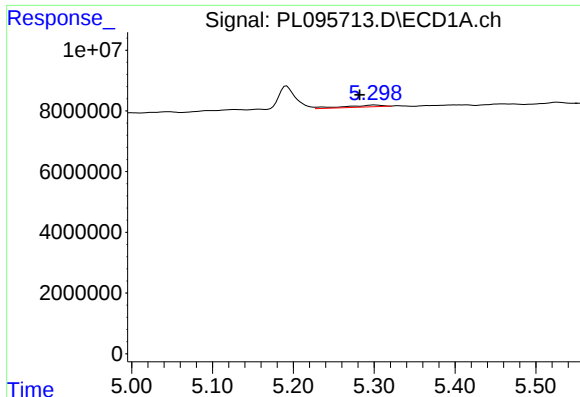

#24 Chlordane-2


R.T.: 5.300 min
Delta R.T.: 0.018 min
Response: 1943683
Conc: 7.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

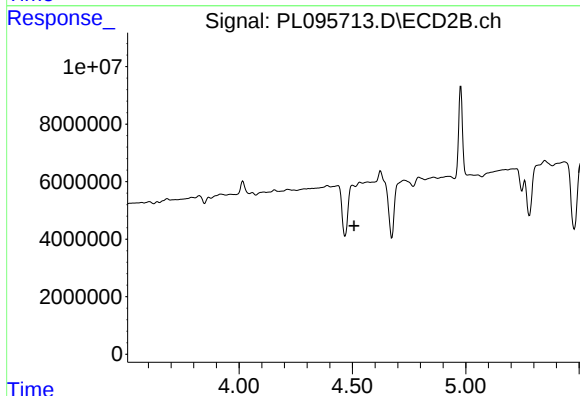


#24 Chlordane-2

R.T.: 4.501 min
Delta R.T.: -0.007 min
Response: -2270030
Conc: N.D.

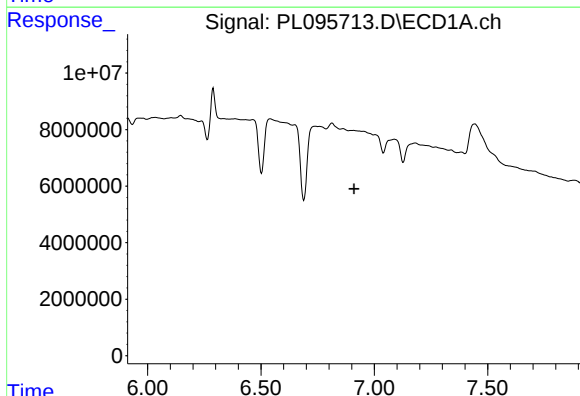


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.911 min
Response: 0
Conc: N.D.

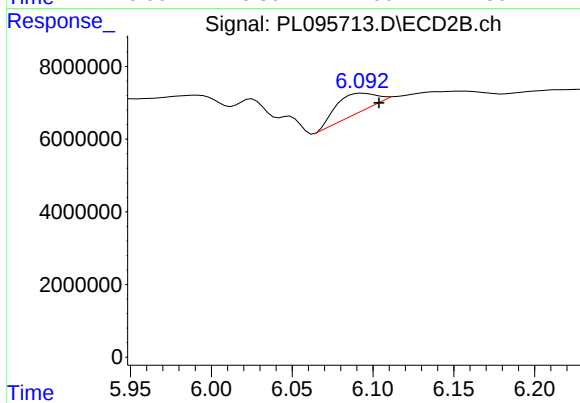

#27 Chlordane-5


R.T.: 6.093 min
Delta R.T.: -0.010 min
Response: 8701360
Conc: 30.29 ng/ml

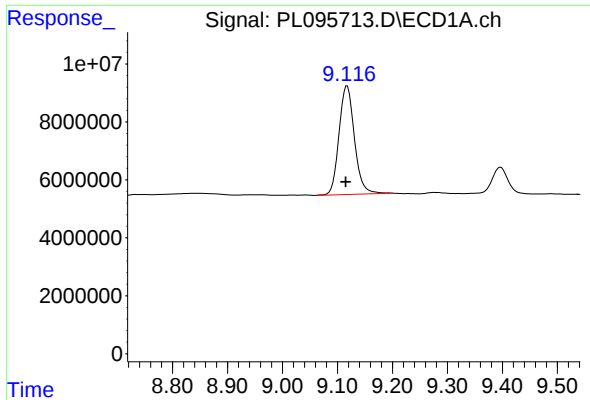

#28 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.002 min
Response: 73139401
Conc: 21.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

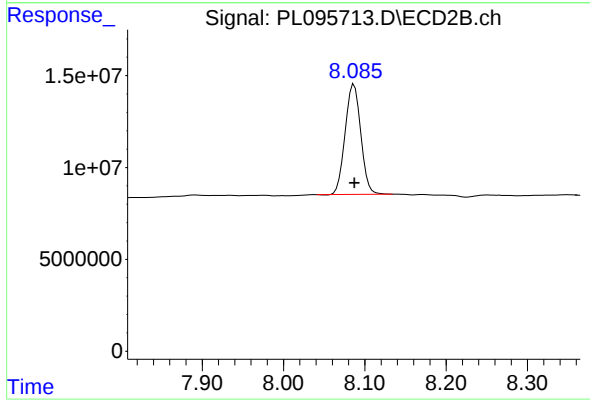

#28 Decachlorobiphenyl

R.T.: 8.087 min
Delta R.T.: 0.000 min
Response: 80094870
Conc: 19.42 ng/ml