

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051625\
 Data File : PL095719.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2025 13:23
 Operator : AR\AJ
 Sample : Q2055-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-02-051525

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 01:56:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
 Quant Title : GC Extractables
 QLast Update : Tue May 13 14:38:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.592	2.908	39464369	49391630	9.658	10.545
28)	SA Decachlor...	9.114	8.084	28236317	29439104	8.323	7.137
Target Compounds							
7)	B delta-BHC	4.817	0.000	4340224	0	0.799	N.D. #
9)	A Endosulfan I	6.142f	5.285f	31459800	8791206	6.426	1.700 #
10)	B gamma-Chl...	5.979	0.000	16459387	0	3.074	N.D. #
11)	B alpha-Chl...	6.071	0.000	61017331	0	11.739	N.D. #
13)	MA Dieldrin	6.409f	0.000	8847427	0	1.795	N.D. #
23)	Chlordane-1	0.000	3.918	0	10403643	N.D.	43.229 #
24)	Chlordane-2	0.000	4.536f	0	4200285	N.D.	15.783 #
25)	Chlordane-3	5.979	0.000	16459387	0	16.993	N.D. #
26)	Chlordane-4	6.071	0.000	61017331	0	52.566	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051625\
Data File : PL095719.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2025 13:23
Operator : AR\AJ
Sample : Q2055-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OR-02-051525

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 01:56:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
Quant Title : GC Extractables
QLast Update : Tue May 13 14:38:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

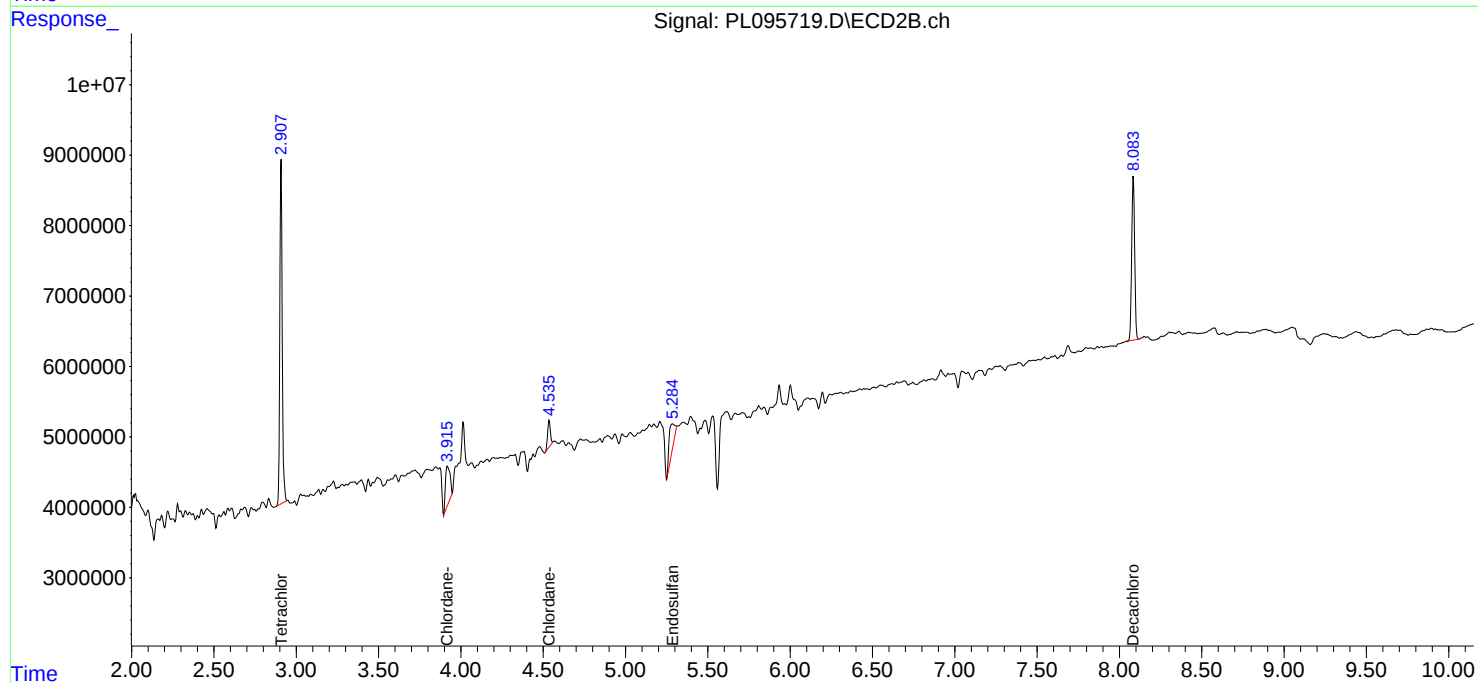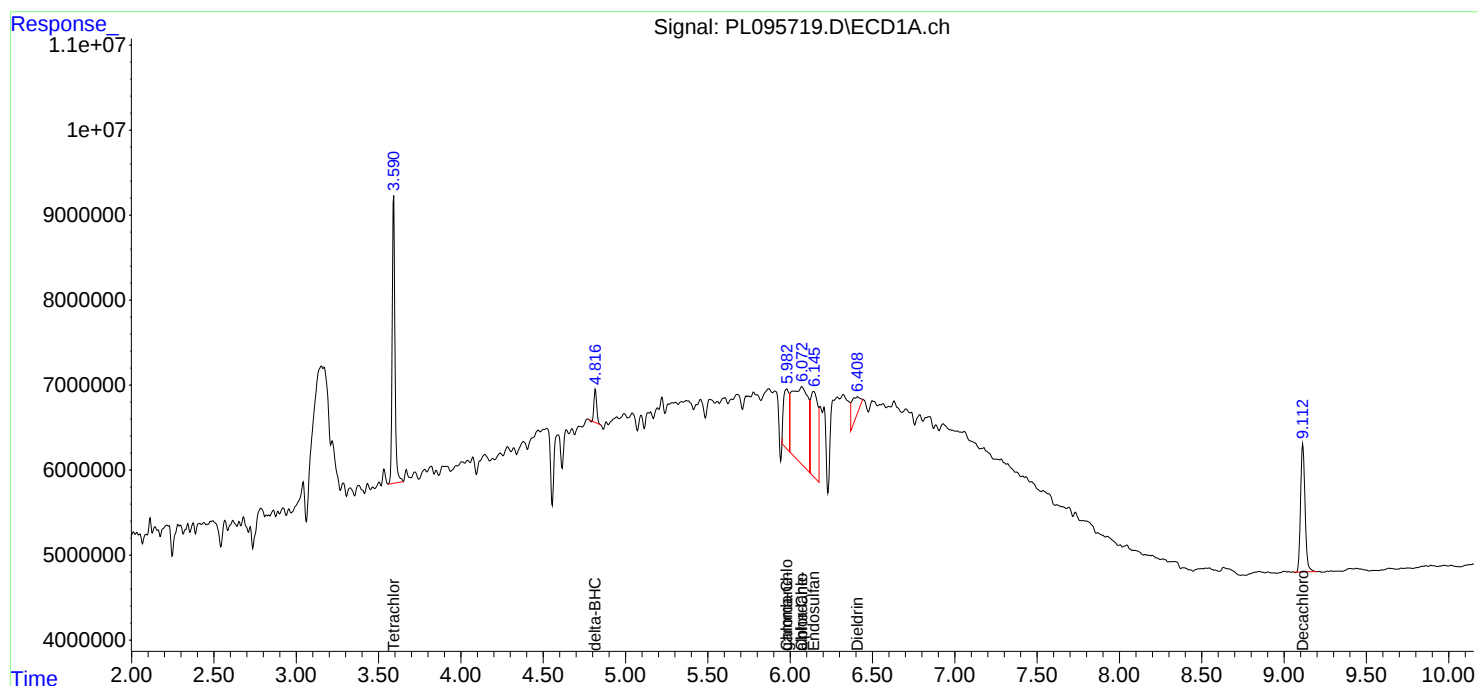


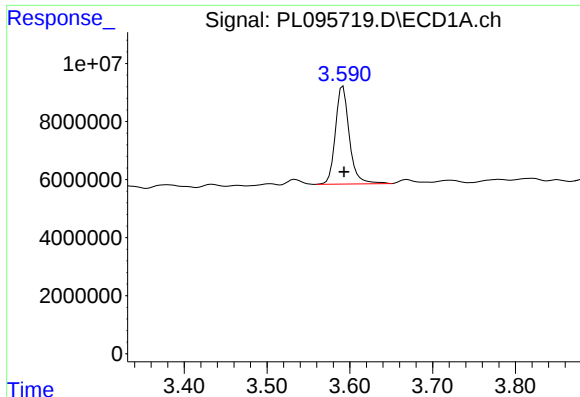

#1 Tetrachloro-m-xylene


R.T.: 3.592 min
Delta R.T.: -0.001 min
Response: 39464369
Conc: 9.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-051525

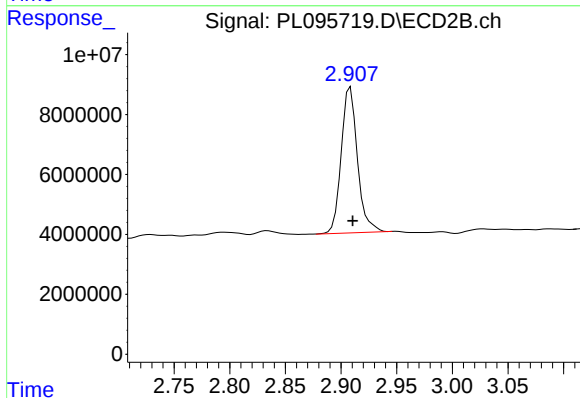


#1 Tetrachloro-m-xylene

R.T.: 2.908 min
Delta R.T.: -0.002 min
Response: 49391630
Conc: 10.54 ng/ml

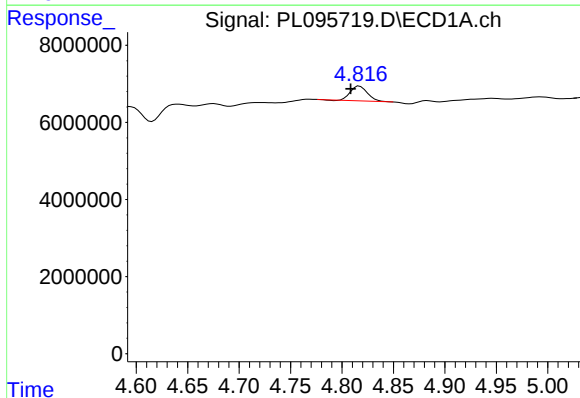


#7 delta-BHC

R.T.: 4.817 min
Delta R.T.: 0.009 min
Response: 4340224
Conc: 0.80 ng/ml

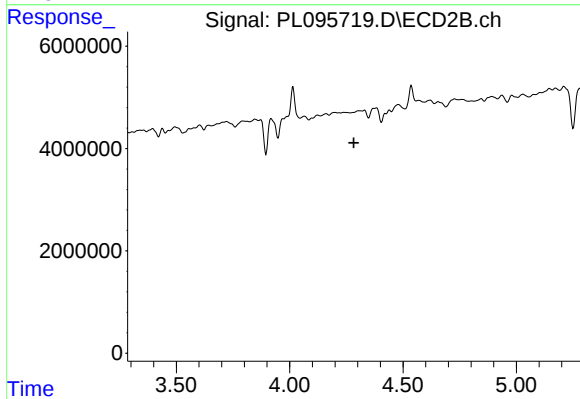

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.283 min
Response: 0
Conc: N.D.

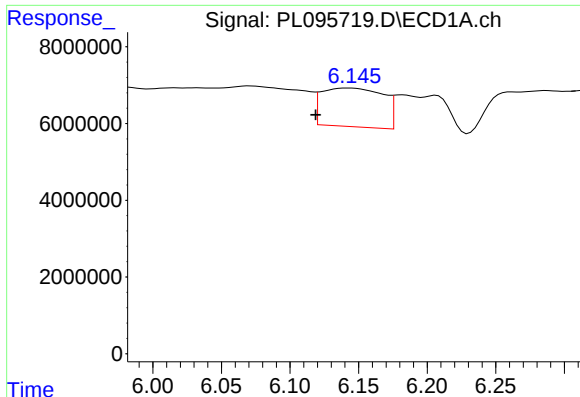

#9 Endosulfan I


R.T.: 6.142 min
Delta R.T.: 0.023 min
Response: 31459800
Conc: 6.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-051525

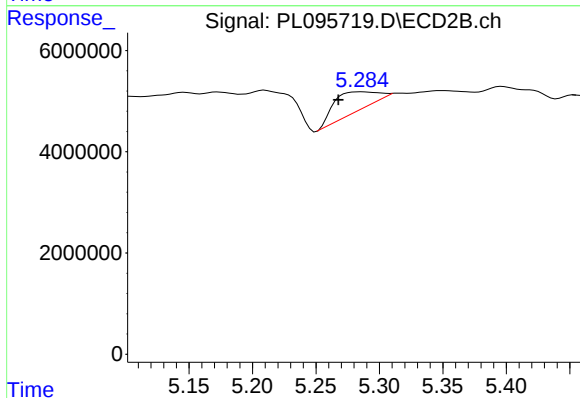


#9 Endosulfan I

R.T.: 5.285 min
Delta R.T.: 0.018 min
Response: 8791206
Conc: 1.70 ng/ml

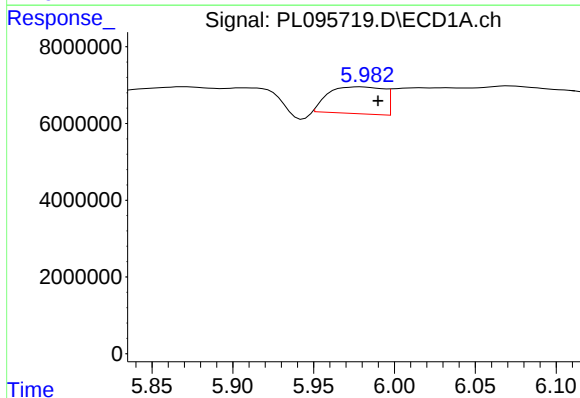


#10 gamma-Chlordane

R.T.: 5.979 min
Delta R.T.: -0.010 min
Response: 16459387
Conc: 3.07 ng/ml

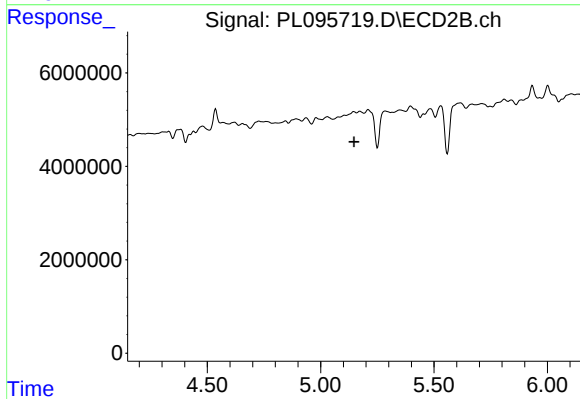

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.148 min
Response: 0
Conc: N.D.

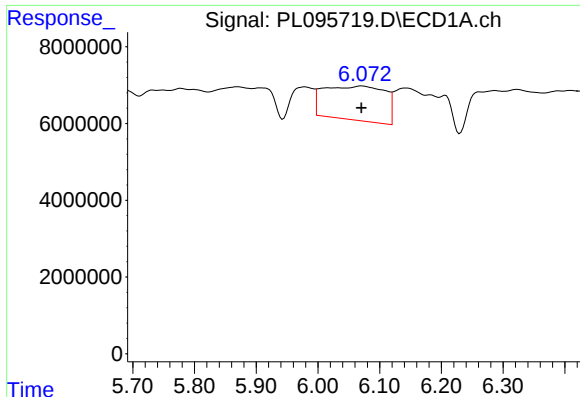

#11 alpha-Chlordane


R.T.: 6.071 min
Delta R.T.: 0.000 min
Response: 61017331
Conc: 11.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-051525

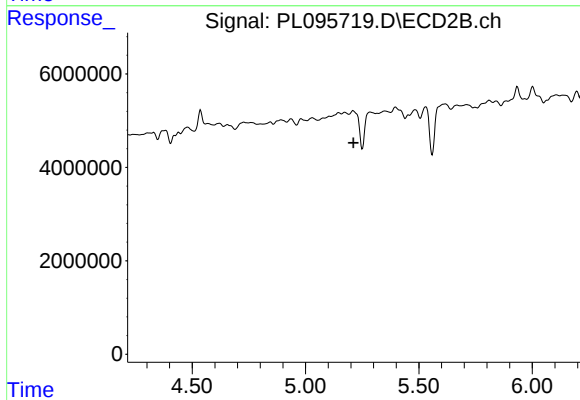


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.212 min
Response: 0
Conc: N.D.

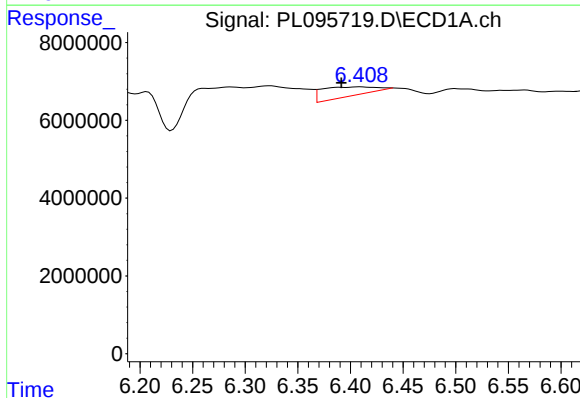


#13 Dieldrin

R.T.: 6.409 min
Delta R.T.: 0.018 min
Response: 8847427
Conc: 1.80 ng/ml

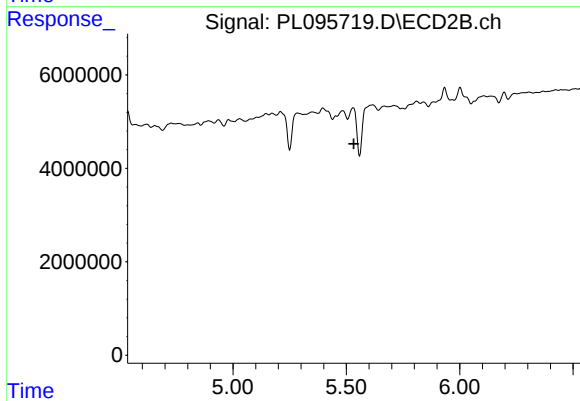

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 5.533 min
Response: 0
Conc: N.D.

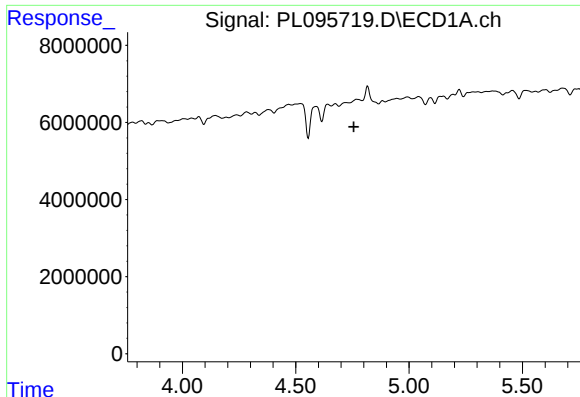

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.756 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-02-051525

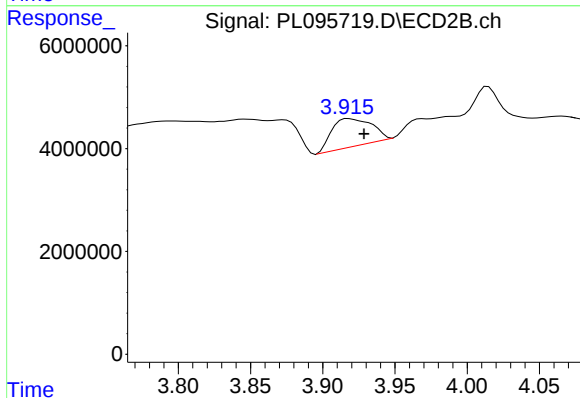


#23 Chlordane-1

R.T.: 3.918 min
Delta R.T.: -0.011 min
Response: 10403643
Conc: 43.23 ng/ml

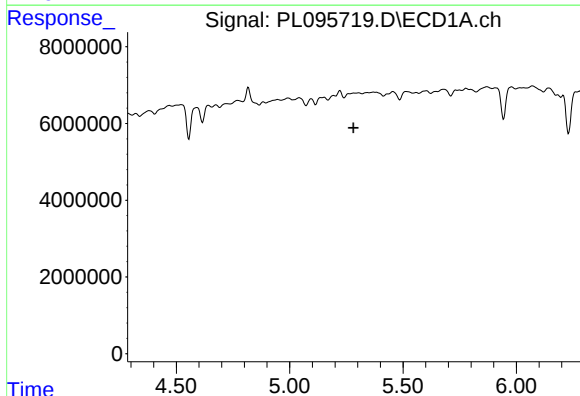


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.282 min
Response: 0
Conc: N.D.

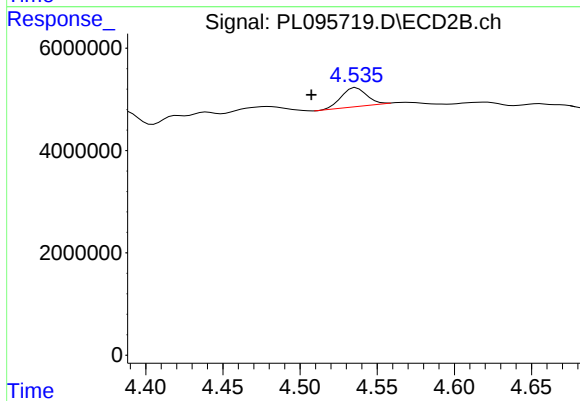

#24 Chlordane-2


R.T.: 4.536 min
Delta R.T.: 0.029 min
Response: 4200285
Conc: 15.78 ng/ml

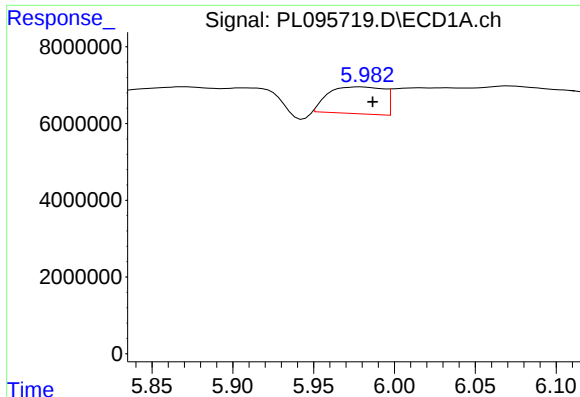

#25 Chlordane-3


R.T.: 5.979 min
Delta R.T.: -0.007 min
Response: 16459387
Conc: 16.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-051525

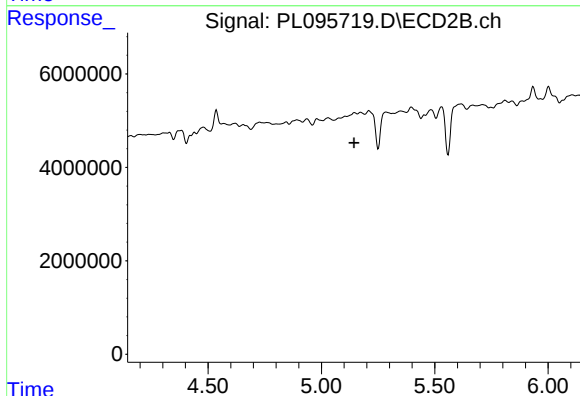


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.144 min
Response: 0
Conc: N.D.

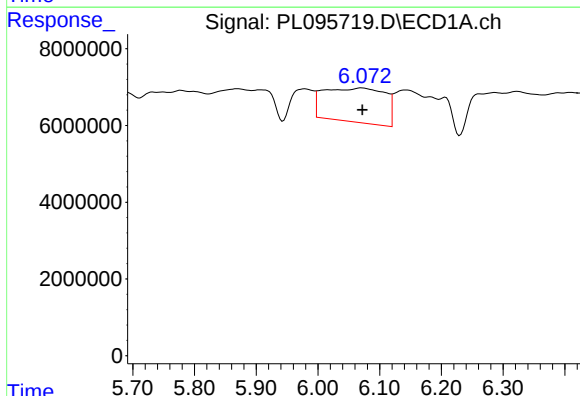


#26 Chlordane-4

R.T.: 6.071 min
Delta R.T.: -0.001 min
Response: 61017331
Conc: 52.57 ng/ml

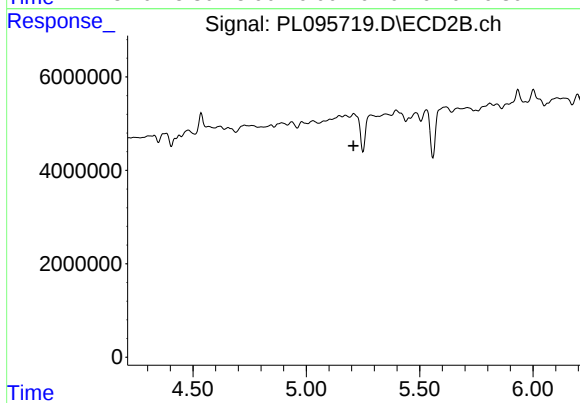

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.208 min
Response: 0
Conc: N.D.

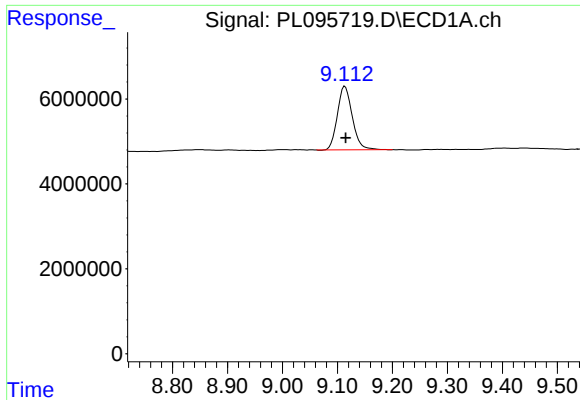

#28 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: -0.002 min
Response: 28236317
Conc: 8.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-051525

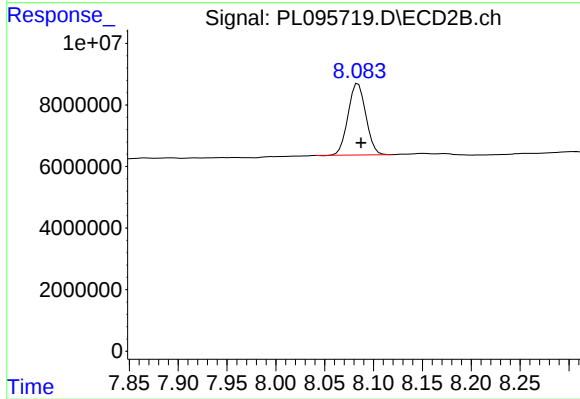

#28 Decachlorobiphenyl

R.T.: 8.084 min
Delta R.T.: -0.003 min
Response: 29439104
Conc: 7.14 ng/ml