

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051625\
 Data File : PL095724.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2025 14:32
 Operator : AR\AJ
 Sample : Q2032-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-24

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 01:56:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
 Quant Title : GC Extractables
 QLast Update : Tue May 13 14:38:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.591	2.908	87393160	81700412	21.388	17.442
28)	SA Decachlor...	9.113	8.084	49262894	58295180	14.521	14.133
Target Compounds							
9)	A Endosulfan I	0.000	5.283f	0	10061995	N.D.	1.945 #
23)	Chlordane-1	0.000	3.921	0	339742	N.D.	1.412 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051625\
Data File : PL095724.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2025 14:32
Operator : AR\AJ
Sample : Q2032-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-24

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 01:56:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
Quant Title : GC Extractables
QLast Update : Tue May 13 14:38:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

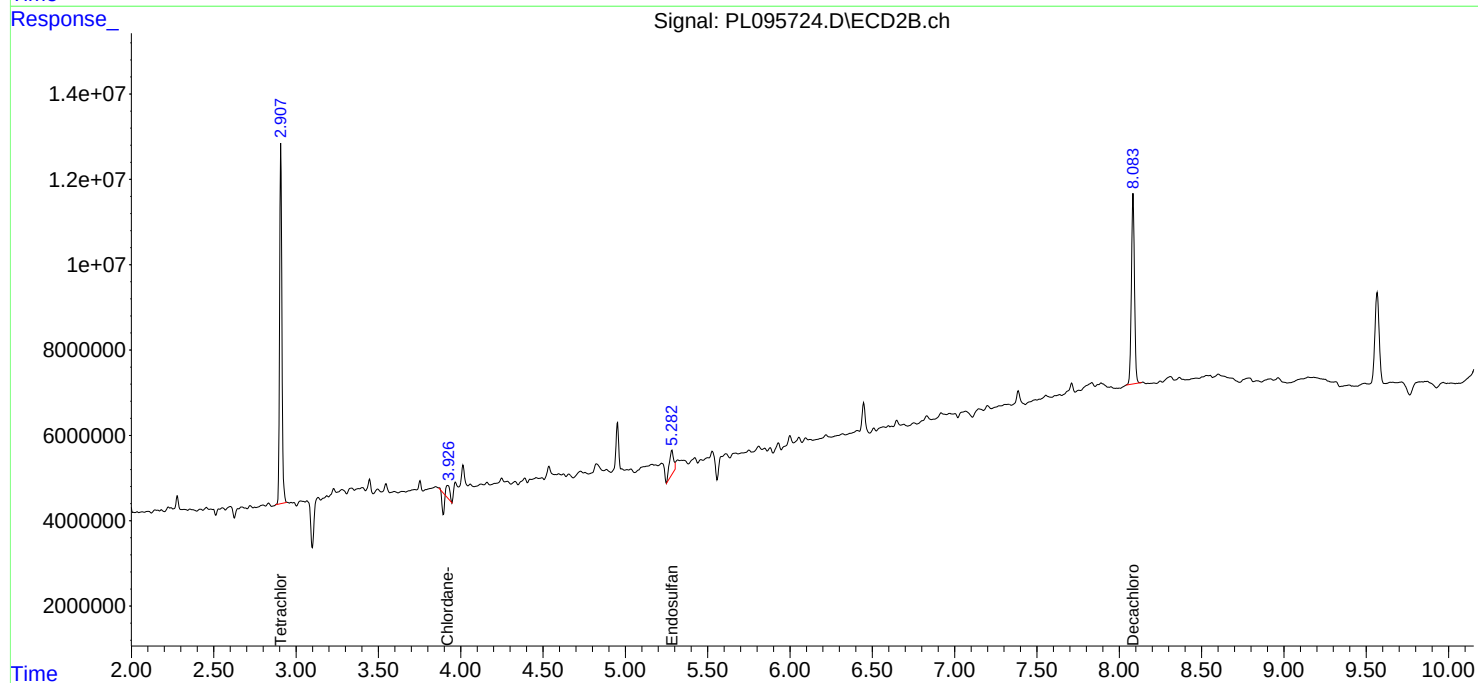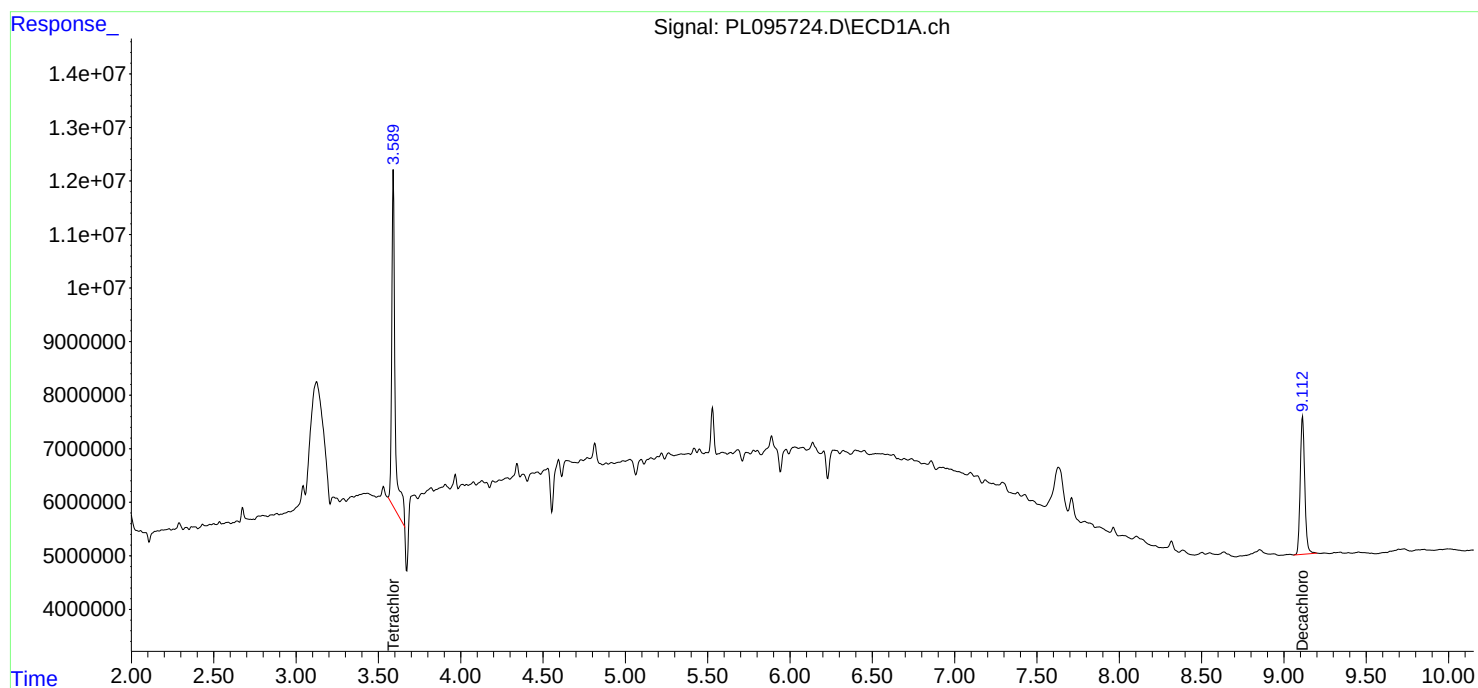


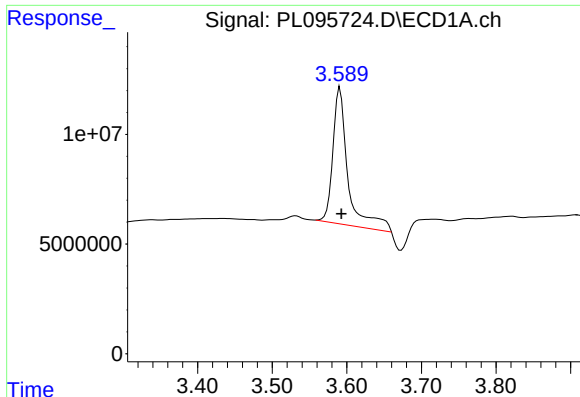

#1 Tetrachloro-m-xylene


R.T.: 3.591 min
Delta R.T.: -0.002 min
Response: 87393160
Conc: 21.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-24

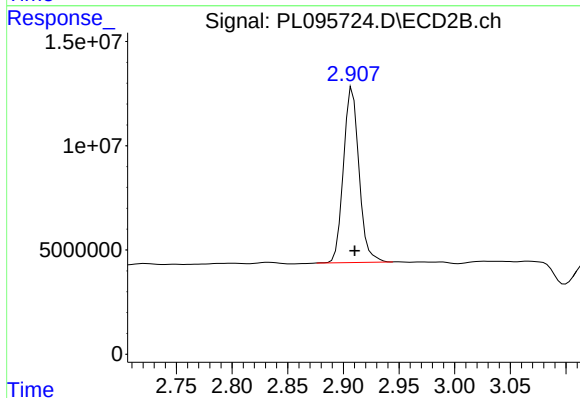


#1 Tetrachloro-m-xylene

R.T.: 2.908 min
Delta R.T.: -0.002 min
Response: 81700412
Conc: 17.44 ng/ml

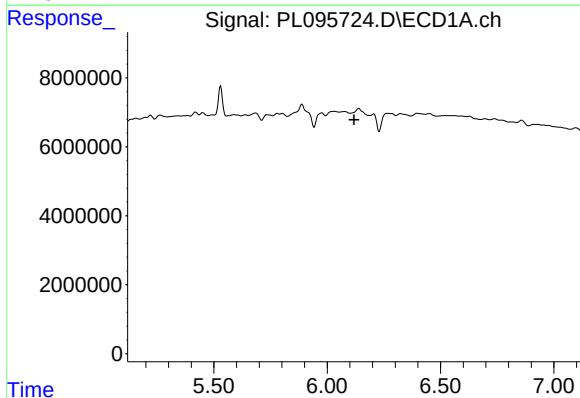


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.119 min
Response: 0
Conc: N.D.

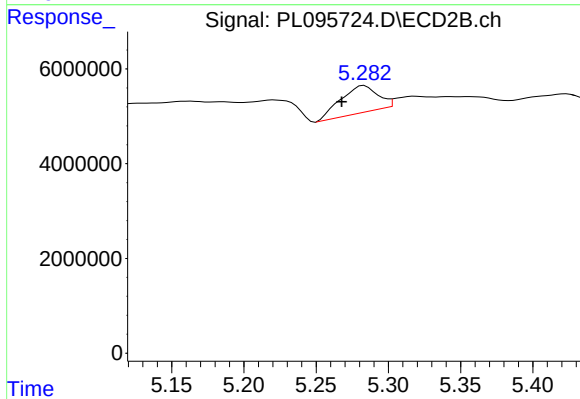

#9 Endosulfan I


R.T.: 5.283 min
Delta R.T.: 0.016 min
Response: 10061995
Conc: 1.95 ng/ml

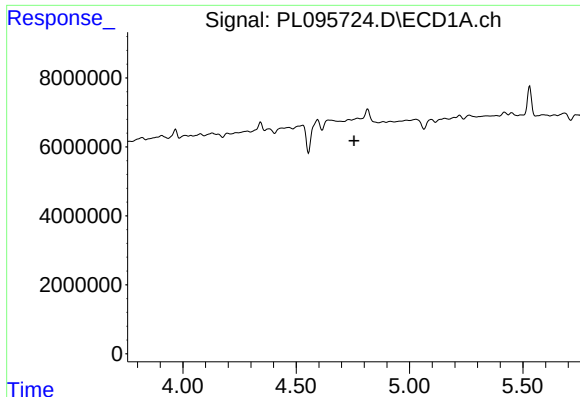

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.756 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-24

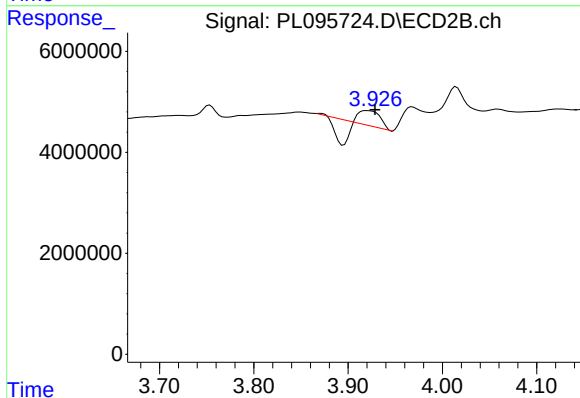


#23 Chlordane-1

R.T.: 3.921 min
Delta R.T.: -0.008 min
Response: 339742
Conc: 1.41 ng/ml

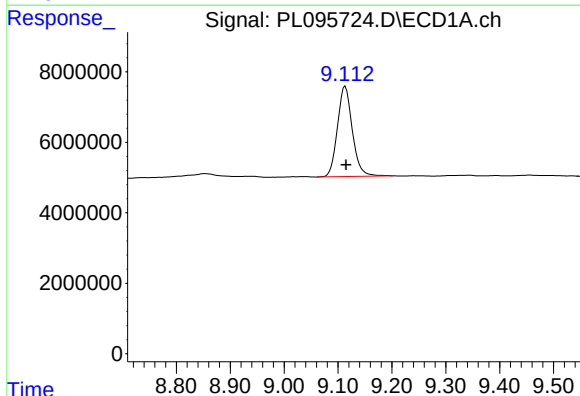

#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: -0.002 min
Response: 49262894
Conc: 14.52 ng/ml

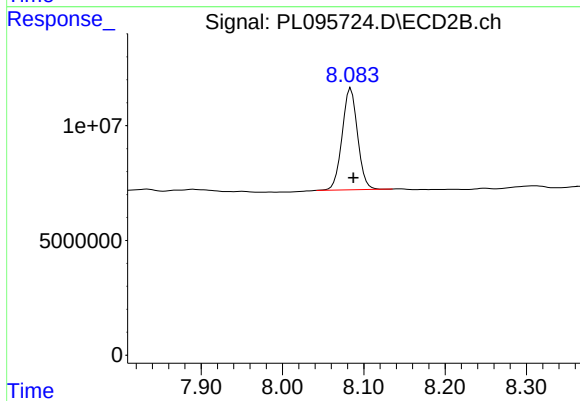

#28 Decachlorobiphenyl

R.T.: 8.084 min
Delta R.T.: -0.003 min
Response: 58295180
Conc: 14.13 ng/ml